


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL081221\
 Data File : VL037408.D
 Acq On : 12 Aug 2021 9:37
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081221AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Aug 11 09:01:07 2021
 Last Update : Wed Aug 11 09:01:07 2021

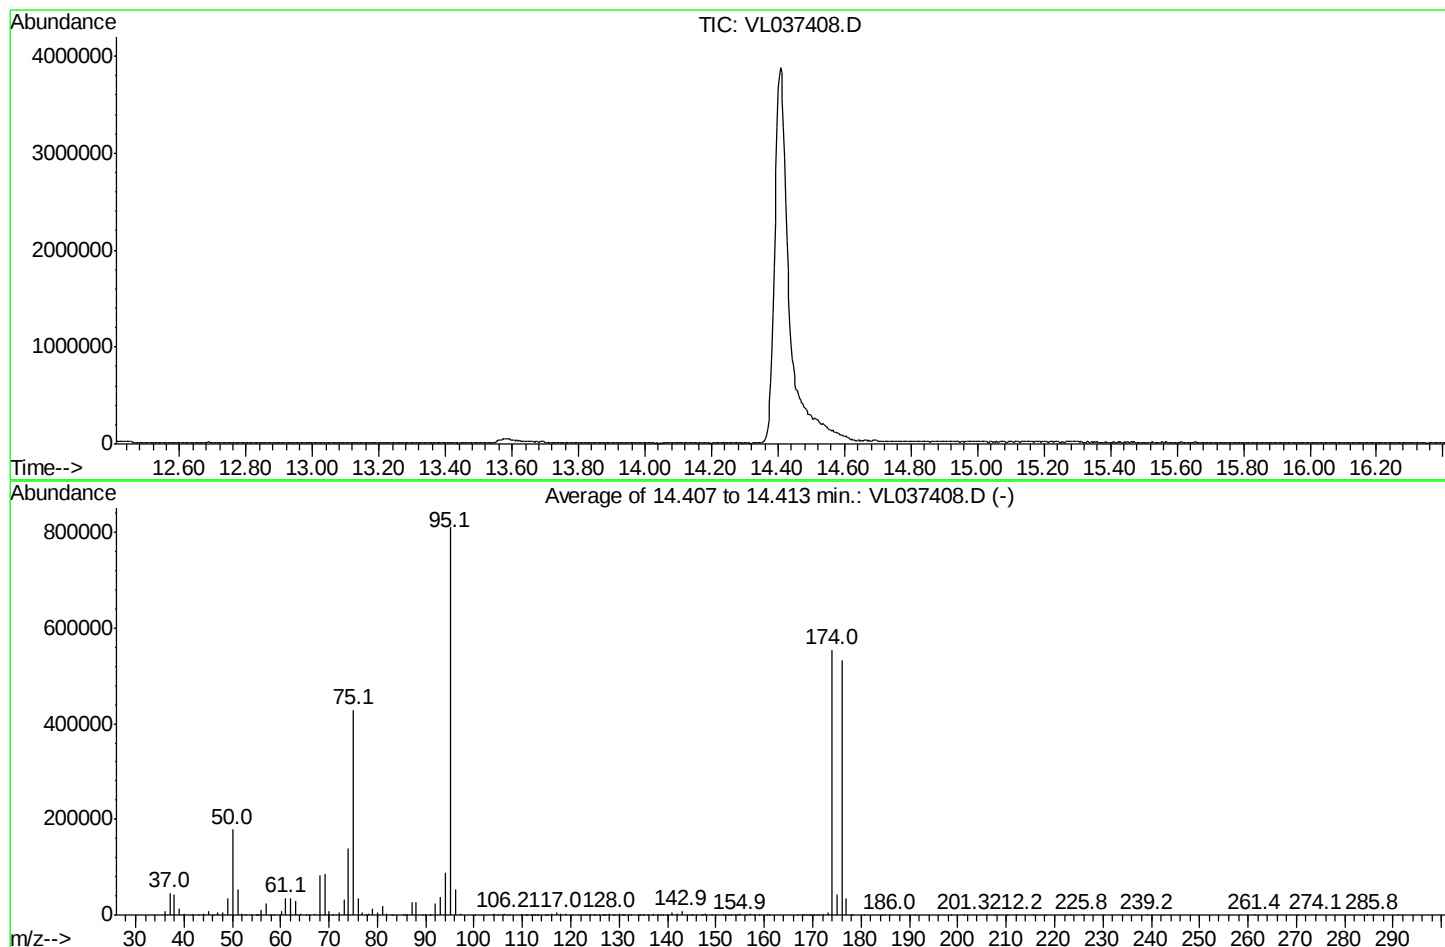

AutoFind: Scans 3614, 3615, 3616; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.0	178517	PASS
75	95	30	66	52.9	428757	PASS
95	95	100	100	100.0	810752	PASS
96	95	5	9	6.8	54728	PASS
173	174	0.00	2	0.9	5262	PASS
174	95	50	120	68.5	555392	PASS
175	174	4	9	7.5	41821	PASS
176	174	93	101	95.8	532181	PASS
177	176	5	9	6.6	34890	PASS