

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_L\Data\VL081224\  
 Data File : VL041535.D  
 Acq On : 12 Aug 2024 14:07  
 Operator : SY/MD  
 Sample : P3496-06DL 200X  
 Misc : 400mL/MSVOA\_L  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_L  
 ClientSampleId :

Quant Time: Aug 13 02:13:47 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_L\methods\VL072524AIR.M  
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA\_L Fri Aug 26 06:05:16 2022  
 QLast Update : Tue Aug 13 02:09:20 2024  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-----------------------------|--------|-------|----------|----------|--------|----------|
| -----                       |        |       |          |          |        |          |
| Internal Standards          |        |       |          |          |        |          |
| 1) Bromochloromethane       | 5.198  | 49    | 960135   | 10.000   | ppbv   | 0.01     |
| 33) 1,4-Difluorobenzene     | 6.655  | 114   | 2513402  | 10.000   | ppbv   | 0.00     |
| 55) Chlorobenzene-d5        | 11.468 | 117   | 2347282  | 10.000   | ppbv   | # 0.00   |
| System Monitoring Compounds |        |       |          |          |        |          |
| 68) 1-Bromo-4-Fluorobenzene | 13.777 | 95    | 1759698  | 9.742    | ppbv   | 0.00     |
| Spiked Amount               | 10.000 | Range | 65 - 135 | Recovery | =      | 97.400%  |
| Target Compounds            |        |       |          |          |        |          |
|                             |        |       |          |          | Qvalue |          |
| 9) Propene                  | 2.710  | 41    | 54298    | 1.034    | ppbv   | 100      |
| 10) Heptane                 | 7.581  | 43    | 6146     | 0.052    | ppbv # | 78       |
| 13) Ethanol                 | 3.263  | 45    | 35585    | 7.583    | ppbv   | 81       |
| 15) Acetone                 | 3.475  | 43    | 1221887  | 11.201   | ppbv   | 96       |
| 16) 1,3-Butadiene           | 2.980  | 39    | 45367    | 0.778    | ppbv # | 23       |
| 17) tert-Butyl alcohol      | 3.906  | 59    | 13937    | 0.140    | ppbv # | 94       |
| 19) Isopropyl Alcohol       | 3.600  | 45    | 17932    | 0.281    | ppbv # | 93       |
| 20) Methylene Chloride      | 3.941  | 84    | 17922    | 0.441    | ppbv   | 98       |
| 23) Vinyl Acetate           | 4.790  | 43    | 1679974  | 20.164   | ppbv # | 90       |
| 25) Ethyl Acetate           | 5.009  | 43    | 24111    | 0.111    | ppbv # | 1        |
| 26) Hexane                  | 5.218  | 57    | 6226     | 0.069    | ppbv # | 1        |
| 34) 2-Butanone              | 4.790  | 43    | 1679974  | 13.818   | ppbv   | 99       |
| 39) 1,2-Dichloropropane     | 6.655  | 63    | 628500   | 8.939    | ppbv # | 26       |
| -----                       |        |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_L\Data\VL081224\  
Data File : VL041535.D  
Acq On : 12 Aug 2024 14:07  
Operator : SY/MD  
Sample : P3496-06DL 200X  
Misc : 400mL/MSVOA\_L  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_L  
ClientSampleId :

Quant Time: Aug 13 02:13:47 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_L\methods\VL072524AIR.M  
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA\_L Fri Aug 26 06:05:16 2022  
QLast Update : Tue Aug 13 02:09:20 2024  
Response via : Initial Calibration




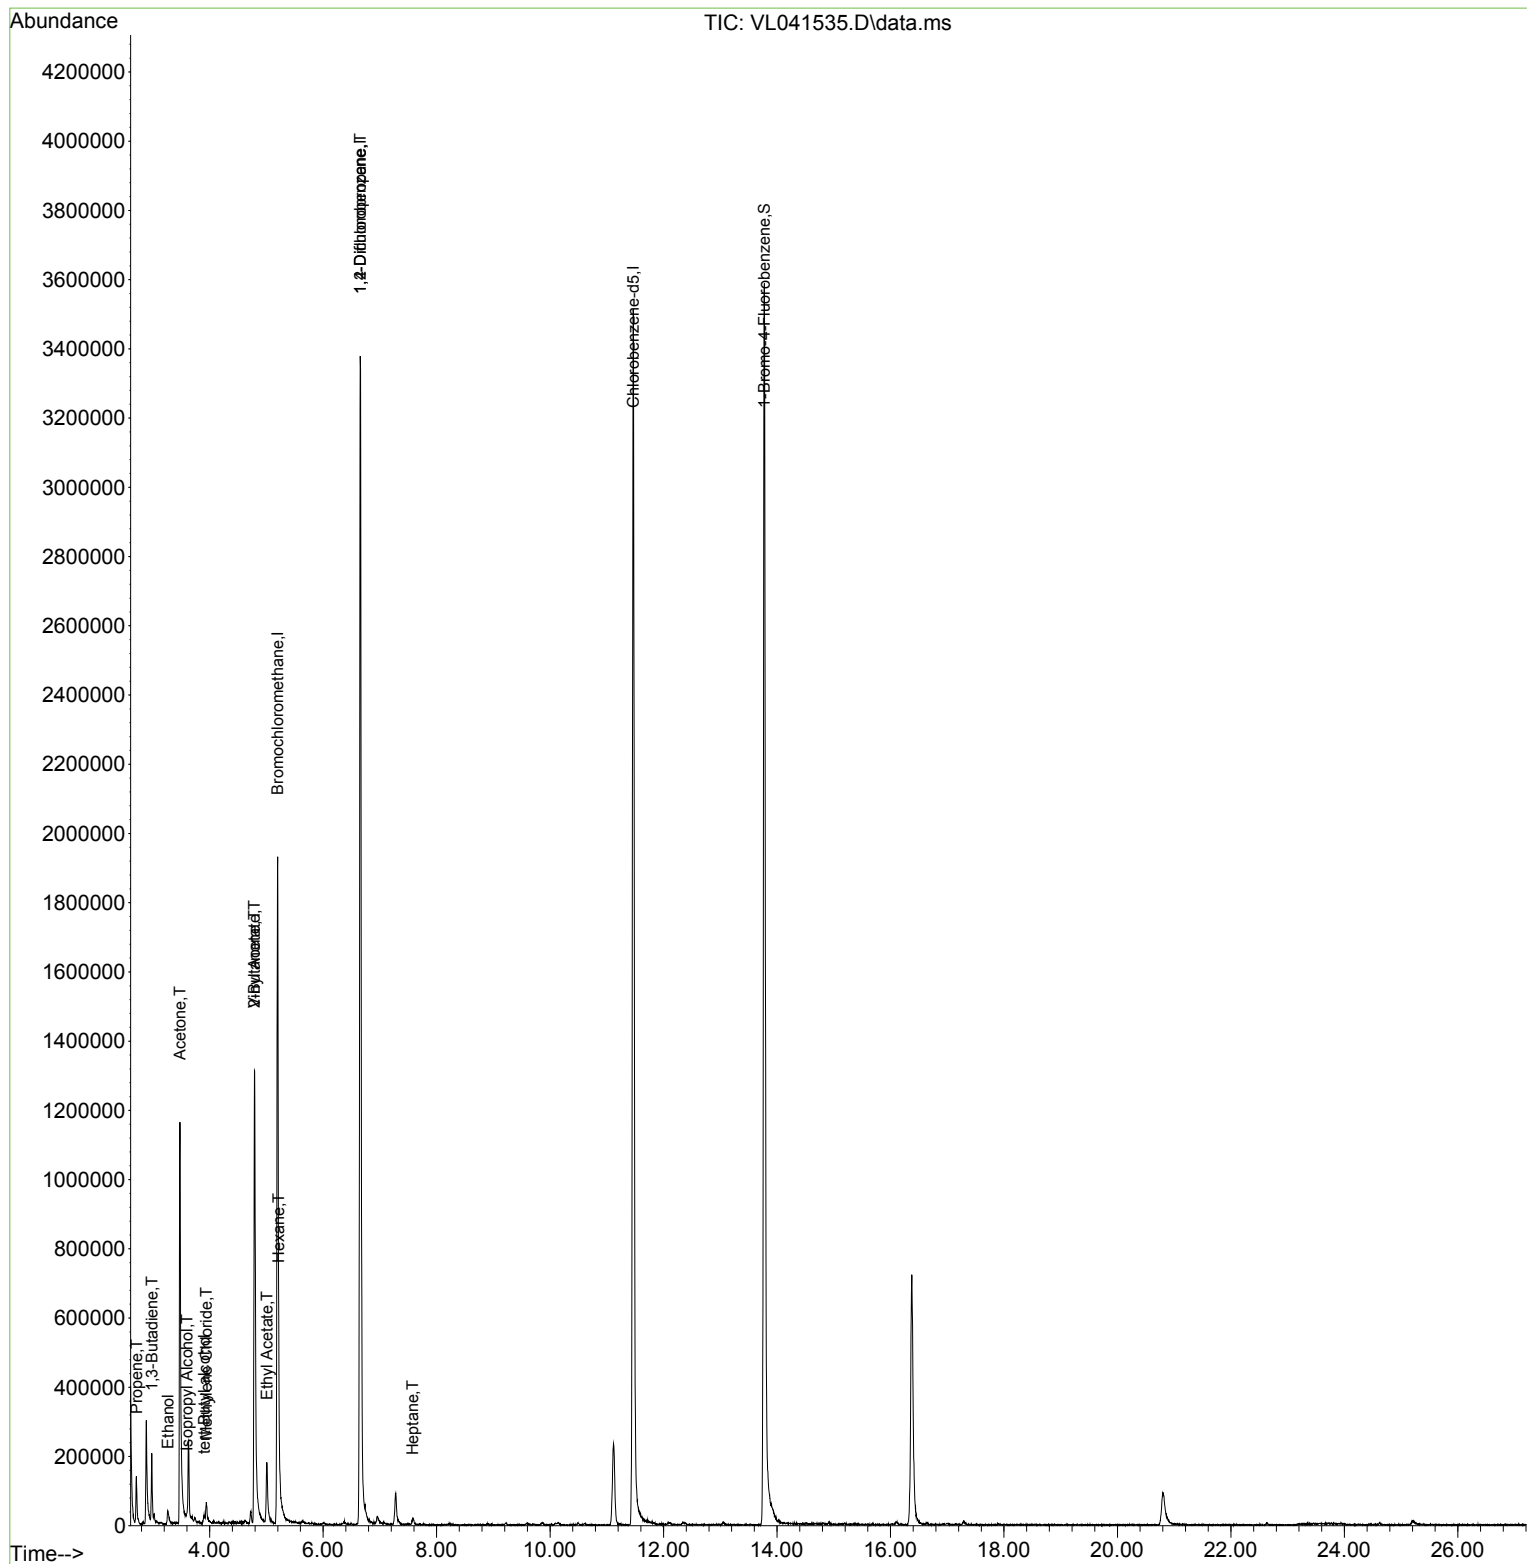


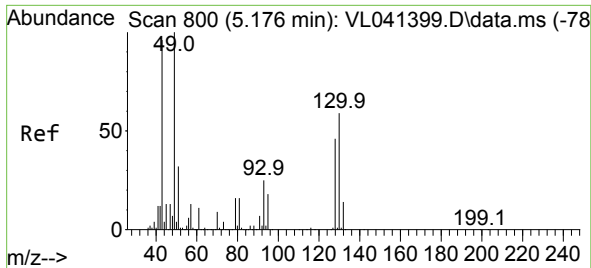

#1  
Bromochloromethane  
Concen: 10.000 ppbv  
RT: 5.198 min Scan# 80  
Delta R.T. 0.010 min  
Lab File: VL041535.D  
Acq: 12 Aug 2024 14:07




Instrument :  
MSVOA\_L  
ClientSampleId :


Tgt Ion: 49 Resp: 960135  
Ion Ratio Lower Upper  
49 100  
128 47.8 23.8 71.4  
130 60.6 30.8 92.4

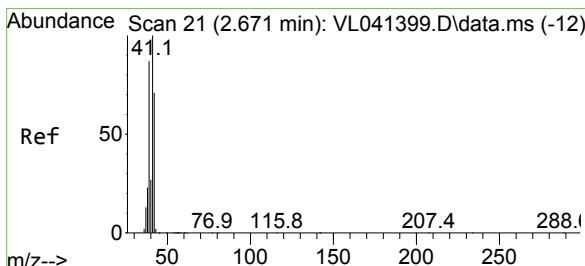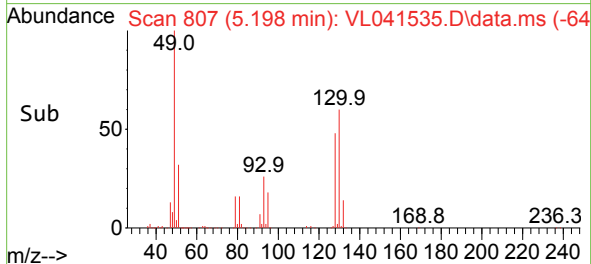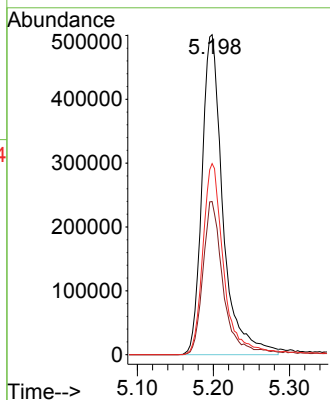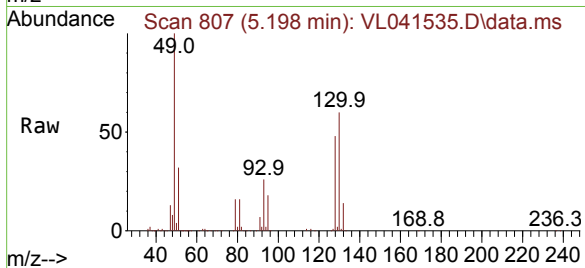

#9  
Propene  
Concen: 1.034 ppbv  
RT: 2.710 min Scan# 33  
Delta R.T. 0.016 min  
Lab File: VL041535.D  
Acq: 12 Aug 2024 14:07

Tgt Ion: 41 Resp: 54298  
Ion Ratio Lower Upper  
41 100  
42 70.1 55.9 83.9


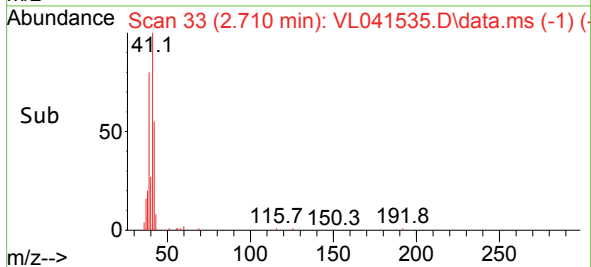
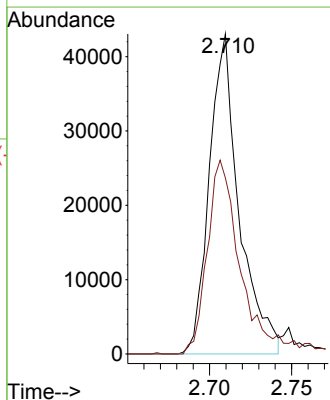
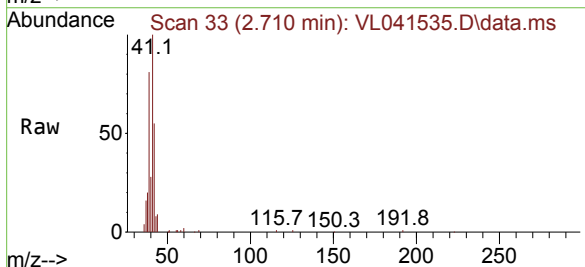




#10  
Heptane  
Concen: 0.052 ppbv  
RT: 7.581 min Scan# 11  
Delta R.T. 0.003 min  
Lab File: VL041535.D  
Acq: 12 Aug 2024 14:07




Instrument :  
MSVOA\_L  
ClientSampleId :


Tgt Ion: 43 Resp: 6146  
Ion Ratio Lower Upper  
43 100  
57 65.6 40.5 60.7#

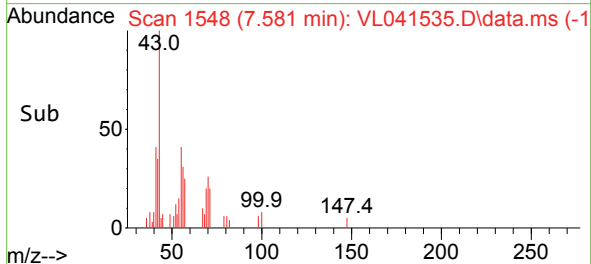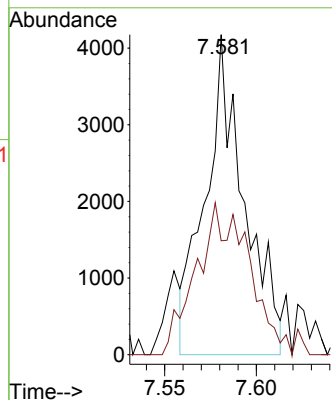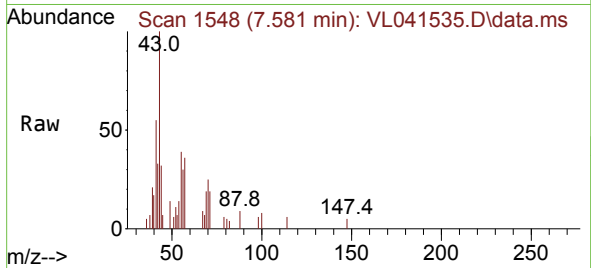

#13  
Ethanol  
Concen: 7.583 ppbv  
RT: 3.263 min Scan# 205  
Delta R.T. 0.019 min  
Lab File: VL041535.D  
Acq: 12 Aug 2024 14:07

Tgt Ion: 45 Resp: 35585  
Ion Ratio Lower Upper  
45 100  
46 44.3 13.4 53.4


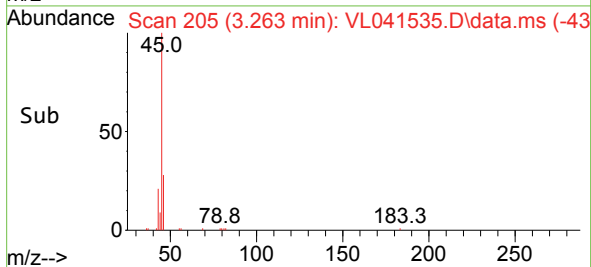
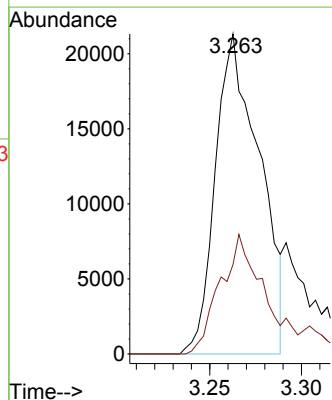
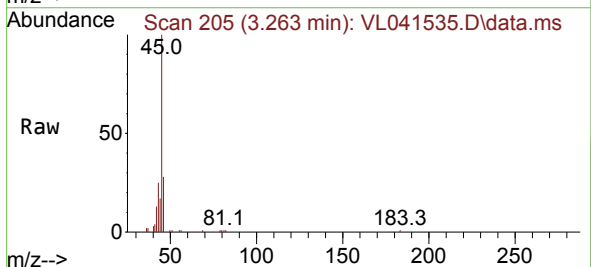




#15  
Acetone  
Concen: 11.201 ppbv  
RT: 3.475 min Scan# 21  
Delta R.T. 0.007 min  
Lab File: VL041535.D  
Acq: 12 Aug 2024 14:07




Instrument :  
MSVOA\_L  
ClientSampleId :


Tgt Ion: 43 Resp: 1221887  
Ion Ratio Lower Upper  
43 100  
58 28.9 21.4 32.2

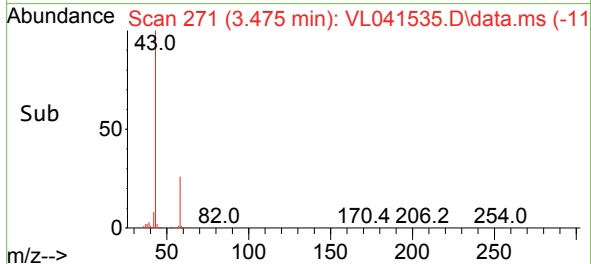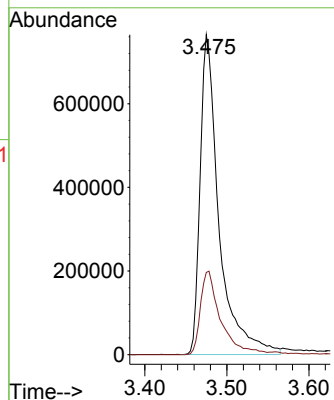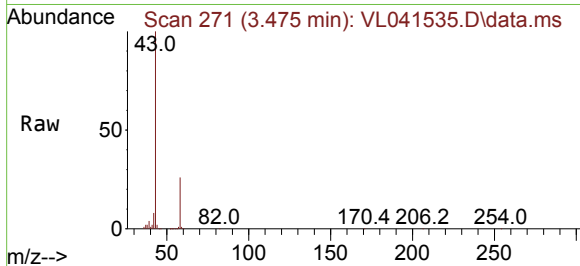

#16  
1,3-Butadiene  
Concen: 0.778 ppbv  
RT: 2.980 min Scan# 117  
Delta R.T. -0.006 min  
Lab File: VL041535.D  
Acq: 12 Aug 2024 14:07

Tgt Ion: 39 Resp: 45367  
Ion Ratio Lower Upper  
39 100  
54 10.6 62.5 93.7#

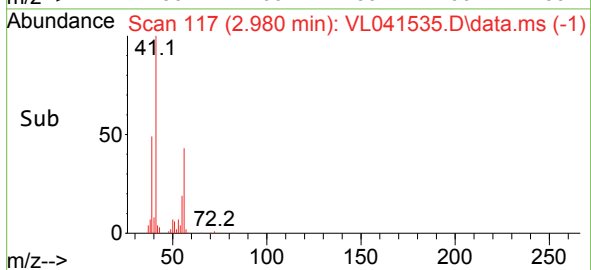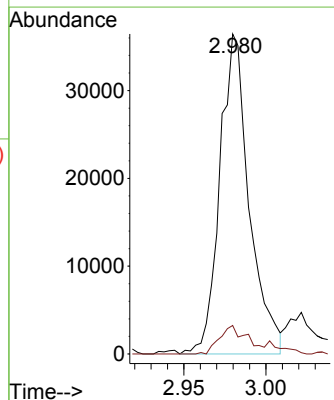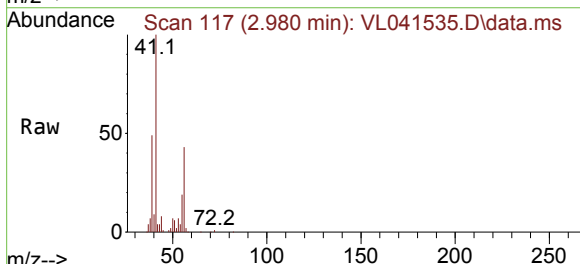



#17

tert-Butyl alcohol

Concen: 0.140 ppbv

RT: 3.906 min Scan# 405

Delta R.T. 0.029 min

Lab File: VL041535.D

Acq: 12 Aug 2024 14:07

Instrument :

MSVOA\_L





ClientSampleId :

Tgt Ion: 59 Resp: 13937

Ion Ratio Lower Upper

59 100

57 13.0 8.6 12.8#

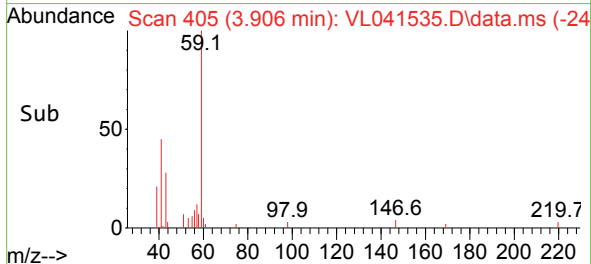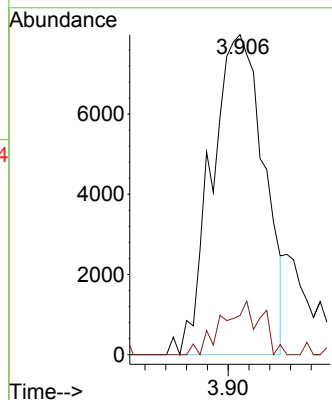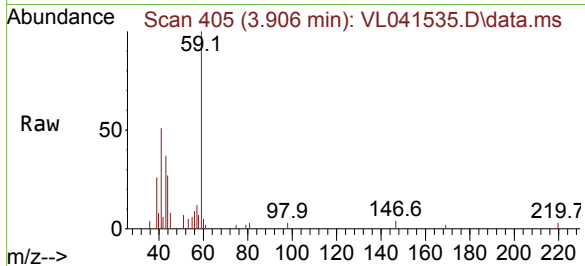

#19

Isopropyl Alcohol

Concen: 0.281 ppbv

RT: 3.600 min Scan# 310

Delta R.T. 0.026 min

Lab File: VL041535.D




Acq: 12 Aug 2024 14:07


Tgt Ion: 45 Resp: 17932

Ion Ratio Lower Upper

45 100


58 0.0 1.9 2.9#

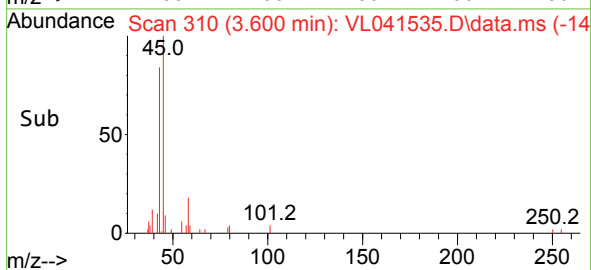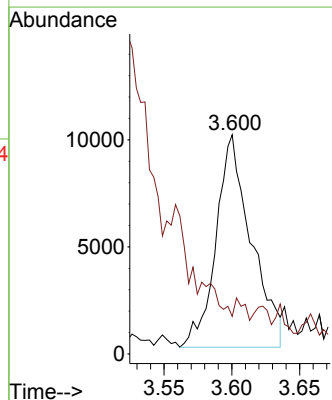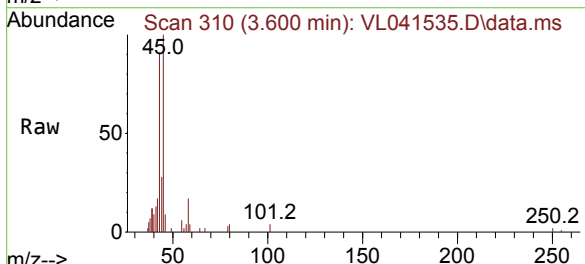






#20  
Methylene Chloride  
Concen: 0.441 ppbv  
RT: 3.941 min Scan# 416  
Delta R.T. 0.010 min  
Lab File: VL041535.D  
Acq: 12 Aug 2024 14:07

Instrument :  
MSVOA\_L  
ClientSampleId :

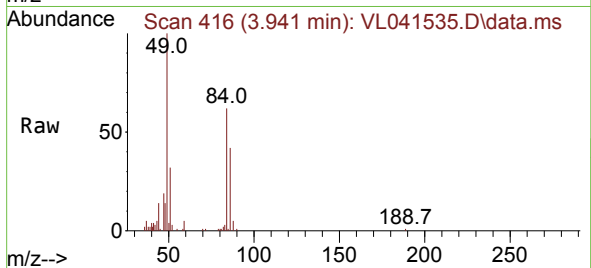

Tgt Ion: 84 Resp: 17922




| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 84  | 100   |       |       |
| 49  | 155.0 | 126.6 | 190.0 |
| 51  | 50.1  | 38.6  | 58.0  |
| 86  | 67.3  | 53.0  | 79.4  |

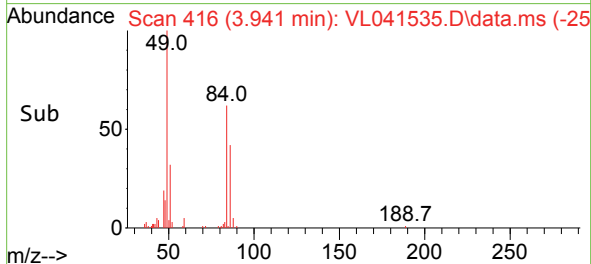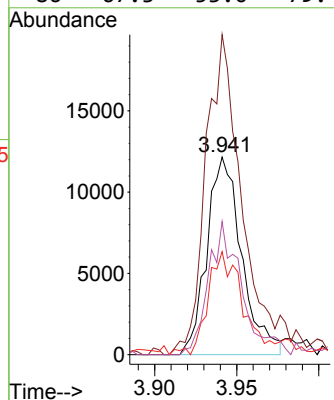


#23  
Vinyl Acetate  
Concen: 20.164 ppbv  
RT: 4.790 min Scan# 680  
Delta R.T. 0.164 min  
Lab File: VL041535.D  
Acq: 12 Aug 2024 14:07

Tgt Ion: 43 Resp: 1679974


| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 43  | 100   |       |       |
| 86  | 0.0   | 4.6   | 6.8#  |
| 42  | 7.0   | 7.9   | 11.9# |
| 44  | 2.7   | 4.2   | 6.4#  |

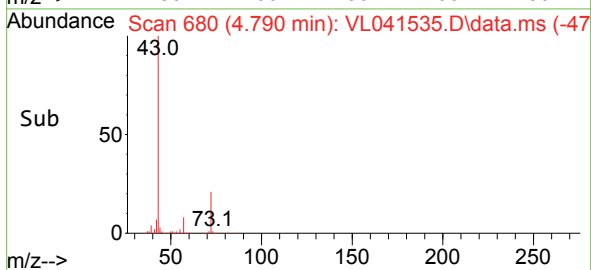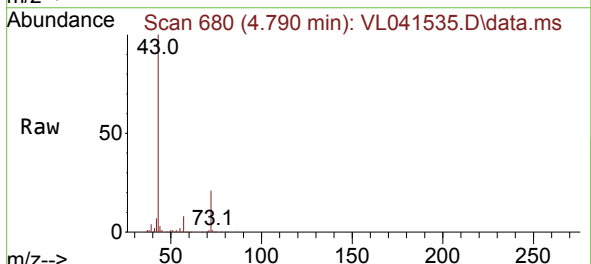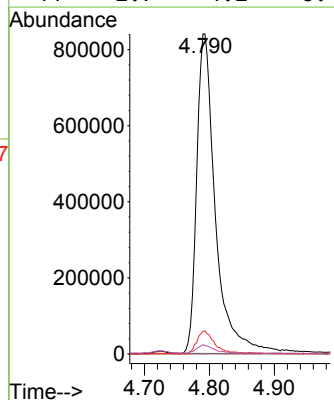






#25  
Ethyl Acetate  
Concen: 0.111 ppbv  
RT: 5.009 min Scan# 741  
Delta R.T. -0.193 min  
Lab File: VL041535.D  
Acq: 12 Aug 2024 14:07

Instrument :  
MSVOA\_L  
ClientSampleId :



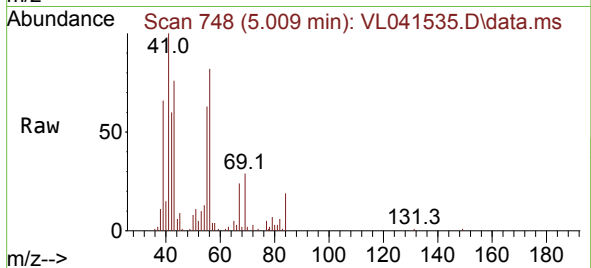



Tgt Ion: 43 Resp: 24111  
Ion Ratio Lower Upper  
43 100  
45 99.8 8.5 12.7#  
61 0.8 8.0 12.0#  
70 4.1 5.9 8.9#

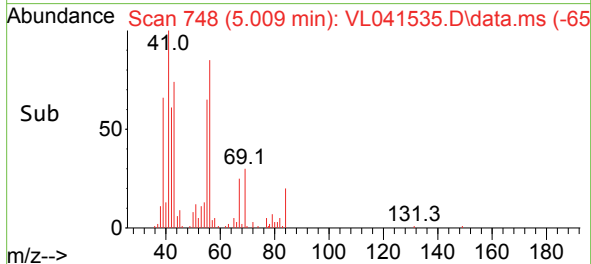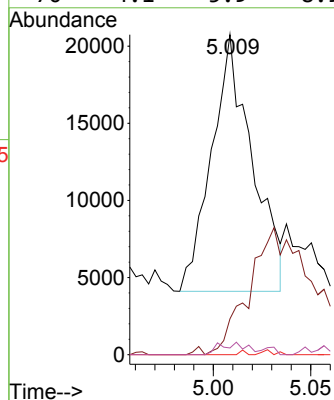

#26  
Hexane  
Concen: 0.069 ppbv  
RT: 5.218 min Scan# 813  
Delta R.T. 0.007 min  
Lab File: VL041535.D  
Acq: 12 Aug 2024 14:07

Tgt Ion: 57 Resp: 6226  
Ion Ratio Lower Upper  
57 100  
41 231.6 74.0 111.0#  
43 0.0 193.6 290.4#  
56 119.3 43.1 64.7#

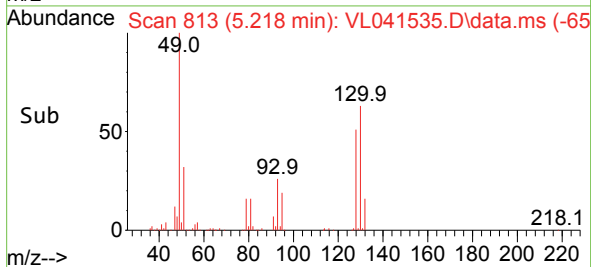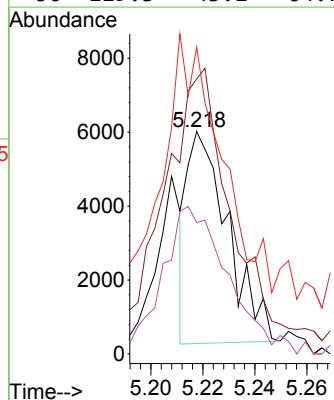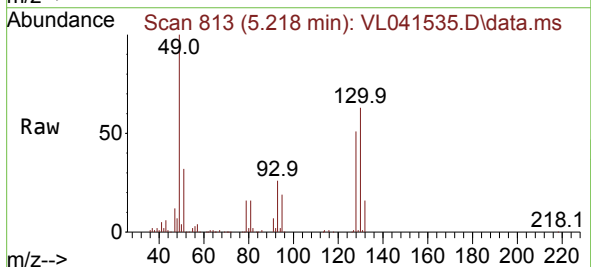



#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 6.655 min Scan# 11

Delta R.T. 0.003 min

Lab File: VL041535.D

Acq: 12 Aug 2024 14:07

Instrument :

MSVOA\_L

ClientSampleId :





Tgt Ion:114 Resp: 2513402

Ion Ratio Lower Upper

114 100

63 25.2 20.3 30.5

88 17.8 14.3 21.5

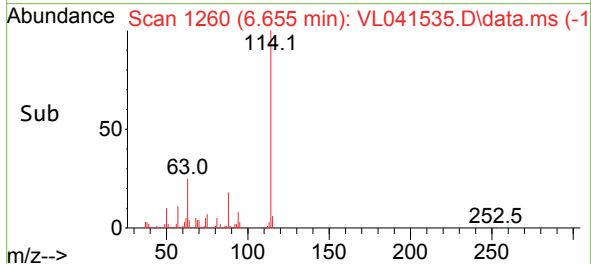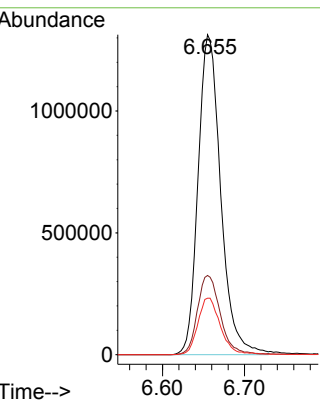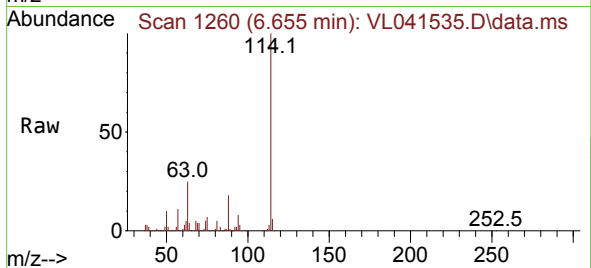

#34

2-Butanone

Concen: 13.818 ppbv

RT: 4.790 min Scan# 680

Delta R.T. 0.007 min

Lab File: VL041535.D




Acq: 12 Aug 2024 14:07


Tgt Ion: 43 Resp: 1679974

Ion Ratio Lower Upper

43 100

72 21.3 17.3 25.9

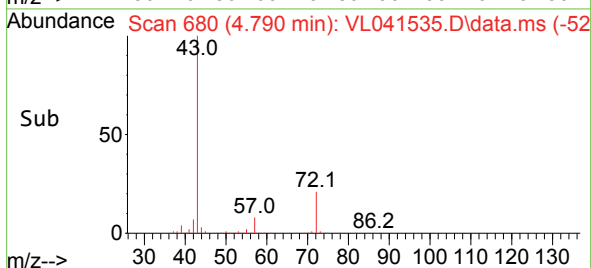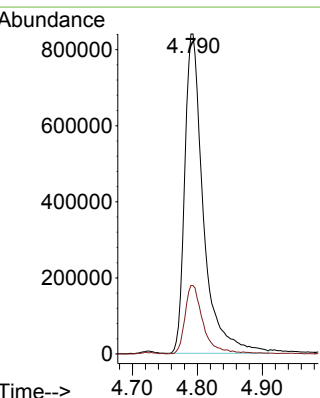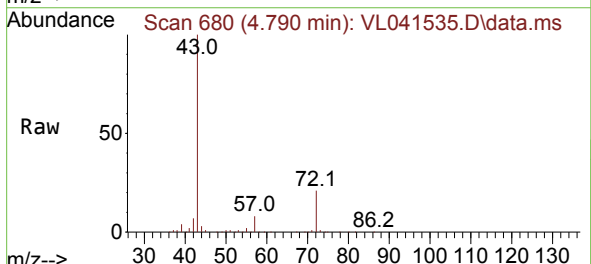

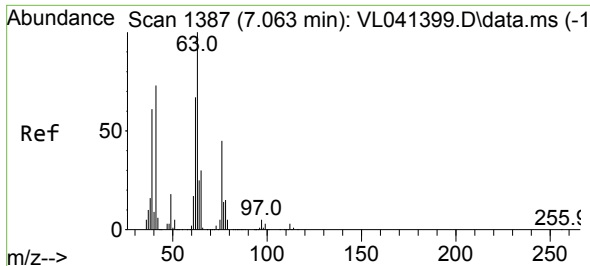

#39

1,2-Dichloropropane

Concen: 8.939 ppbv

RT: 6.655 min Scan# 1

Delta R.T. -0.418 min


Lab File: VL041535.D

Acq: 12 Aug 2024 14:07

Instrument :

MSVOA\_L

ClientSampleId :

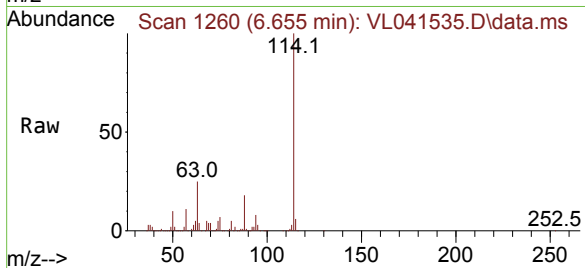




Tgt Ion: 63 Resp: 628500

Ion Ratio Lower Upper

63 100

41 0.3 58.3 87.5#

62 18.4 53.9 80.9#

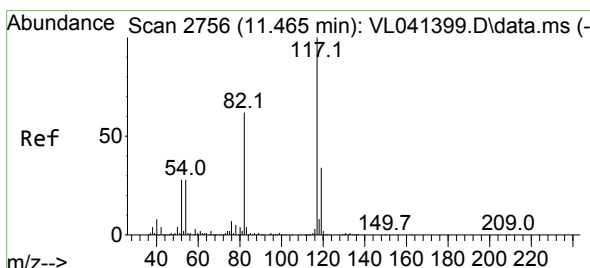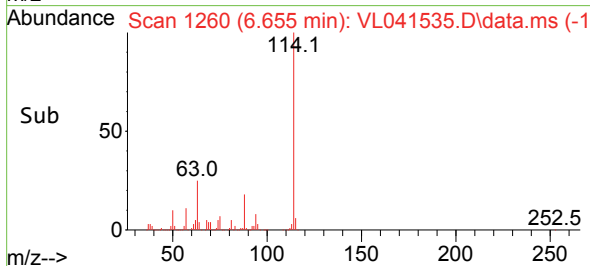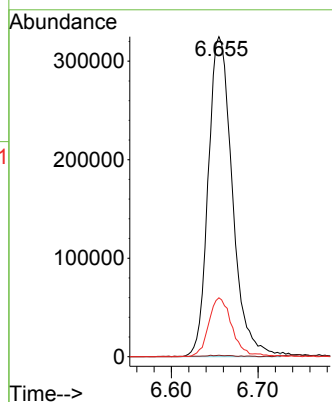

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 11.468 min Scan# 2757

Delta R.T. 0.003 min

Lab File: VL041535.D

Acq: 12 Aug 2024 14:07




Tgt Ion: 117 Resp: 2347282


Ion Ratio Lower Upper

117 100

82 64.1 51.0 76.6


119 33.2 45.2 67.8#

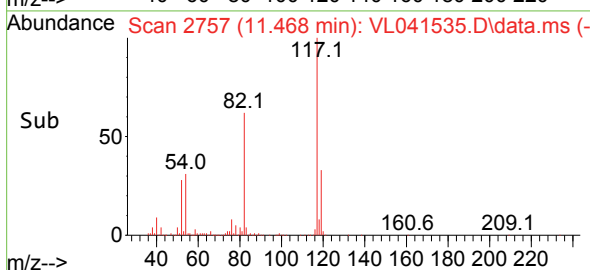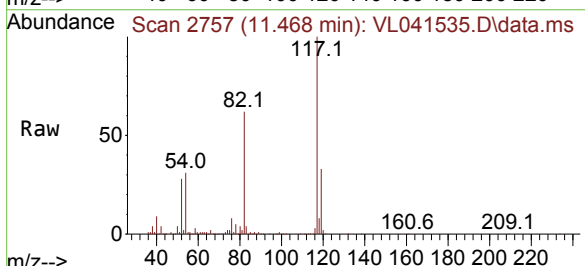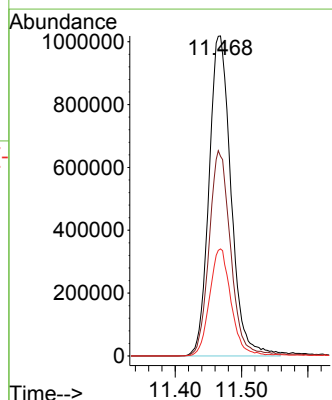

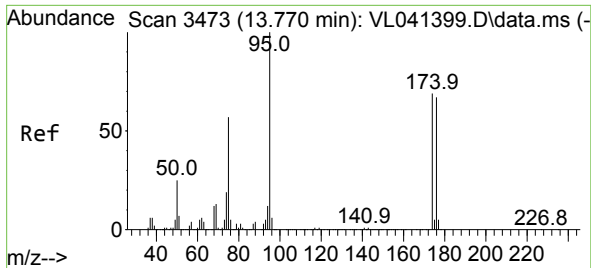

#68  
 1-Bromo-4-Fluorobenzene  
 Concen: 9.742 ppbv  
 RT: 13.777 min Scan# 34  
 Delta R.T. 0.003 min  
 Lab File: VL041535.D  
 Acq: 12 Aug 2024 14:07

Instrument :  
 MSVOA\_L  
 ClientSampleId :

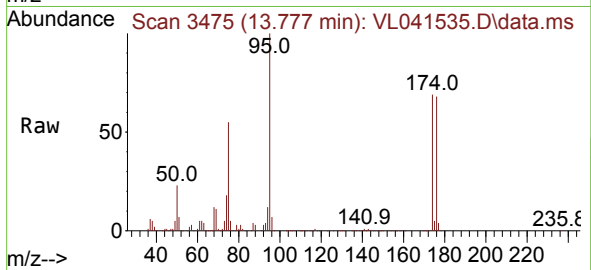

Tgt Ion: 95 Resp: 1759698  

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 95  | 100   |       |       |
| 174 | 71.7  | 56.3  | 84.5  |
| 175 | 4.9   | 4.0   | 6.0   |

