


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL081224\
Data File : VL041526.D
Acq On : 12 Aug 2024 8:07
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Aug 13 02:09:20 2024

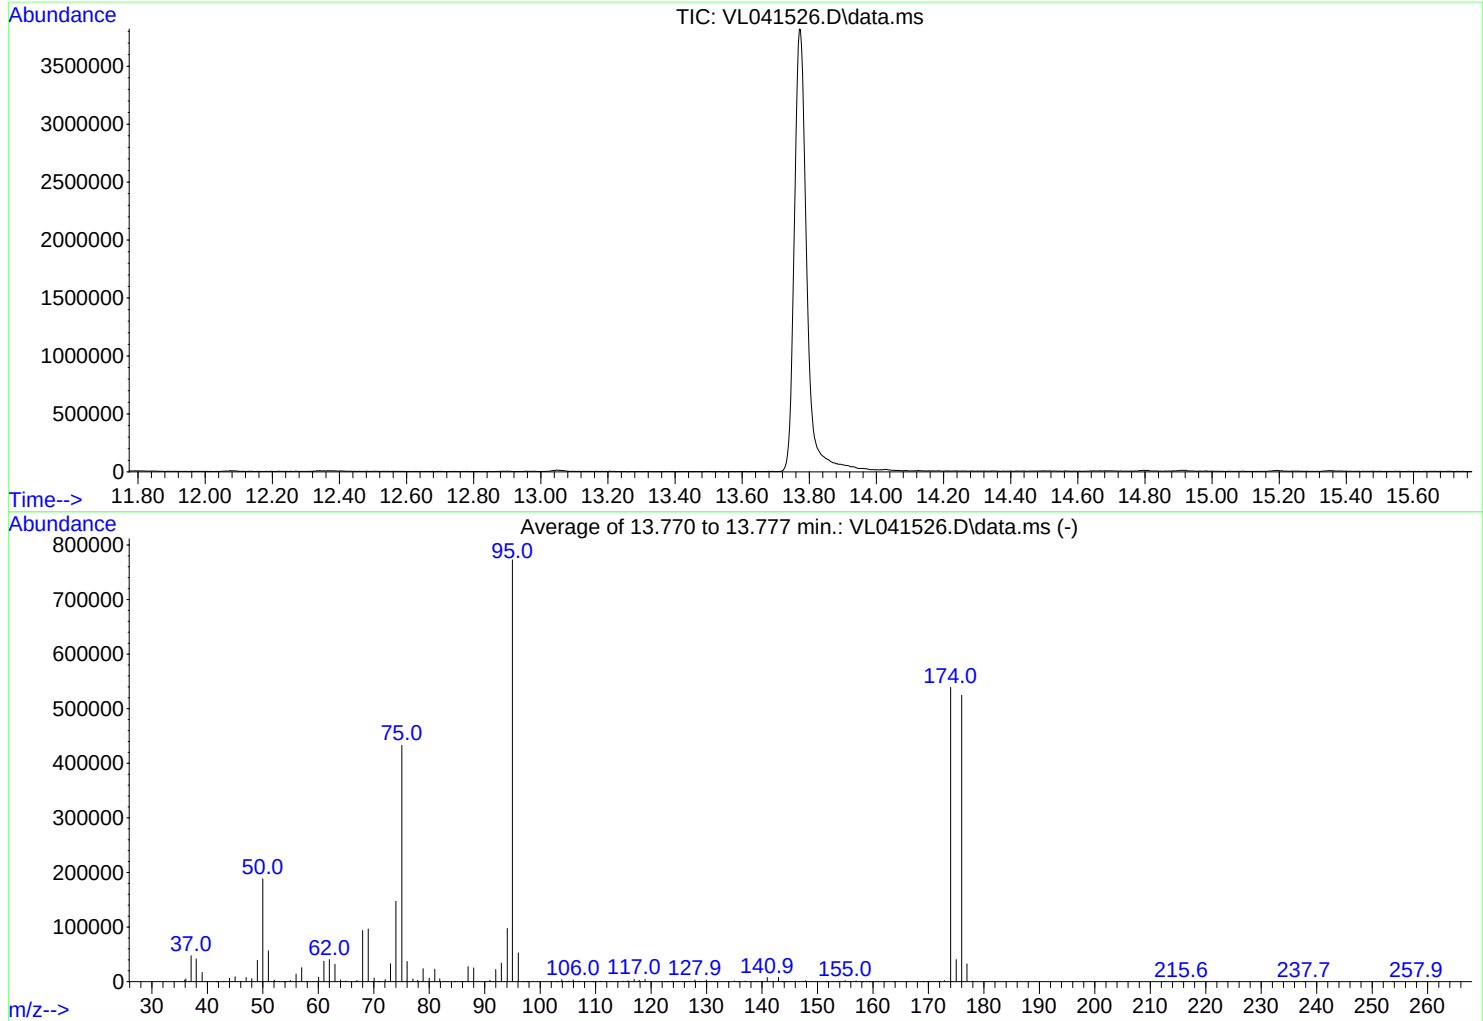

AutoFind: Scans 3473, 3474, 3475; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	188523	PASS
75	95	30	66	56.0	432981	PASS
95	95	100	100	100.0	772672	PASS
96	95	5	9	6.8	52669	PASS
173	174	0.00	2	0.3	1634	PASS
174	95	50	120	69.7	538880	PASS
175	174	4	9	7.5	40432	PASS
176	174	93	101	97.4	524672	PASS
177	176	5	9	6.2	32579	PASS

Average of 13.770 to 13.777 min.: VL041526.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	3000	46.20	243	56.00	14028	66.95	2361
36.10	5109	47.00	7707	57.00	25659	68.00	9357
37.05	47475	48.00	5345	57.95	1005	69.00	9654
38.00	41693	49.00	39083	59.05	219	70.05	685
39.05	16937	50.00	188523	60.05	8336	70.80	87
39.95	566	51.00	56592	61.00	37533	72.05	3776
41.70	51	52.05	2704	62.00	40483	73.00	32720
42.95	468	53.00	279	63.00	31949	74.00	147157
44.00	6179	53.80	114	64.00	3355	75.05	432981
45.00	8964	54.00	79	64.95	1105	76.00	37045
45.95	568	54.95	2226	65.95	165	77.05	5100

Average of 13.770 to 13.777 min.: VL041526.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.90	2567	88.00	25349	103.90	3441	112.80	504
78.90	23819	90.95	2679	104.80	346	114.95	779
80.00	6457	92.00	22192	105.10	772	115.80	1697
81.00	22997	93.00	34067	105.95	3331	116.00	909
81.90	5209	94.05	97219	107.00	862	116.95	4234
82.75	295	95.00	772672	107.90	117	117.85	2452
83.05	425	96.05	52669	109.50	66	118.90	4164
84.60	70	96.90	719	110.00	346	120.05	166
85.85	626	97.10	571	110.85	749	122.40	57
86.15	472	97.70	58	111.10	168	123.00	144
87.00	27704	103.00	63	111.85	1022	123.70	153

Average of 13.770 to 13.777 min.: VL041526.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.05	452	130.95	544	142.00	851	148.95	595
124.65	242	131.60	69	142.95	7496	149.70	223
125.05	251	132.05	186	143.70	98	150.05	667
125.75	320	133.90	81	143.90	468	151.60	119
126.20	128	135.05	1154	144.20	72	151.95	362
126.90	349	135.60	118	145.00	625	152.80	351
127.90	2943	135.85	209	145.20	270	153.50	168
128.75	807	136.95	1132	145.80	332	153.85	613
129.10	314	139.00	481	146.05	889	155.00	2051
129.95	2900	140.00	752	146.70	600	155.80	415
130.80	394	140.95	7780	147.85	1686	156.95	1526

Average of 13.770 to 13.777 min.: VL041526.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.75	240	169.80	112	177.95	959		
158.10	66	170.20	236	215.60	89		
158.85	771	170.45	436	237.70	51		
159.30	117	170.90	199	253.70	72		
159.80	69	171.85	973	257.95	136		
160.60	200	172.10	719				
160.95	765	172.90	1634				
163.80	88	174.00	538880				
166.30	175	175.00	40432				
168.60	223	176.00	524672				
169.05	122	176.95	32579				