

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL081325\
 Data File : VL042857.D
 Acq On : 13 Aug 2025 18:21
 Operator : SY/MD
 Sample : Q2794-01DL 10X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 IA1DL

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2025
 Supervised By :Mahesh Dadoda 08/18/2025

Quant Time: Aug 14 02:19:57 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL081325AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 14 2025

QLast Update : Thu Aug 14 02:12:54 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.800	49	132826	10.000	ppbv	0.01
33) 1,4-Difluorobenzene	3.975	114	406342	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.898	117	347245	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.390	95	260346	9.997	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	100.000%
Target Compounds						
					Qvalue	
9) Propene	1.493	41	1690m	0.182	ppbv	
10) Heptane	5.001	43	4291m	0.172	ppbv	
13) Ethanol	1.726	45	158844	186.947	ppbv	93
15) Acetone	1.842	43	61695	3.511	ppbv	98
19) Isopropyl Alcohol	1.894	45	71252	6.789	ppbv #	37
25) Ethyl Acetate	2.852	43	16896	0.397	ppbv #	90
26) Hexane	2.836	57	4508	0.230	ppbv #	18
30) Cyclohexane	3.878	84	2051m	0.119	ppbv	
34) 2-Butanone	2.574	43	4200m	0.153	ppbv	
36) Benzene	3.674	78	4851	0.125	ppbv #	89
44) 2,2,4-Trimethylpentane	4.658	57	15104m	0.229	ppbv	
53) Toluene	6.956	91	46683	1.009	ppbv	97
58) Ethyl Benzene	9.371	91	9634	0.157	ppbv	90
59) m/p-Xylene	9.549	91	22807	0.475	ppbv #	100
60) o-Xylene	9.982	91	9054	0.187	ppbv	98
74) 1,2,4-Trimethylbenzene	11.549	105	8568	0.157	ppbv #	62

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL081325\
Data File : VL042857.D
Acq On : 13 Aug 2025 18:21
Operator : SY/MD
Sample : Q2794-01DL 10X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
IA1DL

Quant Time: Aug 14 02:19:57 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL081325AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Thu Aug 14 02:12:54 2025
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 08/14/2025
Supervised By : Mahesh Dadoda 08/18/2025

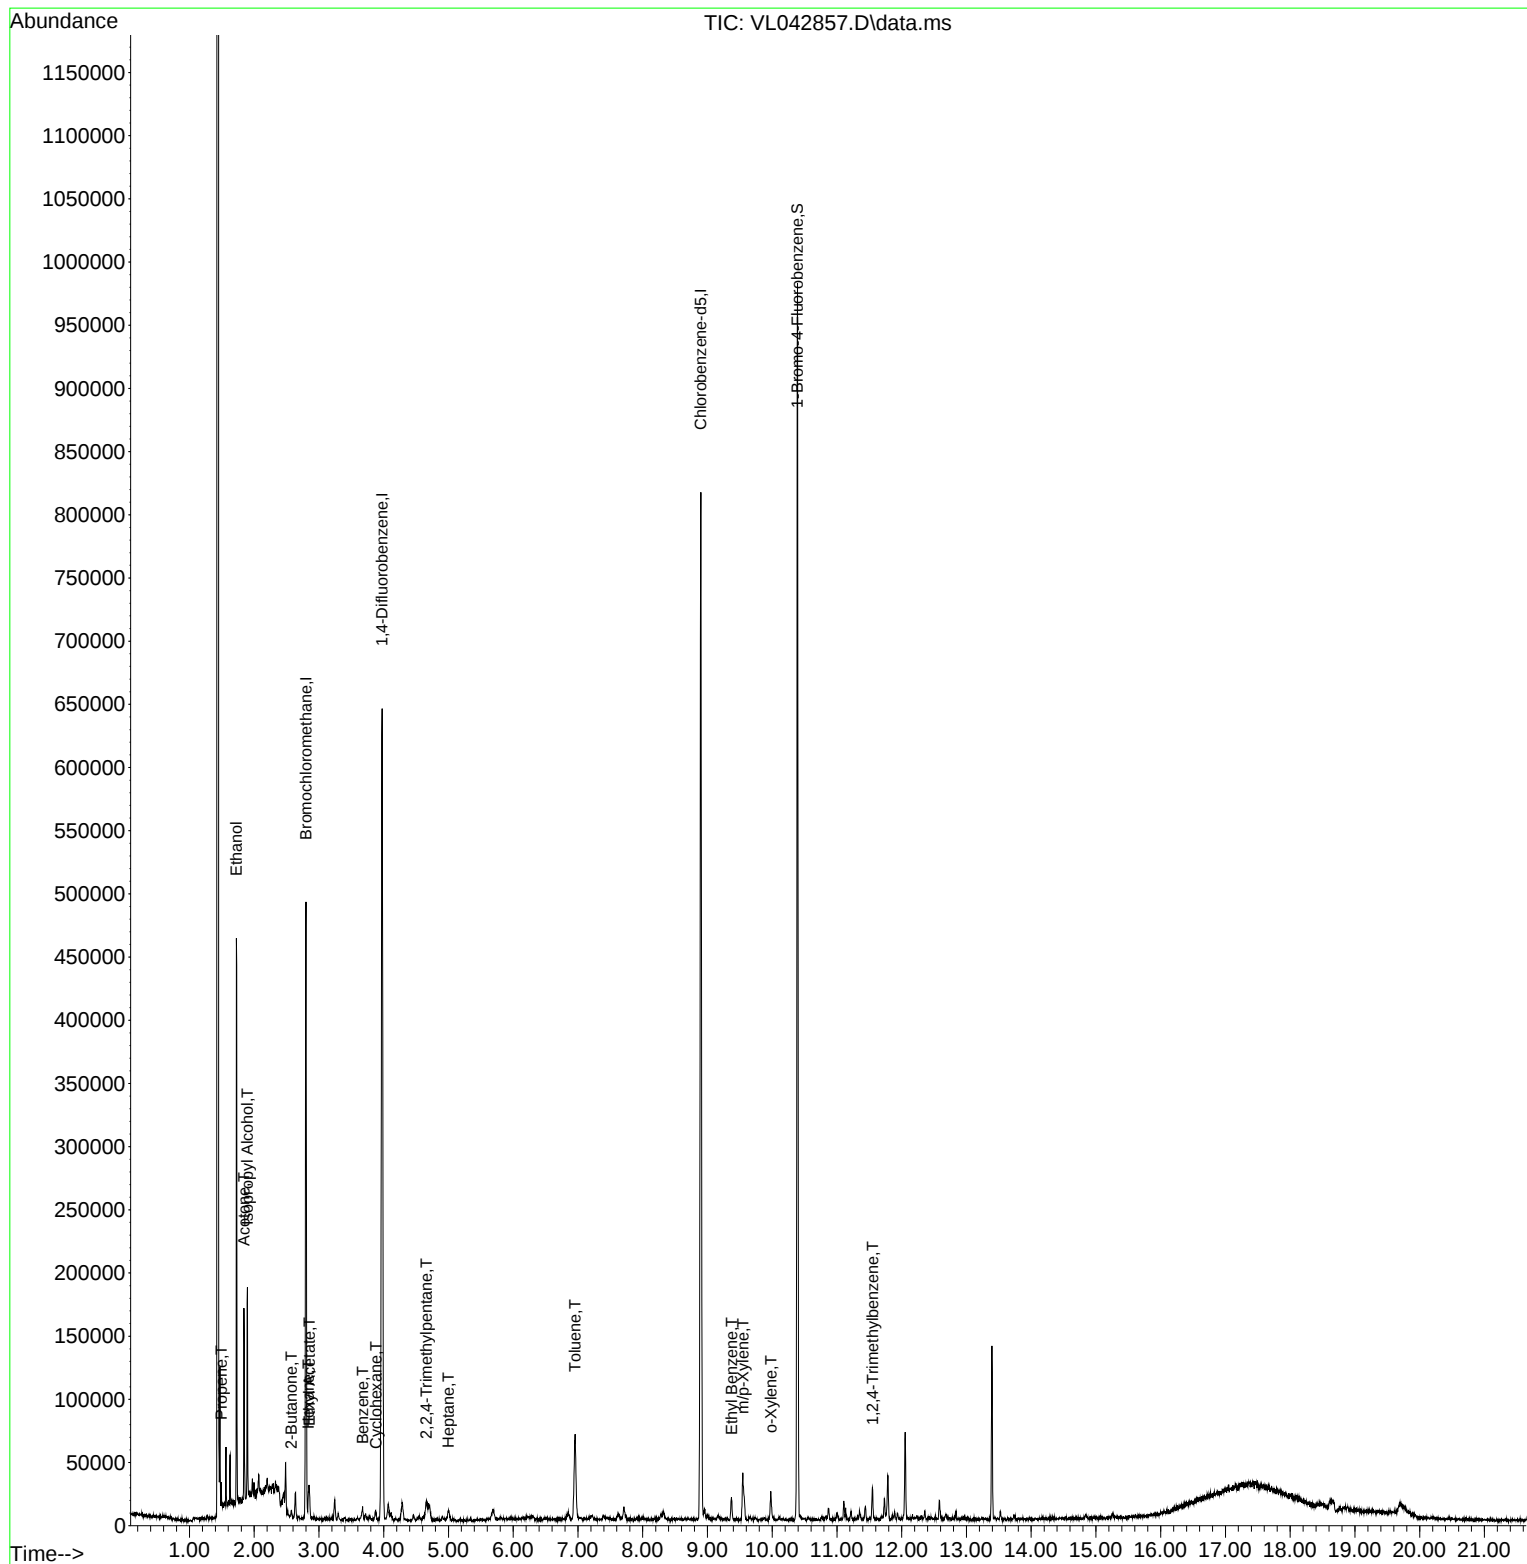



#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.800 min Scan# 81
Delta R.T. 0.010 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21




Instrument :
MSVOA_L
ClientSampleId :
IA1DL



Tgt Ion: 49 Resp: 132820
Ion Ratio Lower Upper
49 100
128 47.0 23.7 71.1
130 60.1 30.6 91.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/14/2025
Supervised By :Mahesh Dadoda 08/18/2025

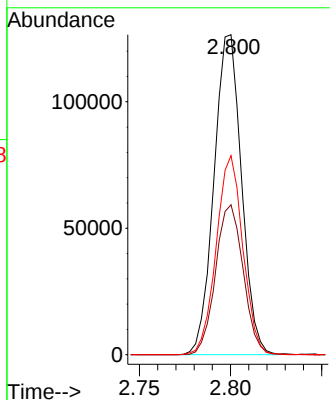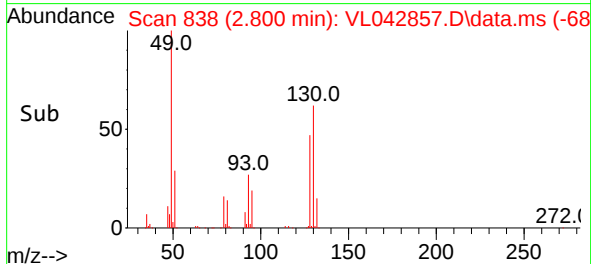

#9
Propene
Concen: 0.182 ppbv m
RT: 1.493 min Scan# 434
Delta R.T. 0.007 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21


Tgt Ion: 41 Resp: 1690
Ion Ratio Lower Upper
41 100
42 172.8 53.0 79.4#

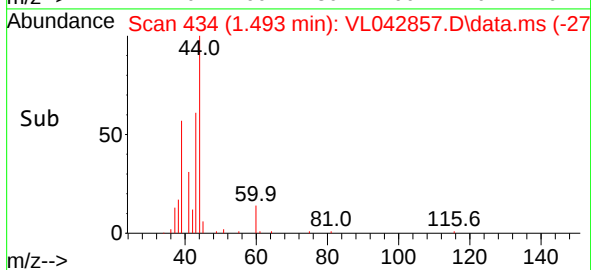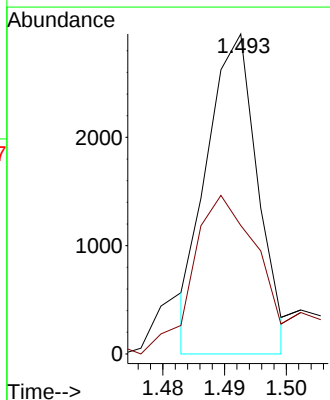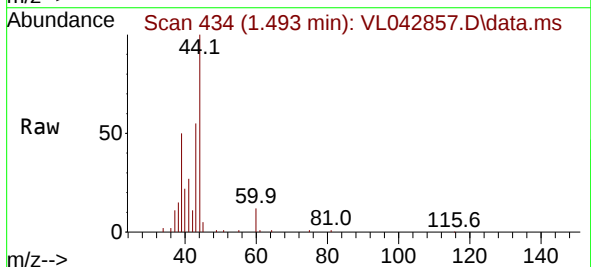



#10
Heptane
Concen: 0.172 ppbv m
RT: 5.001 min Scan# 11
Delta R.T. 0.013 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21




Instrument :
MSVOA_L
ClientSampleId :
IA1DL



Tgt Ion: 43 Resp: 429
Ion Ratio Lower Upper
43 100
57 48.0 41.4 62.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/14/2025
Supervised By :Mahesh Dadoda 08/18/2025

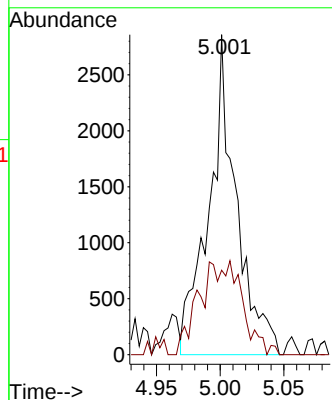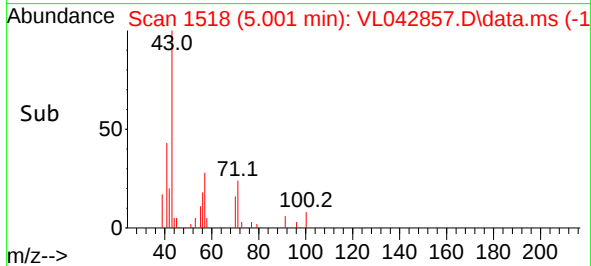

#13
Ethanol
Concen: 186.947 ppbv
RT: 1.726 min Scan# 506
Delta R.T. 0.003 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21

Tgt Ion: 45 Resp: 158844
Ion Ratio Lower Upper
45 100
46 38.9 17.5 69.9

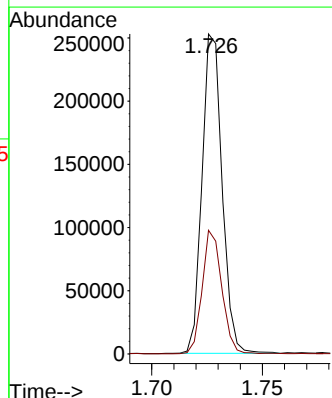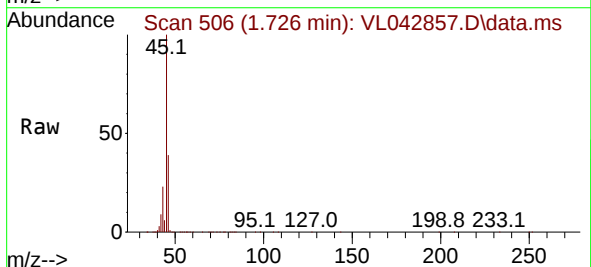







#15
Acetone
Concen: 3.511 ppbv
RT: 1.842 min Scan# 541
Delta R.T. 0.003 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21

Instrument :
MSVOA_L
ClientSampleId :
IA1DL

Tgt Ion: 43 Resp: 6169
Ion Ratio Lower Upper
43 100
58 26.8 22.4 33.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/14/2025
Supervised By :Mahesh Dadoda 08/18/2025

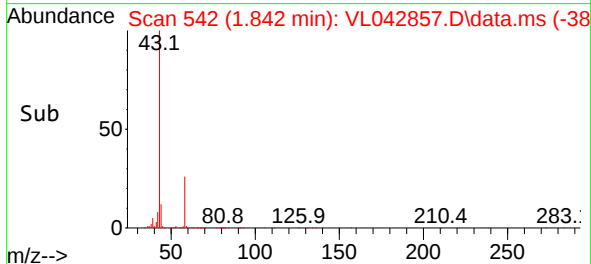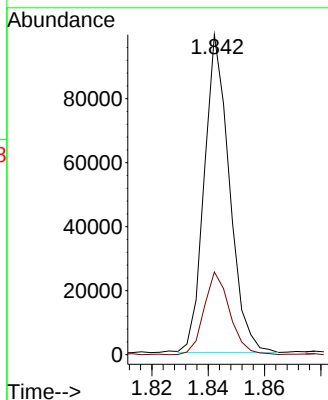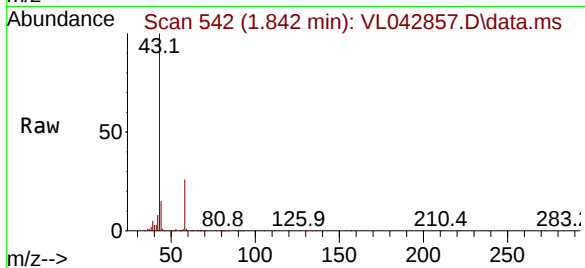

#19
Isopropyl Alcohol
Concen: 6.789 ppbv
RT: 1.894 min Scan# 558
Delta R.T. 0.007 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21


Tgt Ion: 45 Resp: 71252
Ion Ratio Lower Upper
45 100
58 1.3 32.7 49.1#

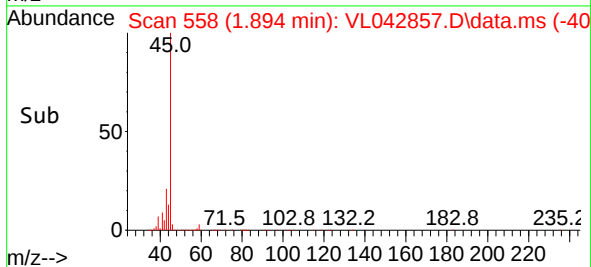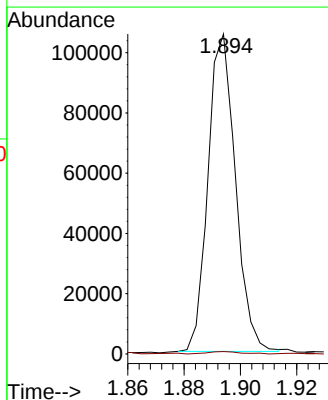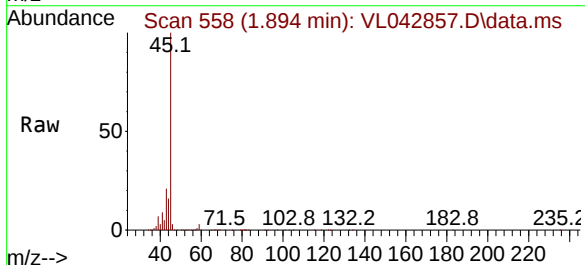



#25
Ethyl Acetate
Concen: 0.397 ppbv
RT: 2.852 min Scan# 81
Delta R.T. 0.013 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21




Instrument :
MSVOA_L
ClientSampleId :
IA1DL




Tgt Ion: 43 Resp: 16890
Ion Ratio Lower Upper
43 100
45 15.4 8.1 12.1
61 13.2 7.4 11.2
70 10.8 7.3 10.9

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 08/14/2025
Supervised By :Mahesh Dadoda 08/18/2025

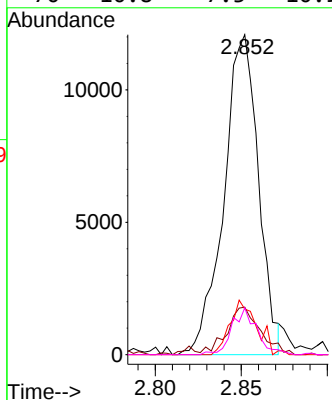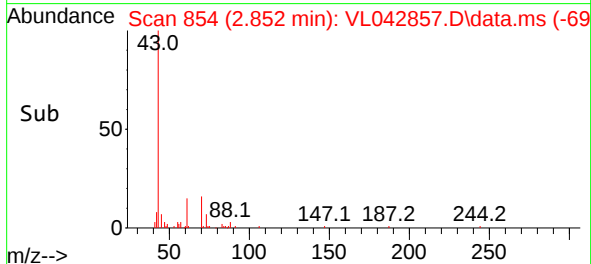


#26
Hexane
Concen: 0.230 ppbv
RT: 2.836 min Scan# 849
Delta R.T. 0.007 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21

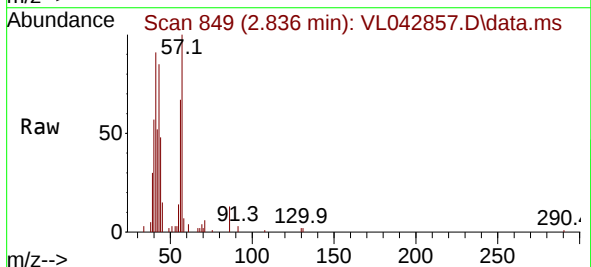


Tgt Ion: 57 Resp: 4508
Ion Ratio Lower Upper
57 100
41 118.4 68.6 103.0#
43 398.0 168.5 252.7#
56 57.4 41.5 62.3

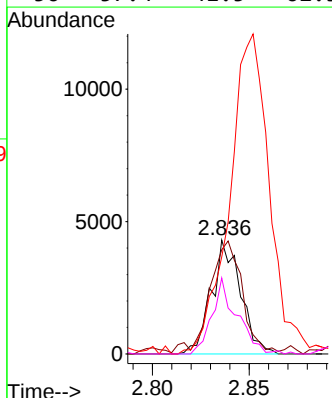

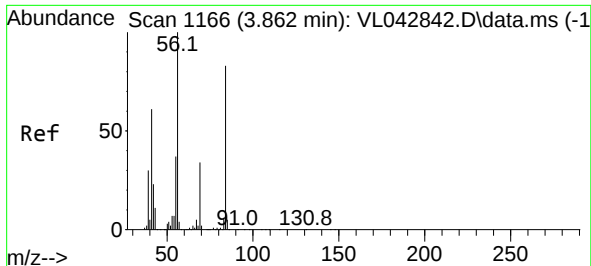

#30
Cyclohexane
Concen: 0.119 ppbv m
RT: 3.878 min Scan# 1166
Delta R.T. 0.016 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21




Instrument :
MSVOA_L
ClientSampleId :
IA1DL



Tgt Ion: 84 Resp: 205
Ion Ratio Lower Upper
84 100
56 126.0 98.8 148.2
41 99.7 61.3 91.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/14/2025
Supervised By :Mahesh Dadoda 08/18/2025

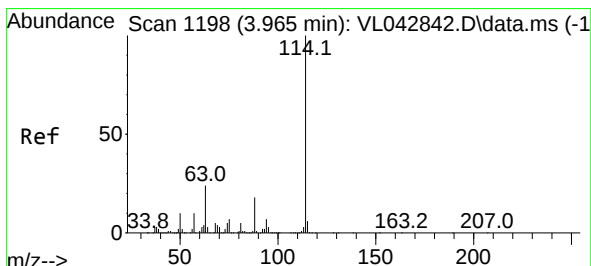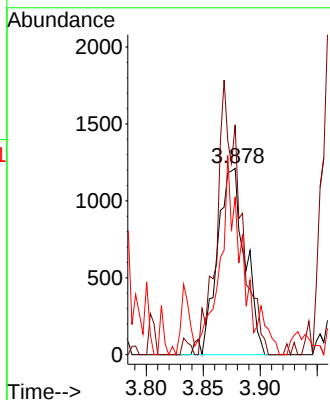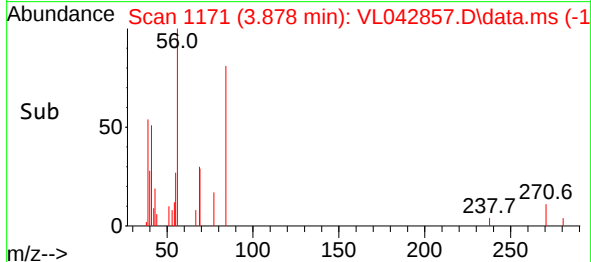

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.975 min Scan# 1201
Delta R.T. 0.010 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21


Tgt Ion:114 Resp: 406342
Ion Ratio Lower Upper
114 100
63 24.6 19.7 29.5
88 17.9 14.4 21.6

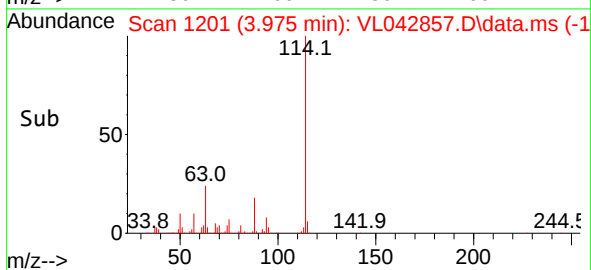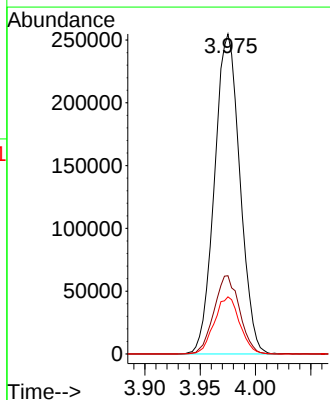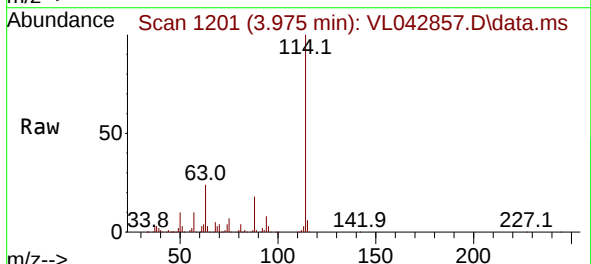

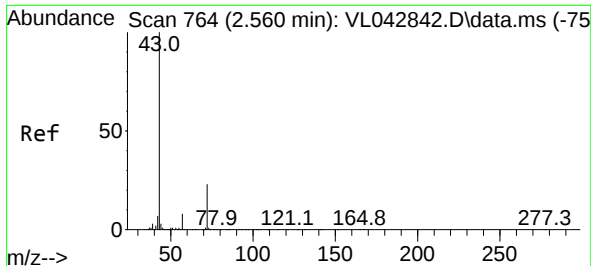

#34
2-Butanone
Concen: 0.153 ppbv m
RT: 2.574 min Scan# 764
Delta R.T. 0.013 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21




Instrument :
MSVOA_L
ClientSampleId :
IA1DL

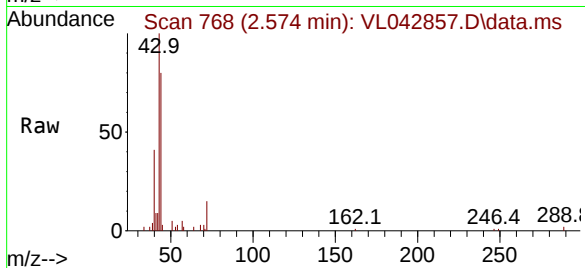


Tgt Ion: 43 Resp: 4200
Ion Ratio Lower Upper
43 100
72 13.1 18.6 28.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 08/14/2025
Supervised By :Mahesh Dadoda 08/18/2025

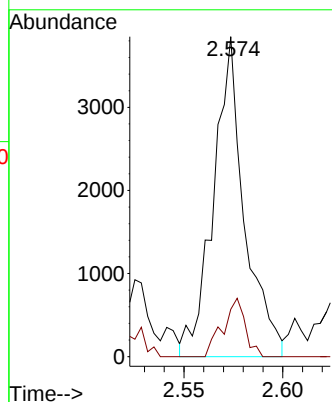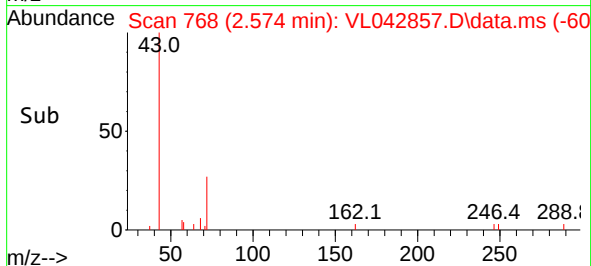


#36
Benzene
Concen: 0.125 ppbv
RT: 3.674 min Scan# 1108
Delta R.T. 0.010 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21

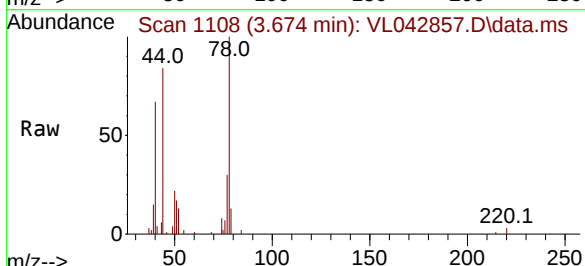

Tgt Ion: 78 Resp: 4851
Ion Ratio Lower Upper
78 100
77 29.7 17.7 26.5
50 19.5 13.9 20.9

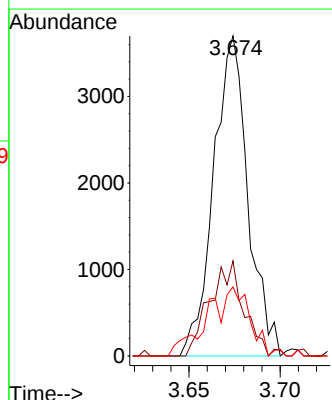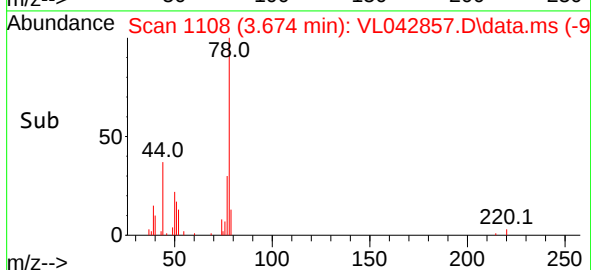

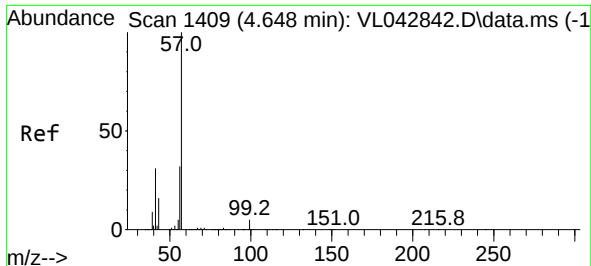

#44

2,2,4-Trimethylpentane

Concen: 0.229 ppbv

RT: 4.658 min Scan# 1409

Delta R.T. 0.010 min

Lab File: VL042857.D

Acq: 13 Aug 2025 18:21

Instrument :

MSVOA_L

ClientSampleId :

IA1DL





Tgt Ion:	57	Resp:	15104
Ion	Ratio	Lower	Upper
57	100		
41	43.7	24.8	37.2
56	32.8	25.5	38.3

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2025

Supervised By :Mahesh Dadoda 08/18/2025

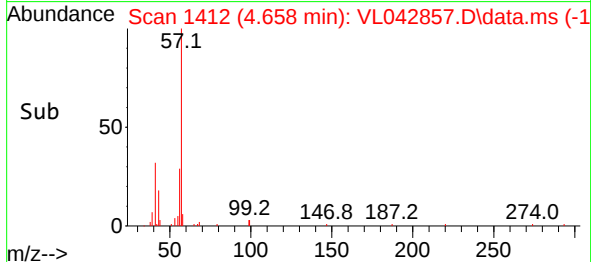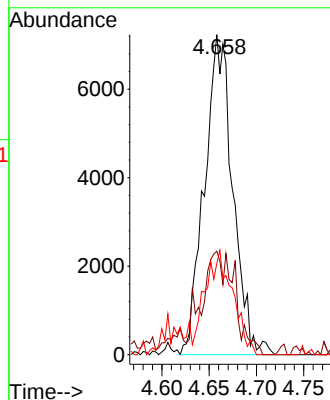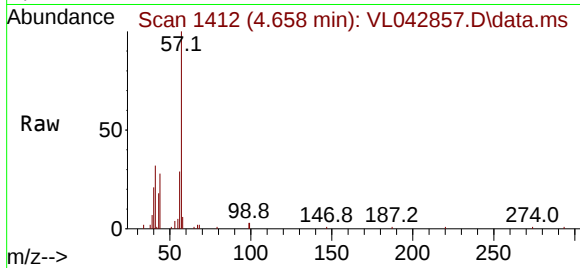

#53

Toluene

Concen: 1.009 ppbv




RT: 6.956 min Scan# 2122


Delta R.T. 0.013 min

Lab File: VL042857.D

Acq: 13 Aug 2025 18:21


Tgt Ion:	91	Resp:	46683
Ion	Ratio	Lower	Upper
91	100		
92	62.1	47.8	71.6

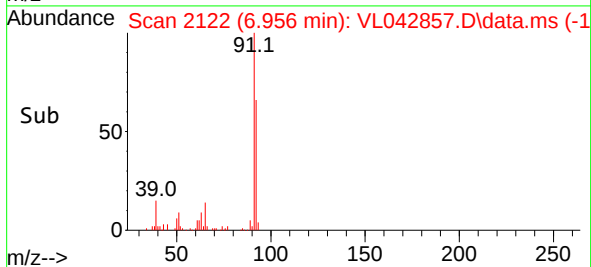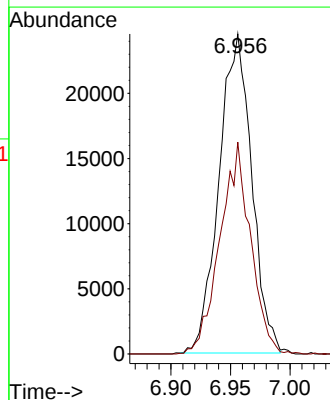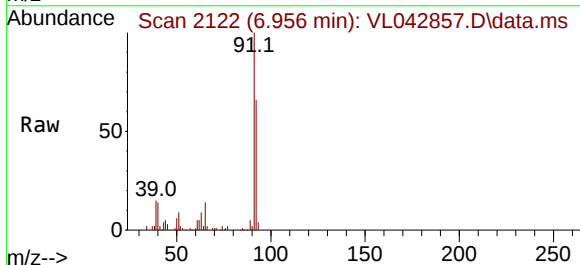



#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.898 min Scan# 2719
Delta R.T. 0.010 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21




Instrument :
MSVOA_L
ClientSampleId :
IA1DL



Tgt Ion:117 Resp: 347249
Ion Ratio Lower Upper
117 100
82 65.1 54.6 81.8
119 31.7 25.9 38.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/14/2025
Supervised By :Mahesh Dadoda 08/18/2025

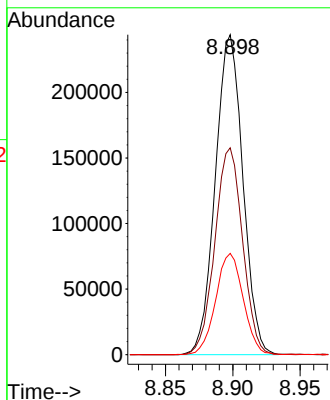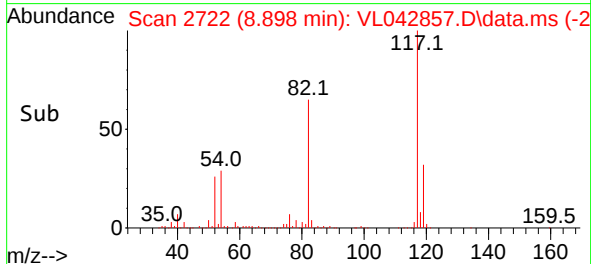

#58
Ethyl Benzene
Concen: 0.157 ppbv
RT: 9.371 min Scan# 2868
Delta R.T. 0.007 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21

Tgt Ion: 91 Resp: 9634
Ion Ratio Lower Upper
91 100
106 35.4 23.9 35.9

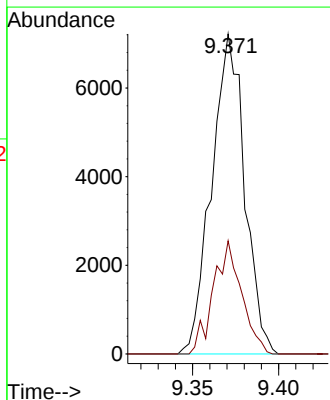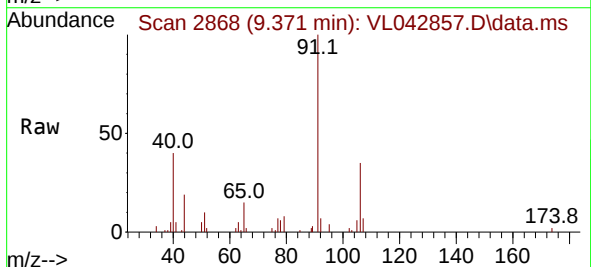







#59
m/p-Xylene
Concen: 0.475 ppbv
RT: 9.549 min Scan# 2921
Delta R.T. 0.007 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21

Instrument :
MSVOA_L
ClientSampleId :
IA1DL

Tgt Ion: 91 Resp: 2280
Ion Ratio Lower Upper
91 100
106 47.3 0.0 0.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/14/2025
Supervised By :Mahesh Dadoda 08/18/2025

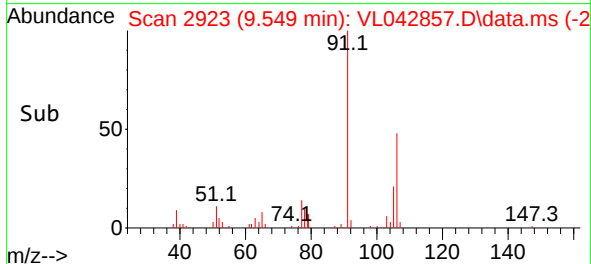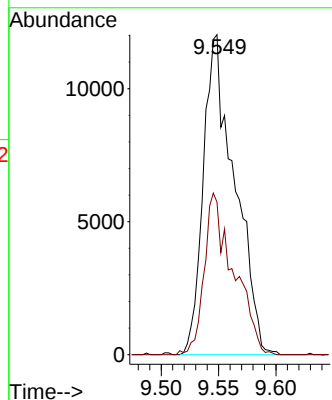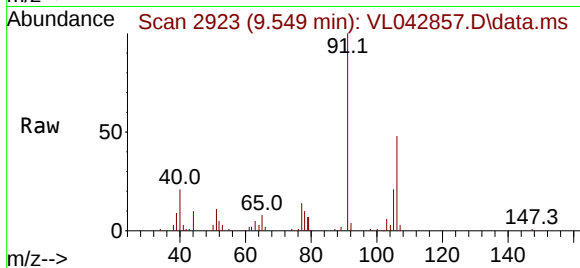

#60
o-Xylene
Concen: 0.187 ppbv
RT: 9.982 min Scan# 3057
Delta R.T. 0.010 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21


Tgt Ion: 91 Resp: 9054
Ion Ratio Lower Upper
91 100
106 45.0 21.8 65.4

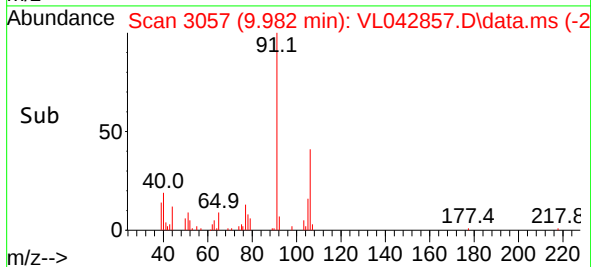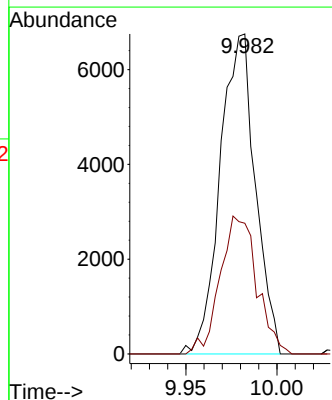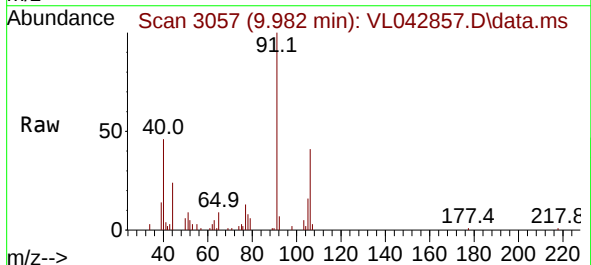

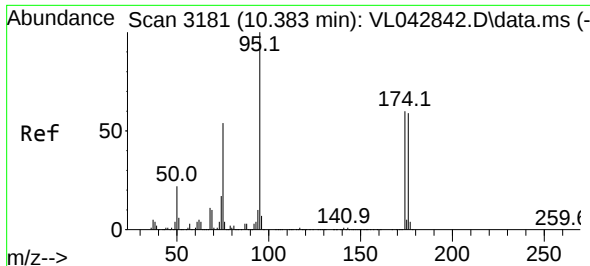

#68
1-Bromo-4-Fluorobenzene
Concen: 9.997 ppbv
RT: 10.390 min Scan# 3181
Delta R.T. 0.007 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21




Instrument :
MSVOA_L
ClientSampleId :
IA1DL

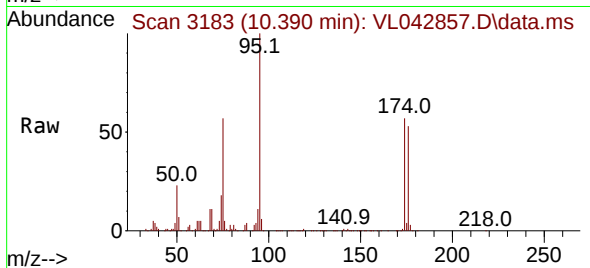

Tgt Ion: 95 Resp: 260340
Ion Ratio Lower Upper
95 100
174 57.4 48.4 72.6
175 4.2 3.8 5.8

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 08/14/2025
Supervised By :Mahesh Dadoda 08/18/2025

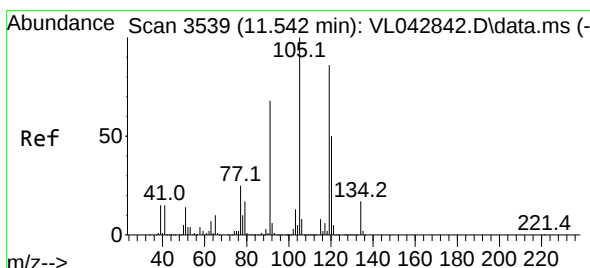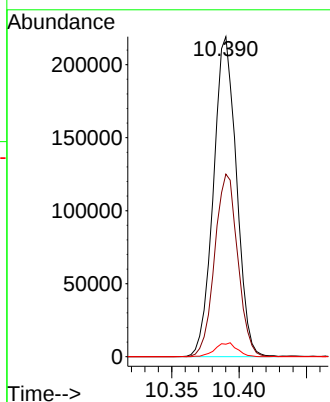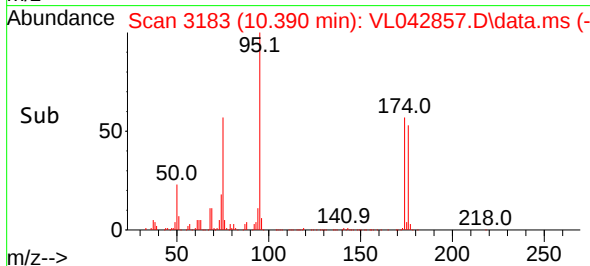

#74
1,2,4-Trimethylbenzene
Concen: 0.157 ppbv
RT: 11.549 min Scan# 3541
Delta R.T. 0.007 min
Lab File: VL042857.D
Acq: 13 Aug 2025 18:21

Tgt Ion:105 Resp: 8568
Ion Ratio Lower Upper
105 100
120 46.8 39.8 59.6
91 12.9 54.2 81.4#
77 12.6 19.8 29.6#

