

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL081518\
 Data File : VL032367.D
 Acq On : 16 Aug 2018 1:51
 Operator : SY/AP
 Sample : J4457-03
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SG06-MIVI

Manual Integrations
 APPROVED

apatel
 8/20/2018 5:03:32 PM

Quant Time: Aug 16 22:23:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL081518AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Aug 16 2018
 QLast Update : Wed Aug 15 14:58:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.84	49	1551266	10.00	ppbv	0.02
33) 1,4-Difluorobenzene	7.39	114	2297078	10.00	ppbv	0.04
55) Chlorobenzene-d5	12.33	117	3745267	10.00	ppbv	0.02

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
68) 1-Bromo-4-Fluorobenzene		14.66	95	3254576	11.39	ppbv	0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	113.90%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
4) Chloromethane	3.21	50	138122	1.62	ppbv	95
9) Propene	3.06	41	17692276	287.68	ppbv	89
10) Heptane	8.37	43	29870052	161.25	ppbv #	81
11) Trichlorofluoromethane	4.06	101	35836	0.21	ppbv	84
13) Ethanol	3.70	45	1774945	112.37	ppbv	95
15) Acetone	3.94	43	27173757m	184.37	ppbv	
20) Methylene Chloride	4.49	84	335865	6.03	ppbv #	95
26) Hexane	5.87	57	35189675m	249.91	ppbv	
27) Carbon Disulfide	4.69	76	4456527	33.91	ppbv	99
30) Cyclohexane	7.36	84	31463432	293.34	ppbv #	82
34) 2-Butanone	5.40	43	17674436	113.05	ppbv #	86
35) Carbon Tetrachloride	7.23	117	29799m	0.22	ppbv	
36) Benzene	7.10	78	20975647	107.71	ppbv #	79
52) Tetrachloroethene	11.47	164	247983	4.32	ppbv	91
53) Toluene	10.04	91	34216314m	160.28	ppbv	
58) Ethyl Benzene	12.96	91	17734442	39.36	ppbv #	86
59) m/p-Xylene	13.22	91	26712563	69.79	ppbv	90
60) o-Xylene	13.94	91	10593159	28.16	ppbv	97
62) Isopropylbenzene	14.91	105	1658760	3.10	ppbv	98
64) n-propylbenzene	15.81	120	553497	3.99	ppbv	95
67) sec-Butylbenzene	17.54	105	600521	0.88	ppbv	99
69) p-Isopropyltoluene	17.89	119	346237m	0.67	ppbv	
70) n-Butylbenzene	18.79	91	358119	0.63	ppbv #	38
72) 4-Ethyltoluene	16.08	105	2997556	7.14	ppbv	99
73) 1,3,5-Trimethylbenzene	16.24	105	2291785	5.68	ppbv	98
74) 1,2,4-Trimethylbenzene	17.01	105	3871857	9.02	ppbv #	71
79) Naphthalene	22.49	128	131547	0.64	ppbv	99
80) Naphthalene,2-methyl-	25.17	142	31022	0.36	ppbv	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL081518\
Data File : VL032367.D
Acq On : 16 Aug 2018 1:51
Operator : SY/AP
Sample : J4457-03
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
SG06-MIVI

Manual Integrations
APPROVED

apatel
8/20/2018 5:03:32 PM

Quant Time: Aug 16 22:23:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL081518AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Aug
QLast Update : Wed Aug 15 14:58:02 2018
Response via : Initial Calibration

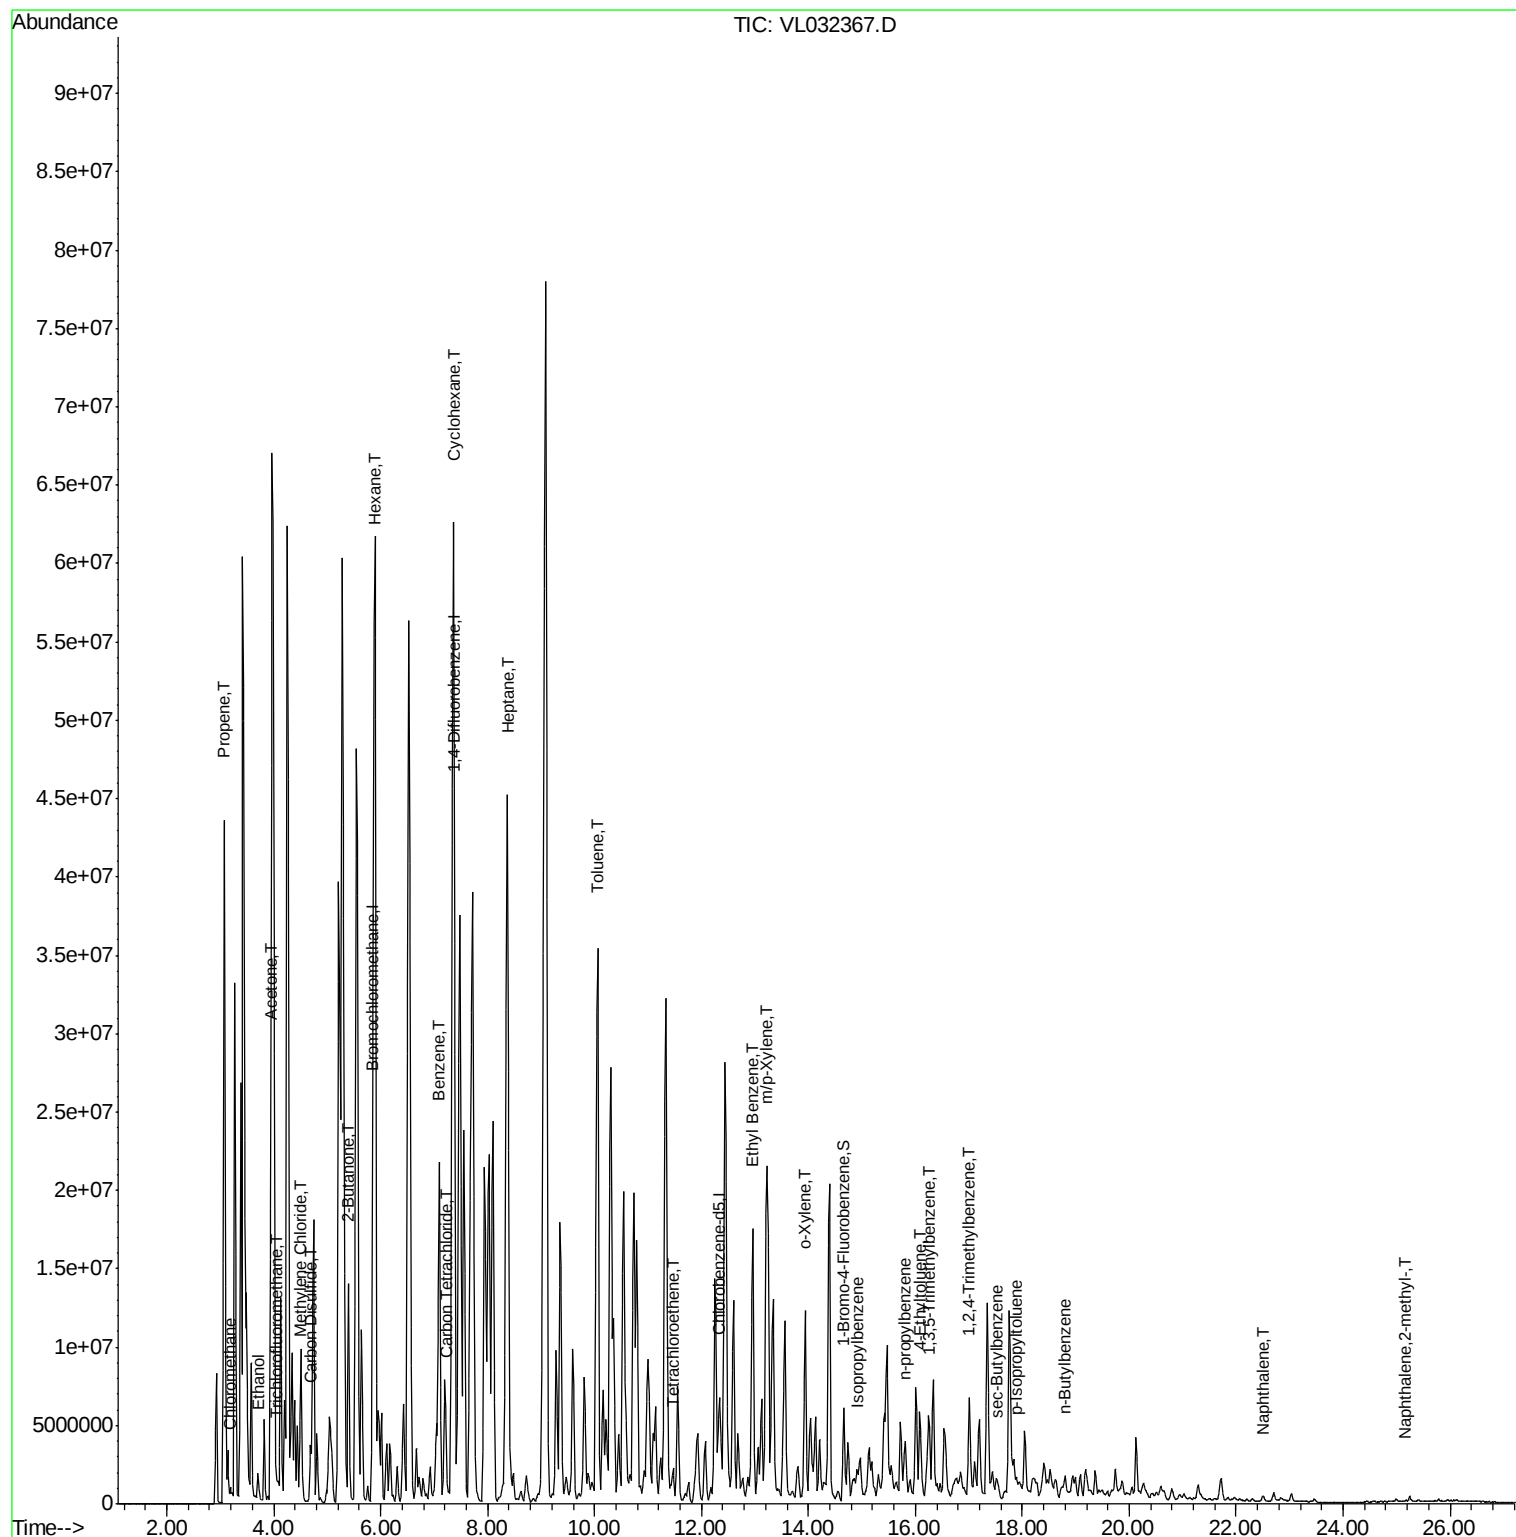



#1





Bromochloromethane
 Concen: 10.00 ppbv
 RT: 5.84 min Scan# 1478
 Delta R.T. 0.02 min
 Lab File: VL032367.D
 Acq: 16 Aug 2018 1:51

Instrument :
 MSVOA_L
 ClientSampleId :
 SG06-MIVI

Tot Ion	Ratio	Lower	Upper
49	100		
128	41.2	20.5	61.6
130	53.2	26.2	78.5

Manual Integrations
 APPROVED




apatel
 8/20/2018 5:03:32 PM

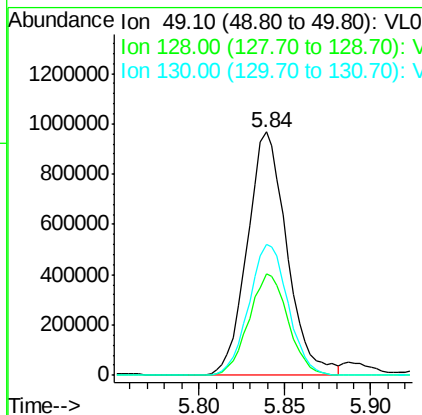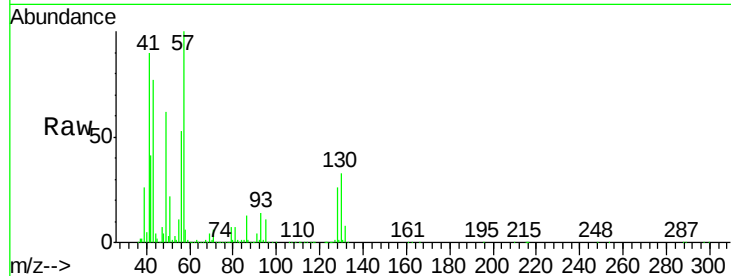


#4

Chloromethane
 Concen: 1.62 ppbv
 RT: 3.21 min Scan# 659
 Delta R.T. -0.00 min
 Lab File: VL032367.D
 Acq: 16 Aug 2018 1:51

Tgt Ion	Ratio	Lower	Upper
50	100		
52	30.8	26.8	40.2

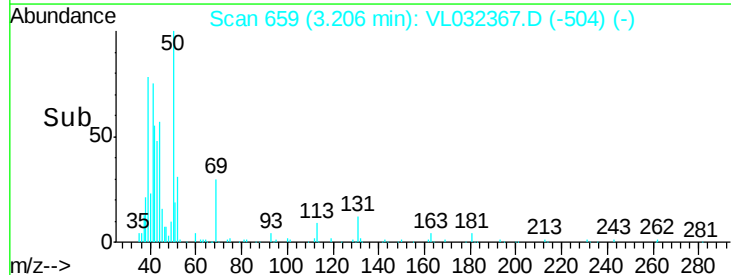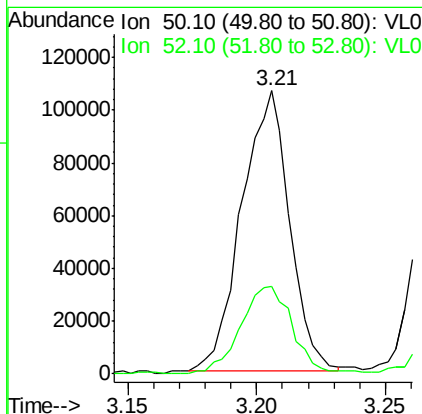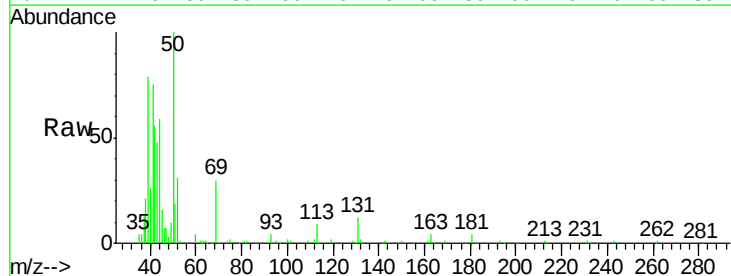







#9
 Propene
 Concen: 287.68 ppbv
 RT: 3.06 min Scan# 615
 Delta R.T. -0.01 min
 Lab File: VL032367.D
 Acq: 16 Aug 2018 1:51

Instrument :
 MSVOA_L
 ClientSampleId :
 SG06-MIVI

Tot Ion: 41 Resp:17692276
 Ion Ratio Lower Upper
 41 100
 42 60.6 55.9 83.9




Manual Integrations
 APPROVED


apatel
 8/20/2018 5:03:32 PM

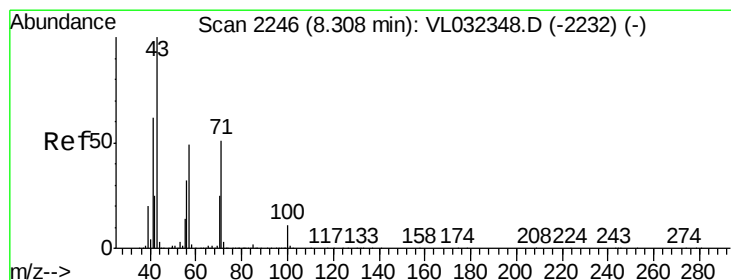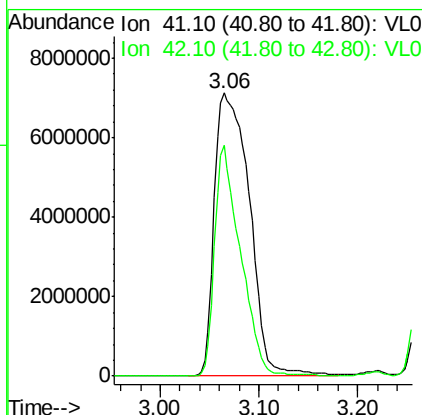

#10
 Heptane
 Concen: 161.25 ppbv
 RT: 8.37 min Scan# 2264
 Delta R.T. 0.06 min
 Lab File: VL032367.D
 Acq: 16 Aug 2018 1:51

Tgt Ion: 43 Resp:29870052
 Ion Ratio Lower Upper
 43 100
 57 62.2 39.5 59.3#

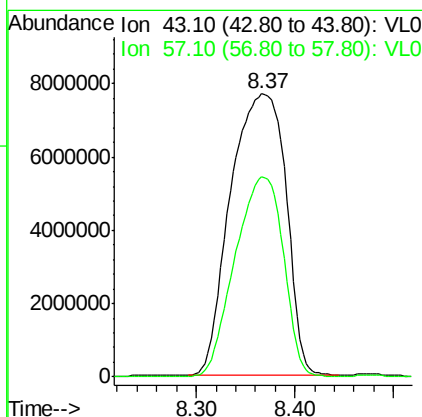

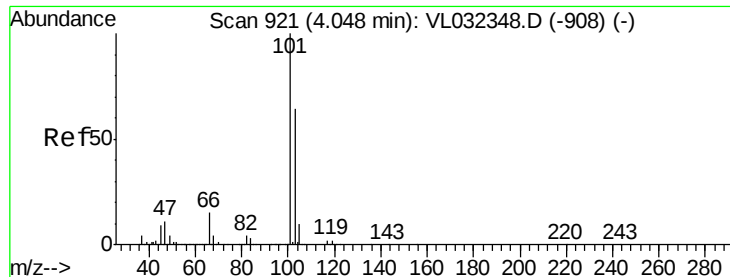





#11
Trichlorofluoromethane
Concen: 0.21 ppbv
RT: 4.06 min Scan# 926
Delta R.T. 0.02 min
Lab File: VL032367.D
Acq: 16 Aug 2018 1:51

Instrument :
MSVOA_L
ClientSampleId :
SG06-MIVI

Tot Ion	Ratio	Lower	Upper
101	100		
103	76.4	51.4	77.0




Manual Integrations
APPROVED


apatel
8/20/2018 5:03:32 PM

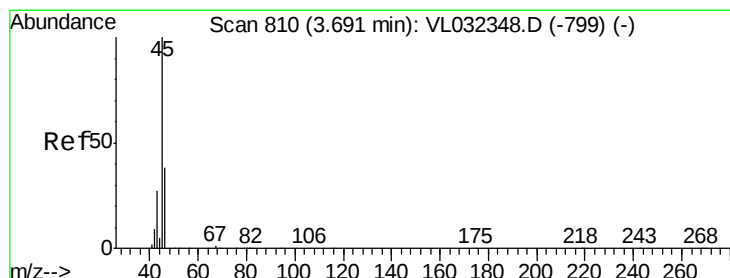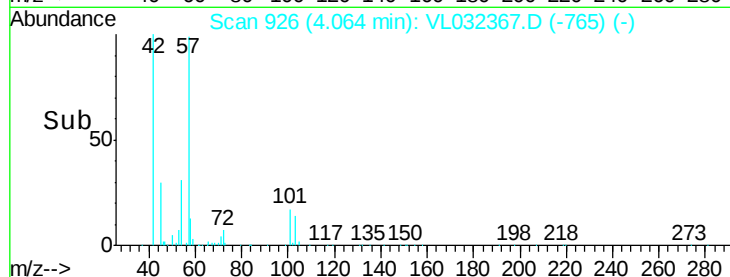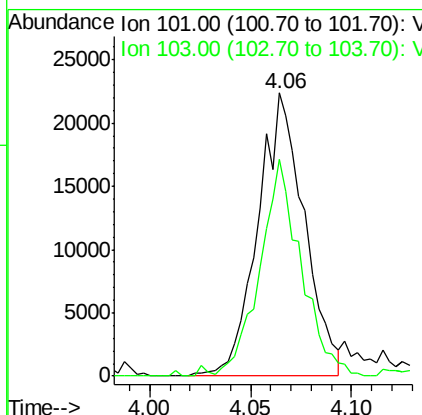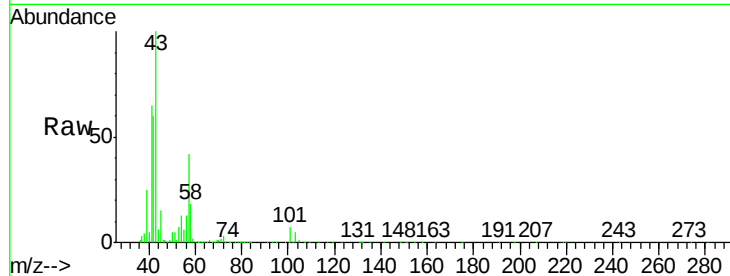

#13
Ethanol
Concen: 112.37 ppbv
RT: 3.70 min Scan# 814
Delta R.T. 0.01 min
Lab File: VL032367.D
Acq: 16 Aug 2018 1:51

Tgt Ion	Ratio	Lower	Upper
45	100		
46	36.2	15.6	62.4

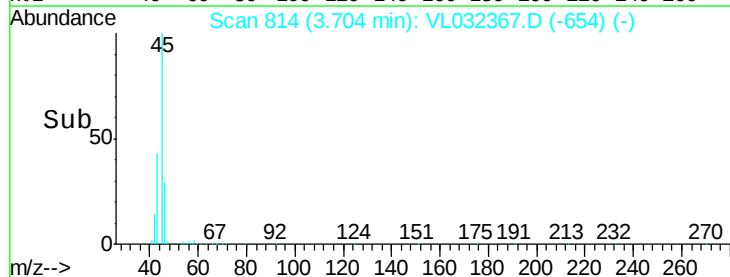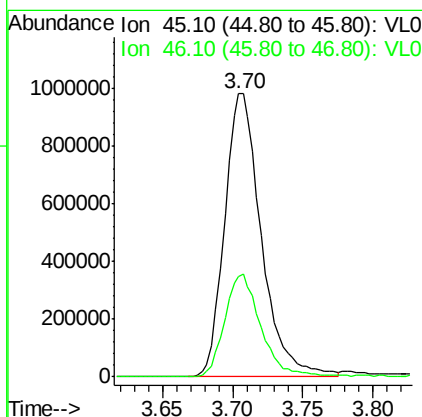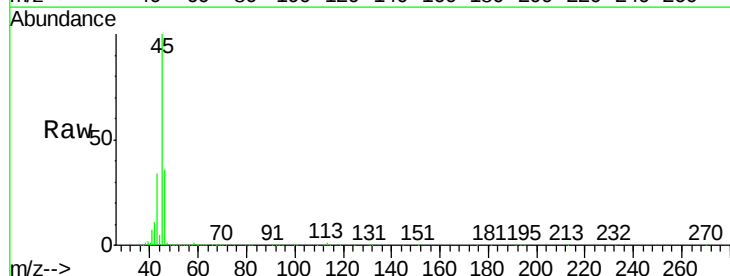



#15

Acetone

Concen: 184.37 ppbv m

RT: 3.94 min Scan# 887

Delta R.T. -0.01 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51

Instrument :

MSVOA_L

ClientSampleId :

SG06-MIVI

Tot Ion: 43 Resp: 27173757

Ion Ratio Lower Upper





43 100

58 66.0 22.4 33.6#

Manual Integrations
APPROVED

apatel

8/20/2018 5:03:32 PM

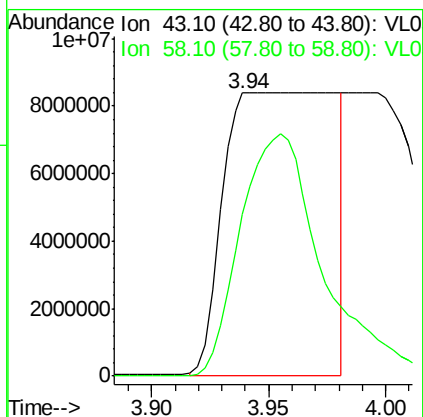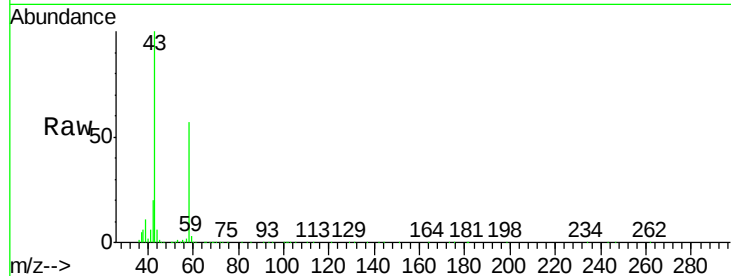

#20

Methylene Chloride

Concen: 6.03 ppbv

RT: 4.49 min Scan# 1057

Delta R.T. 0.03 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51

Tgt Ion: 84 Resp: 335865




Ion Ratio Lower Upper


84 100

49 142.8 117.3 175.9

51 34.3 36.6 55.0#

86 60.8 49.8 74.8

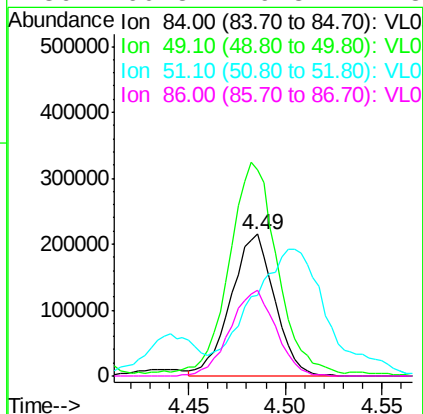







#26
Hexane
Concen: 249.91 ppbv m
RT: 5.87 min Scan# 1488
Delta R.T. 0.04 min
Lab File: VL032367.D
Acq: 16 Aug 2018 1:51

Instrument :
MSVOA_L
ClientSampleId :
SG06-MIVI

Tot Ion: 57 Resp: 35189675
Ion Ratio Lower Upper
57 100
41 14.9 68.0 102.0#
43 5.9 175.3 262.9#
56 15.0 42.0 63.0#




Manual Integrations
APPROVED


apatel
8/20/2018 5:03:32 PM

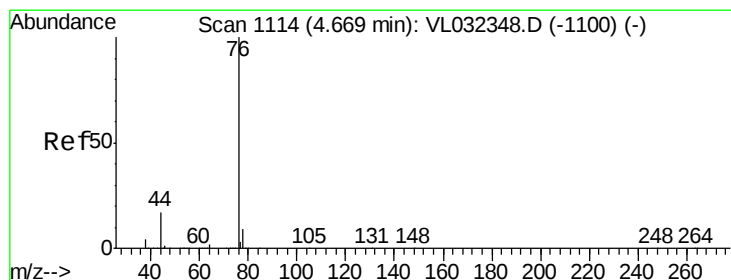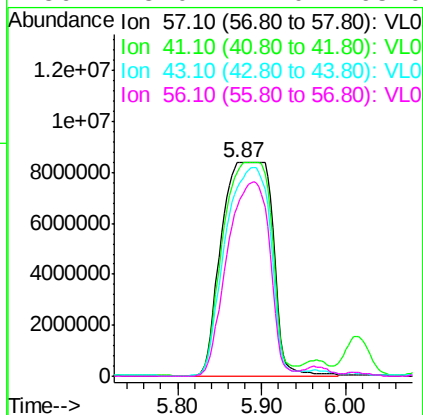

#27
Carbon Disulfide
Concen: 33.91 ppbv
RT: 4.69 min Scan# 1121
Delta R.T. 0.02 min
Lab File: VL032367.D
Acq: 16 Aug 2018 1:51

Tgt Ion: 76 Resp: 4456527
Ion Ratio Lower Upper
76 100
44 18.8 14.4 21.6
78 9.3 7.4 11.0

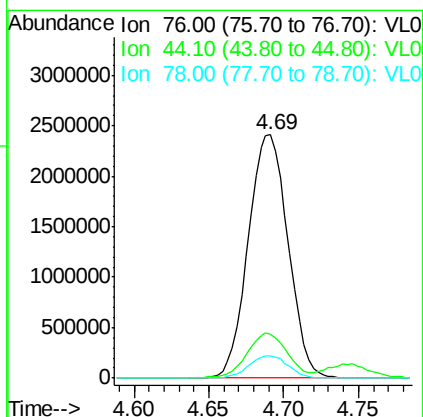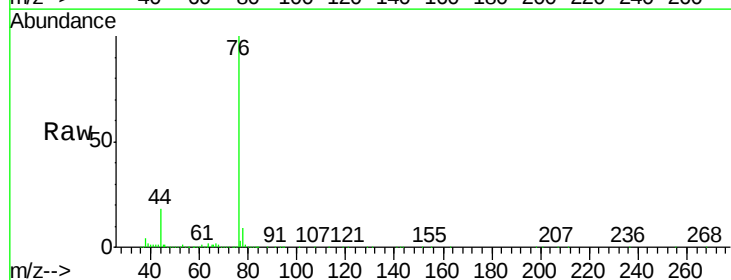







#30
Cvclohexane
Concen: 293.34 ppbv
RT: 7.36 min Scan# 1952
Delta R.T. 0.05 min
Lab File: VL032367.D
Acq: 16 Aug 2018 1:51

Instrument :
MSVOA_L
ClientSampled :
SG06-MIVI

Tot Ion: 84 Resp: 31463432
Ion Ratio Lower Upper
84 100
56 114.2 115.7 173.5#
41 91.4 67.9 101.9




Manual Integrations
APPROVED


apatel
8/20/2018 5:03:32 PM

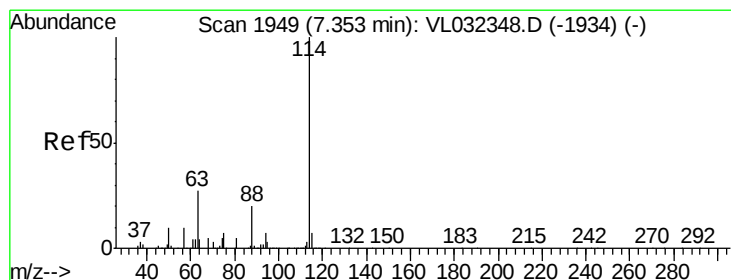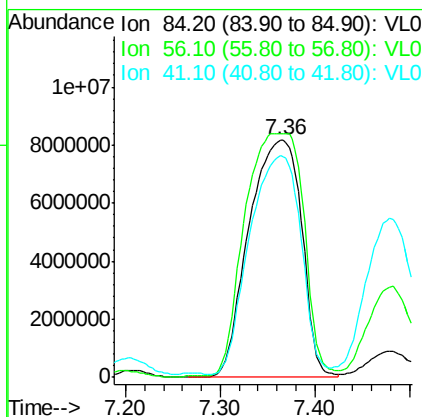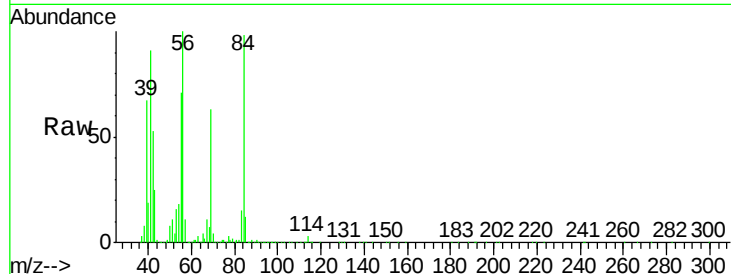

#33
1,4-Difluorobenzene
Concen: 10.00 ppbv
RT: 7.39 min Scan# 1961
Delta R.T. 0.04 min
Lab File: VL032367.D
Acq: 16 Aug 2018 1:51

Tgt Ion: 114 Resp: 2297078
Ion Ratio Lower Upper
114 100
63 45.2 22.0 33.0#
88 18.0 15.3 22.9

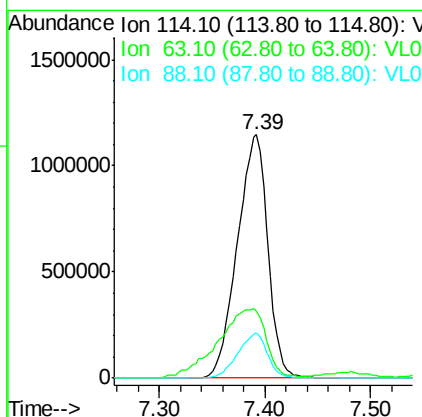

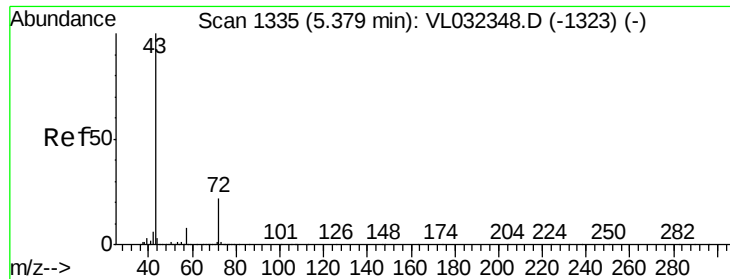





#34
2-Butanone
Concen: 113.05 ppbv
RT: 5.40 min Scan# 1340
Delta R.T. 0.02 min
Lab File: VL032367.D
Acq: 16 Aug 2018 1:51

Instrument :
MSVOA_L
ClientSampleId :
SG06-MIVI

Tot Ion: 43 Resp:17674436
Ion Ratio Lower Upper
43 100
72 29.1 17.9 26.9#




Manual Integrations
APPROVED


apatel
8/20/2018 5:03:32 PM

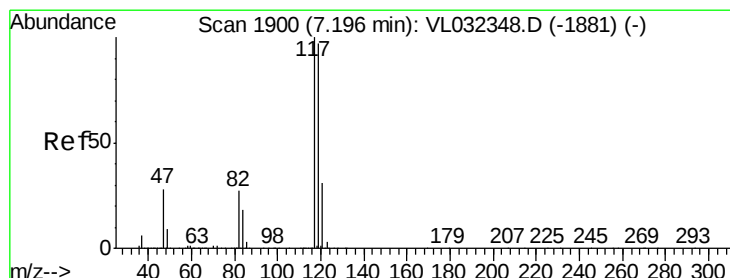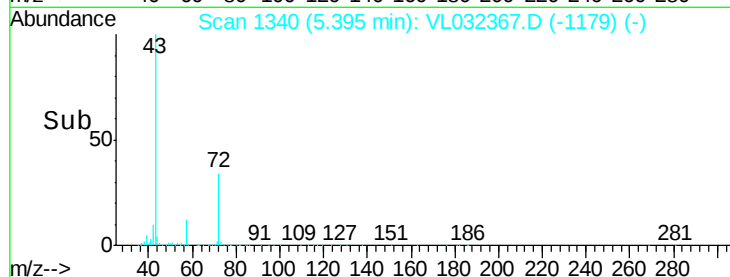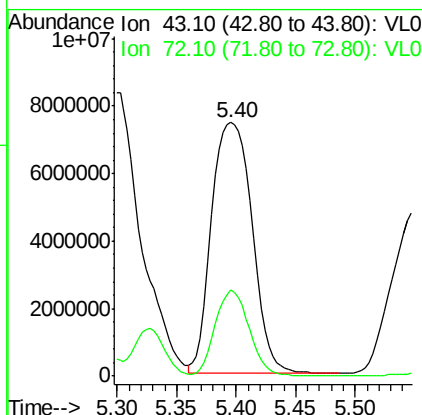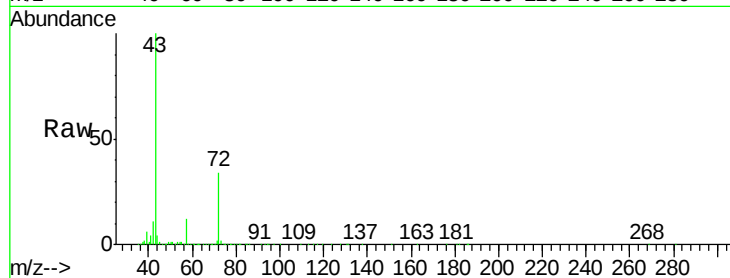

#35
Carbon Tetrachloride
Concen: 0.22 ppbv m
RT: 7.23 min Scan# 1911
Delta R.T. 0.04 min
Lab File: VL032367.D
Acq: 16 Aug 2018 1:51

Tgt Ion:117 Resp: 29799
Ion Ratio Lower Upper
117 100
119 103.8 77.2 115.8
121 23.6 25.1 37.7#

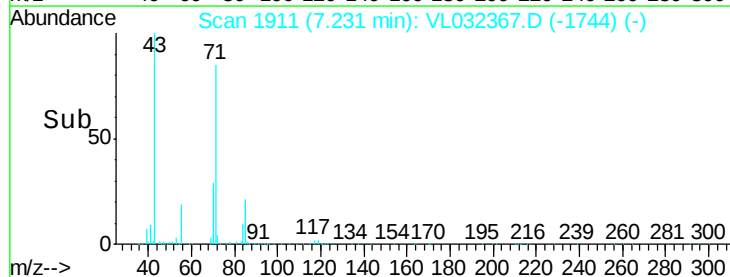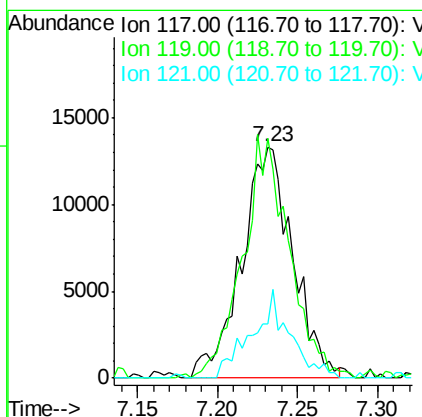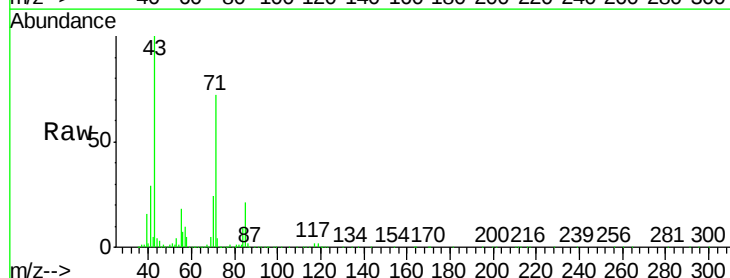



#36

Benzene

Concen: 107.71 ppbv

RT: 7.10 min Scan# 1869

Delta R.T. 0.03 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51

Instrument :

MSVOA_L

ClientSampleId :

SG06-MIVI

Tot Ion: 78 Resp: 20975647

Ion Ratio Lower Upper

78 100


77 33.5 18.0 27.0#

50 26.8 15.1 22.7#




Manual Integrations
APPROVED

apatel

8/20/2018 5:03:32 PM

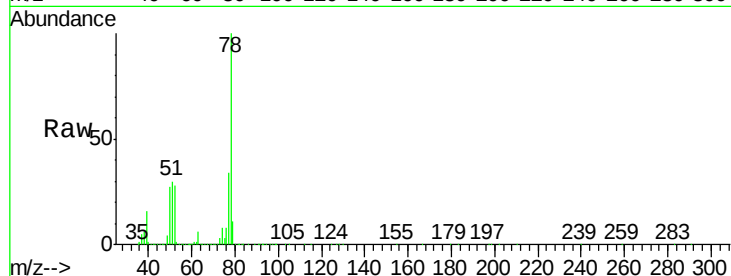

Abundance Ion 78.10 (77.80 to 78.80): VL0
Ion 77.10 (76.80 to 77.80): VL0
Ion 50.10 (49.80 to 50.80): VL0

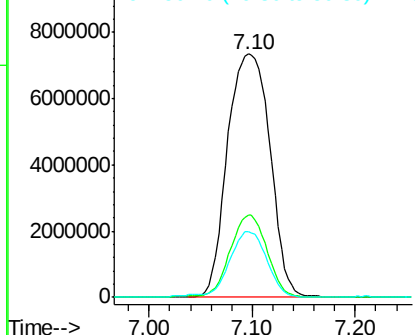

#52

Tetrachloroethene

Concen: 4.32 ppbv

RT: 11.47 min Scan# 3229

Delta R.T. 0.03 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51

Tgt Ion: 164 Resp: 247983


Ion Ratio Lower Upper

164 100



166 122.4 103.5 155.3


129 103.7 90.9 136.3

131 94.2 86.7 130.1



Abundance Ion 163.90 (163.60 to 164.60): V
Ion 165.90 (165.60 to 166.60): V
Ion 129.00 (128.70 to 129.70): V
Ion 131.00 (130.70 to 131.70): V

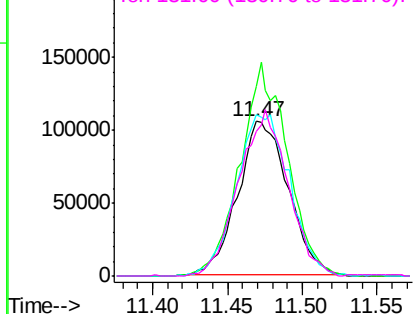



#53

Toluene

Concen: 160.28 ppbv m

RT: 10.04 min Scan# 2786

Delta R.T. 0.03 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51

Instrument :

MSVOA_L

ClientSampleId :

SG06-MIVI

Tot Ion: 91 Resp: 34216314

Ion Ratio Lower Upper





91 100

92 0.0 48.7 73.1#

Manual Integrations
APPROVED

apatel

8/20/2018 5:03:32 PM

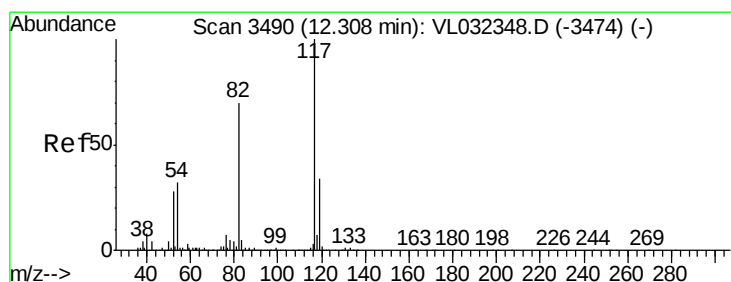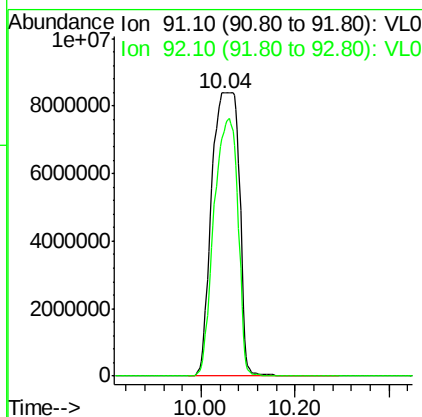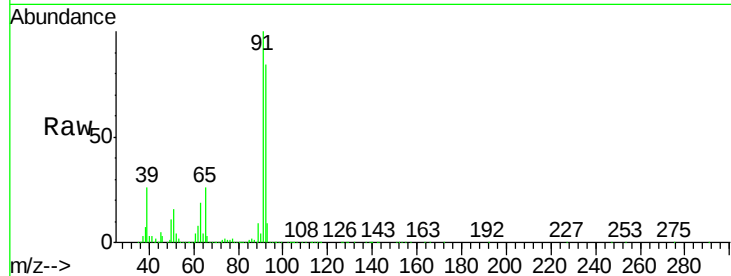

#55

Chlorobenzene-d5

Concen: 10.00 ppbv

RT: 12.33 min Scan# 3497

Delta R.T. 0.02 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51




Tgt Ion: 117 Resp: 3745267


Ion Ratio Lower Upper

117 100

82 73.1 55.1 82.7

119 32.4 46.0 69.0#

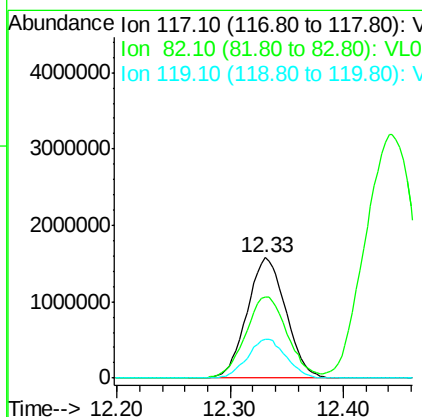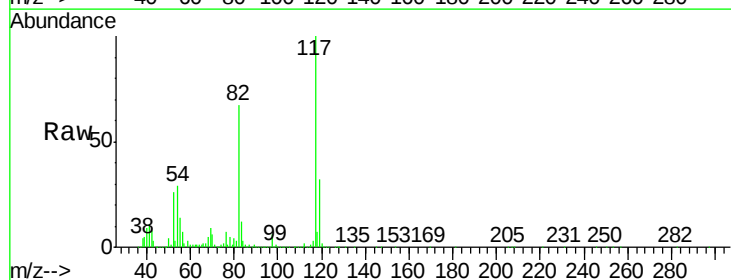

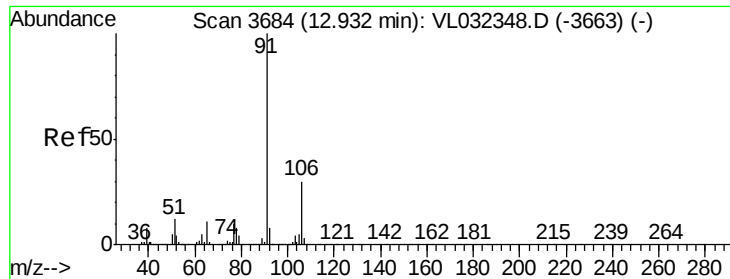

#58

Ethyl Benzene

Concen: 39.36 ppbv

RT: 12.96 min Scan# 3692

Delta R.T. 0.03 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51

Instrument :

MSVOA_L

ClientSampled :

SG06-MIVI

Tot Ion: 91 Resp:17734442

Ion Ratio Lower Upper





91 100

106 37.9 24.3 36.5#

Manual Integrations
APPROVED

apatel

8/20/2018 5:03:32 PM

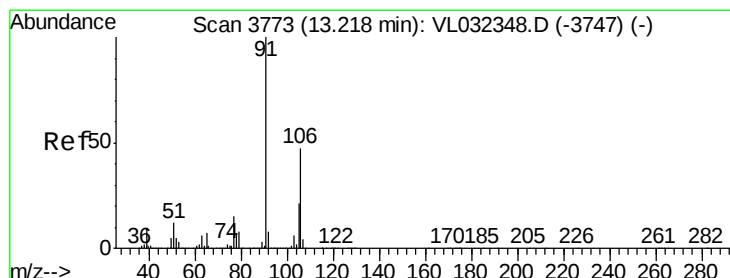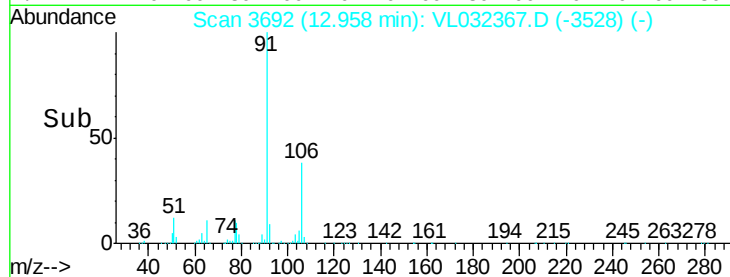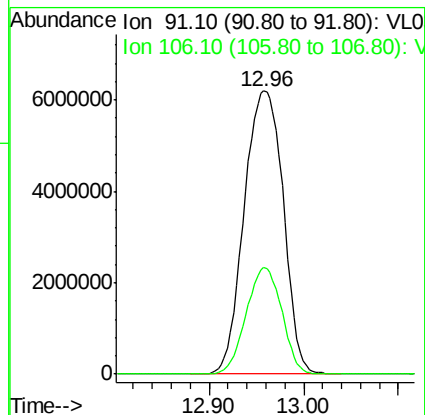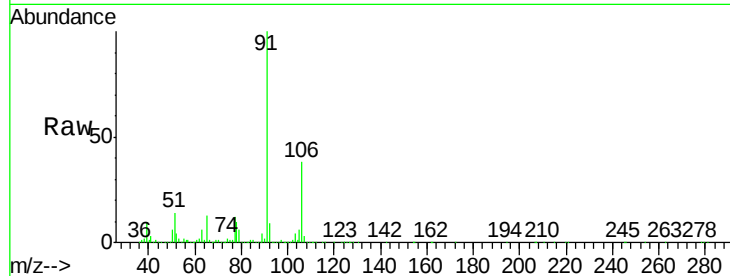

#59

m/p-Xylene

Concen: 69.79 ppbv

RT: 13.22 min Scan# 3773

Delta R.T. 0.00 min

Lab File: VL032367.D




Acq: 16 Aug 2018 1:51


Tgt Ion: 91 Resp:26712563

Ion Ratio Lower Upper

91 100

106 53.0 37.0 55.4

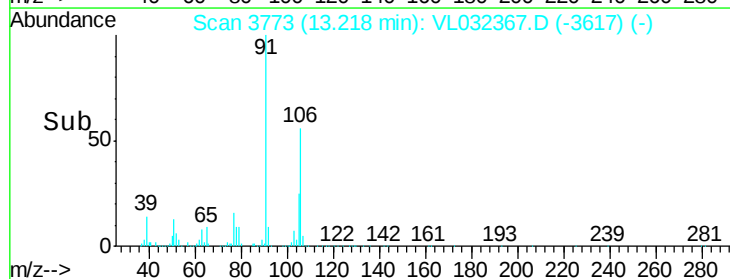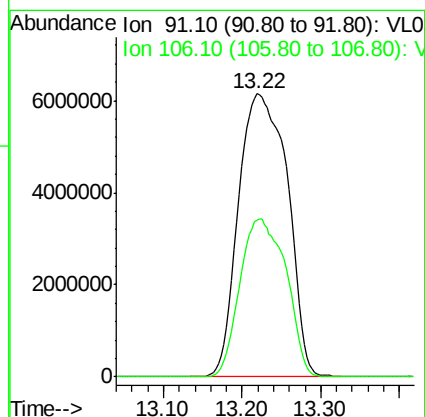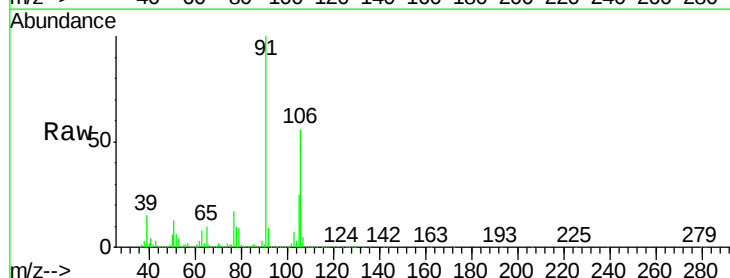



#60

o-Xylene

Concen: 28.16 ppbv

RT: 13.94 min Scan# 3998

Delta R.T. 0.02 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51

Instrument :

MSVOA_L

ClientSampleId :

SG06-MIVI

Tot Ion: 91 Resp: 10593159

Ion Ratio Lower Upper


91 100

106 46.3 22.3 66.8

Manual Integrations
APPROVED




apatel

8/20/2018 5:03:32 PM

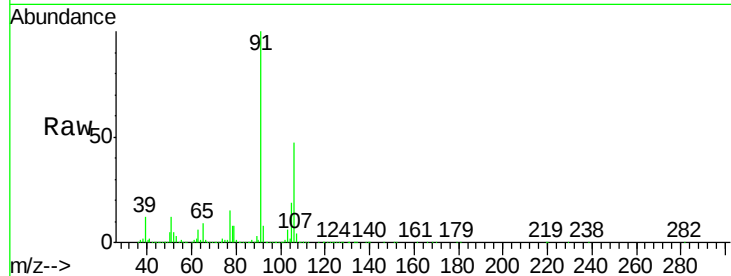

Abundance Ion 91.10 (90.80 to 91.80): VL0

Ion 106.10 (105.80 to 106.80): V

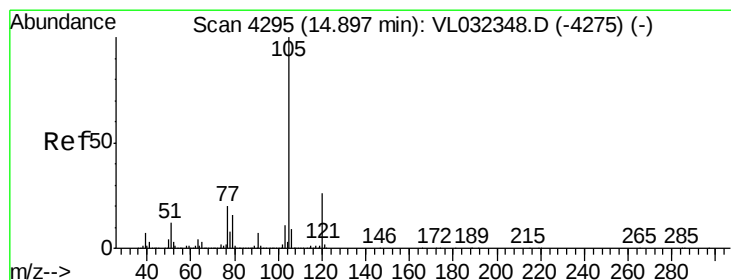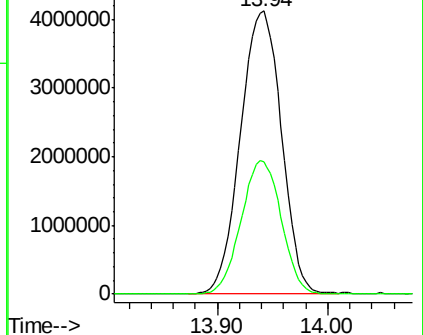

#62

Isopropylbenzene

Concen: 3.10 ppbv

RT: 14.91 min Scan# 4299

Delta R.T. 0.01 min

Lab File: VL032367.D


Acq: 16 Aug 2018 1:51

Tgt Ion: 105 Resp: 1658760

Ion Ratio Lower Upper



105 100


120 24.6 20.6 30.8



Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

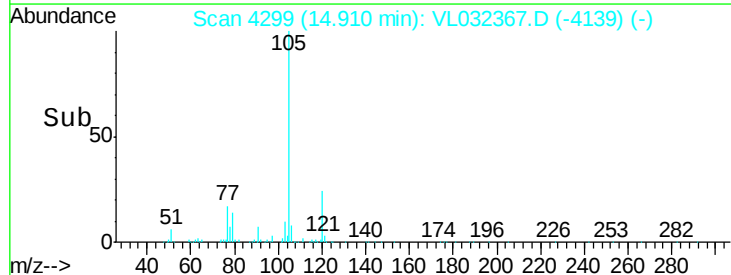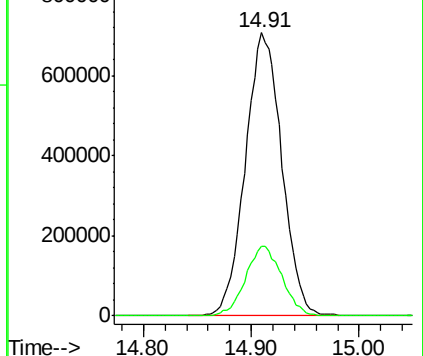



#64

n-propylbenzene

Concen: 3.99 ppbv

RT: 15.81 min Scan# 4578

Delta R.T. 0.01 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51

Instrument :

MSVOA_L

ClientSampleId :

SG06-MIVI

Tot Ion:120 Resp: 553497

Ion Ratio Lower Upper


120 100

91 490.5 382.2 573.2

Manual Integrations
APPROVED




apatel

8/20/2018 5:03:32 PM



Abundance Ion 120.20 (119.90 to 120.90): V

Ion 91.10 (90.80 to 91.80): VL0

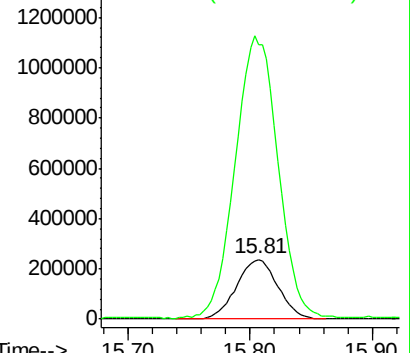

#67

sec-Butylbenzene

Concen: 0.88 ppbv

RT: 17.54 min Scan# 5116

Delta R.T. 0.01 min

Lab File: VL032367.D


Acq: 16 Aug 2018 1:51

Tgt Ion:105 Resp: 600521

Ion Ratio Lower Upper



105 100


134 17.7 14.4 21.6



Abundance Ion 105.10 (104.80 to 105.80): V

Ion 134.20 (133.90 to 134.90): V

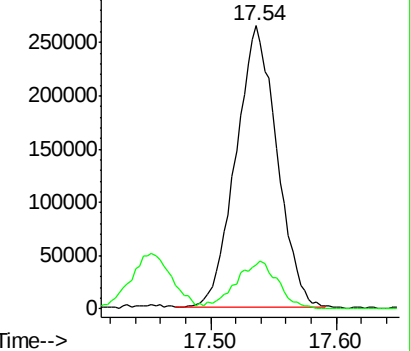

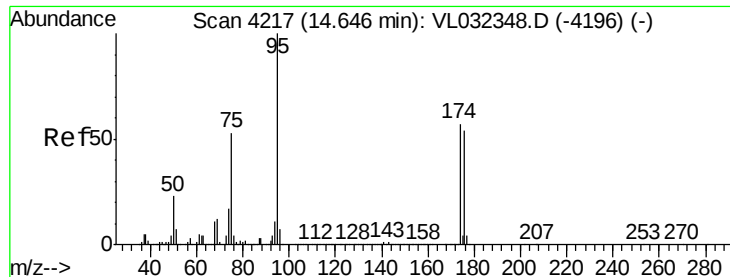

#68

1-Bromo-4-Fluorobenzene

Concen: 11.39 ppbv

RT: 14.66 min Scan# 4222

Delta R.T. 0.02 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51

Instrument :

MSVOA_L

ClientSampled :

SG06-MIVI

Tot Ion: 95 Resp: 3254576

Ion Ratio Lower Upper

95 100


174 51.5 46.2 69.4

175 3.8 3.4 5.0

Manual Integrations
APPROVED

apatel




8/20/2018 5:03:32 PM

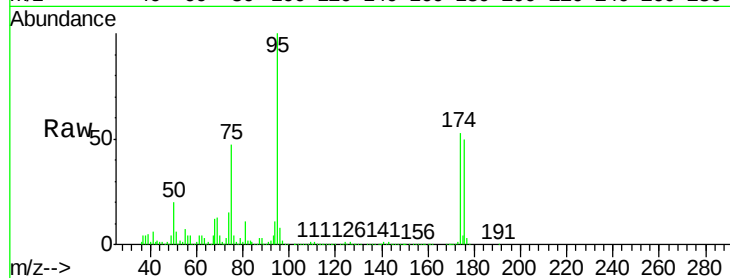

Abundance Ion 95.10 (94.80 to 95.80): VL0

Ion 174.00 (173.70 to 174.70): V

Ion 175.00 (174.70 to 175.70): V

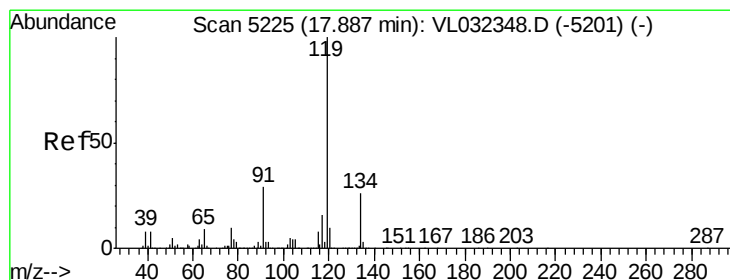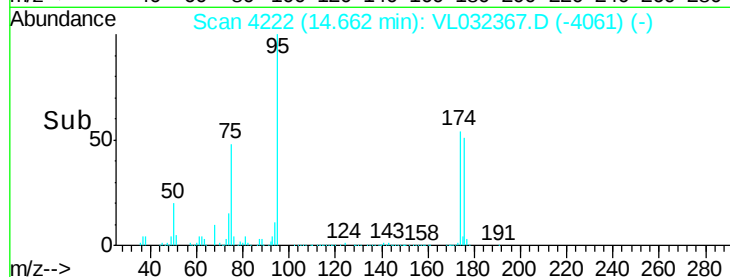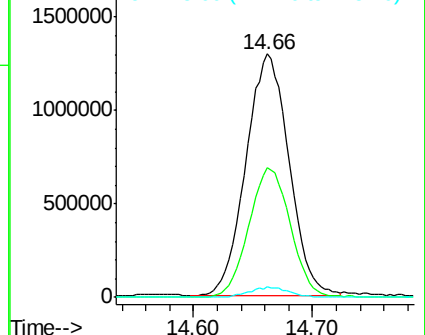

#69

p-Isopropyltoluene

Concen: 0.67 ppbv m

RT: 17.89 min Scan# 5227

Delta R.T. 0.01 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51


Tgt Ion: 119 Resp: 346237

Ion Ratio Lower Upper

119 100

134 23.3 20.4 30.6



91 0.0 23.6 35.4#

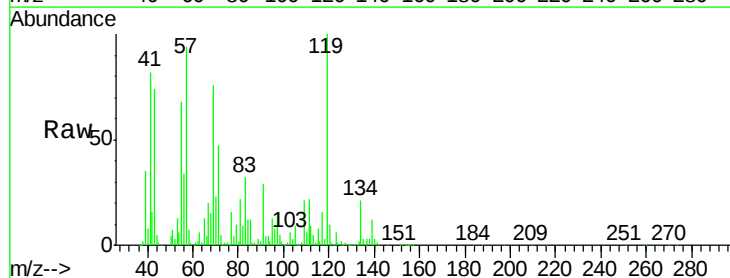


Abundance Ion 119.10 (118.80 to 119.80): V

Ion 134.20 (133.90 to 134.90): V

Ion 91.10 (90.80 to 91.80): VL0

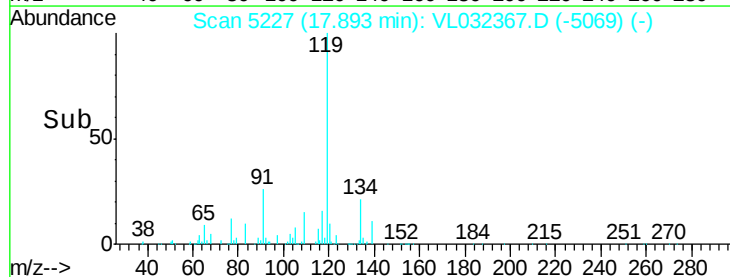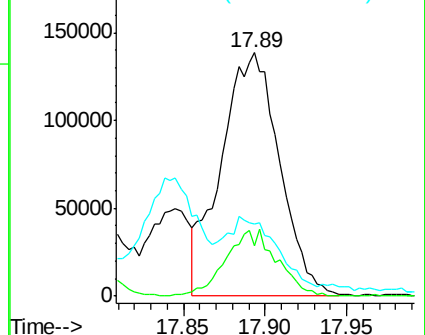



#70

n-Butylbenzene

Concen: 0.63 ppbv

RT: 18.79 min Scan# 5506

Delta R.T. 0.01 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51

Instrument :

MSVOA_L

ClientSampleId :

SG06-MIVI

Tot Ion: 91 Resp: 358119

Ion Ratio Lower Upper


91 100

92 36.9 43.9 65.9#

134 96.2 17.3 25.9#

Manual Integrations
APPROVED




apatel
8/20/2018 5:03:32 PM

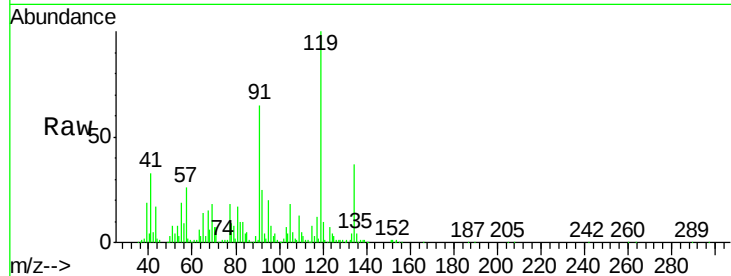

Abundance Ion 91.10 (90.80 to 91.80): VL0

Ion 92.10 (91.80 to 92.80): VL0

Ion 134.20 (133.90 to 134.90): VL0

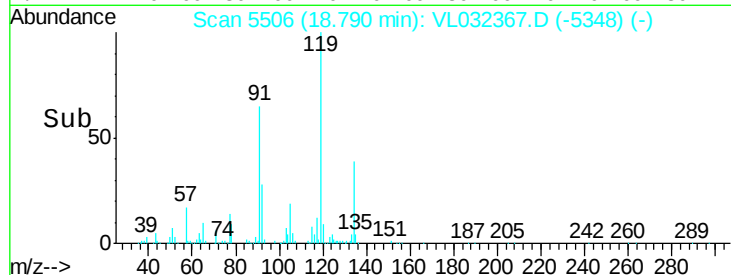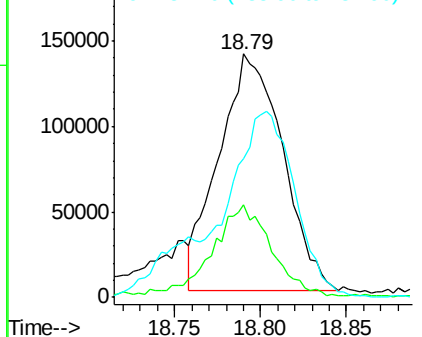

#72

4-Ethyltoluene

Concen: 7.14 ppbv

RT: 16.08 min Scan# 4664

Delta R.T. 0.01 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51

Tgt Ion: 105 Resp: 2997556

Ion Ratio Lower Upper

105 100

120 29.3 23.4 35.0

91 12.2 10.0 15.0




77 13.4 11.3 16.9


Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

Ion 91.10 (90.80 to 91.80): VL0

Ion 77.10 (76.80 to 77.80): VL0

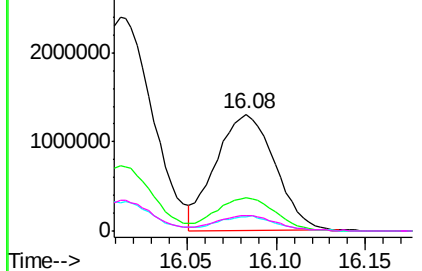



#73

1,3,5-Trimethylbenzene

Concen: 5.68 ppbv

RT: 16.24 min Scan# 4713

Delta R.T. 0.01 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51

Instrument :

MSVOA_L

ClientSampleId :

SG06-MIVI

Tot Ion:105 Resp: 2291785

Ion Ratio Lower Upper


105 100

120 44.3 36.3 54.5

Manual Integrations
APPROVED




apatel

8/20/2018 5:03:32 PM



Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

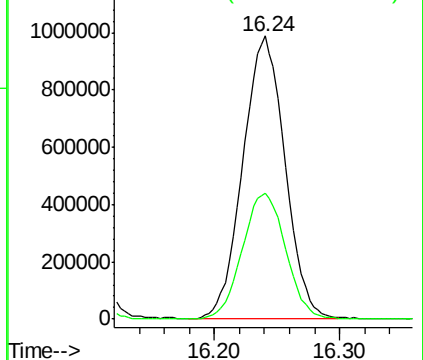

#74

1,2,4-Trimethylbenzene

Concen: 9.02 ppbv

RT: 17.01 min Scan# 4951

Delta R.T. 0.01 min

Lab File: VL032367.D

Acq: 16 Aug 2018 1:51

Tgt Ion:105 Resp: 3871857

Ion Ratio Lower Upper

105 100

120 43.9 37.6 56.4

91 10.8 39.9 59.9#




77 13.7 17.8 26.8#


Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

Ion 91.10 (90.80 to 91.80): VL0

Ion 77.10 (76.80 to 77.80): VL0

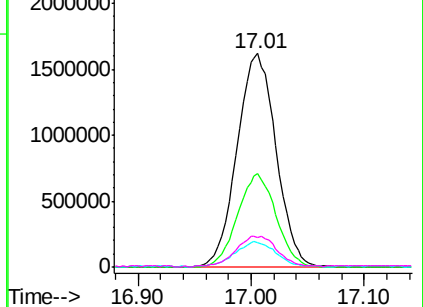







#79
Naphthalene
Concen: 0.64 ppbv
RT: 22.49 min Scan# 6658
Delta R.T. 0.00 min
Lab File: VL032367.D
Acq: 16 Aug 2018 1:51

Instrument :
MSVOA_L
ClientSampled :
SG06-MIVI

Tot Ion:	128	Resp:	131547
Ion Ratio	Lower	Upper	
128	100		
127	13.0	10.3	15.5
129	11.1	8.6	13.0

Manual Integrations
APPROVED

apatel
8/20/2018 5:03:32 PM

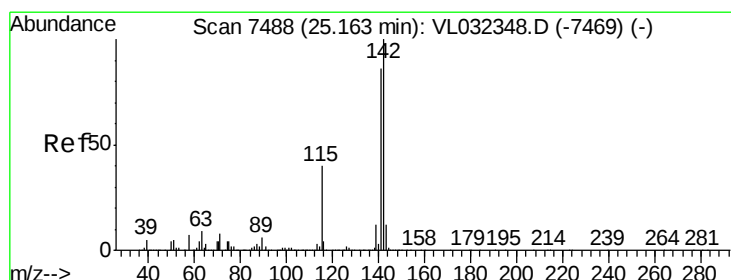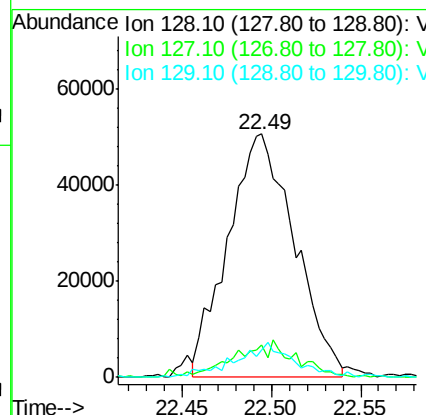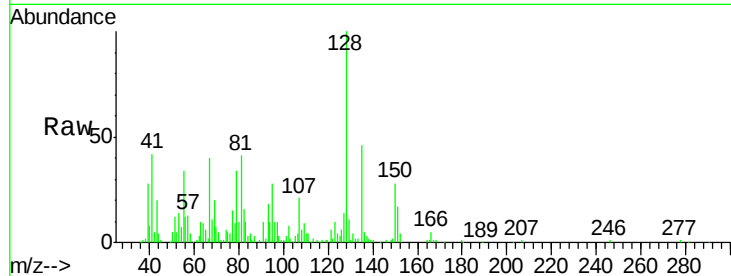

#80
Naphthalene, 2-methyl-
Concen: 0.36 ppbv
RT: 25.17 min Scan# 7489
Delta R.T. 0.00 min
Lab File: VL032367.D
Acq: 16 Aug 2018 1:51

Tgt Ion:	142	Resp:	31022
Ion Ratio	Lower	Upper	
142	100		
141	86.0	66.7	100.1
115	42.1	31.0	46.6

