

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL081523\
 Data File : VL040637.D
 Acq On : 15 Aug 2023 18:04
 Operator : SY/MD
 Sample : VL0815ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0815ABL01

Quant Time: Aug 16 05:56:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL081523AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Wed Aug 16 05:43:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.192	49	924764	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.658	114	2503906	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.474	117	2121179	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	13.786	95	1729961	10.255	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.500%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL081523\
Data File : VL040637.D
Acq On : 15 Aug 2023 18:04
Operator : SY/MD
Sample : VL0815ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0815ABL01

Quant Time: Aug 16 05:56:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL081523AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Wed Aug 16 05:43:50 2023
Response via : Initial Calibration




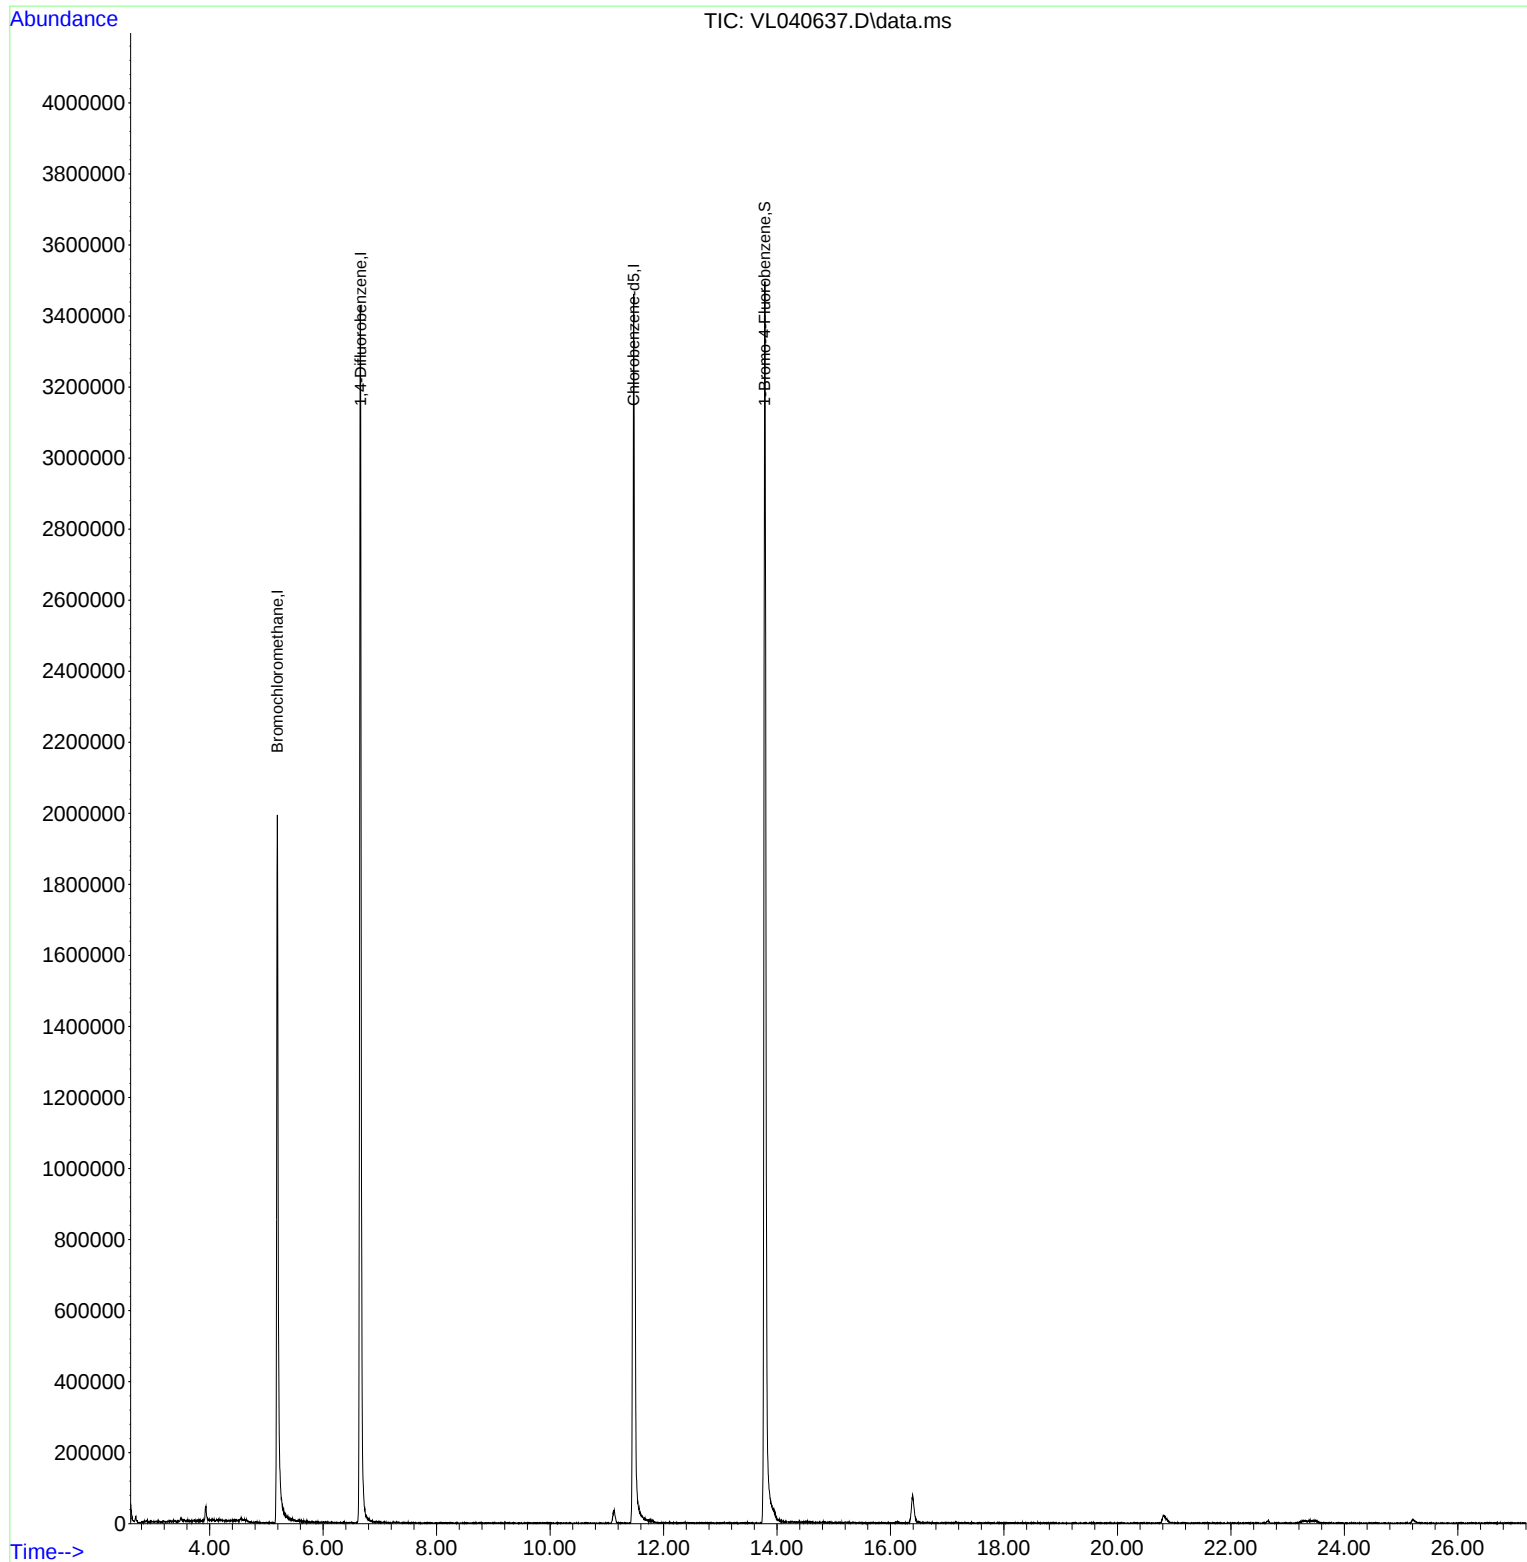


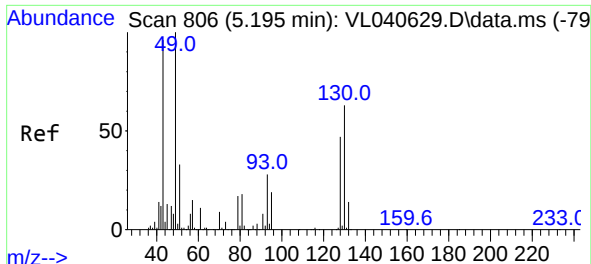

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.192 min Scan# 806
Delta R.T. -0.003 min
Lab File: VL040637.D
Acq: 15 Aug 2023 18:04




Instrument :
MSVOA_L
ClientSampleId :
VL0815ABL01


Tgt Ion: 49 Resp: 924764
Ion Ratio Lower Upper
49 100
128 52.5 24.9 74.7
130 65.9 32.2 96.6

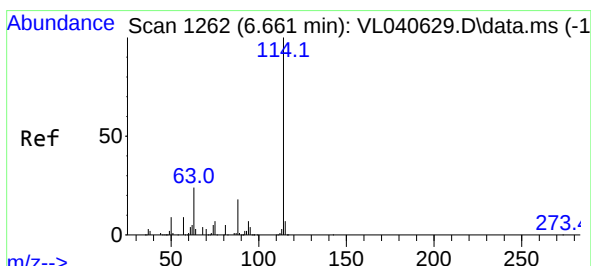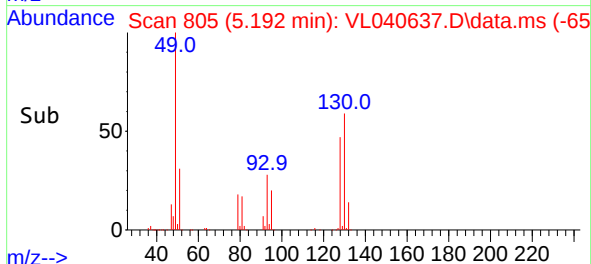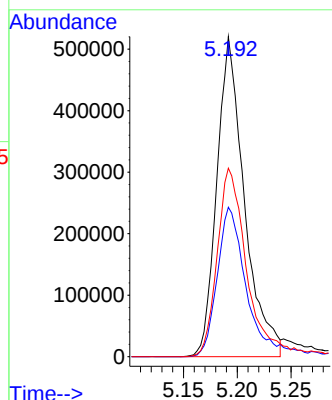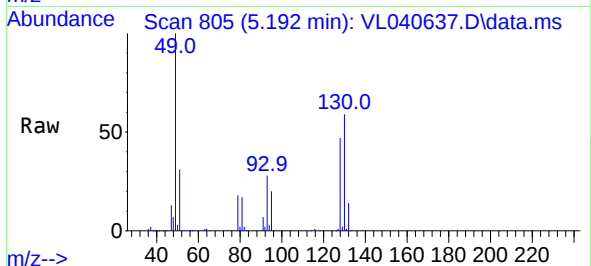

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.658 min Scan# 1261
Delta R.T. -0.003 min
Lab File: VL040637.D
Acq: 15 Aug 2023 18:04

Tgt Ion: 114 Resp: 2503906
Ion Ratio Lower Upper
114 100
63 25.8 20.2 30.2
88 18.3 14.1 21.1


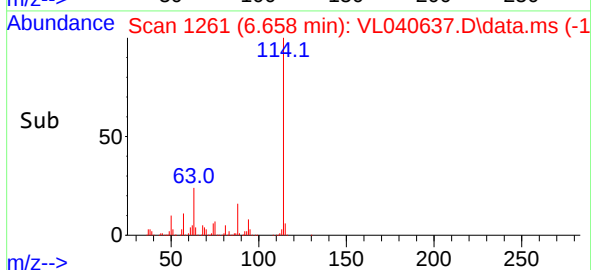
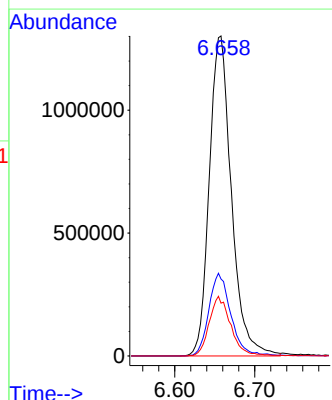
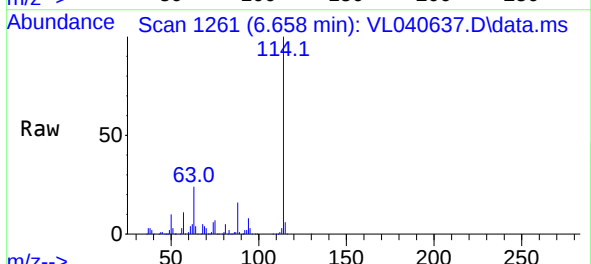


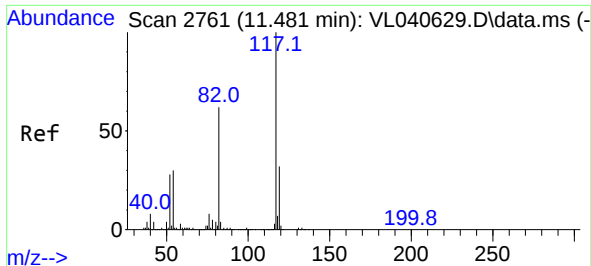

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.474 min Scan# 2117
Delta R.T. -0.007 min
Lab File: VL040637.D
Acq: 15 Aug 2023 18:04

Instrument :
MSVOA_L
ClientSampleId :
VL0815ABL01

Tgt Ion:117 Resp: 2121179
Ion Ratio Lower Upper
117 100
82 68.6 49.5 74.3
119 33.2 24.5 36.7

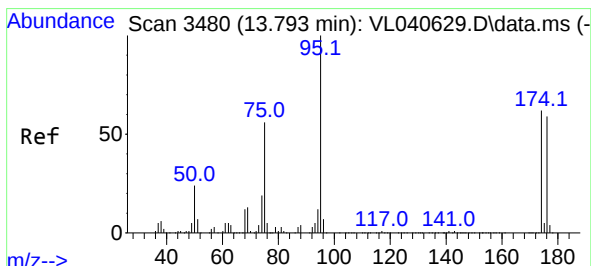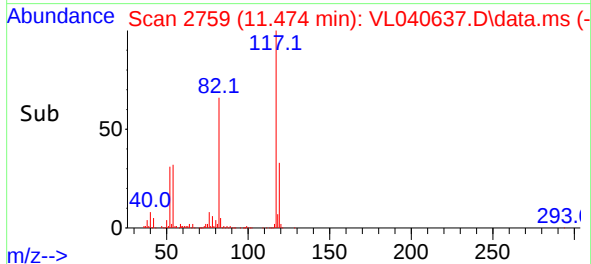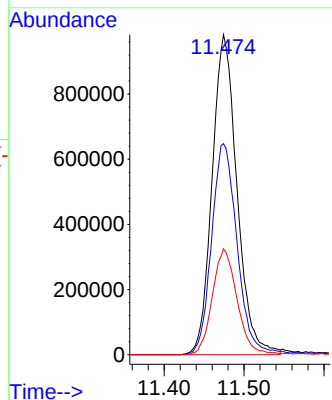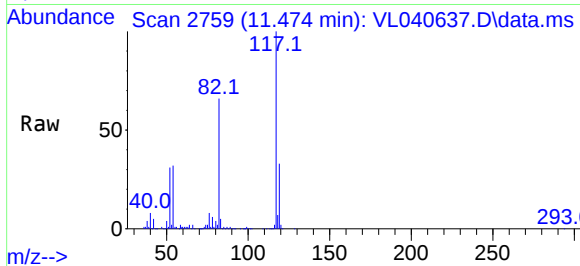

#68
1-Bromo-4-Fluorobenzene
Concen: 10.255 ppbv
RT: 13.786 min Scan# 3478
Delta R.T. -0.007 min
Lab File: VL040637.D
Acq: 15 Aug 2023 18:04

Tgt Ion: 95 Resp: 1729961
Ion Ratio Lower Upper
95 100
174 60.8 49.1 73.7
175 4.2 3.7 5.5

