
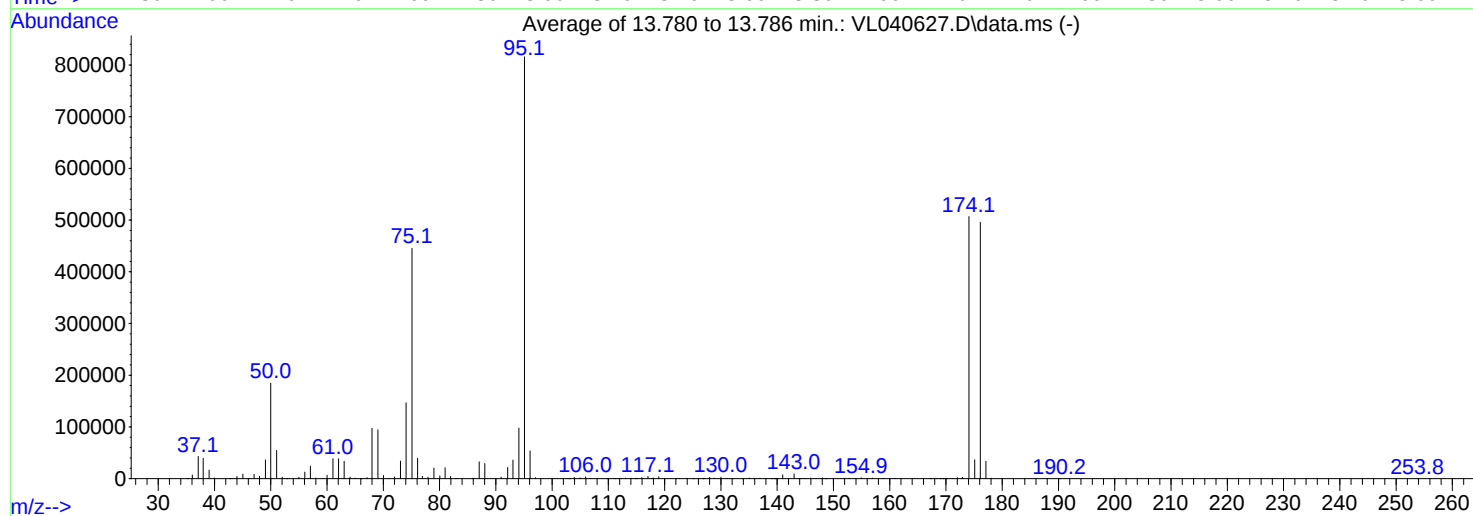


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL081523\
 Data File : VL040627.D
 Acq On : 15 Aug 2023 8:58
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL081523AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Wed Aug 16 05:43:50 2023

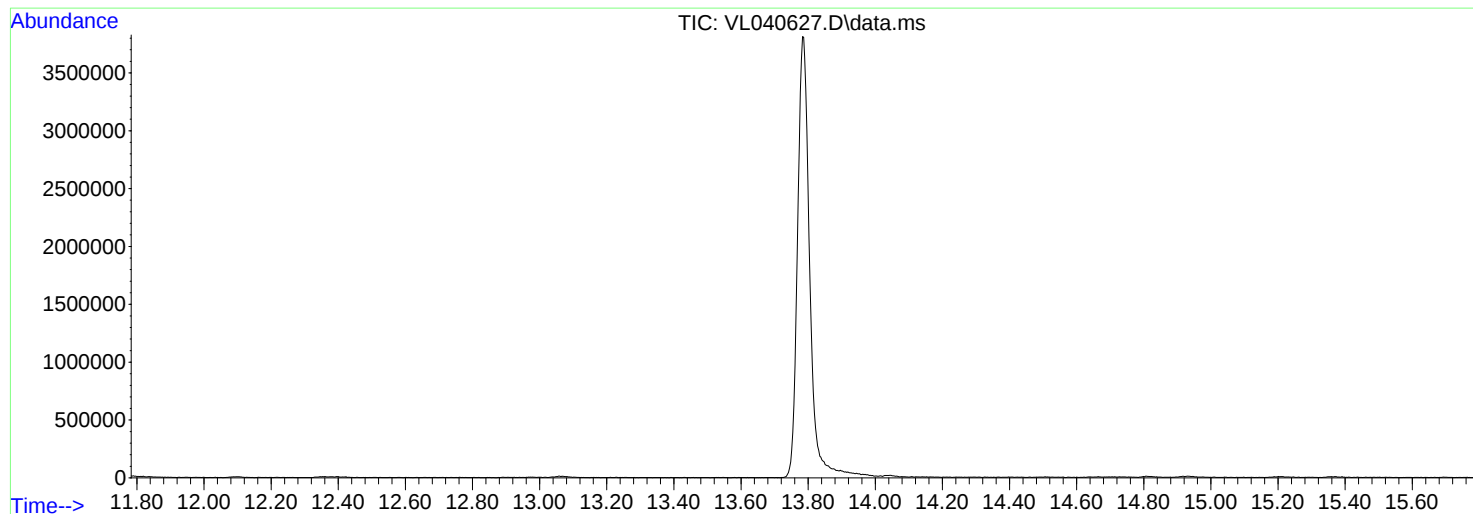

AutoFind: Scans 3476, 3477, 3478; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.7	184875	PASS
75	95	30	66	54.6	445376	PASS
95	95	100	100	100.0	815723	PASS
96	95	5	9	6.6	53949	PASS
173	174	0.00	2	0.5	2624	PASS
174	95	50	120	62.1	506923	PASS
175	174	4	9	7.2	36651	PASS
176	174	93	101	97.8	495637	PASS
177	176	5	9	6.7	33371	PASS

Average of 13.780 to 13.786 min.: VL040627.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.20	53	46.25	652	57.05	24131	66.10	10
36.05	7234	47.05	8231	58.00	1239	67.10	206
37.10	42984	48.00	4807	59.10	287	68.00	9740
38.00	39301	49.05	36296	60.00	6450	69.05	9441
39.05	16726	50.00	184875	61.05	38784	70.05	6304
39.95	1184	51.05	54424	62.05	38528	70.95	288
42.70	58	52.05	2862	63.05	33344	72.00	3516
43.10	262	52.80	131	64.10	2996	73.05	34173
44.00	4276	53.05	244	64.90	546	74.05	146581
45.05	8821	55.00	2856	65.05	1117	75.10	445376
46.10	357	56.05	12766	65.90	62	76.10	39413

Average of 13.780 to 13.786 min.: VL040627.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.95	4208	90.95	3041	105.95	3375	115.95	2030
77.95	2901	92.10	21685	106.80	754	117.05	4309
79.00	20411	93.05	35899	109.70	185	117.90	968
80.05	5492	94.10	97848	110.00	83	118.05	1348
81.00	20901	95.10	815723	110.80	642	118.95	3702
81.95	4440	96.10	53949	111.20	154	122.00	75
82.90	575	97.05	1862	111.85	309	122.60	200
83.15	428	102.70	280	112.30	288	123.95	889
85.85	686	103.00	153	113.05	924	125.10	62
87.05	32573	103.95	2604	114.80	152	125.95	317
88.05	29381	104.95	1536	115.15	573	126.80	90

Average of 13.780 to 13.786 min.: VL040627.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.95	119	136.95	1107	145.05	337	153.00	202
127.95	2520	139.00	53	145.95	1238	154.00	336
128.80	1191	139.50	135	146.90	268	154.95	1665
130.00	2803	139.70	80	147.90	372	155.90	328
130.90	439	140.00	282	148.10	1425	156.90	1200
131.20	544	141.00	7499	148.60	111	158.70	214
131.90	84	142.00	664	148.80	220	159.00	765
132.05	123	143.00	9399	149.10	327	160.80	540
133.85	207	143.80	317	149.95	837	161.10	202
135.05	1377	144.25	194	151.85	317	167.30	90
135.85	192	144.70	306	152.70	247	168.30	196

Average of 13.780 to 13.786 min.: VL040627.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
169.00	185	178.05	904				
169.50	54	190.20	50				
170.10	66	253.80	56				
171.15	217						
172.05	1991						
172.70	731						
172.95	2624						
174.10	506923						
175.10	36651						
176.10	495637						
177.10	33371						