

Data File : VL035422.D
Acq On : 17 Aug 2020 15:30
Operator : SY/AP
Sample : VSTDIC001
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDIC001

Quant Time: Aug 17 16:31:12 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081720AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Aug 17 09:05:17 2020
QLast Update : Mon Aug 17 09:05:17 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.68	49	1147566	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	0.00	114	0	0.00	ppbv	-7.19
55) Chlorobenzene-d5	12.11	117	5235106	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.45	95	3668232	8.27	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	82.70%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	3.05	85	241498	1.585	ppbv	97
3) Chlorodifluoromethane	2.99	51	153773	1.046	ppbv	93
4) Chloromethane	3.14	50	80695	1.042	ppbv	95
5) Vinyl Chloride	3.26	62	92971	1.181	ppbv	94
6) Bromomethane	3.48	94	83380	1.932	ppbv	100
7) Chloroethane	3.56	64	34279	1.313	ppbv	96
8) Dichlorotetrafluoroethane	3.19	85	307426	1.770	ppbv #	57
9) Propene	3.01	41	63144	0.905	ppbv	99
10) Heptane	8.14	43	163621	0.928	ppbv #	82
11) Trichlorofluoromethane	3.96	101	363714	1.989	ppbv	100
12) 1,1,2-Trichlorotrifluoroet	4.49	101	270625	2.272	ppbv #	77
13) Ethanol	3.62	45	27170	1.219	ppbv	98
14) Bromoethene	3.74	108	116850	2.236	ppbv #	94
15) Acetone	3.86	43	147515	0.977	ppbv #	78
16) 1,3-Butadiene	3.33	39	58521	0.846	ppbv #	74
17) tert-Butyl alcohol	4.30	59	185997	1.298	ppbv	99
18) 1,1-Dichloroethene	4.30	96	115808	2.164	ppbv #	63
19) Isopropyl Alcohol	3.98	45	101842	0.956	ppbv #	95
20) Methylene Chloride	4.35	84	119582	2.135	ppbv #	63
21) Allyl Chloride	4.42	41	69358	0.786	ppbv #	80
22) trans-1,2-Dichloroethene	4.90	96	124424	2.334	ppbv #	62
23) Vinyl Acetate	5.09	43	195708	0.884	ppbv #	93
24) 1,1-Dichloroethane	5.02	63	202611	1.284	ppbv	95
25) Ethyl Acetate	5.69	43	283118	0.936	ppbv #	94
26) Hexane	5.70	57	160847	1.224	ppbv #	75
27) Carbon Disulfide	4.56	76	209899	1.641	ppbv #	87
28) Methyl tert-Butyl Ether	5.05	73	283629	1.399	ppbv	91
29) Chloroform	5.76	83	318794	1.580	ppbv	100
30) Cyclohexane	7.15	84	168851	1.618	ppbv #	59
31) cis-1,2-Dichloroethene	5.56	61	162782	1.216	ppbv #	71
32) 1,1,1-Trichloroethane	6.53	97	294640	1.465	ppbv #	90
56) 1,1,1,2-Tetrachloroethane	12.15	131	269950	1.048	ppbv #	1
57) Chlorobenzene	12.17	112	503032	1.064	ppbv #	77
58) Ethyl Benzene	12.74	91	723109	0.834	ppbv	95
59) m/p-Xylene	13.02	91	651937	0.902	ppbv #	33
60) o-Xylene	13.72	91	596358	0.838	ppbv	89
61) Styrene	13.56	104	466055	0.959	ppbv #	86
62) Isopropylbenzene	14.70	105	1001253	0.953	ppbv	94
63) 1,1,2,2-Tetrachloroethane	13.70	83	428358	0.776	ppbv	99
64) n-propylbenzene	15.59	120	288946	1.085	ppbv	70
65) tert-Butylbenzene	16.78	119	976269	1.085	ppbv #	78

Data File : VL035422.D
Acq On : 17 Aug 2020 15:30
Operator : SY/AP
Sample : VSTDICC001
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC001

Quant Time: Aug 17 16:31:12 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081720AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Aug 17 09:05:17 2020
QLast Update : Mon Aug 17 09:05:17 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
66) Benzyl Chloride	17.03	91	168899	0.573	ppbv #	91
67) sec-Butylbenzene	17.33	105	1316160	0.991	ppbv	92
69) p-Isopropyltoluene	17.69	119	1151228	1.064	ppbv #	88
70) n-Butylbenzene	18.59	91	1085243	0.858	ppbv #	94
71) 2-Chlorotoluene	15.48	91	703913	0.819	ppbv	82
72) 4-Ethyltoluene	15.87	105	785927	0.943	ppbv #	92
73) 1,3,5-Trimethylbenzene	16.03	105	735560	0.935	ppbv #	85
74) 1,2,4-Trimethylbenzene	16.80	105	810568	0.962	ppbv #	90
75) 1,3-Dichlorobenzene	17.03	146	618420	1.348	ppbv	92
76) 1,4-Dichlorobenzene	17.17	146	599934	1.275	ppbv	90
77) 1,2-Dichlorobenzene	17.85	146	602374	1.303	ppbv	91
78) Hexachloro-1,3-Butadiene	23.42	225	482274	1.358	ppbv	100
79) Naphthalene	22.25	128	1126851	1.145	ppbv	97
80) Naphthalene,2-methyl-	25.01	142	405637	0.988	ppbv #	90
81) 1,2,4-Trichlorobenzene	21.98	180	673091	1.443	ppbv	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data File : VL035422.D

```
Acq On       : 17 Aug 2020 15:30
Operator     : SY/AP
Sample       : VSTDICC001
Misc         : 400ml/MSVOA_L
ALS Vial     : 1      Sample Multipl
```

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC001

Quant Time: Aug 17 16:31:12 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081720AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Aug 17 09:05:17 2020
QLast Update : Mon Aug 17 09:05:17 2020
Response via : Initial Calibration

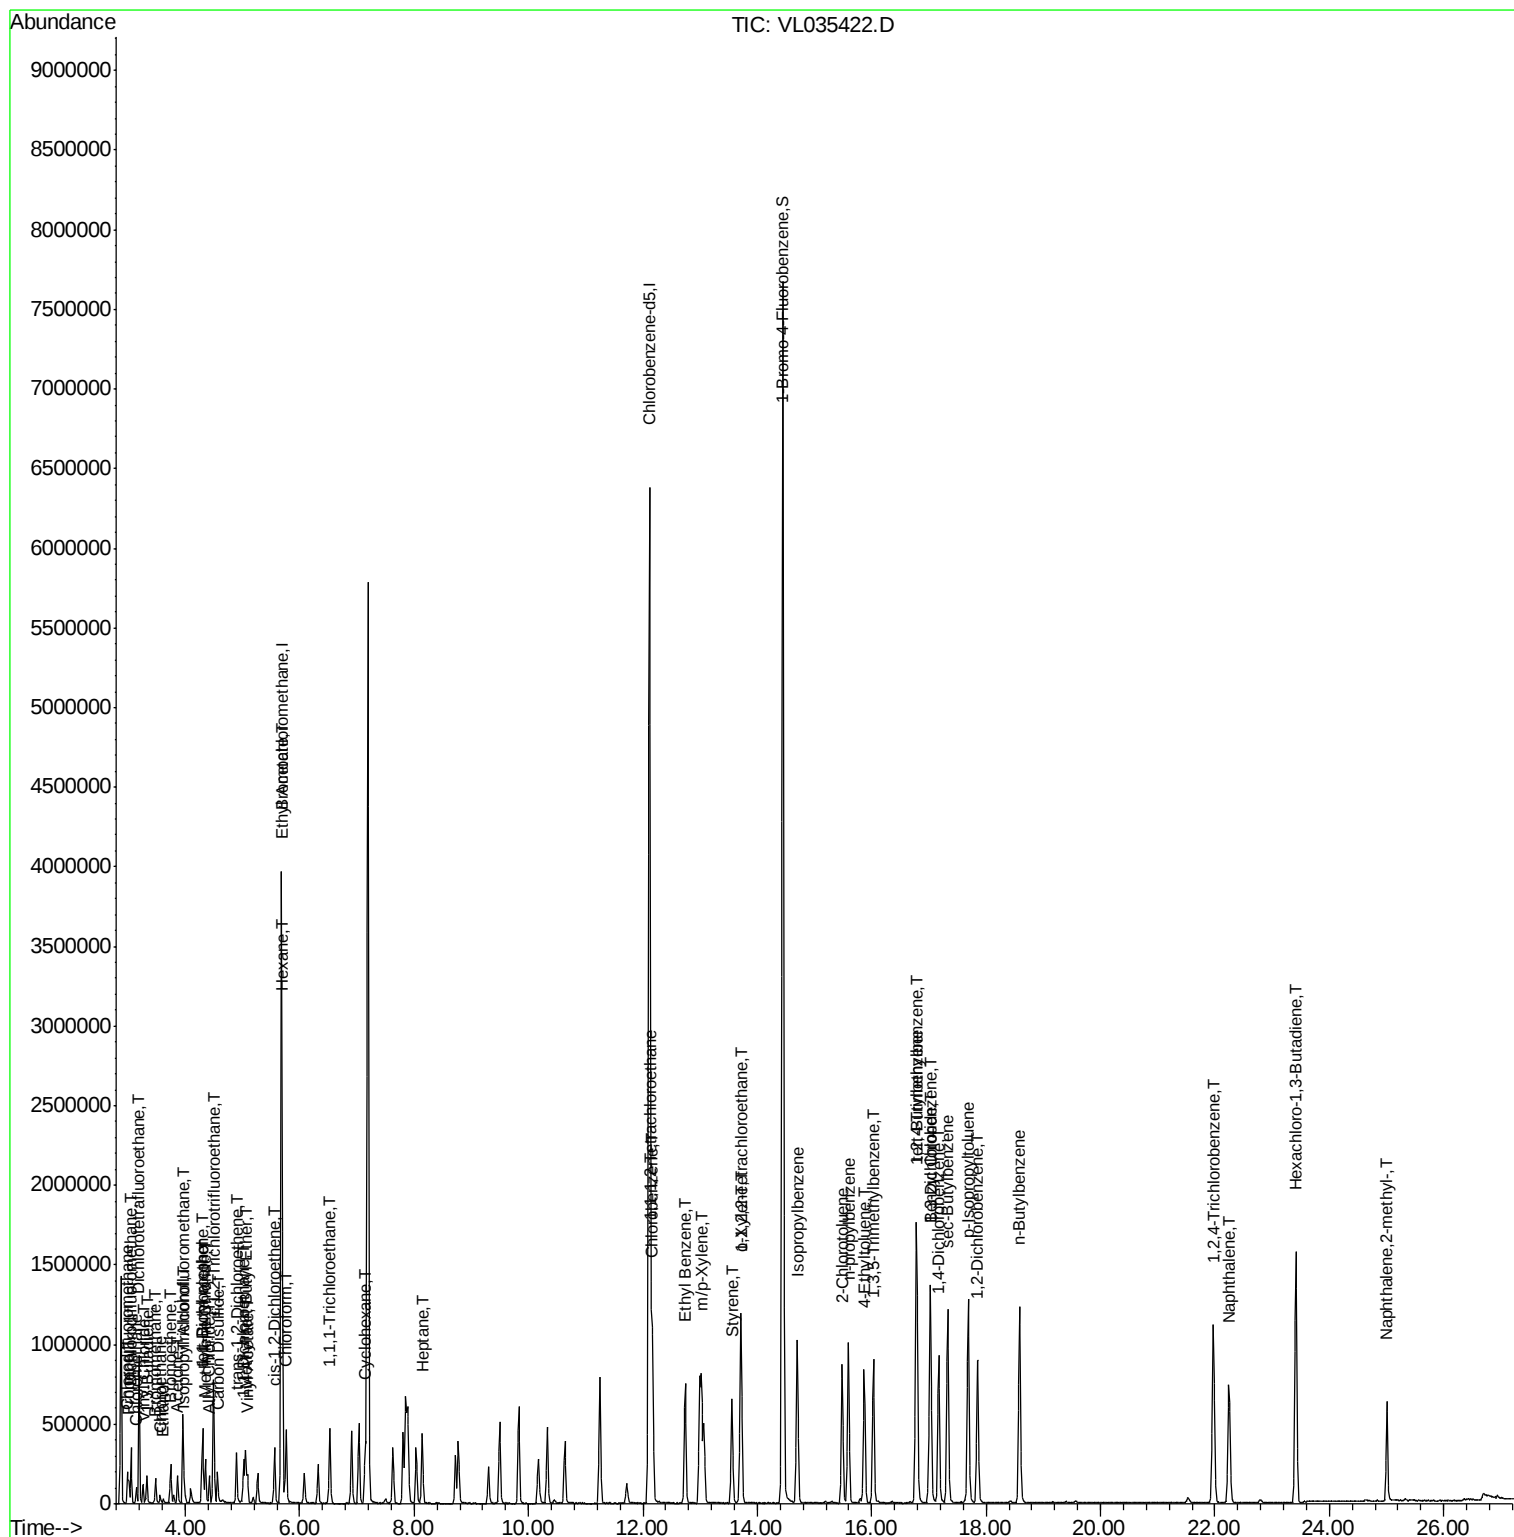



#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.68 min Scan# 899

Delta R.T. 0.00 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :

VSTDIC001





Tgt Ion: 49 Resp: 1147566

Ion Ratio Lower Upper

49 100

128 103.1 20.9 62.7#

130 132.4 26.7 80.1#

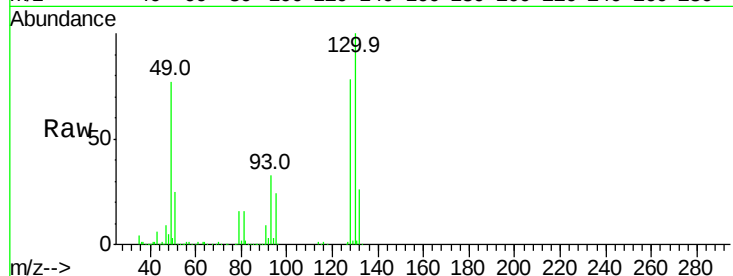

#2

Dichlorodifluoromethane

Concen: 1.585 ppbv

RT: 3.05 min Scan# 82

Delta R.T. 0.01 min

Lab File: VL035422.D




Acq: 17 Aug 2020 15:30


Tgt Ion: 85 Resp: 241498

Ion Ratio Lower Upper

85 100

87 32.1 27.1 40.7



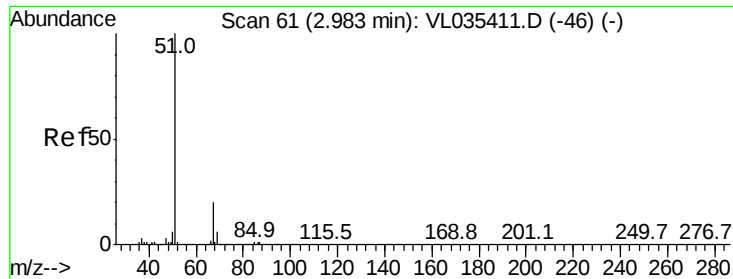

#3

Chlorodifluoromethane

Concen: 1.046 ppbv

RT: 2.99 min Scan# 64

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :


VSTDIC001

Tgt Ion: 51 Resp: 153773

Ion Ratio Lower Upper




51 100

67 21.8 15.0 22.6

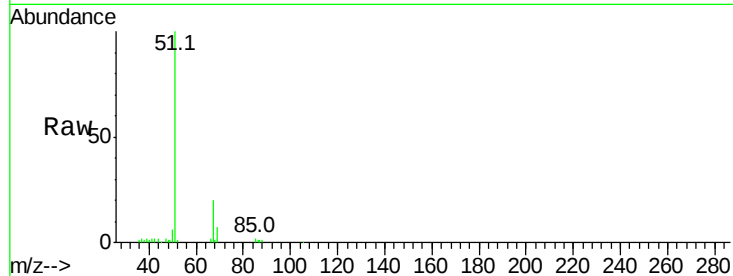

Abundance Ion 51.00 (50.70 to 51.70): VL0

Ion 67.00 (66.70 to 67.70): VL0

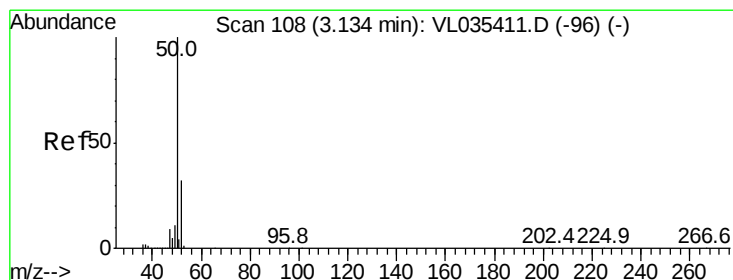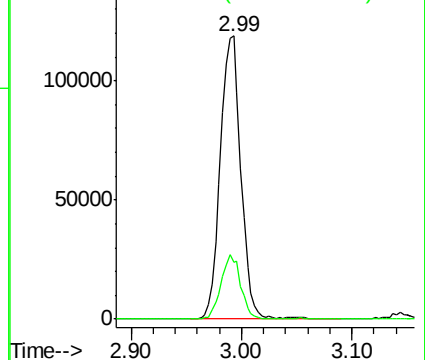

#4

Chloromethane

Concen: 1.042 ppbv

RT: 3.14 min Scan# 111

Delta R.T. 0.01 min

Lab File: VL035422.D


Acq: 17 Aug 2020 15:30

Tgt Ion: 50 Resp: 80695

Ion Ratio Lower Upper



50 100


52 29.5 25.9 38.9



Abundance Ion 50.10 (49.80 to 50.80): VL0

Ion 52.10 (51.80 to 52.80): VL0

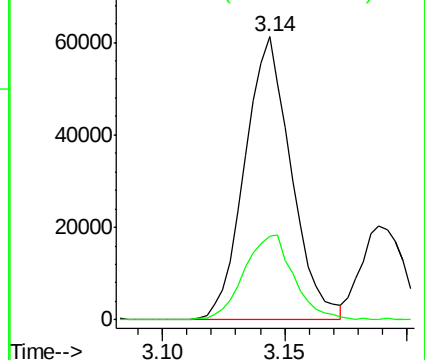



#5

Vinyl Chloride

Concen: 1.181 ppbv

RT: 3.26 min Scan# 147

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :





VSTDIC001

Tgt Ion: 62 Resp: 92971

Ion Ratio Lower Upper

62 100

64 34.3 25.0 37.4

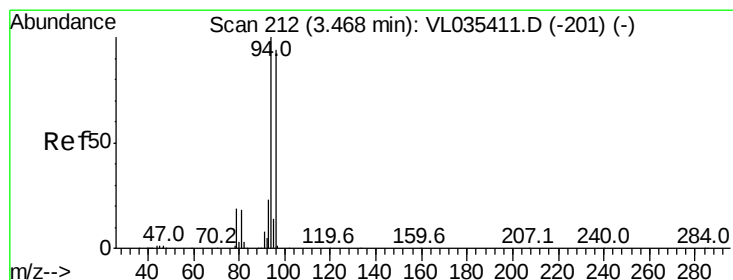

#6

Bromomethane

Concen: 1.932 ppbv

RT: 3.48 min Scan# 215

Delta R.T. 0.01 min

Lab File: VL035422.D




Acq: 17 Aug 2020 15:30


Tgt Ion: 94 Resp: 83380

Ion Ratio Lower Upper

94 100

96 93.6 75.0 112.6



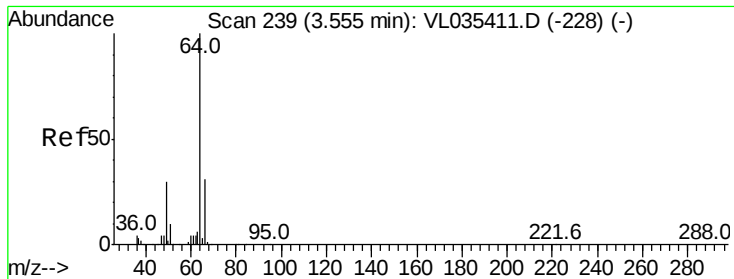

#7

Chloroethane

Concen: 1.313 ppbv

RT: 3.56 min Scan# 242

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :





VSTDIC001

Tgt Ion: 64 Resp: 34279

Ion Ratio Lower Upper

64 100

66 32.6 24.5 36.7

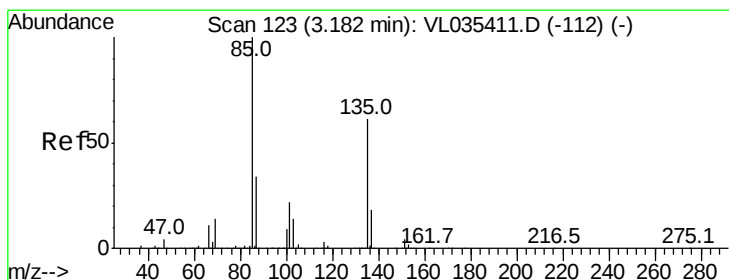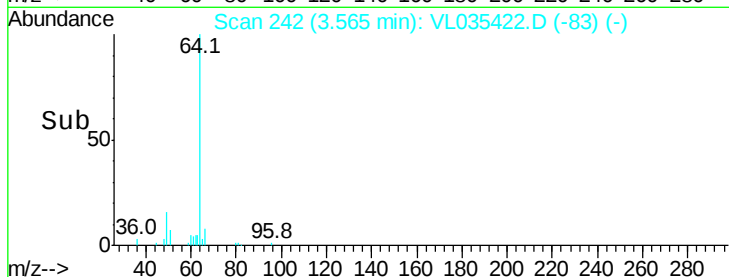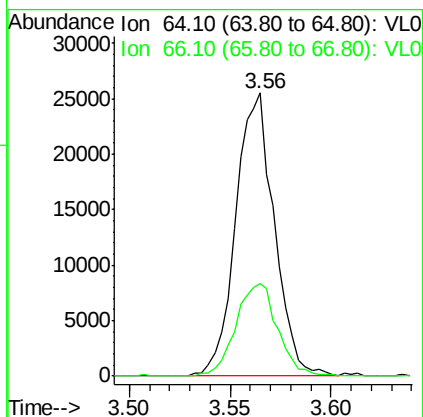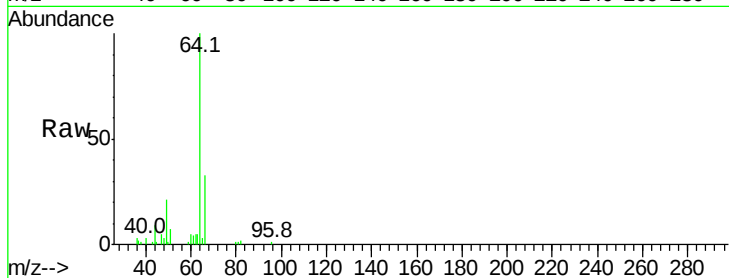

#8

Dichlorotetrafluoroethane

Concen: 1.770 ppbv

RT: 3.19 min Scan# 126

Delta R.T. 0.01 min

Lab File: VL035422.D




Acq: 17 Aug 2020 15:30


Tgt Ion: 85 Resp: 307426

Ion Ratio Lower Upper

85 100

135 93.4 48.6 72.8#

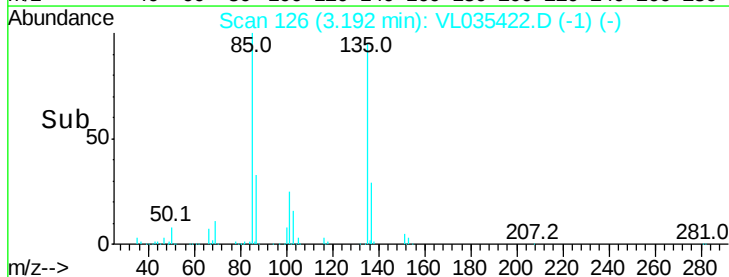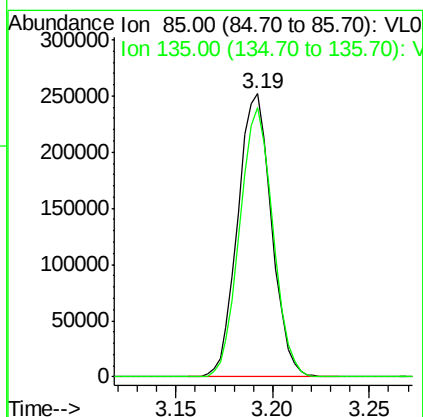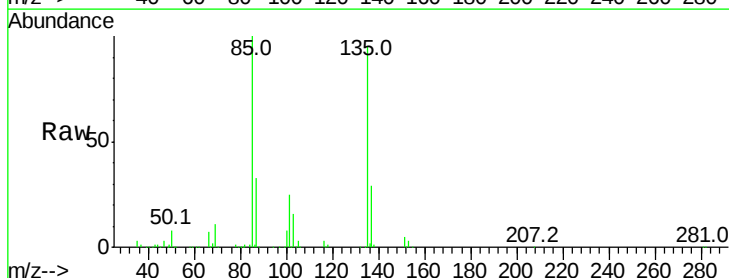



#9

Propene

Concen: 0.905 ppbv

RT: 3.01 min Scan# 69

Delta R.T. 0.00 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :





VSTDIC001

Tgt Ion: 41 Resp: 63144

Ion Ratio Lower Upper

41 100

42 68.2 55.5 83.3

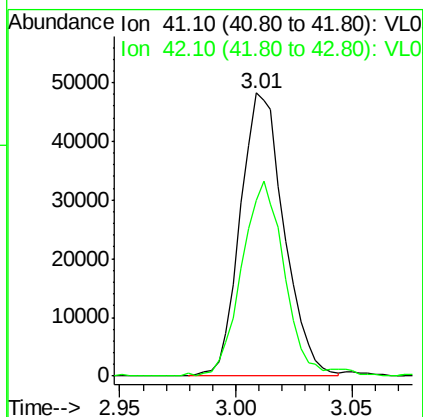

#10

Heptane

Concen: 0.928 ppbv

RT: 8.14 min Scan# 1665

Delta R.T. 0.00 min

Lab File: VL035422.D




Acq: 17 Aug 2020 15:30


Tgt Ion: 43 Resp: 163621

Ion Ratio Lower Upper

43 100

57 62.2 39.8 59.6#

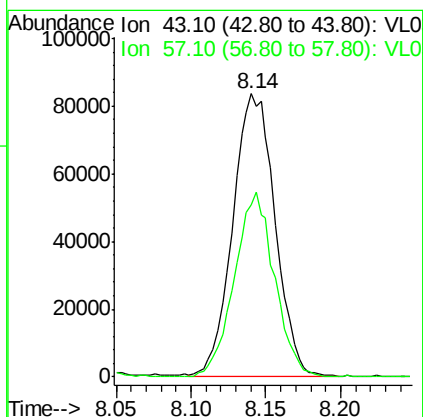



#11

Trichlorofluoromethane

Concen: 1.989 ppbv

RT: 3.96 min Scan# 364

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :





VSTDIC001

Tgt Ion:101 Resp: 363714

Ion Ratio Lower Upper

101 100

103 65.6 52.6 78.8

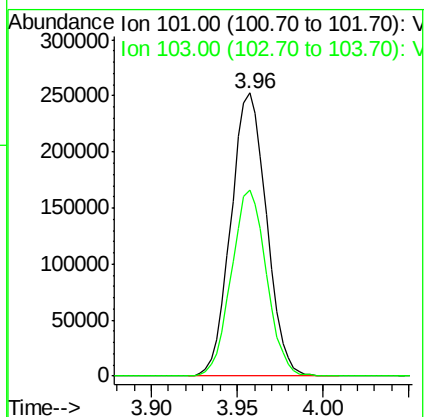

#12

1,1,2-Trichlorotrifluoroethane

Concen: 2.272 ppbv

RT: 4.49 min Scan# 531

Delta R.T. 0.01 min

Lab File: VL035422.D




Acq: 17 Aug 2020 15:30


Tgt Ion:101 Resp: 270625

Ion Ratio Lower Upper

101 100

151 85.2 53.6 80.4#

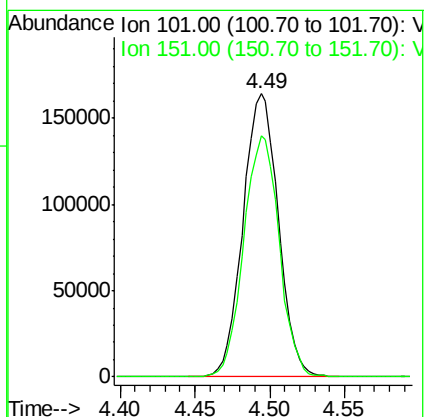



#13

Ethanol

Concen: 1.219 ppbv

RT: 3.62 min Scan# 258

Delta R.T. 0.02 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :





VSTDIC001

Tgt Ion: 45 Resp: 27170

Ion Ratio Lower Upper

45 100

46 36.3 14.2 56.6

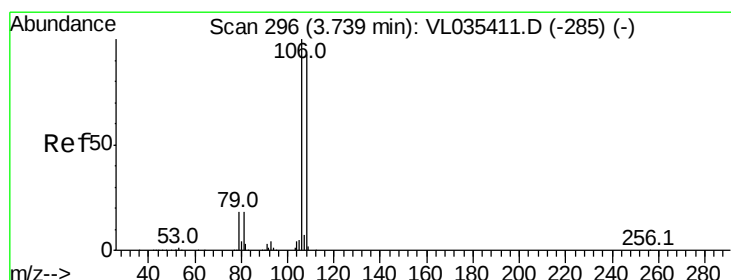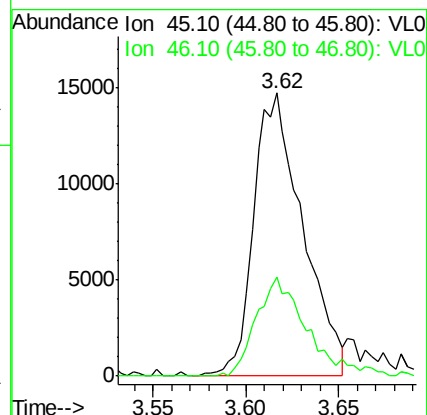

#14

Bromoethene

Concen: 2.236 ppbv

RT: 3.74 min Scan# 298

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30




Tgt Ion: 108 Resp: 116850


Ion Ratio Lower Upper

108 100

106 104.0 86.7 130.1

79 14.0 16.8 25.2#

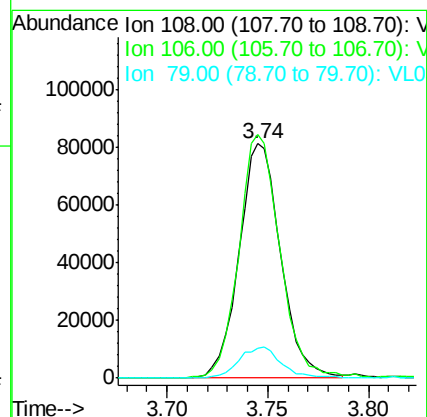



#15

Acetone

Concen: 0.977 ppbv

RT: 3.86 min Scan# 335

Delta R.T. 0.02 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :





VSTDIC001

Tgt Ion: 43 Resp: 147515

Ion Ratio Lower Upper

43 100

58 37.4 21.0 31.6#

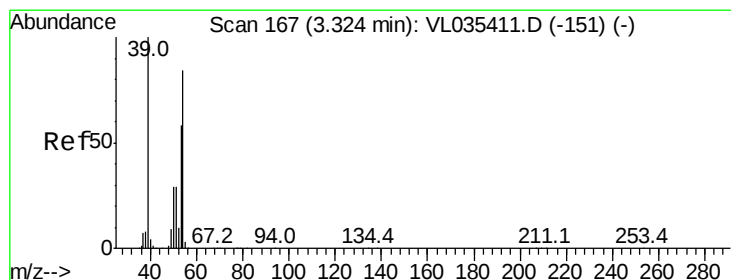

#16

1,3-Butadiene

Concen: 0.846 ppbv

RT: 3.33 min Scan# 169

Delta R.T. 0.01 min

Lab File: VL035422.D




Acq: 17 Aug 2020 15:30


Tgt Ion: 39 Resp: 58521

Ion Ratio Lower Upper

39 100

54 103.3 64.4 96.6#



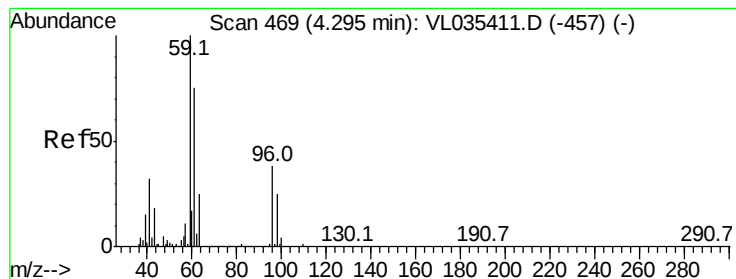

#17

tert-Butyl alcohol

Concen: 1.298 ppbv

RT: 4.30 min Scan# 472

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :


VSTDIC001

Tgt Ion: 59 Resp: 185997

Ion Ratio Lower Upper




59 100

57 10.5 8.9 13.3

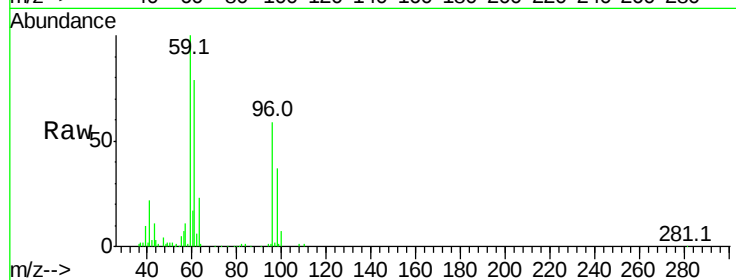

Abundance Ion 59.10 (58.80 to 59.80): VL0

Ion 57.10 (56.80 to 57.80): VL0

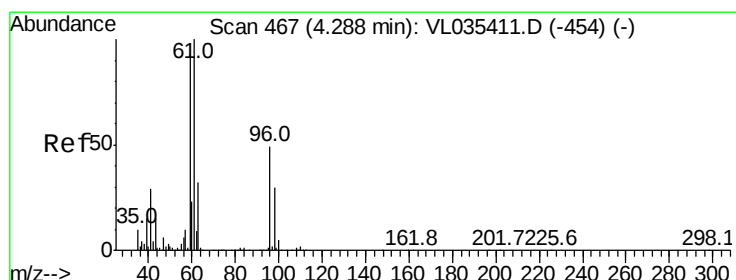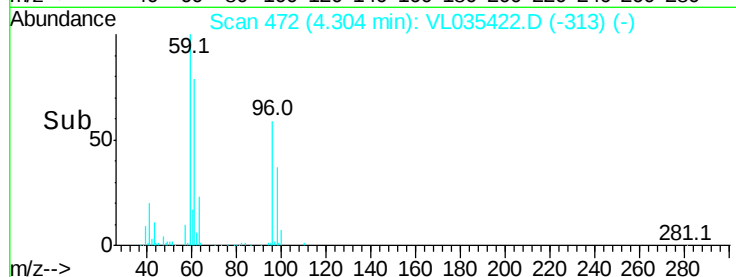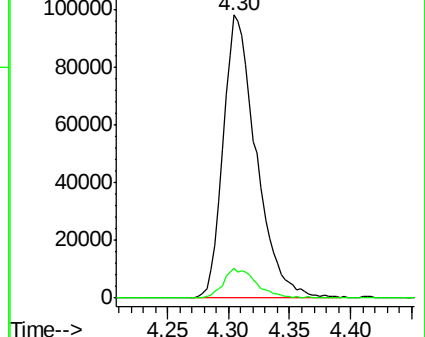

#18

1,1-Dichloroethene

Concen: 2.164 ppbv

RT: 4.30 min Scan# 470

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30


Tgt Ion: 96 Resp: 115808

Ion Ratio Lower Upper

96 100

61 129.4 161.8 242.6#



98 64.3 49.3 73.9

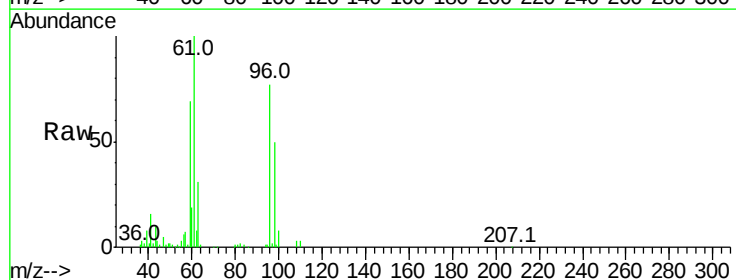


Abundance Ion 96.00 (95.70 to 96.70): VL0

Ion 61.10 (60.80 to 61.80): VL0

Ion 98.00 (97.70 to 98.70): VL0

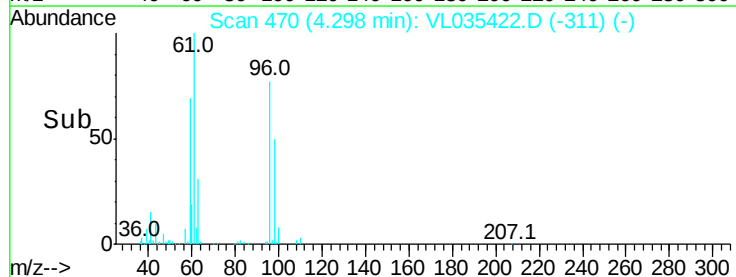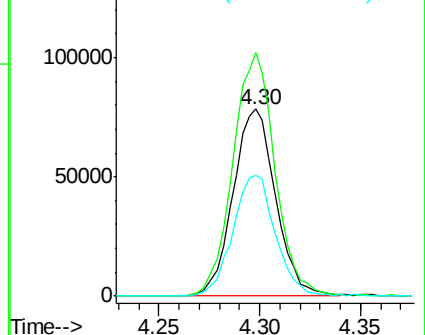

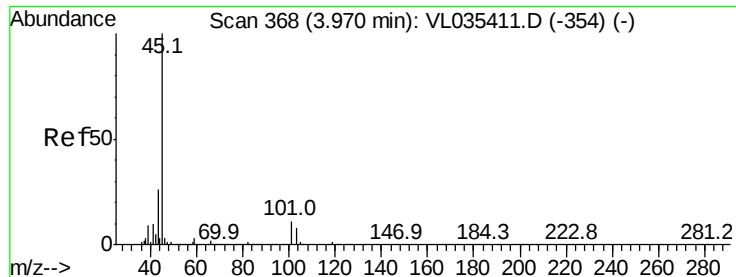

#19

Isopropyl Alcohol

Concen: 0.956 ppbv

RT: 3.98 min Scan# 372

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :





VSTDIC001

Tgt Ion: 45 Resp: 101842

Ion Ratio Lower Upper

45 100

58 3.2 1.0 1.6#

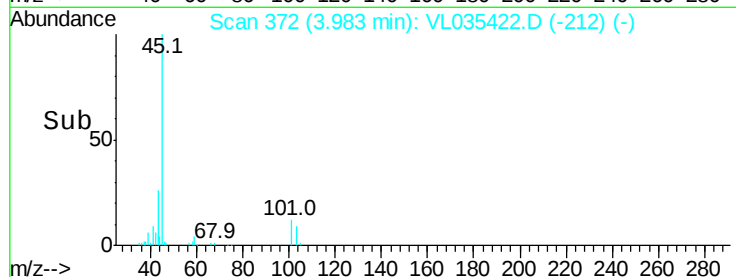

#20

Methylene Chloride

Concen: 2.135 ppbv

RT: 4.35 min Scan# 486

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Tgt Ion: 84 Resp: 119582




Ion Ratio Lower Upper


84 100

49 81.0 118.6 177.8#

51 26.8 36.4 54.6#

86 60.5 50.2 75.4

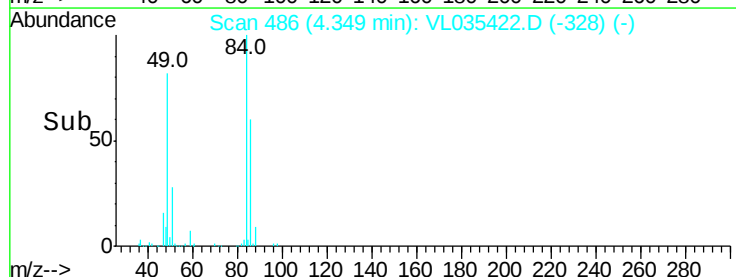

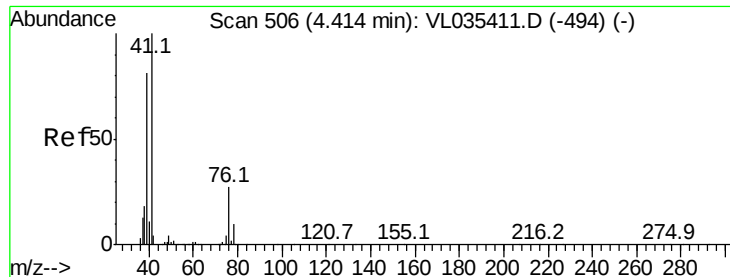

#21

Allyl Chloride

Concen: 0.786 ppbv

RT: 4.42 min Scan# 508

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :

VSTDIC001





Tgt Ion: 41 Resp: 69358

Ion Ratio Lower Upper

41 100

76 59.7 22.8 34.2#

39 88.3 66.2 99.2

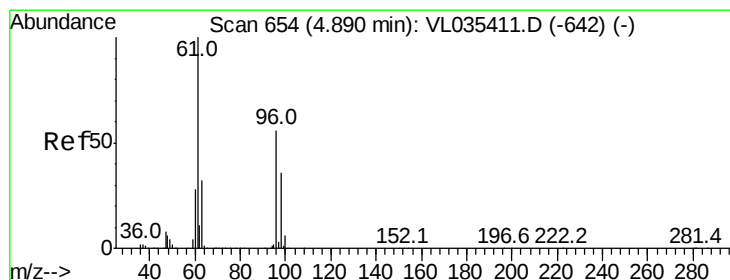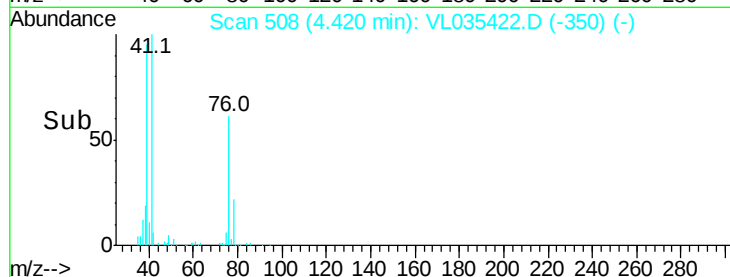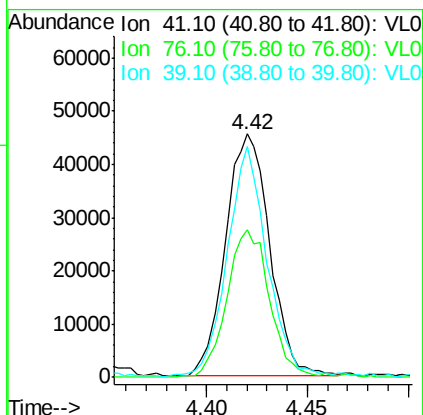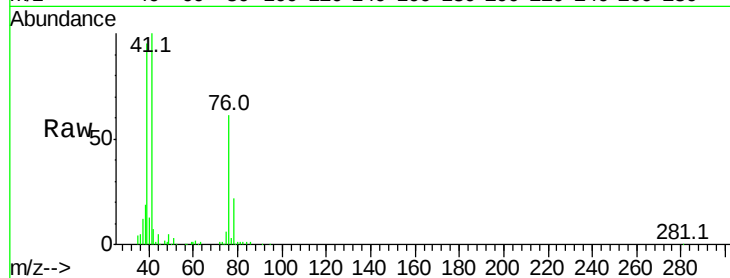

#22

trans-1,2-Dichloroethene

Concen: 2.334 ppbv

RT: 4.90 min Scan# 656

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30




Tgt Ion: 96 Resp: 124424


Ion Ratio Lower Upper

96 100

61 107.4 142.2 213.2#

98 61.9 51.8 77.8

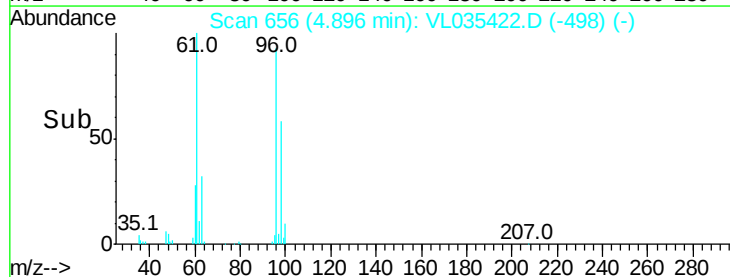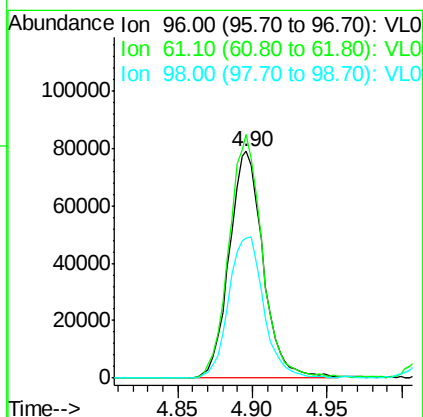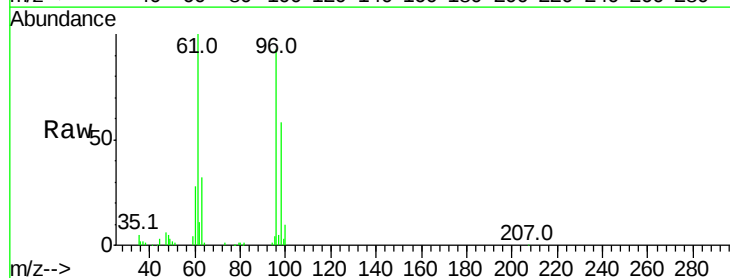



#23

Vinyl Acetate

Concen: 0.884 ppbv

RT: 5.09 min Scan# 715

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :

VSTDIC001

Tgt Ion: 43 Resp: 195708


Ion Ratio Lower Upper

43 100

86 12.2 6.5 9.7#

42 8.1 8.3 12.5#

44 5.5 4.0 6.0



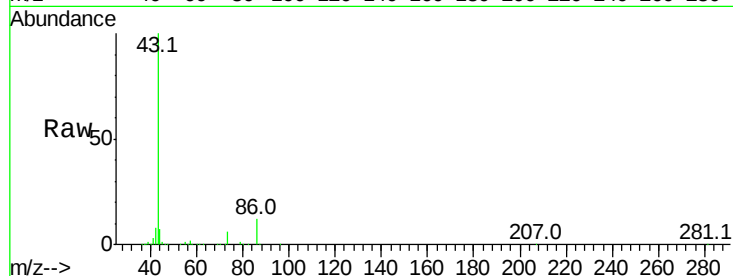


Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 86.10 (85.80 to 86.80): VL0

Ion 42.10 (41.80 to 42.80): VL0

Ion 44.10 (43.80 to 44.80): VL0

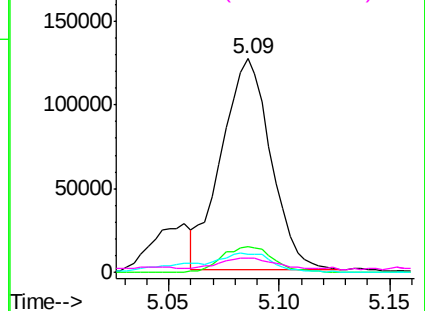

#24

1,1-Dichloroethane

Concen: 1.284 ppbv

RT: 5.02 min Scan# 695

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30


Tgt Ion: 63 Resp: 202611

Ion Ratio Lower Upper

63 100

98 6.2 2.1 6.5



100 3.4 1.3 3.8




Abundance Ion 63.10 (62.80 to 63.80): VL0

Ion 98.00 (97.70 to 98.70): VL0

Ion 100.00 (99.70 to 100.70): VL0




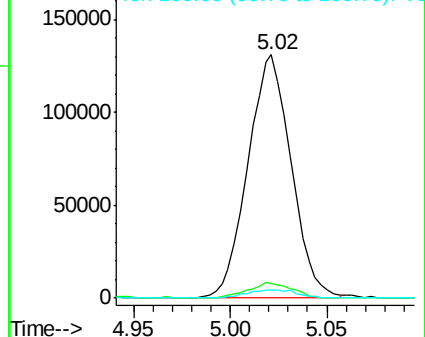




#25
Ethyl Acetate
Concen: 0.936 ppbv
RT: 5.69 min Scan# 904
Delta R.T. 0.01 min
Lab File: VL035422.D
Acq: 17 Aug 2020 15:30




Instrument :
MSVOA_L
ClientSampleId :
VSTDIC001


Tgt Ion:	43	Resp:	283118
Ion	Ratio	Lower	Upper
43	100		
45	10.3	8.3	12.5
61	13.1	7.6	11.4#
70	11.3	6.0	9.0#

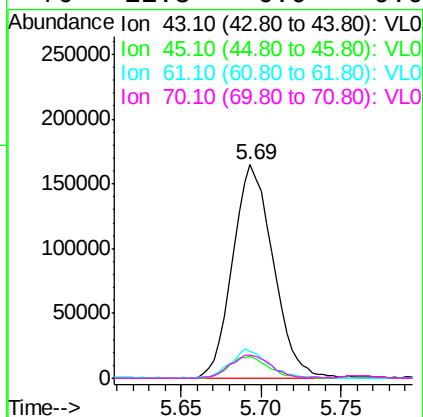

#26
Hexane
Concen: 1.224 ppbv
RT: 5.70 min Scan# 906
Delta R.T. 0.01 min
Lab File: VL035422.D
Acq: 17 Aug 2020 15:30

Tgt Ion:	57	Resp:	160847
Ion	Ratio	Lower	Upper
57	100		
41	68.8	75.5	113.3#
43	177.7	181.7	272.5#
56	52.2	42.4	63.6

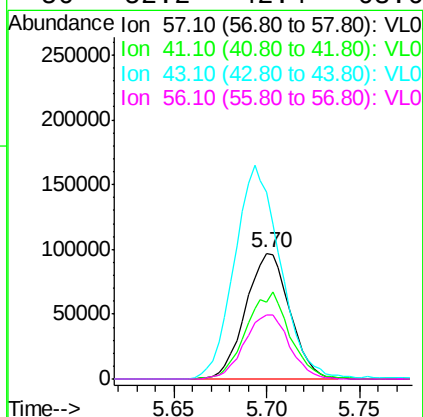

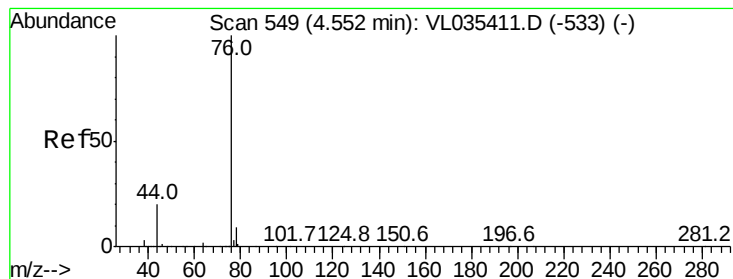

#27

Carbon Disulfide

Concen: 1.641 ppbv

RT: 4.56 min Scan# 551

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :

VSTDIC001


Tgt Ion: 76 Resp: 209899

Ion Ratio Lower Upper

76 100

44 12.7 16.8 25.2#




78 10.3 7.3 10.9



Abundance Ion 76.00 (75.70 to 76.70): VL0

Ion 44.10 (43.80 to 44.80): VL0

Ion 78.00 (77.70 to 78.70): VL0

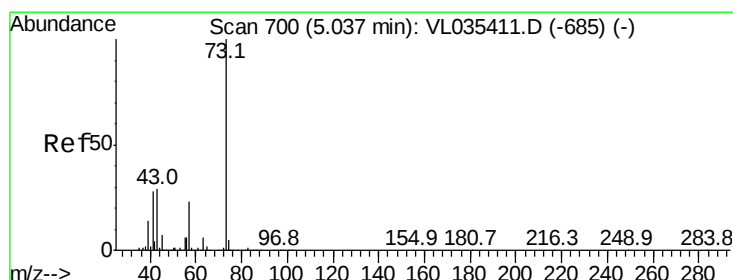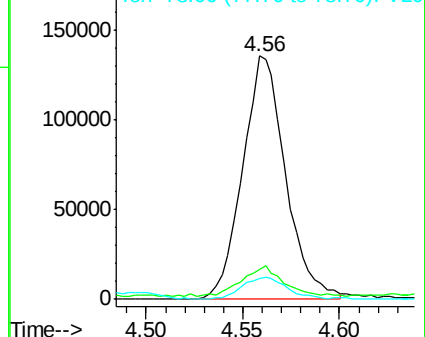

#28

Methyl tert-Butyl Ether

Concen: 1.399 ppbv

RT: 5.05 min Scan# 705

Delta R.T. 0.02 min

Lab File: VL035422.D


Acq: 17 Aug 2020 15:30

Tgt Ion: 73 Resp: 283629

Ion Ratio Lower Upper



73 100


57 18.5 18.3 27.5



Abundance Ion 73.10 (72.80 to 73.80): VL0

Ion 57.10 (56.80 to 57.80): VL0

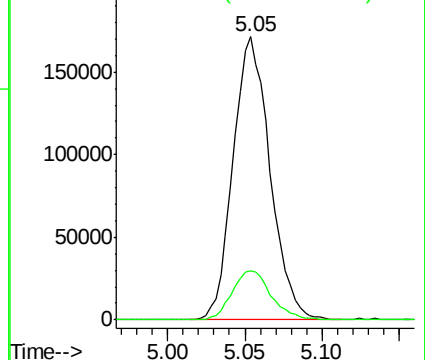



#29

Chloroform

Concen: 1.580 ppbv

RT: 5.76 min Scan# 926

Delta R.T. 0.00 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :





VSTDIC001

Tgt Ion: 83 Resp: 318794

Ion Ratio Lower Upper

83 100

85 65.5 52.7 79.1

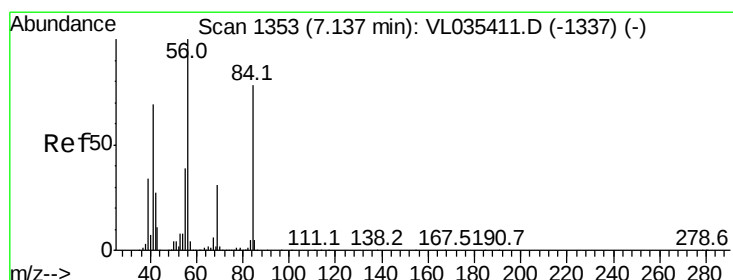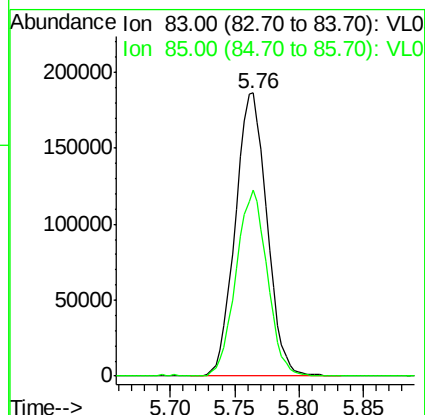

#30

Cyclohexane

Concen: 1.618 ppbv

RT: 7.15 min Scan# 1356

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30




Tgt Ion: 84 Resp: 168851


Ion Ratio Lower Upper

84 100

56 97.3 114.9 172.3#

41 47.5 72.3 108.5#

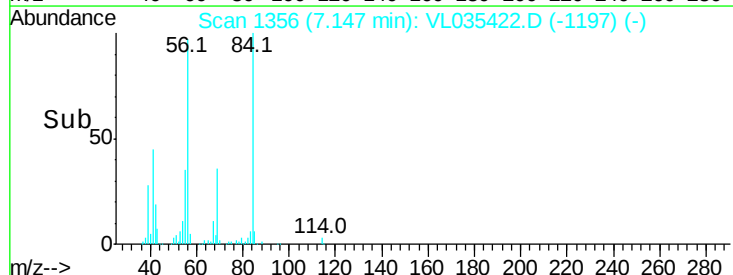

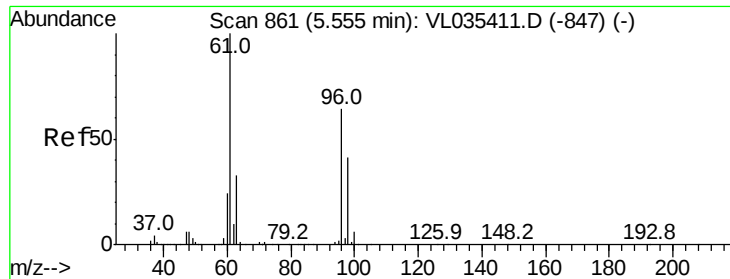

#31

cis-1,2-Dichloroethene

Concen: 1.216 ppbv

RT: 5.56 min Scan# 863

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :

VSTDIC001


Tgt Ion: 61 Resp: 162782

Ion Ratio Lower Upper

61 100

96 90.0 51.4 77.0#




98 56.2 32.9 49.3#

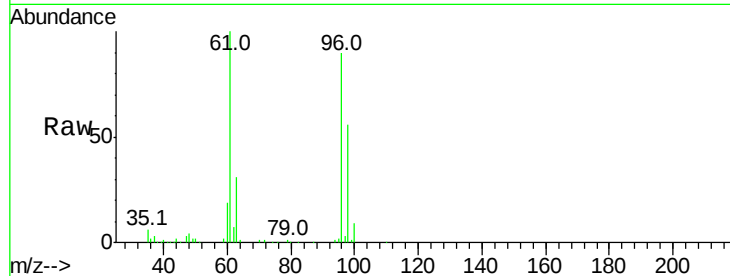

Abundance Ion 61.10 (60.80 to 61.80): VL0

Ion 96.00 (95.70 to 96.70): VL0

Ion 98.00 (97.70 to 98.70): VL0

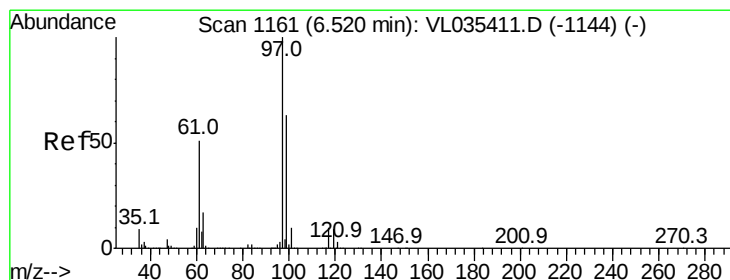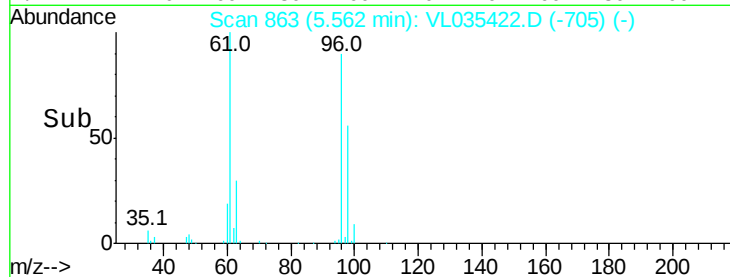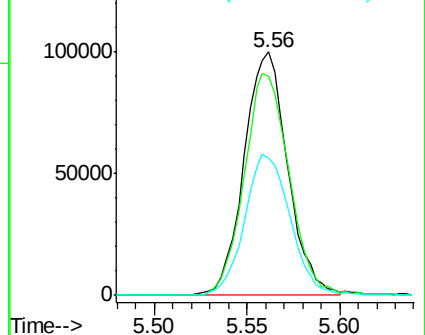

#32

1,1,1-Trichloroethane

Concen: 1.465 ppbv

RT: 6.53 min Scan# 1163

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30


Tgt Ion: 97 Resp: 294640

Ion Ratio Lower Upper

97 100

99 66.1 51.4 77.0



61 37.2 41.0 61.6#

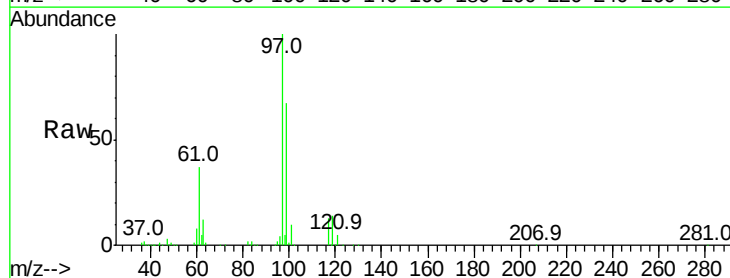


Abundance Ion 97.00 (96.70 to 97.70): VL0

Ion 99.00 (98.70 to 99.70): VL0

Ion 61.10 (60.80 to 61.80): VL0

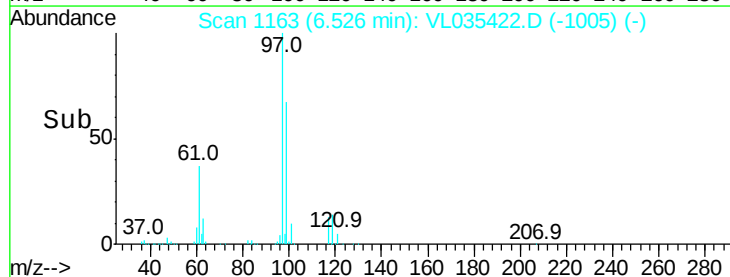
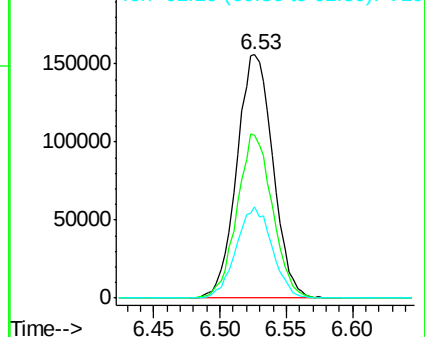


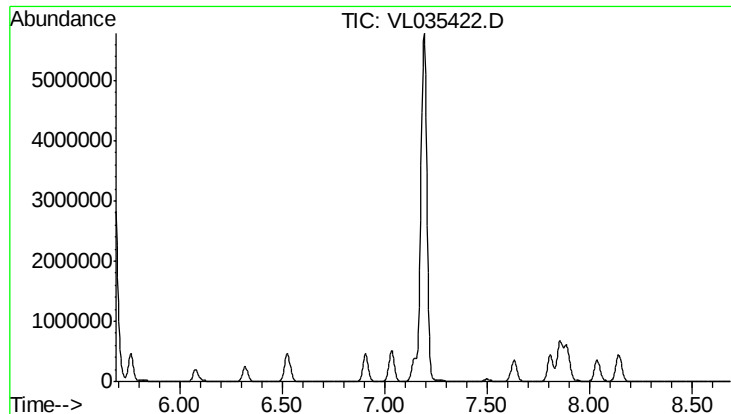

#33
 1,4-Difluorobenzene
 Concen: 0.000 ppbv
 Expected RT: 7.19 min
 Lab File: VL035422.D
 Acq: 17 Aug 2020 15:30




Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDIC001


Tgt Ion: 114
 Sig Exp Ratio
 114 100
 63 28.9
 88 19.9

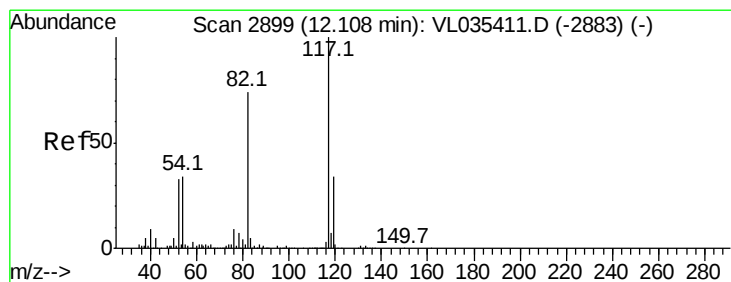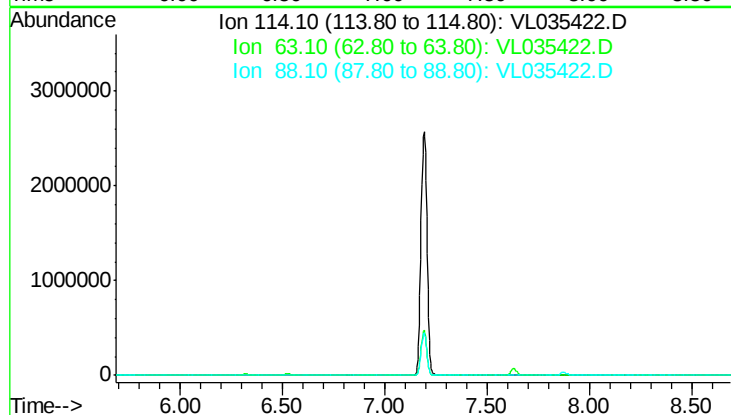

#55
 Chlorobenzene-d5
 Concen: 10.000 ppbv
 RT: 12.11 min Scan# 2901
 Delta R.T. 0.01 min
 Lab File: VL035422.D
 Acq: 17 Aug 2020 15:30

Tgt Ion: 117 Resp: 5235106
 Ion Ratio Lower Upper
 117 100
 82 51.1 57.4 86.0#
 119 37.3 28.4 42.6

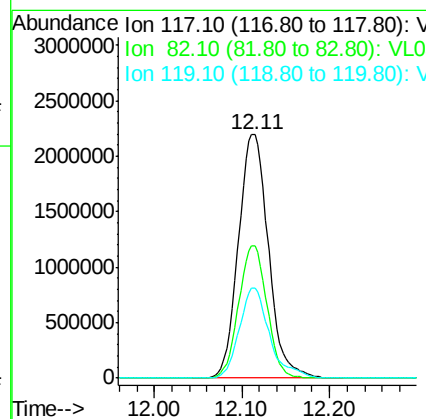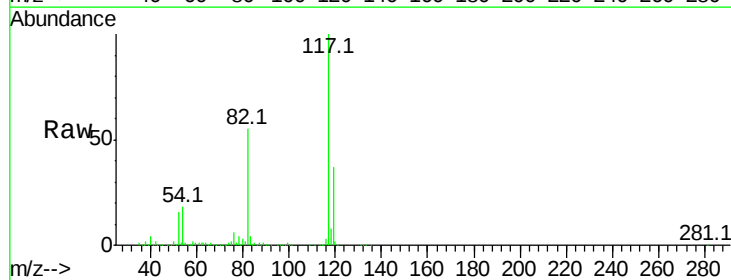

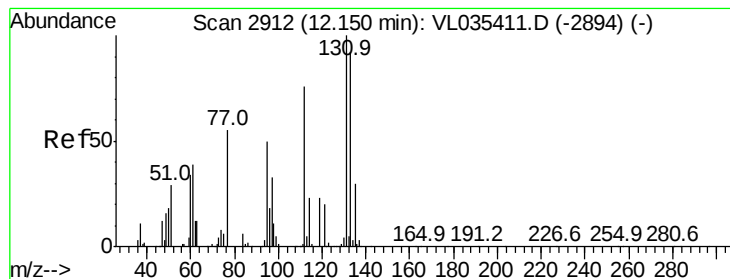

#56

1,1,1,2-Tetrachloroethane

Concen: 1.048 ppbv

RT: 12.15 min Scan# 2913

Delta R.T. 0.00 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :

VSTDIC001


Tgt Ion:131 Resp: 269950

Ion Ratio Lower Upper

131 100

133 96.3 76.1 114.1




119 723.2 50.7 76.1#

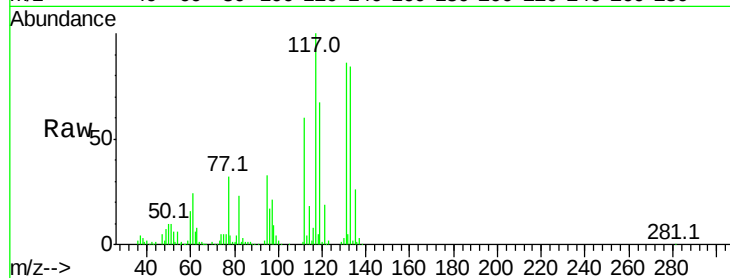

Abundance Ion 131.00 (130.70 to 131.70): V

Ion 133.00 (132.70 to 133.70): V

Ion 119.00 (118.70 to 119.70): V

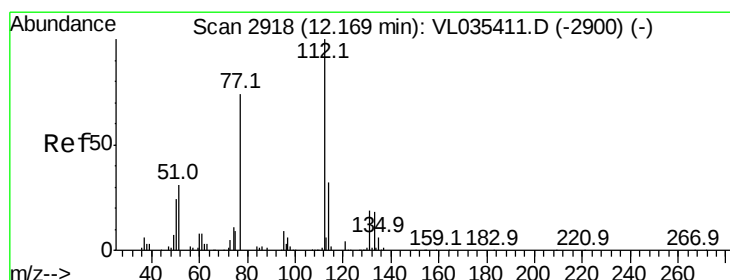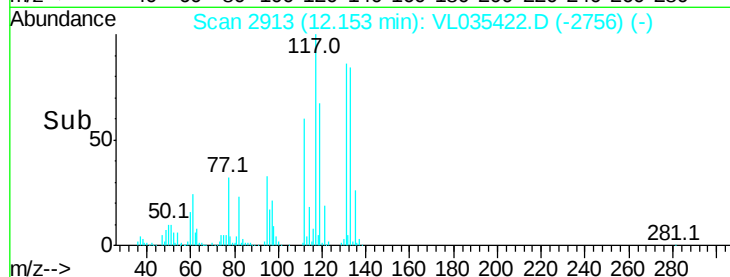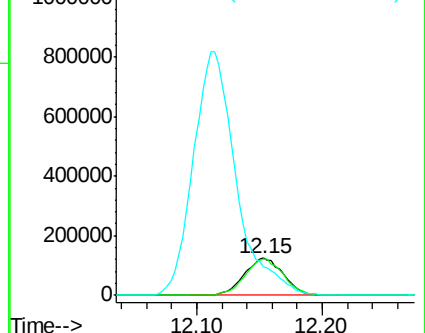

#57

Chlorobenzene

Concen: 1.064 ppbv

RT: 12.17 min Scan# 2919

Delta R.T. 0.00 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30


Tgt Ion:112 Resp: 503032

Ion Ratio Lower Upper

112 100

77 49.2 60.6 91.0#



114 30.5 28.5 34.9

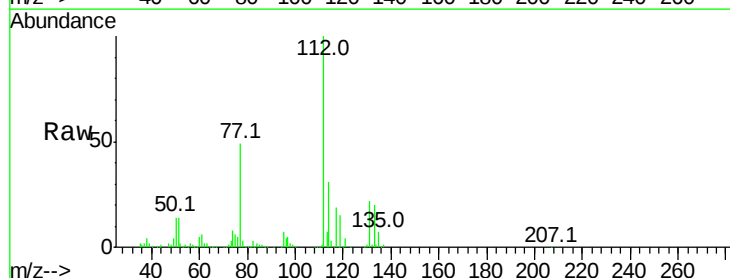


Abundance Ion 112.10 (111.80 to 112.80): V

Ion 77.10 (76.80 to 77.80): V

Ion 114.10 (113.80 to 114.80): V

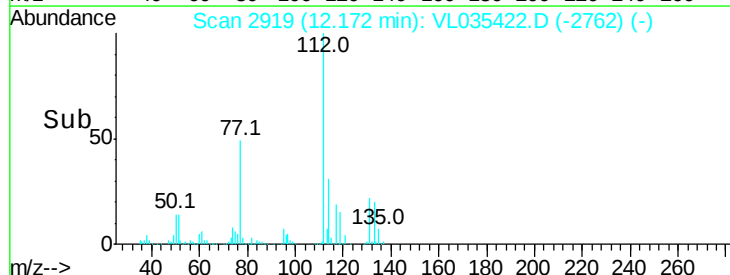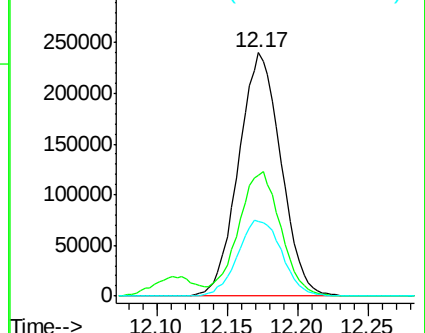

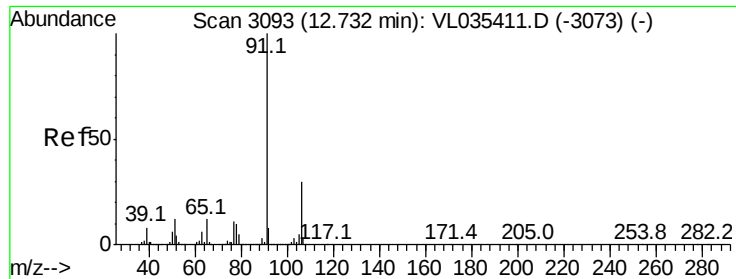

#58

Ethyl Benzene

Concen: 0.834 ppbv

RT: 12.74 min Scan# 3095

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :





VSTDIC001

Tgt Ion: 91 Resp: 723109

Ion Ratio Lower Upper

91 100

106 32.9 24.1 36.1

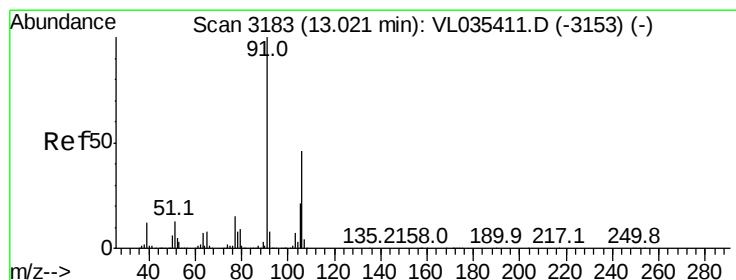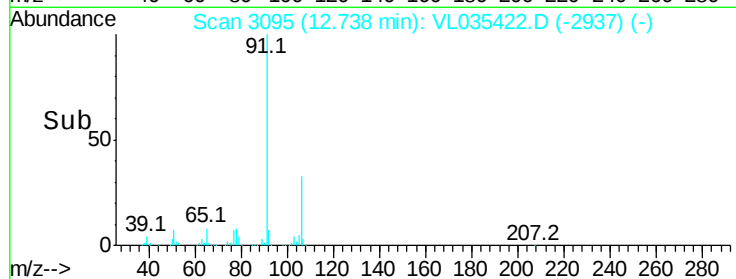

#59

m/p-Xylene

Concen: 0.902 ppbv

RT: 13.02 min Scan# 3184

Delta R.T. 0.00 min

Lab File: VL035422.D




Acq: 17 Aug 2020 15:30


Tgt Ion: 91 Resp: 651937

Ion Ratio Lower Upper

91 100

106 0.0 34.0 51.0#


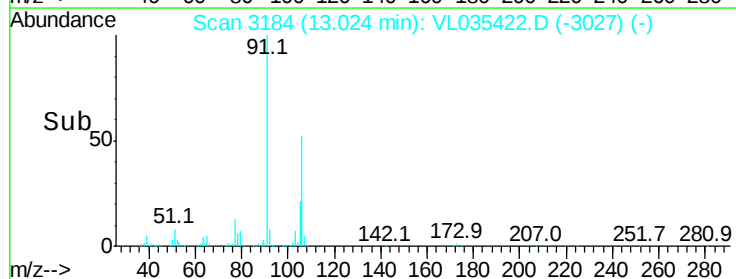

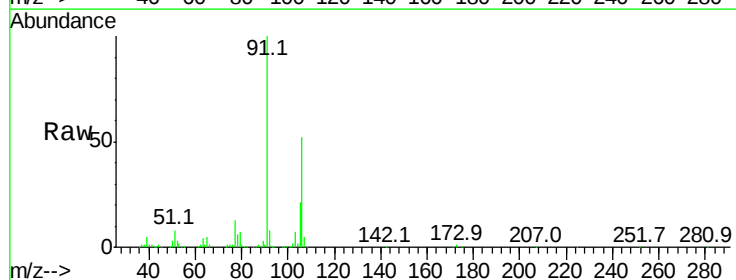


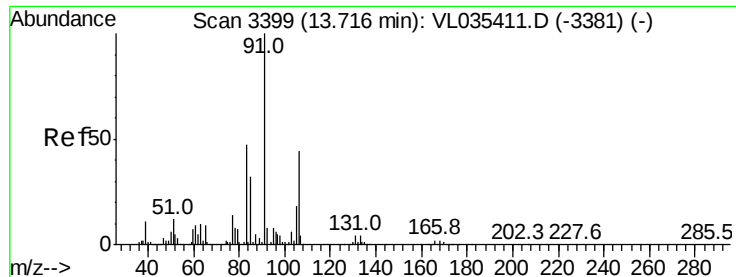

#60
o-Xylene
Concen: 0.838 ppbv
RT: 13.72 min Scan# 3400
Delta R.T. 0.00 min
Lab File: VL035422.D
Acq: 17 Aug 2020 15:30




Instrument :
MSVOA_L
ClientSampleId :
VSTDIC001


Tgt Ion: 91 Resp: 596358
Ion Ratio Lower Upper
91 100
106 50.3 21.8 65.3

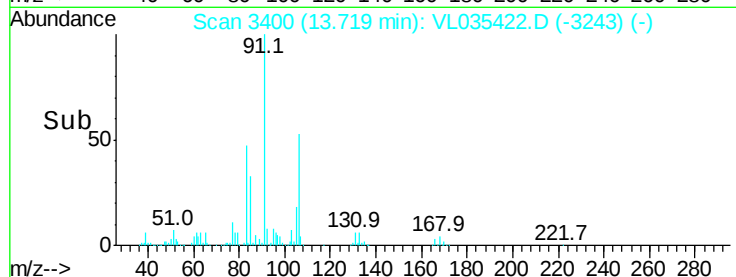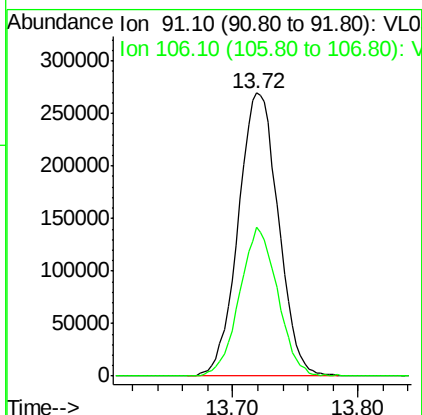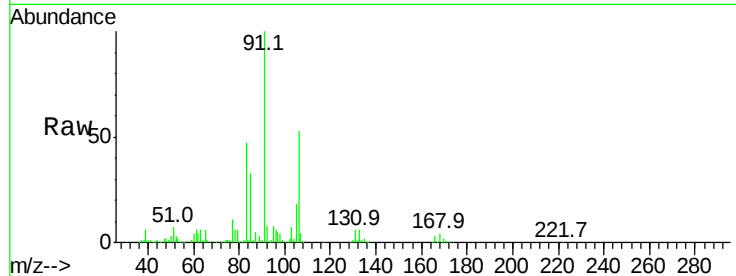

#61
Styrene
Concen: 0.959 ppbv
RT: 13.56 min Scan# 3350
Delta R.T. 0.01 min
Lab File: VL035422.D
Acq: 17 Aug 2020 15:30

Tgt Ion: 104 Resp: 466055
Ion Ratio Lower Upper
104 100
78 40.7 45.4 68.2#
103 44.9 37.8 56.8

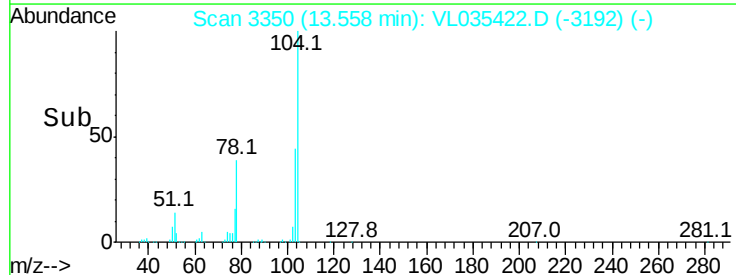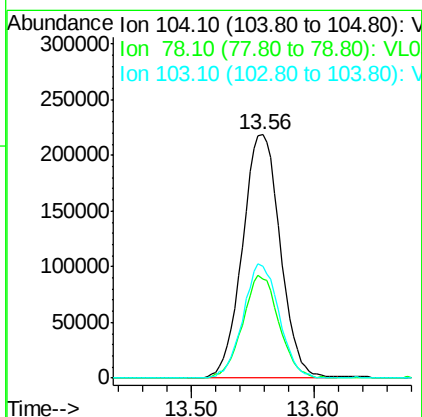

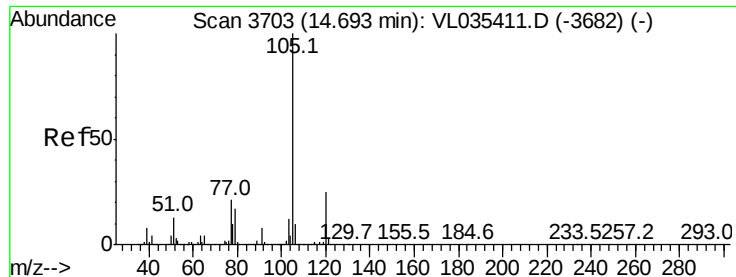

#62

Isopropylbenzene

Concen: 0.953 ppbv

RT: 14.70 min Scan# 3705

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :


VSTDIC001

Tgt Ion:105 Resp: 1001253

Ion Ratio Lower Upper

105 100

120 28.4 20.3 30.5

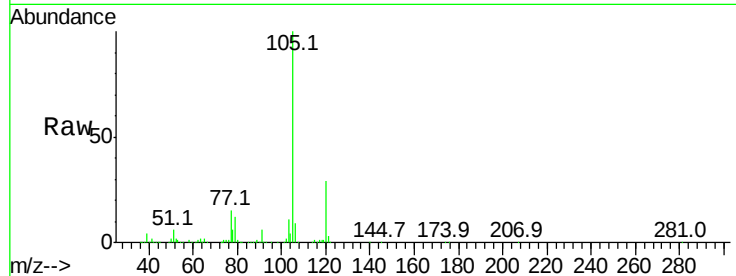

Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

14.70

400000



300000

200000

100000

0

Time--> 14.60 14.70 14.80

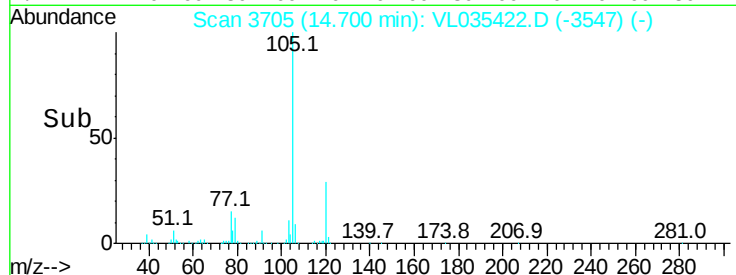

#63

1,1,2,2-Tetrachloroethane

Concen: 0.776 ppbv

RT: 13.70 min Scan# 3395

Delta R.T. 0.00 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30


Tgt Ion: 83 Resp: 428358

Ion Ratio Lower Upper

83 100

131 11.7 4.5 13.4

85 65.8 32.7 98.1

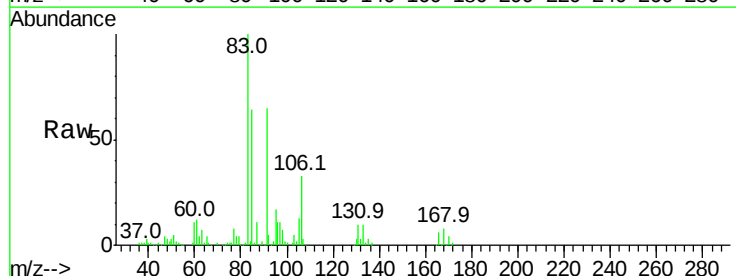

Abundance Ion 83.00 (82.70 to 83.70): VL0

Ion 131.00 (130.70 to 131.70): V

Ion 85.00 (84.70 to 85.70): VL0

13.70

250000

200000


150000


100000

50000

0

Time--> 13.60 13.70 13.80




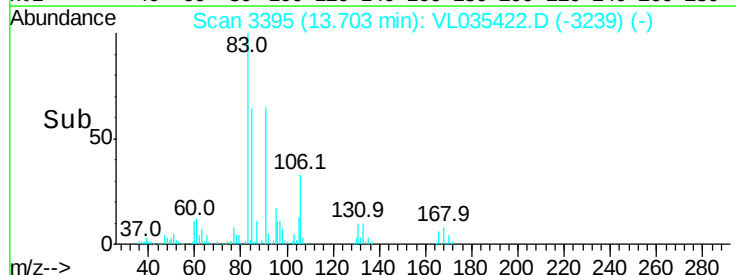


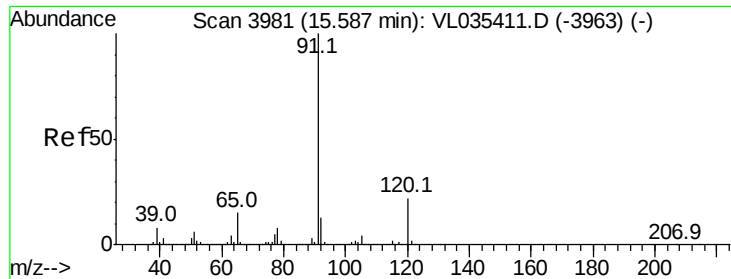

#64
n-propylbenzene
Concen: 1.085 ppbv
RT: 15.59 min Scan# 3983
Delta R.T. 0.01 min
Lab File: VL035422.D
Acq: 17 Aug 2020 15:30




Instrument :
MSVOA_L
ClientSampleId :
VSTDIC001


Tgt Ion:120 Resp: 288946
Ion Ratio Lower Upper
120 100
91 400.5 385.5 578.3

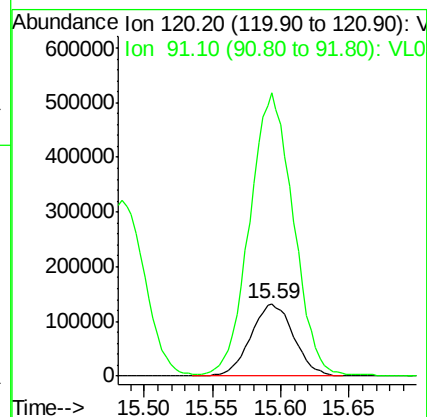

#65
tert-Butylbenzene
Concen: 1.085 ppbv
RT: 16.78 min Scan# 4352
Delta R.T. 0.01 min
Lab File: VL035422.D
Acq: 17 Aug 2020 15:30

Tgt Ion:119 Resp: 976269
Ion Ratio Lower Upper
119 100
91 66.2 72.0 108.0#
134 22.1 15.7 23.5

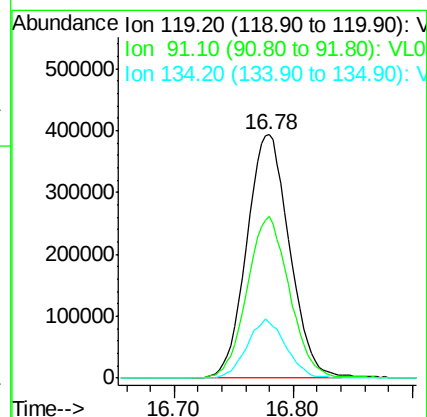

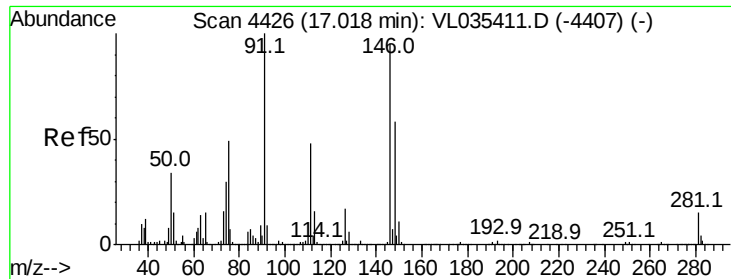

#66

Benzyl Chloride

Concen: 0.573 ppbv

RT: 17.03 min Scan# 4429

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :

VSTDIC001


Tgt Ion: 91 Resp: 168899

Ion Ratio Lower Upper

91 100

126 21.1 13.3 19.9#




128 6.4 4.1 6.1#



Abundance Ion 91.10 (90.80 to 91.80): VL0

Ion 126.10 (125.80 to 126.80): V

Ion 128.10 (127.80 to 128.80): V

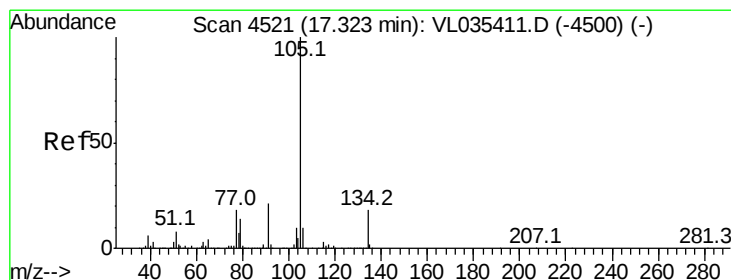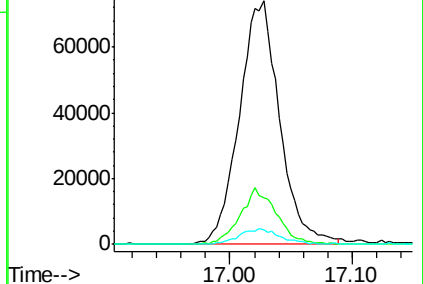

#67

sec-Butylbenzene

Concen: 0.991 ppbv

RT: 17.33 min Scan# 4523

Delta R.T. 0.01 min

Lab File: VL035422.D


Acq: 17 Aug 2020 15:30

Tgt Ion: 105 Resp: 1316160

Ion Ratio Lower Upper



105 100


134 21.0 14.1 21.1



Abundance Ion 105.10 (104.80 to 105.80): V

Ion 134.20 (133.90 to 134.90): V




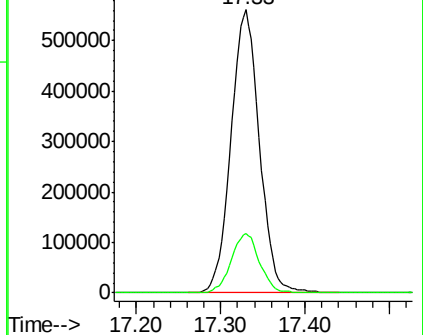




#68
 1-Bromo-4-Fluorobenzene
 Concen: 8.274 ppbv
 RT: 14.45 min Scan# 3626
 Delta R.T. 0.01 min
 Lab File: VL035422.D
 Acq: 17 Aug 2020 15:30




Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDIC001


Tgt Ion: 95 Resp: 3668232
 Ion Ratio Lower Upper
 95 100
 174 95.4 44.0 66.0#
 175 7.0 3.2 4.8#

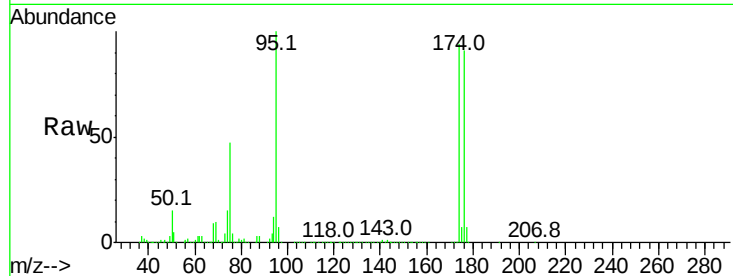

#69
 p-Isopropyltoluene
 Concen: 1.064 ppbv
 RT: 17.69 min Scan# 4634
 Delta R.T. 0.01 min
 Lab File: VL035422.D
 Acq: 17 Aug 2020 15:30

Tgt Ion: 119 Resp: 1151228
 Ion Ratio Lower Upper
 119 100
 134 28.2 20.6 30.8
 91 23.6 26.6 39.8#


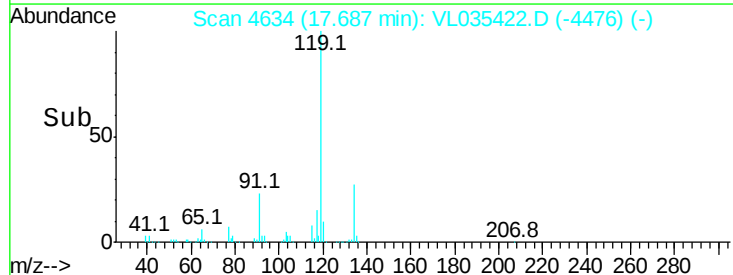






#70
n-Butylbenzene
Concen: 0.858 ppbv
RT: 18.59 min Scan# 4914
Delta R.T. 0.01 min
Lab File: VL035422.D
Acq: 17 Aug 2020 15:30




Instrument :
MSVOA_L
ClientSampleId :
VSTDIC001


Tgt Ion: 91 Resp: 1085243
Ion Ratio Lower Upper
91 100
92 54.1 44.8 67.2
134 28.7 17.3 25.9#

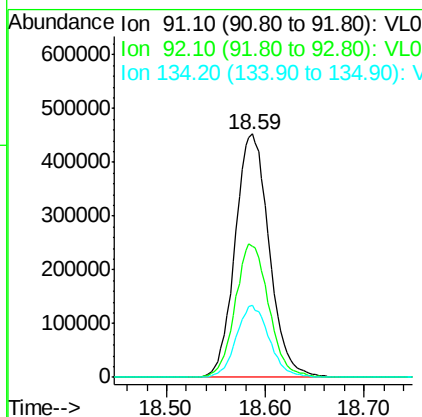

#71
2-Chlorotoluene
Concen: 0.819 ppbv
RT: 15.48 min Scan# 3949
Delta R.T. 0.01 min
Lab File: VL035422.D
Acq: 17 Aug 2020 15:30

Tgt Ion: 91 Resp: 703913
Ion Ratio Lower Upper
91 100
126 38.3 11.4 45.6

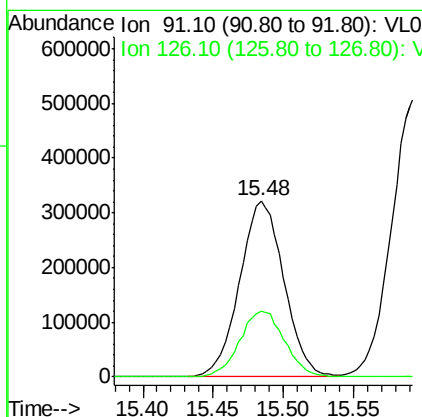

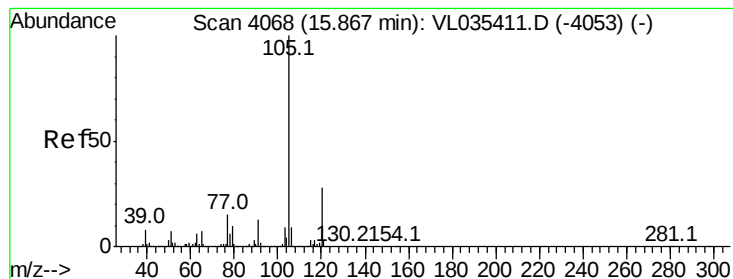

#72

4-Ethyltoluene

Concen: 0.943 ppbv

RT: 15.87 min Scan# 4070

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30





Instrument :

MSVOA_L

ClientSampleId :

VSTDIC001

Tgt Ion:	105	Resp:	785927
Ion Ratio	Lower	Upper	
105	100		
120	32.7	22.7	34.1
91	10.8	10.8	16.2
77	10.6	11.9	17.9#

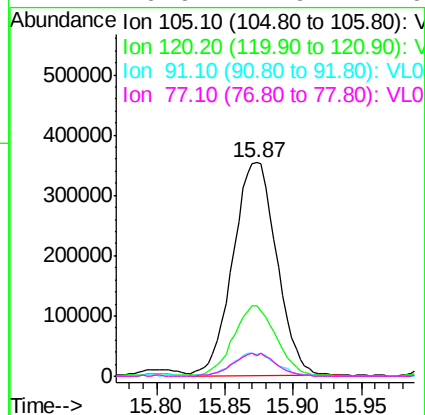

#73

1,3,5-Trimethylbenzene

Concen: 0.935 ppbv




RT: 16.03 min Scan# 4119


Delta R.T. 0.00 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Tgt Ion:	105	Resp:	735560
Ion Ratio	Lower	Upper	
105	100		
120	54.0	35.6	53.4#









#74
 1,2,4-Trimethylbenzene
 Concen: 0.962 ppbv
 RT: 16.80 min Scan# 4357
 Delta R.T. 0.00 min
 Lab File: VL035422.D
 Acq: 17 Aug 2020 15:30




Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDIC001


Tgt Ion	Ratio	Lower	Upper
105	100		
120	53.0	37.8	56.8
91	42.8	40.0	60.0
77	16.9	18.8	28.2

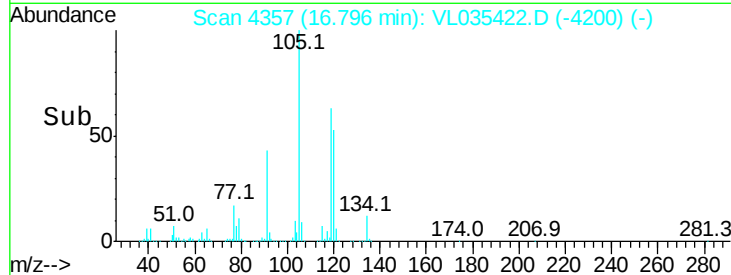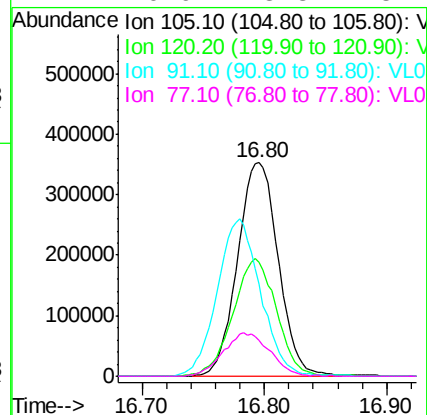

#75
 1,3-Dichlorobenzene
 Concen: 1.348 ppbv
 RT: 17.03 min Scan# 4430
 Delta R.T. 0.01 min
 Lab File: VL035422.D
 Acq: 17 Aug 2020 15:30

Tgt Ion	Ratio	Lower	Upper
146	100		
111	38.2	25.6	76.8
148	64.4	32.3	96.9

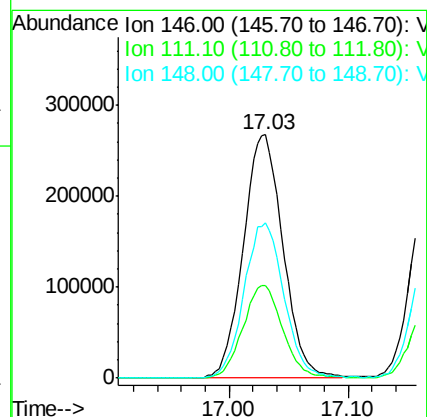

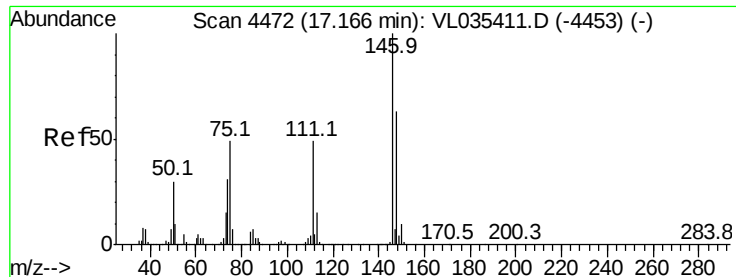

#76

1,4-Dichlorobenzene

Concen: 1.275 ppbv

RT: 17.17 min Scan# 4474

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :

VSTDIC001


Tgt Ion:146 Resp: 599934

Ion Ratio Lower Upper

146 100

111 37.3 24.8 74.4




148 66.9 32.1 96.3

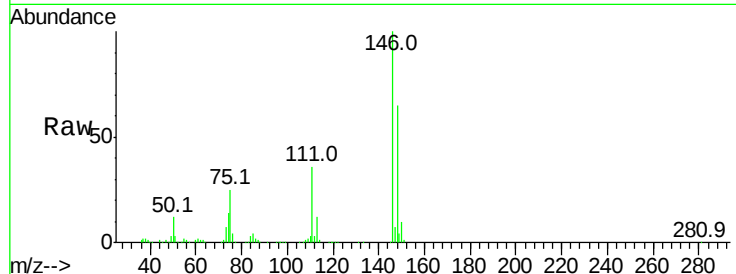

Abundance Ion 146.00 (145.70 to 146.70): V

Ion 111.10 (110.80 to 111.80): V

Ion 148.00 (147.70 to 148.70): V

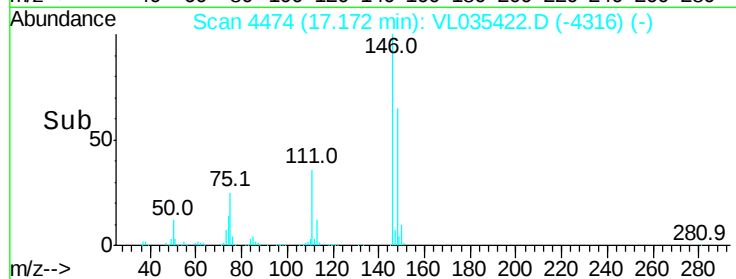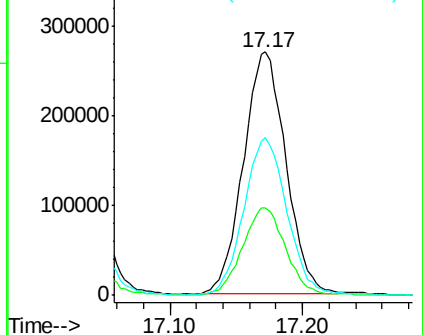

#77

1,2-Dichlorobenzene

Concen: 1.303 ppbv

RT: 17.85 min Scan# 4686

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30


Tgt Ion:146 Resp: 602374

Ion Ratio Lower Upper

146 100

111 39.5 26.3 78.9



148 64.6 32.0 96.0




Abundance Ion 146.00 (145.70 to 146.70): V

Ion 111.10 (110.80 to 111.80): V

Ion 148.00 (147.70 to 148.70): V

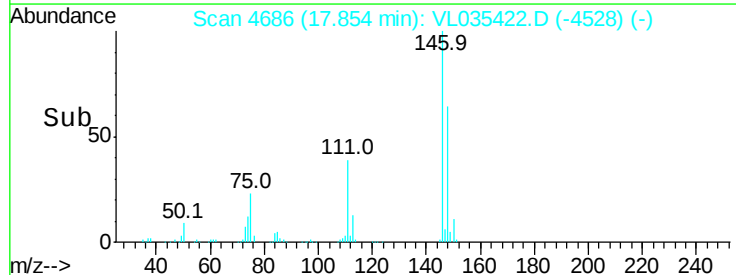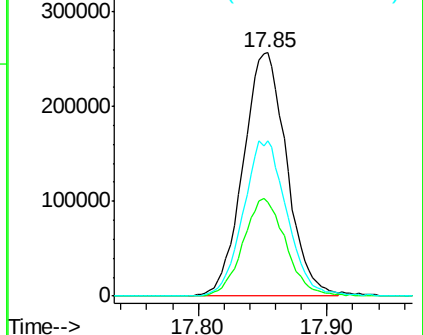

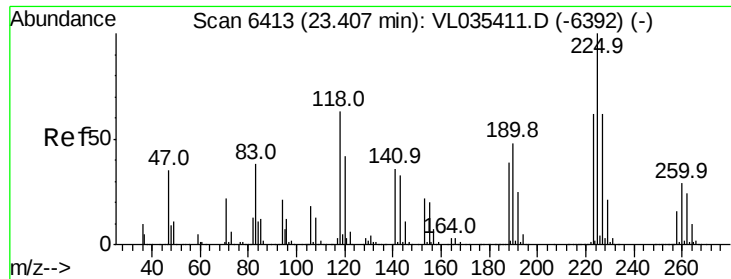

#78

Hexachloro-1,3-Butadiene

Concen: 1.358 ppbv

RT: 23.42 min Scan# 6416

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30

Instrument :

MSVOA_L

ClientSampleId :

VSTDIC001


Tgt Ion:225 Resp: 482274

Ion Ratio Lower Upper

225 100

223 62.9 50.3 75.5




227 63.4 51.0 76.6



Abundance Ion 224.90 (224.60 to 225.60): V

Ion 222.90 (222.60 to 223.60): V

Ion 226.90 (226.60 to 227.60): V

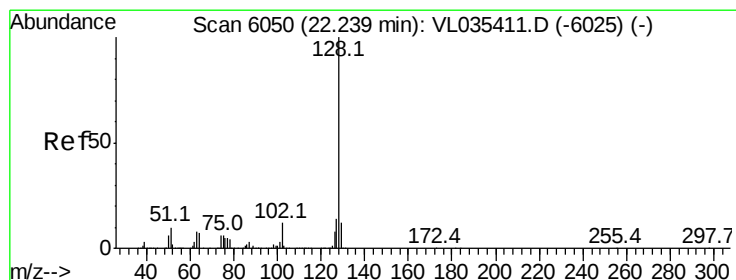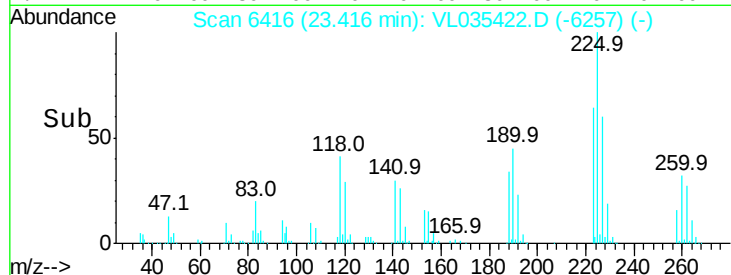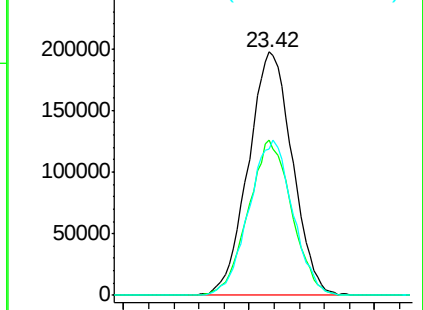

#79

Naphthalene

Concen: 1.145 ppbv

RT: 22.25 min Scan# 6053

Delta R.T. 0.01 min

Lab File: VL035422.D

Acq: 17 Aug 2020 15:30


Tgt Ion:128 Resp: 1126851

Ion Ratio Lower Upper

128 100

127 12.6 11.4 17.0



129 11.2 9.5 14.3




Abundance Ion 128.10 (127.80 to 128.80): V

Ion 127.10 (126.80 to 127.80): V

Ion 129.10 (128.80 to 129.80): V




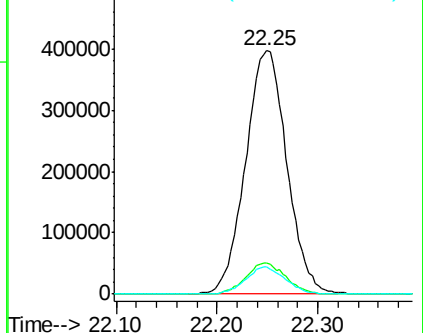




#80
Naphthalene, 2-methyl-
Concen: 0.988 ppbv
RT: 25.01 min Scan# 6912
Delta R.T. 0.01 min
Lab File: VL035422.D
Acq: 17 Aug 2020 15:30

Instrument :
MSVOA_L
ClientSampleId :
VSTDIC001

Tgt Ion	Ratio	Lower	Upper
142	100		
141	85.6	67.1	100.7
115	29.4	36.1	54.1

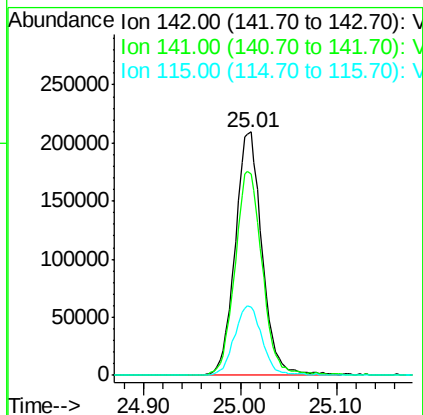

#81
1,2,4-Trichlorobenzene
Concen: 1.443 ppbv
RT: 21.98 min Scan# 5968
Delta R.T. 0.01 min
Lab File: VL035422.D
Acq: 17 Aug 2020 15:30

Tgt Ion	Ratio	Lower	Upper
180	100		
182	95.9	76.6	115.0
184	30.8	24.8	37.2

