

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL081722\
 Data File : VL039551.D
 Acq On : 17 Aug 2022 16:57
 Operator : SY/AP
 Sample : N4125-02
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 IA1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 08/18/2022
 Supervised By :Mahesh Dadoda 08/19/2022

Quant Time: Aug 18 05:38:43 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081722AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Aug 17 12:06:24 2022

QLast Update : Wed Aug 17 12:06:24 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.208	49	1078662	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.664	114	2740177	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.471	117	2436989	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.783	95	1873592	10.213	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.100%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	2.754	85	29654	0.205	ppbv	94
3) Chlorodifluoromethane	2.700	51	48102m	0.372	ppbv	
4) Chloromethane	2.838	50	36970	0.478	ppbv	91
9) Propene	2.726	41	73777	1.253	ppbv #	74
10) Heptane	7.587	43	190997	1.396	ppbv	99
11) Trichlorofluoromethane	3.587	101	32094	0.202	ppbv	86
13) Ethanol	3.256	45	544391	128.438	ppbv	82
15) Acetone	3.488	43	2001775	16.426	ppbv	100
17) tert-Butyl alcohol	3.922	59	33376m	0.321	ppbv	
19) Isopropyl Alcohol	3.600	45	223737	3.757	ppbv #	100
20) Methylene Chloride	3.954	84	1313195	26.466	ppbv	92
25) Ethyl Acetate	5.224	43	1340752	5.160	ppbv	98
26) Hexane	5.230	57	616143	5.782	ppbv	90
27) Carbon Disulfide	4.140	76	12724	0.112	ppbv #	63
30) Cyclohexane	6.613	84	9367m	0.106	ppbv	
32) 1,1,1-Trichloroethane	6.021	97	6261m	0.040	ppbv	
34) 2-Butanone	4.806	43	302819	2.198	ppbv	98
35) Carbon Tetrachloride	6.507	117	8139m	0.053	ppbv	
36) Benzene	6.381	78	38634	0.185	ppbv #	80
44) 2,2,4-Trimethylpentane	7.333	57	42113m	0.120	ppbv	
50) 4-Methyl-2-Pentanone	8.204	43	111765m	0.527	ppbv	
52) Tetrachloroethene	10.613	164	3290m	0.040	ppbv	
53) Toluene	9.230	91	826644	3.533	ppbv	99
58) Ethyl Benzene	12.098	91	107983	0.383	ppbv	91
59) m/p-Xylene	12.349	91	360184	1.420	ppbv #	100
60) o-Xylene	13.066	91	102587	0.422	ppbv	96
61) Styrene	12.912	104	21166m	0.163	ppbv	
74) 1,2,4-Trimethylbenzene	16.117	105	48611m	0.167	ppbv	
79) Naphthalene	21.387	128	34492m	0.166	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL081722\
Data File : VL039551.D
Acq On : 17 Aug 2022 16:57
Operator : SY/AP
Sample : N4125-02
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
IA1

Quant Time: Aug 18 05:38:43 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081722AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Aug
QLast Update : Wed Aug 17 12:06:24 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

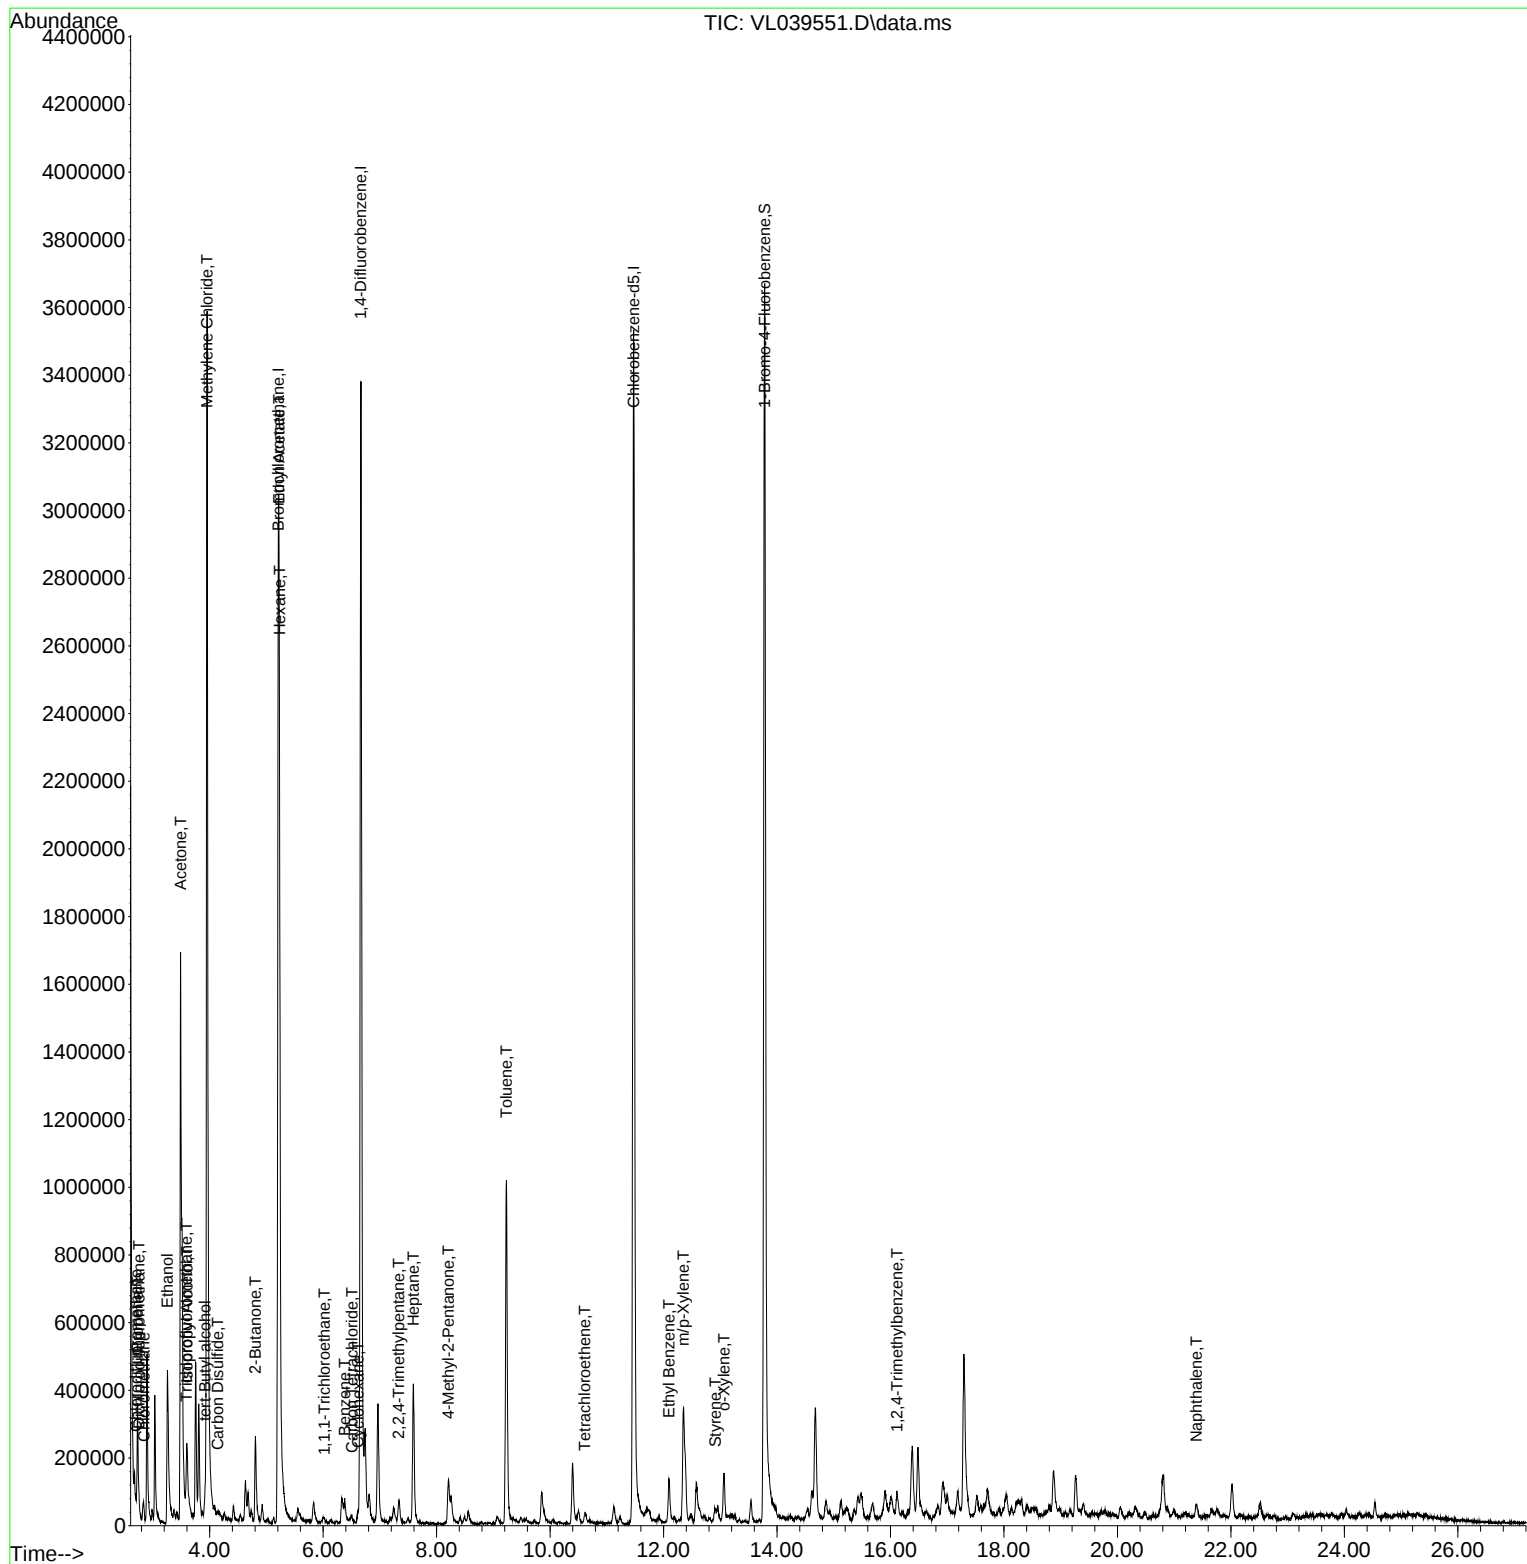



#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.208 min Scan# 81
Delta R.T. 0.001 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57




Instrument :
MSVOA_L
ClientSampleId :
IA1

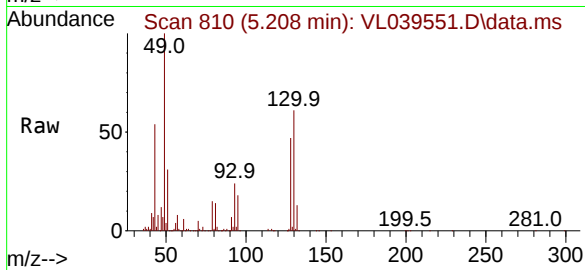

Tgt Ion: 49 Resp: 107866
Ion Ratio Lower Upper
49 100
128 48.1 25.7 77.0
130 62.0 31.6 95.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

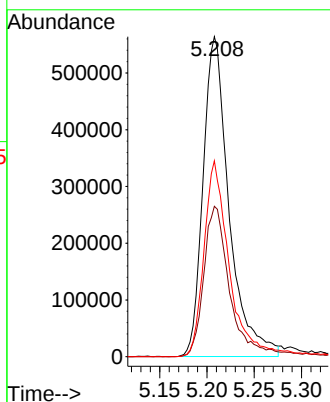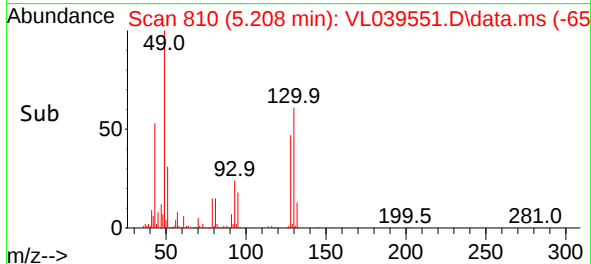

#2
Dichlorodifluoromethane
Concen: 0.205 ppbv
RT: 2.754 min Scan# 47
Delta R.T. 0.004 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57


Tgt Ion: 85 Resp: 29654
Ion Ratio Lower Upper
85 100
87 28.8 25.9 38.9

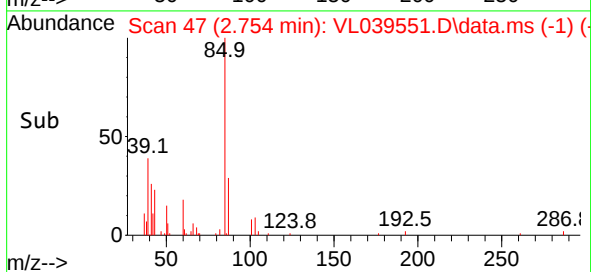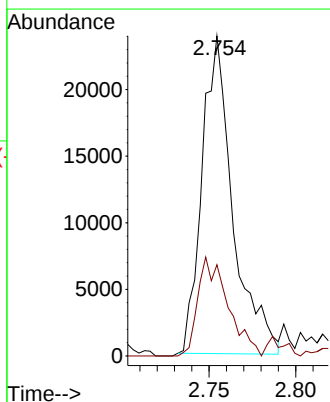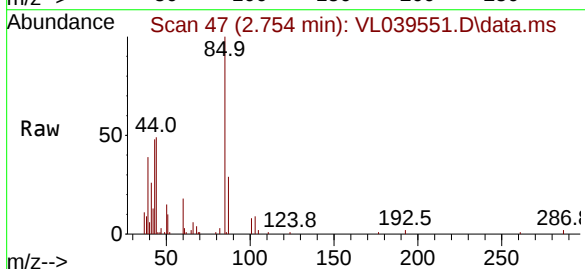



#3
Chlorodifluoromethane
Concen: 0.372 ppbv m
RT: 2.700 min Scan# 30
Delta R.T. 0.007 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57




Instrument :
MSVOA_L
ClientSampleId :
IA1



Tgt Ion: 51 Resp: 4810
Ion Ratio Lower Upper
51 100
67 17.5 14.7 22.1




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

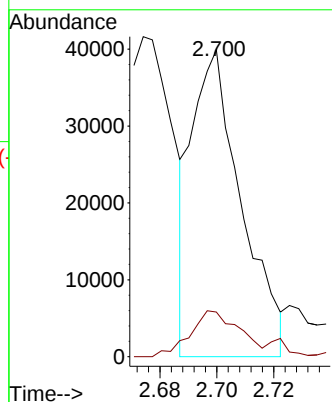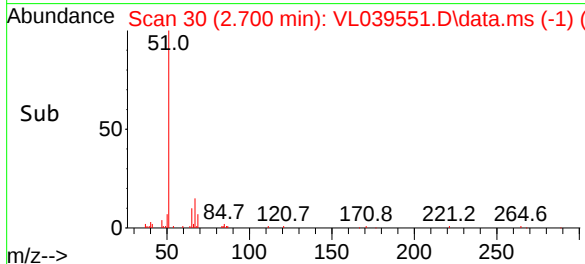

#4
Chloromethane
Concen: 0.478 ppbv
RT: 2.838 min Scan# 73
Delta R.T. 0.004 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57


Tgt Ion: 50 Resp: 36970
Ion Ratio Lower Upper
50 100
52 25.5 24.3 36.5

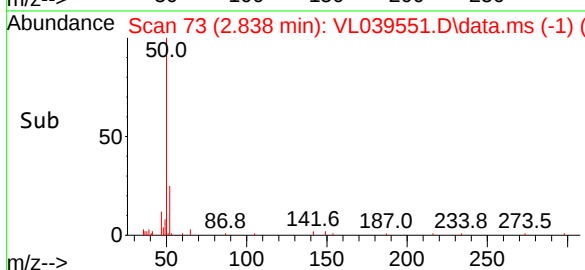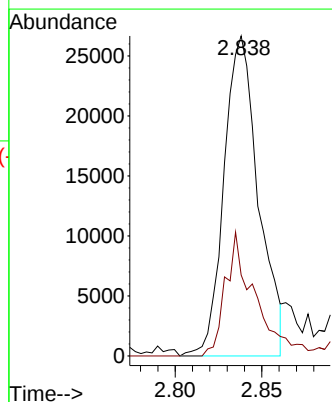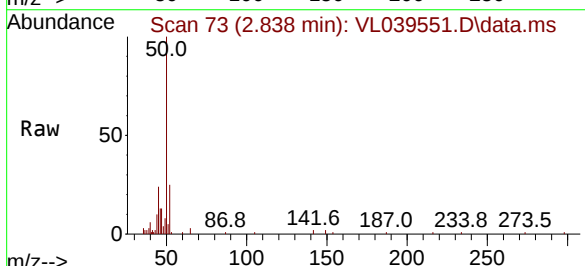



#9
 Propene
 Concen: 1.253 ppbv
 RT: 2.726 min Scan# 31
 Delta R.T. 0.010 min
 Lab File: VL039551.D
 Acq: 17 Aug 2022 16:57




Instrument :
 MSVOA_L
 ClientSampleId :
 IA1




Tgt Ion: 41 Resp: 7377
 Ion Ratio Lower Upper
 41 100
 42 48.2 55.4 83.0

Manual Integrations
 APPROVED



Reviewed By :Semsettin Yesilyurt 08/18/2022
 Supervised By :Mahesh Dadoda 08/19/2022

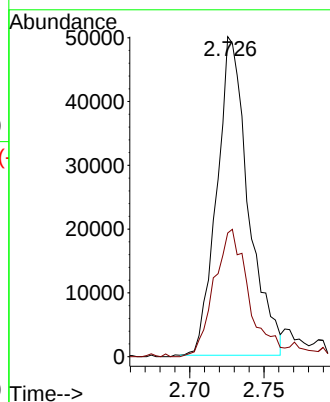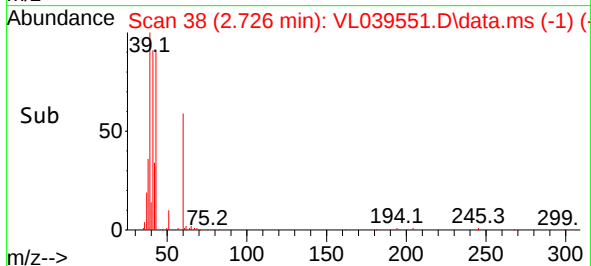


#10
 Heptane
 Concen: 1.396 ppbv
 RT: 7.587 min Scan# 1550
 Delta R.T. 0.001 min
 Lab File: VL039551.D
 Acq: 17 Aug 2022 16:57

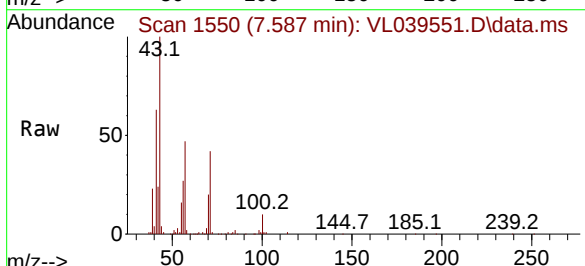


Tgt Ion: 43 Resp: 190997
 Ion Ratio Lower Upper
 43 100
 57 50.4 39.8 59.6

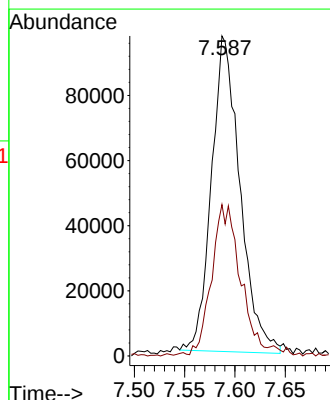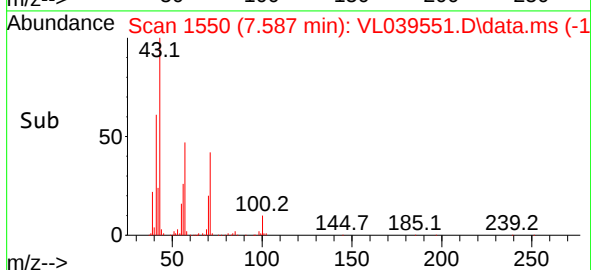



#11
Trichlorofluoromethane
Concen: 0.202 ppbv
RT: 3.587 min Scan# 309
Delta R.T. 0.007 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57




Instrument :
MSVOA_L
ClientSampleId :
IA1



Tgt Ion:101 Resp: 32094
Ion Ratio Lower Upper
101 100
103 52.1 50.6 76.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

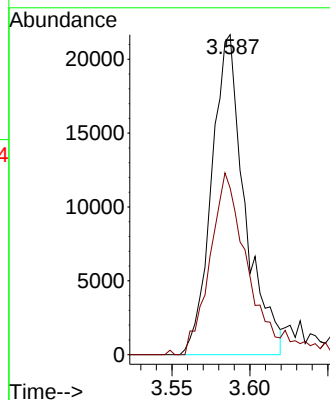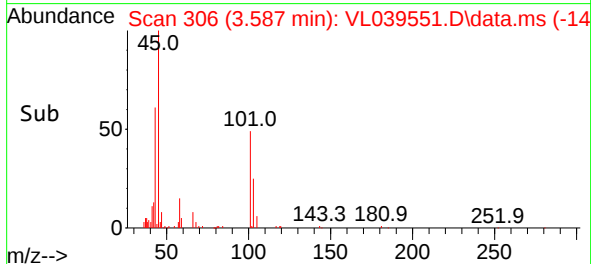

#13
Ethanol
Concen: 128.438 ppbv
RT: 3.256 min Scan# 203
Delta R.T. -0.003 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57

Tgt Ion: 45 Resp: 544391
Ion Ratio Lower Upper
45 100
46 36.2 19.3 77.1

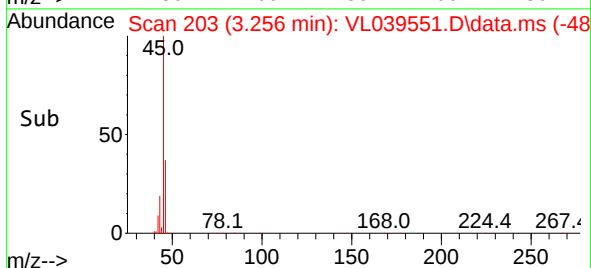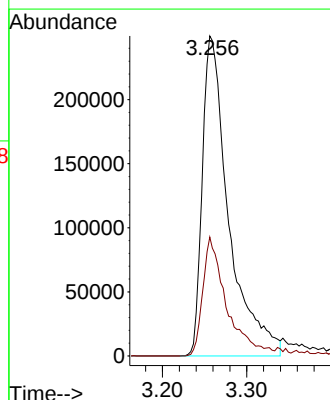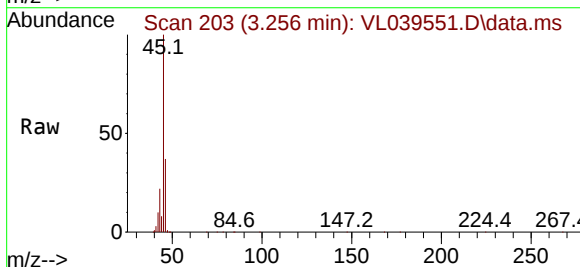







#15
Acetone
Concen: 16.426 ppbv
RT: 3.488 min Scan# 21
Delta R.T. 0.004 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57

Instrument :
MSVOA_L
ClientSampleId :
IA1

Tgt Ion: 43 Resp: 200177
Ion Ratio Lower Upper
43 100
58 25.9 20.7 31.1




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

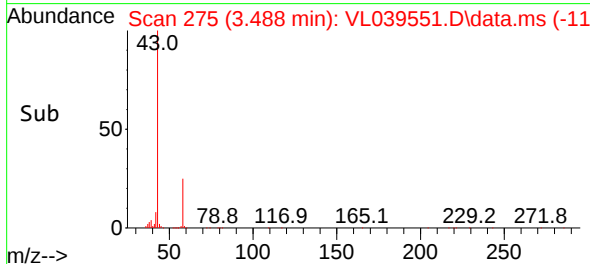

#17
tert-Butyl alcohol
Concen: 0.321 ppbv m
RT: 3.922 min Scan# 410
Delta R.T. 0.030 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57

Tgt Ion: 59 Resp: 33376
Ion Ratio Lower Upper
59 100
57 14.0 8.6 12.8#

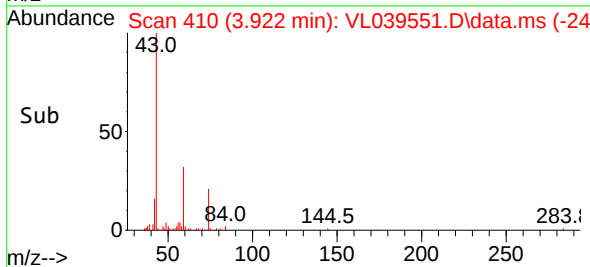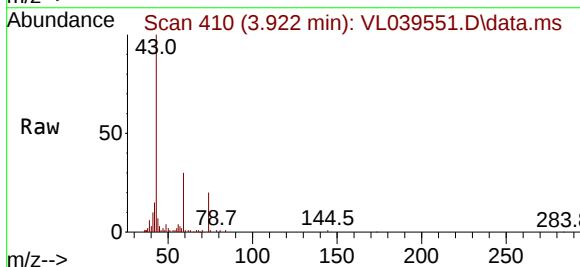







#19
Isopropyl Alcohol
Concen: 3.757 ppbv
RT: 3.600 min Scan# 312
Delta R.T. 0.010 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57

Instrument :
MSVOA_L
ClientSampleId :
IA1

Tgt Ion: 45 Resp: 22373
Ion Ratio Lower Upper
45 100
58 231.7 0.0 0.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

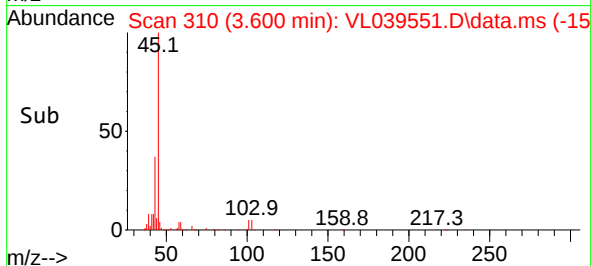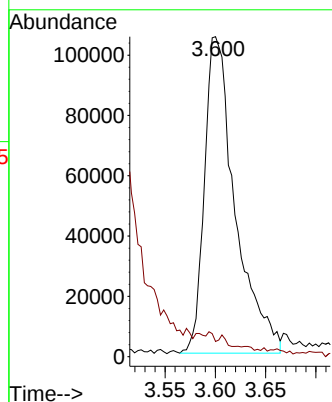

#20
Methylene Chloride
Concen: 26.466 ppbv
RT: 3.954 min Scan# 420
Delta R.T. 0.007 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57


Tgt Ion: 84 Resp: 1313195
Ion Ratio Lower Upper
84 100
49 164.6 122.2 183.4
51 49.2 35.8 53.6
86 65.4 48.4 72.6

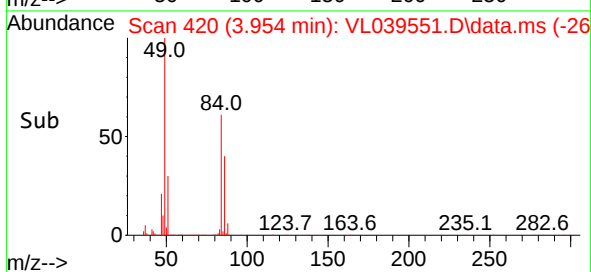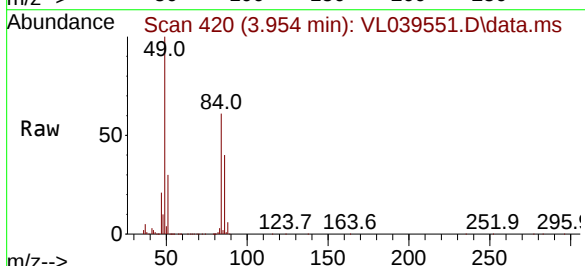



#25
Ethyl Acetate
Concen: 5.160 ppbv
RT: 5.224 min Scan# 815
Delta R.T. 0.007 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57




Instrument :
MSVOA_L
ClientSampleId :
IA1



Tgt Ion: 43 Resp: 1340752
Ion Ratio Lower Upper
43 100
45 10.3 8.2 12.4
61 9.0 8.6 12.8
70 7.1 5.7 8.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

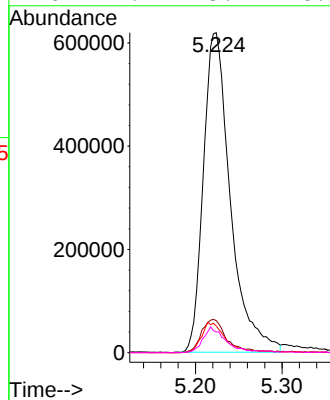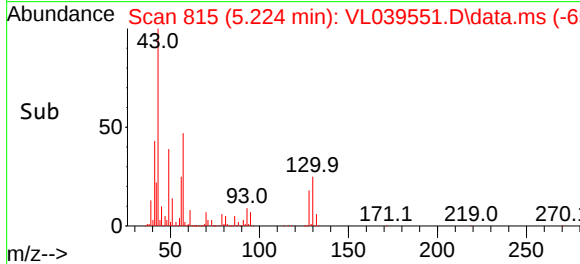

#26
Hexane
Concen: 5.782 ppbv
RT: 5.230 min Scan# 817
Delta R.T. 0.007 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57

Tgt Ion: 57 Resp: 616143
Ion Ratio Lower Upper
57 100
41 95.6 79.4 119.2
43 226.1 199.7 299.5
56 53.7 44.0 66.0

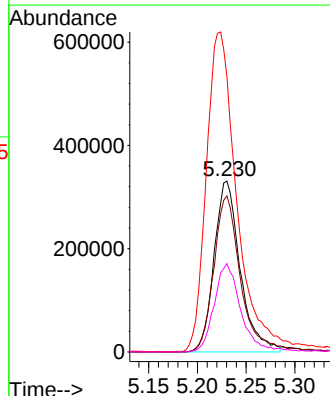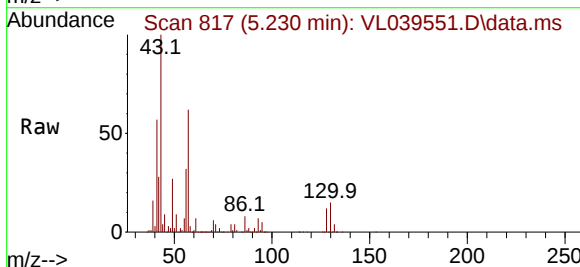







#27
Carbon Disulfide
Concen: 0.112 ppbv
RT: 4.140 min Scan# 41
Delta R.T. 0.001 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57

Instrument :
MSVOA_L
ClientSampleId :
IA1

Tgt Ion: 76 Resp: 12724
Ion Ratio Lower Upper
76 100
44 44.5 16.3 24.5
78 12.2 7.8 11.6




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

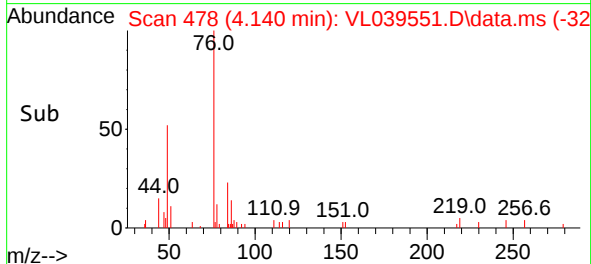

#30
Cyclohexane
Concen: 0.106 ppbv m
RT: 6.613 min Scan# 1247
Delta R.T. 0.007 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57


Tgt Ion: 84 Resp: 9367
Ion Ratio Lower Upper
84 100
56 0.0 0.0 0.0
41 146.9 0.0 0.0

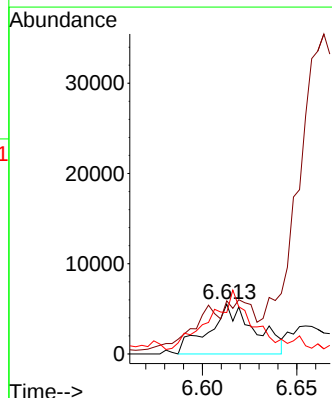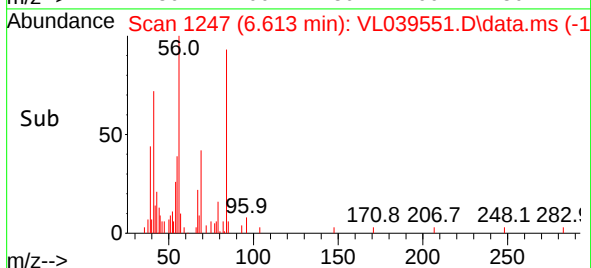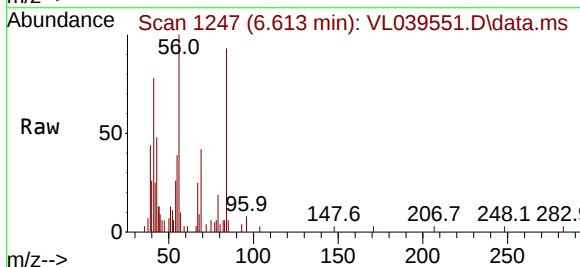



#32
1,1,1-Trichloroethane
Concen: 0.040 ppbv m
RT: 6.021 min Scan# 1063
Delta R.T. 0.007 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57




Instrument :
MSVOA_L
ClientSampleId :
IA1



Tgt Ion: 97 Resp: 626
Ion Ratio Lower Upper
97 100
99 0.0 52.4 78.6
61 0.0 42.9 64.3




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

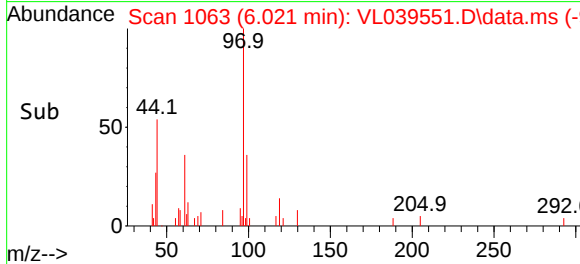

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.664 min Scan# 1263
Delta R.T. 0.004 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57


Tgt Ion:114 Resp: 2740177
Ion Ratio Lower Upper
114 100
63 24.9 20.6 31.0
88 18.5 14.6 22.0

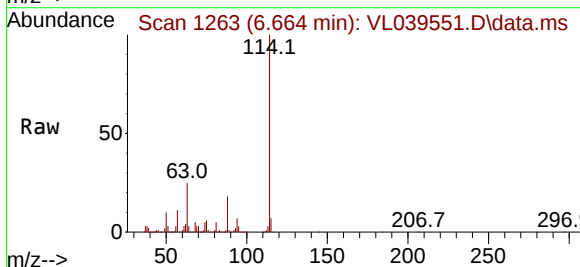

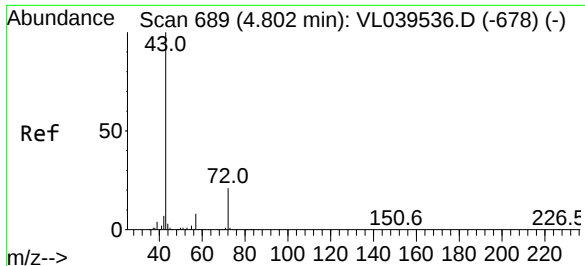

#34
2-Butanone
Concen: 2.198 ppbv
RT: 4.806 min Scan# 685
Delta R.T. 0.004 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57




Instrument :
MSVOA_L
ClientSampleId :
IA1



Tgt Ion: 43 Resp: 302819
Ion Ratio Lower Upper
43 100
72 22.5 17.4 26.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

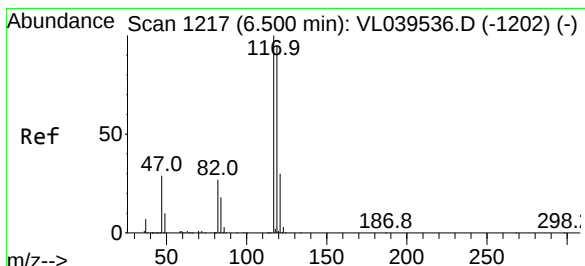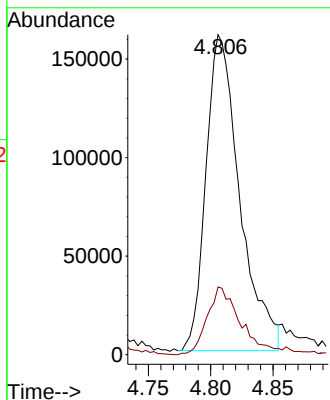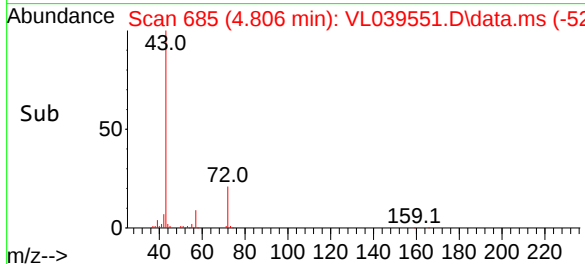

#35
Carbon Tetrachloride
Concen: 0.053 ppbv m
RT: 6.507 min Scan# 1214
Delta R.T. 0.007 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57

Tgt Ion:117 Resp: 8139
Ion Ratio Lower Upper
117 100
119 86.5 76.2 114.4
121 27.4 24.4 36.6

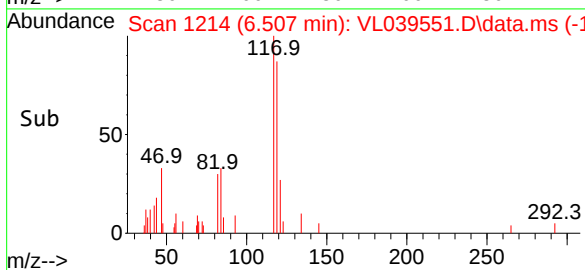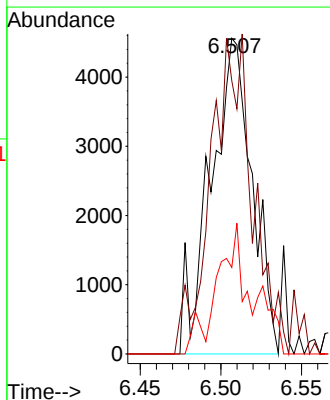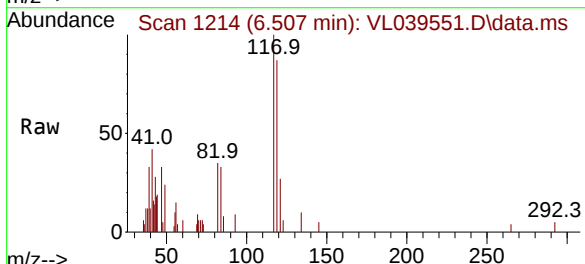



#36

Benzene

Concen: 0.185 ppbv

RT: 6.381 min Scan# 1179

Delta R.T. 0.004 min

Lab File: VL039551.D

Acq: 17 Aug 2022 16:57

Instrument :

MSVOA_L

ClientSampleId :

IA1





Tgt Ion: 78 Resp: 38634

Ion	Ratio	Lower	Upper
78	100		
77	18.5	18.6	27.8
50	33.4	15.0	22.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

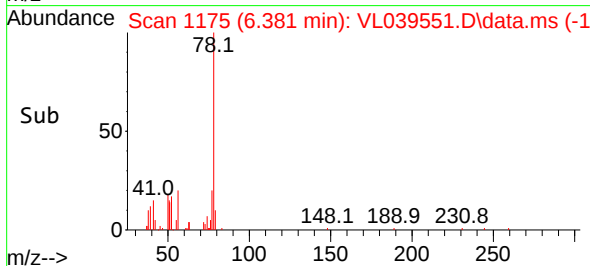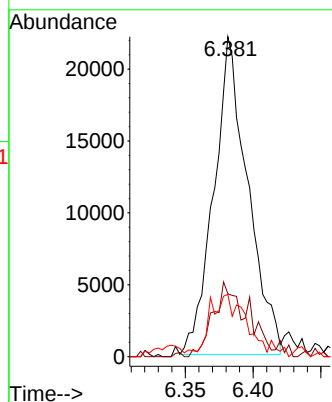

#44

2,2,4-Trimethylpentane

Concen: 0.120 ppbv m

RT: 7.333 min Scan# 1471




Delta R.T. -0.003 min


Lab File: VL039551.D

Acq: 17 Aug 2022 16:57

Tgt Ion: 57 Resp: 42113

Ion	Ratio	Lower	Upper
57	100		
41	54.0	27.8	41.6#
56	49.0	25.5	38.3#

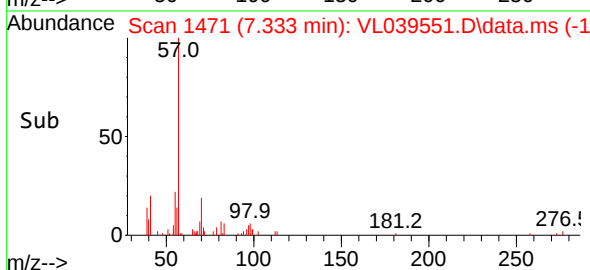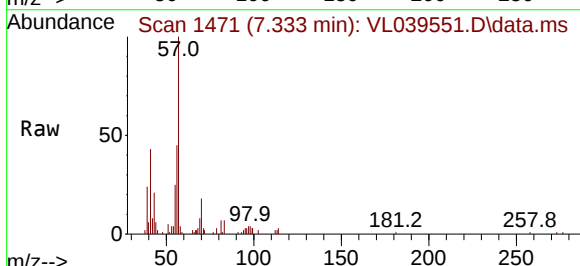







#50
4-Methyl-2-Pentanone
Concen: 0.527 ppbv m
RT: 8.204 min Scan# 1742
Delta R.T. 0.017 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57

Instrument :
MSVOA_L
ClientSampleId :
IA1

Tgt Ion: 43 Resp: 111768
Ion Ratio Lower Upper
43 100
58 32.6 28.0 42.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

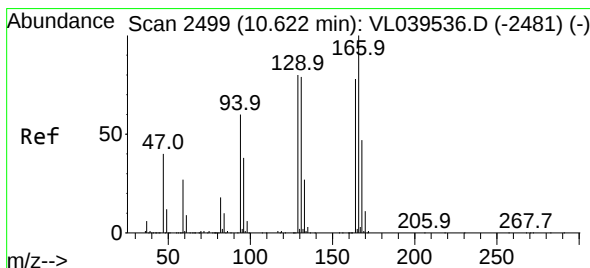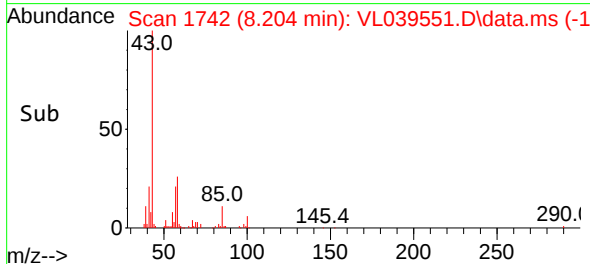

#52
Tetrachloroethene
Concen: 0.040 ppbv m
RT: 10.613 min Scan# 2491
Delta R.T. -0.009 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57

Tgt Ion:164 Resp: 3290
Ion Ratio Lower Upper
164 100
166 77.2 102.0 153.0#
129 110.5 81.7 122.5
131 38.3 80.2 120.2#

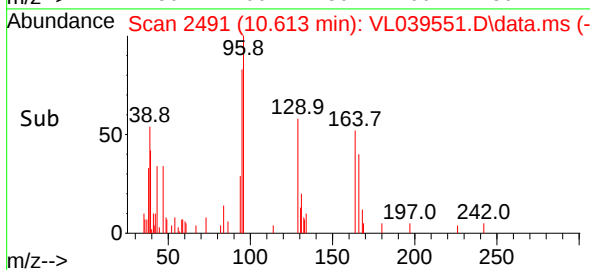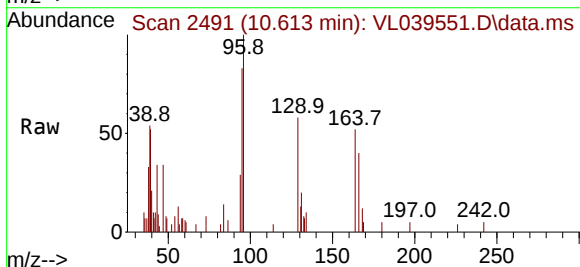







#53
Toluene
Concen: 3.533 ppbv
RT: 9.230 min Scan# 2065
Delta R.T. 0.004 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57

Instrument :
MSVOA_L
ClientSampleId :
IA1

Tgt Ion: 91 Resp: 826644
Ion Ratio Lower Upper
91 100
92 60.5 47.9 71.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

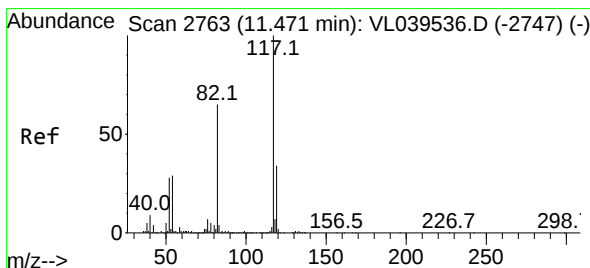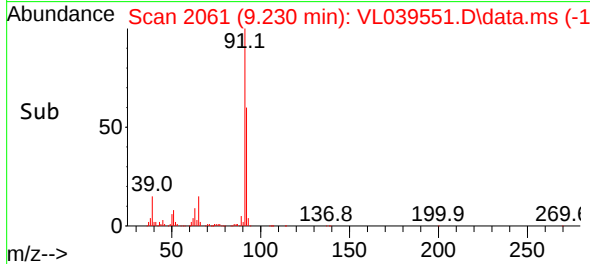

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.471 min Scan# 2758
Delta R.T. 0.001 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57


Tgt Ion:117 Resp: 2436989
Ion Ratio Lower Upper
117 100
82 65.3 49.1 73.7
119 33.0 25.9 38.9

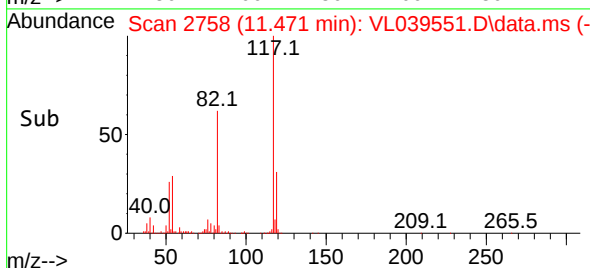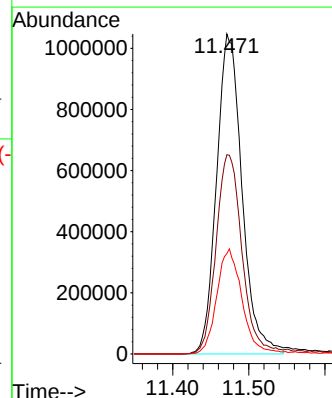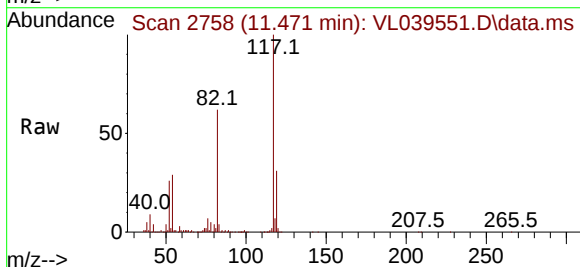

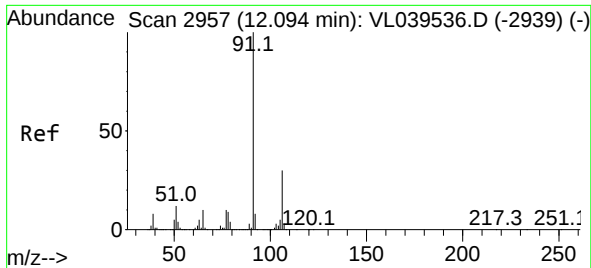

#58
Ethyl Benzene
Concen: 0.383 ppbv
RT: 12.098 min Scan# 2957
Delta R.T. 0.004 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57




Instrument :
MSVOA_L
ClientSampleId :
IA1

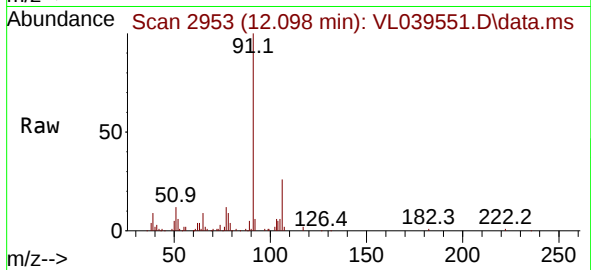

Tgt Ion: 91 Resp: 10798
Ion Ratio Lower Upper
91 100
106 25.5 24.2 36.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

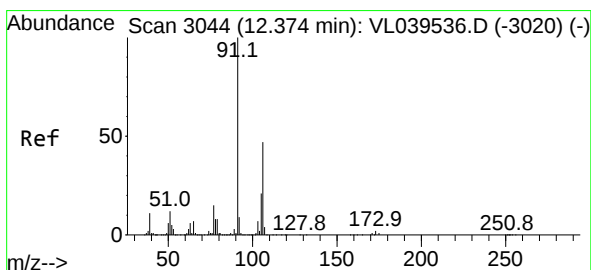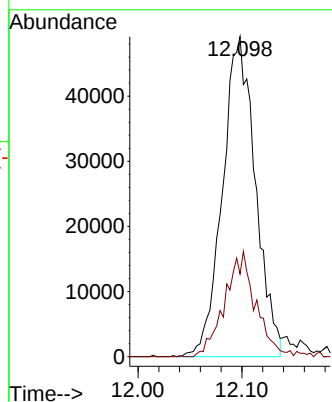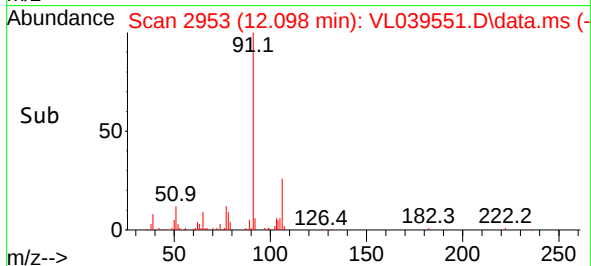

#59
m/p-Xylene
Concen: 1.420 ppbv
RT: 12.349 min Scan# 3031
Delta R.T. -0.025 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57

Tgt Ion: 91 Resp: 360184
Ion Ratio Lower Upper
91 100
106 46.5 0.0 0.0#

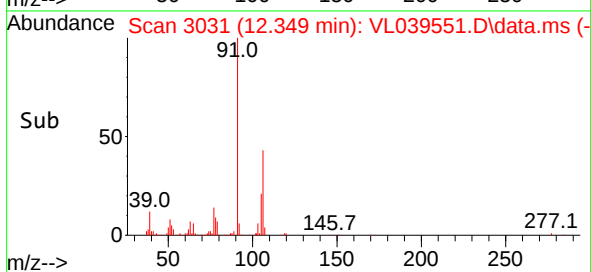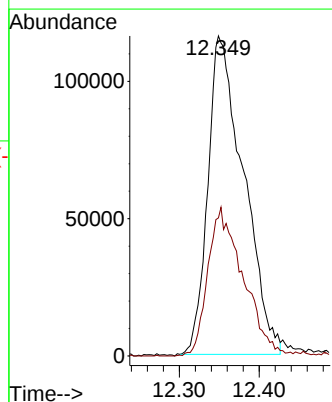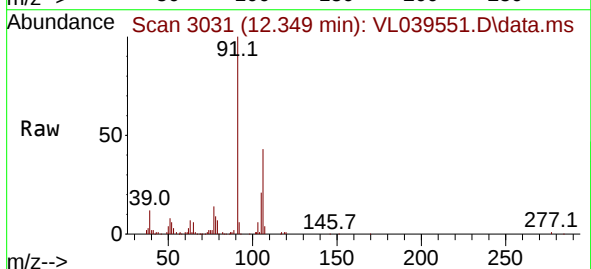

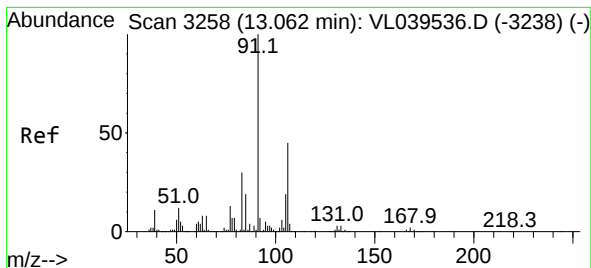

#60

o-Xylene

Concen: 0.422 ppbv

RT: 13.066 min Scan# 31

Delta R.T. 0.004 min

Lab File: VL039551.D

Acq: 17 Aug 2022 16:57

Instrument :

MSVOA_L

ClientSampleId :

IA1

Tgt Ion: 91 Resp: 10258

Ion Ratio Lower Upper

91 100





106 48.0 22.7 68.0

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 08/18/2022

Supervised By :Mahesh Dadoda 08/19/2022

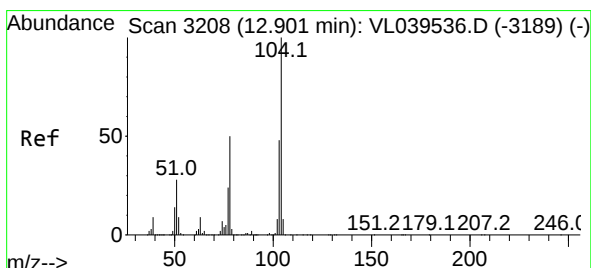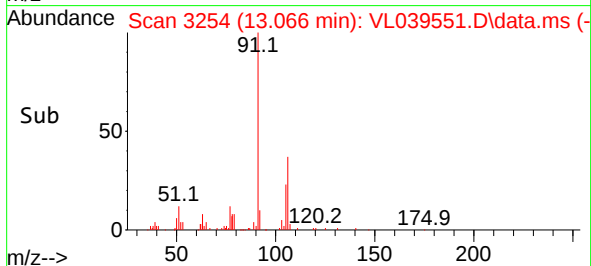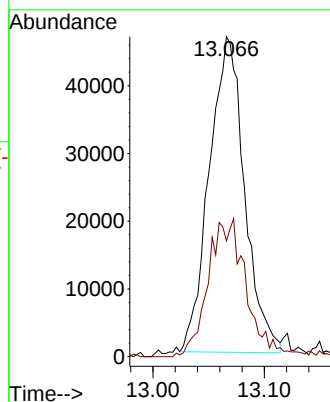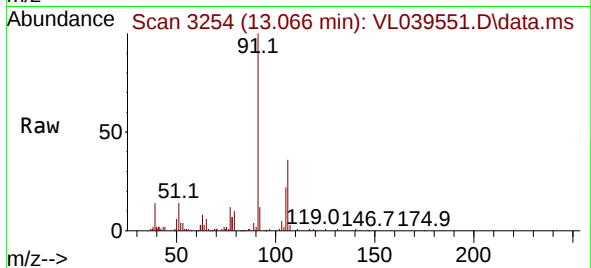

#61

Styrene

Concen: 0.163 ppbv m

RT: 12.912 min Scan# 3206

Delta R.T. 0.010 min

Lab File: VL039551.D

Acq: 17 Aug 2022 16:57




Tgt Ion:104 Resp: 21166


Ion Ratio Lower Upper

104 100

78 56.4 40.0 60.0


103 50.4 38.2 57.2

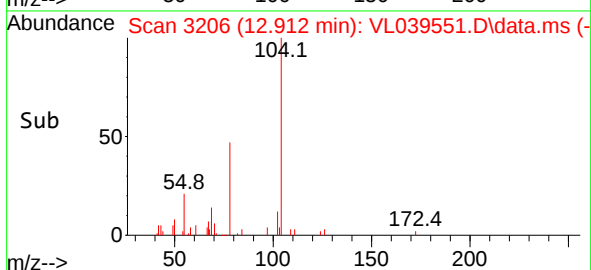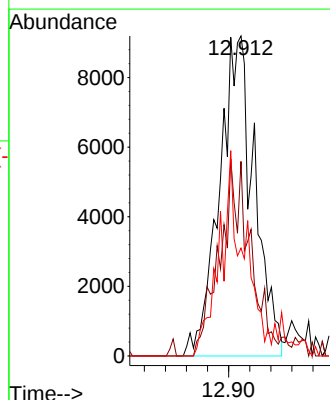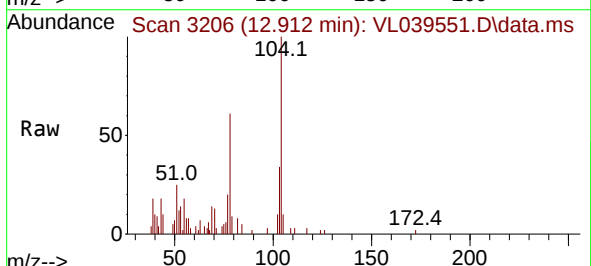

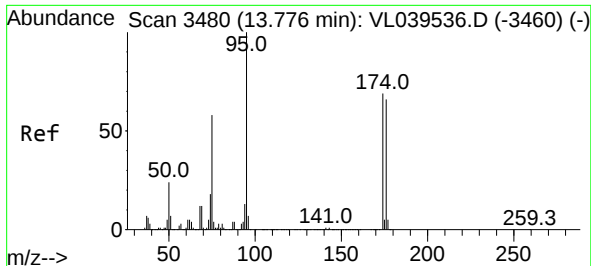

#68
1-Bromo-4-Fluorobenzene
Concen: 10.213 ppbv
RT: 13.783 min Scan# 3480
Delta R.T. 0.007 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57




Instrument :
MSVOA_L
ClientSampleId :
IA1

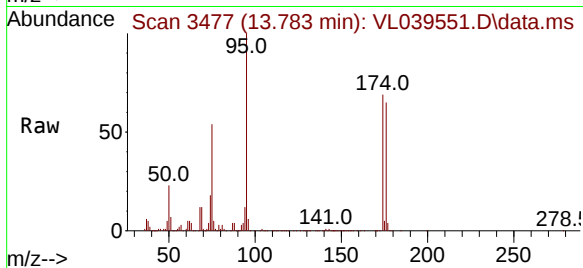


Tgt Ion: 95 Resp: 1873592
Ion Ratio Lower Upper
95 100
174 73.1 56.3 84.5
175 5.5 4.3 6.5

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

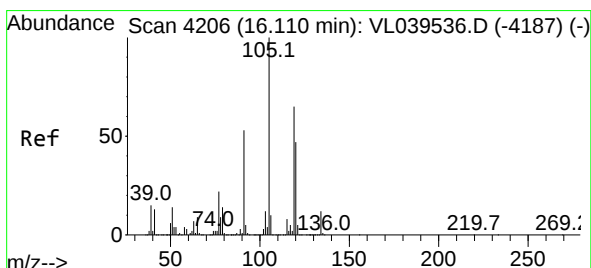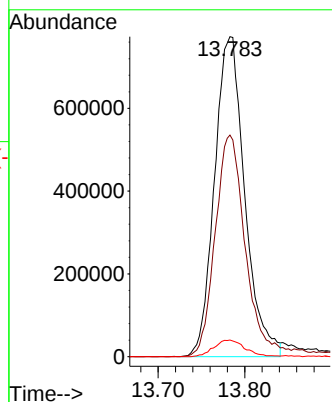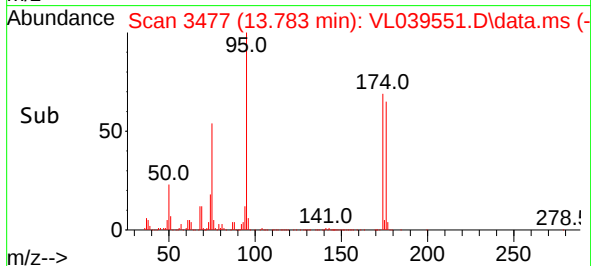


#74
1,2,4-Trimethylbenzene
Concen: 0.167 ppbv m
RT: 16.117 min Scan# 4203
Delta R.T. 0.007 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57

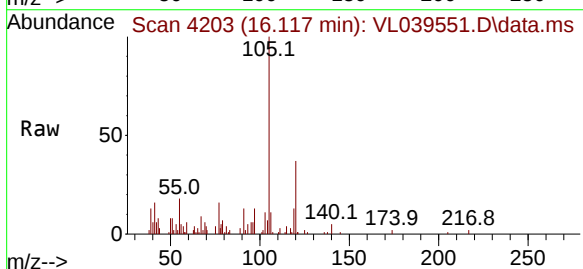


Tgt Ion:105 Resp: 48611
Ion Ratio Lower Upper
105 100
120 36.8 37.8 56.8#
91 13.5 43.8 65.6#
77 15.6 17.8 26.6#

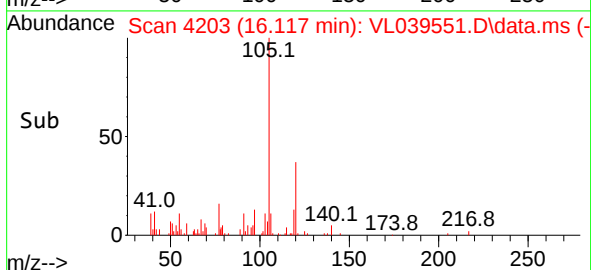

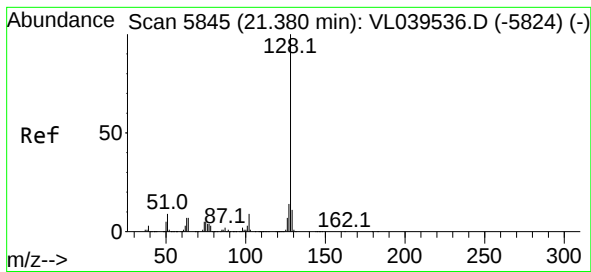

#79
Naphthalene
Concen: 0.166 ppbv m
RT: 21.387 min Scan# 5845
Delta R.T. 0.007 min
Lab File: VL039551.D
Acq: 17 Aug 2022 16:57

Instrument :
MSVOA_L
ClientSampleId :
IA1

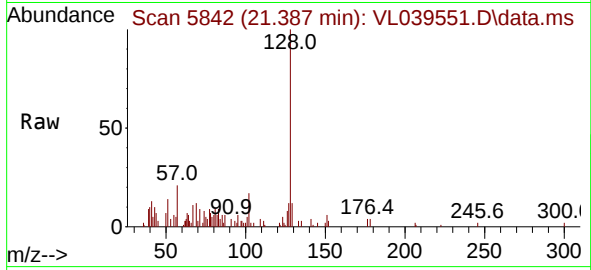

Tgt Ion:128 Resp: 34492
Ion Ratio Lower Upper
128 100
127 12.3 10.8 16.2
129 12.1 9.1 13.7

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 08/18/2022
Supervised By :Mahesh Dadoda 08/19/2022

