
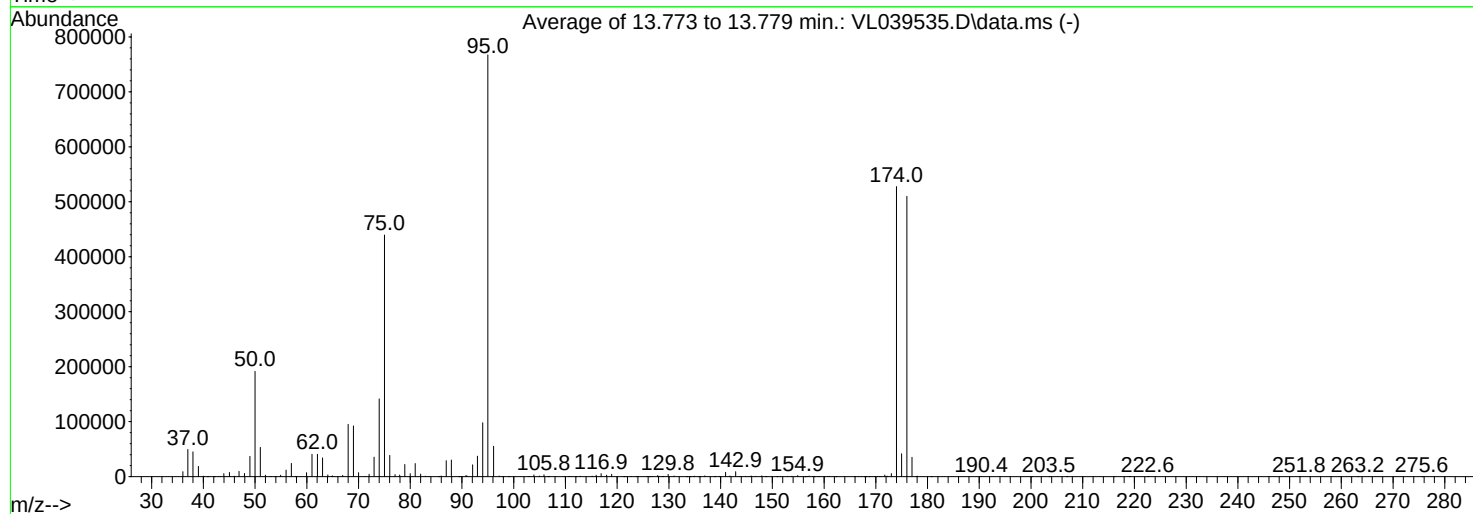


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL081722\
 Data File : VL039535.D
 Acq On : 17 Aug 2022 2:58
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081722AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Aug 17 12:06:24 2022
 Last Update : Wed Aug 17 12:06:24 2022

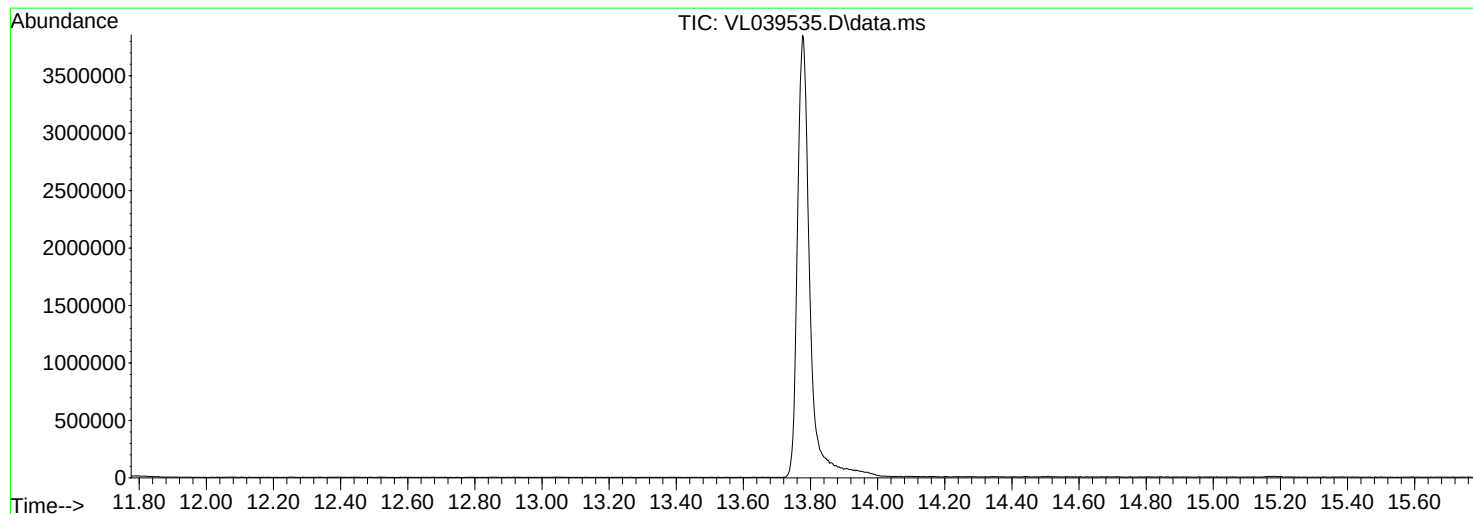

AutoFind: Scans 3479, 3480, 3481; Background Corrected with Scan 3456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.0	191680	PASS
75	95	30	66	57.3	439616	PASS
95	95	100	100	100.0	767339	PASS
96	95	5	9	7.2	55344	PASS
173	174	0.00	2	1.1	5635	PASS
174	95	50	120	68.8	527723	PASS
175	174	4	9	7.9	41720	PASS
176	174	93	101	96.7	510123	PASS
177	176	5	9	6.9	35360	PASS

Average of 13.773 to 13.779 min.: VL039535.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	9103	46.00	1049	54.95	2508	64.95	1421
37.00	49437	46.90	9539	56.00	12065	65.30	251
38.00	45195	47.95	5940	57.00	24261	66.05	271
39.05	18504	49.00	37147	57.85	489	66.95	241
40.05	922	50.00	191680	58.10	729	68.00	95115
40.80	84	51.00	53171	59.95	7396	69.00	92195
42.10	95	52.00	2564	61.00	40688	70.00	7367
42.95	442	52.90	164	62.05	40691	71.25	445
43.30	184	53.10	249	63.05	34160	72.05	4350
43.95	5455	53.80	152	64.05	3138	73.00	35440
45.05	7720	54.00	162	64.80	539	74.00	141483

Average of 13.773 to 13.779 min.: VL039535.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.00	439616	85.95	1137	96.10	55344	109.80	570
76.05	38640	86.95	29013	97.20	1291	110.60	194
77.05	3658	87.95	30408	97.90	148	110.85	669
77.95	2936	89.40	77	99.00	83	111.10	280
78.95	22075	89.80	93	102.90	231	111.65	303
80.00	5678	90.80	2280	103.10	167	112.00	151
80.95	24027	91.00	1036	103.90	3126	112.85	927
82.00	4736	92.05	21523	104.95	1058	115.15	936
82.90	896	93.00	37365	105.85	3365	115.95	2698
83.60	227	94.00	98227	106.60	143	116.90	5474
85.50	133	95.00	767339	106.95	754	117.95	2586

Average of 13.773 to 13.779 min.: VL039535.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.95	4506	128.10	666	135.95	145	145.30	279
121.30	55	128.70	303	136.95	1464	145.70	530
121.80	143	128.95	670	138.80	87	145.90	1186
122.75	285	129.85	4066	139.05	459	146.80	674
123.70	126	131.00	1242	139.75	596	147.95	1472
124.10	457	133.40	132	140.95	7792	148.70	100
125.70	381	133.65	193	141.80	1310	148.95	427
125.90	175	134.10	131	142.90	8997	149.95	636
126.20	114	134.80	205	143.70	288	150.90	129
126.80	171	135.00	1024	143.95	323	151.60	216
127.85	2059	135.70	109	144.80	640	152.90	467

Average of 13.773 to 13.779 min.: VL039535.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
153.75	524	160.00	60	169.75	358	177.80	286
154.90	1956	160.65	372	170.35	582	178.00	994
155.95	367	161.05	646	170.70	414	180.70	79
156.30	117	162.30	78	171.00	356	190.45	175
156.55	670	165.90	72	171.75	2915	200.10	54
156.80	297	166.70	208	172.20	871	203.50	88
157.10	1341	167.20	352	173.00	5635	206.90	78
157.80	345	167.80	61	174.00	527723	216.00	57
158.10	127	168.10	65	175.00	41720	219.00	59
158.80	347	168.70	135	176.00	510123	222.60	91
159.10	386	169.30	236	177.00	35360	251.85	185

Average of 13.773 to 13.779 min.: VL039535.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
263.20	53						
275.60	63						