


Data Path : Y:\voasrv\HPCHEM1\MSVOA L\Data\VL081821\
 Data File : VL037484.D
 Acq On : 18 Aug 2021 8:01
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081621AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Aug 17 02:13:47 2021
 Last Update : Tue Aug 17 02:13:47 2021

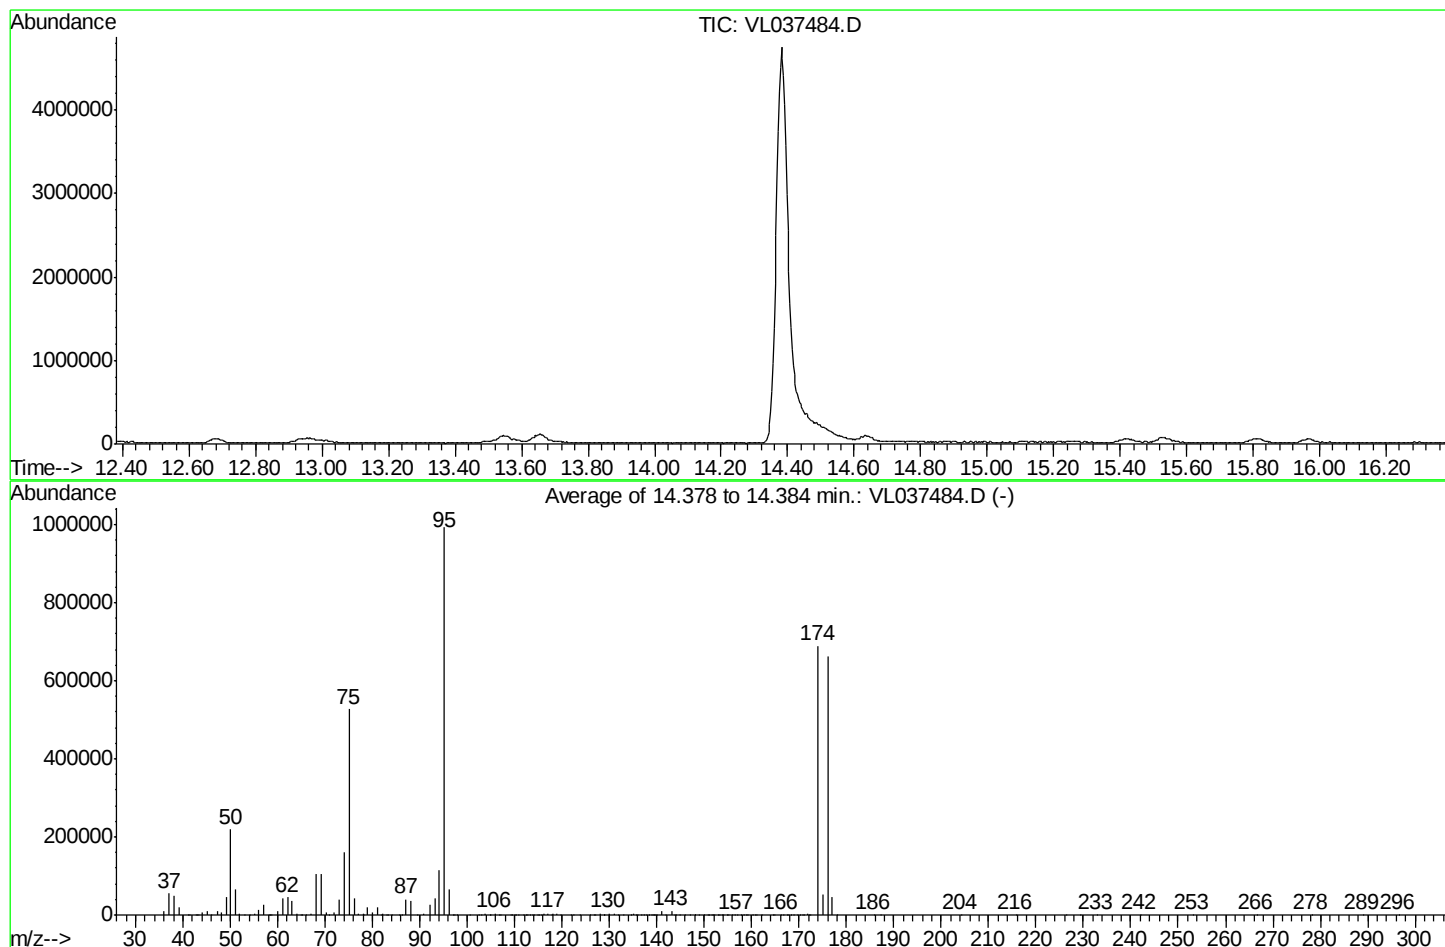

AutoFind: Scans 3605, 3606, 3607; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.0	218346	PASS
75	95	30	66	53.0	526229	PASS
95	95	100	100	100.0	992554	PASS
96	95	5	9	6.8	67029	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.4	688426	PASS
175	174	4	9	7.8	53514	PASS
176	174	93	101	95.9	660522	PASS
177	176	5	9	7.2	47442	PASS