


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL081822\
 Data File : VL039557.D
 Acq On : 18 Aug 2022 12:31
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081722AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Aug 17 12:06:24 2022
 Last Update : Wed Aug 17 12:06:24 2022

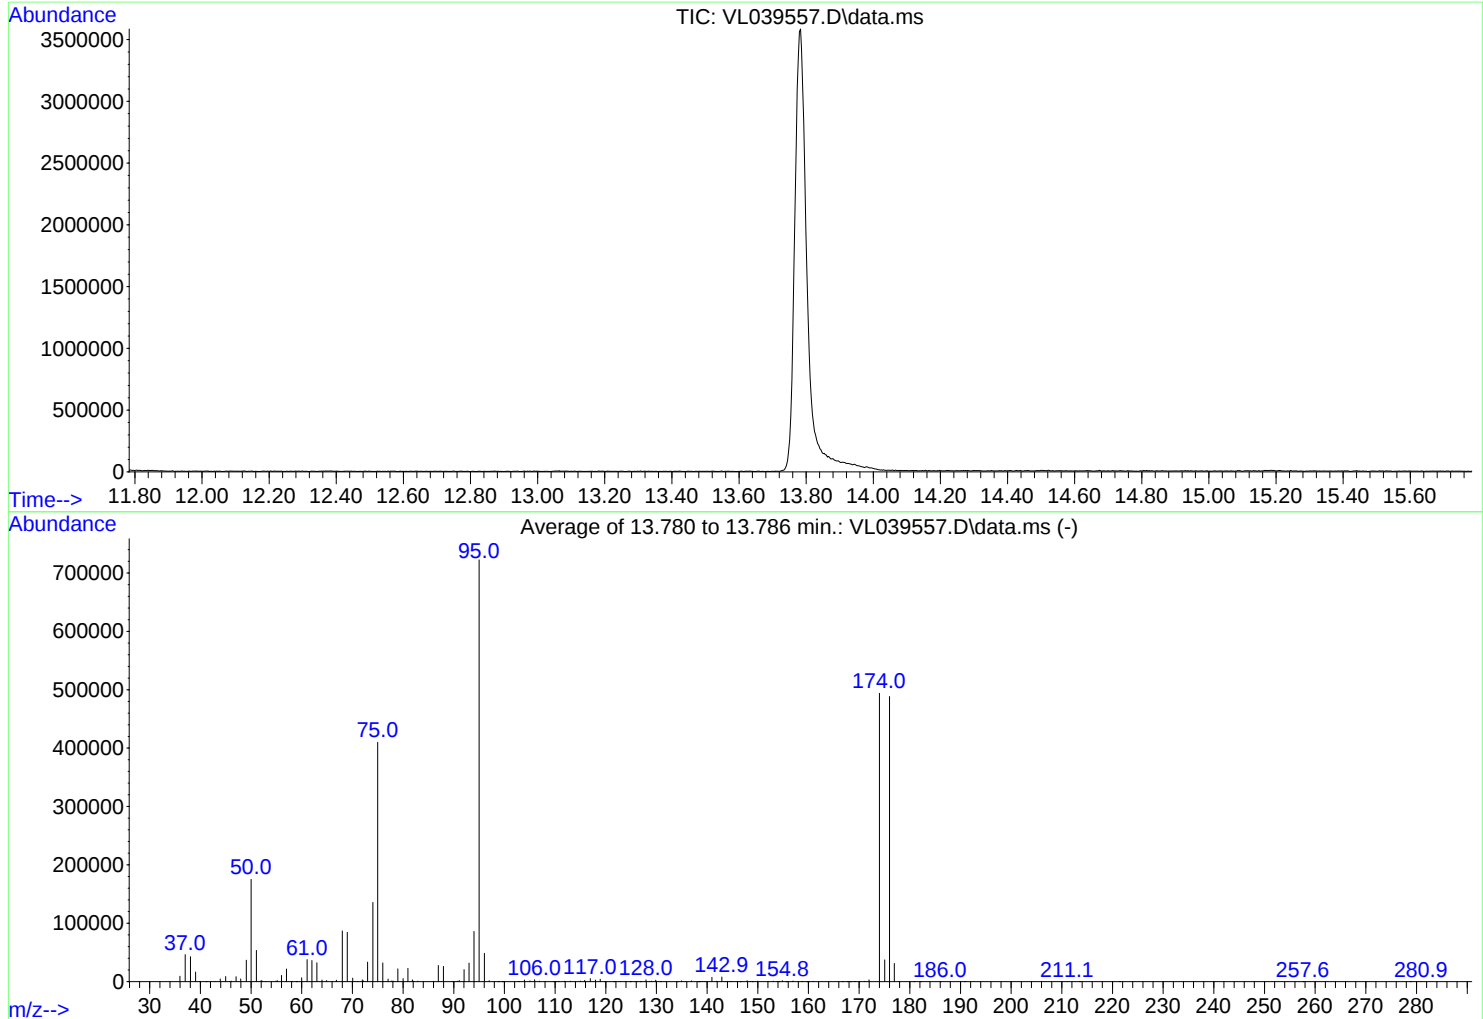

AutoFind: Scans 3476, 3477, 3478; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.2	175168	PASS
75	95	30	66	56.7	409963	PASS
95	95	100	100	100.0	722475	PASS
96	95	5	9	6.7	48592	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.4	493952	PASS
175	174	4	9	7.5	37253	PASS
176	174	93	101	98.9	488427	PASS
177	176	5	9	6.4	31309	PASS

Average of 13.780 to 13.786 min.: VL039557.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	9427	47.05	8671	57.00	21536	66.00	241
37.00	46235	47.95	4564	57.90	319	66.85	242
38.05	42909	49.05	36856	58.15	627	68.00	8682
39.05	16407	50.00	175168	58.90	80	69.00	8429
39.95	639	51.05	53344	59.10	166	70.05	5996
41.10	57	52.00	1879	60.00	6550	71.00	169
42.90	347	52.20	1075	61.05	37803	71.95	3152
43.90	4650	52.90	327	62.00	36149	72.20	1442
45.00	8878	54.90	728	63.00	32435	73.00	33419
45.80	196	55.15	2029	64.00	2818	74.05	135803
46.15	712	56.00	10833	64.90	2036	75.00	409963

Average of 13.780 to 13.786 min.: VL039557.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.00	32120	86.95	27581	98.80	72	110.00	98
77.05	4531	87.95	26019	99.55	128	110.75	678
77.80	1518	89.70	164	102.80	185	111.85	923
78.10	889	90.70	835	103.00	400	112.10	244
78.95	22056	91.10	1844	103.95	2769	113.00	775
80.00	5303	92.05	20523	105.05	1270	115.00	1062
80.95	22669	93.00	31747	105.95	3261	115.85	2277
81.85	3129	94.00	86069	106.90	836	116.95	5217
82.10	764	95.00	722475	108.00	299	117.95	2743
82.90	836	96.05	48592	109.65	398	118.90	4103
85.95	555	97.00	1633	109.80	111	119.80	82

Average of 13.780 to 13.786 min.: VL039557.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
120.00	167	128.70	633	138.50	75	145.90	703
121.60	105	129.05	744	139.05	407	146.50	72
121.85	186	129.85	2397	139.60	209	146.85	216
122.85	179	130.80	491	139.85	447	147.90	1750
123.90	343	131.00	385	140.95	7342	148.60	429
124.80	79	131.85	260	141.90	980	148.90	70
125.00	429	134.10	51	142.90	7940	149.95	826
125.80	170	134.95	1511	143.60	274	152.05	237
126.00	145	135.80	377	144.00	609	153.05	829
126.80	98	136.90	1447	144.50	188	153.80	486
127.95	2967	138.30	52	144.85	523	154.10	60

Average of 13.780 to 13.786 min.: VL039557.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.85	1576	166.70	66	176.95	31309	280.90	196
155.60	103	167.70	78	177.85	696		
155.90	381	168.30	113	180.80	105		
156.80	291	169.10	248	182.10	90		
156.95	1117	169.30	307	186.00	89		
158.00	314	170.15	674	190.80	61		
158.70	602	171.10	490	211.10	168		
158.90	240	171.95	3050	213.50	77		
159.70	76	174.00	493952	221.40	75		
160.00	85	175.05	37253	257.60	52		
160.95	643	176.00	488427	278.80	155		