


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL082018\
 Data File : VL032405.D
 Acq On : 20 Aug 2018 13:01
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081518AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Aug 15 14:58:02 2018
 Last Update : Wed Aug 15 14:58:02 2018

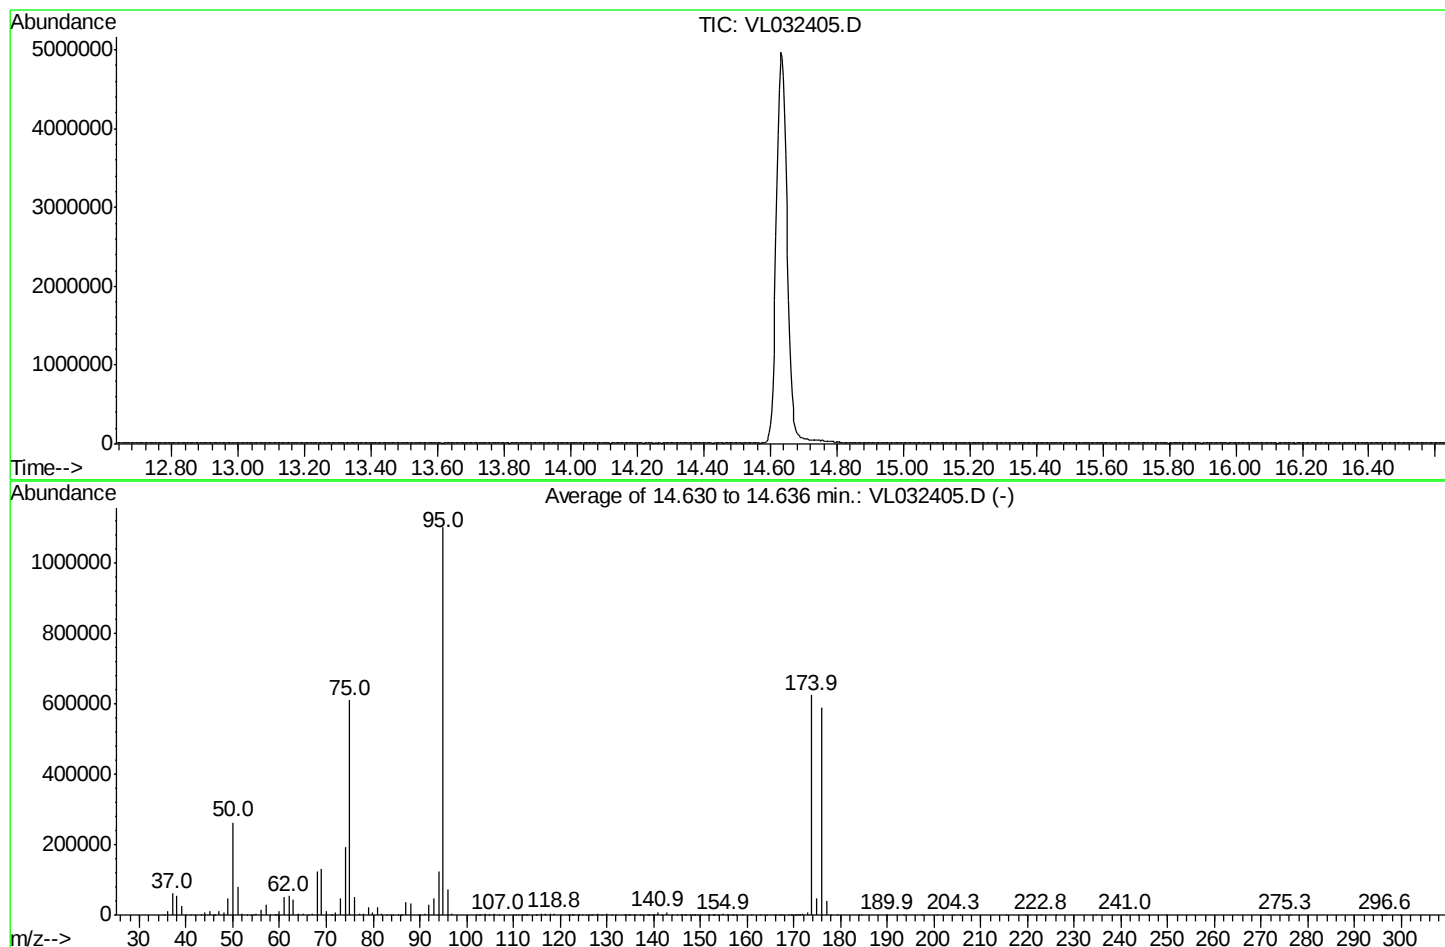

AutoFind: Scans 4212, 4213, 4214; Background Corrected with Scan 4188

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	262634	PASS
75	95	30	66	55.4	609450	PASS
95	95	100	100	100.0	1100458	PASS
96	95	5	9	6.6	73125	PASS
173	174	0.00	2	0.9	5848	PASS
174	95	50	120	56.7	623829	PASS
175	174	4	9	7.4	45938	PASS
176	174	93	101	94.3	588540	PASS
177	176	5	9	6.8	39872	PASS