


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL082020\
 Data File : VL035469.D
 Acq On : 20 Aug 2020 8:20
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081720AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Aug 17 19:28:30 2020
 Last Update : Mon Aug 17 19:28:30 2020

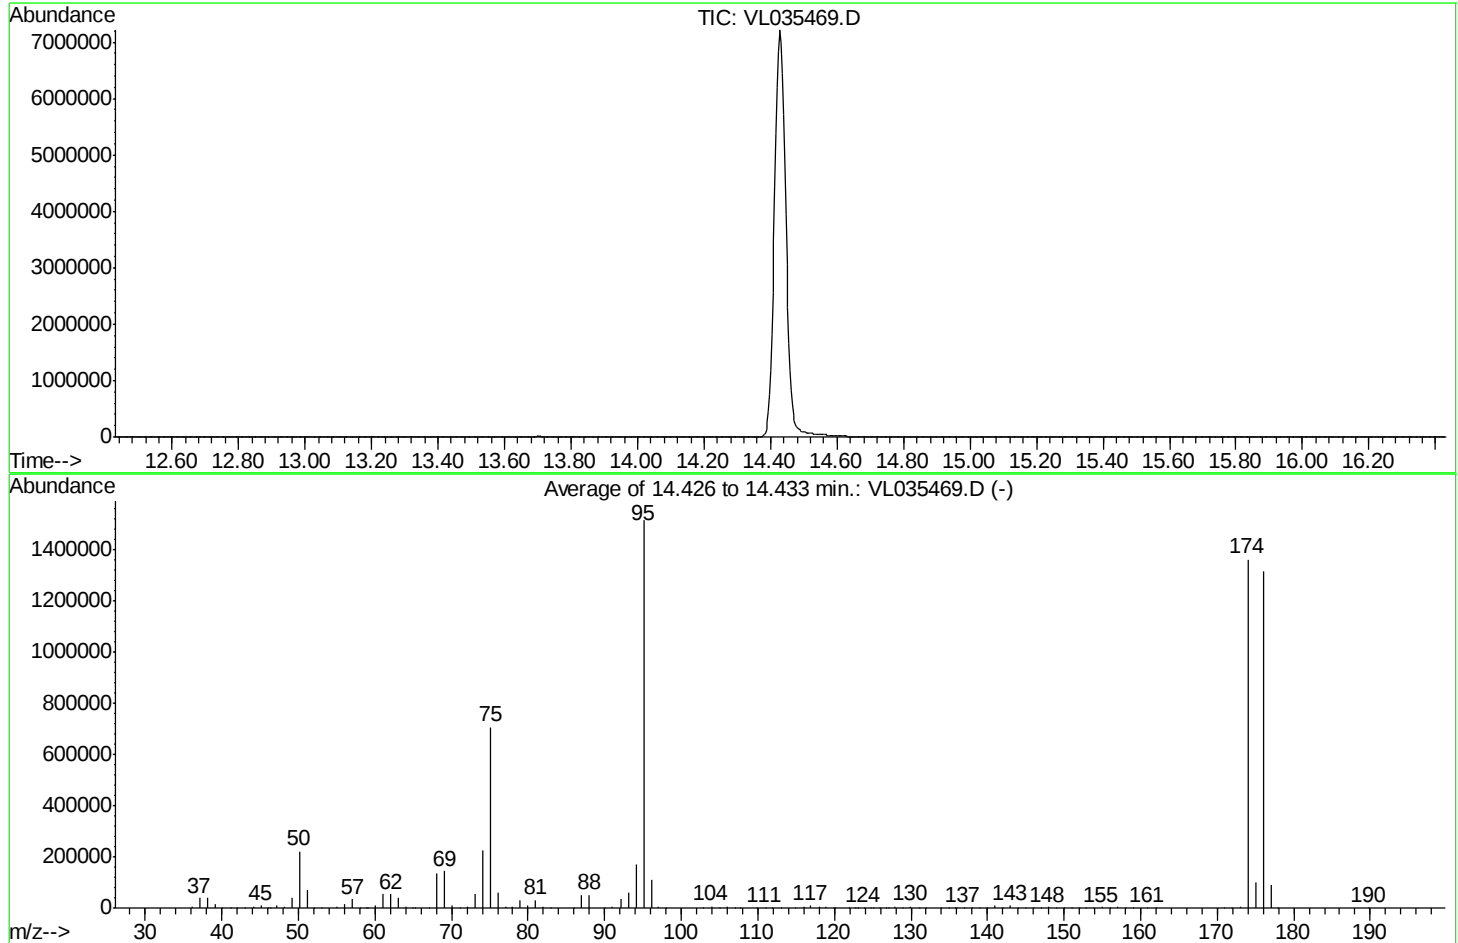

AutoFind: Scans 3620, 3621, 3622; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	14.6	220778	PASS
75	95	30	66	46.6	706112	PASS
95	95	100	100	100.0	1514837	PASS
96	95	5	9	7.3	110696	PASS
173	174	0.00	2	0.6	7517	PASS
174	95	50	120	90.0	1362773	PASS
175	174	4	9	7.5	101640	PASS
176	174	93	101	96.7	1317205	PASS
177	176	5	9	7.0	92213	PASS