
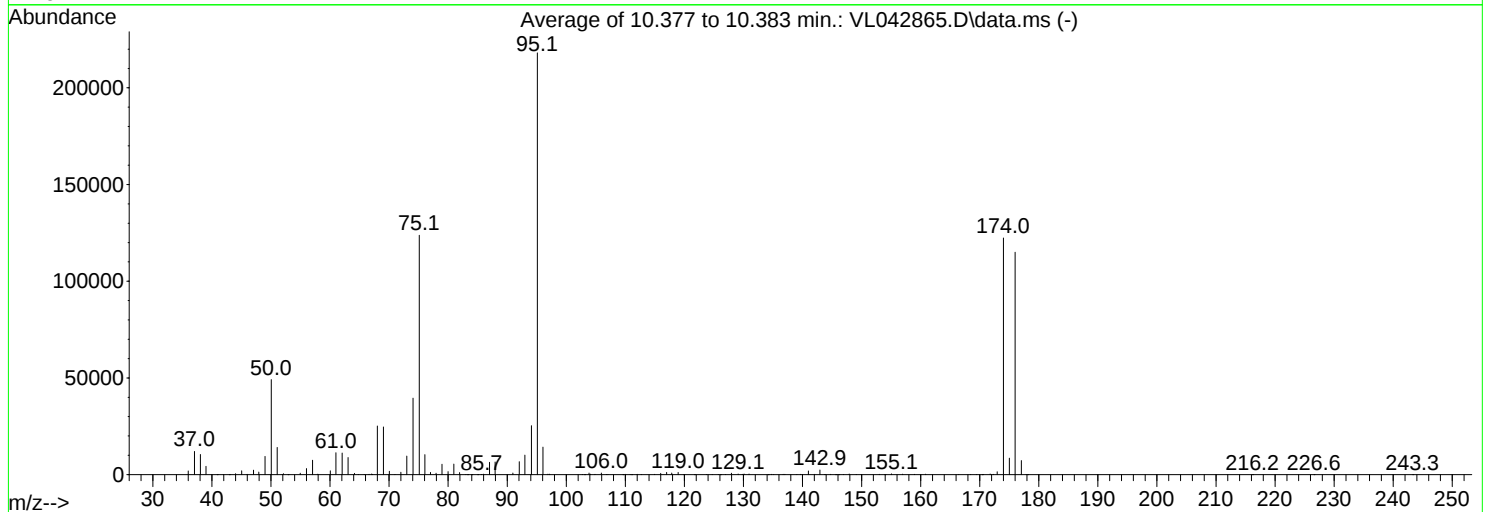


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL082125\
Data File : VL042865.D
Acq On : 21 Aug 2025 12:15
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL081325AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Aug 14 02:12:54 2025

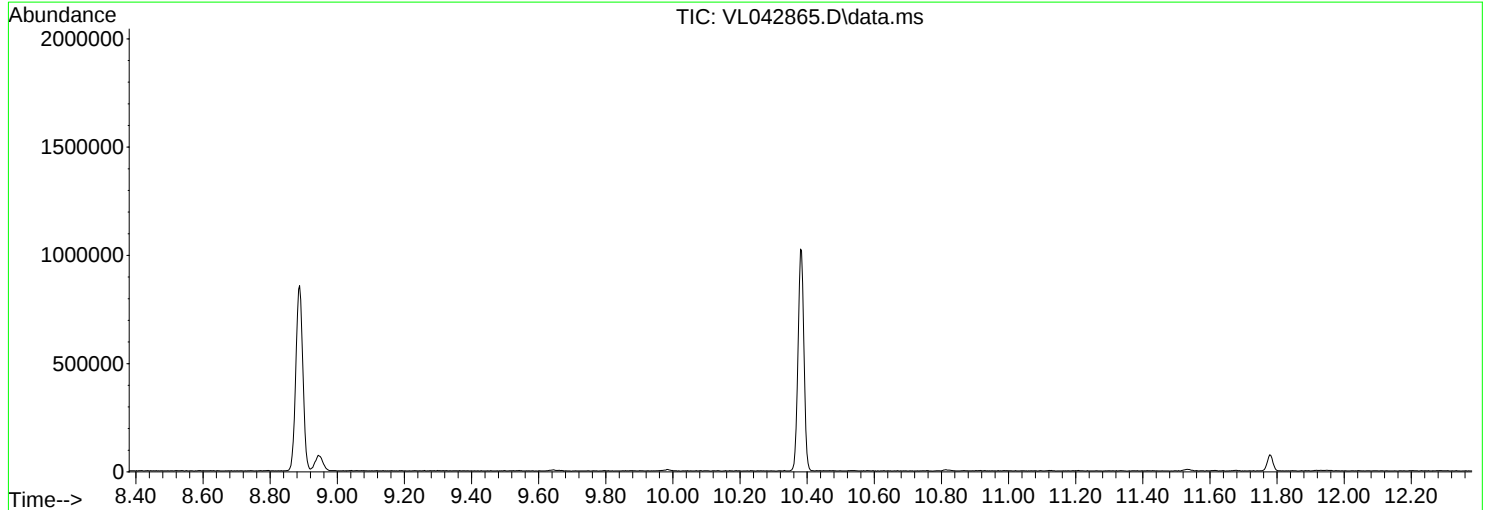

AutoFind: Scans 3179, 3180, 3181; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.5	49152	PASS
75	95	30	66	56.7	123755	PASS
95	95	100	100	100.0	218091	PASS
96	95	5	9	6.5	14275	PASS
173	174	0.00	2	1.2	1509	PASS
174	95	50	120	56.1	122349	PASS
175	174	4	9	7.0	8540	PASS
176	174	93	101	94.0	114984	PASS
177	176	5	9	6.3	7278	PASS

Average of 10.377 to 10.383 min.: VL042865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	1901	47.95	1328	60.05	1973	69.05	2465
37.05	12011	49.00	9457	61.00	11325	70.05	1711
38.05	10425	50.05	49152	62.05	11161	71.00	111
39.00	4299	51.05	14034	63.05	8883	72.00	125
40.90	20	51.90	93	64.15	708	73.00	9616
41.95	108	52.10	469	64.80	50	74.05	39549
42.95	7	52.90	39	65.80	79	75.10	123755
44.00	506	54.95	762	66.60	174	76.05	10332
45.05	1989	56.00	3135	67.00	328	77.00	1141
45.95	184	57.05	7438	67.20	164	77.95	723
47.05	2284	57.95	273	68.00	25117	78.95	5375

Average of 10.377 to 10.383 min.: VL042865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.00	1537	90.95	856	104.10	270	114.95	207
80.95	5449	92.05	6707	104.85	205	116.00	676
81.95	1093	93.00	10074	105.95	864	117.00	1123
83.00	126	94.10	25357	106.80	73	117.85	836
83.30	35	95.10	218091	107.05	99	118.95	1136
84.00	42	96.05	14275	109.60	29	119.90	32
85.00	28	96.90	258	110.05	137	121.70	35
85.65	57	97.20	238	110.80	92	123.75	74
86.00	231	102.75	51	111.05	45	124.70	53
87.00	6369	103.10	39	112.00	201	125.75	112
87.95	6531	103.85	828	112.70	119	126.10	28

Average of 10.377 to 10.383 min.: VL042865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.95	76	139.05	68	146.95	103	166.45	66
127.95	761	139.70	149	147.90	317	168.45	67
129.10	347	141.00	1901	149.10	49	169.50	65
129.80	209	142.05	129	149.95	85	170.40	18
130.10	329	142.95	2388	153.00	151	170.65	80
130.95	330	143.70	58	153.90	30	171.75	327
134.20	26	143.90	49	154.10	66	172.30	194
134.75	151	144.75	211	155.05	393	172.95	1509
135.10	70	145.60	41	156.95	254	174.00	122349
136.70	153	145.85	66	158.95	178	175.00	8540
137.00	199	146.10	43	160.85	256	176.00	114984

Average of 10.377 to 10.383 min.: VL042865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
177.05	7278						
177.85	114						
178.10	43						
216.20	17						
226.60	21						
243.30	17						

Instrument :

MSVOA_L

ClientSampleId :

BFB