
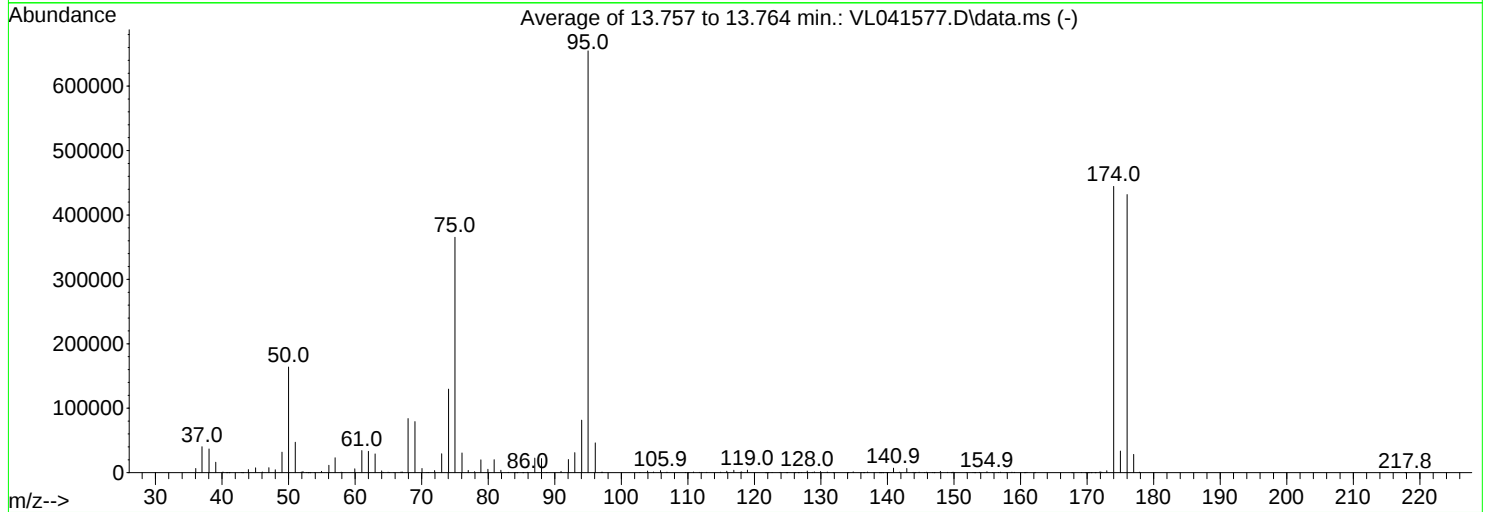


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL082224\
Data File : VL041577.D
Acq On : 22 Aug 2024 7:32
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Aug 23 01:15:26 2024

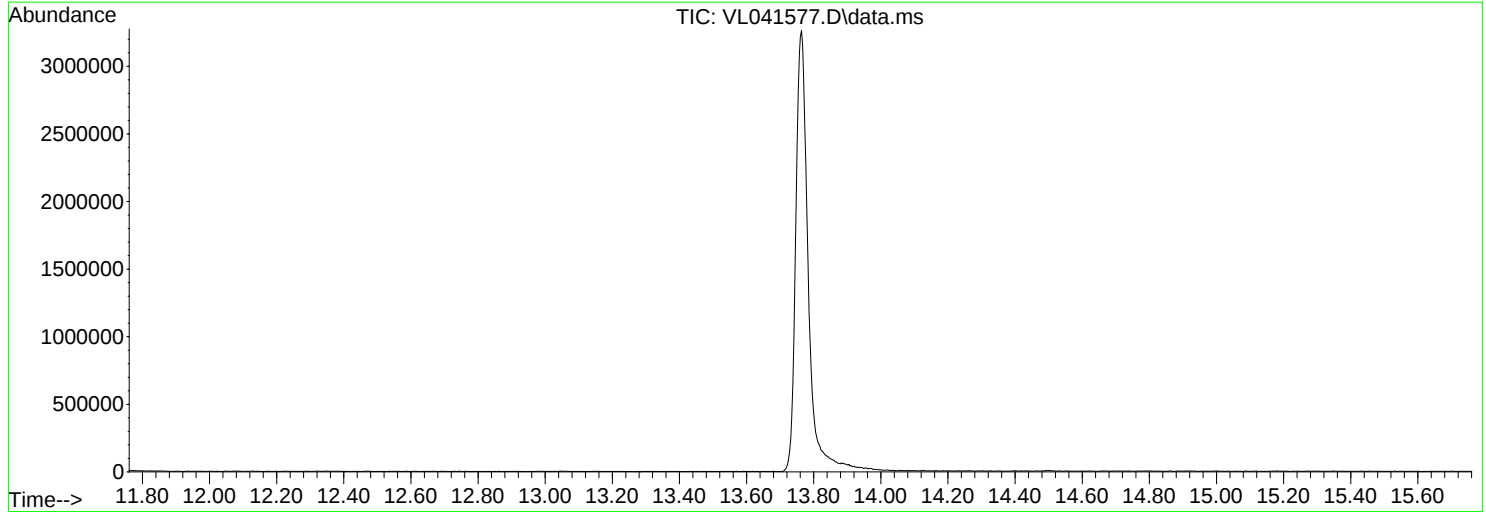

AutoFind: Scans 3469, 3470, 3471; Background Corrected with Scan 3447

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	25.0	163904	PASS
75	95	30	66	55.8	365397	PASS
95	95	100	100	100.0	654805	PASS
96	95	5	9	7.1	46304	PASS
173	174	0.00	2	0.6	2884	PASS
174	95	50	120	67.9	444501	PASS
175	174	4	9	7.5	33512	PASS
176	174	93	101	97.1	431659	PASS
177	176	5	9	6.5	28253	PASS

Average of 13.757 to 13.764 min.: VL041577.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	6563	46.05	902	53.20	116	64.00	268
37.00	40128	47.05	7706	53.95	219	64.20	54
38.05	36779	48.00	4489	54.95	2115	64.95	81
39.05	16248	49.00	31781	56.05	11452	65.20	24
40.15	960	50.00	163904	57.00	23155	65.85	239
40.70	97	51.00	47189	57.90	817	66.90	1001
41.05	139	51.90	806	58.10	299	67.10	913
42.95	375	52.00	823	59.95	6034	67.95	84084
43.10	59	52.15	1678	61.00	34240	69.00	79325
43.95	4689	52.70	284	62.00	32952	70.05	6417
45.05	7422	52.90	120	63.00	28963	70.80	174

Average of 13.757 to 13.764 min.: VL041577.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
71.05	253	81.90	3858	93.00	30984	109.65	321
71.95	3270	83.00	419	94.05	81376	110.00	64
73.00	29365	83.95	133	95.00	654805	110.85	987
74.05	129621	84.30	82	96.10	46304	111.80	403
75.00	365397	85.20	67	97.00	730	112.10	512
76.05	30573	85.95	440	97.20	653	112.85	471
77.00	3568	87.00	22525	102.80	301	114.95	659
77.95	1611	88.00	21928	103.95	2448	115.85	2271
78.90	19915	88.80	251	104.85	938	116.90	3666
79.95	5336	90.95	2108	105.90	3174	117.90	691
80.90	20197	92.05	20275	106.85	660	118.10	1273

Average of 13.757 to 13.764 min.: VL041577.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.95	3949	129.00	1327	139.00	106	145.90	781
121.70	150	129.95	1722	139.30	74	146.75	374
122.00	137	130.95	1068	139.80	174	147.00	151
122.65	209	131.85	142	140.10	236	147.95	1976
123.85	597	134.00	92	140.90	6916	149.00	431
124.85	156	134.85	1296	141.85	869	149.60	78
126.00	71	136.05	170	142.90	6404	149.85	702
126.60	55	136.40	86	143.85	614	150.10	270
127.10	207	137.00	981	144.10	148	151.90	251
127.95	2470	138.00	172	144.75	721	152.85	294
128.70	502	138.80	69	145.60	304	153.10	125

Average of 13.757 to 13.764 min.: VL041577.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
153.85	436	167.70	98	176.00	431659		
154.95	1479	169.15	277	177.00	28253		
155.80	227	169.80	76	177.90	680		
156.70	257	170.20	118	217.80	90		
157.00	787	170.60	130				
157.90	349	171.20	110				
158.70	703	171.95	1491				
159.05	485	172.20	737				
160.60	98	172.95	2884				
160.95	499	174.00	444501				
162.10	62	175.00	33512				