


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL082320\
 Data File : VL035490.D
 Acq On : 23 Aug 2020 7:34
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL082320AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Aug 17 19:28:30 2020
 Last Update : Mon Aug 17 19:28:30 2020

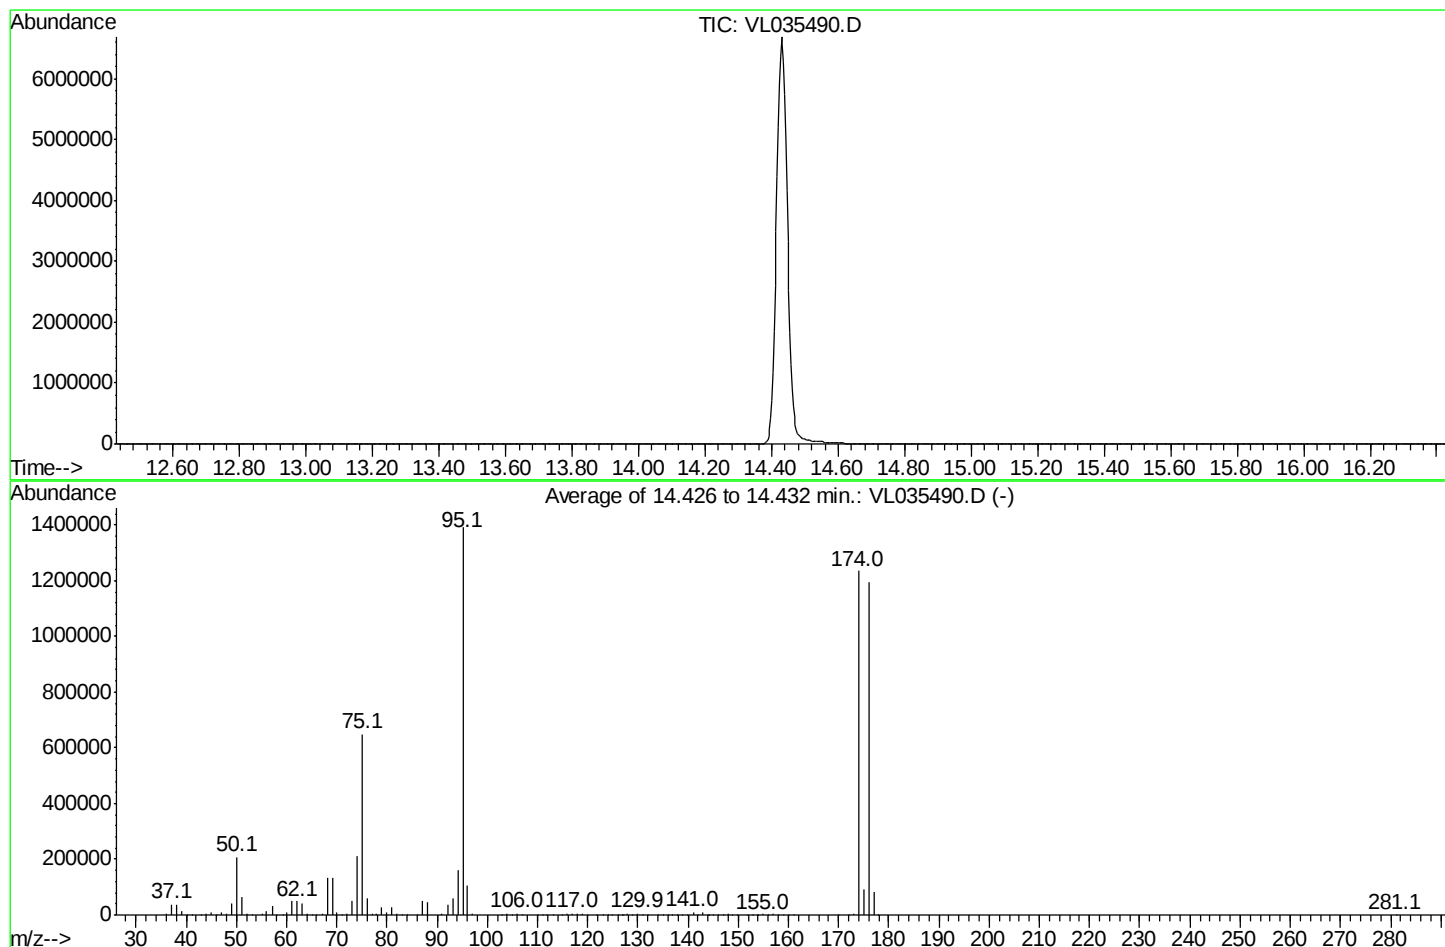

AutoFind: Scans 3620, 3621, 3622; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	14.9	207466	PASS
75	95	30	66	46.6	648618	PASS
95	95	100	100	100.0	1391274	PASS
96	95	5	9	7.5	104752	PASS
173	174	0.00	2	0.5	6675	PASS
174	95	50	120	88.8	1235114	PASS
175	174	4	9	7.5	92074	PASS
176	174	93	101	96.6	1192960	PASS
177	176	5	9	7.1	84221	PASS