

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL082720\
 Data File : VL035523.D
 Acq On : 27 Aug 2020 17:41
 Operator : SY/AP
 Sample : CAN 10608
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 CAN 10608

Quant Time: Aug 28 01:28:02 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL082720AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Aug 27 06:46:28 2020
 QLast Update : Thu Aug 27 06:46:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.69	49	986756	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.20	114	4039457	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.13	117	4038229	10.00	ppbv	0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.46	95	2966194	10.34	ppbv	0.01
Spiked Amount	10.000	Range	65 - 135	Recovery	=	103.40%


Target Compounds					Ovalue
9) Propene	3.03	41	3218	0.076	ppbv 91
15) Acetone	3.90	43	8646	0.079	ppbv # 7
20) Methylene Chloride	4.36	84	10843	0.134	ppbv 91
30) Cyclohexane	7.19	84	4317	0.037	ppbv # 12
39) 1,2-Dichloropropane	7.20	63	740738	8.386	ppbv # 32

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL082720\
Data File : VL035523.D
Acq On : 27 Aug 2020 17:41
Operator : SY/AP
Sample : CAN 10608
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10608

Quant Time: Aug 28 01:28:02 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL082720AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Aug 27 06:46:28 2020
QLast Update : Thu Aug 27 06:46:28 2020
Response via : Initial Calibration




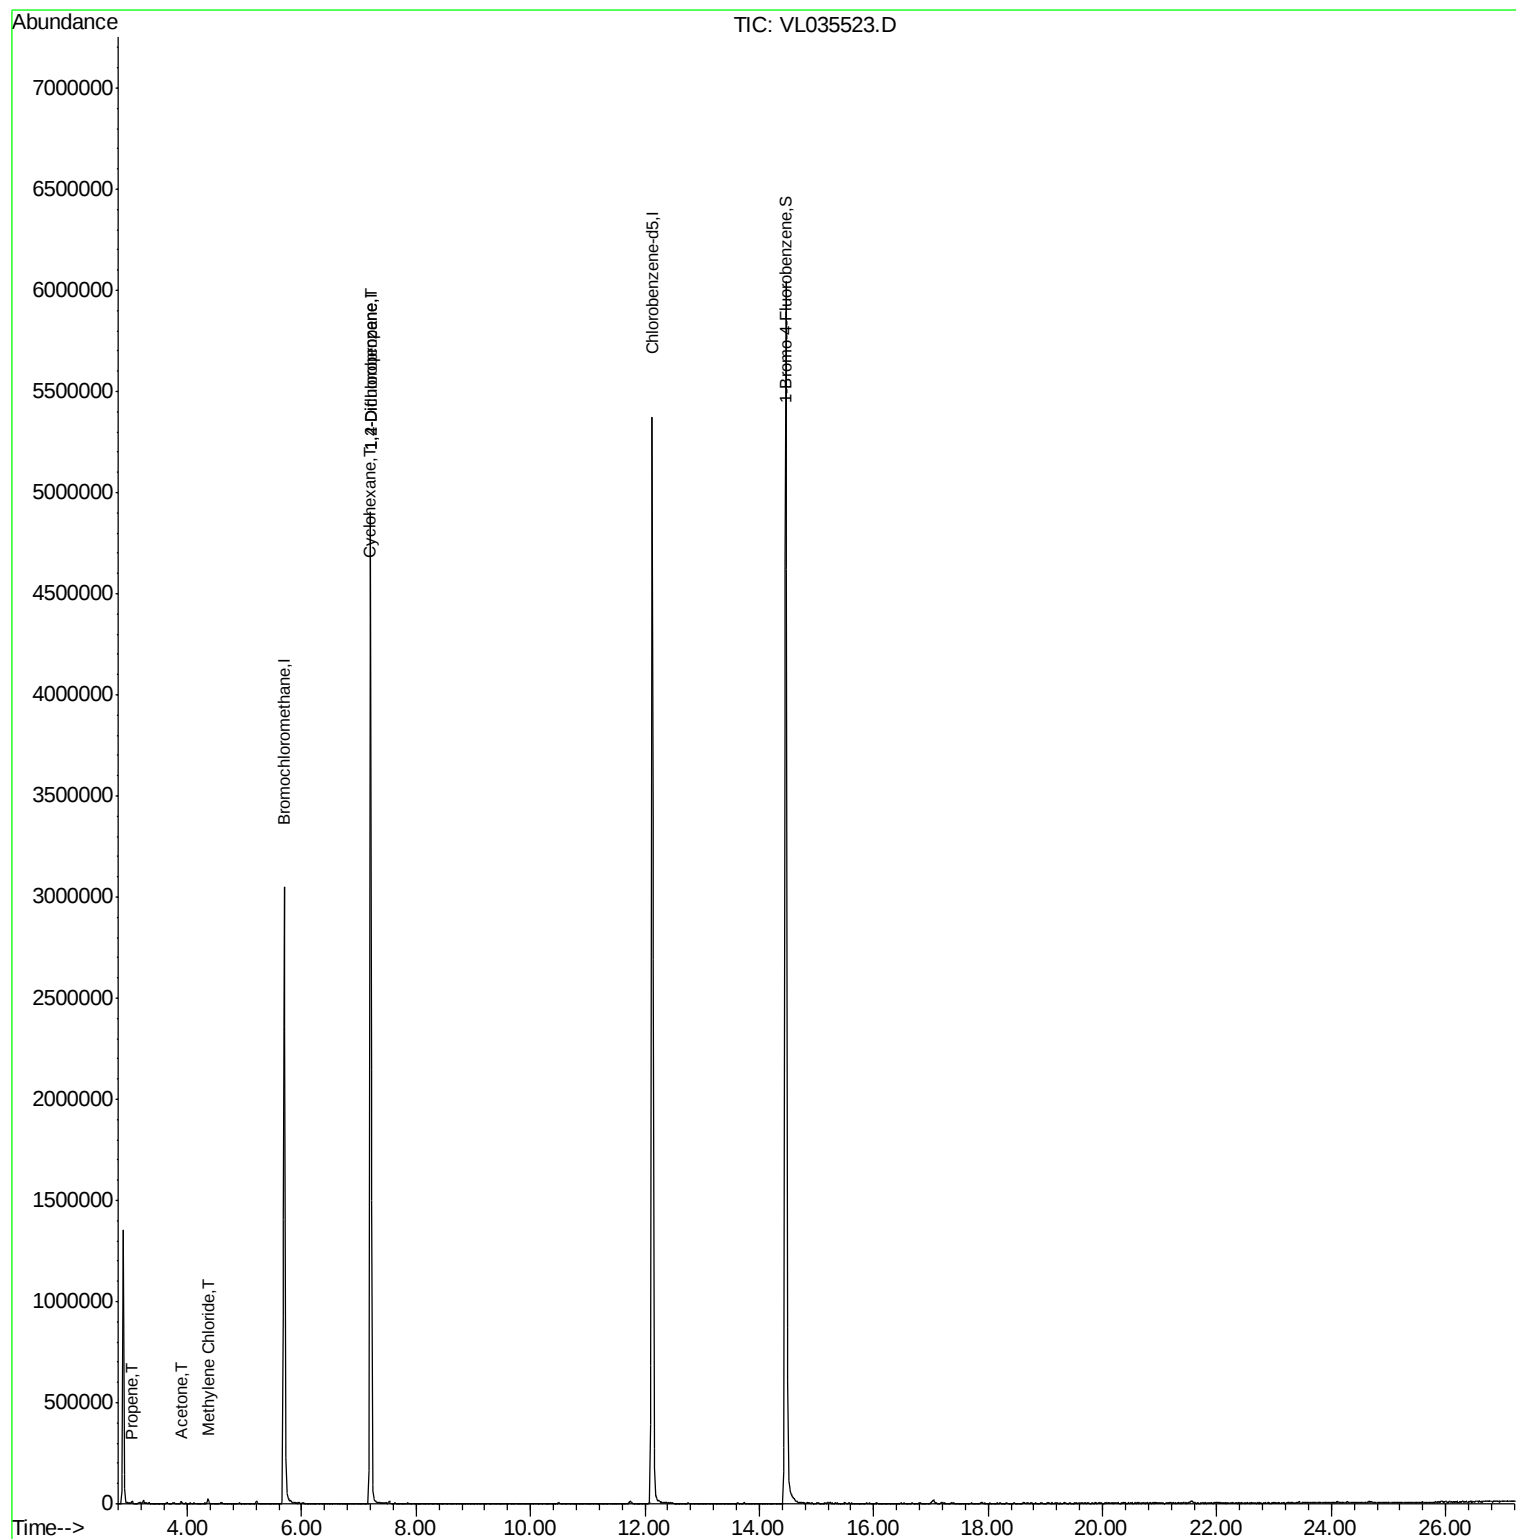




#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.69 min Scan# 903
Delta R.T. 0.01 min
Lab File: VL035523.D
Acq: 27 Aug 2020 17:41




Instrument :
MSVOA_L
ClientSampleId :
CAN 10608


Tot Ion: 49 Resp: 986756
Ion Ratio Lower Upper
49 100
128 96.2 50.0 150.1
130 122.9 64.4 193.2

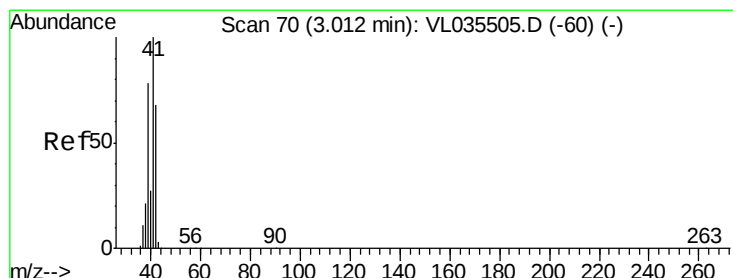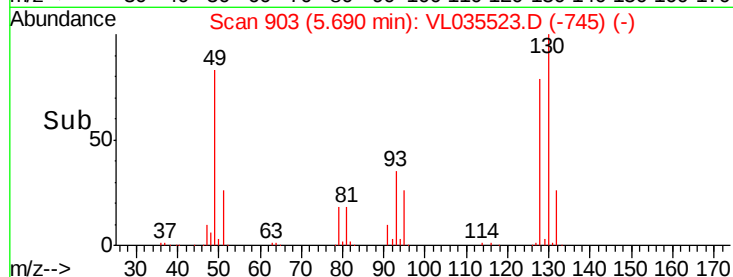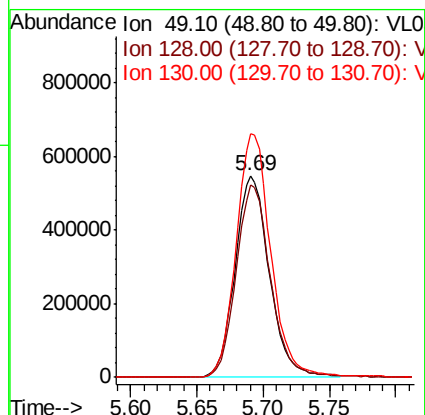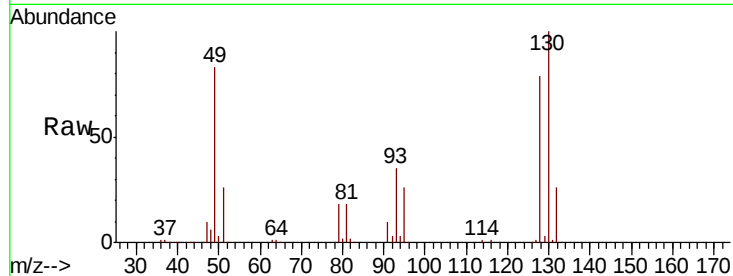

#9
Propene
Concen: 0.076 ppbv
RT: 3.03 min Scan# 76
Delta R.T. 0.02 min
Lab File: VL035523.D
Acq: 27 Aug 2020 17:41

Tgt Ion: 41 Resp: 3218
Ion Ratio Lower Upper
41 100
42 63.2 56.3 84.5

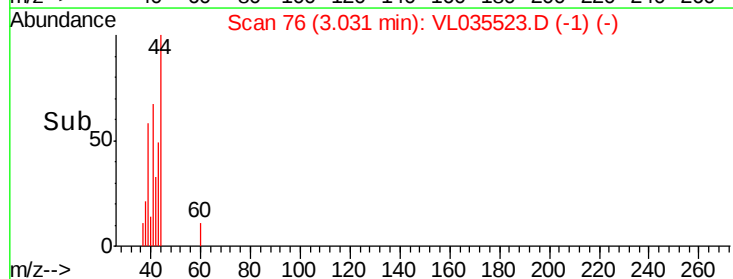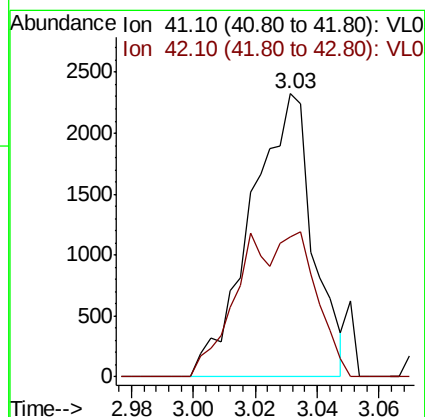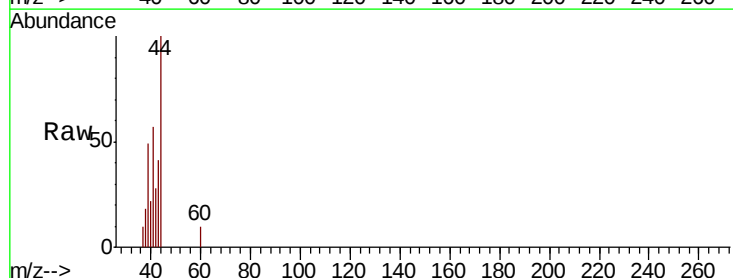

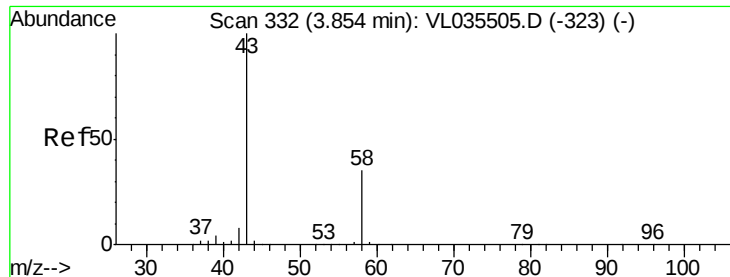

#15

Acetone

Concen: 0.079 ppbv

RT: 3.90 min Scan# 345

Delta R.T. 0.04 min

Lab File: VL035523.D

Acq: 27 Aug 2020 17:41

Instrument :

MSVOA_L

ClientSampleId :


CAN 10608

Tot Ion: 43 Resp: 8646

Ion Ratio Lower Upper




43 100

58 89.7 28.4 42.6#

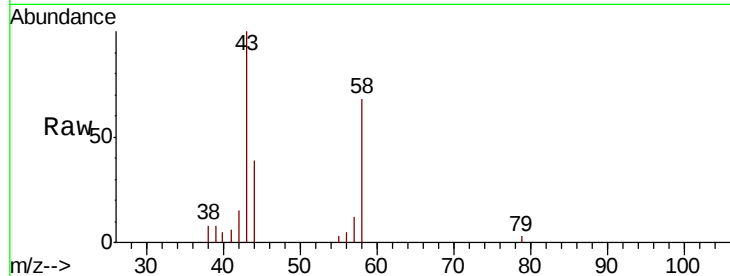

Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 58.10 (57.80 to 58.80): VL0

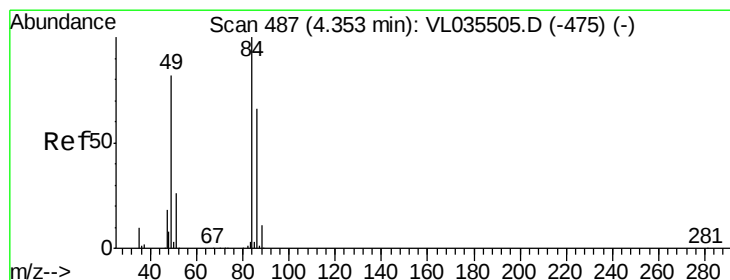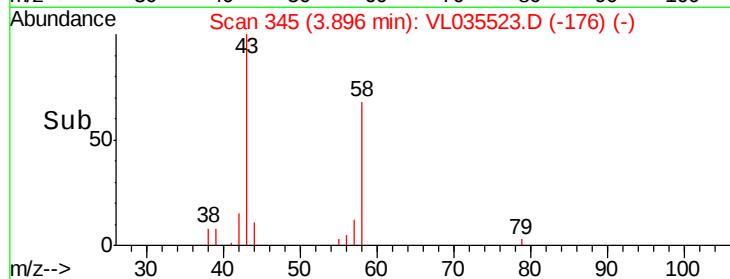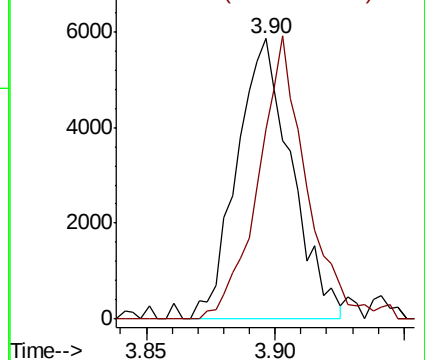

#20

Methylene Chloride

Concen: 0.134 ppbv

RT: 4.36 min Scan# 490

Delta R.T. 0.01 min

Lab File: VL035523.D

Acq: 27 Aug 2020 17:41

Tgt Ion: 84 Resp: 10843


Ion Ratio Lower Upper

84 100

49 70.8 65.4 98.0

51 23.8 21.5 32.3

86 60.1 52.9 79.3


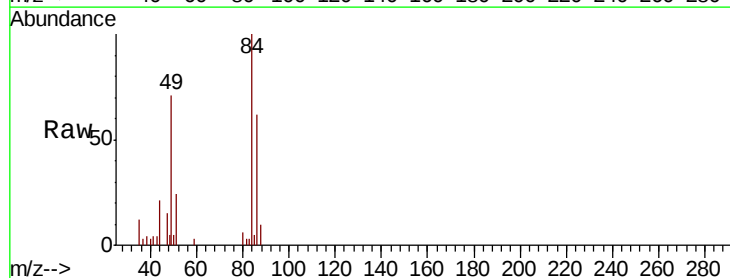



Abundance Ion 84.00 (83.70 to 84.70): VL0

Ion 49.10 (48.80 to 49.80): VL0

Ion 51.10 (50.80 to 51.80): VL0

Ion 86.00 (85.70 to 86.70): VL0

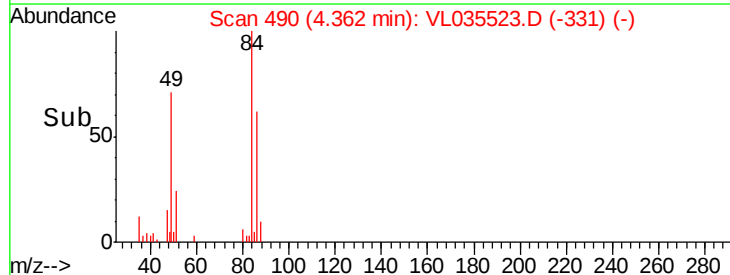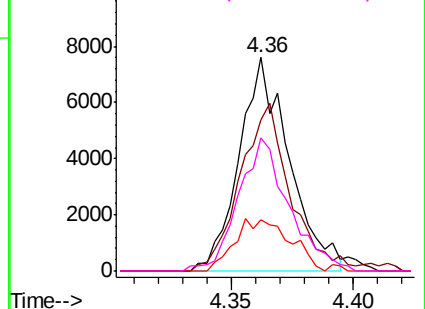


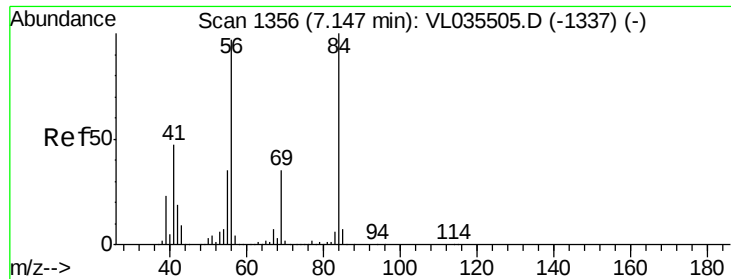




#30
Cvclohexane
Concen: 0.037 ppbv
RT: 7.19 min Scan# 1369
Delta R.T. 0.04 min
Lab File: VL035523.D
Acq: 27 Aug 2020 17:41

Instrument :
MSVOA_L
ClientSampleId :
CAN 10608

Tot Ion: 84 Resp: 4317
Ion Ratio Lower Upper
84 100
56 0.0 80.1 120.1#
41 5.7 38.1 57.1#

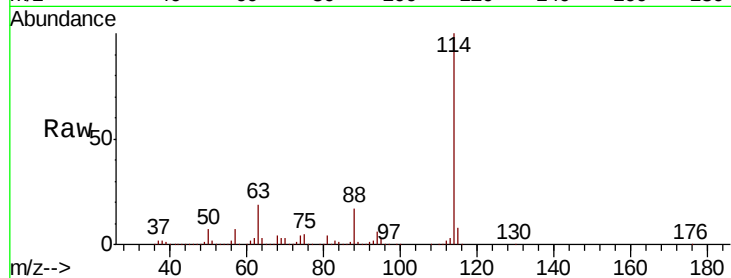


Abundance Ion 84.20 (83.90 to 84.90): VL0
Ion 56.10 (55.80 to 56.80): VL0
Ion 41.10 (40.80 to 41.80): VL0

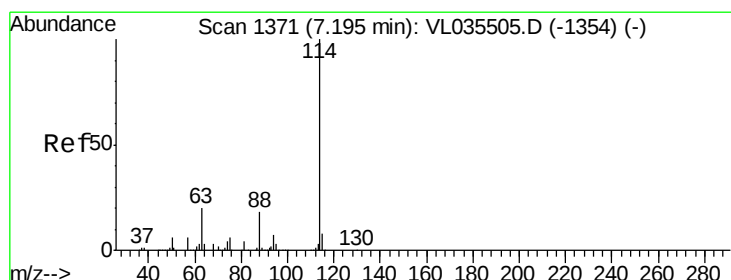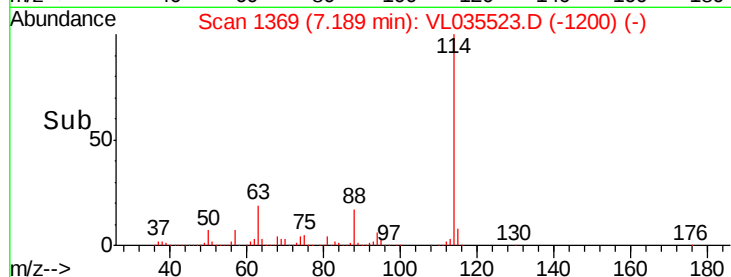
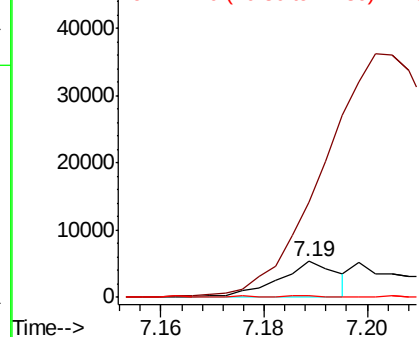



#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.20 min Scan# 1374
Delta R.T. 0.01 min
Lab File: VL035523.D
Acq: 27 Aug 2020 17:41

Tgt Ion: 114 Resp: 4039457
Ion Ratio Lower Upper
114 100
63 18.4 14.7 22.1
88 16.7 13.4 20.2

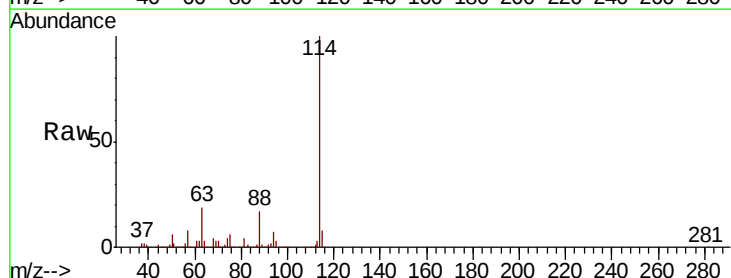

Abundance Ion 114.10 (113.80 to 114.80): V
Ion 63.10 (62.80 to 63.80): VL0
Ion 88.10 (87.80 to 88.80): VL0

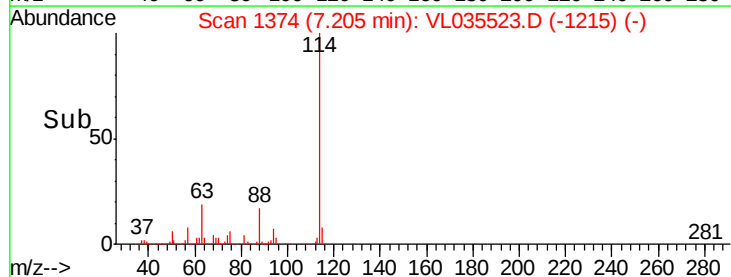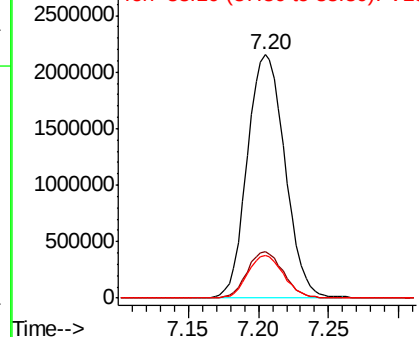

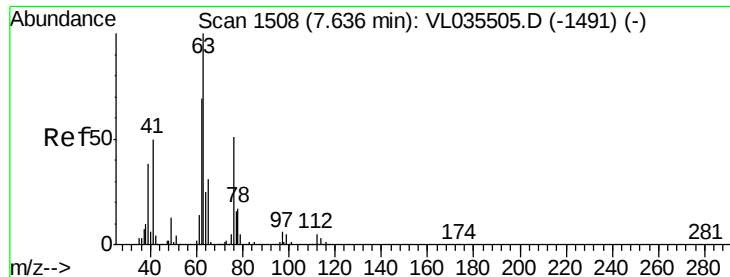

#39

1,2-Dichloropropane

Concen: 8.386 ppbv

RT: 7.20 min Scan# 1374

Delta R.T. -0.43 min

Lab File: VL035523.D

Acq: 27 Aug 2020 17:41

Instrument :

MSVOA_L

ClientSampled :

CAN 10608


Tot Ion: 63 Resp: 740738

Ion Ratio Lower Upper

63 100

41 0.0 40.0 60.0#




62 15.7 55.4 83.0#

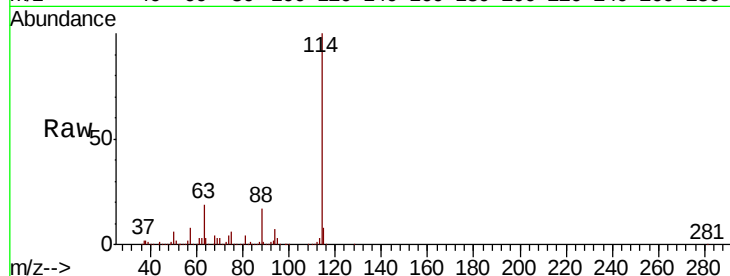

Abundance Ion 63.10 (62.80 to 63.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 62.10 (61.80 to 62.80): VL0

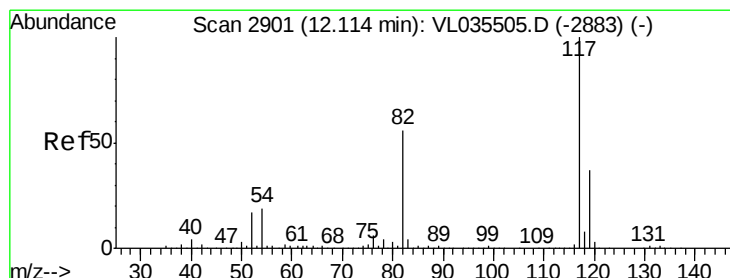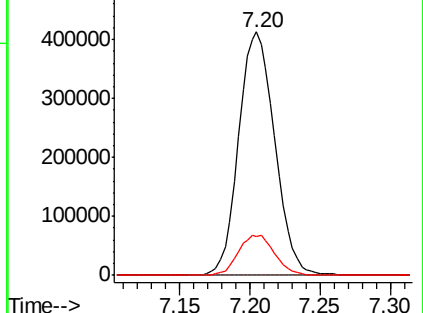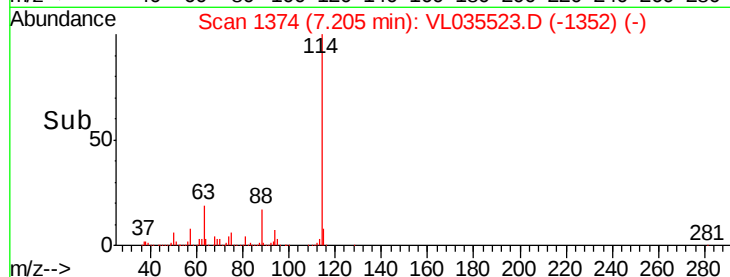

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.13 min Scan# 2906

Delta R.T. 0.02 min

Lab File: VL035523.D

Acq: 27 Aug 2020 17:41


Tgt Ion: 117 Resp: 4038229

Ion Ratio Lower Upper

117 100

82 55.4 41.6 62.4



119 34.5 29.3 43.9

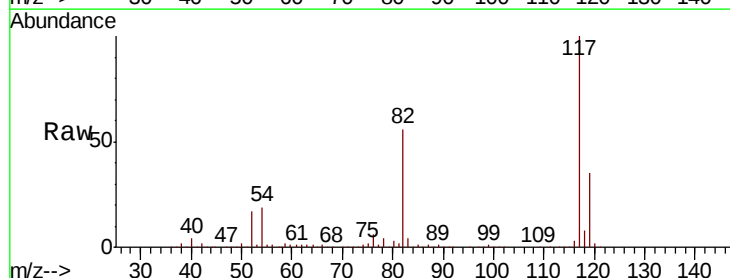


Abundance Ion 117.10 (116.80 to 117.80): V

Ion 82.10 (81.80 to 82.80): VL0

Ion 119.10 (118.80 to 119.80): V

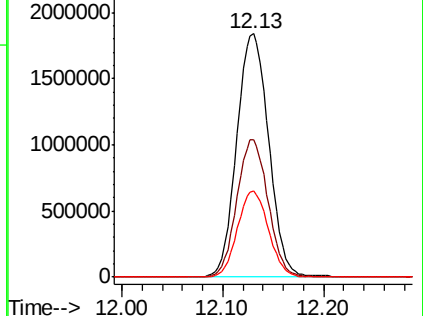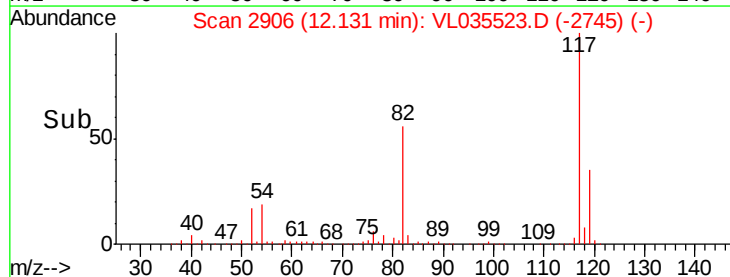

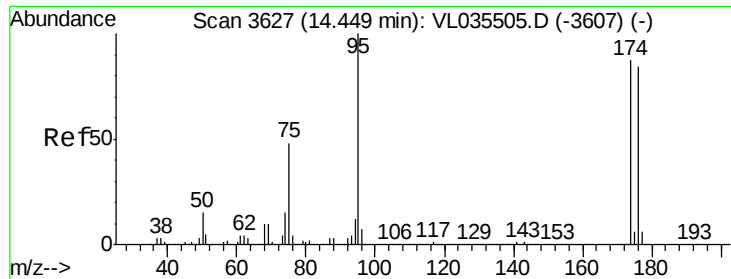

#68

1-Bromo-4-Fluorobenzene

Concen: 10.343 ppbv

RT: 14.46 min Scan# 3631

Delta R.T. 0.01 min

Lab File: VL035523.D

Acq: 27 Aug 2020 17:41

Instrument :

MSVOA_L

ClientSampleId :

CAN 10608


Tot Ion: 95 Resp: 2966194

Ion Ratio Lower Upper

95 100

174 88.0 69.6 104.4

175 6.3 5.1 7.7

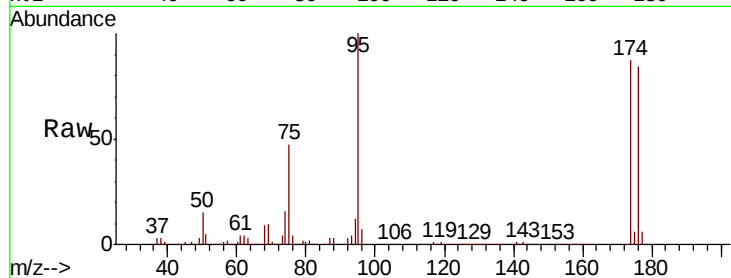

Abundance Ion 95.10 (94.80 to 95.80): VL0

Ion 174.00 (173.70 to 174.70): V

Ion 175.00 (174.70 to 175.70): V

