

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL082720\
Data File : VL035519.D
Acq On : 27 Aug 2020 13:56
Operator : SY/AP
Sample : QC081820 CAN 10328
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC081820 CAN 10328

Quant Time: Aug 28 11:15:33 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL082720AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Aug 27 06:46:28 2020
QLast Update : Thu Aug 27 06:46:28 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.69	49	977831	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.20	114	4117045	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.13	117	4164338	10.00	ppbv	0.01

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.46	95	3030567	10.25	ppbv	0.01
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.50%


Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL082720\
Data File : VL035519.D
Acq On : 27 Aug 2020 13:56
Operator : SY/AP
Sample : QC081820 CAN 10328
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC081820 CAN 10328

Quant Time: Aug 28 11:15:33 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL082720AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Aug 27 06:46:28 2020
QLast Update : Thu Aug 27 06:46:28 2020
Response via : Initial Calibration

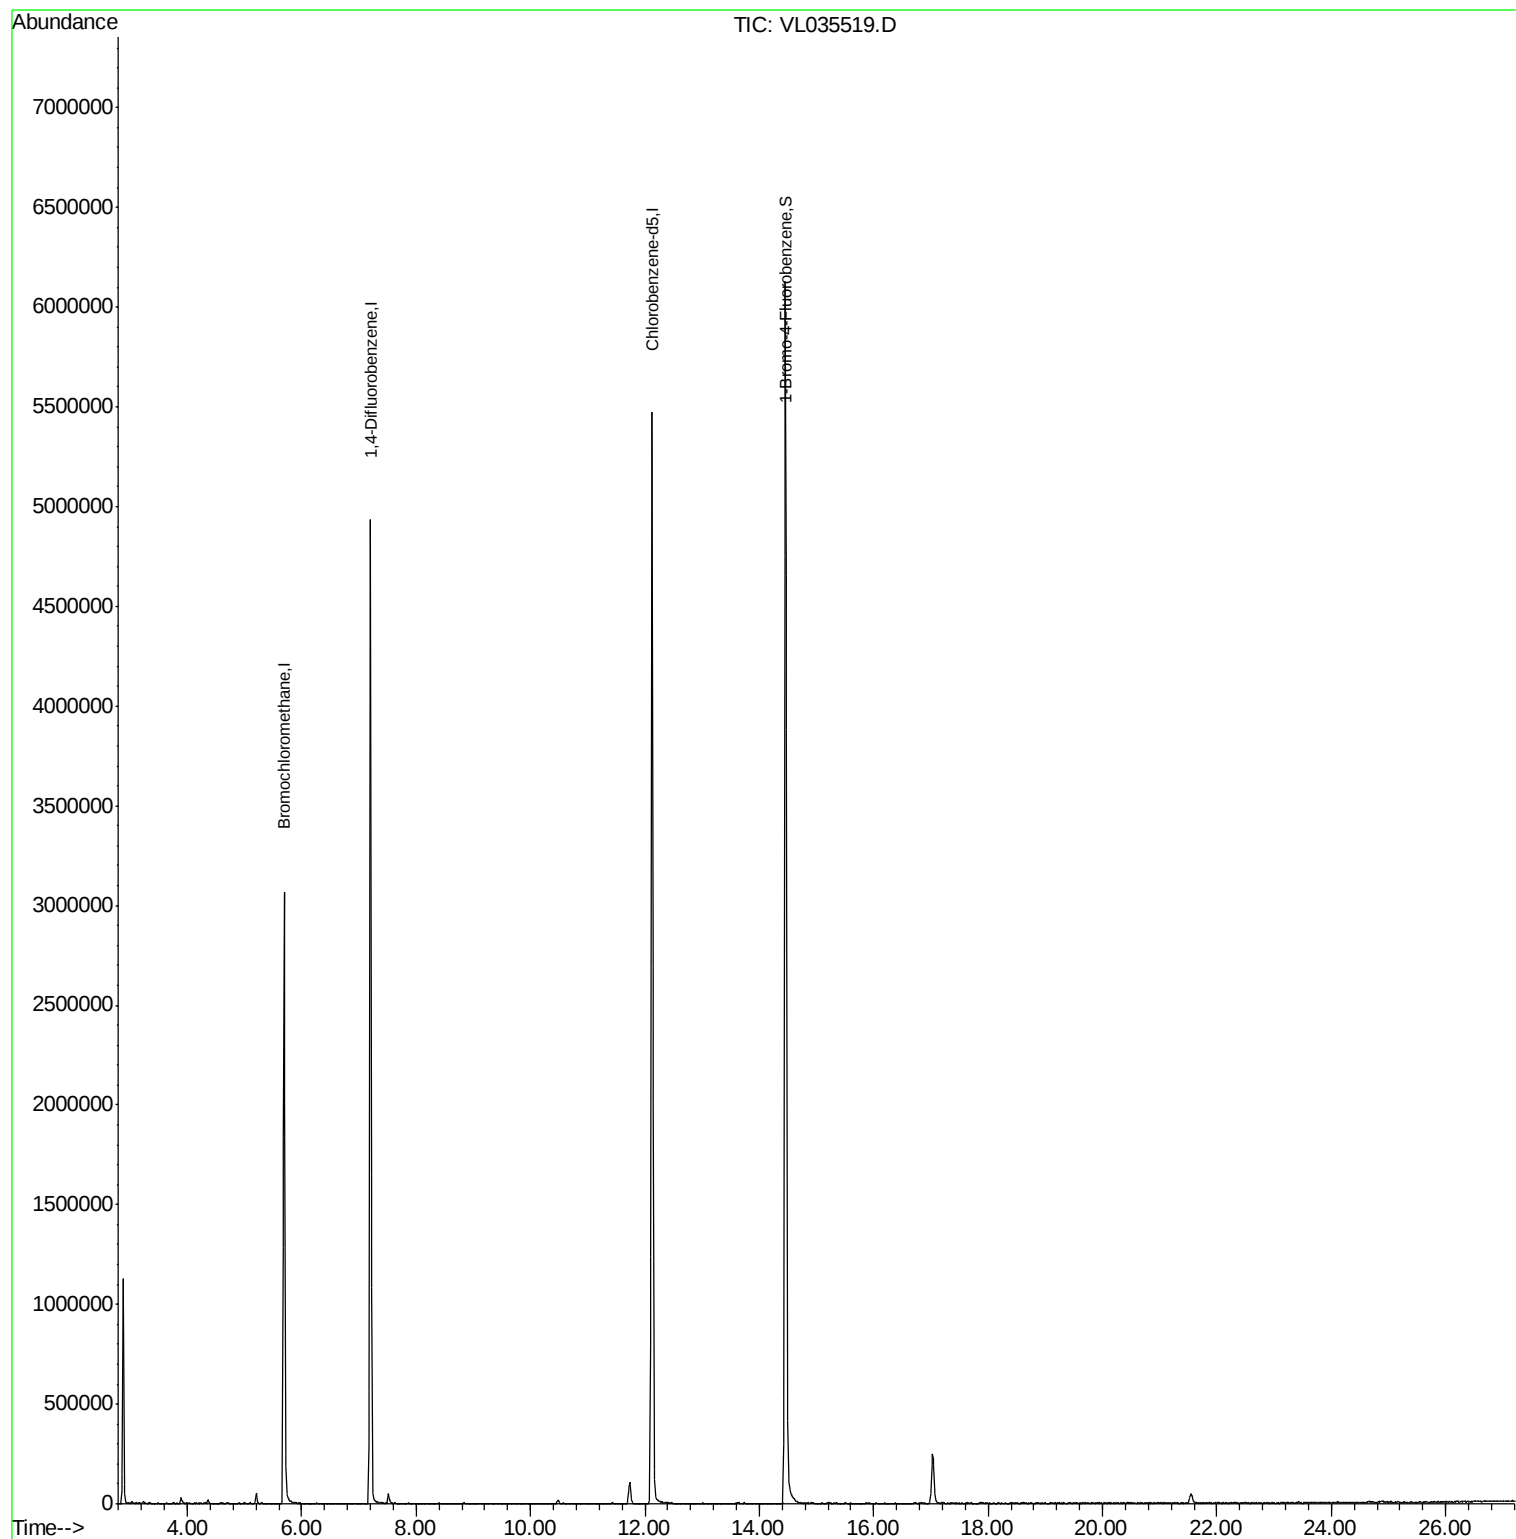



#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.69 min Scan# 902

Delta R.T. 0.00 min

Lab File: VL035519.D

Acq: 27 Aug 2020 13:56

Instrument :

MSVOA_L

ClientSampleId :

QC081820 CAN 10328


Tot Ion: 49 Resp: 977831

Ion Ratio Lower Upper

49 100

128 97.3 50.0 150.1




130 126.1 64.4 193.2

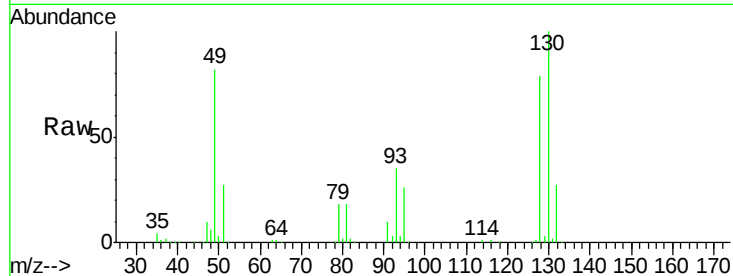

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

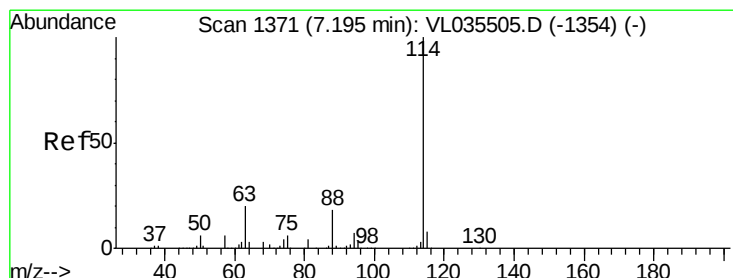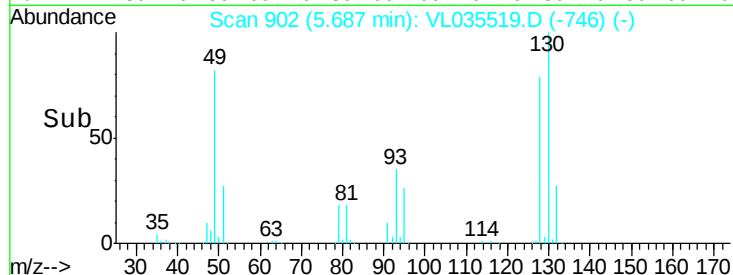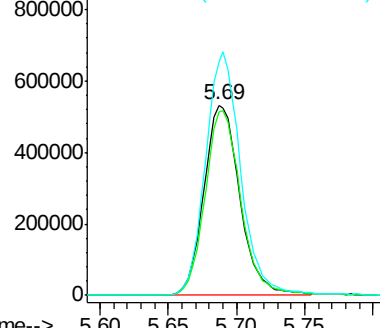

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.20 min Scan# 1373

Delta R.T. 0.01 min

Lab File: VL035519.D

Acq: 27 Aug 2020 13:56


Tgt Ion: 114 Resp: 4117045

Ion Ratio Lower Upper

114 100

63 18.3 14.7 22.1



88 16.6 13.4 20.2

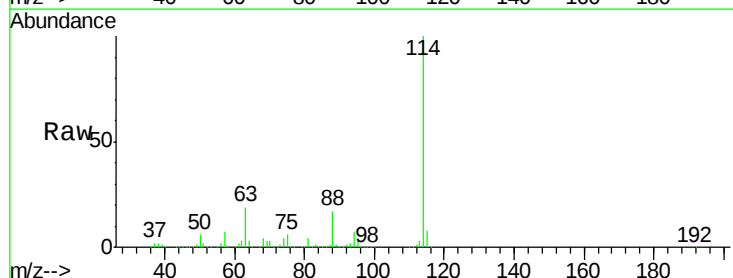


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0

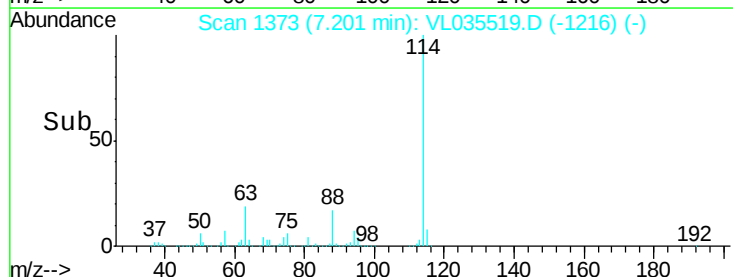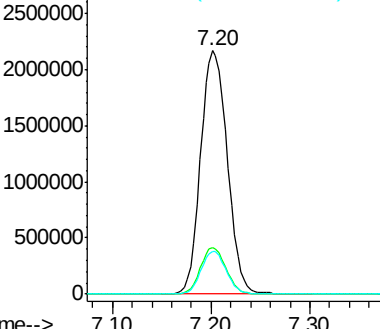


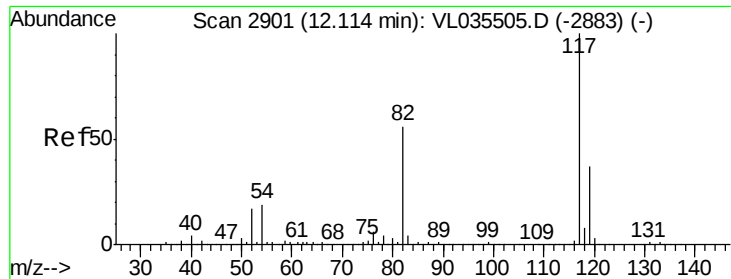




#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.13 min Scan# 2905
Delta R.T. 0.01 min
Lab File: VL035519.D
Acq: 27 Aug 2020 13:56

Instrument :
MSVOA_L
ClientSampleId :
QC081820 CAN 10328

Tot Ion:117 Resp: 4164338
Ion Ratio Lower Upper
117 100
82 54.8 41.6 62.4
119 34.5 29.3 43.9

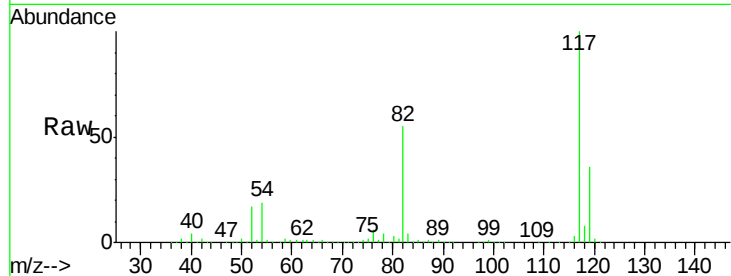


Abundance Ion 117.10 (116.80 to 117.80): V
Ion 82.10 (81.80 to 82.80): V
Ion 119.10 (118.80 to 119.80): V

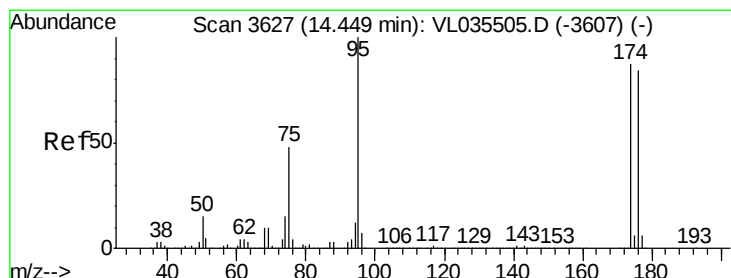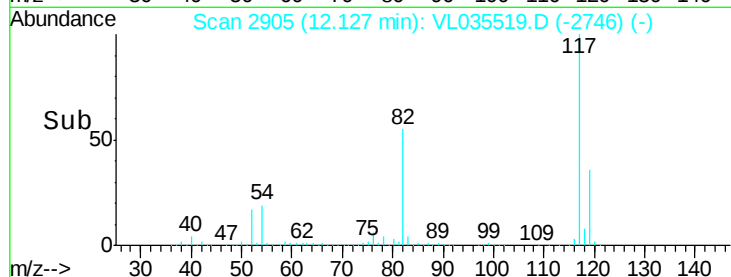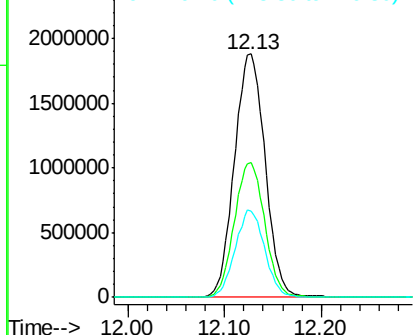

#68
1-Bromo-4-Fluorobenzene
Concen: 10.248 ppbv
RT: 14.46 min Scan# 3631
Delta R.T. 0.01 min
Lab File: VL035519.D
Acq: 27 Aug 2020 13:56

Tgt Ion: 95 Resp: 3030567
Ion Ratio Lower Upper
95 100
174 88.0 69.6 104.4
175 6.3 5.1 7.7

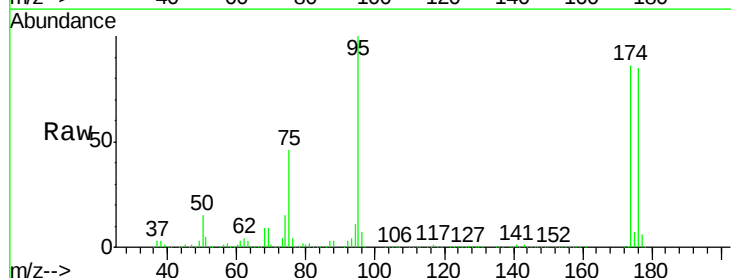

Abundance Ion 95.10 (94.80 to 95.80): V
Ion 174.00 (173.70 to 174.70): V
Ion 175.00 (174.70 to 175.70): V

