


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL082720\
Data File : VL035504.D
Acq On : 27 Aug 2020 1:31
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL082720AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Aug 27 06:46:28 2020
Last Update : Thu Aug 27 06:46:28 2020

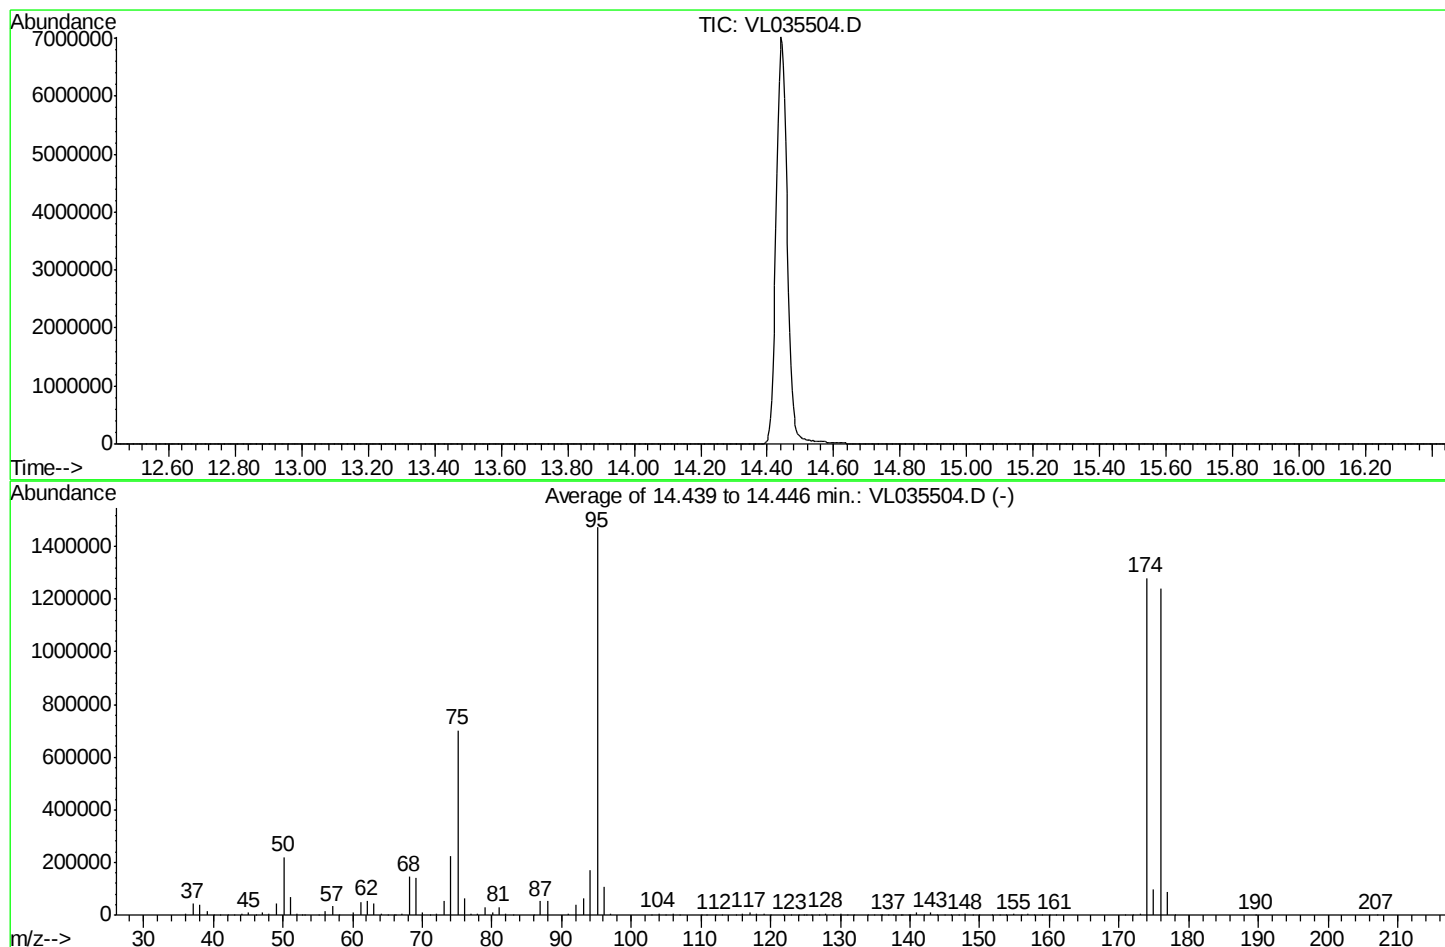

AutoFind: Scans 3624, 3625, 3626; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	15.0	221354	PASS
75	95	30	66	47.6	701866	PASS
95	95	100	100	100.0	1473536	PASS
96	95	5	9	7.3	108202	PASS
173	174	0.00	2	0.6	7342	PASS
174	95	50	120	86.8	1279658	PASS
175	174	4	9	7.4	95133	PASS
176	174	93	101	97.0	1240917	PASS
177	176	5	9	7.1	88138	PASS