



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL083122\
Data File : VL039602.D
Acq On : 31 Aug 2022 8:36
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081722AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Aug 26 06:05:16 2022

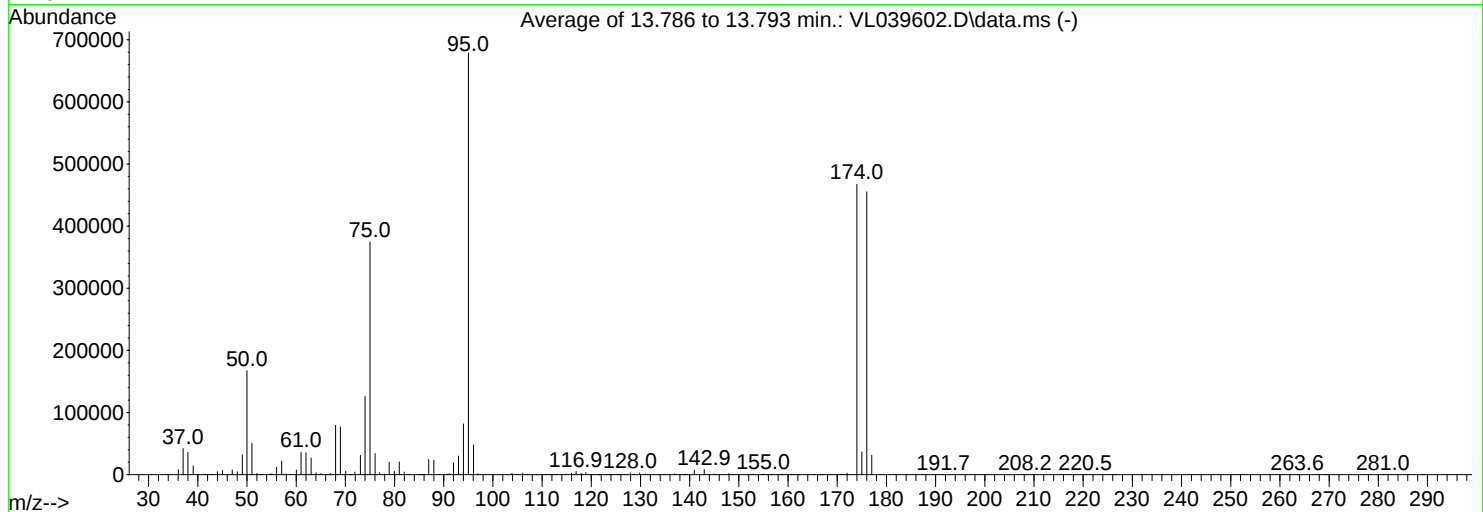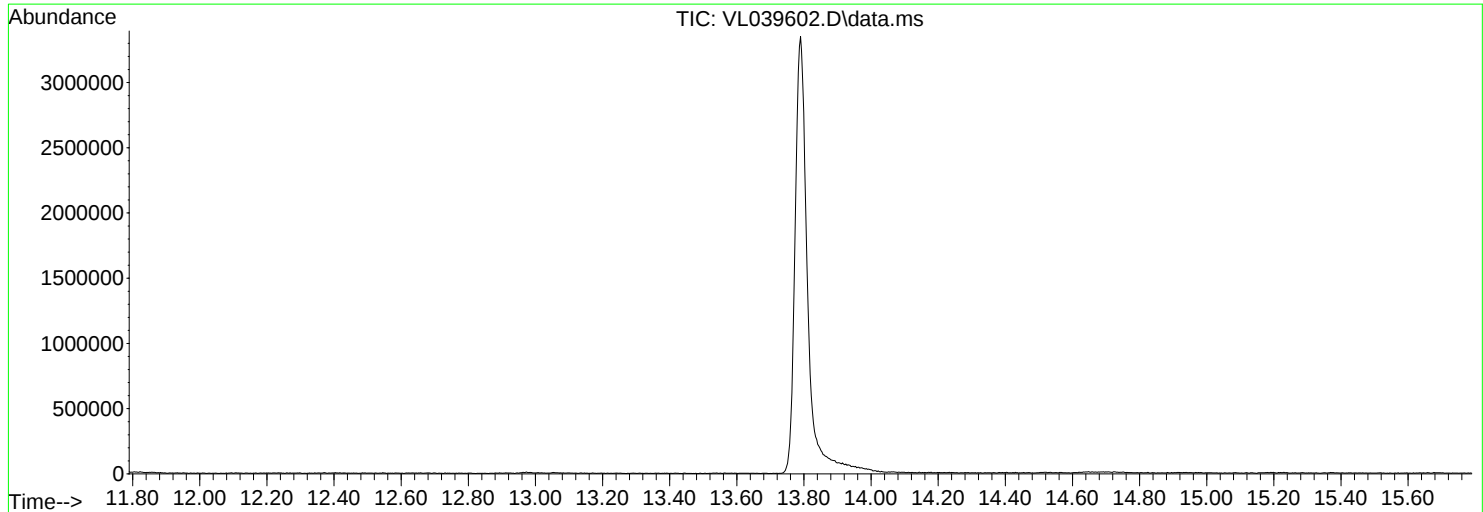

AutoFind: Scans 3478, 3479, 3480; Background Corrected with Scan 3456

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.7	167381	PASS
75	95	30	66	55.2	374528	PASS
95	95	100	100	100.0	678955	PASS
96	95	5	9	7.1	47880	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.8	467349	PASS
175	174	4	9	7.8	36501	PASS
176	174	93	101	97.4	455296	PASS
177	176	5	9	6.9	31288	PASS

Average of 13.786 to 13.793 min.: VL039602.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7719	46.20	625	56.00	11792	66.25	251
37.00	42011	47.00	7791	57.05	21845	66.95	1931
38.00	35824	48.05	4625	57.95	1296	68.00	7934
39.05	14280	49.05	32304	58.85	225	69.00	7702
40.15	672	50.00	167381	60.05	7469	70.05	5424
41.50	82	51.00	50432	61.00	36077	70.85	136
42.90	333	52.05	2129	62.00	35397	71.95	4189
43.05	276	52.70	76	63.05	26813	73.05	31037
44.00	4878	53.15	215	64.05	3061	74.00	126179
45.00	6767	54.85	1348	65.05	1982	75.00	374528
45.90	204	55.10	964	65.70	116	76.05	34125

Average of 13.786 to 13.793 min.: VL039602.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.95	3429	86.10	434	102.95	289	111.90	311
78.00	1067	86.95	24312	103.75	1489	112.10	350
78.90	19760	88.00	23360	103.95	1693	112.75	371
79.95	5367	90.80	885	104.85	888	113.00	199
80.95	20485	91.10	1485	106.05	2626	114.90	718
81.95	4144	92.00	18987	107.05	657	115.95	2259
82.75	514	93.00	29997	108.80	60	116.90	5094
84.00	283	94.00	81667	110.00	304	117.70	624
85.20	65	95.00	678955	110.75	557	117.95	1748
85.60	136	96.05	47880	111.00	244	118.90	3478
85.85	419	96.95	1389	111.60	88	119.70	297

Average of 13.786 to 13.793 min.: VL039602.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
121.50	112	128.85	883	139.05	503	147.95	1606
121.70	101	129.85	2672	139.60	179	148.85	649
123.00	156	131.05	1056	139.95	508	149.50	189
123.60	66	131.90	104	140.95	6900	149.95	863
123.90	284	133.70	110	142.00	908	151.70	109
124.10	131	134.60	275	142.95	8260	151.95	200
125.30	135	135.00	349	143.90	416	152.70	253
125.80	61	135.15	767	144.90	921	152.95	738
126.75	320	135.85	430	145.75	404	153.70	55
127.20	71	136.95	1380	146.00	255	154.05	543
127.95	2721	138.80	93	146.90	368	154.60	371

Average of 13.786 to 13.793 min.: VL039602.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.00	1136	166.00	67	175.00	36501	269.30	51
155.70	72	166.50	154	176.00	455296	281.00	66
156.35	377	167.20	187	177.00	31288	289.00	64
156.70	229	168.00	52	177.90	789		
156.95	879	168.30	203	184.00	107		
158.70	95	169.00	186	191.65	129		
158.90	788	170.05	551	208.20	132		
160.50	154	170.60	210	218.20	99		
160.95	539	170.90	510	220.50	124		
162.10	151	172.00	2595	226.50	93		
165.20	78	174.00	467349	263.60	64		