


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL090518\  
Data File : VL032452.D  
Acq On : 5 Sep 2018 9:31  
Operator : SY/AP  
Sample : BFB  
Misc : 400ml/MSVOA L  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_L  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL083118AIR.M  
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Fri Aug 31 21:33:46 2018  
Last Update : Fri Aug 31 21:33:46 2018

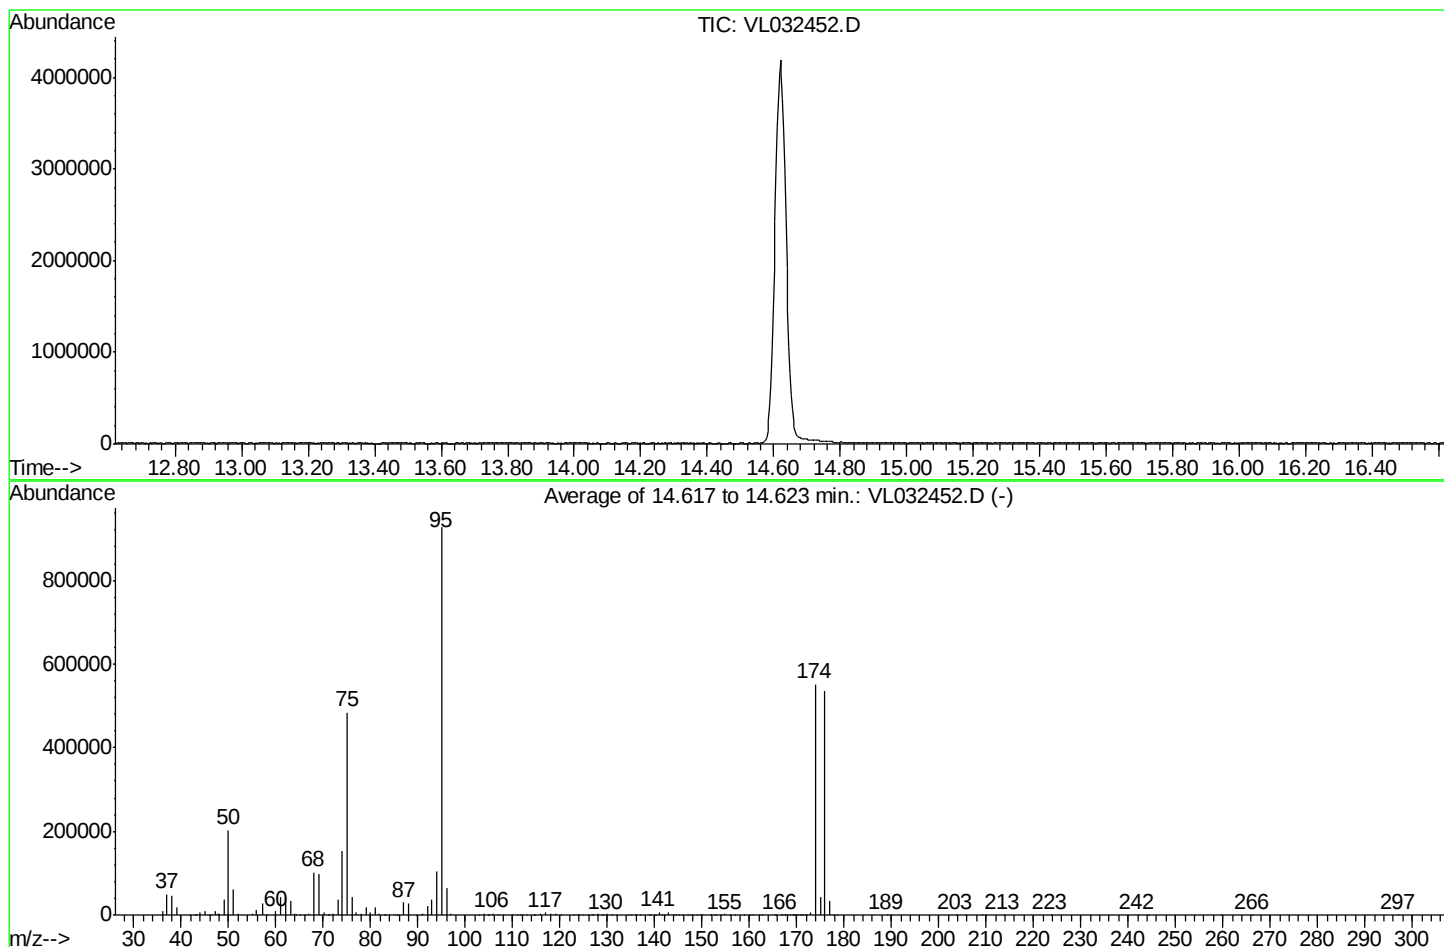

AutoFind: Scans 4208, 4209, 4210; Background Corrected with Scan 4182

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 8            | 40           | 21.9      | 203008  | PASS             |
| 75          | 95           | 30           | 66           | 52.2      | 484096  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 926698  | PASS             |
| 96          | 95           | 5            | 9            | 6.9       | 63581   | PASS             |
| 173         | 174          | 0.00         | 2            | 1.4       | 7689    | PASS             |
| 174         | 95           | 50           | 120          | 59.6      | 552106  | PASS             |
| 175         | 174          | 4            | 9            | 7.9       | 43816   | PASS             |
| 176         | 174          | 93           | 101          | 96.9      | 534762  | PASS             |
| 177         | 176          | 5            | 9            | 6.4       | 34144   | PASS             |