


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL090519\
 Data File : VL034119.D
 Acq On : 5 Sep 2019 1:50
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL090519AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Sep 05 10:21:45 2019
 Last Update : Thu Sep 05 10:21:45 2019

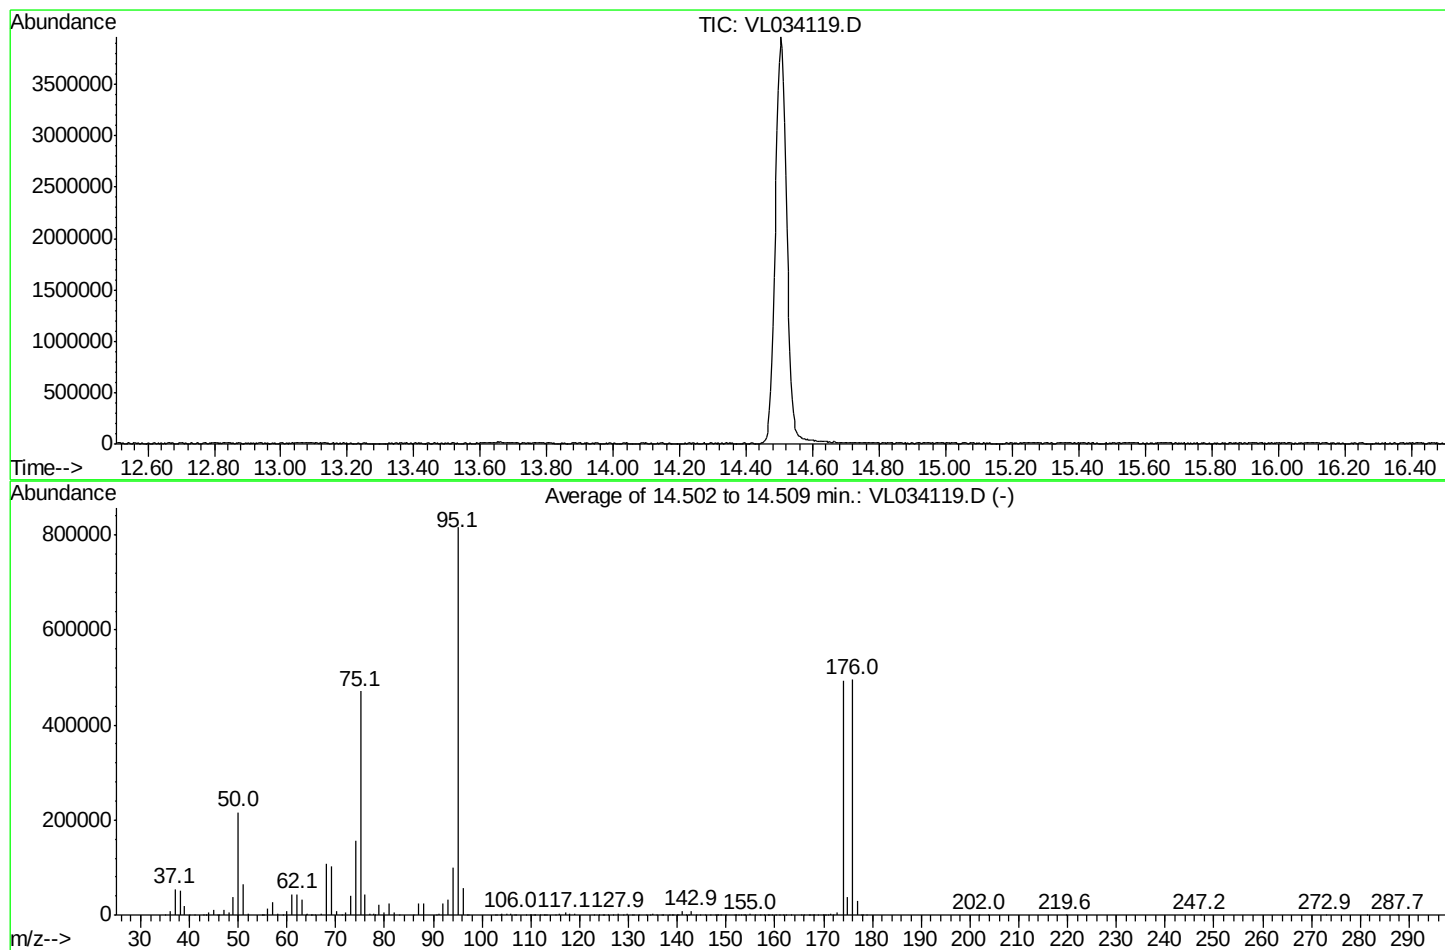

AutoFind: Scans 3597, 3598, 3599; Background Corrected with Scan 3573

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.5	216128	PASS
75	95	30	66	57.8	471466	PASS
95	95	100	100	100.0	816320	PASS
96	95	5	9	7.1	57832	PASS
173	174	0.00	2	0.9	4212	PASS
174	95	50	120	60.3	492330	PASS
175	174	4	9	7.5	37013	PASS
176	174	93	101	100.5	494954	PASS
177	176	5	9	6.0	29816	PASS