
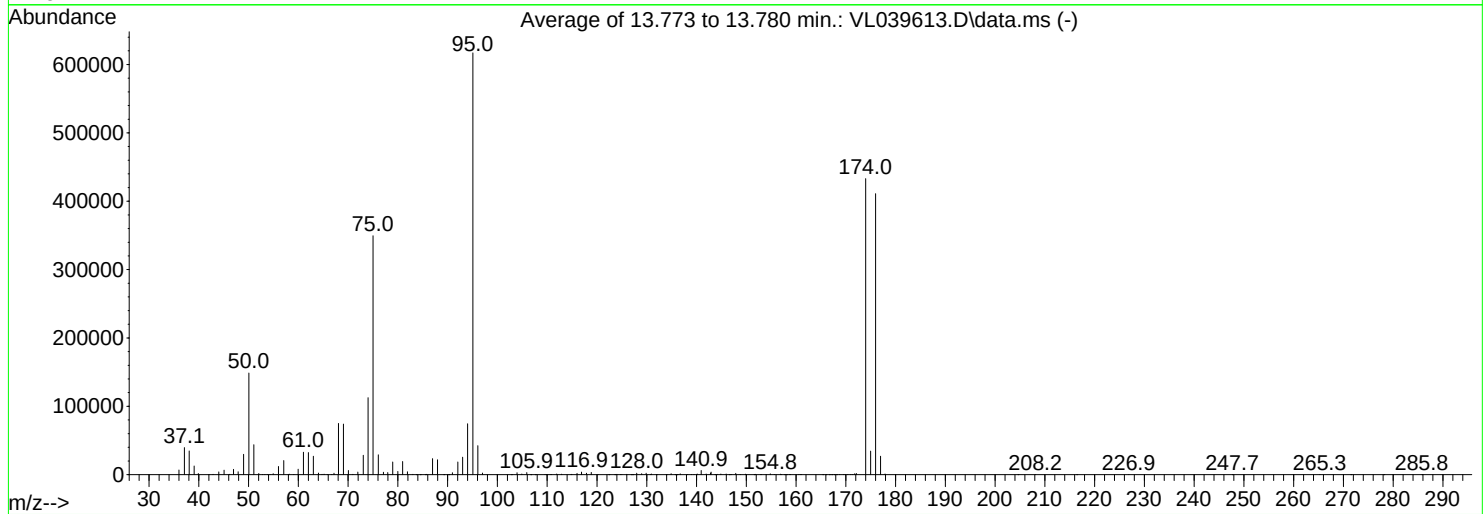


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL090722\
 Data File : VL039613.D
 Acq On : 7 Sep 2022 8:29
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081722AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Fri Aug 26 06:05:16 2022

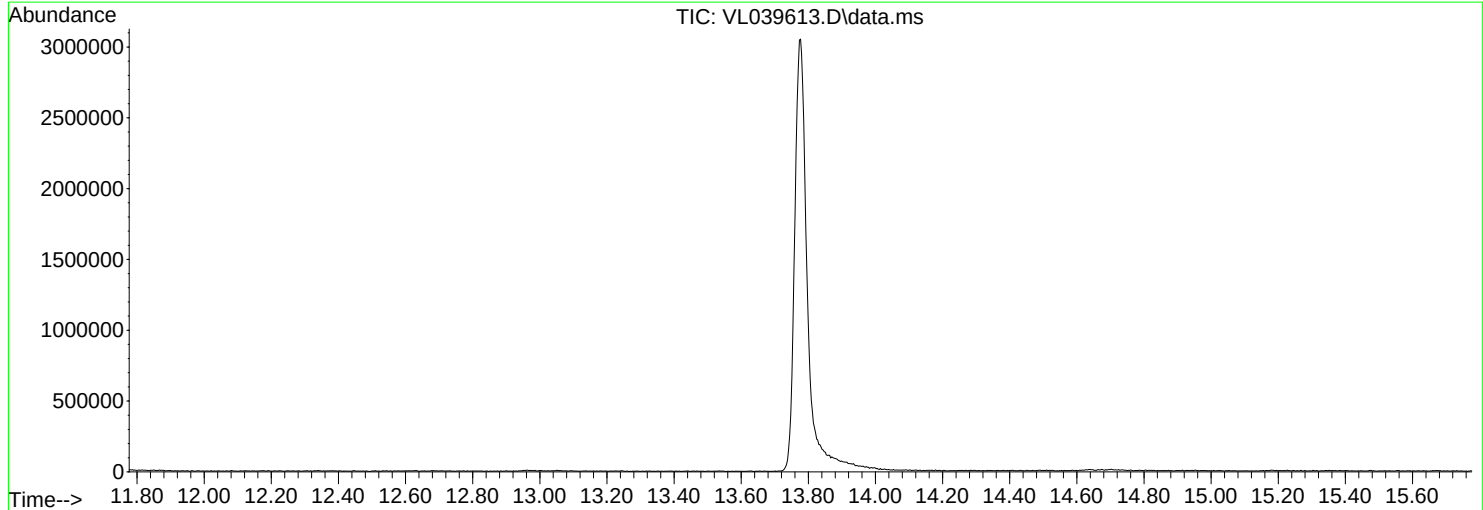

AutoFind: Scans 3474, 3475, 3476; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.1	148672	PASS
75	95	30	66	56.6	349504	PASS
95	95	100	100	100.0	617109	PASS
96	95	5	9	6.9	42395	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.2	433003	PASS
175	174	4	9	8.0	34555	PASS
176	174	93	101	94.9	410987	PASS
177	176	5	9	6.6	26989	PASS

Average of 13.773 to 13.780 min.: VL039613.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	6785	47.90	4242	57.05	20672	65.80	361
37.10	39595	49.00	29667	58.00	293	66.70	270
38.05	34739	50.05	148672	58.15	618	67.15	203
39.05	12672	51.05	43720	59.10	285	68.05	7503
39.90	1578	52.05	1689	59.95	8044	69.05	73925
42.05	202	52.80	151	61.00	32781	70.05	6002
42.85	437	53.25	173	62.00	32253	70.95	386
44.00	4064	53.75	147	63.00	26957	71.95	3676
45.05	6644	54.30	143	64.05	2352	73.05	28400
46.15	510	54.95	1523	64.75	606	74.00	112547
46.95	7759	56.00	11856	65.15	701	75.00	349504

Average of 13.773 to 13.780 min.: VL039613.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	28976	85.75	567	97.00	2303	110.60	231
77.10	3623	86.95	23405	102.80	77	110.85	301
77.95	3086	87.95	21773	103.95	2894	111.90	837
78.95	18456	89.20	79	104.90	961	112.90	682
80.00	4787	90.20	70	105.90	3132	114.80	184
80.95	19215	90.95	2732	106.70	73	114.95	563
81.90	4159	92.05	18616	106.80	377	116.00	1932
83.00	431	93.00	25475	107.60	80	116.90	3745
83.70	90	94.00	74512	109.55	215	117.90	2094
84.50	76	95.05	617109	109.80	57	118.85	3288
85.50	56	96.05	42395	110.10	130	120.20	176

Average of 13.773 to 13.780 min.: VL039613.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.40	85	130.80	500	140.15	964	147.90	1853
123.60	85	130.95	940	140.95	6036	148.80	360
124.00	444	131.90	63	141.95	848	149.85	754
124.75	351	133.90	55	142.80	2388	151.60	75
125.00	211	134.90	1422	142.95	3791	151.85	539
126.00	413	135.70	96	143.70	124	152.90	361
126.90	100	136.10	116	144.15	522	153.05	210
127.20	60	136.75	1270	144.90	839	154.00	167
128.00	2113	138.20	143	145.95	861	154.85	1117
129.00	1328	139.00	233	146.60	74	155.65	193
129.90	2066	139.50	275	147.00	128	156.90	668

Average of 13.773 to 13.780 min.: VL039613.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.10	335	167.20	54	174.00	433003	271.50	57
157.70	74	167.70	84	175.00	34555	278.10	54
158.10	71	168.15	120	176.00	410987	285.80	83
158.65	366	168.75	152	177.00	26989		
158.90	275	169.60	317	177.90	907		
160.60	134	169.90	250	204.60	119		
160.90	293	170.40	314	208.15	154		
161.10	285	171.00	265	216.40	76		
165.40	61	171.40	141	226.90	140		
166.00	64	171.80	1434	247.70	93		
166.70	64	172.15	1560	265.30	141		