


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL090723\
Data File : VL040666.D
Acq On : 7 Sep 2023 9:56
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL081523AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Aug 16 05:43:50 2023

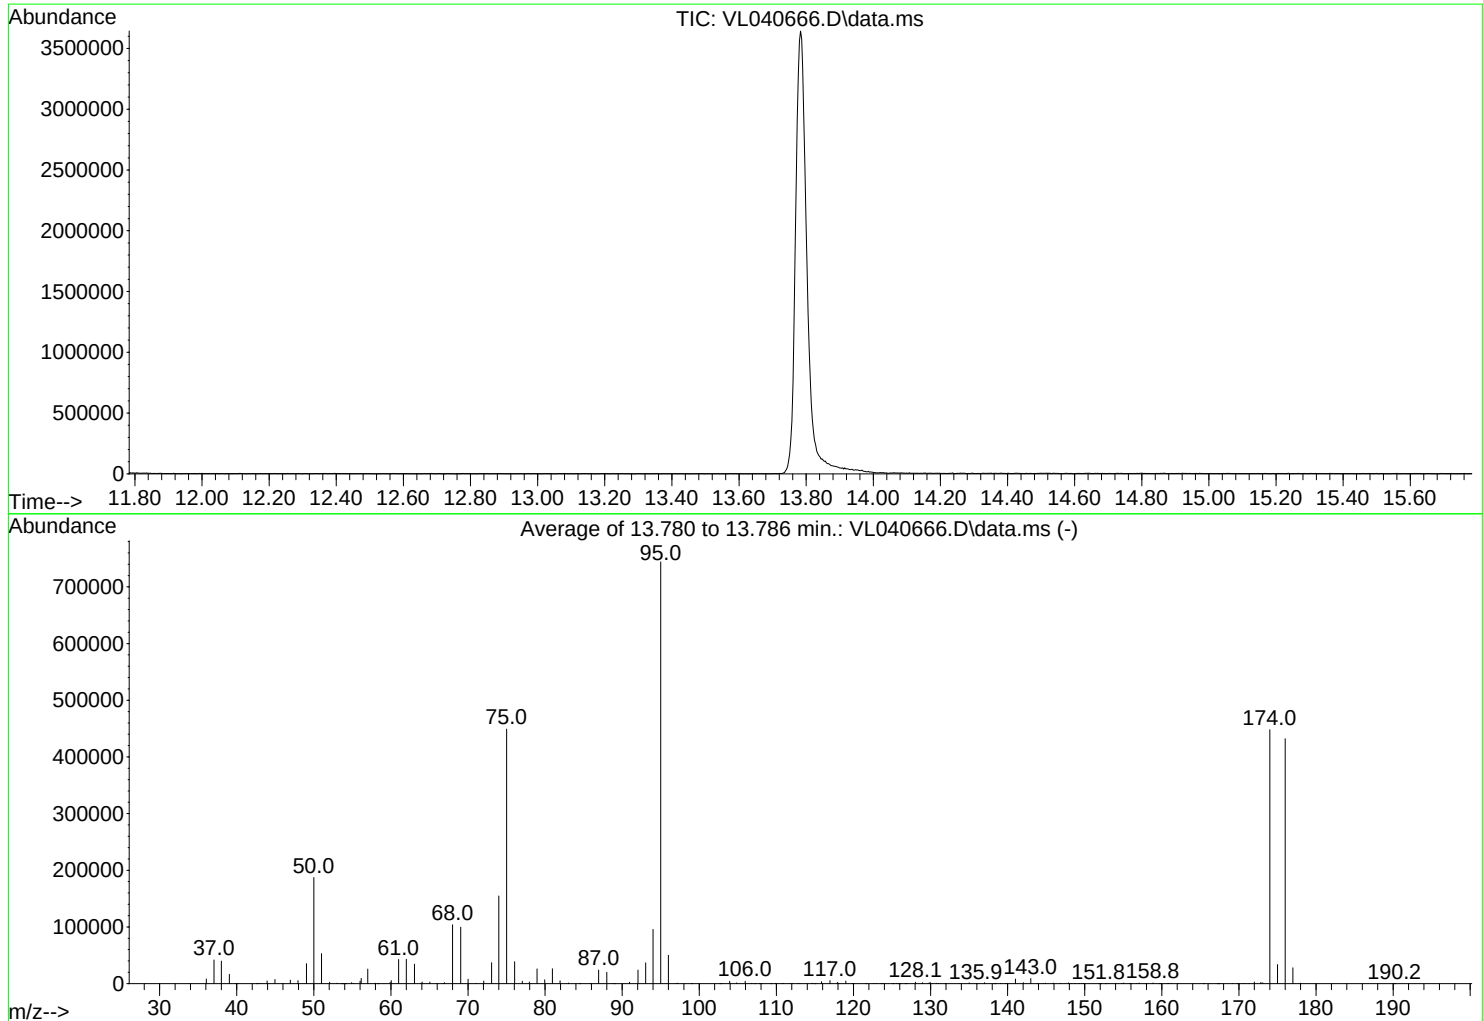

AutoFind: Scans 3476, 3477, 3478; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.2	187243	PASS
75	95	30	66	60.4	449301	PASS
95	95	100	100	100.0	744213	PASS
96	95	5	9	6.7	49918	PASS
173	174	0.00	2	0.5	2202	PASS
174	95	50	120	60.2	447915	PASS
175	174	4	9	7.5	33557	PASS
176	174	93	101	96.5	432341	PASS
177	176	5	9	6.5	27909	PASS

Average of 13.780 to 13.786 min.: VL040666.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8258	45.95	538	54.90	1705	63.05	3451
37.05	41717	46.95	6190	55.10	470	63.90	78
38.00	39883	47.95	5511	56.00	4643	64.05	293
39.05	16364	49.05	35443	56.15	9408	65.05	281
39.85	281	50.00	187243	57.00	25845	66.00	201
40.20	249	51.00	53104	57.95	947	66.80	588
42.60	89	52.05	2588	58.30	125	66.95	1755
42.90	172	53.00	805	59.90	2468	68.00	103837
43.15	338	53.60	156	60.05	5266	69.05	99645
43.95	4831	53.80	132	61.00	42707	70.00	7984
44.95	7372	54.10	149	62.00	42949	71.05	522

Average of 13.780 to 13.786 min.: VL040666.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
72.05	4484	83.05	1213	95.00	744213	107.20	156
73.05	37000	84.50	66	96.00	49918	107.80	119
74.00	154709	85.90	500	97.00	258	108.15	246
75.00	449301	86.95	24120	97.20	810	109.30	99
76.05	38845	88.00	20045	99.00	57	109.85	495
77.05	4326	88.70	248	102.70	101	110.70	333
77.95	2805	89.00	127	103.05	262	110.90	523
78.95	25907	90.95	2570	103.95	4202	111.75	599
79.95	6824	92.05	23939	104.85	1426	112.05	685
80.95	26389	93.05	36765	105.95	4361	112.80	471
81.95	5167	94.00	95728	106.80	710	113.05	408

Average of 13.780 to 13.786 min.: VL040666.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
114.65	745	123.60	134	129.95	2406	139.70	197
115.00	103	123.95	426	130.75	684	139.90	244
115.85	3326	125.10	82	131.00	362	141.00	8338
116.95	5374	125.60	176	131.90	67	142.05	1649
117.90	2276	125.80	110	133.80	162	143.00	8944
118.10	832	126.00	58	135.00	1366	143.90	440
119.00	4616	126.70	121	135.90	84	144.60	339
119.85	143	126.95	273	137.00	1824	144.90	888
121.60	56	128.05	2609	138.30	107	145.90	1048
122.60	234	128.95	1725	138.50	204	146.85	469
123.00	332	129.80	1066	139.10	472	147.90	1450

Average of 13.780 to 13.786 min.: VL040666.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.20	422	155.05	1152	162.15	258	172.85	2202
148.70	288	155.80	99	165.40	52	173.10	1516
149.30	251	156.05	323	167.20	92	174.00	447915
149.60	248	156.70	272	167.40	90	175.00	33557
149.85	733	157.05	1112	169.20	299	176.00	432341
151.80	75	157.90	79	169.80	135	177.00	27909
152.10	149	158.85	1169	170.00	345	178.00	842
152.70	123	159.70	74	170.50	179	190.20	51
153.10	375	160.70	310	170.80	403		
154.00	526	160.90	510	171.30	307		
154.80	422	161.20	495	172.00	2754		