

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL090820\
 Data File : VL035556.D
 Acq On : 8 Sep 2020 14:36
 Operator : SY/AP
 Sample : QC090220 CAN 10401
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC090220 CAN 10401

Manual Integrations
 APPROVED

MMDadoda
 9/10/2020 10:45:18 AM

Quant Time: Sep 09 02:51:02 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL082720AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Aug 27 06:46:28 2020
 QLast Update : Thu Aug 27 06:46:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.66	49	1129902	10.00	ppbv	-0.02
33) 1,4-Difluorobenzene	7.17	114	4747219	10.00	ppbv	-0.03
55) Chlorobenzene-d5	12.09	117	4766267	10.00	ppbv	-0.03

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.42	95	3473807	10.26	ppbv	-0.03
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.60%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
20) Methylene Chloride	4.34	84	11288m	0.122	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL090820\
Data File : VL035556.D
Acq On : 8 Sep 2020 14:36
Operator : SY/AP
Sample : OC090220 CAN 10401
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
QC090220 CAN 10401

Manual Integrations
APPROVED

MMDadoda
9/10/2020 10:45:18 AM

Quant Time: Sep 09 02:51:02 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL082720AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Aug
QLast Update : Thu Aug 27 06:46:28 2020
Response via : Initial Calibration

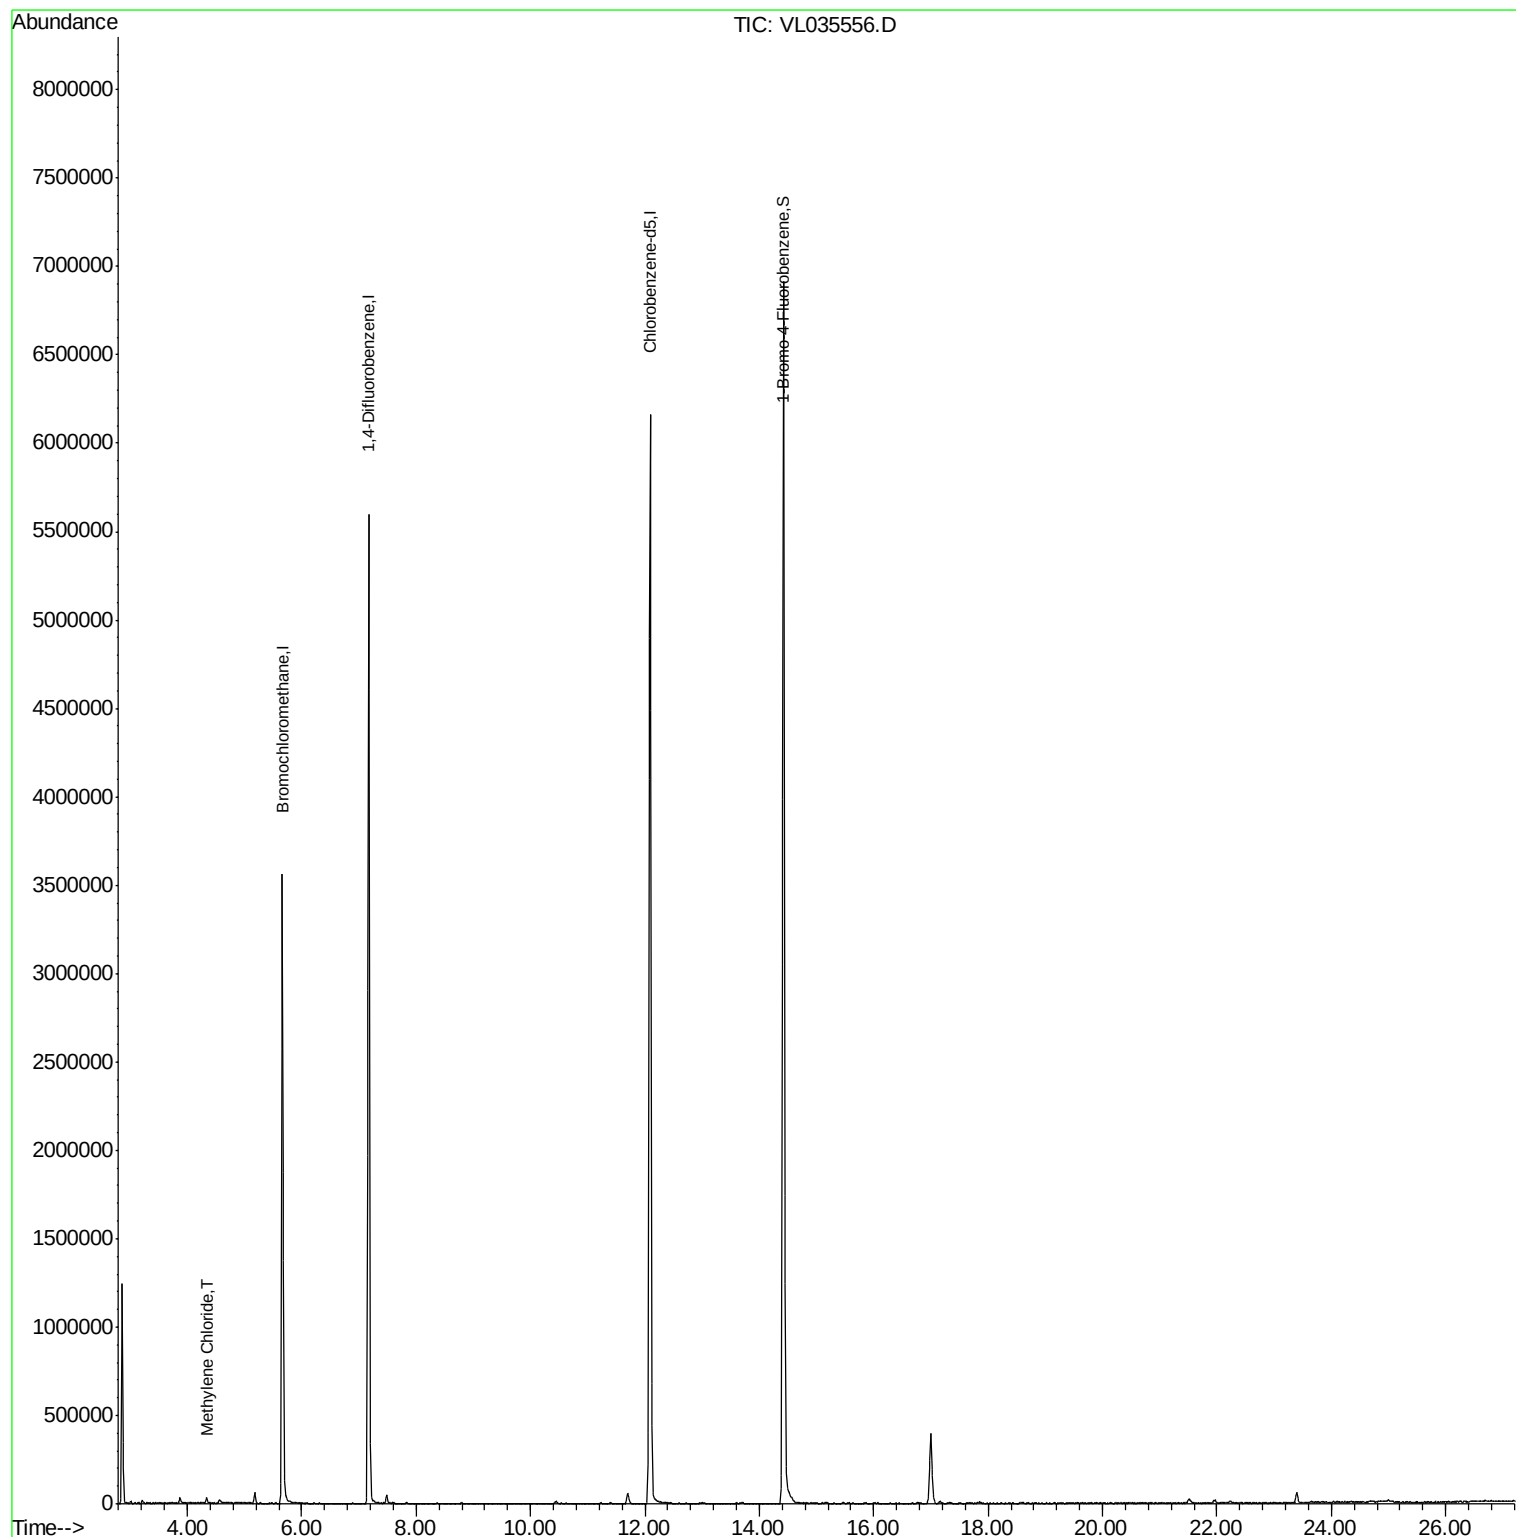

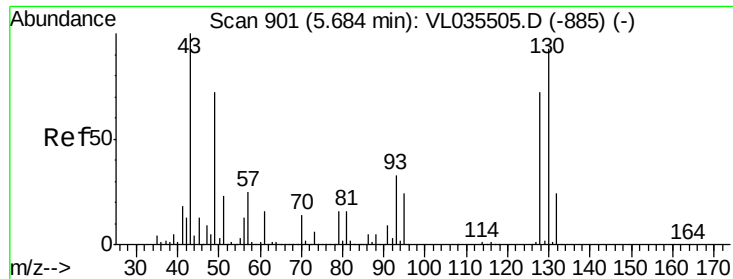

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.66 min Scan# 894

Delta R.T. -0.02 min

Lab File: VL035556.D

Acq: 8 Sep 2020 14:36

Instrument :

MSVOA_L

ClientSampleId :

QC090220 CAN 10401

Tot Ion: 49 Resp: 1129902

Ion Ratio Lower Upper

49 100





128 97.8 50.0 150.1

130 124.8 64.4 193.2

Manual Integrations
APPROVED

MMDadoda

9/10/2020 10:45:18 AM

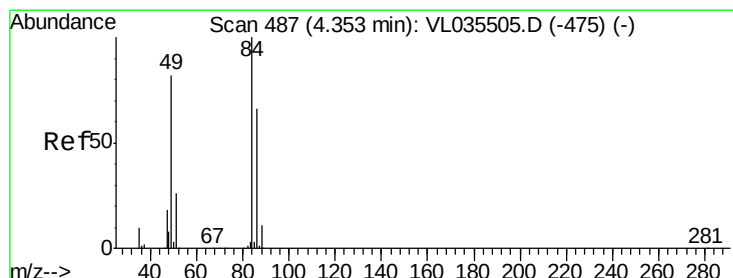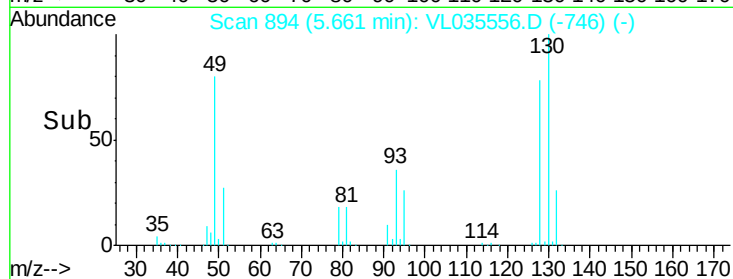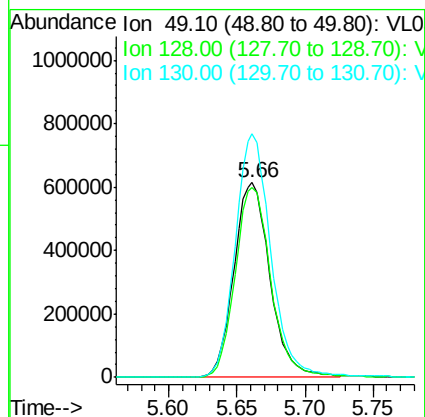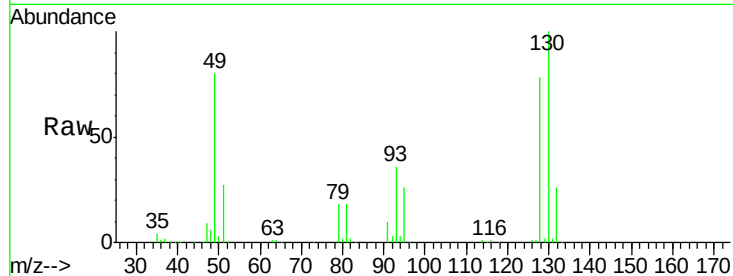

#20

Methylene Chloride

Concen: 0.122 ppbv m

RT: 4.34 min Scan# 483

Delta R.T. -0.01 min

Lab File: VL035556.D

Acq: 8 Sep 2020 14:36

Tgt Ion: 84 Resp: 11288




Ion Ratio Lower Upper


84 100

49 72.5 65.4 98.0

51 22.1 21.5 32.3

86 63.3 52.9 79.3

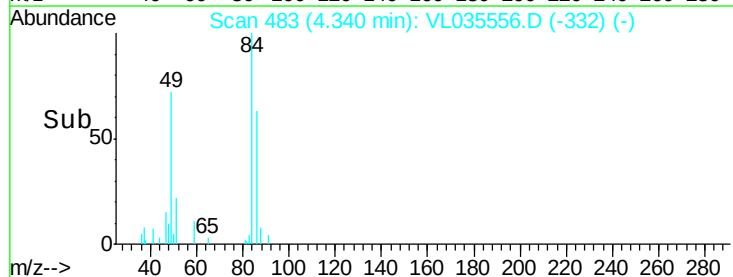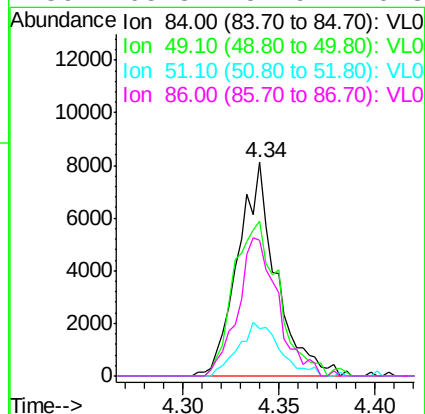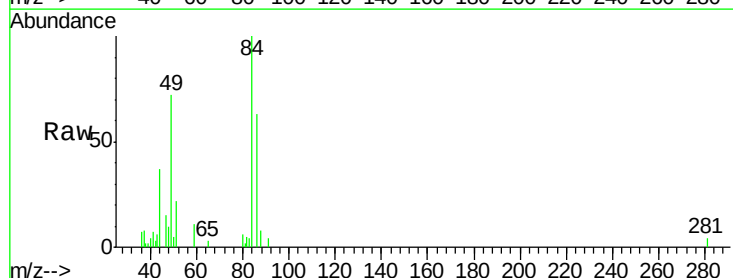

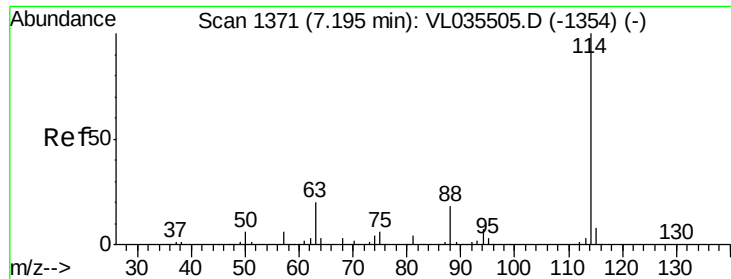





#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.17 min Scan# 1363
 Delta R.T. -0.03 min
 Lab File: VL035556.D
 Acq: 8 Sep 2020 14:36

Instrument :
 MSVOA_L
 ClientSampleId :
 QC090220 CAN 10401

Tot Ion:114 Resp: 4747219
 Ion Ratio Lower Upper
 114 100
 63 18.7 14.7 22.1
 88 17.0 13.4 20.2




Manual Integrations
 APPROVED


MMDadoda
 9/10/2020 10:45:18 AM

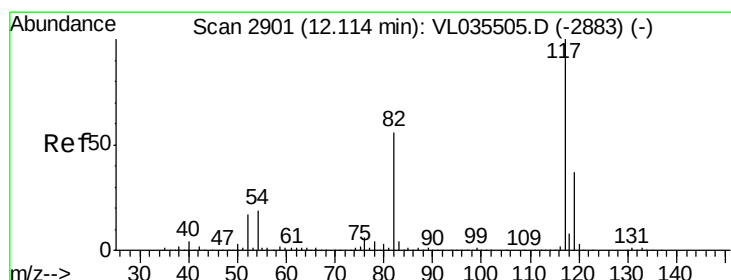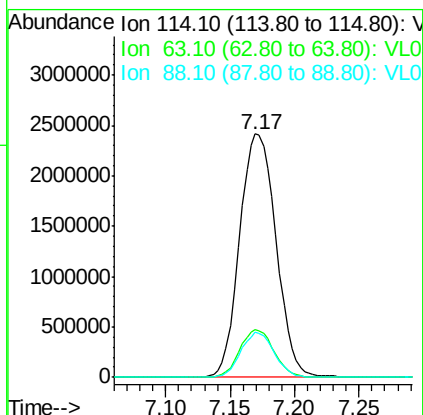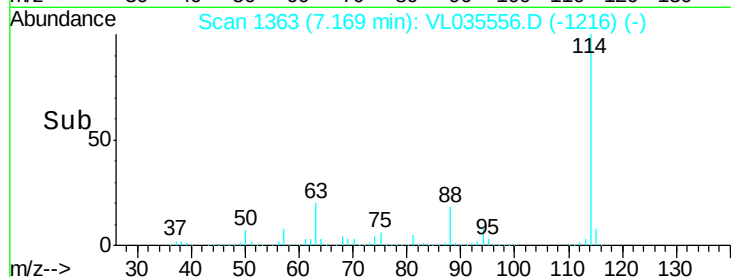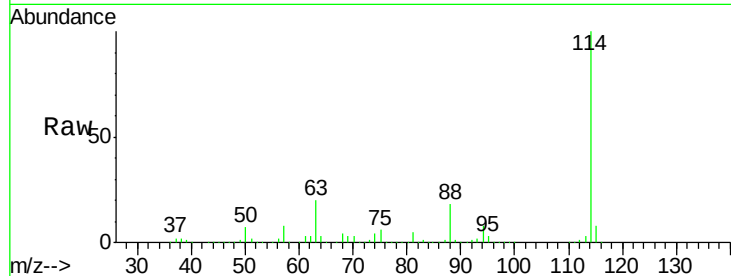

#55
 Chlorobenzene-d5
 Concen: 10.000 ppbv
 RT: 12.09 min Scan# 2893
 Delta R.T. -0.03 min
 Lab File: VL035556.D
 Acq: 8 Sep 2020 14:36

Tgt Ion:117 Resp: 4766267
 Ion Ratio Lower Upper
 117 100
 82 55.0 41.6 62.4
 119 35.0 29.3 43.9

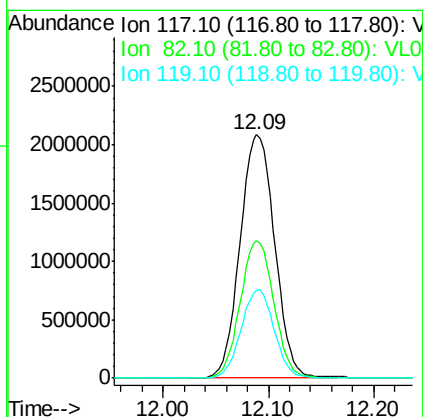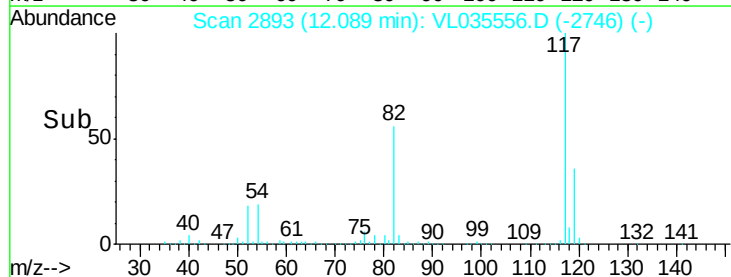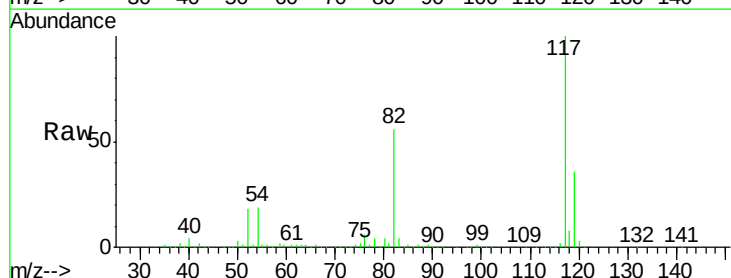

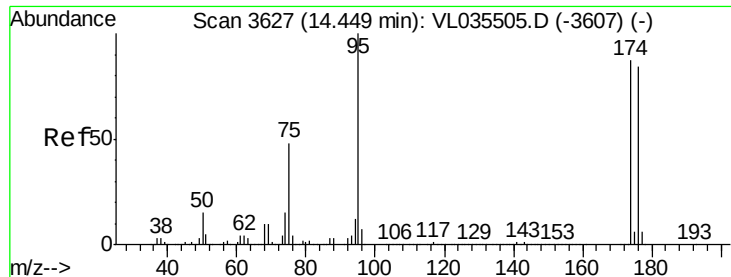

#68
 1-Bromo-4-Fluorobenzene
 Concen: 10.263 ppbv
 RT: 14.42 min Scan# 3619
 Delta R.T. -0.03 min
 Lab File: VL035556.D
 Acq: 8 Sep 2020 14:36

Instrument :
 MSVOA_L
 ClientSampleId :
 QC090220 CAN 10401

Tot Ion: 95 Resp: 3473807
 Ion Ratio Lower Upper
 95 100
 174 87.0 69.6 104.4
 175 6.3 5.1 7.7

Manual Integrations
 APPROVED

MMDadoda
 9/10/2020 10:45:18 AM

