

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL090820\
 Data File : VL035566.D
 Acq On : 8 Sep 2020 21:40
 Operator : SY/AP
 Sample : QC090320 CAN 10439
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC090320 CAN 10439

Quant Time: Sep 09 04:42:30 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL082720AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Aug 27 06:46:28 2020
 QLast Update : Thu Aug 27 06:46:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.66	49	1081622	10.00	ppbv	-0.03
33) 1,4-Difluorobenzene	7.17	114	4407631	10.00	ppbv	-0.03
55) Chlorobenzene-d5	12.09	117	4501048	10.00	ppbv	-0.03

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.42	95	3306516	10.34	ppbv	-0.03
Spiked Amount	10.000	Range	65 - 135	Recovery	=	103.40%


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
20) Methylene Chloride	4.33	84	87405	0.984	ppbv	95
26) Hexane	5.68	57	35281	0.295	ppbv #	47




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL090820\
Data File : VL035566.D
Acq On : 8 Sep 2020 21:40
Operator : SY/AP
Sample : QC090320 CAN 10439
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC090320 CAN 10439

Quant Time: Sep 09 04:42:30 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL082720AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Aug 27 06:46:28 2020
QLast Update : Thu Aug 27 06:46:28 2020
Response via : Initial Calibration

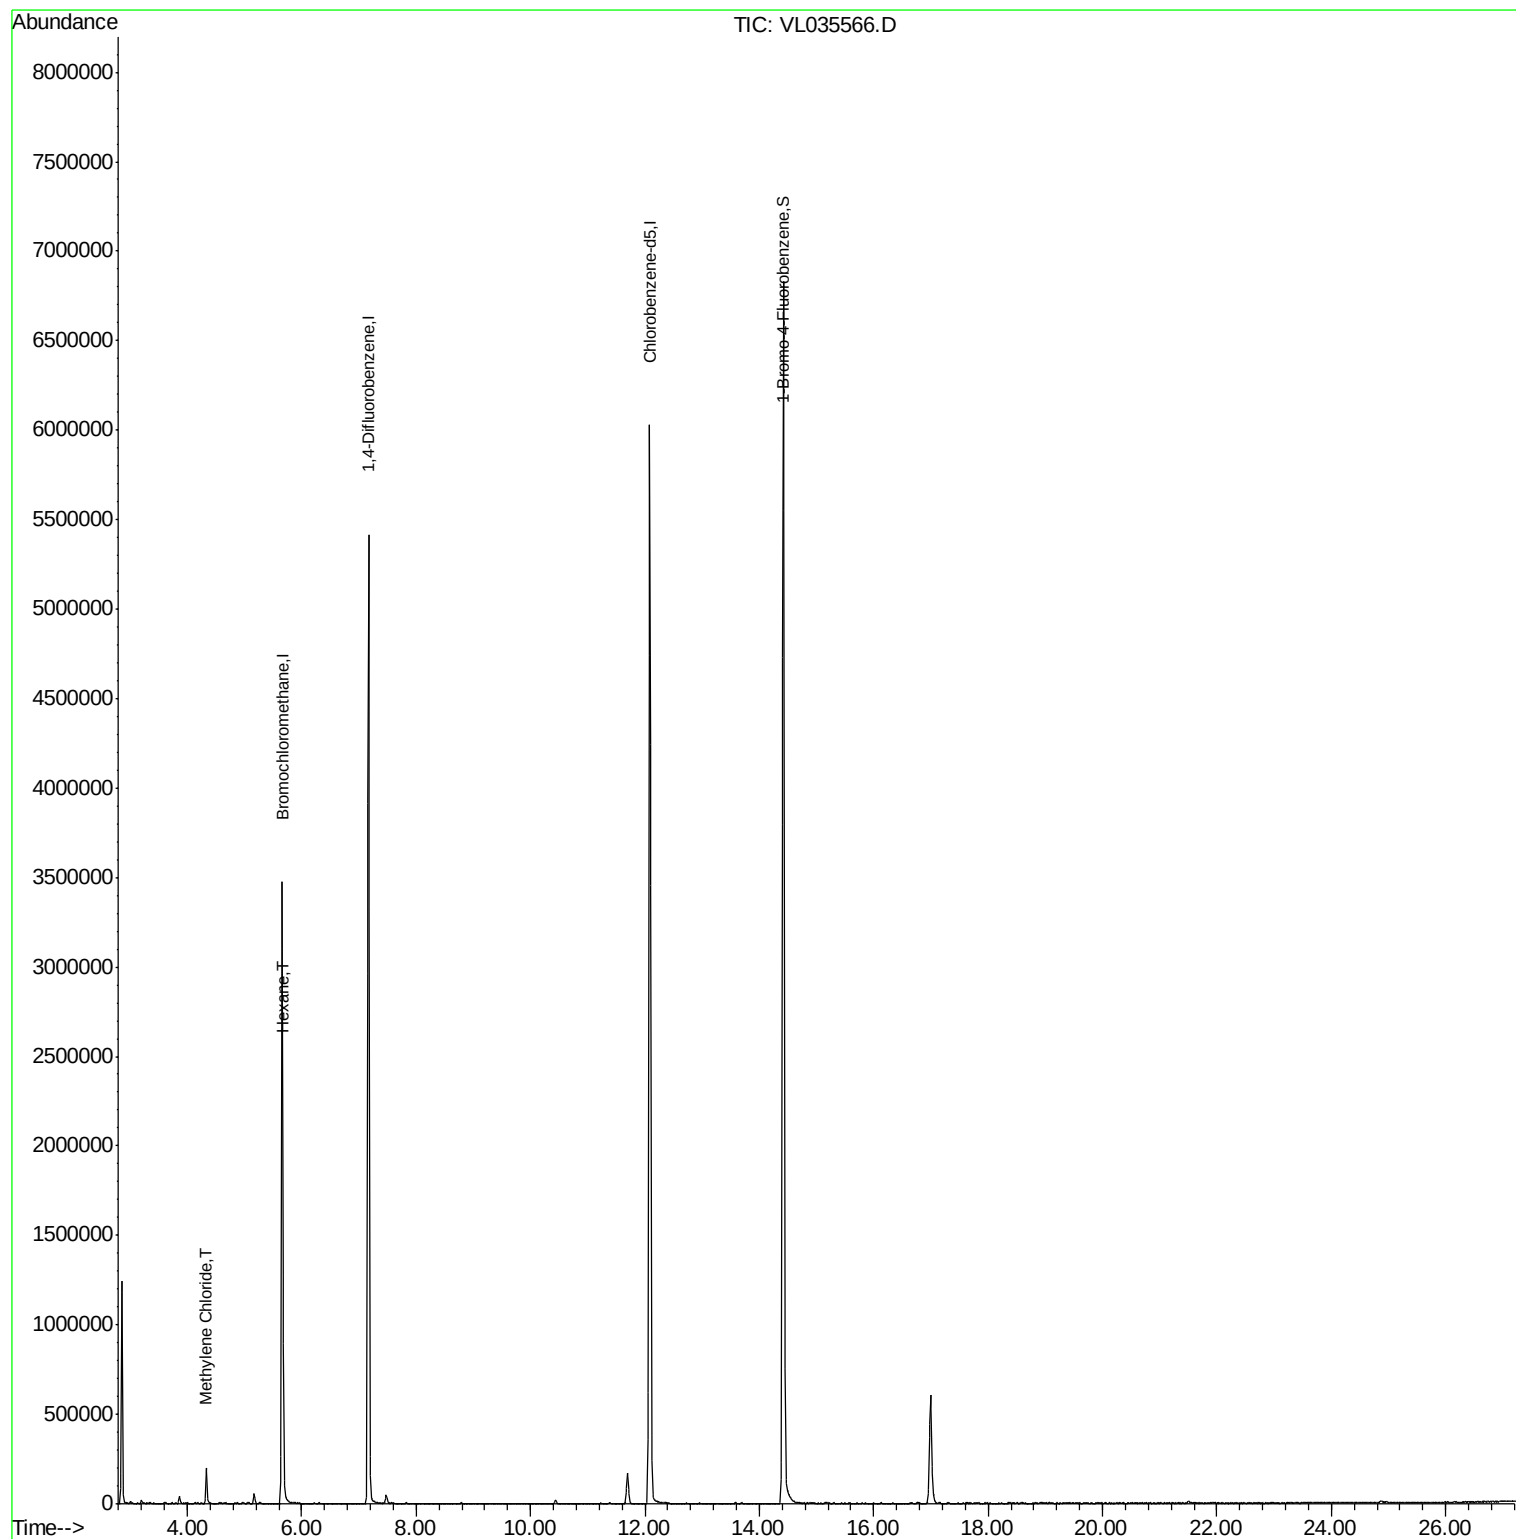

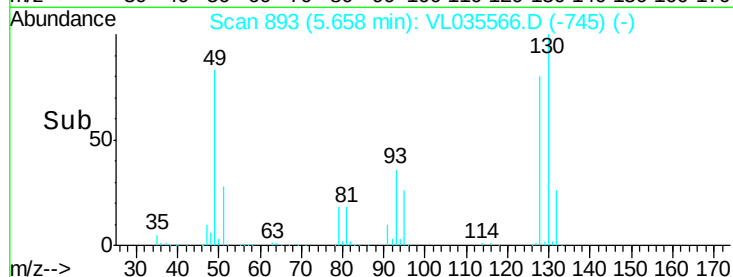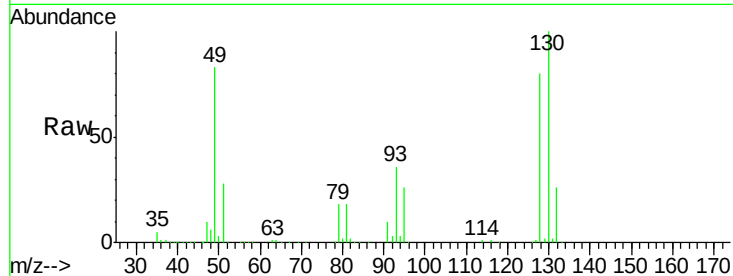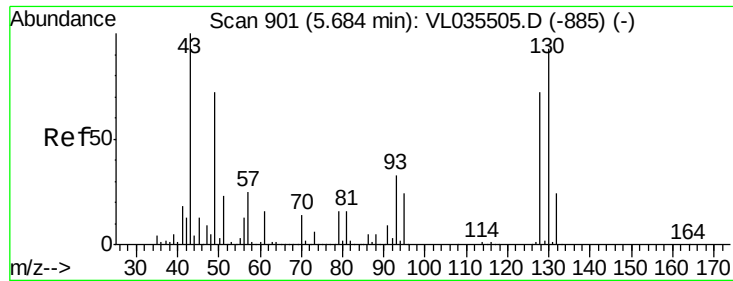

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.66 min Scan# 893

Delta R.T. -0.03 min

Lab File: VL035566.D

Acq: 8 Sep 2020 21:40

Instrument :

MSVOA_L

ClientSampleId :

QC090320 CAN 10439





Tot Ion: 49 Resp: 1081622

Ion Ratio Lower Upper

49 100

128 95.9 50.0 150.1

130 122.3 64.4 193.2

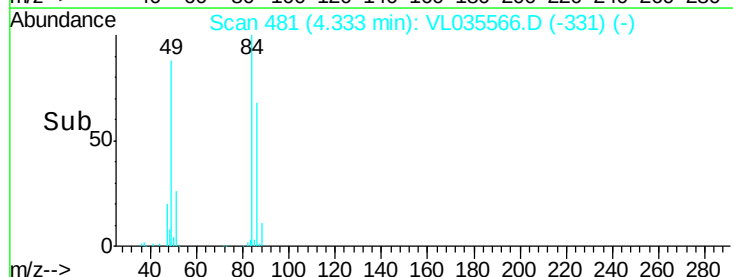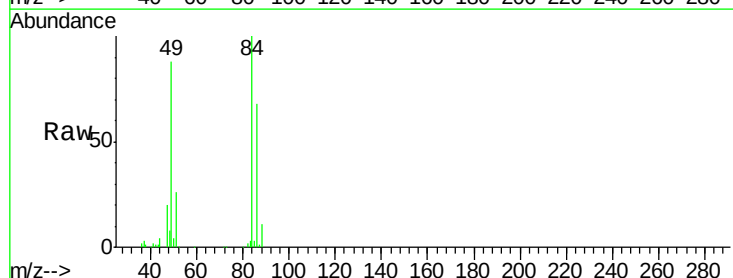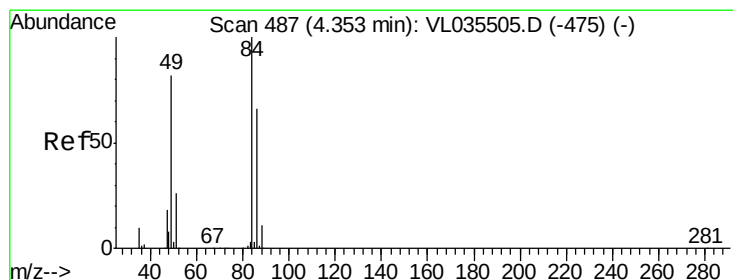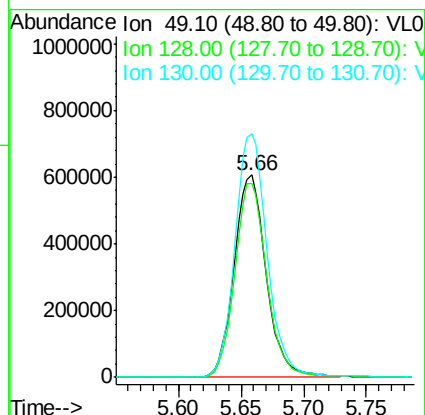

#20

Methylene Chloride

Concen: 0.984 ppbv

RT: 4.33 min Scan# 481

Delta R.T. -0.02 min

Lab File: VL035566.D

Acq: 8 Sep 2020 21:40

Tgt Ion: 84 Resp: 87405


Ion Ratio Lower Upper


84 100

49 88.0 65.4 98.0

51 25.6 21.5 32.3

86 68.1 52.9 79.3




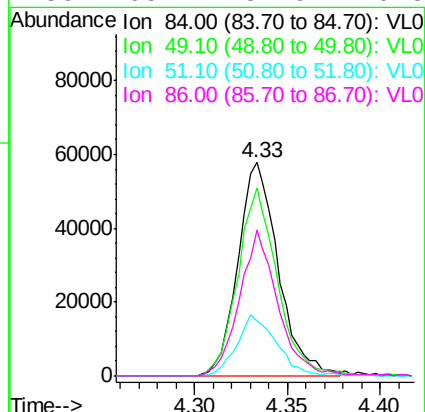


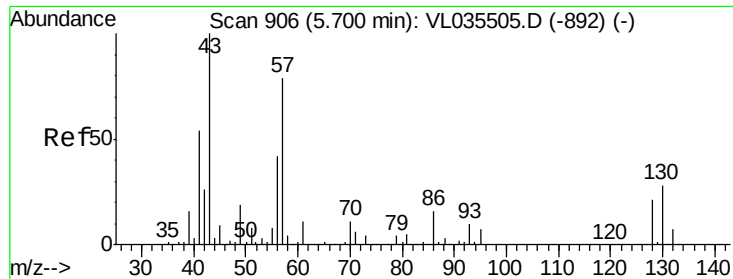

#26
Hexane
Concen: 0.295 ppbv
RT: 5.68 min Scan# 899
Delta R.T. -0.02 min
Lab File: VL035566.D
Acq: 8 Sep 2020 21:40




Instrument :
MSVOA_L
ClientSampleId :
QC090320 CAN 10439


Tot Ion: 57 Resp: 35281
Ion Ratio Lower Upper
57 100
41 78.4 55.9 83.9
43 61.0 141.8 212.8#
56 57.3 41.8 62.8

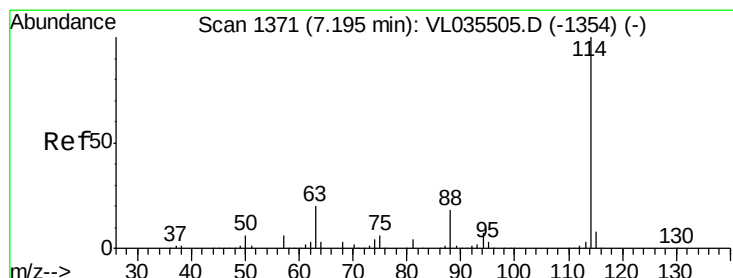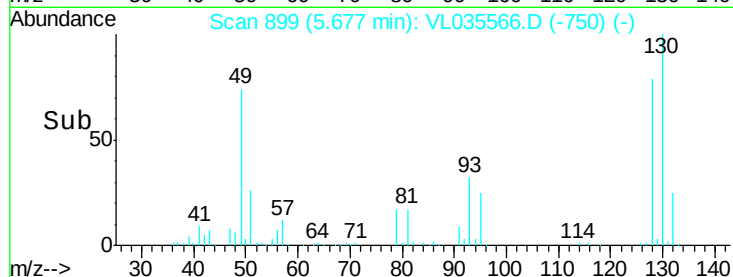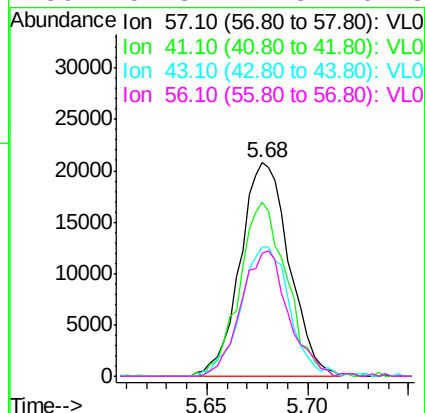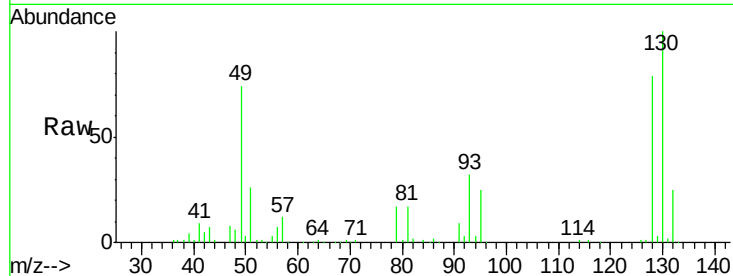

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.17 min Scan# 1362
Delta R.T. -0.03 min
Lab File: VL035566.D
Acq: 8 Sep 2020 21:40

Tgt Ion: 114 Resp: 4407631
Ion Ratio Lower Upper
114 100
63 18.7 14.7 22.1
88 17.0 13.4 20.2


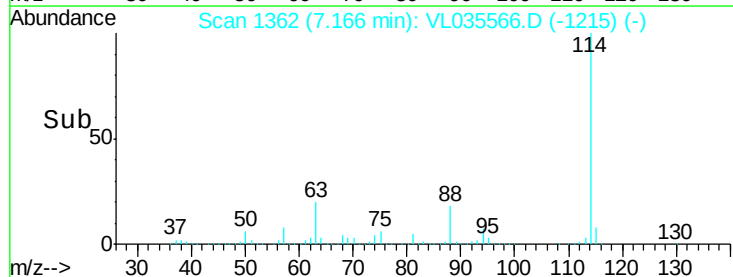
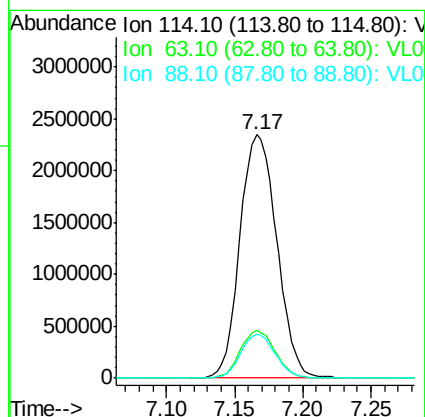
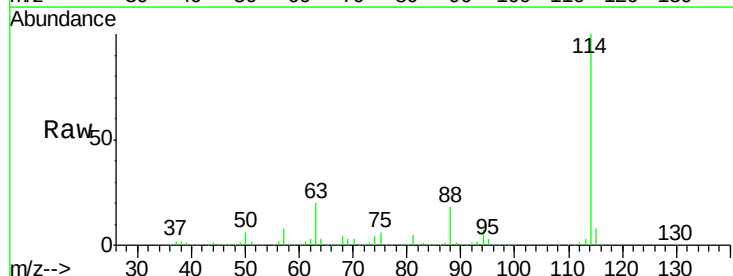


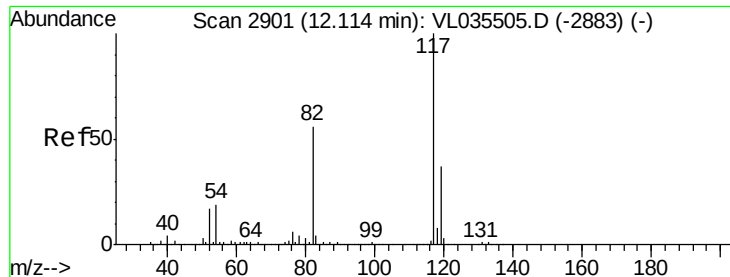

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.09 min Scan# 2892
Delta R.T. -0.03 min
Lab File: VL035566.D
Acq: 8 Sep 2020 21:40

Instrument :
MSVOA_L
ClientSampleId :
QC090320 CAN 10439

Tot Ion:117 Resp: 4501048
Ion Ratio Lower Upper
117 100
82 55.9 41.6 62.4
119 34.8 29.3 43.9

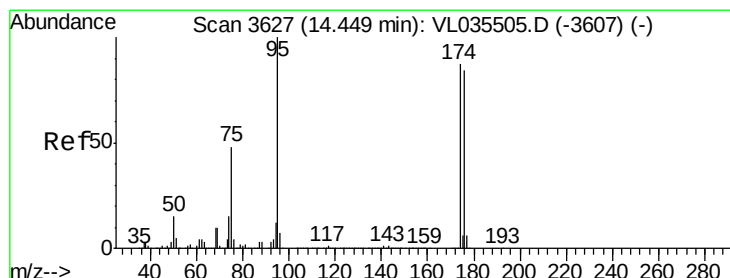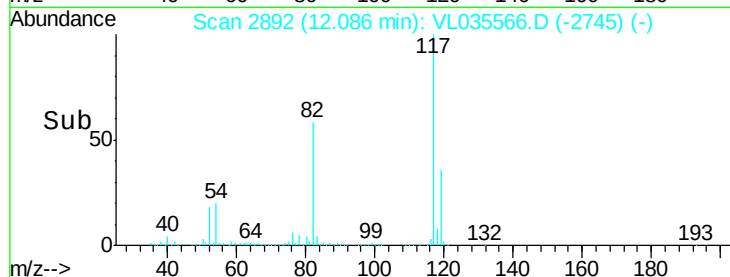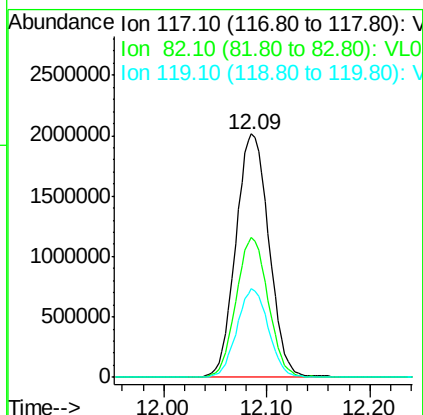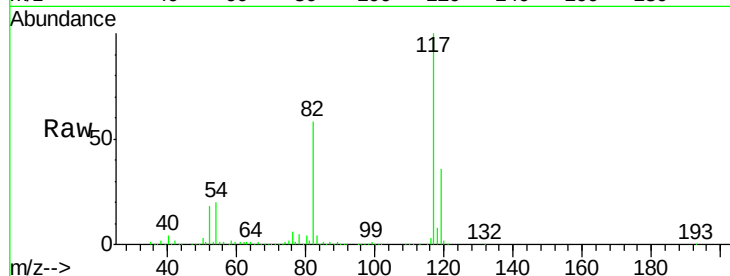

#68
1-Bromo-4-Fluorobenzene
Concen: 10.344 ppbv
RT: 14.42 min Scan# 3618
Delta R.T. -0.03 min
Lab File: VL035566.D
Acq: 8 Sep 2020 21:40

Tgt Ion: 95 Resp: 3306516
Ion Ratio Lower Upper
95 100
174 85.1 69.6 104.4
175 6.2 5.1 7.7

