


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL091019\  
Data File : VL034137.D  
Acq On : 10 Sep 2019 9:19  
Operator : SY/AP  
Sample : BFB  
Misc : 400ml/MSVOA L  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_L  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL090519AIR.M  
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Thu Sep 05 10:21:45 2019  
Last Update : Thu Sep 05 10:21:45 2019

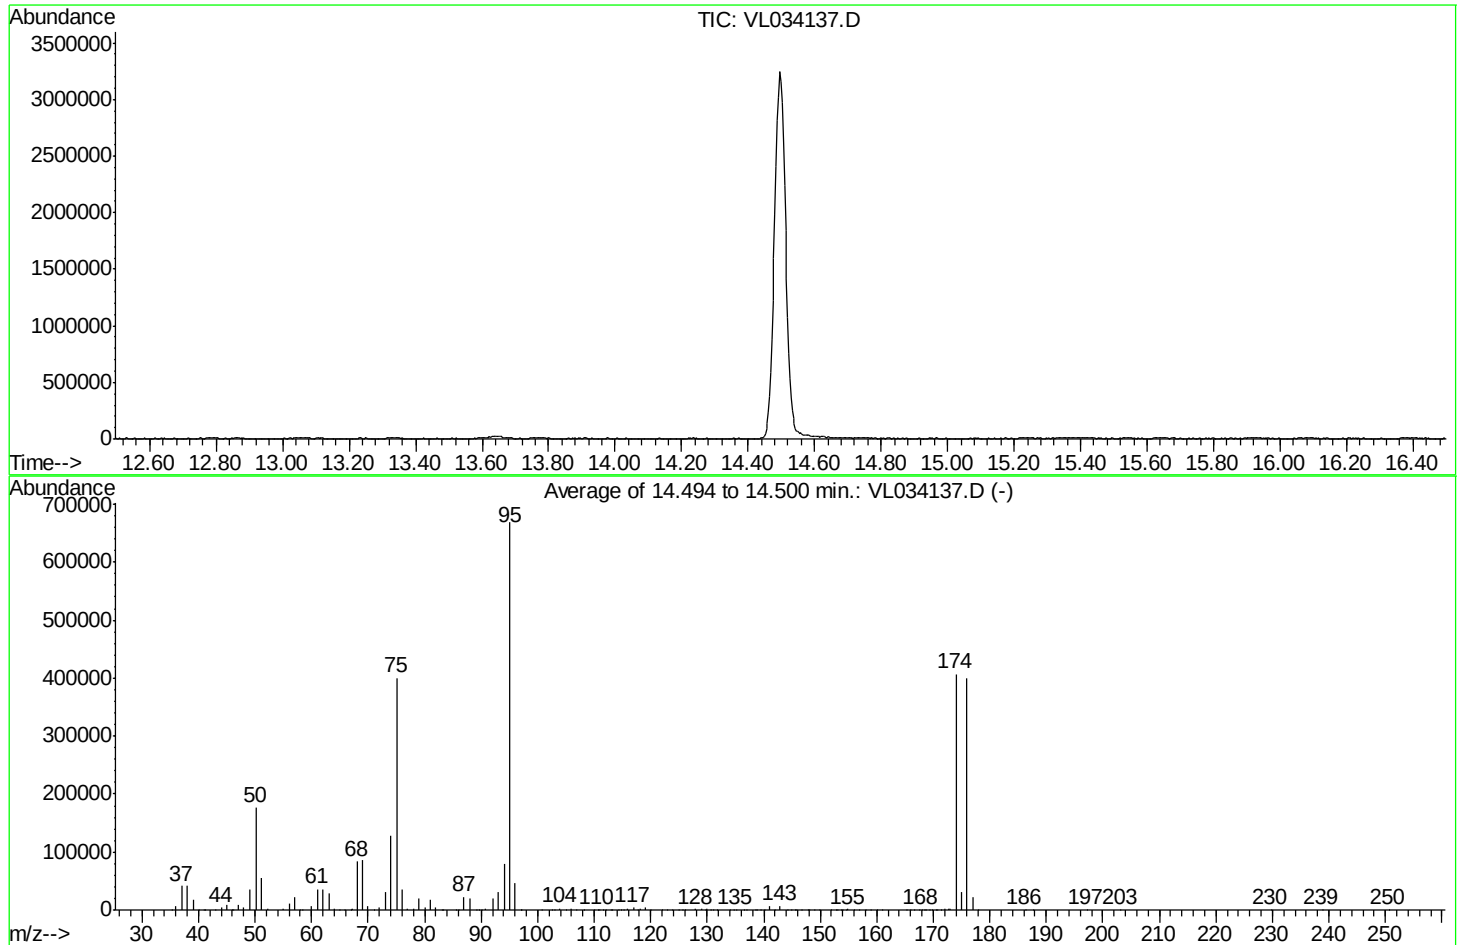

AutoFind: Scans 3641, 3642, 3643; Background Corrected with Scan 3615

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 8            | 40           | 26.4      | 176490  | PASS             |
| 75          | 95           | 30           | 66           | 59.9      | 400554  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 668693  | PASS             |
| 96          | 95           | 5            | 9            | 6.9       | 46264   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.6       | 2445    | PASS             |
| 174         | 95           | 50           | 120          | 60.9      | 407338  | PASS             |
| 175         | 174          | 4            | 9            | 7.6       | 31117   | PASS             |
| 176         | 174          | 93           | 101          | 98.3      | 400533  | PASS             |
| 177         | 176          | 5            | 9            | 5.6       | 22378   | PASS             |