

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL091020\
Data File : VL035589.D
Acq On : 10 Sep 2020 18:38
Operator : SY/AP
Sample : CAN 10295
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10295

Quant Time: Sep 11 09:41:53 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL082720AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Aug 27 06:46:28 2020
QLast Update : Thu Aug 27 06:46:28 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.66	49	1032474	10.00	ppbv	-0.02
33) 1,4-Difluorobenzene	7.17	114	4129767	10.00	ppbv	-0.03
55) Chlorobenzene-d5	12.09	117	4144499	10.00	ppbv	-0.03

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.42	95	3131995	10.64	ppbv	-0.03
Spiked Amount	10.000	Range	65 - 135	Recovery	=	106.40%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL091020\
Data File : VL035589.D
Acq On : 10 Sep 2020 18:38
Operator : SY/AP
Sample : CAN 10295
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10295

Quant Time: Sep 11 09:41:53 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL082720AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Aug 27 06:46:28 2020
QLast Update : Thu Aug 27 06:46:28 2020
Response via : Initial Calibration

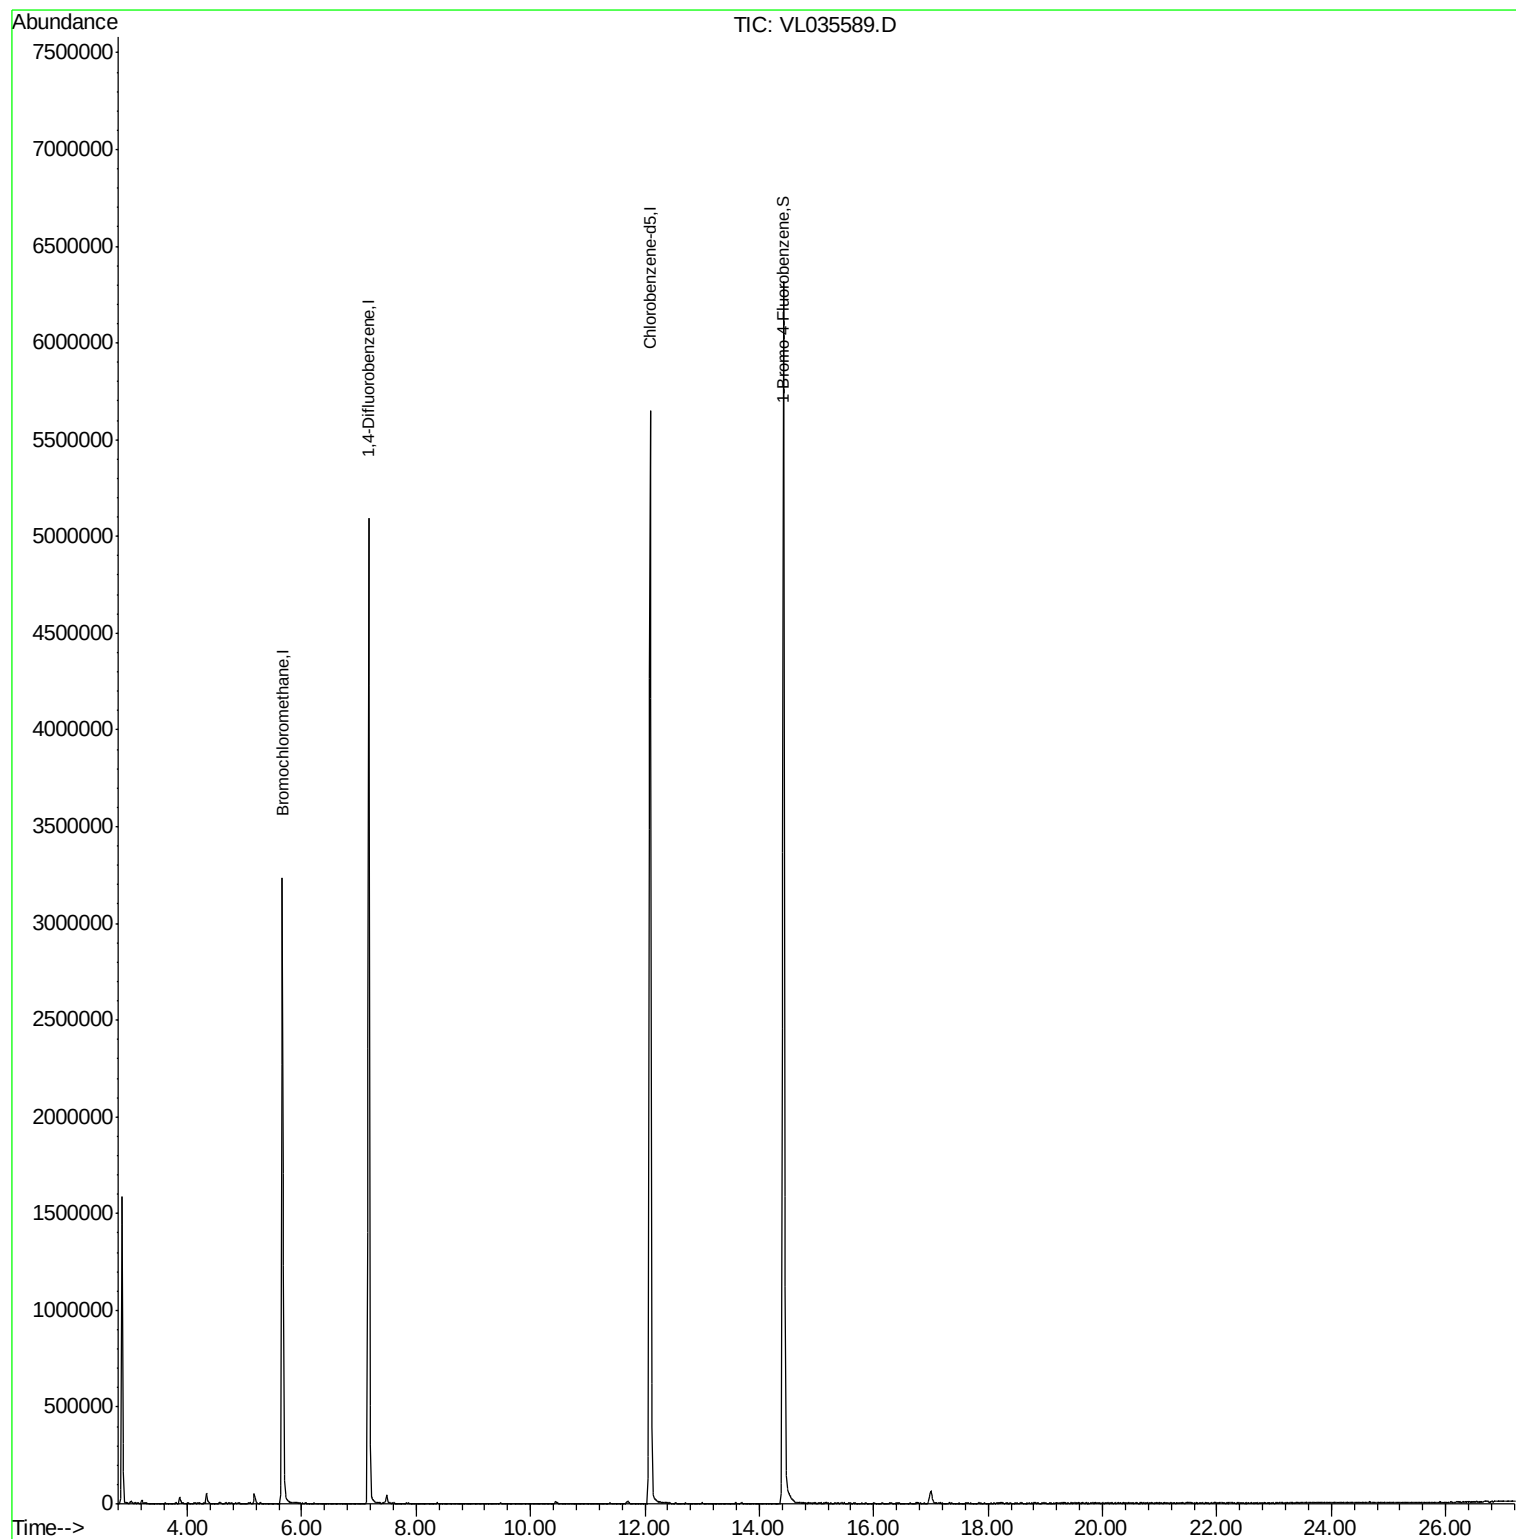

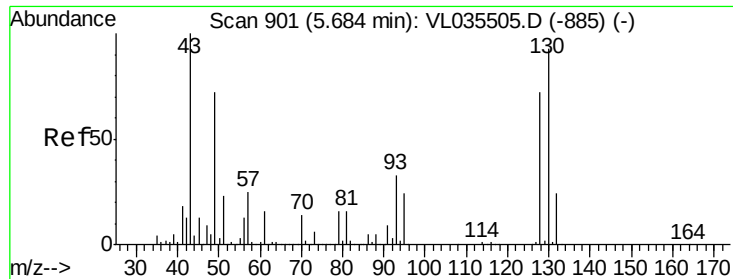

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.66 min Scan# 894

Delta R.T. -0.02 min

Lab File: VL035589.D

Acq: 10 Sep 2020 18:38

Instrument :

MSVOA_L

ClientSampleId :

CAN 10295


Tot Ion: 49 Resp: 1032474

Ion Ratio Lower Upper

49 100

128 92.2 50.0 150.1




130 118.7 64.4 193.2

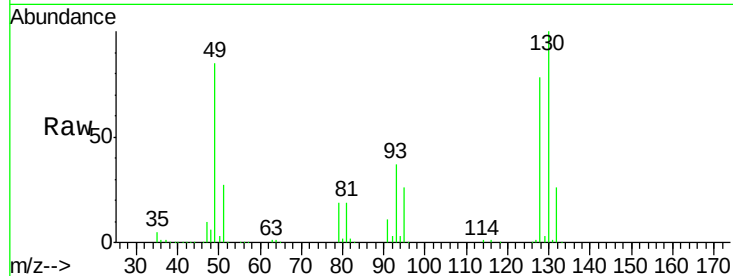

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

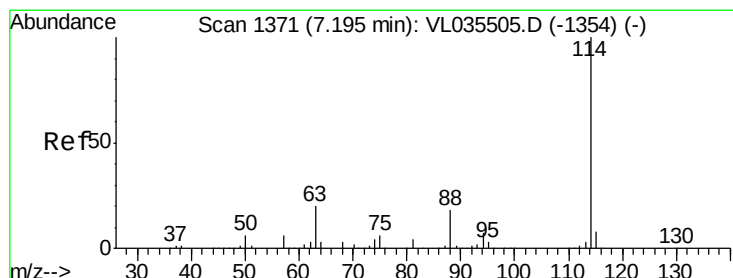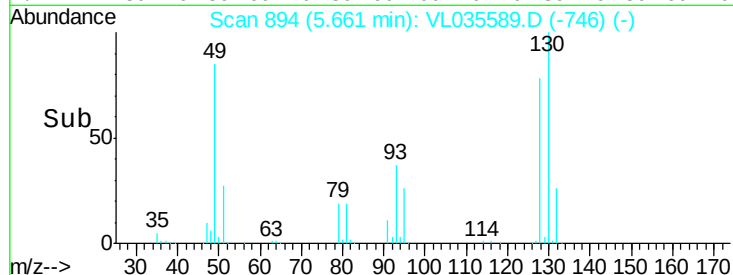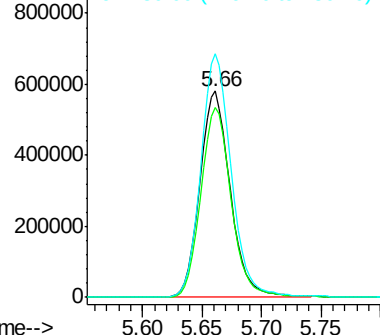

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.17 min Scan# 1363

Delta R.T. -0.03 min

Lab File: VL035589.D

Acq: 10 Sep 2020 18:38


Tgt Ion: 114 Resp: 4129767

Ion Ratio Lower Upper

114 100

63 18.9 14.7 22.1



88 17.0 13.4 20.2

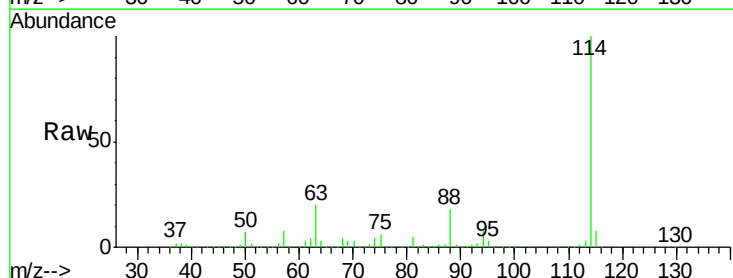


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



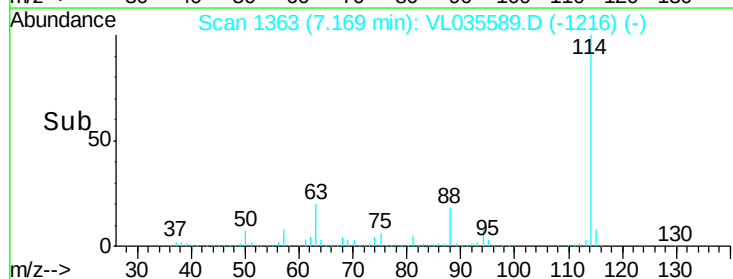
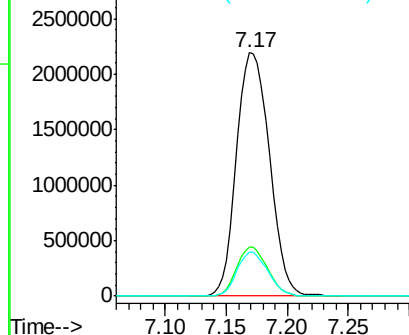


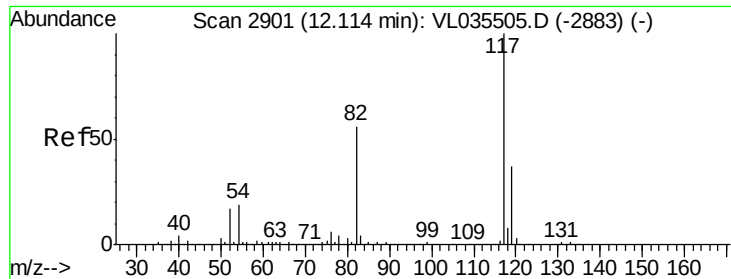

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.09 min Scan# 2893
Delta R.T. -0.03 min
Lab File: VL035589.D
Acq: 10 Sep 2020 18:38

Instrument :
MSVOA_L
ClientSampleId :
CAN 10295

Tot Ion:117 Resp: 4144499
Ion Ratio Lower Upper
117 100
82 56.9 41.6 62.4
119 34.9 29.3 43.9

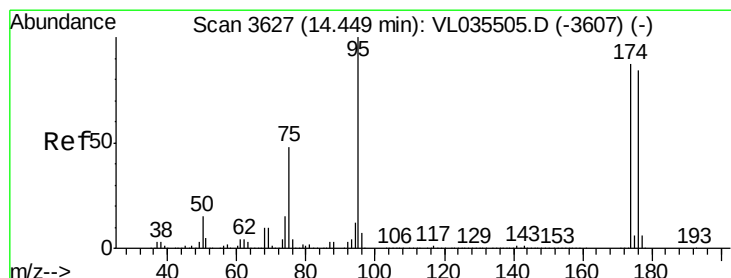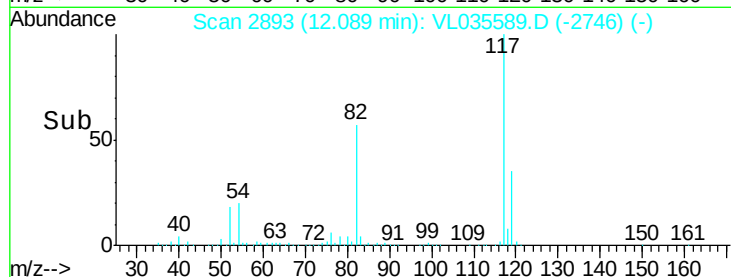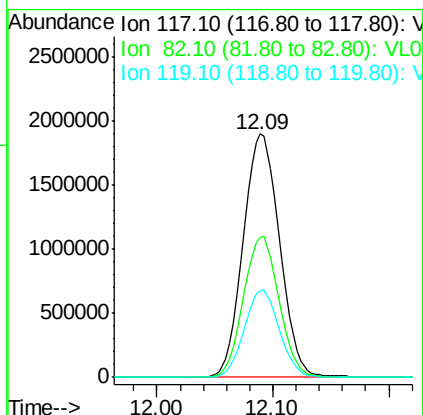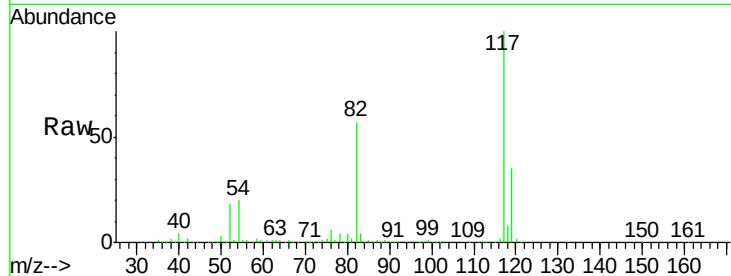

#68
1-Bromo-4-Fluorobenzene
Concen: 10.641 ppbv
RT: 14.42 min Scan# 3619
Delta R.T. -0.03 min
Lab File: VL035589.D
Acq: 10 Sep 2020 18:38

Tgt Ion: 95 Resp: 3131995
Ion Ratio Lower Upper
95 100
174 81.8 69.6 104.4
175 5.9 5.1 7.7

