
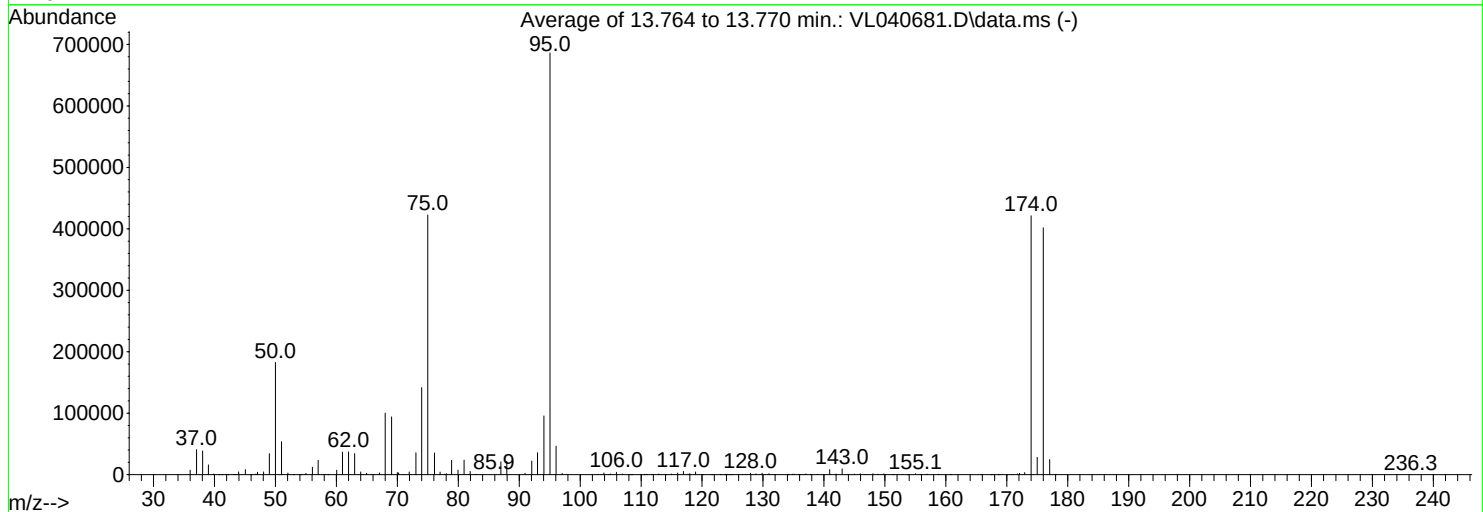


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL091423\
Data File : VL040681.D
Acq On : 14 Sep 2023 12:29
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091423AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Sep 14 19:50:34 2023

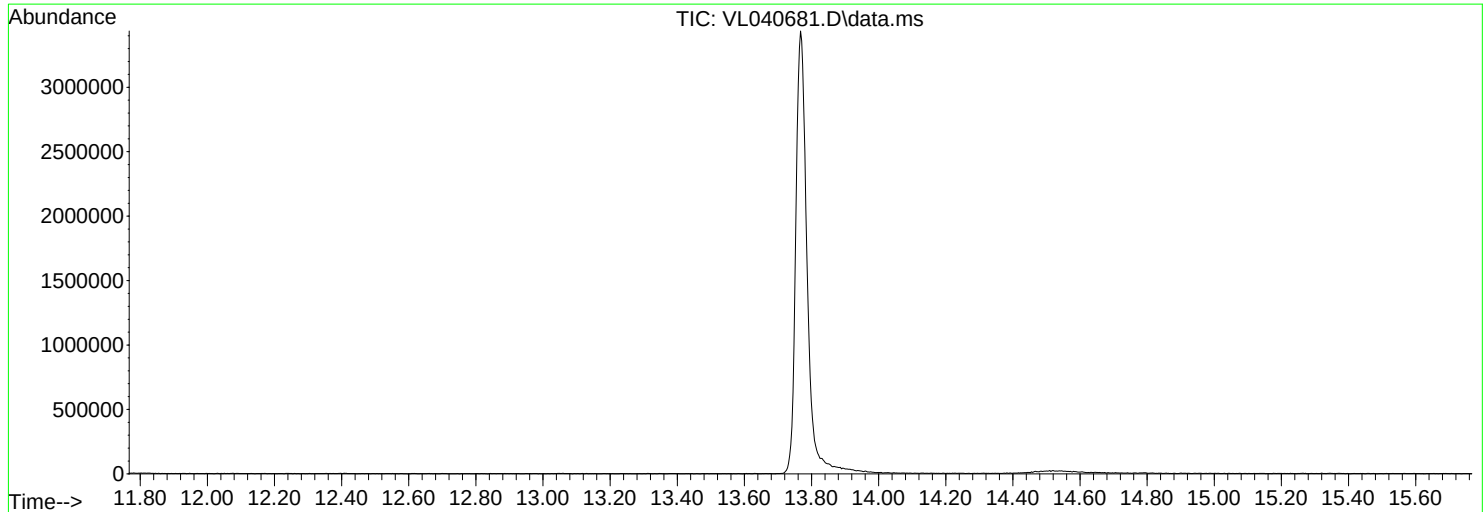

AutoFind: Scans 3471, 3472, 3473; Background Corrected with Scan 3447

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	26.6	182571	PASS
75	95	30	66	61.6	422464	PASS
95	95	100	100	100.0	686357	PASS
96	95	5	9	6.8	46347	PASS
173	174	0.00	2	0.8	3323	PASS
174	95	50	120	61.4	421163	PASS
175	174	4	9	6.7	28117	PASS
176	174	93	101	95.4	401749	PASS
177	176	5	9	6.1	24547	PASS

Average of 13.764 to 13.770 min.: VL040681.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	7249	43.95	4329	52.90	119	61.00	3685
37.05	40632	45.05	8444	53.10	317	62.00	3691
38.05	38600	45.90	131	53.90	265	63.00	3428
39.00	15890	46.15	549	54.20	92	64.00	435
39.85	1009	46.80	1118	55.00	2017	64.95	2407
40.70	56	47.05	3819	56.05	11929	65.75	317
41.20	146	48.05	4436	57.00	23168	66.20	287
41.80	189	49.00	34195	57.85	481	67.05	2827
42.20	66	50.00	182571	58.20	279	68.00	100181
43.10	276	51.00	53752	58.60	93	69.05	93957
43.30	89	52.05	2577	60.05	7186	70.00	3424

Average of 13.764 to 13.770 min.: VL040681.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
70.20	2754	79.95	7386	93.00	35595	105.95	4062
71.00	332	80.95	23712	94.05	95456	106.95	1085
71.95	4343	81.95	5326	95.05	686357	108.00	92
73.05	35619	82.80	293	96.05	46347	108.40	74
74.00	141568	83.05	638	97.05	2145	109.95	333
75.00	422464	83.70	226	102.80	179	110.50	148
76.10	35456	85.90	775	102.95	334	110.90	652
77.00	4191	87.00	20755	103.90	2975	111.10	175
77.80	789	87.95	21744	104.60	280	111.75	615
78.05	1585	90.95	2372	104.90	527	112.10	345
78.90	23352	92.05	22043	105.00	1036	112.90	1080

Average of 13.764 to 13.770 min.: VL040681.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
114.00	51	123.90	164	131.85	133	140.05	366
115.00	953	124.20	72	134.10	54	140.95	8293
116.00	2630	124.70	87	134.85	918	142.00	1109
116.95	5185	125.10	288	135.10	806	143.00	9302
117.70	731	125.85	276	135.80	229	143.80	505
118.00	1601	126.65	261	136.15	232	144.15	500
118.95	4451	127.15	343	136.60	267	144.95	1091
120.05	155	127.95	2402	137.05	1418	145.95	1485
121.60	95	128.85	1419	137.80	72	146.75	384
123.00	140	129.85	2305	138.70	262	147.10	278
123.70	157	131.00	1519	139.00	163	148.05	1505

Average of 13.764 to 13.770 min.: VL040681.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.85	692	157.95	191	171.10	311		
149.85	1384	158.85	861	171.80	1358		
150.10	339	160.70	85	172.10	2034		
151.30	54	160.95	448	172.95	3323		
152.10	269	165.80	61	174.00	421163		
152.95	487	167.45	110	175.00	28117		
153.70	85	167.90	196	176.00	401749		
153.90	224	168.60	87	177.05	24547		
155.05	1568	168.90	275	178.10	651		
155.85	292	170.00	56	236.30	362		
156.90	1097	170.80	319				