

Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL091621\
 Data File : VL037626.D
 Acq On : 16 Sep 2021 22:05
 Operator : SY/AP
 Sample : M3780-03
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 IA1

Manual Integrations
 APPROVED

MMDadoda
 9/20/2021 5:27:24 PM

Quant Time: Sep 17 10:10:24 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL091621AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Sep 16 13:42:46 2021
 QLast Update : Thu Sep 16 13:42:46 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.65	49	1586785	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.16	114	4550471	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.07	117	3900966	10.00	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.39	95	2850785	10.11	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.10%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.04	85	44150	0.154	ppbv	97
3) Chlorodifluoromethane	2.98	51	157610m	0.527	ppbv	
4) Chloromethane	3.13	50	130846	1.183	ppbv	95
9) Propene	3.01	41	1153773	10.928	ppbv #	64
10) Heptane	8.10	43	261027m	1.060	ppbv	
11) Trichlorofluoromethane	3.94	101	50185	0.218	ppbv	94
13) Ethanol	3.66	45	73810876m	7147.433	ppbv	
15) Acetone	3.83	43	11469529	69.569	ppbv	97
19) Isopropyl Alcohol	4.04	45	23401013	260.870	ppbv #	93
20) Methylene Chloride	4.33	84	371700	4.723	ppbv	96
25) Ethyl Acetate	5.65	43	2697080	6.755	ppbv #	91
26) Hexane	5.67	57	553577	2.919	ppbv #	1
29) Chloroform	5.74	83	2168691	7.830	ppbv	98
30) Cyclohexane	7.11	84	79319m	0.489	ppbv	
34) 2-Butanone	5.23	43	832486	4.502	ppbv	99
35) Carbon Tetrachloride	7.00	117	18448m	0.072	ppbv	
36) Benzene	6.87	78	469710	1.238	ppbv #	95
41) Tetrahydrofuran	6.04	42	273542m	3.147	ppbv	
44) 2,2,4-Trimethylpentane	7.85	57	556603	0.873	ppbv #	89
52) Tetrachloroethene	11.19	164	16501m	0.113	ppbv	
53) Toluene	9.78	91	2414057	5.724	ppbv	99
58) Ethyl Benzene	12.69	91	628524	1.214	ppbv	98
59) m/p-Xylene	12.94	91	2217851	4.915	ppbv	98
60) o-Xylene	13.67	91	751916	1.751	ppbv	95
61) Styrene	13.51	104	350272	1.654	ppbv	94
64) n-propylbenzene	15.53	120	24437m	0.158	ppbv	
69) p-Isopropyltoluene	17.63	119	331086	0.552	ppbv #	91
72) 4-Ethyltoluene	15.81	105	149477m	0.303	ppbv	
73) 1,3,5-Trimethylbenzene	15.97	105	130799	0.285	ppbv	86
74) 1,2,4-Trimethylbenzene	16.74	105	497960	1.029	ppbv #	72
76) 1,4-Dichlorobenzene	17.11	146	119233m	0.402	ppbv	
79) Naphthalene	22.17	128	230171m	0.774	ppbv	
80) Naphthalene,2-methyl-	24.95	142	29242m	0.430	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL091621\
Data File : VL037626.D
Acq On : 16 Sep 2021 22:05
Operator : SY/AP
Sample : M3780-03
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
IA1

Manual Integrations
APPROVED

MMDadoda
9/20/2021 5:27:24 PM

Quant Time: Sep 17 10:10:24 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL091621AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Sep
QLast Update : Thu Sep 16 13:42:46 2021
Response via : Initial Calibration

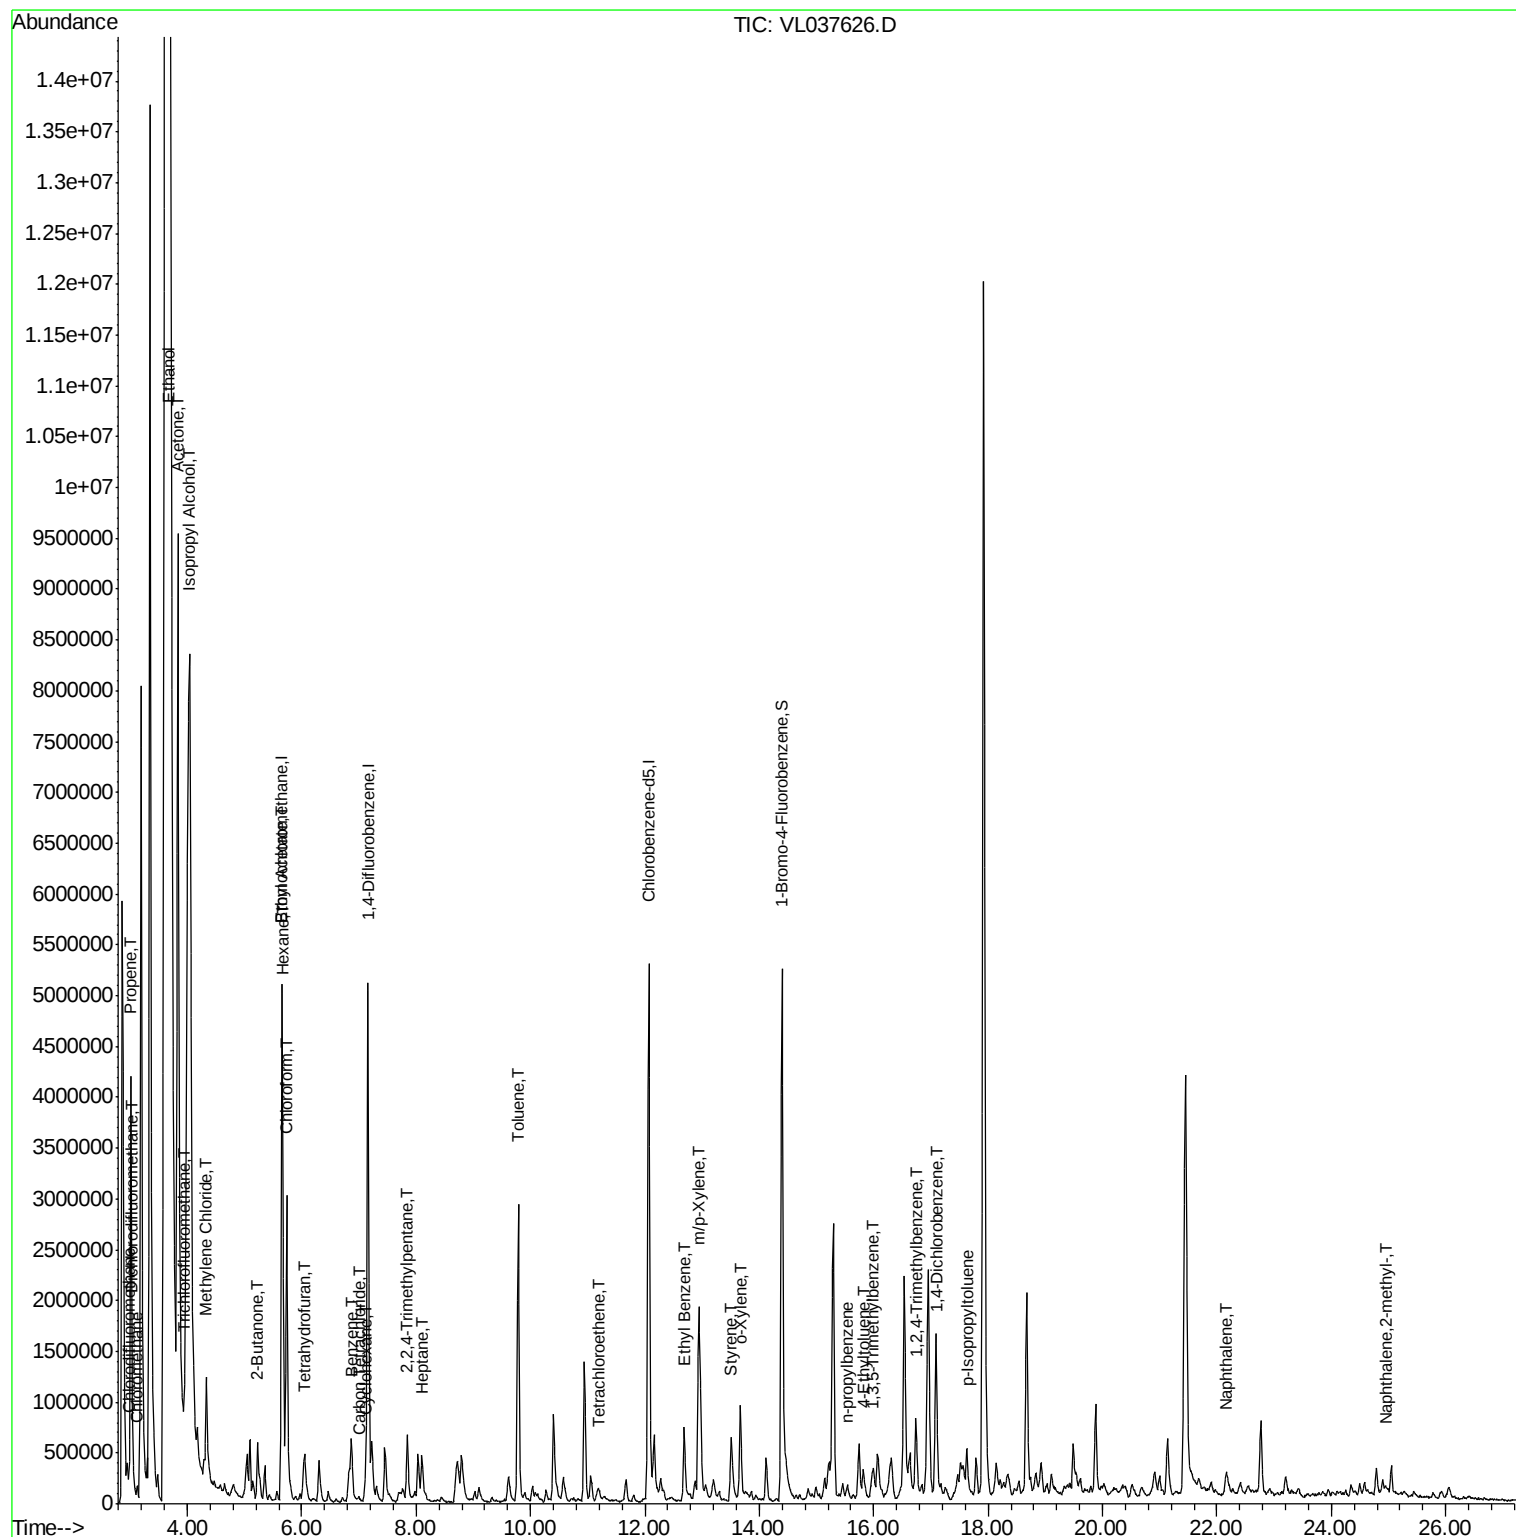

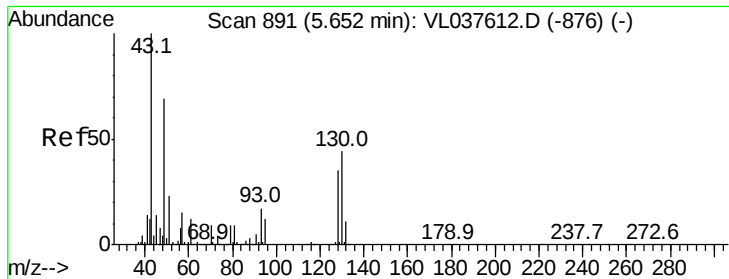

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.65 min Scan# 891

Delta R.T. 0.00 min

Lab File: VL037626.D

Acq: 16 Sep 2021 22:05

Instrument :

MSVOA_L

ClientSampled :

IA1

Tot Ion: 49 Resp: 1586785

Ion Ratio Lower Upper

49 100


128 51.9 27.9 83.6

130 67.7 33.9 101.7

Manual Integrations
APPROVED

MMDadoda

9/20/2021 5:27:24 PM

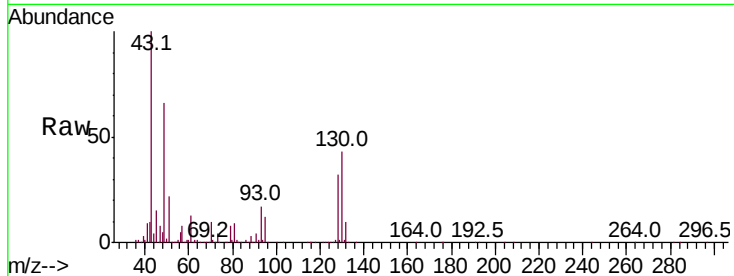

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

5.65

800000



600000

400000

200000

0

Time-->

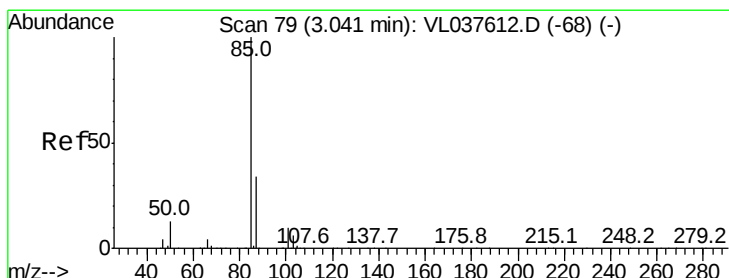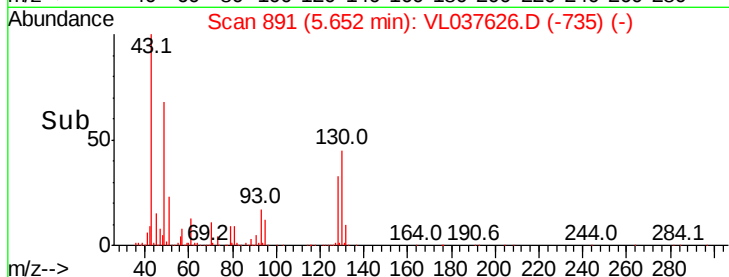

#2

Dichlorodifluoromethane

Concen: 0.154 ppbv

RT: 3.04 min Scan# 79

Delta R.T. 0.00 min

Lab File: VL037626.D


Acq: 16 Sep 2021 22:05

Tgt Ion: 85 Resp: 44150

Ion Ratio Lower Upper

85 100

87 31.8 26.8 40.2

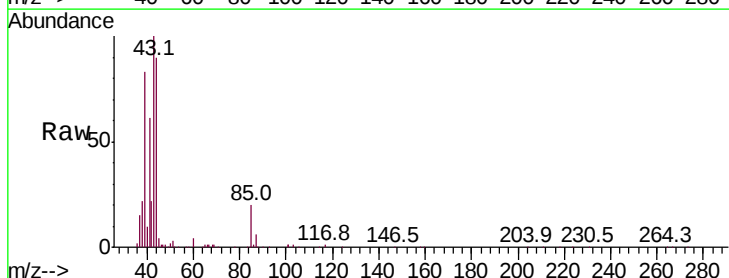

Abundance Ion 85.00 (84.70 to 85.70): VL0

Ion 87.00 (86.70 to 87.70): VL0

3.04

40000


30000


20000

10000

0

Time-->

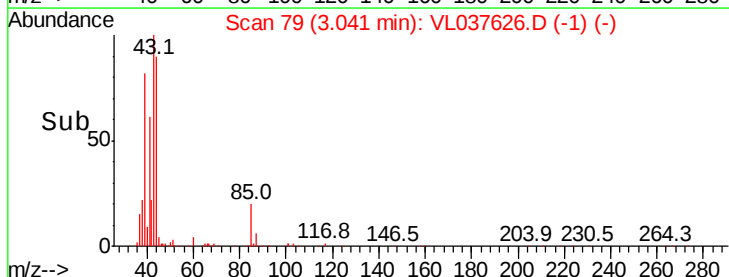

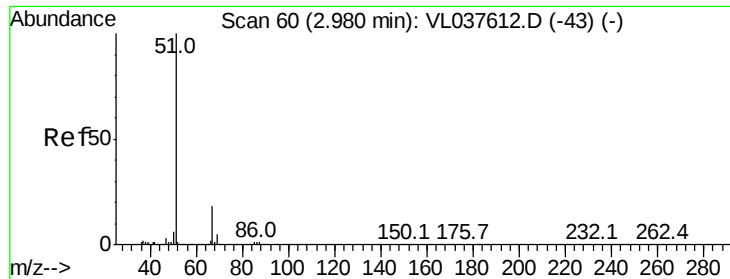





#3
Chlorodifluoromethane
Concen: 0.527 ppbv
RT: 2.98 min Scan# 59
Delta R.T. -0.00 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Instrument :
MSVOA_L
ClientSampled :
IA1

Tot Ion: 51 Resp: 157610
Ion Ratio Lower Upper
51 100
67 13.2 14.0 21.0#




Manual Integrations
APPROVED


MMDadoda
9/20/2021 5:27:24 PM

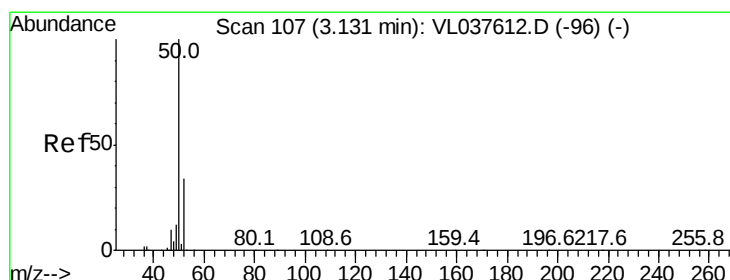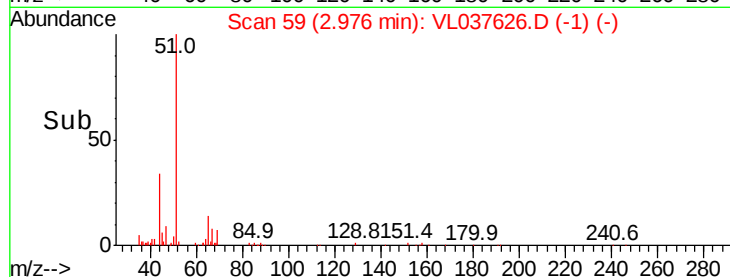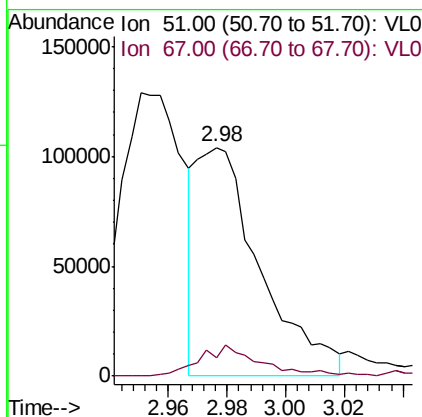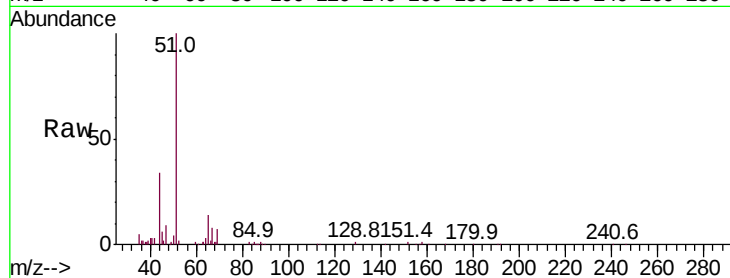

#4
Chloromethane
Concen: 1.183 ppbv
RT: 3.13 min Scan# 107
Delta R.T. 0.00 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Tgt Ion: 50 Resp: 130846
Ion Ratio Lower Upper
50 100
52 30.8 27.1 40.7

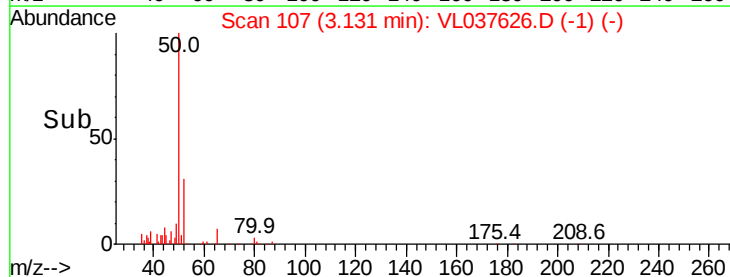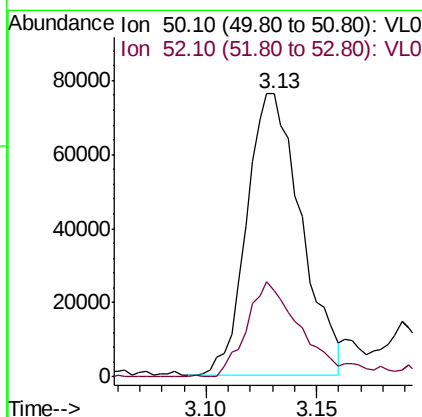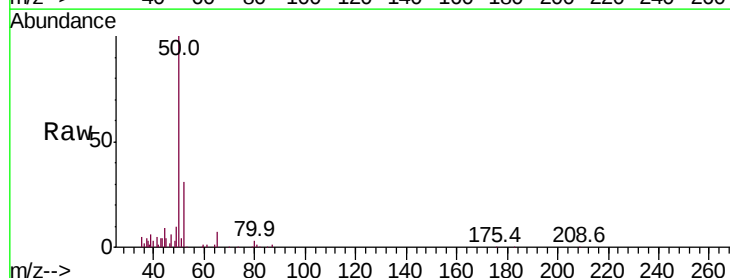

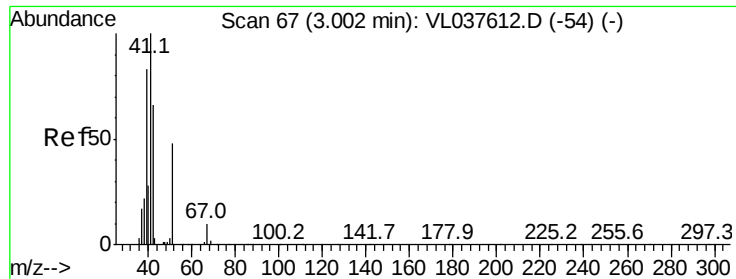





#9
 Propene
 Concen: 10.928 ppbv
 RT: 3.01 min Scan# 70
 Delta R.T. 0.01 min
 Lab File: VL037626.D
 Acq: 16 Sep 2021 22:05

Instrument :
 MSVOA_L
 ClientSampleId :
 IA1

Tot Ion: 41 Resp: 1153773
 Ion Ratio Lower Upper
 41 100
 42 41.9 57.2 85.8#




Manual Integrations
 APPROVED


MMDadoda
 9/20/2021 5:27:24 PM

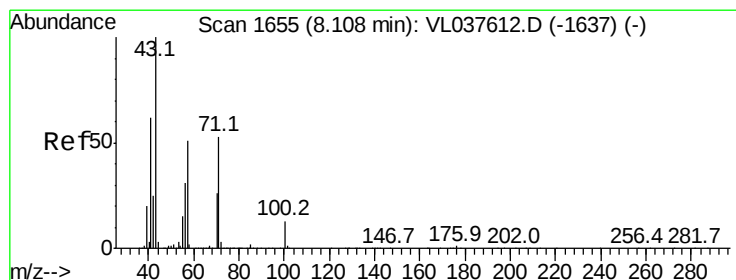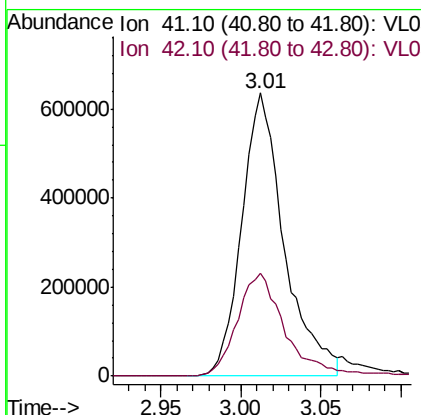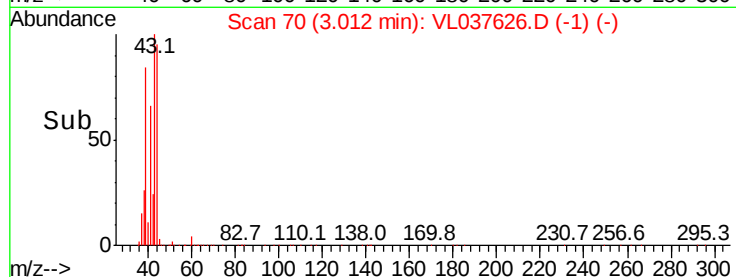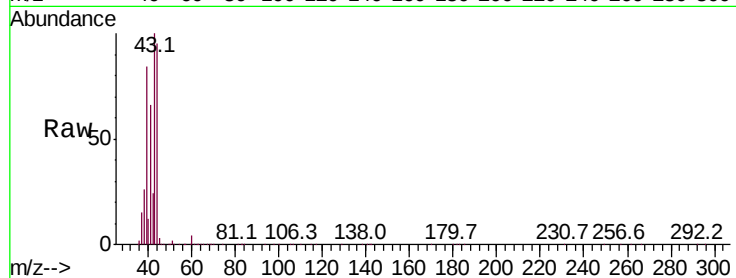

#10
 Heptane
 Concen: 1.060 ppbv m
 RT: 8.10 min Scan# 1653
 Delta R.T. -0.01 min
 Lab File: VL037626.D
 Acq: 16 Sep 2021 22:05

Tgt Ion: 43 Resp: 261027
 Ion Ratio Lower Upper
 43 100
 57 36.6 40.1 60.1#

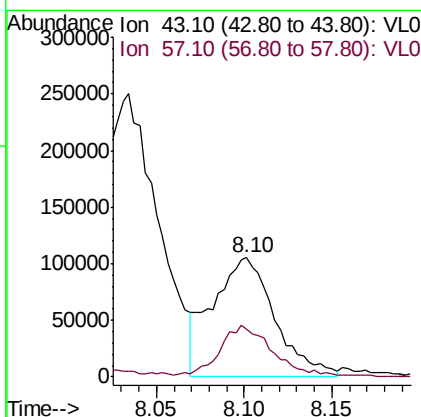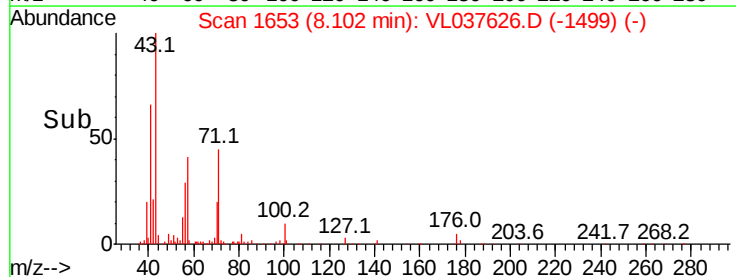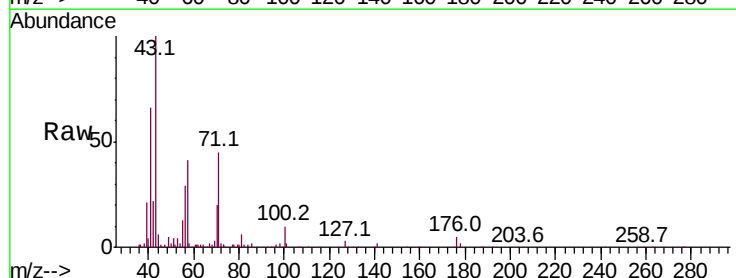

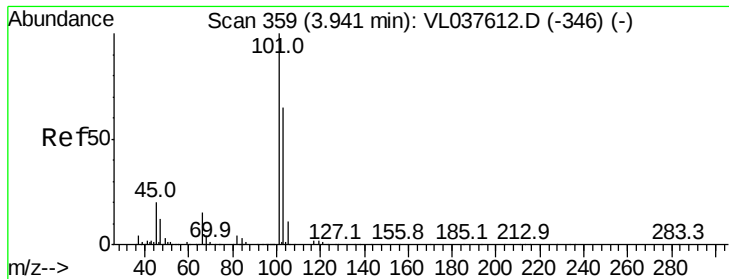





#11
 Trichlorofluoromethane
 Concen: 0.218 ppbv
 RT: 3.94 min Scan# 358
 Delta R.T. -0.00 min
 Lab File: VL037626.D
 Acq: 16 Sep 2021 22:05

Instrument :
 MSVOA_L
 ClientSampleId :
 IA1

Tot Ion	Ratio	Lower	Upper
101	100		
103	60.4	51.9	77.9




Manual Integrations
 APPROVED


MMDadoda
 9/20/2021 5:27:24 PM

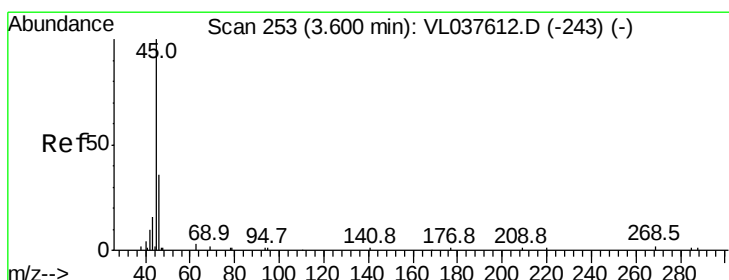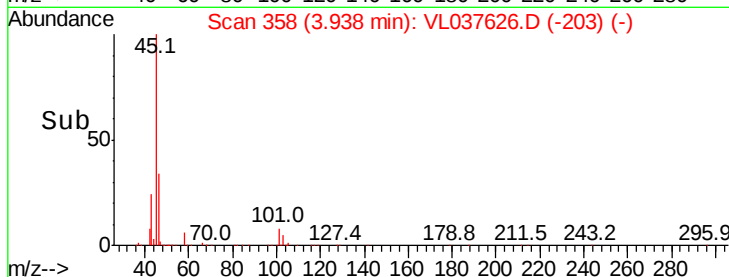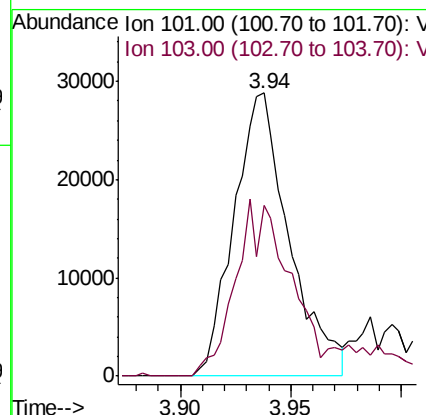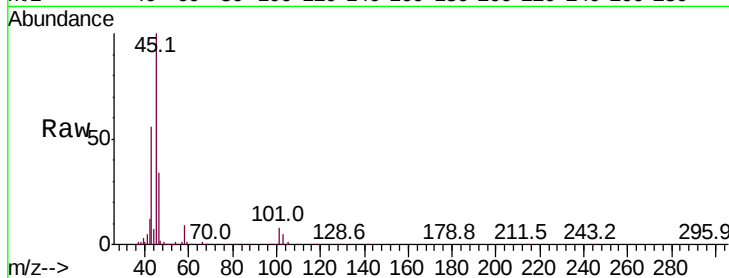

#13
 Ethanol
 Concen: 7147.433 ppbv m
 RT: 3.66 min Scan# 273
 Delta R.T. 0.06 min
 Lab File: VL037626.D
 Acq: 16 Sep 2021 22:05

Tgt Ion	Ratio	Lower	Upper
45	100		
46	59.1	17.2	68.8

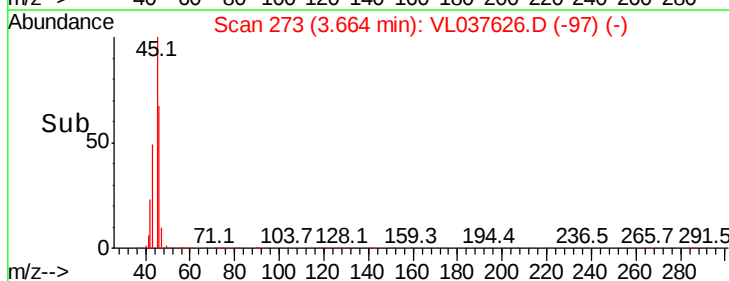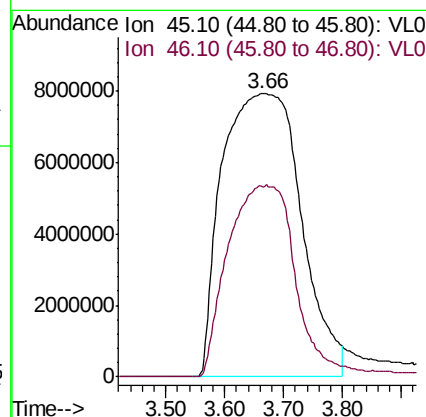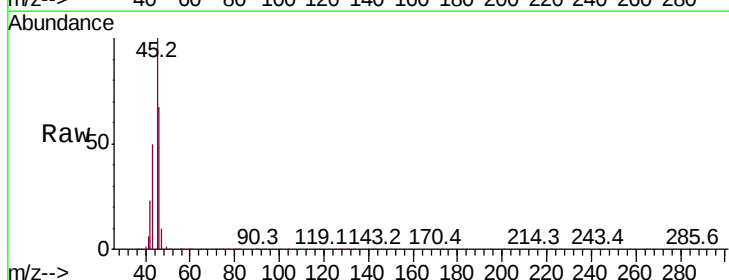

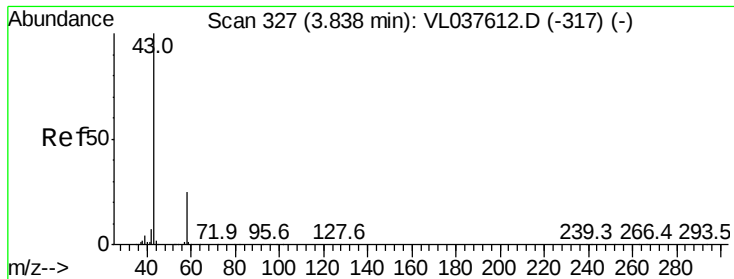

#15

Acetone

Concen: 69.569 ppbv

RT: 3.83 min Scan# 325

Delta R.T. -0.01 min

Lab File: VL037626.D

Acq: 16 Sep 2021 22:05

Instrument :

MSVOA_L

ClientSampleId :

IA1

Tot Ion: 43 Resp:11469529

Ion Ratio Lower Upper





43 100

58 32.5 24.9 37.3

Manual Integrations
APPROVED

MMDadoda

9/20/2021 5:27:24 PM

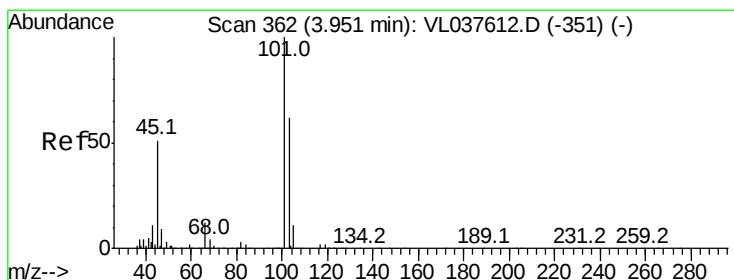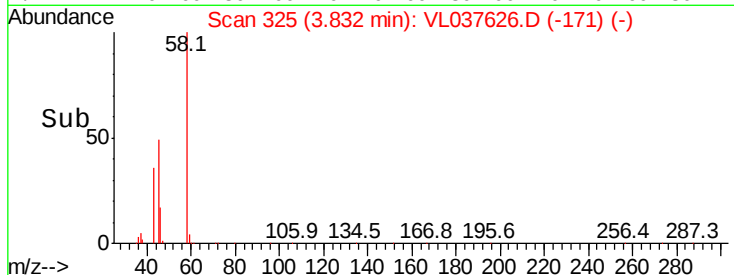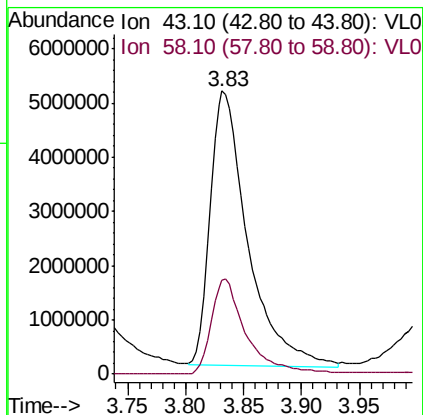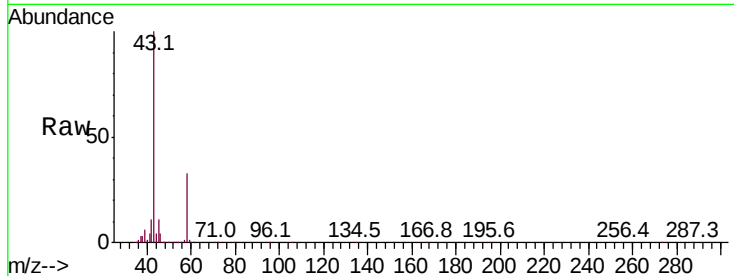

#19

Isopropyl Alcohol

Concen: 260.870 ppbv

RT: 4.04 min Scan# 389

Delta R.T. 0.09 min

Lab File: VL037626.D




Acq: 16 Sep 2021 22:05


Tgt Ion: 45 Resp:23401013

Ion Ratio Lower Upper

45 100

58 1.3 2.9 4.3#

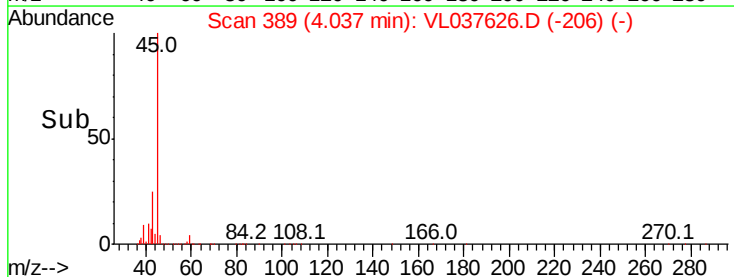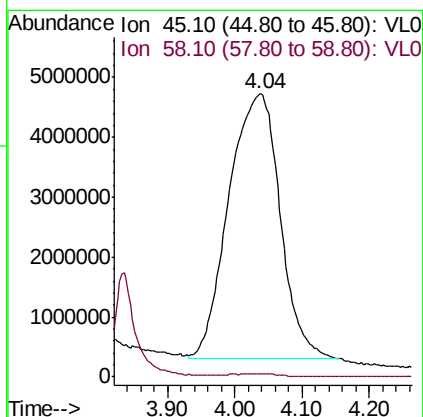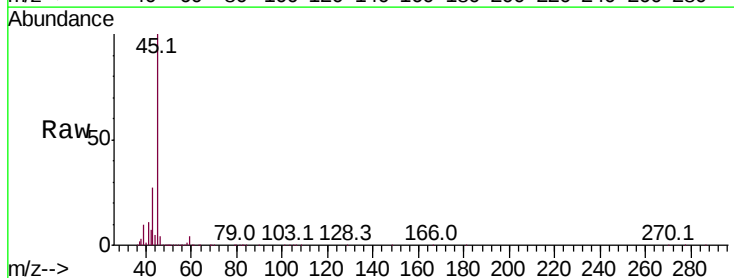

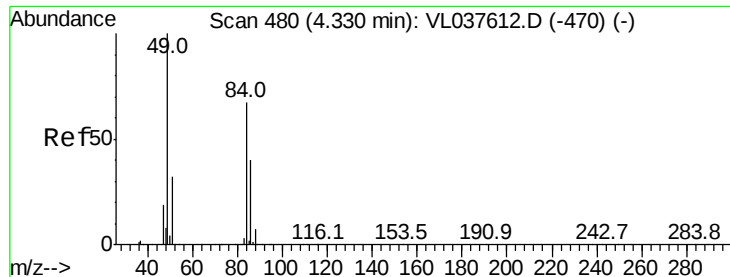





#20
Methvlene Chloride
Concen: 4.723 ppbv
RT: 4.33 min Scan# 480
Delta R.T. 0.00 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Instrument :
MSVOA_L
ClientSampleId :
IA1

Tot Ion	84	Resp	371700
Ion Ratio	Lower	Upper	
84	100		
49	143.2	120.0	180.0
51	45.7	38.0	57.0
86	58.7	48.2	72.2




Manual Integrations
APPROVED


MMDadoda
9/20/2021 5:27:24 PM

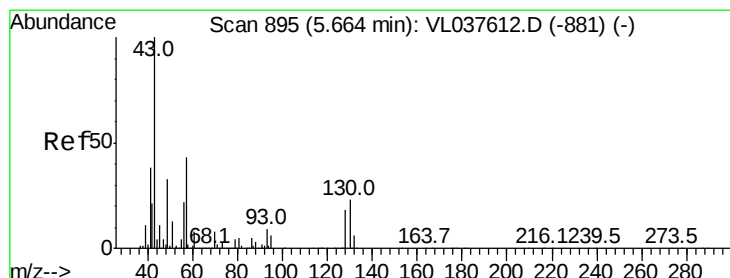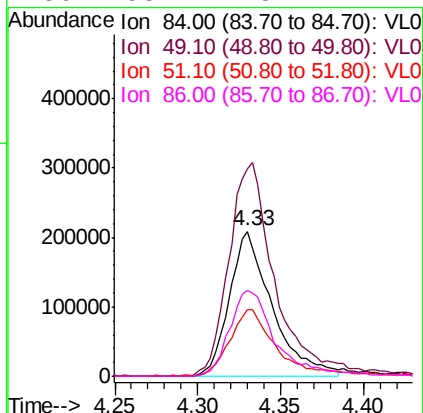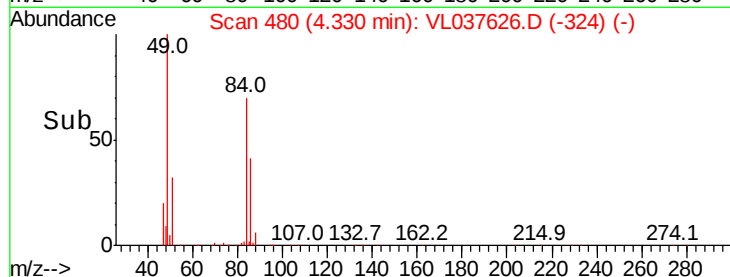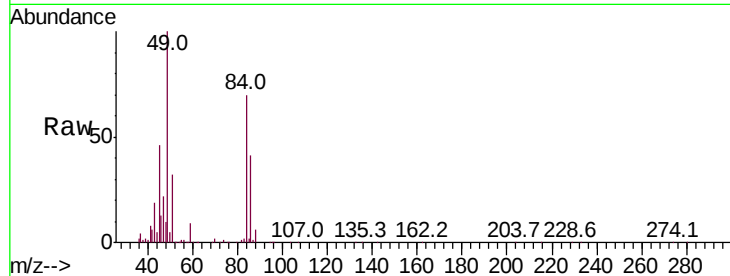

#25
Ethyl Acetate
Concen: 6.755 ppbv
RT: 5.65 min Scan# 892
Delta R.T. -0.01 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Tgt Ion	43	Resp	2697080
Ion Ratio	Lower	Upper	
43	100		
45	15.1	8.0	12.0#
61	11.6	7.5	11.3#
70	8.7	5.6	8.4#

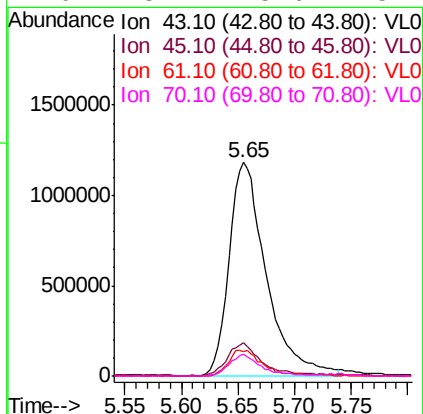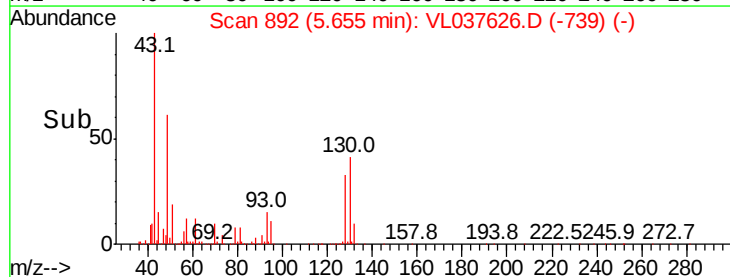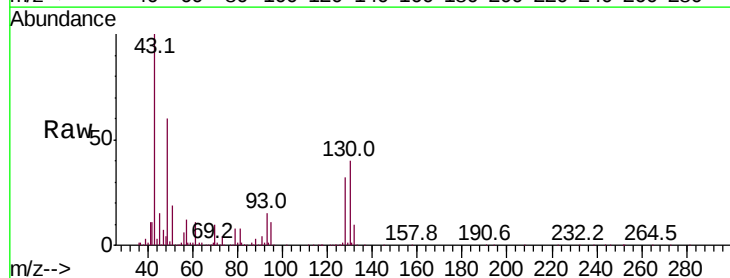

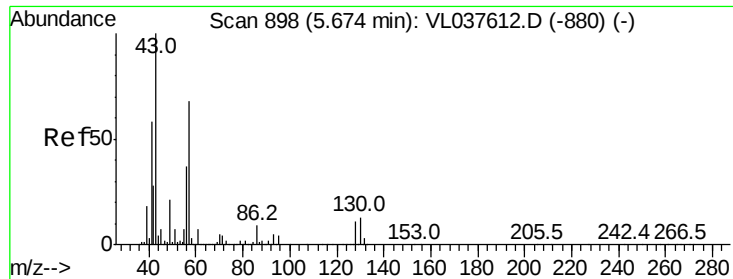





#26
Hexane
Concen: 2.919 ppbv
RT: 5.67 min Scan# 897
Delta R.T. -0.00 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Instrument :
MSVOA_L
ClientSampleId :
IA1

Tot Ion	Ratio	Lower	Upper
57	100		
41	99.7	70.9	106.3
43	499.2	170.4	255.6#
56	59.1	42.6	64.0




Manual Integrations
APPROVED


MMDadoda
9/20/2021 5:27:24 PM

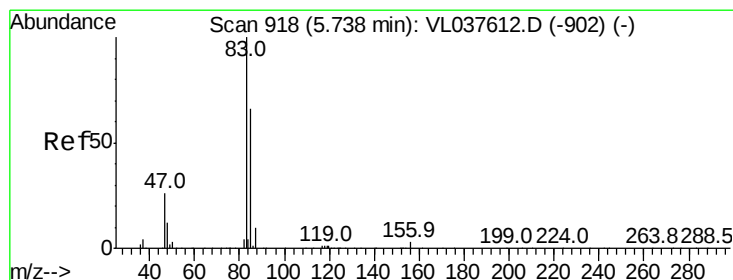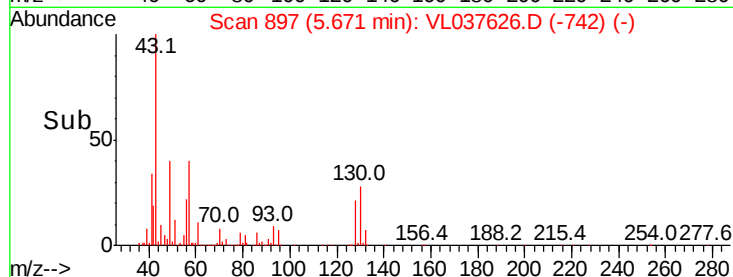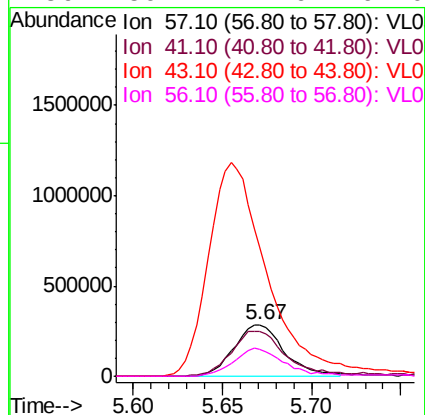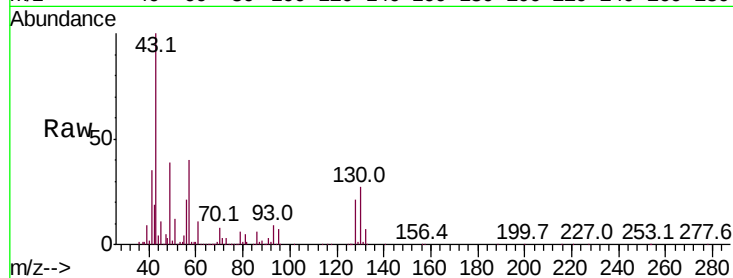

#29
Chloroform
Concen: 7.830 ppbv
RT: 5.74 min Scan# 917
Delta R.T. -0.00 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Tgt Ion	Ratio	Lower	Upper
83	100		
85	67.1	52.6	79.0

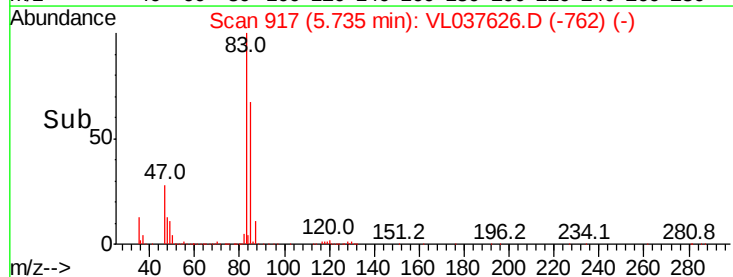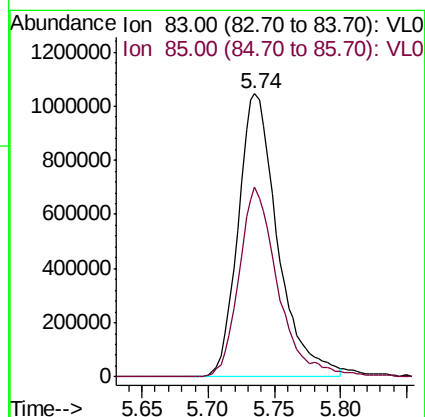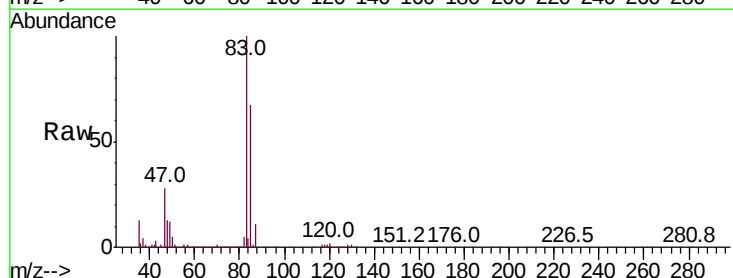

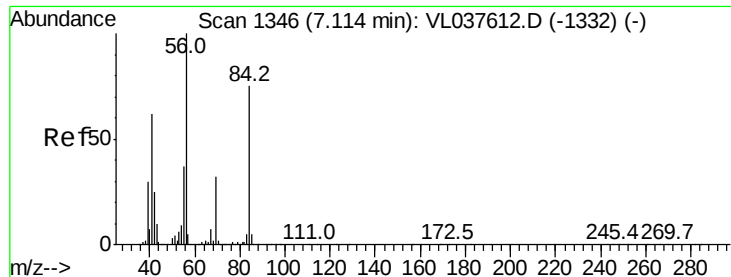





#30
Cvclohexane
Concen: 0.489 ppbv m
RT: 7.11 min Scan# 1344
Delta R.T. -0.01 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Instrument :
MSVOA_L
ClientSampleId :
IA1

Tot Ion	Ratio	Lower	Upper
84	100		
56	123.9	113.6	170.4
41	0.0	67.9	101.9#




Manual Integrations
APPROVED


MMDadoda
9/20/2021 5:27:24 PM

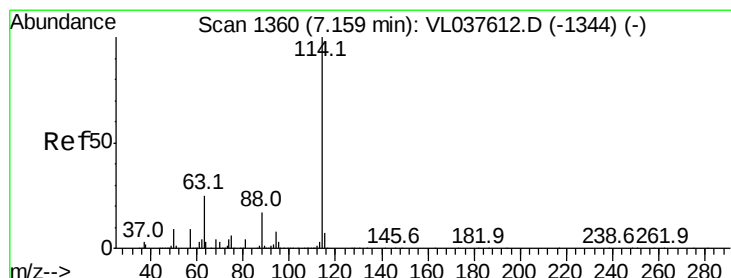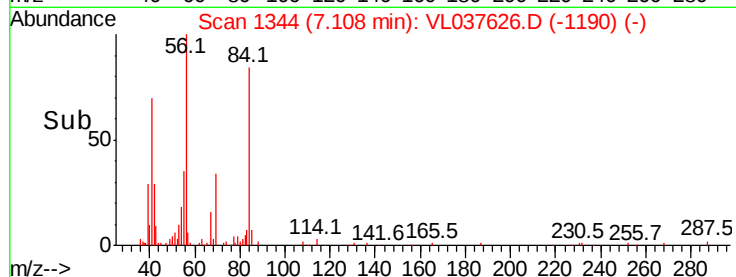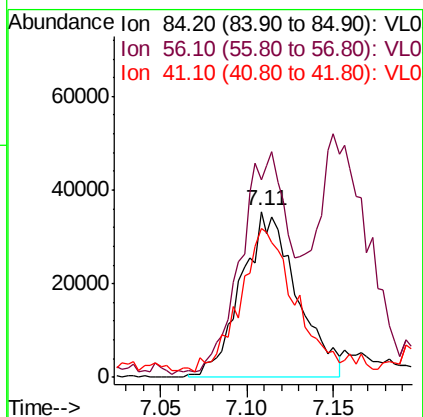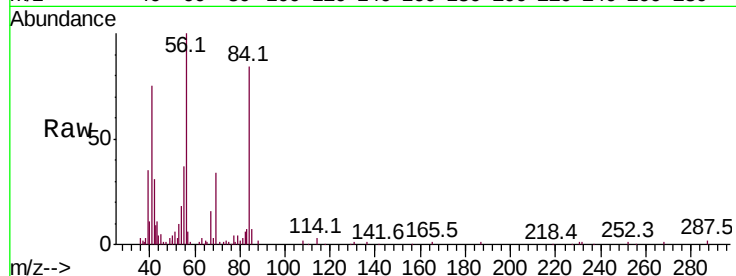

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.16 min Scan# 1359
Delta R.T. -0.00 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Tgt Ion	Ratio	Lower	Upper
114	100		
63	24.2	19.6	29.4
88	17.8	14.2	21.4

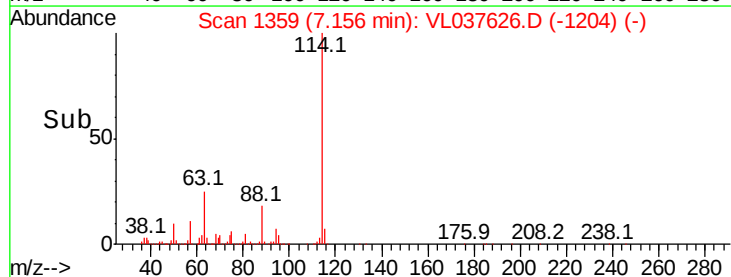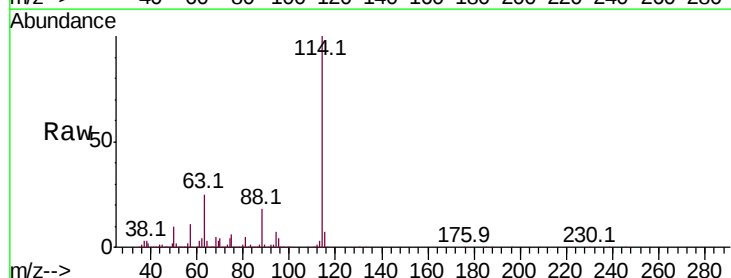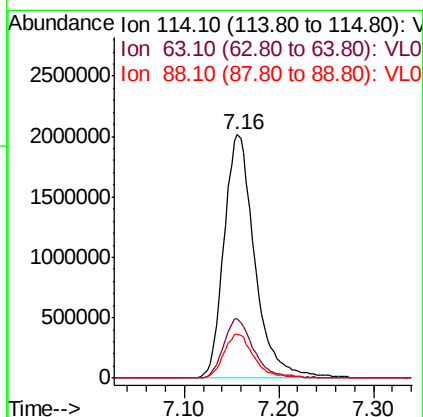

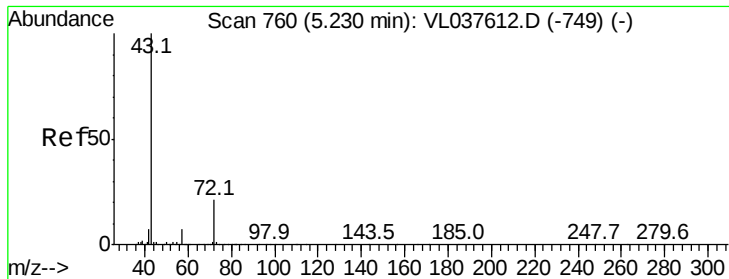

#34

2-Butanone

Concen: 4.502 ppbv

RT: 5.23 min Scan# 759

Delta R.T. -0.00 min

Lab File: VL037626.D

Acq: 16 Sep 2021 22:05

Instrument :

MSVOA_L

ClientSampled :

IA1

Tot Ion: 43 Resp: 832486

Ion Ratio Lower Upper

43 100





72 23.5 18.4 27.6

Manual Integrations

APPROVED

MMDadoda

9/20/2021 5:27:24 PM

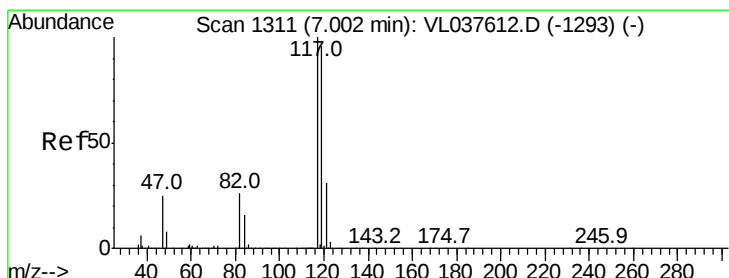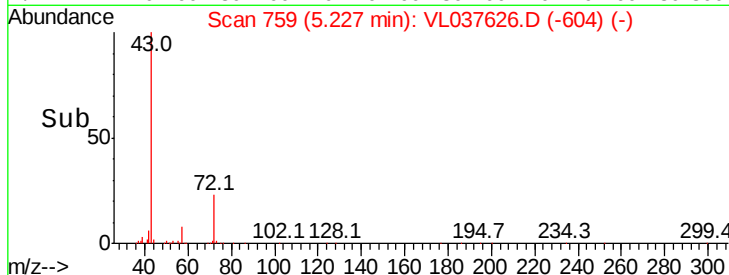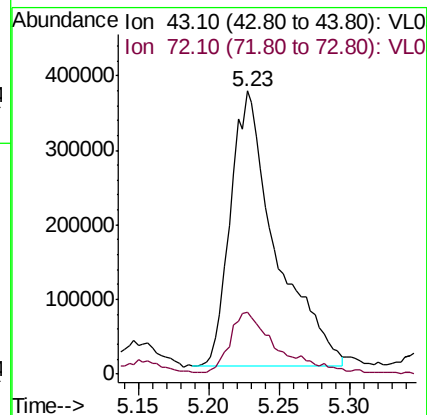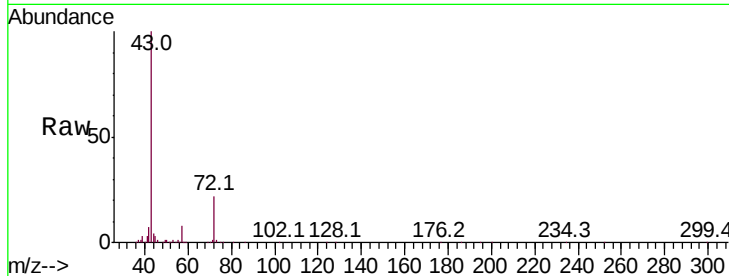

#35

Carbon Tetrachloride

Concen: 0.072 ppbv m

RT: 7.00 min Scan# 1310

Delta R.T. -0.00 min

Lab File: VL037626.D

Acq: 16 Sep 2021 22:05




Tgt Ion: 117 Resp: 18448


Ion Ratio Lower Upper

117 100

119 98.4 77.0 115.6

121 21.2 24.5 36.7#

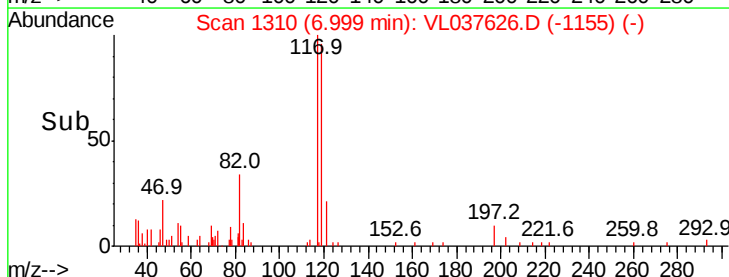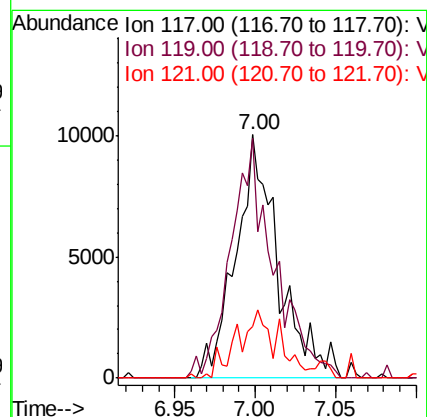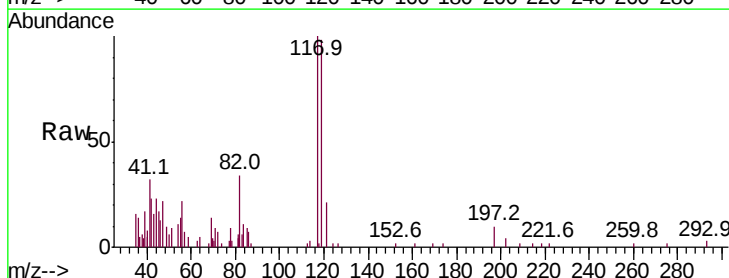

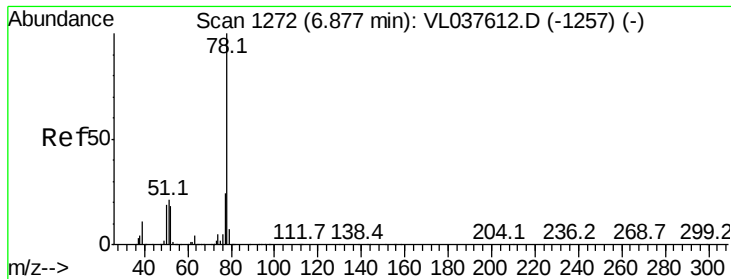





#36
Benzene
Concen: 1.238 ppbv
RT: 6.87 min Scan# 1271
Delta R.T. -0.00 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Instrument :
MSVOA_L
ClientSampled :
IA1

Tot Ion	Ratio	Resp Lower	Upper
78	100		
77	22.9	19.0	28.4
50	14.2	14.8	22.2#




Manual Integrations
APPROVED


MMDadoda
9/20/2021 5:27:24 PM

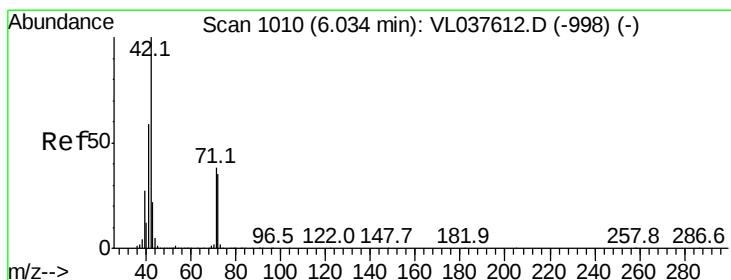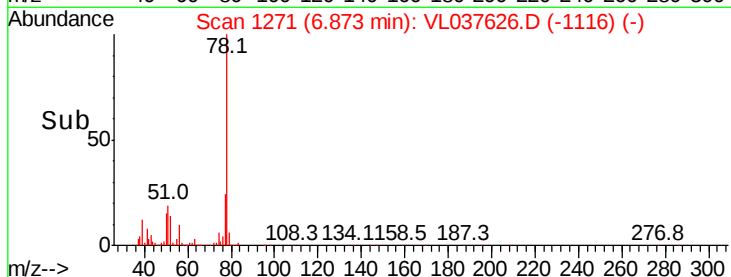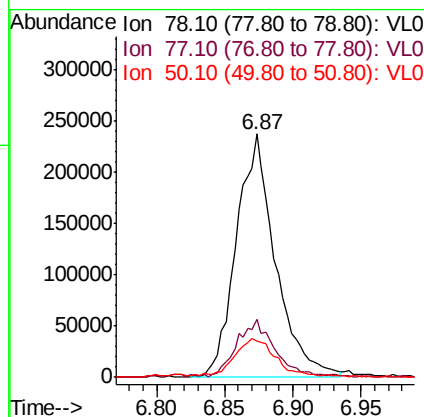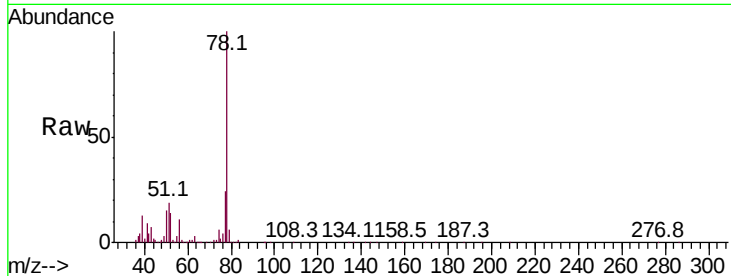

#41
Tetrahydrofuran
Concen: 3.147 ppbv m
RT: 6.04 min Scan# 1013
Delta R.T. 0.01 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Tgt Ion	Ratio	Resp Lower	Upper
42	100		
72	13.0	31.4	47.2#
71	0.0	30.6	46.0#

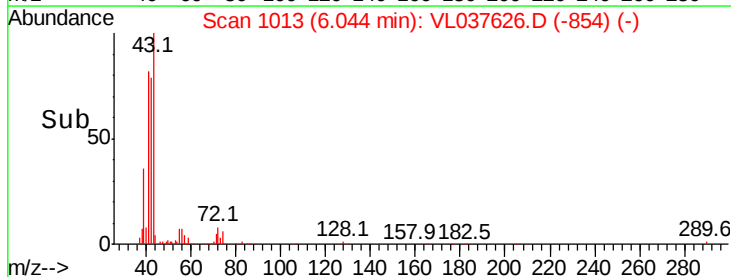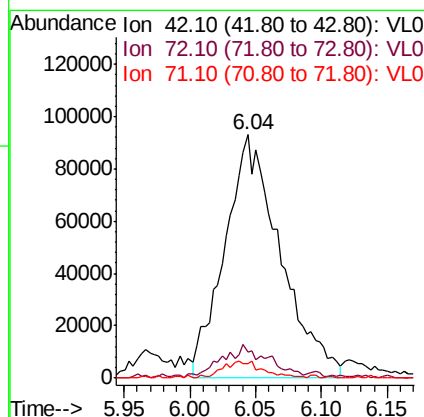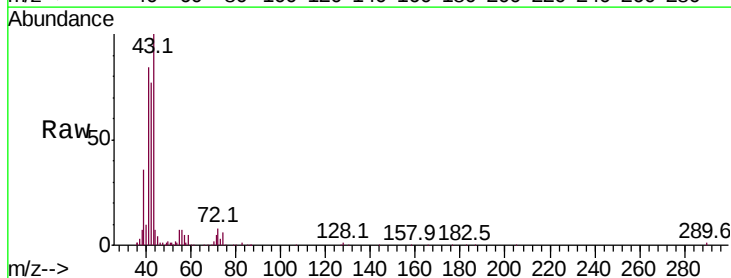

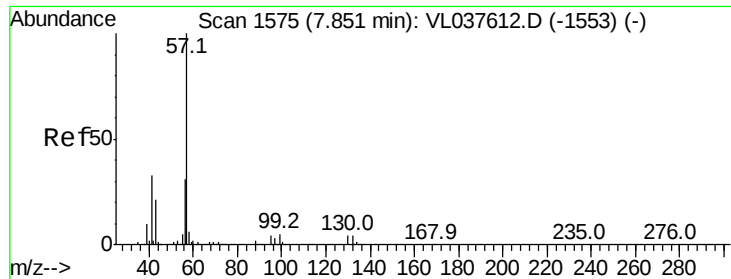

#44

2,2,4-Trimethylpentane

Concen: 0.873 ppbv

RT: 7.85 min Scan# 1574

Delta R.T. -0.00 min

Lab File: VL037626.D

Acq: 16 Sep 2021 22:05

Instrument :

MSVOA_L





ClientSampleId :

IA1

Tot Ion:	57	Resp:	556603
Ion Ratio	Lower	Upper	
57	100		
41	37.9	26.1	39.1
56	38.9	25.7	38.5#

Manual Integrations
APPROVED

MMDadoda
9/20/2021 5:27:24 PM

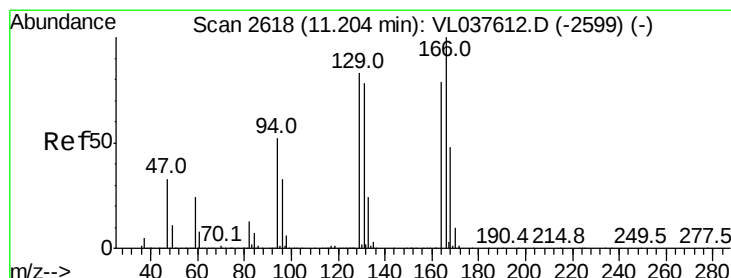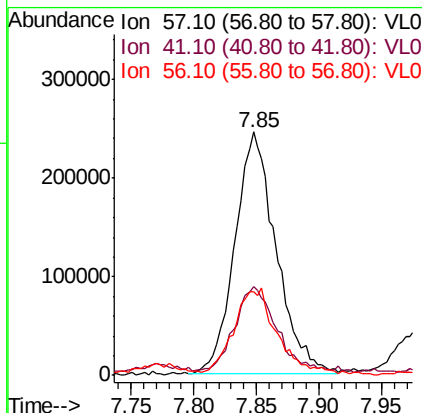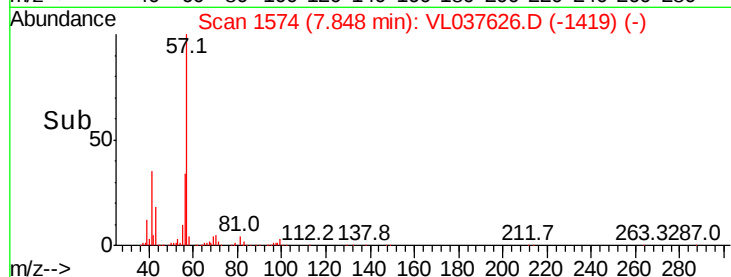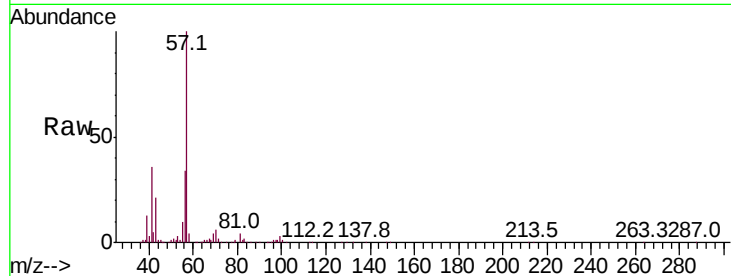

#52

Tetrachloroethene

Concen: 0.113 ppbv m




RT: 11.19 min Scan# 2615


Delta R.T. -0.01 min

Lab File: VL037626.D

Acq: 16 Sep 2021 22:05

Tgt Ion:	164	Resp:	16501
Ion Ratio	Lower	Upper	
164	100		
166	99.6	101.2	151.8#
129	53.1	84.0	126.0#
131	84.2	78.8	118.2

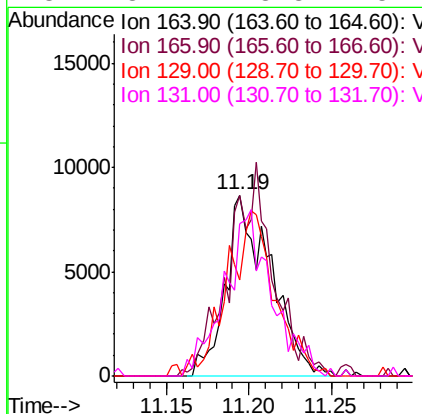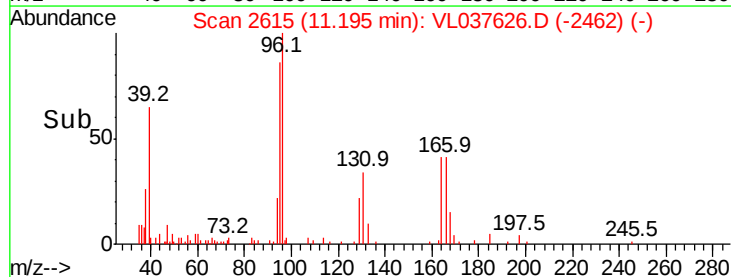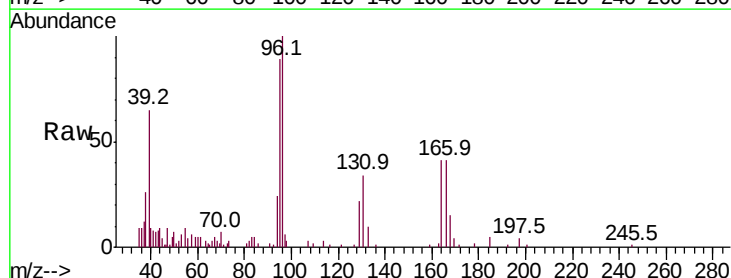

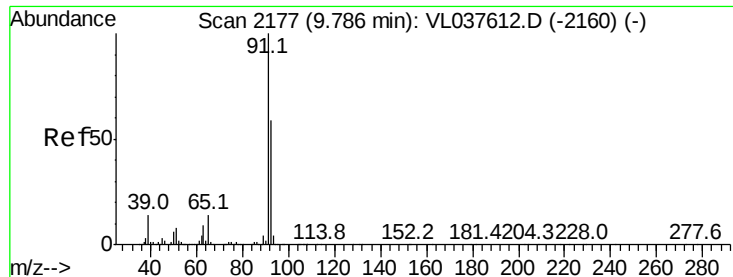

#53

Toluene

Concen: 5.724 ppbv

RT: 9.78 min Scan# 2176

Delta R.T. -0.00 min

Lab File: VL037626.D

Acq: 16 Sep 2021 22:05

Instrument :

MSVOA_L

ClientSampleId :

IA1

Tot Ion: 91 Resp: 2414057

Ion Ratio Lower Upper





91 100

92 60.1 48.9 73.3

Manual Integrations
APPROVED

MMDadoda

9/20/2021 5:27:24 PM

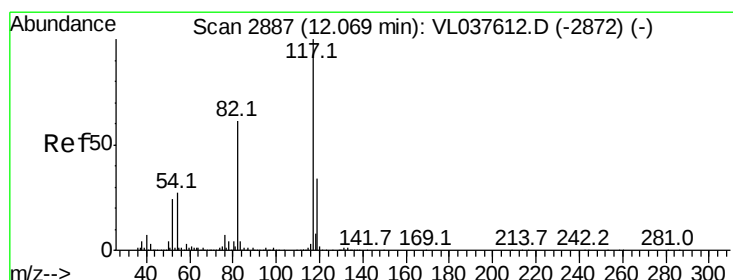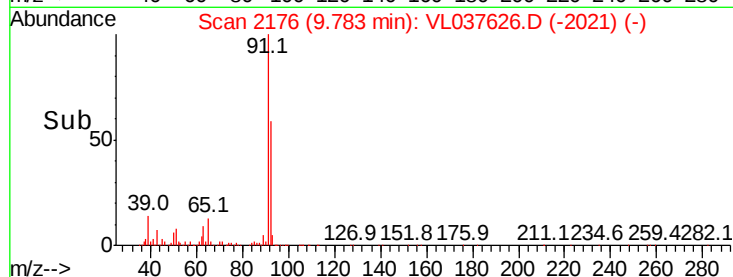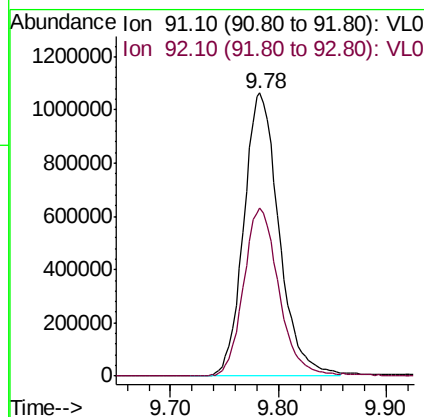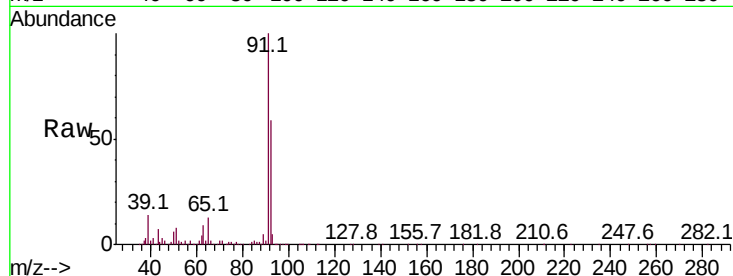

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.07 min Scan# 2886

Delta R.T. -0.00 min

Lab File: VL037626.D

Acq: 16 Sep 2021 22:05




Tgt Ion: 117 Resp: 3900966


Ion Ratio Lower Upper

117 100

82 65.3 50.6 75.8

119 34.6 26.2 39.2

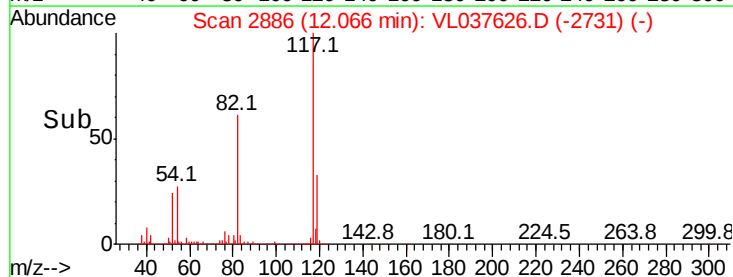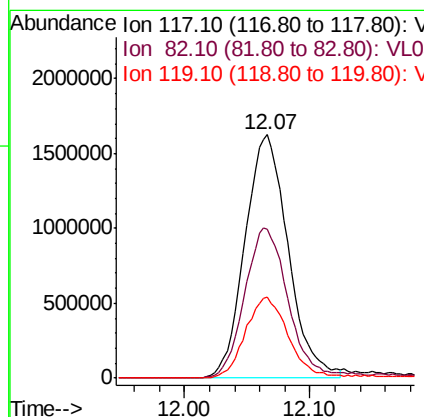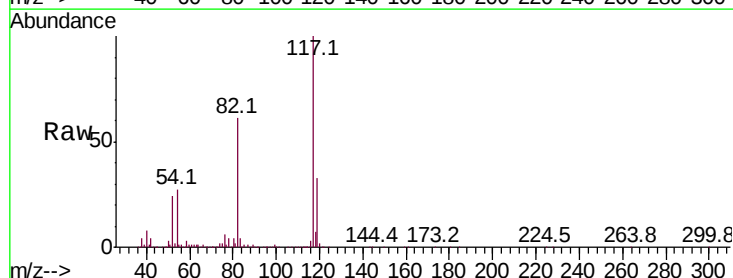

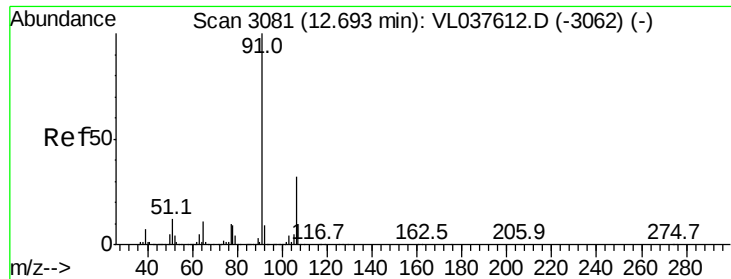





#58
Ethyl Benzene
Concen: 1.214 ppbv
RT: 12.69 min Scan# 3079
Delta R.T. -0.01 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Instrument :
MSVOA_L
ClientSampled :
IA1

Tot Ion: 91 Resp: 628524
Ion Ratio Lower Upper
91 100
106 32.6 25.3 37.9




Manual Integrations
APPROVED


MMDadoda
9/20/2021 5:27:24 PM

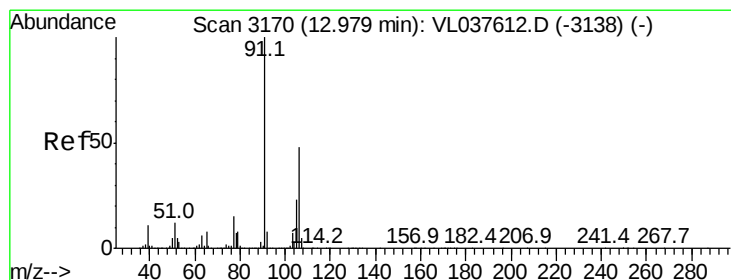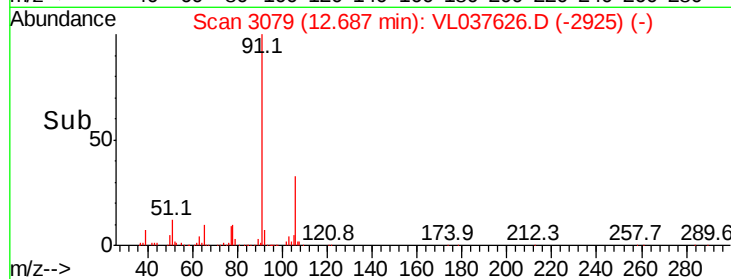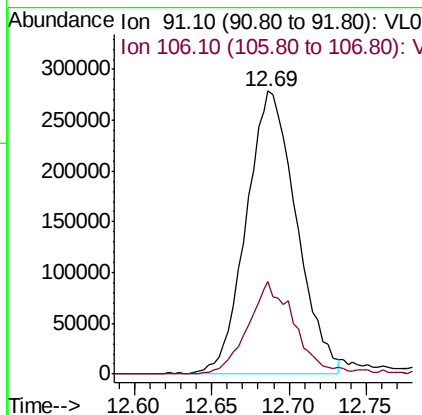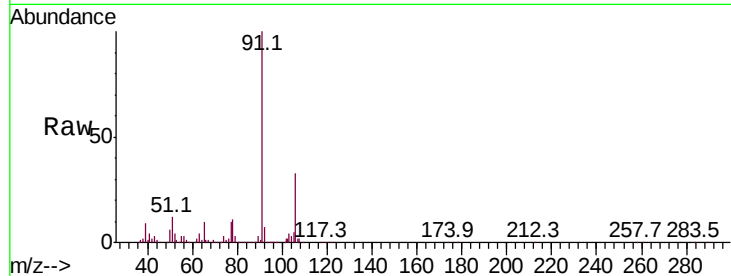

#59
m/p-Xylene
Concen: 4.915 ppbv
RT: 12.94 min Scan# 3159
Delta R.T. -0.04 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Tgt Ion: 91 Resp: 2217851
Ion Ratio Lower Upper
91 100
106 47.2 36.6 55.0

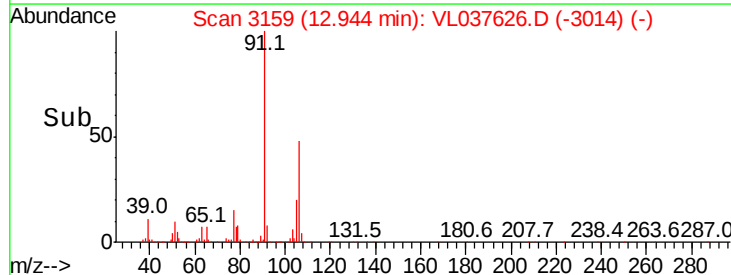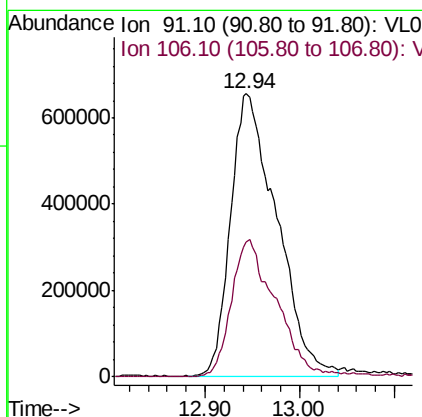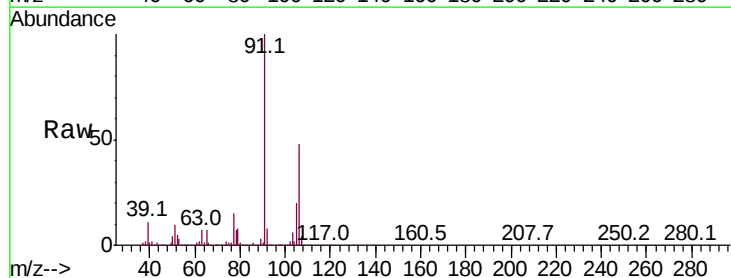

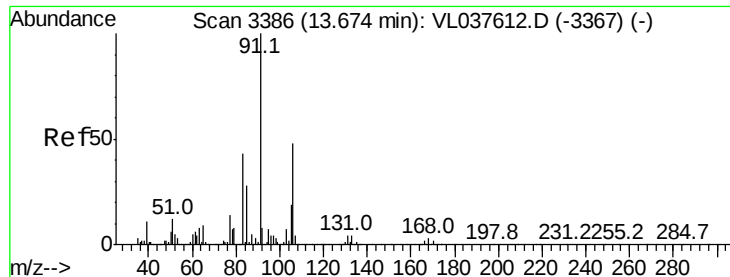





#60
o-Xylene
Concen: 1.751 ppbv
RT: 13.67 min Scan# 3385
Delta R.T. -0.00 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Instrument :
MSVOA_L
ClientSampled :
IA1

Tot Ion	Ratio	Lower	Upper
91	100		
106	49.3	23.0	69.0




Manual Integrations
APPROVED


MMDadoda
9/20/2021 5:27:24 PM

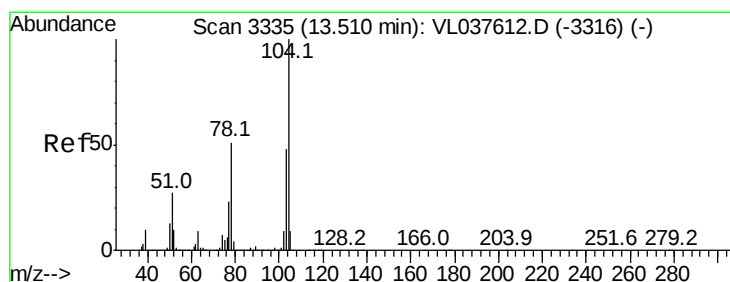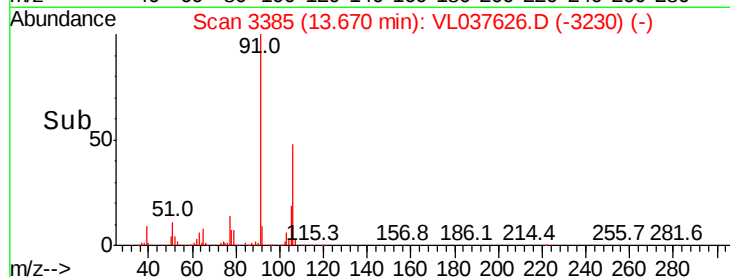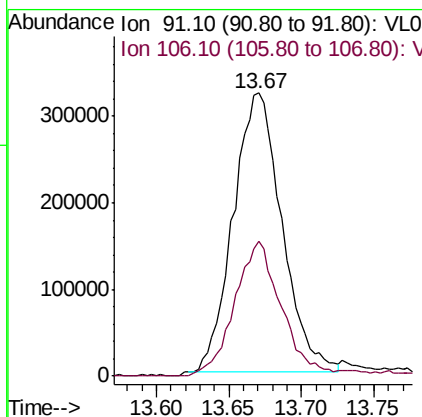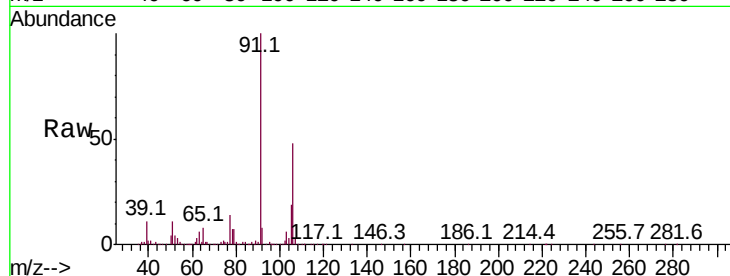

#61
Styrene
Concen: 1.654 ppbv
RT: 13.51 min Scan# 3335
Delta R.T. 0.00 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Tgt Ion	Ratio	Lower	Upper
104	100		
78	53.8	39.7	59.5
103	52.3	38.8	58.2

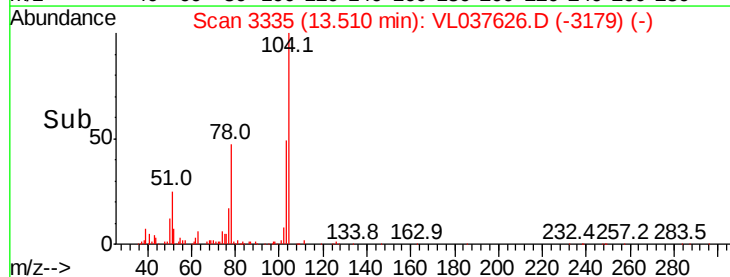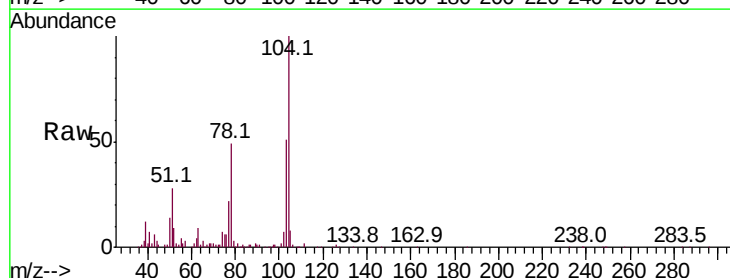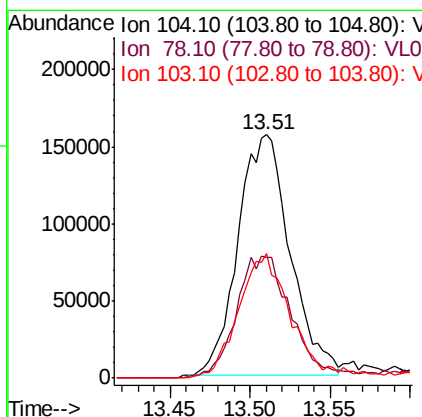

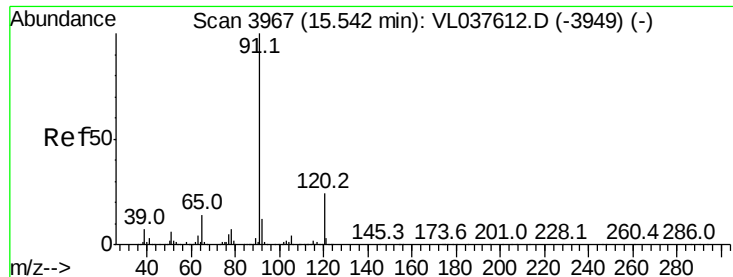





#64
n-propylbenzene
Concen: 0.158 ppbv m
RT: 15.53 min Scan# 3964
Delta R.T. -0.01 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Instrument :
MSVOA_L
ClientSampled :
IA1

Tot Ion:120 Resp: 24437
Ion Ratio Lower Upper
120 100
91 444.0 345.0 517.4




Manual Integrations
APPROVED


MMDadoda
9/20/2021 5:27:24 PM

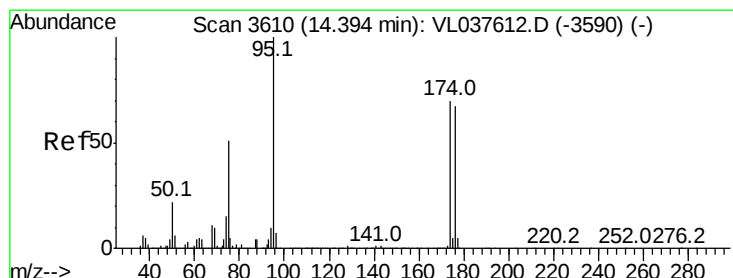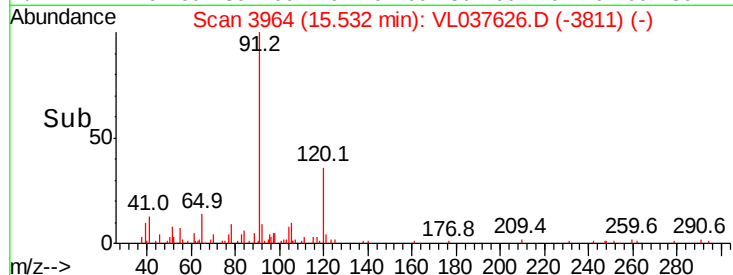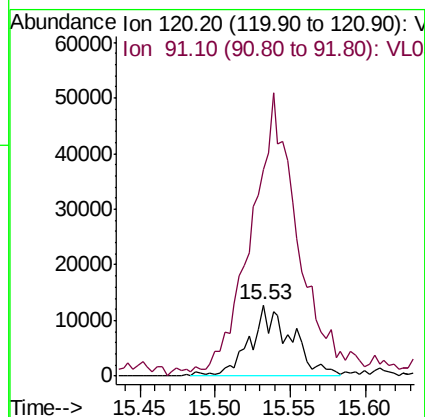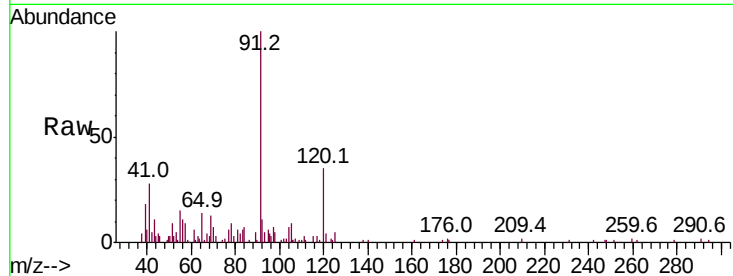

#68
1-Bromo-4-Fluorobenzene
Concen: 10.112 ppbv
RT: 14.39 min Scan# 3610
Delta R.T. 0.00 min
Lab File: VL037626.D
Acq: 16 Sep 2021 22:05

Tgt Ion: 95 Resp: 2850785
Ion Ratio Lower Upper
95 100
174 74.3 56.3 84.5
175 5.9 4.4 6.6

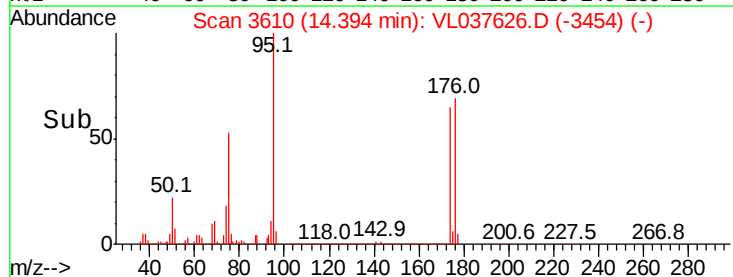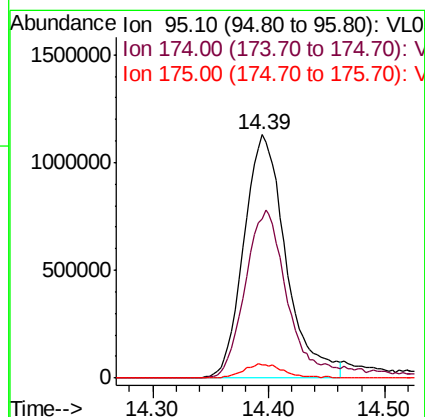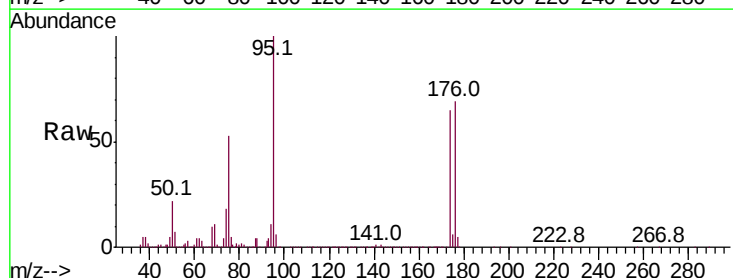

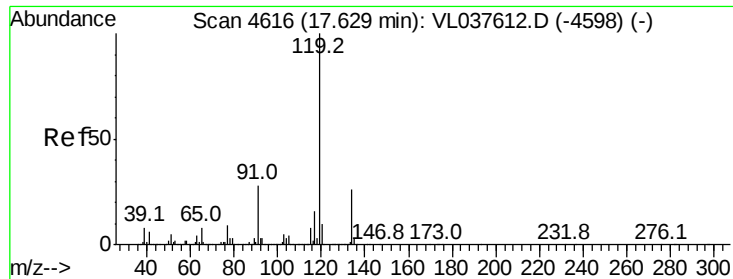





#69
 p-Isopropyltoluene
 Concen: 0.552 ppbv
 RT: 17.63 min Scan# 4616
 Delta R.T. 0.00 min
 Lab File: VL037626.D
 Acq: 16 Sep 2021 22:05

Instrument :
 MSVOA_L
 ClientSampleId :
 IA1

Tot Ion	Ratio	Resp Lower	Upper
119	100		
134	27.0	21.2	31.8
91	36.0	22.2	33.2#




Manual Integrations
 APPROVED


MMDadoda
 9/20/2021 5:27:24 PM

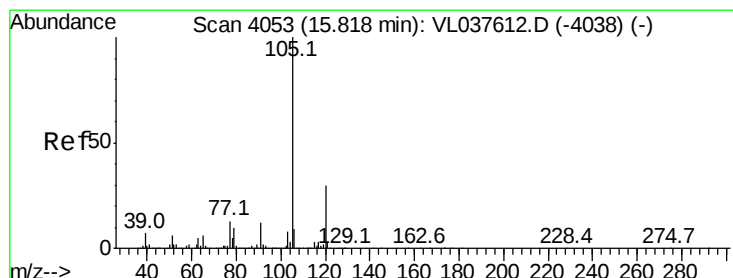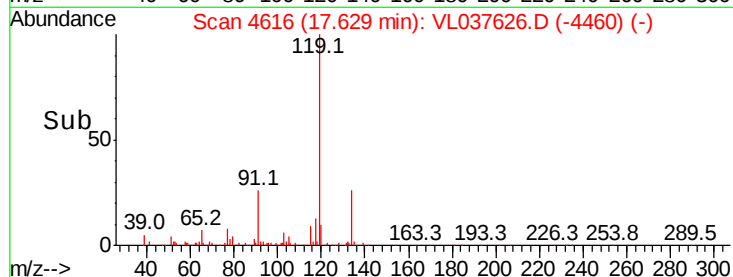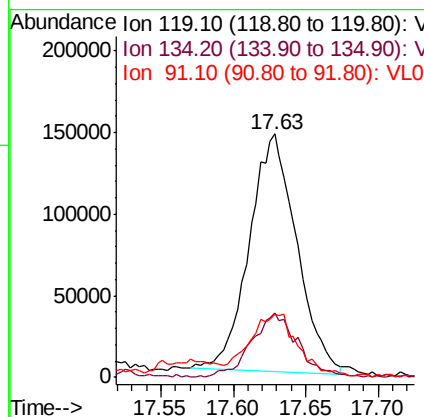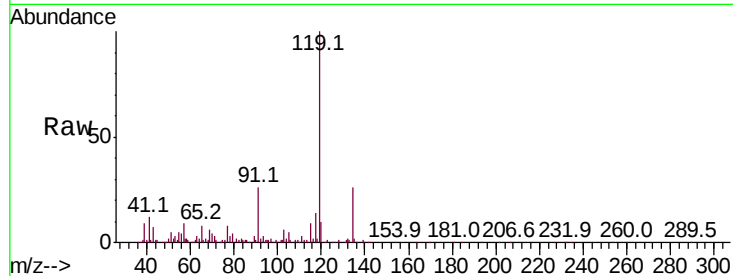

#72
 4-Ethyltoluene
 Concen: 0.303 ppbv m
 RT: 15.81 min Scan# 4050
 Delta R.T. -0.01 min
 Lab File: VL037626.D
 Acq: 16 Sep 2021 22:05

Tgt Ion	Ratio	Resp Lower	Upper
105	100		
120	33.9	24.7	37.1
91	0.0	9.9	14.9#
77	18.2	10.5	15.7#

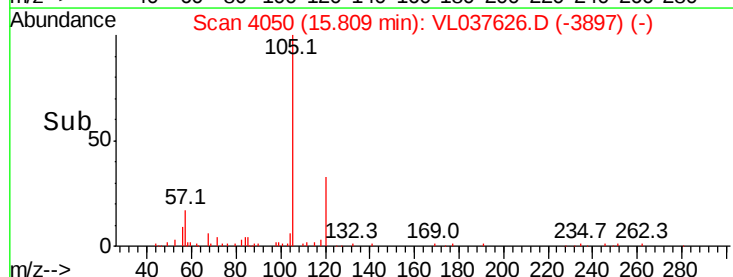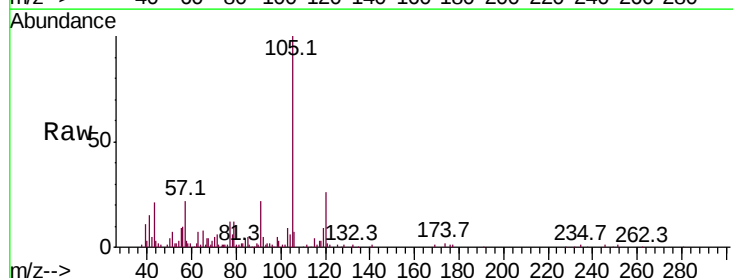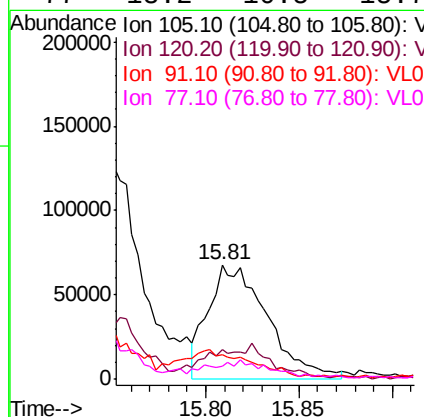

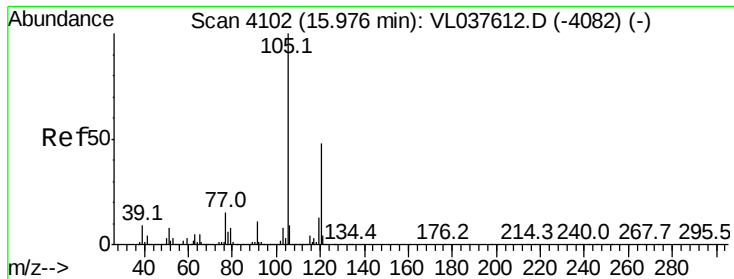

#73

1,3,5-Trimethylbenzene

Concen: 0.285 ppbv

RT: 15.97 min Scan# 4101

Delta R.T. -0.00 min

Lab File: VL037626.D

Acq: 16 Sep 2021 22:05

Instrument :

MSVOA_L

ClientSampled :

IA1

Tot Ion:105 Resp: 130799

Ion Ratio Lower Upper


105 100

120 38.7 38.3 57.5

Manual Integrations
APPROVED




MMDadoda

9/20/2021 5:27:24 PM

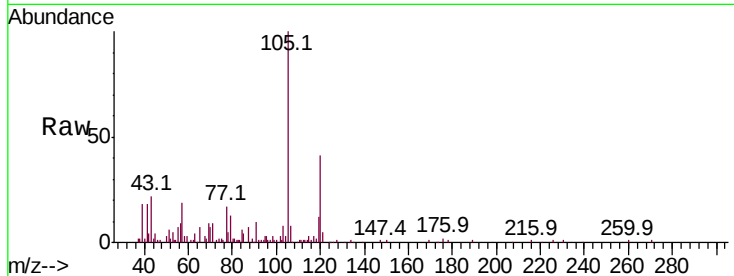

Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

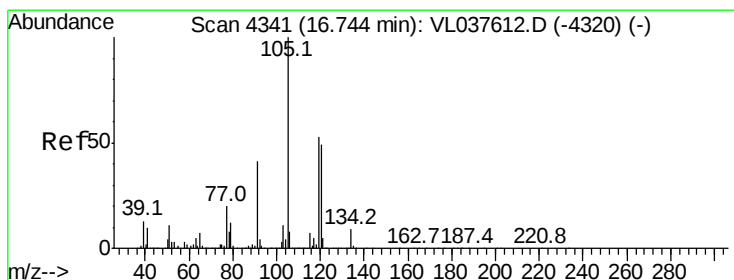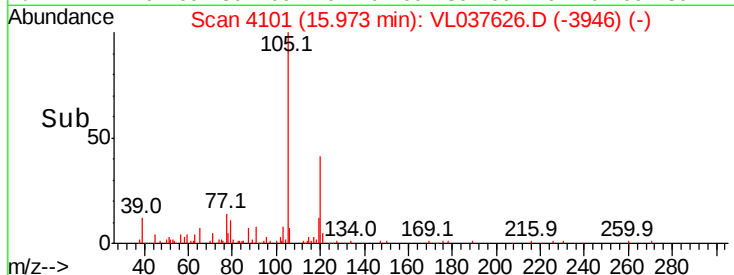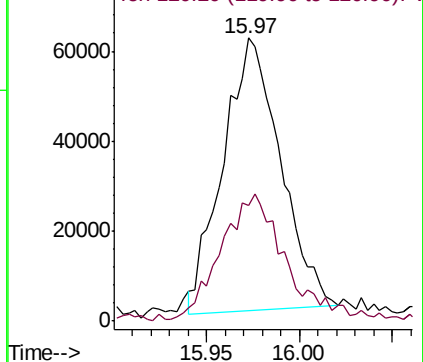

#74

1,2,4-Trimethylbenzene

Concen: 1.029 ppbv

RT: 16.74 min Scan# 4339

Delta R.T. -0.01 min

Lab File: VL037626.D

Acq: 16 Sep 2021 22:05

Tgt Ion:105 Resp: 497960


Ion Ratio Lower Upper

105 100

120 39.8 39.4 59.0

91 10.5 33.3 49.9#

77 11.6 15.7 23.5#


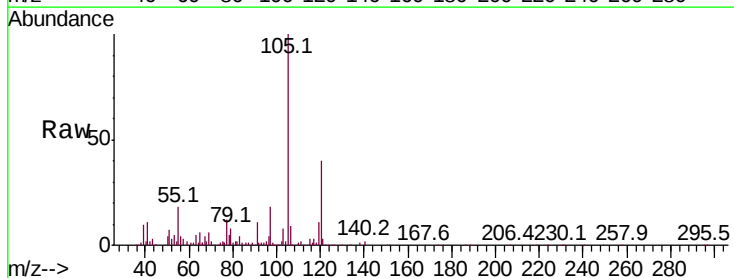



Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

Ion 91.10 (90.80 to 91.80): VL0

Ion 77.10 (76.80 to 77.80): VL0

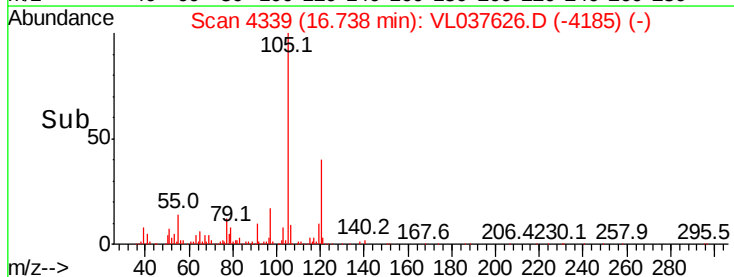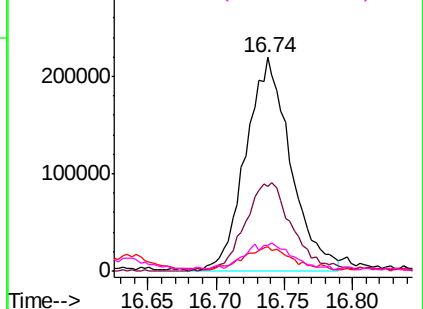

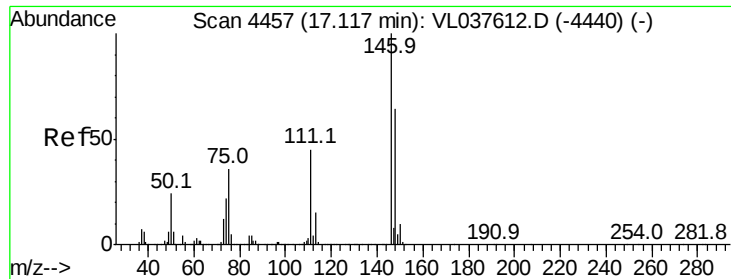





#76
 1,4-Dichlorobenzene
 Concen: 0.402 ppbv m
 RT: 17.11 min Scan# 4457
 Delta R.T. -0.01 min
 Lab File: VL037626.D
 Acq: 16 Sep 2021 22:05

Instrument :
 MSVOA_L
 ClientSampled :
 IA1

Tot Ion	Ratio	Resp	Lower	Upper
146	100	119233		
111	63.7	22.5	67.5	
148	62.8	32.9	98.6	




Manual Integrations
 APPROVED


MMDadoda
 9/20/2021 5:27:24 PM

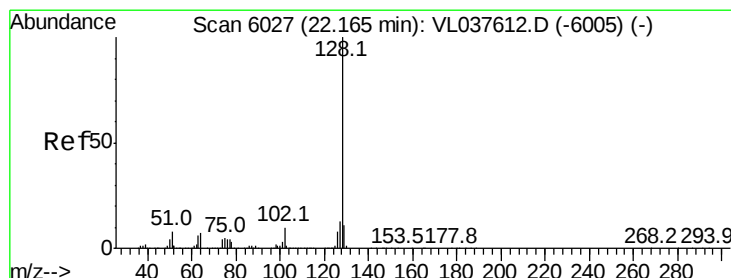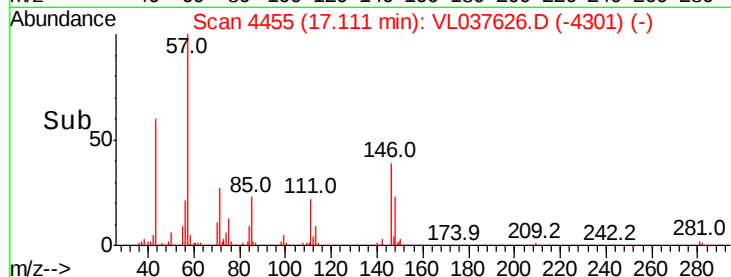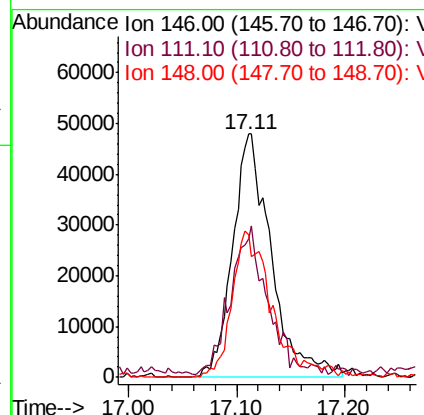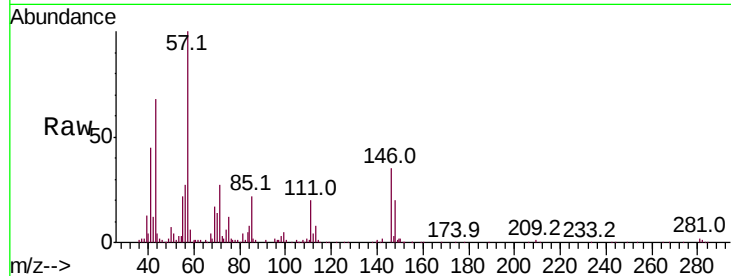

#79
 Naphthalene
 Concen: 0.774 ppbv m
 RT: 22.17 min Scan# 6027
 Delta R.T. 0.00 min
 Lab File: VL037626.D
 Acq: 16 Sep 2021 22:05

Tgt Ion	Ratio	Resp	Lower	Upper
128	100	230171		
127	12.1	10.6	16.0	
129	13.0	8.6	12.8#	

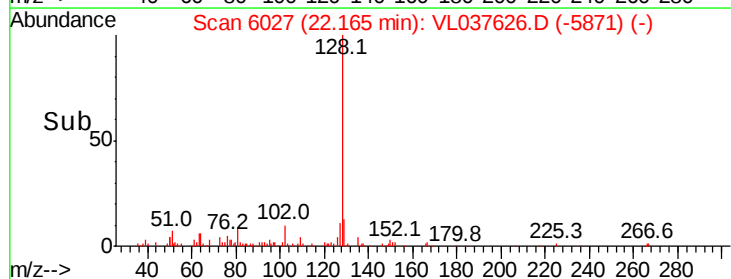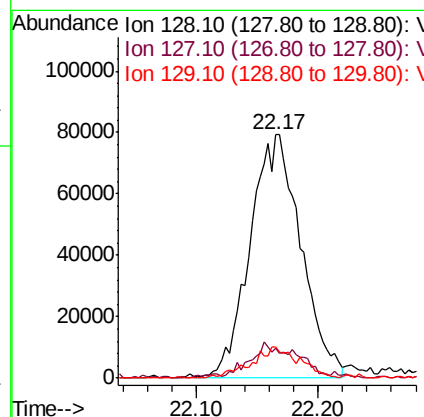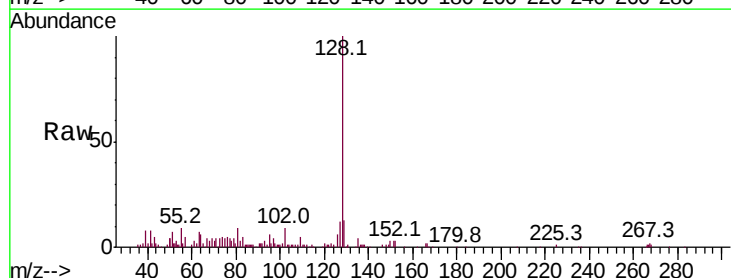

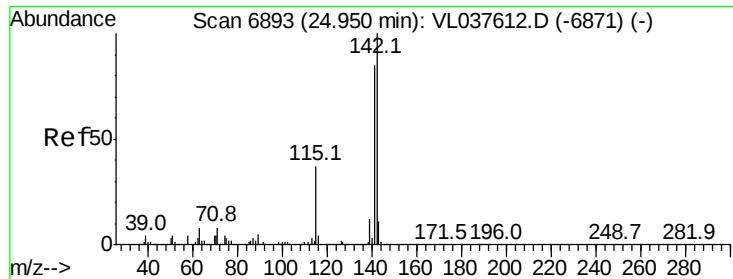

#80
 Naphthalene, 2-methyl-
 Concen: 0.430 ppbv m
 RT: 24.95 min Scan# 6892
 Delta R.T. -0.00 min
 Lab File: VL037626.D
 Acq: 16 Sep 2021 22:05

Instrument :
 MSVOA_L
 ClientSampleId :
 IA1

Tot Ion	Ratio	Lower	Upper
142	100		
141	47.5	70.9	106.3#
115	21.8	29.6	44.4#

Manual Integrations
 APPROVED

MMDadoda
 9/20/2021 5:27:24 PM

