

Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL091621\
 Data File : VL037635.D
 Acq On : 17 Sep 2021 3:52
 Operator : SY/AP
 Sample : VIBLK
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VIBLK

Manual Integrations
 APPROVED

MMDadoda
 9/20/2021 5:27:43 PM

Quant Time: Sep 17 07:00:44 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL091621AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Sep 17 07:00:44 2021
 QLast Update : Thu Sep 16 13:42:46 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.65	49	1534679	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.16	114	4354463	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.06	117	3723530	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.39	95	2525221	9.38	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	93.80%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Ethanol	3.61	45	41287m	4.134	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL091621\
Data File : VL037635.D
Acq On : 17 Sep 2021 3:52
Operator : SY/AP
Sample : VIBLK
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Manual Integrations
APPROVED

MMDadoda
9/20/2021 5:27:43 PM

Quant Time: Sep 17 07:00:44 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL091621AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Sep
QLast Update : Thu Sep 16 13:42:46 2021
Response via : Initial Calibration

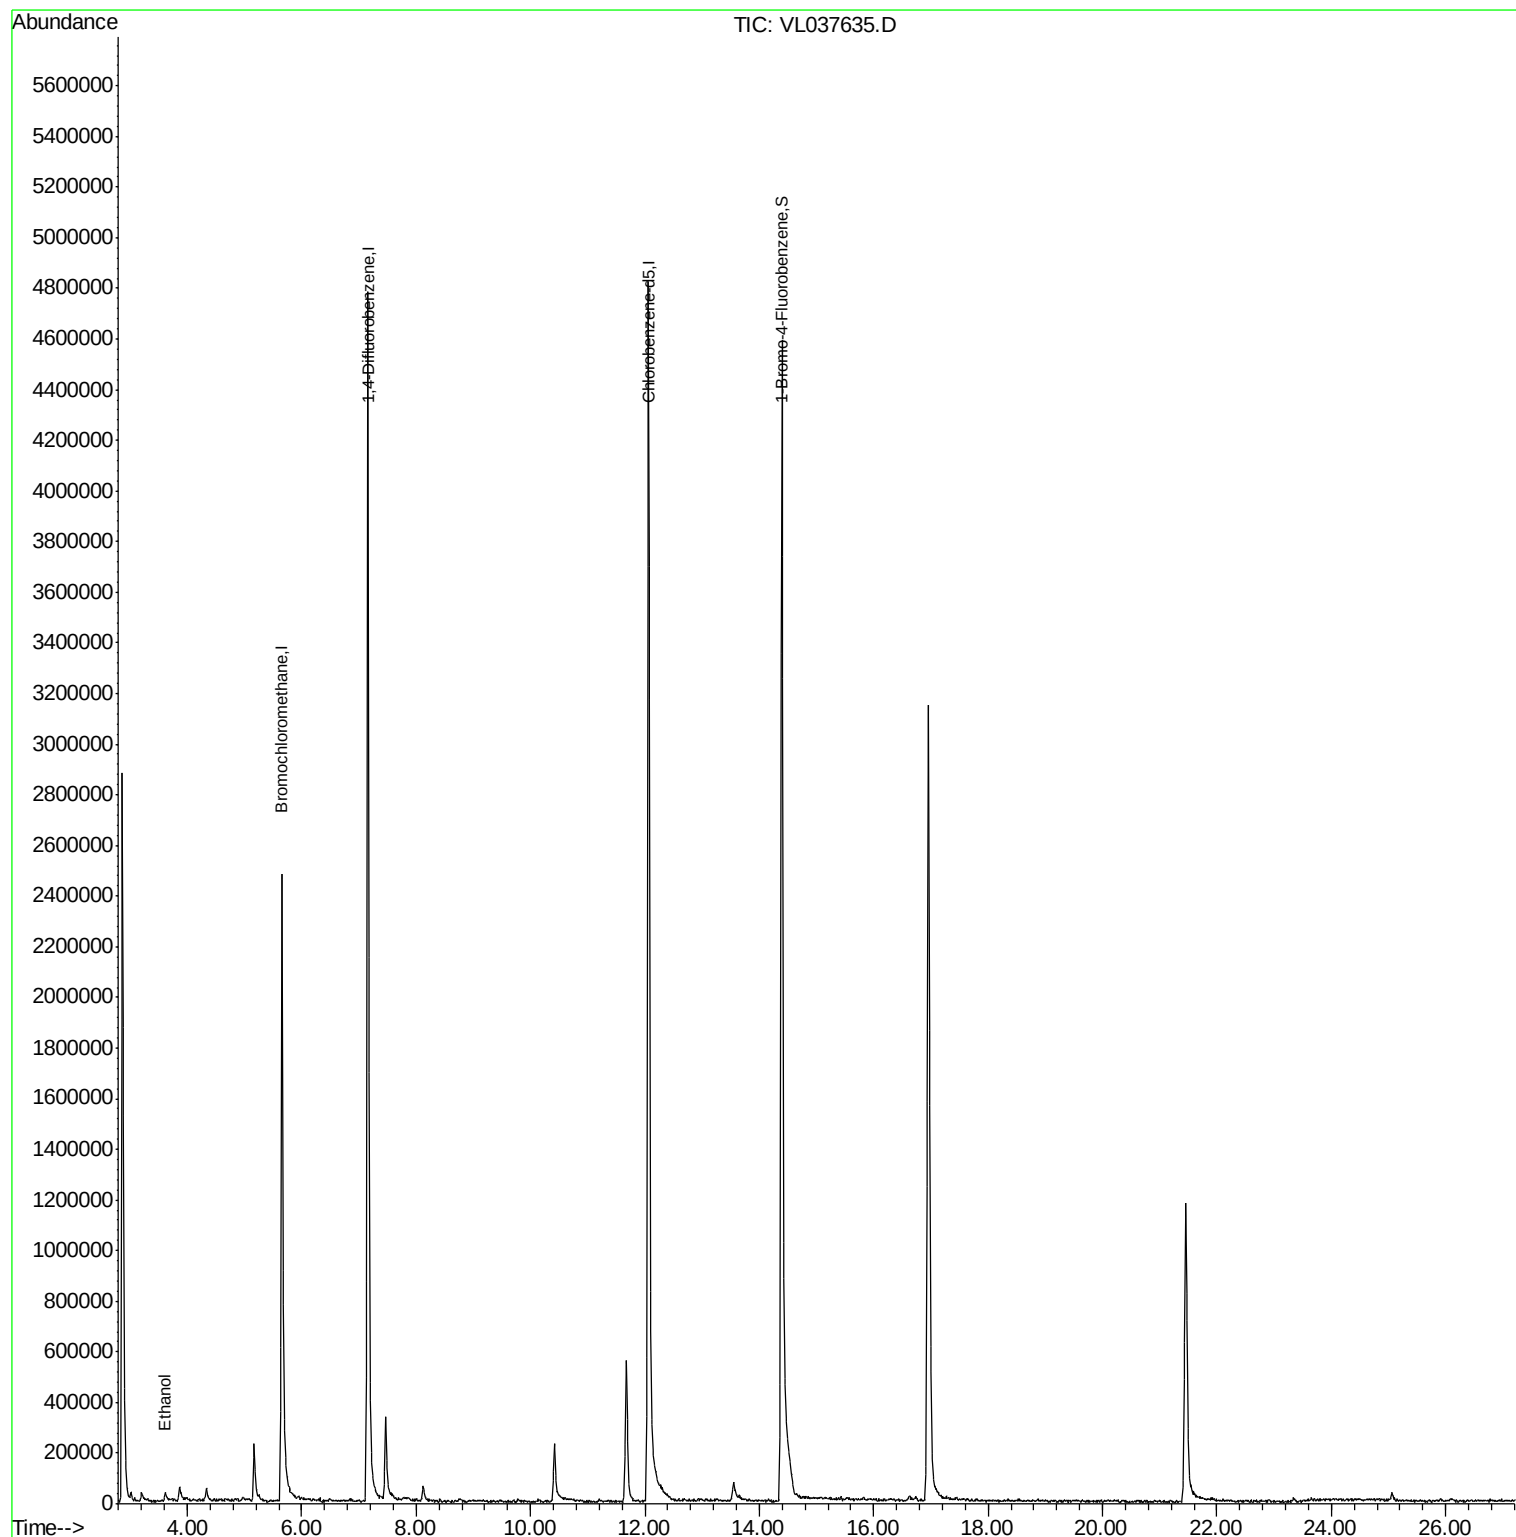

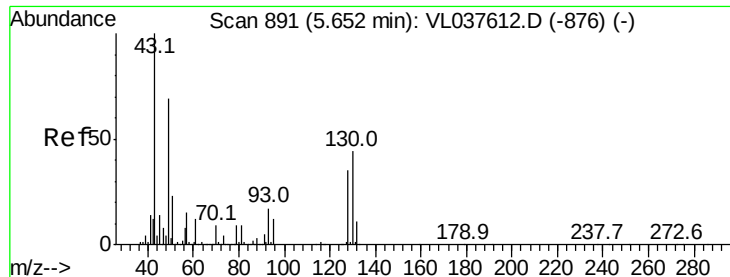

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.65 min Scan# 891

Delta R.T. 0.00 min

Lab File: VL037635.D

Acq: 17 Sep 2021 3:52

Instrument :

MSVOA_L

ClientSampled :

VIBLK

Tot Ion: 49 Resp: 1534679

Ion Ratio Lower Upper

49 100


128 51.6 27.9 83.6

130 68.2 33.9 101.7

Manual Integrations
APPROVED

MMDadoda




9/20/2021 5:27:43 PM

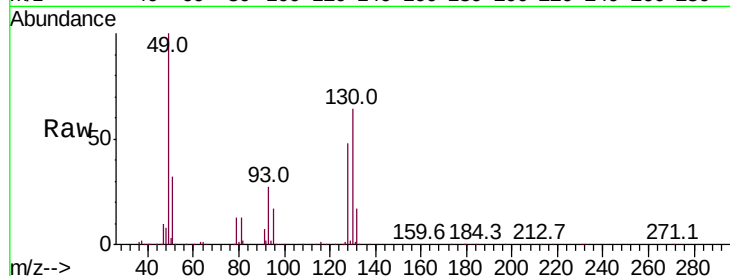

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

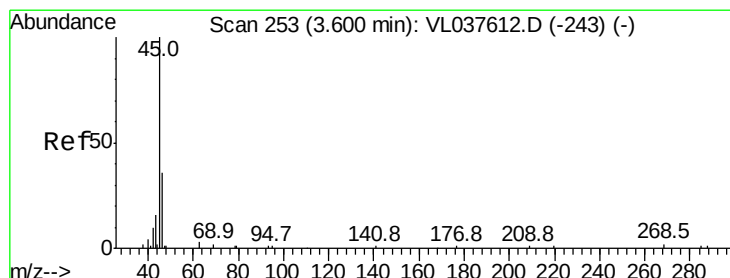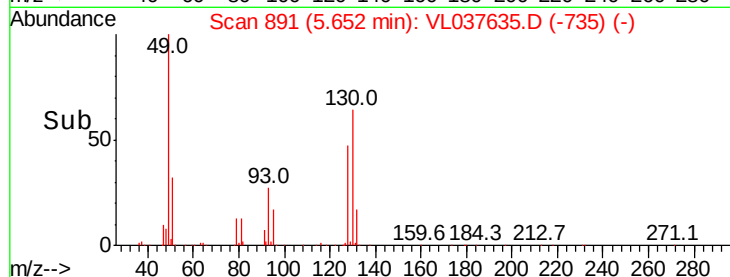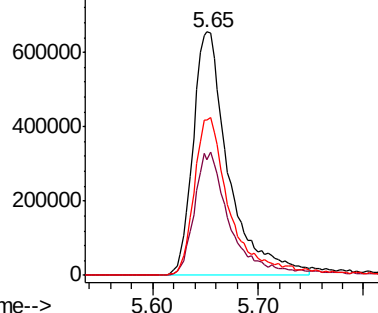

#13

Ethanol

Concen: 4.134 ppbv m

RT: 3.61 min Scan# 256

Delta R.T. 0.01 min

Lab File: VL037635.D


Acq: 17 Sep 2021 3:52

Tgt Ion: 45 Resp: 41287

Ion Ratio Lower Upper



45 100


46 0.0 17.2 68.8#

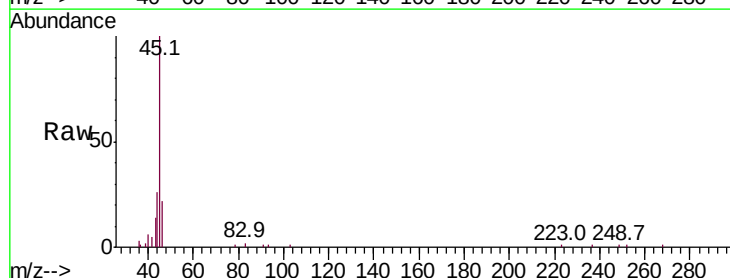

Abundance Ion 45.10 (44.80 to 45.80): VL0

Ion 46.10 (45.80 to 46.80): VL0

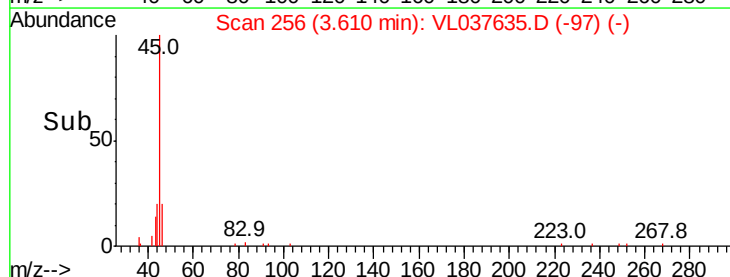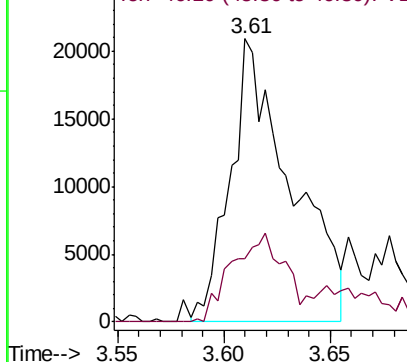

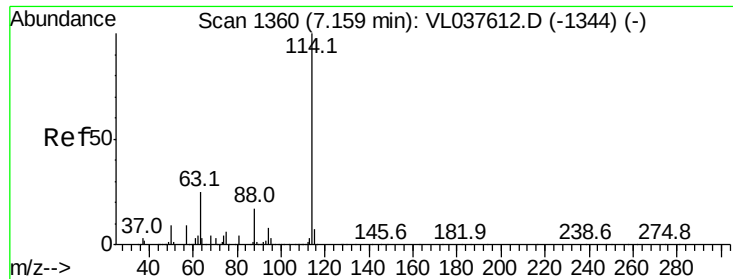





#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.16 min Scan# 1359
 Delta R.T. -0.00 min
 Lab File: VL037635.D
 Acq: 17 Sep 2021 3:52

Instrument :
 MSVOA_L
 ClientSampled :
 VIBLK

Tot Ion:114 Resp: 4354463
 Ion Ratio Lower Upper
 114 100
 63 24.0 19.6 29.4
 88 17.9 14.2 21.4




Manual Integrations
 APPROVED


MMDadoda
 9/20/2021 5:27:43 PM

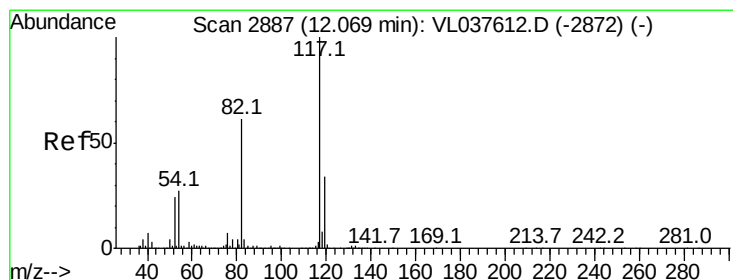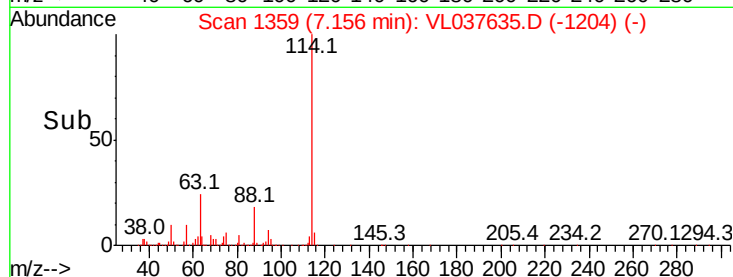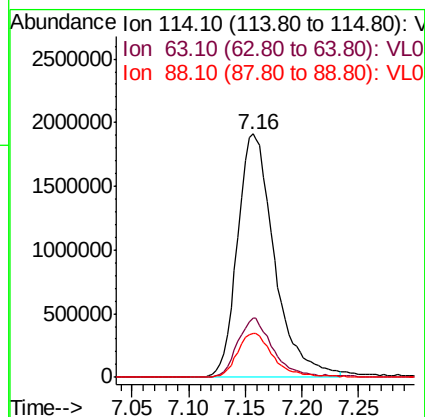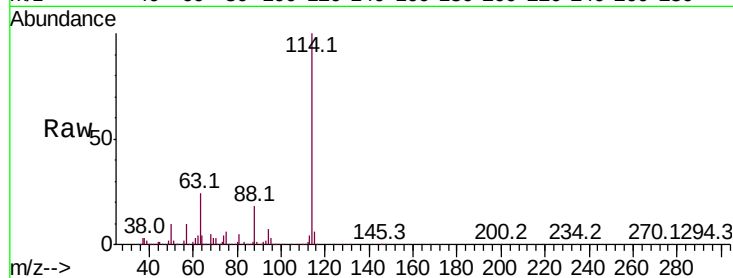

#55
 Chlorobenzene-d5
 Concen: 10.000 ppbv
 RT: 12.06 min Scan# 2885
 Delta R.T. -0.01 min
 Lab File: VL037635.D
 Acq: 17 Sep 2021 3:52

Tgt Ion:117 Resp: 3723530
 Ion Ratio Lower Upper
 117 100
 82 65.0 50.6 75.8
 119 33.7 26.2 39.2

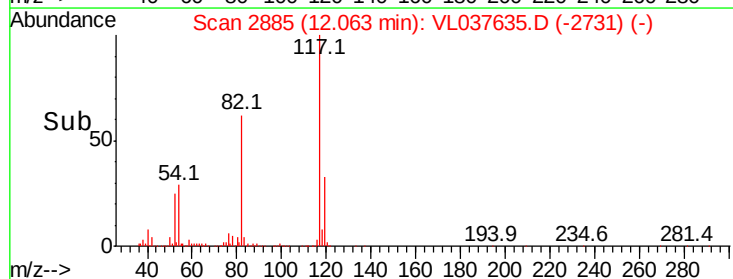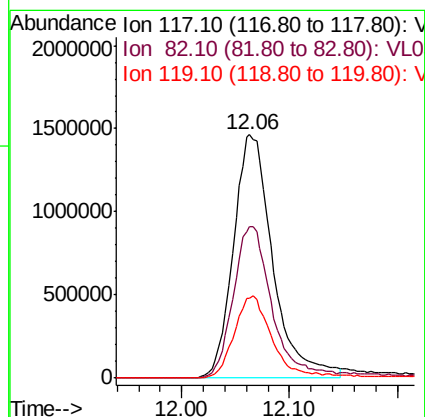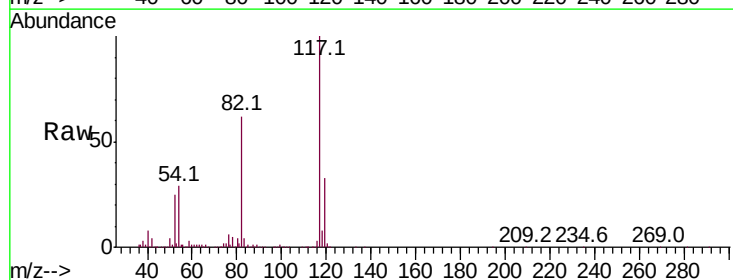

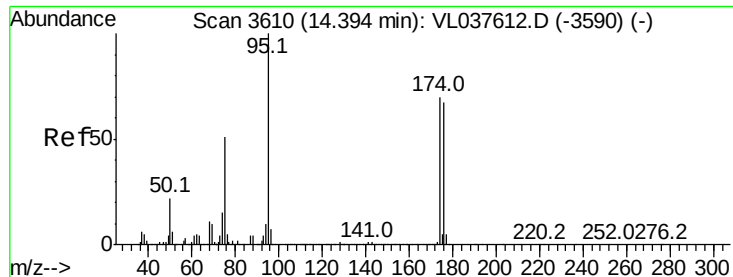

#68

1-Bromo-4-Fluorobenzene

Concen: 9.384 ppbv

RT: 14.39 min Scan# 3609

Delta R.T. -0.00 min

Lab File: VL037635.D

Acq: 17 Sep 2021 3:52

Instrument :

MSVOA_L

ClientSampleId :

VIBLK

Tot Ion: 95 Resp: 2525221

Ion Ratio Lower Upper

95 100

174 79.8 56.3 84.5

175 5.9 4.4 6.6

Manual Integrations
APPROVED

MMDadoda

9/20/2021 5:27:43 PM

