


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL091621\
 Data File : VL037609.D
 Acq On : 16 Sep 2021 8:10
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL091621AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Aug 17 02:13:47 2021
 Last Update : Tue Aug 17 02:13:47 2021

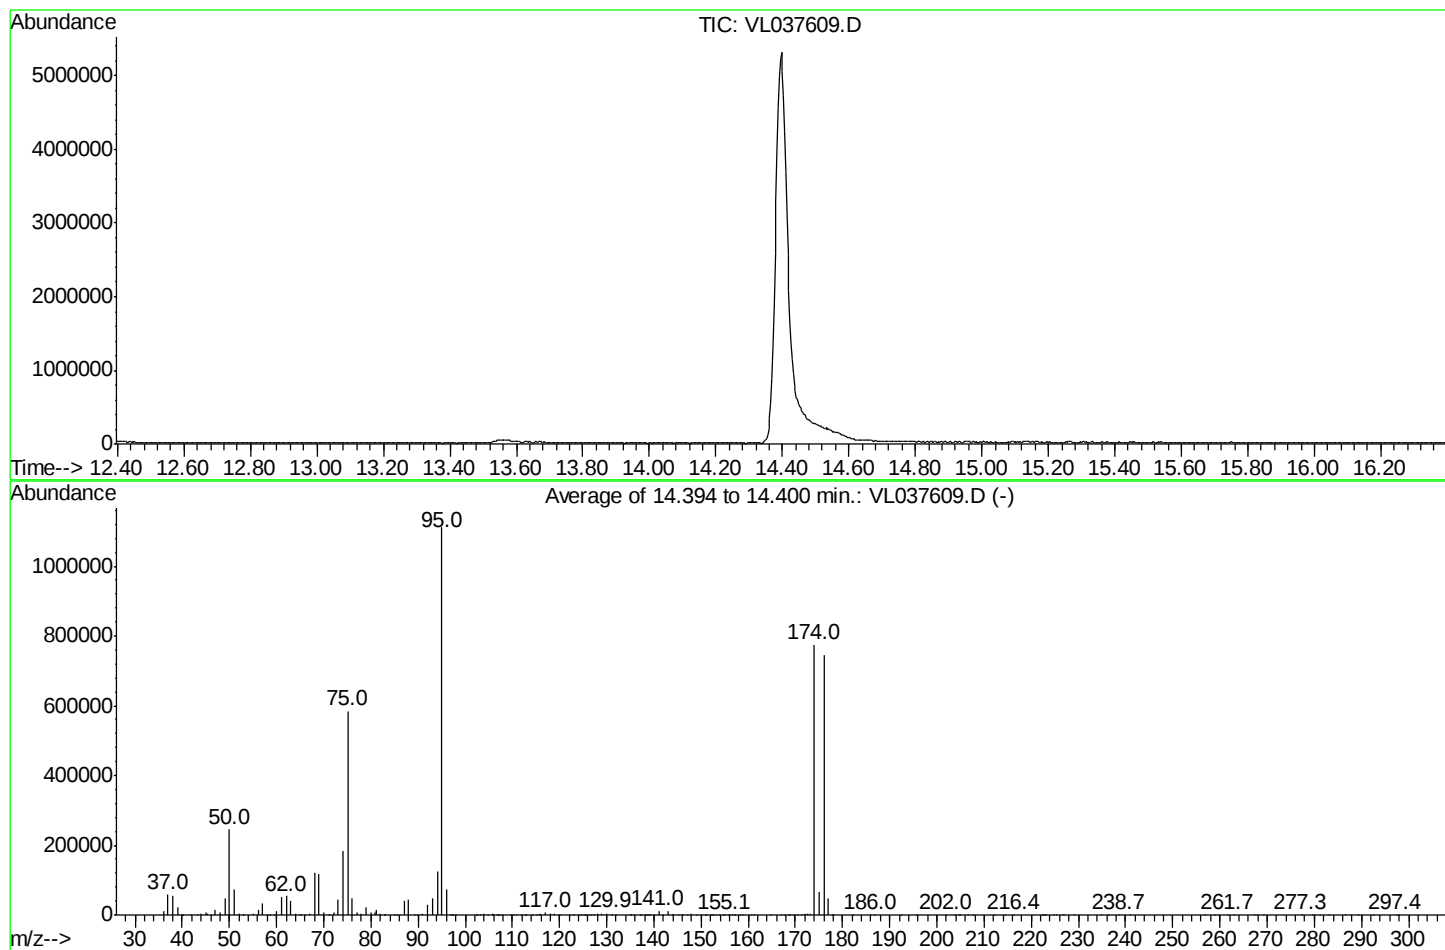

AutoFind: Scans 3610, 3611, 3612; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.0	244416	PASS
75	95	30	66	52.6	584459	PASS
95	95	100	100	100.0	1111535	PASS
96	95	5	9	6.5	72768	PASS
173	174	0.00	2	0.5	3827	PASS
174	95	50	120	69.7	774762	PASS
175	174	4	9	8.4	65141	PASS
176	174	93	101	96.0	743424	PASS
177	176	5	9	6.7	49472	PASS