


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL091624\
Data File : VL041590.D
Acq On : 16 Sep 2024 11:50
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091624AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Sep 17 09:12:21 2024

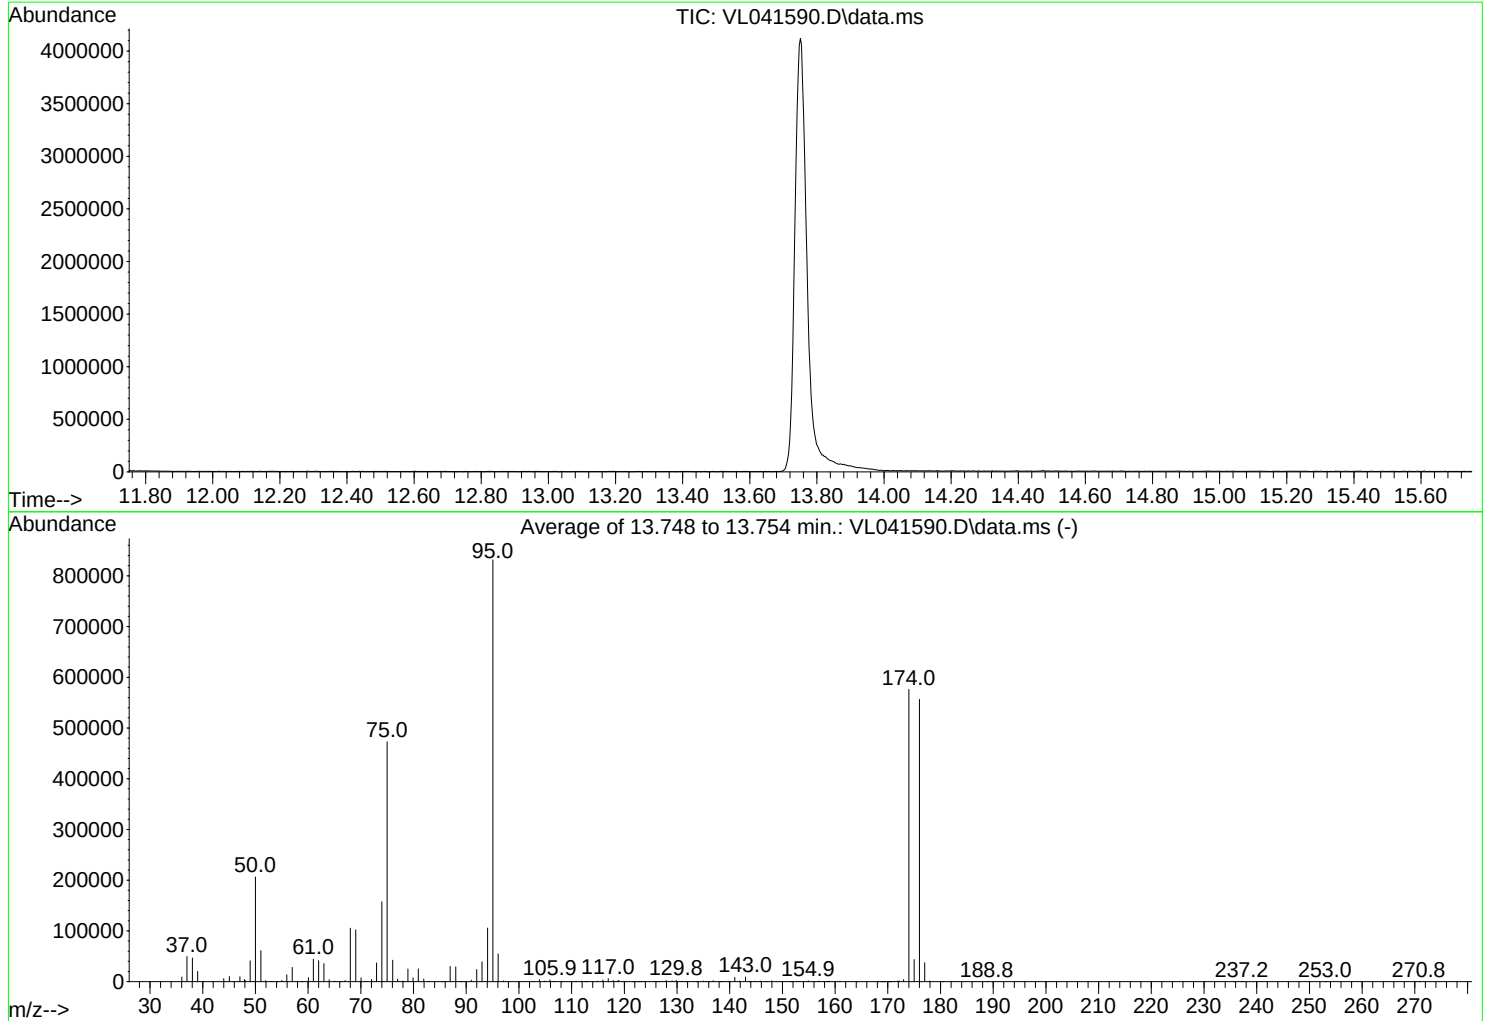

AutoFind: Scans 3466, 3467, 3468; Background Corrected with Scan 3441

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.8	206293	PASS
75	95	30	66	56.9	472747	PASS
95	95	100	100	100.0	831488	PASS
96	95	5	9	6.6	54749	PASS
173	174	0.00	2	0.7	4144	PASS
174	95	50	120	69.3	576085	PASS
175	174	4	9	7.6	43507	PASS
176	174	93	101	96.6	556480	PASS
177	176	5	9	6.7	37259	PASS

Average of 13.748 to 13.754 min.: VL041590.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	9207	46.10	369	55.00	2651	66.10	81
37.00	49400	47.05	9650	55.95	13635	67.00	232
38.05	46728	47.90	4268	57.00	28243	68.00	10530
39.05	20227	48.10	1922	57.95	1076	69.05	10224
40.00	228	49.00	40888	58.75	129	70.05	7554
40.20	436	50.00	206293	60.05	7800	70.95	358
41.80	87	51.05	61229	61.00	44059	72.05	4510
43.05	384	51.95	2027	62.00	41221	73.00	37035
44.00	6083	52.95	329	63.00	35685	74.00	157525
45.05	10009	53.20	312	64.00	3766	75.00	472747
45.80	242	54.10	88	65.05	1292	76.05	42211

Average of 13.748 to 13.754 min.: VL041590.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.00	4985	86.95	30088	102.95	369	112.60	101
77.85	1423	88.00	29163	103.90	3676	112.80	508
78.10	794	89.00	175	104.85	1192	113.05	589
78.95	25048	90.95	3086	105.90	3478	114.90	946
79.90	7463	92.00	24155	106.60	229	115.95	3195
80.90	25109	93.00	39075	106.85	796	116.95	5866
81.95	5309	94.05	105645	108.10	92	117.90	2520
82.95	1070	95.05	831488	109.65	267	118.80	1552
84.05	215	96.05	54749	110.75	616	118.95	2669
85.40	55	97.05	1690	110.95	514	119.90	58
86.00	788	102.65	275	111.85	847	121.65	136

Average of 13.748 to 13.754 min.: VL041590.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
121.90	65	129.85	2699	138.85	449	147.95	1706
122.70	109	130.80	691	139.70	662	148.90	437
123.10	69	131.10	409	140.95	8442	149.85	521
123.70	267	131.70	68	141.85	1166	151.60	184
124.10	231	133.70	174	143.00	9120	151.90	326
124.80	399	133.90	233	143.70	185	152.70	619
125.75	264	134.95	1333	144.05	403	153.10	590
126.10	144	135.60	260	144.85	950	153.85	364
126.70	226	136.00	79	145.80	1198	154.90	1517
127.95	2506	136.85	1801	146.90	410	156.00	398
129.05	1755	138.20	75	147.10	220	156.95	1253

Average of 13.748 to 13.754 min.: VL041590.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.85	315	170.90	339	188.80	87		
158.50	132	171.20	298	235.60	53		
158.90	926	171.85	1361	237.20	61		
160.90	1115	172.15	1652	253.00	80		
164.10	69	173.00	4144	270.80	112		
168.10	88	174.00	576085				
168.70	68	175.00	43507				
169.00	143	176.00	556480				
169.30	102	177.00	37259				
170.10	52	177.90	1144				
170.40	90	180.40	139				