

Data File : VL034184.D
Acq On : 18 Sep 2019 14:39
Operator : SY/AP
Sample : VSTDCCC010
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDCCC010

Quant Time: Sep 19 06:47:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL091719AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Sep 18 12:53:31 2019
QLast Update : Wed Sep 18 12:53:31 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.70	49	1181758	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.22	114	2043178	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.16	117	2231487	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.50	95	1876105	9.68	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	96.80%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	3.03	85	1408964	8.072	ppbv	99
3) Chlorodifluoromethane	2.97	51	1306363	9.428	ppbv	100
4) Chloromethane	3.13	50	783338	9.620	ppbv	92
5) Vinyl Chloride	3.25	62	693459	9.319	ppbv	96
6) Bromomethane	3.47	94	329271	9.484	ppbv	97
7) Chloroethane	3.55	64	245574	9.442	ppbv #	87
8) Dichlorotetrafluoroethane	3.18	85	1429679	9.280	ppbv	99
9) Propene	3.00	41	647303	9.469	ppbv	100
10) Heptane	8.18	43	1710831	9.602	ppbv	100
11) Trichlorofluoromethane	3.95	101	1514120	9.529	ppbv	98
12) 1,1,2-Trichlorotrifluoroet	4.49	101	990391	9.524	ppbv	99
13) Ethanol	3.60	45	143302	8.657	ppbv	96
14) Bromoethene	3.74	108	425008	9.997	ppbv	99
15) Acetone	3.85	43	1294888	8.175	ppbv	100
16) 1,3-Butadiene	3.32	39	689268	9.972	ppbv	98
17) tert-Butyl alcohol	4.30	59	1119714	11.157	ppbv	100
18) 1,1-Dichloroethene	4.30	96	445437	9.821	ppbv	91
19) Isopropyl Alcohol	3.97	45	1039793	10.676	ppbv	100
20) Methylene Chloride	4.35	84	400590	8.772	ppbv	98
21) Allyl Chloride	4.42	41	905610	10.123	ppbv	99
22) trans-1,2-Dichloroethene	4.90	96	451572	9.951	ppbv	98
23) Vinyl Acetate	5.10	43	2241373	9.603	ppbv	99
24) 1,1-Dichloroethane	5.03	63	1475832	9.391	ppbv	99
25) Ethyl Acetate	5.71	43	2734692	9.131	ppbv	100
26) Hexane	5.72	57	1149632	9.227	ppbv	99
27) Carbon Disulfide	4.56	76	1234718	10.746	ppbv	100
28) Methyl tert-Butyl Ether	5.05	73	1763350	9.530	ppbv	100
29) Chloroform	5.79	83	1723260	9.679	ppbv	99
30) Cyclohexane	7.18	84	871839	9.693	ppbv	99
31) cis-1,2-Dichloroethene	5.58	61	1251566	9.854	ppbv	99
32) 1,1,1-Trichloroethane	6.56	97	1642082	9.564	ppbv	99
34) 2-Butanone	5.27	43	1937007	9.285	ppbv	99
35) Carbon Tetrachloride	7.07	117	1633296	9.622	ppbv	99
36) Benzene	6.94	78	2093777	9.279	ppbv	100
37) 1,2-Dichloroethane	6.35	62	1560767	9.724	ppbv	100
38) Trichloroethene	7.89	130	705019	8.744	ppbv	98
39) 1,2-Dichloropropane	7.67	63	942067	9.292	ppbv	98
40) 1,4-Dioxane	7.88	88	319605	9.741	ppbv #	92
41) Tetrahydrofuran	6.08	42	1167985	9.940	ppbv	99
42) Bromodichloromethane	7.85	83	1899299	9.860	ppbv	100
43) Methyl Methacrylate	8.07	69	947849	10.168	ppbv	99

Data File : VL034184.D
Acq On : 18 Sep 2019 14:39
Operator : SY/AP
Sample : VSTDCCC010
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDCCC010

Quant Time: Sep 19 06:47:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL091719AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Sep 18 12:53:31 2019
QLast Update : Wed Sep 18 12:53:31 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 2,2,4-Trimethylpentane	7.92	57	3918320	9.020	ppbv	100
45) t-1,3-Dichloropropene	9.34	75	1243739	11.284	ppbv	95
46) cis-1,3-Dichloropropene	8.76	75	1391093	10.492	ppbv	96
47) 1,1,2-Trichloroethane	9.55	97	857176	9.415	ppbv	97
48) Dibromochloromethane	10.37	129	1421630	9.852	ppbv	99
49) Bromoform	13.13	173	1199470	10.272	ppbv	99
50) 4-Methyl-2-Pentanone	8.80	43	2843468	9.365	ppbv	98
51) 2-Hexanone	10.20	43	2448891	9.611	ppbv #	100
52) Tetrachloroethene	11.30	164	666001	8.933	ppbv	97
53) Toluene	9.87	91	2378162	9.643	ppbv	99
54) 1,2-Dibromoethane	10.69	107	1283265	9.478	ppbv	98
56) 1,1,1,2-Tetrachloroethane	12.20	131	914756	9.192	ppbv #	57
57) Chlorobenzene	12.22	112	1677142	8.632	ppbv	98
58) Ethyl Benzene	12.79	91	3224901	8.957	ppbv	100
59) m/p-Xylene	13.07	91	2511426	8.421	ppbv #	27
60) o-Xylene	13.77	91	2619198	8.783	ppbv	99
61) Styrene	13.61	104	1964997	9.199	ppbv	99
62) Isopropylbenzene	14.75	105	3381970	8.761	ppbv	99
63) 1,1,2,2-Tetrachloroethane	13.76	83	1941206	7.939	ppbv	99
64) n-propylbenzene	15.64	120	868551	8.893	ppbv	90
65) tert-Butylbenzene	16.83	119	2880787	8.541	ppbv	99
66) Benzyl Chloride	17.08	91	1445484	12.113	ppbv	99
67) sec-Butylbenzene	17.38	105	4169914	8.645	ppbv	100
69) p-Isopropyltoluene	17.74	119	3401876	8.710	ppbv	100
70) n-Butylbenzene	18.64	91	3882113	8.536	ppbv	99
71) 2-Chlorotoluene	15.54	91	2814302	8.923	ppbv	100
72) 4-Ethyltoluene	15.92	105	3022083	8.970	ppbv	100
73) 1,3,5-Trimethylbenzene	16.08	105	2889076	8.876	ppbv	97
74) 1,2,4-Trimethylbenzene	16.85	105	2915441	8.436	ppbv	93
75) 1,3-Dichlorobenzene	17.09	146	1596900	8.612	ppbv	99
76) 1,4-Dichlorobenzene	17.23	146	1616834	8.514	ppbv	99
77) 1,2-Dichlorobenzene	17.91	146	1594731	8.497	ppbv	100
78) Hexachloro-1,3-Butadiene	23.46	225	1188618	9.562	ppbv	98
79) Naphthalene	22.32	128	2647931	8.703	ppbv	95
80) Naphthalene,2-methyl-	25.05	142	1433983	10.135	ppbv	99
81) 1,2,4-Trichlorobenzene	22.04	180	1437502	8.529	ppbv	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VL034184.D
Acq On : 18 Sep 2019 14:39
Operator : SY/AP
Sample : VSTDCCC010
Misc : 400ml/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDCCC010

Quant Time: Sep 19 06:47:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL091719AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Sep 18 12:53:31 2019
QLast Update : Wed Sep 18 12:53:31 2019
Response via : Initial Calibration

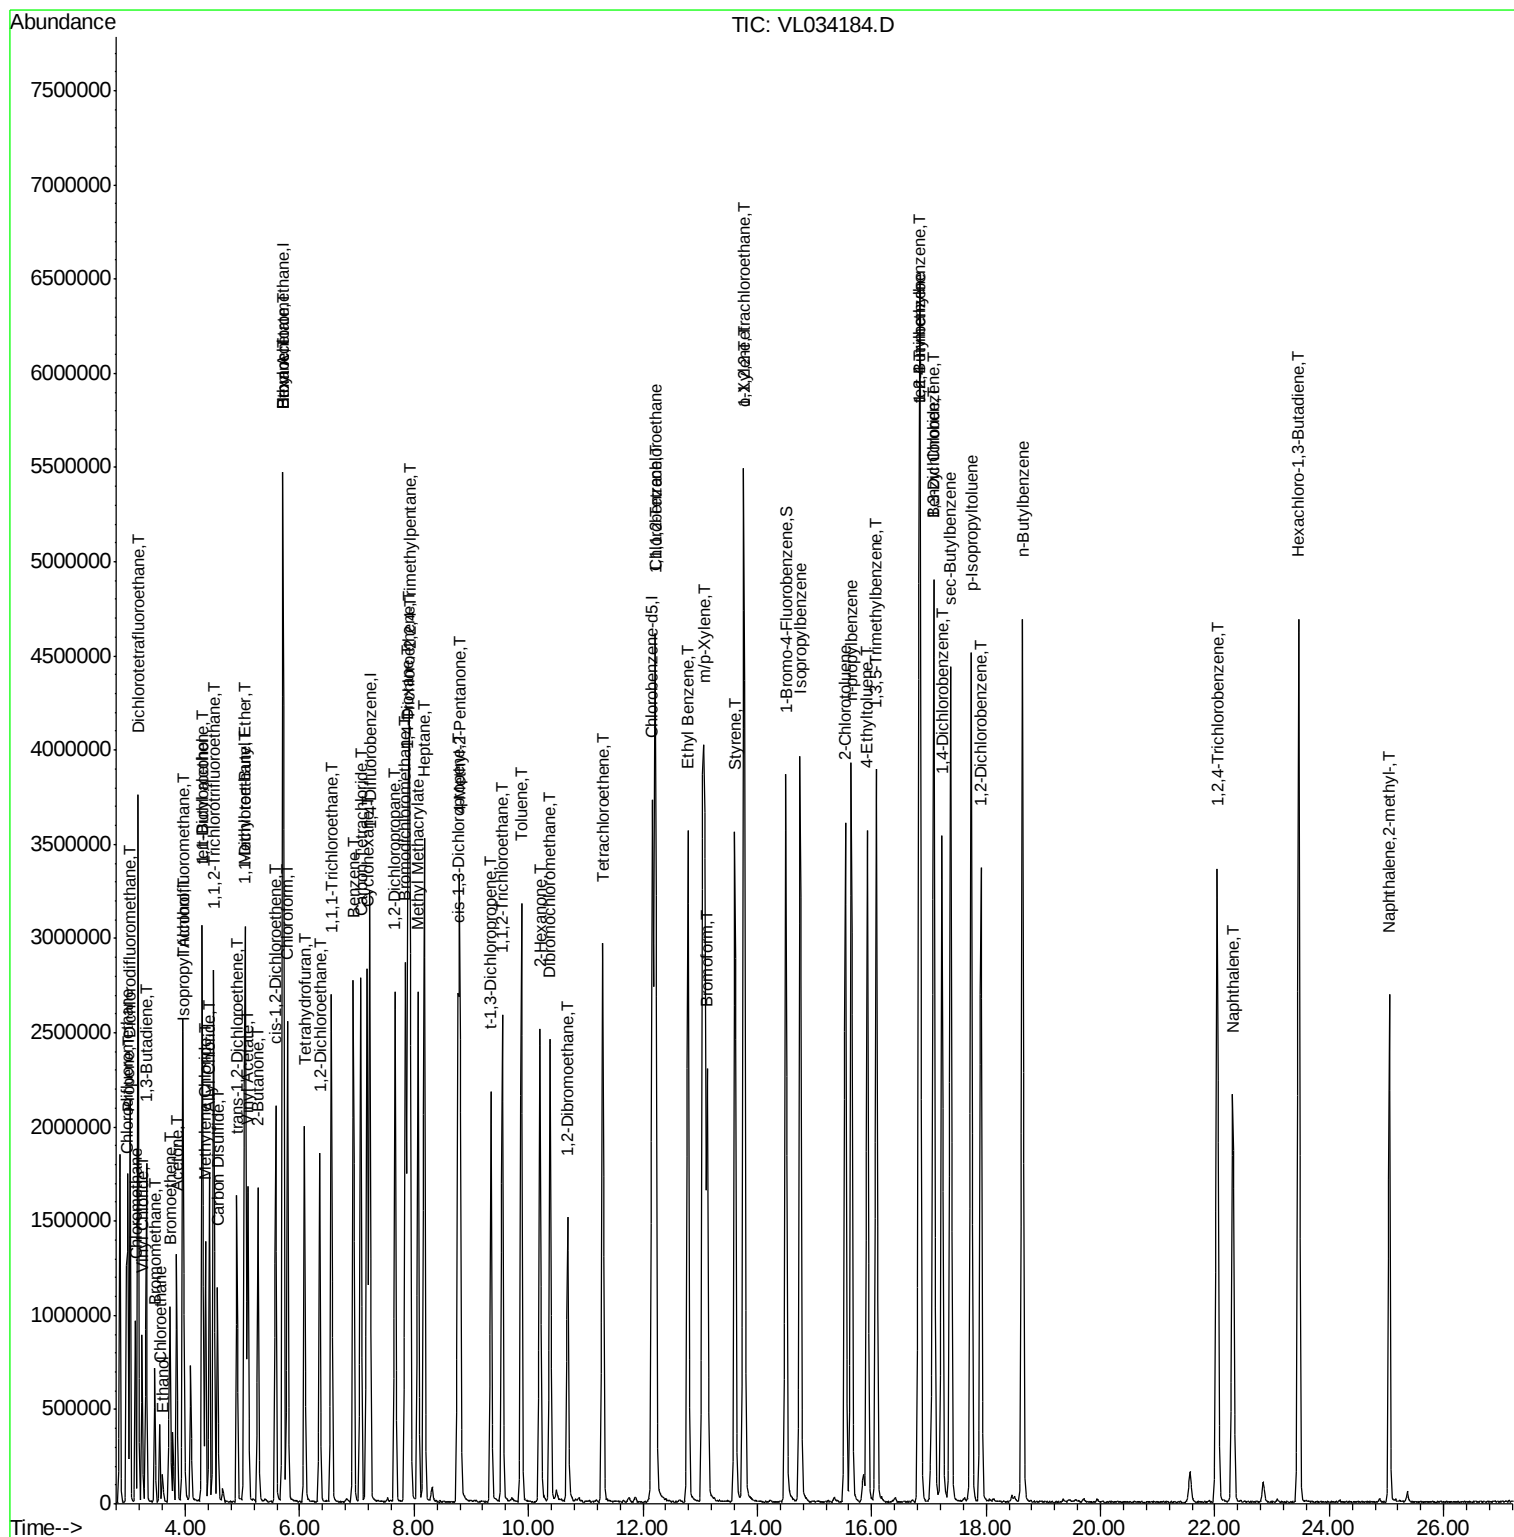



#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.70 min Scan# 906

Delta R.T. -0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :

VSTDCCC010


Tgt Ion: 49 Resp: 1181758

Ion Ratio Lower Upper

49 100

128 34.5 17.6 52.9




130 44.1 22.3 66.9

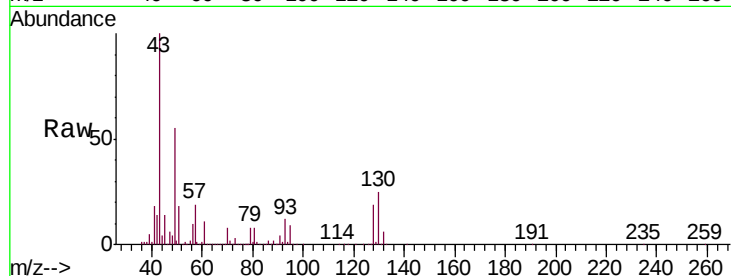

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

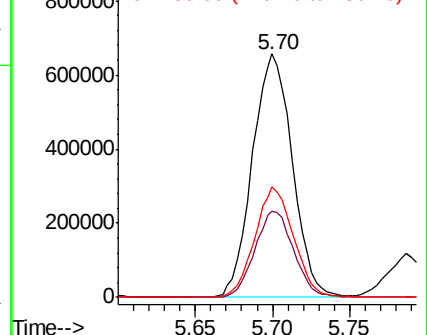

#2

Dichlorodifluoromethane

Concen: 8.072 ppbv

RT: 3.03 min Scan# 77

Delta R.T. 0.00 min

Lab File: VL034184.D


Acq: 18 Sep 2019 14:39

Tgt Ion: 85 Resp: 1408964

Ion Ratio Lower Upper



85 100


87 34.4 27.2 40.8



Abundance Ion 85.00 (84.70 to 85.70): VL0

Ion 87.00 (86.70 to 87.70): VL0

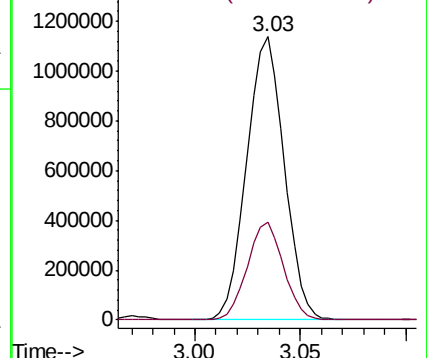



#3

Chlorodifluoromethane

Concen: 9.428 ppbv

RT: 2.97 min Scan# 57

Delta R.T. -0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :


VSTDCCC010

Tgt Ion: 51 Resp: 1306363

Ion Ratio Lower Upper




51 100

67 18.4 14.8 22.2

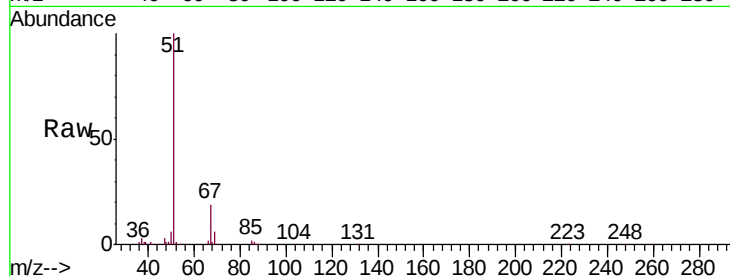

Abundance Ion 51.00 (50.70 to 51.70): VL0

Ion 67.00 (66.70 to 67.70): VL0

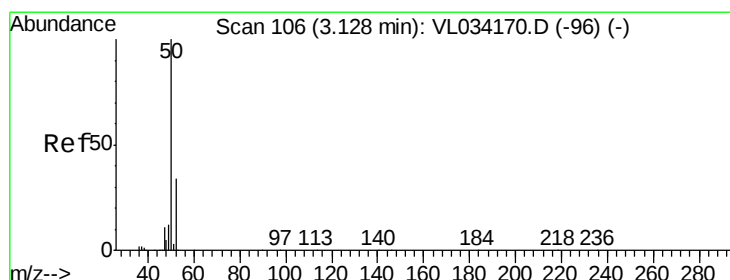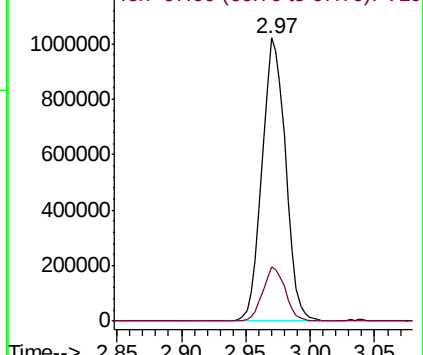

#4

Chloromethane

Concen: 9.620 ppbv

RT: 3.13 min Scan# 106

Delta R.T. 0.00 min

Lab File: VL034184.D


Acq: 18 Sep 2019 14:39

Tgt Ion: 50 Resp: 783338

Ion Ratio Lower Upper



50 100


52 29.5 27.1 40.7



Abundance Ion 50.10 (49.80 to 50.80): VL0

Ion 52.10 (51.80 to 52.80): VL0

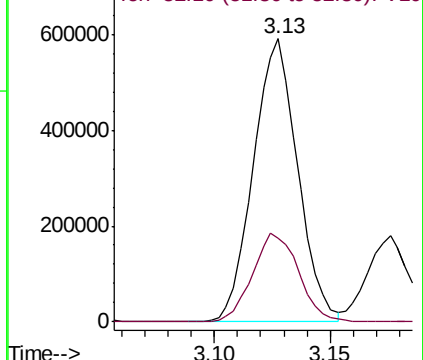



#5

Vinyl Chloride

Concen: 9.319 ppbv

RT: 3.25 min Scan# 143

Delta R.T. -0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :





VSTDCCC010

Tgt Ion: 62 Resp: 693459

Ion Ratio Lower Upper

62 100

64 33.5 25.2 37.8

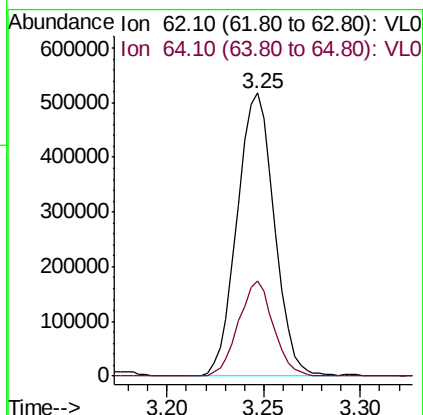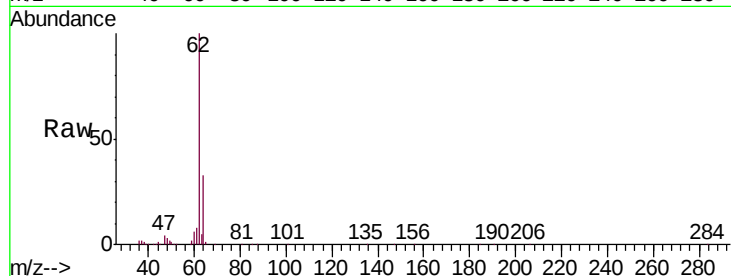

#6

Bromomethane

Concen: 9.484 ppbv

RT: 3.47 min Scan# 211

Delta R.T. -0.00 min

Lab File: VL034184.D




Acq: 18 Sep 2019 14:39


Tgt Ion: 94 Resp: 329271

Ion Ratio Lower Upper

94 100

96 92.3 71.3 106.9

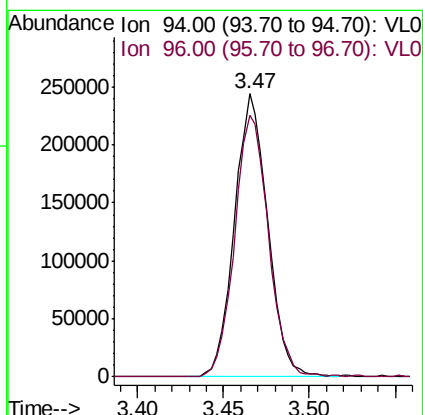



#7

Chloroethane

Concen: 9.442 ppbv

RT: 3.55 min Scan# 238

Delta R.T. -0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :





VSTDCCC010

Tgt Ion: 64 Resp: 245574

Ion Ratio Lower Upper

64 100

66 37.5 24.2 36.4#

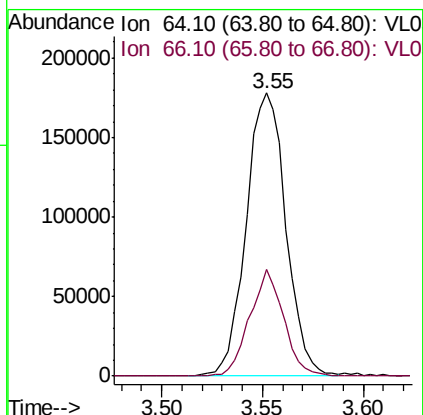

#8

Dichlorotetrafluoroethane

Concen: 9.280 ppbv

RT: 3.18 min Scan# 121

Delta R.T. -0.00 min

Lab File: VL034184.D




Acq: 18 Sep 2019 14:39


Tgt Ion: 85 Resp: 1429679

Ion Ratio Lower Upper

85 100

135 58.1 47.3 70.9

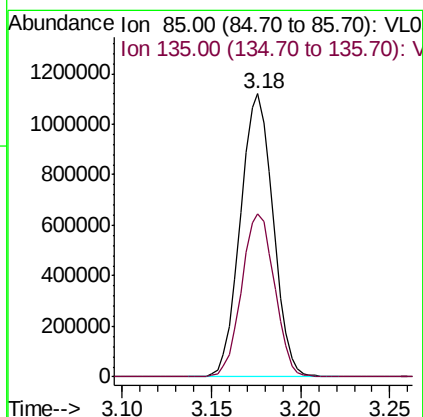



#9

Propene

Concen: 9.469 ppbv

RT: 3.00 min Scan# 65

Delta R.T. 0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :





VSTDCCC010

Tgt Ion: 41 Resp: 647303

Ion Ratio Lower Upper

41 100

42 69.8 55.8 83.6

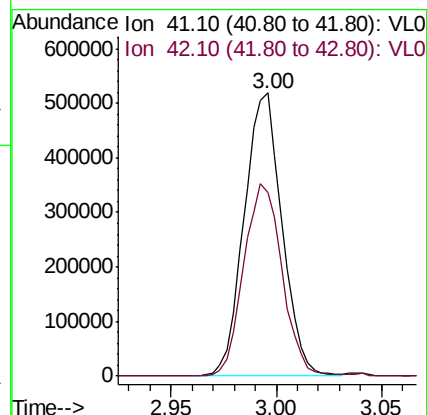

#10

Heptane

Concen: 9.602 ppbv

RT: 8.18 min Scan# 1676

Delta R.T. -0.01 min

Lab File: VL034184.D




Acq: 18 Sep 2019 14:39


Tgt Ion: 43 Resp: 1710831

Ion Ratio Lower Upper

43 100

57 46.9 37.5 56.3



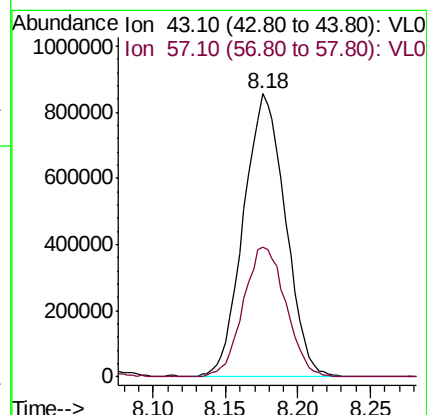





#11
 Trichlorofluoromethane
 Concen: 9.529 ppbv
 RT: 3.95 min Scan# 362
 Delta R.T. -0.01 min
 Lab File: VL034184.D
 Acq: 18 Sep 2019 14:39




Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010


Tgt Ion:101 Resp: 1514120
 Ion Ratio Lower Upper
 101 100
 103 66.8 52.1 78.1

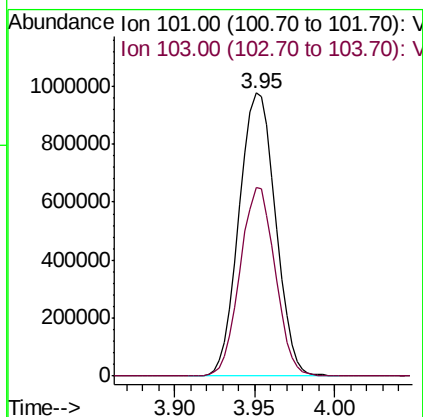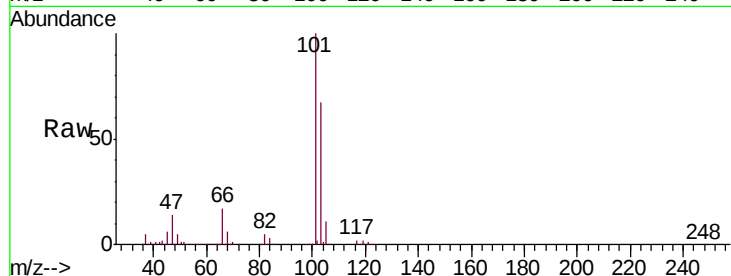

#12
 1,1,2-Trichlorotrifluoroethane
 Concen: 9.524 ppbv
 RT: 4.49 min Scan# 531
 Delta R.T. -0.00 min
 Lab File: VL034184.D
 Acq: 18 Sep 2019 14:39

Tgt Ion:101 Resp: 990391
 Ion Ratio Lower Upper
 101 100
 151 64.2 51.8 77.8

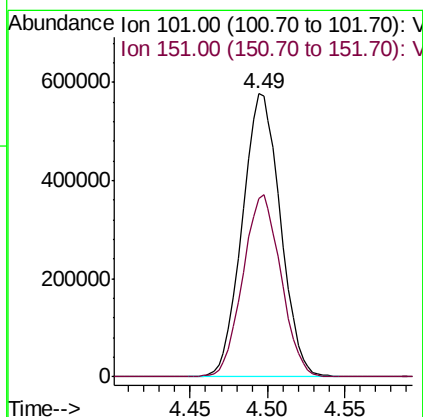



#13

Ethanol

Concen: 8.657 ppbv

RT: 3.60 min Scan# 254

Delta R.T. 0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :





VSTDCCC010

Tgt Ion: 45 Resp: 143302

Ion Ratio Lower Upper

45 100

46 36.1 15.5 61.9

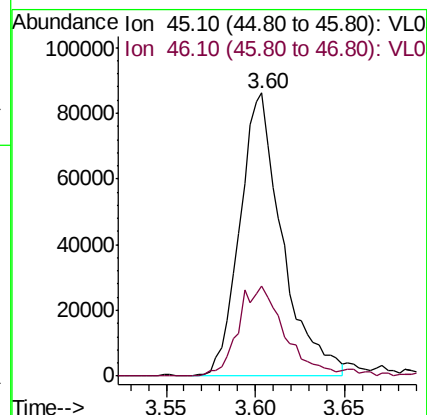

#14

Bromoethene

Concen: 9.997 ppbv

RT: 3.74 min Scan# 296

Delta R.T. 0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39




Tgt Ion: 108 Resp: 425008


Ion Ratio Lower Upper

108 100

106 108.9 86.2 129.4

79 22.7 18.6 27.8

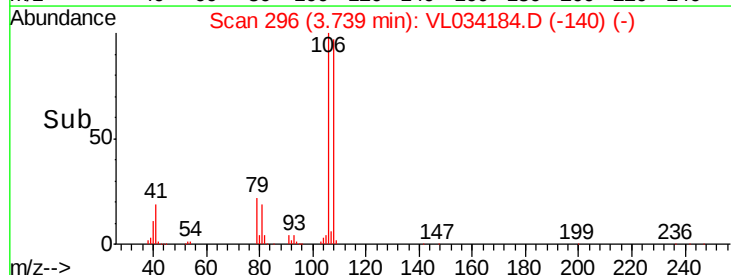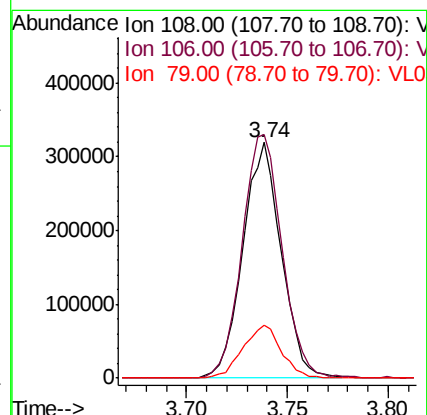



#15

Acetone

Concen: 8.175 ppbv

RT: 3.85 min Scan# 331

Delta R.T. 0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :





VSTDCCC010

Tgt Ion: 43 Resp: 1294888

Ion Ratio Lower Upper

43 100

58 25.7 20.5 30.7

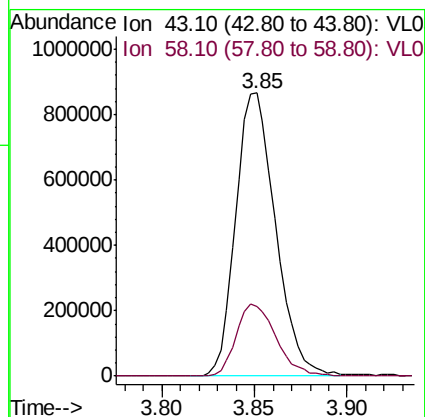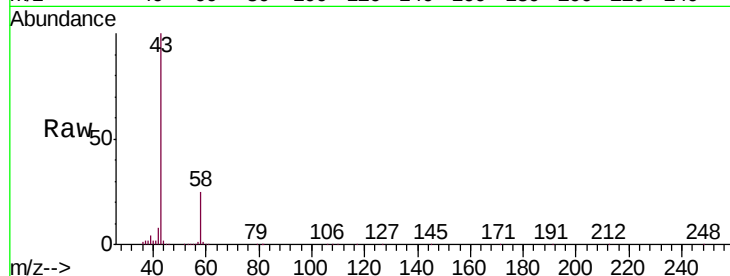

#16

1,3-Butadiene

Concen: 9.972 ppbv

RT: 3.32 min Scan# 165

Delta R.T. -0.00 min

Lab File: VL034184.D




Acq: 18 Sep 2019 14:39


Tgt Ion: 39 Resp: 689268

Ion Ratio Lower Upper

39 100

54 77.6 63.4 95.0

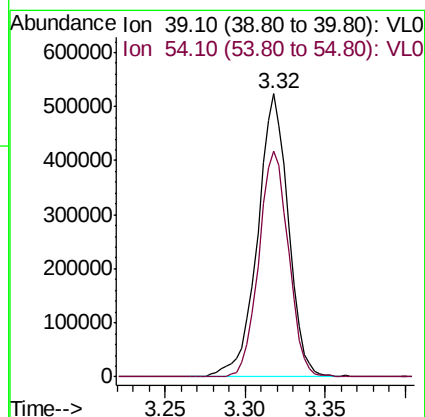

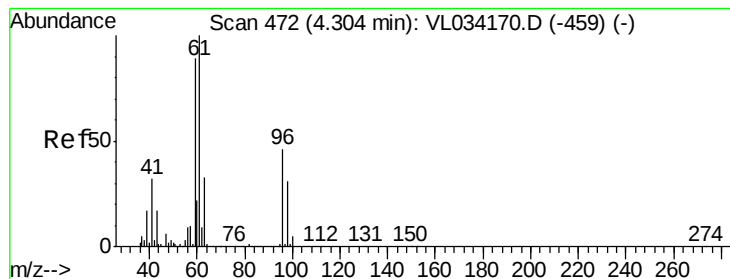

#17

tert-Butyl alcohol

Concen: 11.157 ppbv

RT: 4.30 min Scan# 470

Delta R.T. -0.01 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :


VSTDCCC010

Tgt Ion: 59 Resp: 1119714

Ion Ratio Lower Upper

59 100

57 10.9 8.7 13.1



Abundance Ion 59.10 (58.80 to 59.80): VL0

Ion 57.10 (56.80 to 57.80): VL0

4.30



600000

400000

200000

0

Time-->

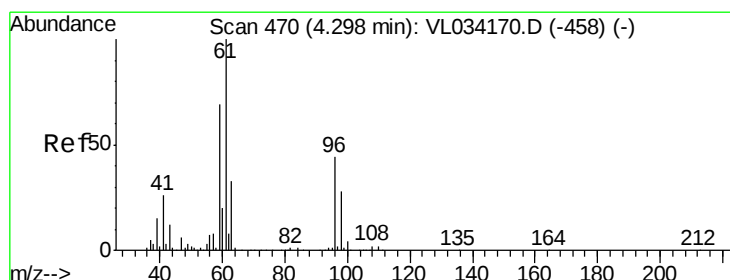

#18

1,1-Dichloroethene

Concen: 9.821 ppbv

RT: 4.30 min Scan# 470

Delta R.T. 0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39


Tgt Ion: 96 Resp: 445437

Ion Ratio Lower Upper

96 100

61 211.5 183.3 274.9

98 63.4 51.4 77.2



Abundance Ion 96.00 (95.70 to 96.70): VL0

Ion 61.10 (60.80 to 61.80): VL0

Ion 98.00 (97.70 to 98.70): VL0

800000


600000


400000

200000

0

Time-->









#19

Isopropyl Alcohol
 Concen: 10.676 ppbv
 RT: 3.97 min Scan# 368
 Delta R.T. 0.00 min
 Lab File: VL034184.D
 Acq: 18 Sep 2019 14:39

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010




Tgt Ion: 45 Resp: 1039793
 Ion Ratio Lower Upper
 45 100
 58 1.7 1.4 2.0

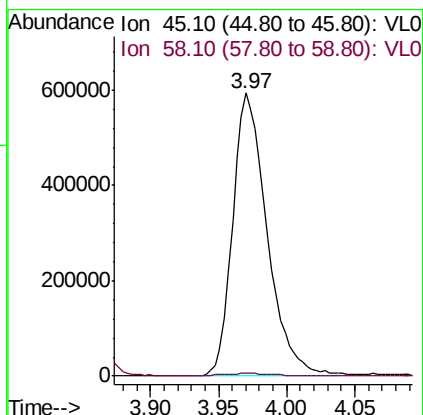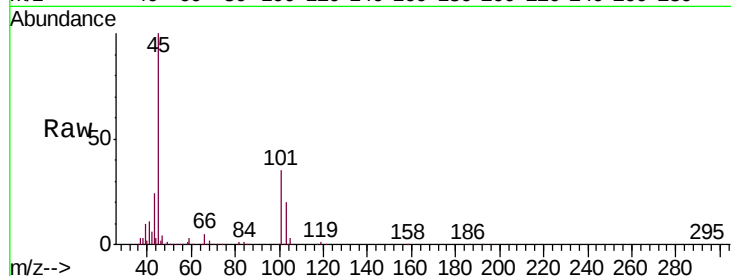


#20

Methylene Chloride
 Concen: 8.772 ppbv
 RT: 4.35 min Scan# 487
 Delta R.T. -0.00 min
 Lab File: VL034184.D
 Acq: 18 Sep 2019 14:39

Tgt Ion: 84 Resp: 400590
 Ion Ratio Lower Upper
 84 100
 49 168.1 133.8 200.8
 51 51.1 43.6 65.4
 86 62.9 53.1 79.7

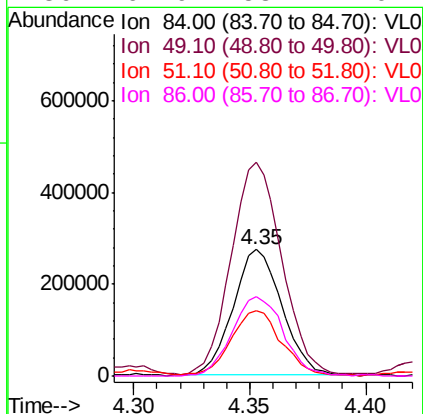



#21

Allyl Chloride

Concen: 10.123 ppbv

RT: 4.42 min Scan# 508

Delta R.T. -0.01 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :

VSTDCCC010


Tgt Ion: 41 Resp: 905610

Ion Ratio Lower Upper

41 100

76 25.7 21.8 32.6




39 81.6 64.8 97.2

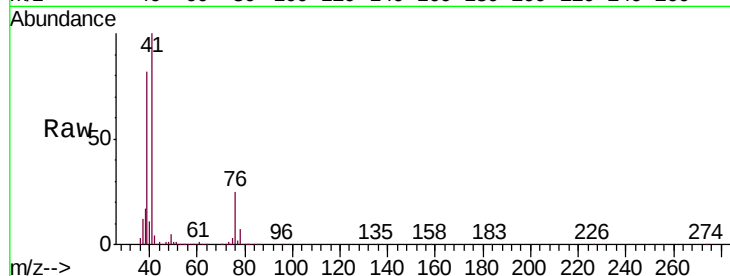

Abundance Ion 41.10 (40.80 to 41.80): VL0

Ion 76.10 (75.80 to 76.80): VL0

Ion 39.10 (38.80 to 39.80): VL0

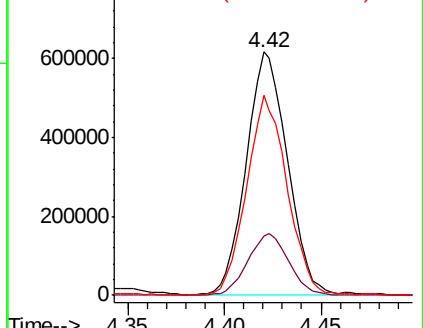

#22

trans-1,2-Dichloroethene

Concen: 9.951 ppbv

RT: 4.90 min Scan# 658

Delta R.T. -0.01 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39


Tgt Ion: 96 Resp: 451572

Ion Ratio Lower Upper

96 100

61 183.1 145.5 218.3



98 59.2 49.9 74.9




Abundance Ion 96.00 (95.70 to 96.70): VL0

Ion 61.10 (60.80 to 61.80): VL0

Ion 98.00 (97.70 to 98.70): VL0

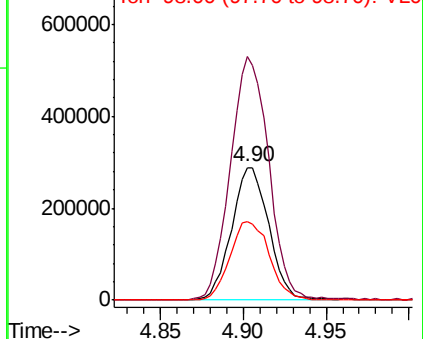




#23
 Vinyl Acetate
 Concen: 9.603 ppbv
 RT: 5.10 min Scan# 718
 Delta R.T. -0.00 min
 Lab File: VL034184.D
 Acq: 18 Sep 2019 14:39




Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Tgt Ion: 43 Resp: 2241373

Ion	Ratio	Lower	Upper
43	100		
86	6.4	5.1	7.7
42	10.2	8.6	12.8
44	6.0	4.7	7.1

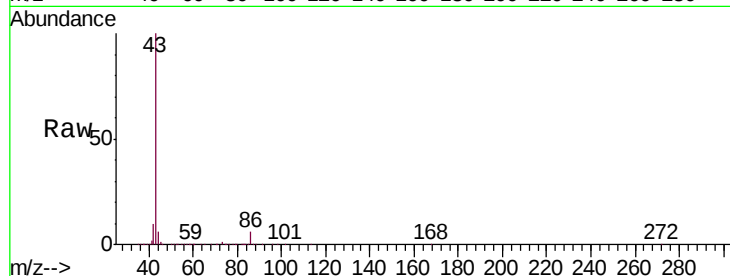


Abundance Ion 43.10 (42.80 to 43.80): VL0
 Ion 86.10 (85.80 to 86.80): VL0
 Ion 42.10 (41.80 to 42.80): VL0
 Ion 44.10 (43.80 to 44.80): VL0

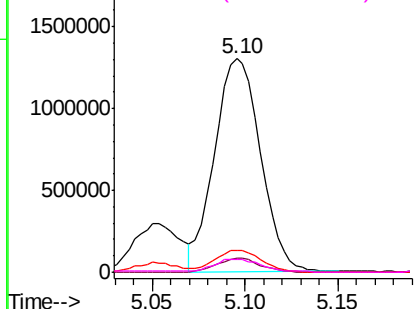



#24
 1,1-Dichloroethane
 Concen: 9.391 ppbv
 RT: 5.03 min Scan# 698
 Delta R.T. -0.01 min
 Lab File: VL034184.D
 Acq: 18 Sep 2019 14:39


Tgt Ion: 63 Resp: 1475832

Ion	Ratio	Lower	Upper
63	100		
98	3.6	1.8	5.3
100	2.6	1.0	3.0

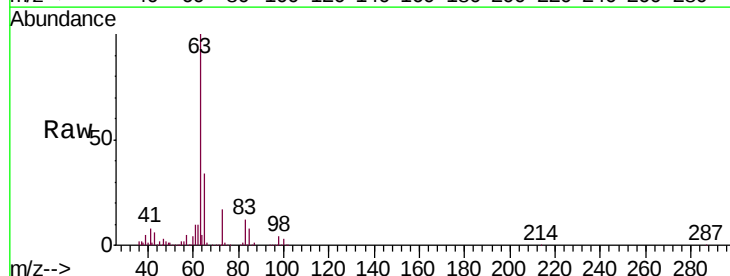

Abundance Ion 63.10 (62.80 to 63.80): VL0
 Ion 98.00 (97.70 to 98.70): VL0
 Ion 100.00 (99.70 to 100.70): VL0

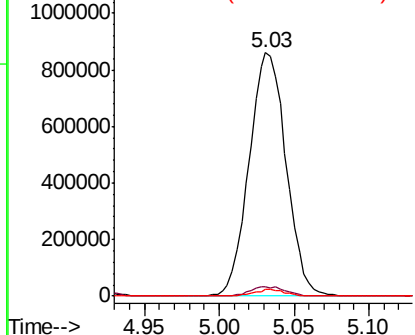




#25
Ethyl Acetate
Concen: 9.131 ppbv
RT: 5.71 min Scan# 908
Delta R.T. -0.00 min
Lab File: VL034184.D
Acq: 18 Sep 2019 14:39




Instrument :
MSVOA_L
ClientSampleId :
VSTDCCC010

Tgt Ion: 43 Resp: 2734692

Ion	Ratio	Lower	Upper
43	100		
45	10.6	8.4	12.6
61	9.2	7.2	10.8
70	6.7	5.3	7.9




Abundance Ion 43.10 (42.80 to 43.80): VL0
Ion 45.10 (44.80 to 45.80): VL0
Ion 61.10 (60.80 to 61.80): VL0
Ion 70.10 (69.80 to 70.80): VL0

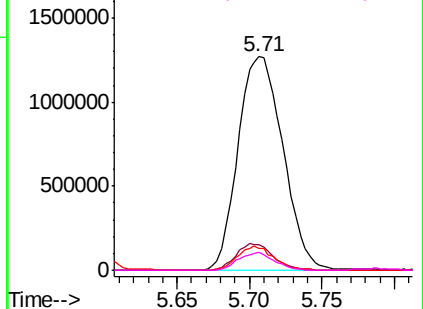



#26
Hexane
Concen: 9.227 ppbv
RT: 5.72 min Scan# 911
Delta R.T. -0.00 min
Lab File: VL034184.D
Acq: 18 Sep 2019 14:39


Tgt Ion: 57 Resp: 1149632

Ion	Ratio	Lower	Upper
57	100		
41	97.8	78.5	117.7
43	239.8	189.5	284.3
56	53.7	43.2	64.8



Abundance Ion 57.10 (56.80 to 57.80): VL0
Ion 41.10 (40.80 to 41.80): VL0
Ion 43.10 (42.80 to 43.80): VL0
Ion 56.10 (55.80 to 56.80): VL0

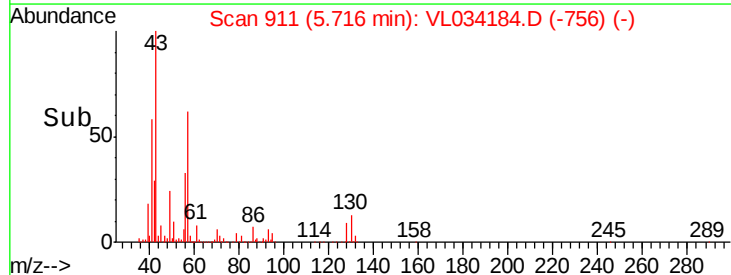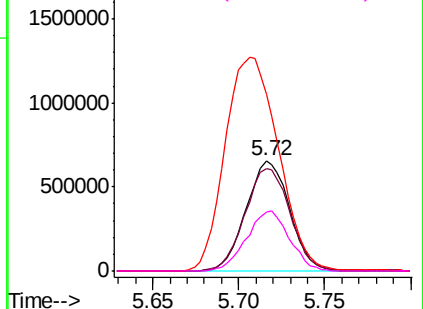



#27

Carbon Disulfide

Concen: 10.746 ppbv

RT: 4.56 min Scan# 552

Delta R.T. -0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :

VSTDCCC010





Tgt Ion: 76 Resp: 1234718

Ion	Ratio	Lower	Upper
76	100		
44	22.0	17.6	26.4
78	9.4	7.6	11.4

76 100

44 22.0 17.6 26.4

78 9.4 7.6 11.4

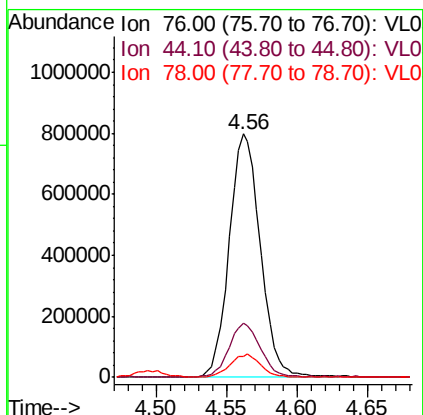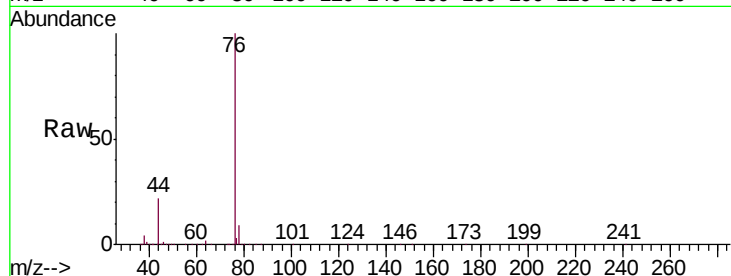

#28

Methyl tert-Butyl Ether

Concen: 9.530 ppbv

RT: 5.05 min Scan# 705

Delta R.T. -0.00 min

Lab File: VL034184.D




Acq: 18 Sep 2019 14:39


Tgt Ion: 73 Resp: 1763350

Ion	Ratio	Lower	Upper
73	100		
57	25.2	20.2	30.2

73 100

57 25.2 20.2 30.2

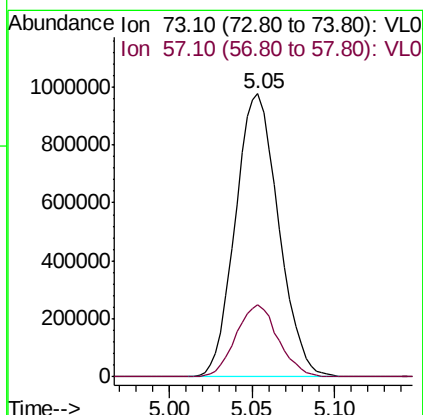



#29

Chloroform

Concen: 9.679 ppbv

RT: 5.79 min Scan# 933

Delta R.T. -0.01 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :





VSTDCCC010

Tgt Ion: 83 Resp: 1723260

Ion Ratio Lower Upper

83 100

85 65.0 52.3 78.5

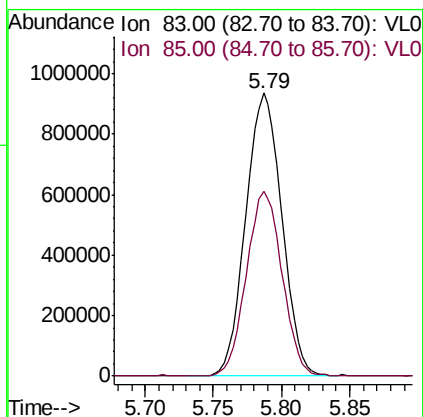

#30

Cyclohexane

Concen: 9.693 ppbv

RT: 7.18 min Scan# 1365

Delta R.T. -0.01 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39




Tgt Ion: 84 Resp: 871839


Ion Ratio Lower Upper

84 100

56 159.4 126.2 189.2

41 107.8 85.8 128.8

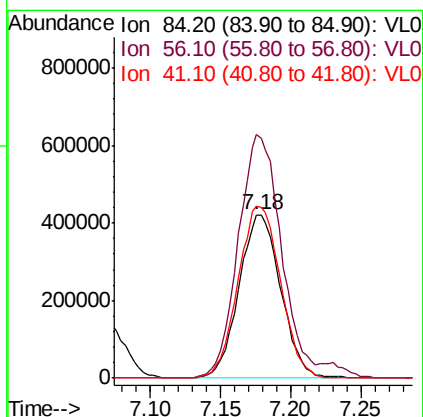







#31

cis-1,2-Dichloroethene
Concen: 9.854 ppbv
RT: 5.58 min Scan# 868
Delta R.T. -0.00 min
Lab File: VL034184.D
Acq: 18 Sep 2019 14:39

Instrument :
MSVOA_L
ClientSampleId :
VSTDCCC010




Tgt Ion: 61 Resp: 1251566
Ion Ratio Lower Upper
61 100
96 52.7 43.0 64.4
98 33.7 27.2 40.8

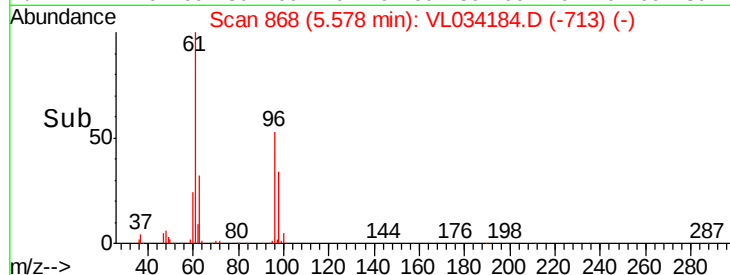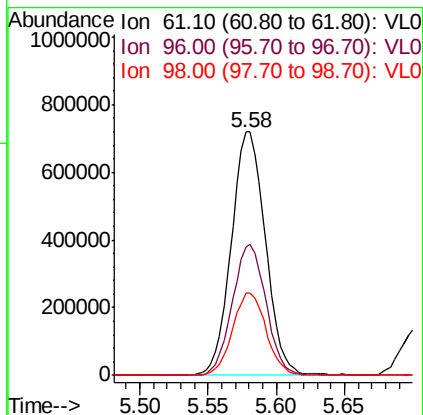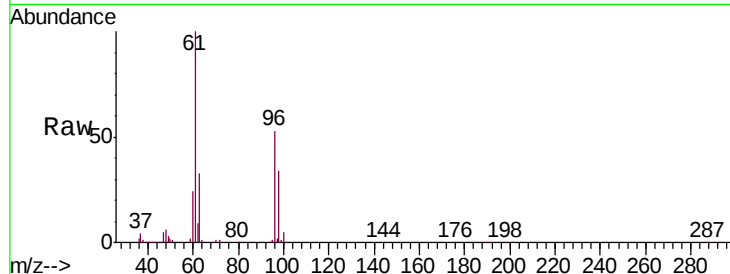


#32

1,1,1-Trichloroethane
Concen: 9.564 ppbv
RT: 6.56 min Scan# 1172
Delta R.T. -0.00 min
Lab File: VL034184.D
Acq: 18 Sep 2019 14:39

Tgt Ion: 97 Resp: 1642082
Ion Ratio Lower Upper
97 100
99 63.7 51.4 77.2
61 60.3 48.4 72.6

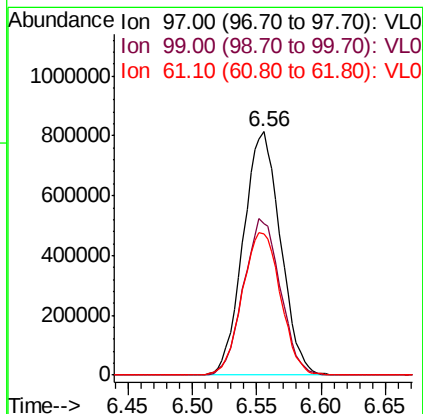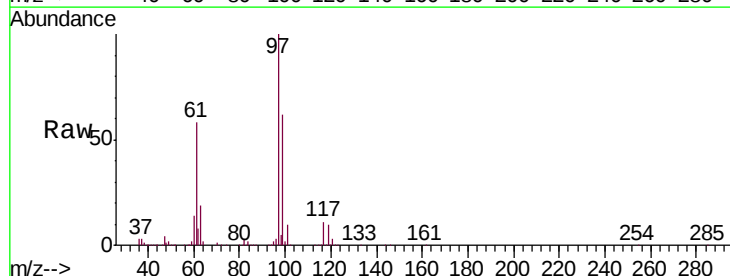







#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.22 min Scan# 1380
 Delta R.T. -0.01 min
 Lab File: VL034184.D
 Acq: 18 Sep 2019 14:39

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Tgt Ion:114 Resp: 2043178
 Ion Ratio Lower Upper
 114 100
 63 34.0 27.8 41.6
 88 21.4 17.1 25.7




Abundance Ion 114.10 (113.80 to 114.80): V
 Ion 63.10 (62.80 to 63.80): VL0
 Ion 88.10 (87.80 to 88.80): VL0


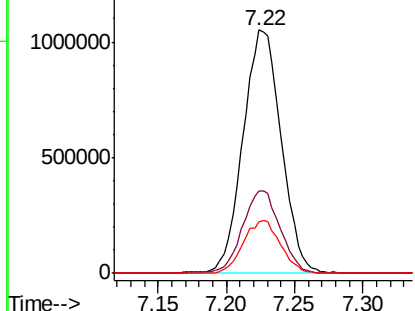



#34
 2-Butanone
 Concen: 9.285 ppbv
 RT: 5.27 min Scan# 771
 Delta R.T. -0.00 min
 Lab File: VL034184.D
 Acq: 18 Sep 2019 14:39

Tgt Ion: 43 Resp: 1937007
 Ion Ratio Lower Upper
 43 100
 72 19.4 15.0 22.6



Abundance Ion 43.10 (42.80 to 43.80): VL0
 Ion 72.10 (71.80 to 72.80): VL0

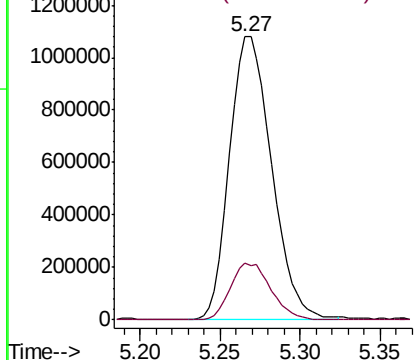



#35

Carbon Tetrachloride

Concen: 9.622 ppbv

RT: 7.07 min Scan# 1331

Delta R.T. -0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :

VSTDCCC010


Tgt Ion:117 Resp: 1633296

Ion Ratio Lower Upper

117 100

119 95.7 75.8 113.6




121 32.8 25.0 37.6



Abundance Ion 117.00 (116.70 to 117.70): V

Ion 119.00 (118.70 to 119.70): V

Ion 121.00 (120.70 to 121.70): V

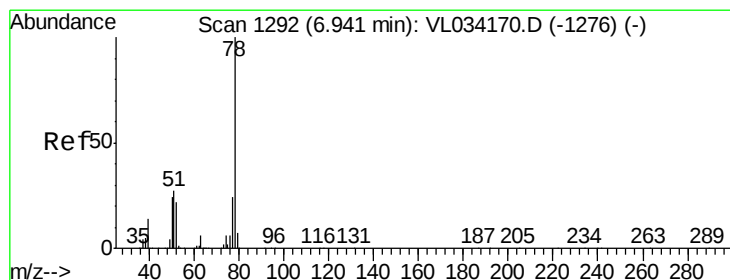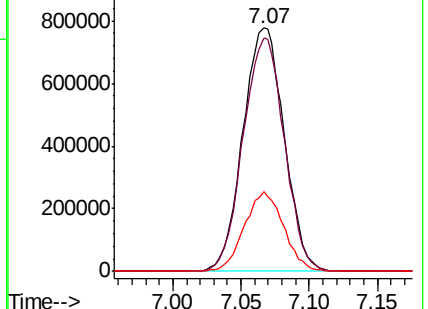

#36

Benzene

Concen: 9.279 ppbv

RT: 6.94 min Scan# 1291

Delta R.T. -0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39


Tgt Ion: 78 Resp: 2093777

Ion Ratio Lower Upper

78 100

77 23.6 19.0 28.4



50 23.8 18.9 28.3




Abundance Ion 78.10 (77.80 to 78.80): VL0

Ion 77.10 (76.80 to 77.80): VL0

Ion 50.10 (49.80 to 50.80): VL0

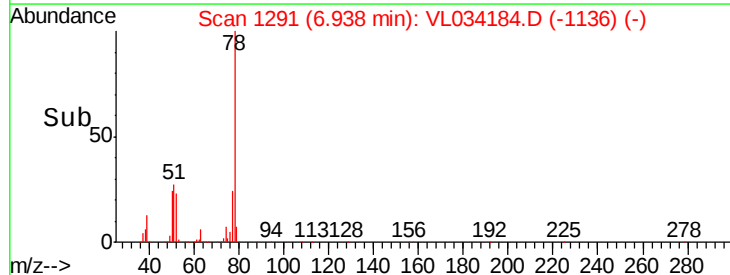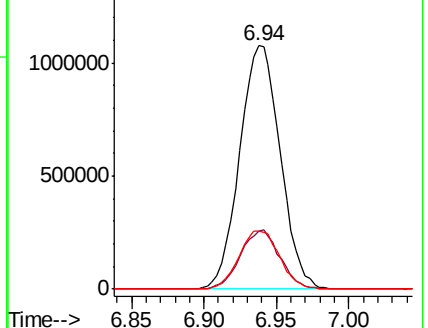



#37

1,2-Dichloroethane

Concen: 9.724 ppbv

RT: 6.35 min Scan# 1108

Delta R.T. -0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :





VSTDCCC010

Tgt Ion: 62 Resp: 1560767

Ion Ratio Lower Upper

62 100

98 4.7 3.8 5.8

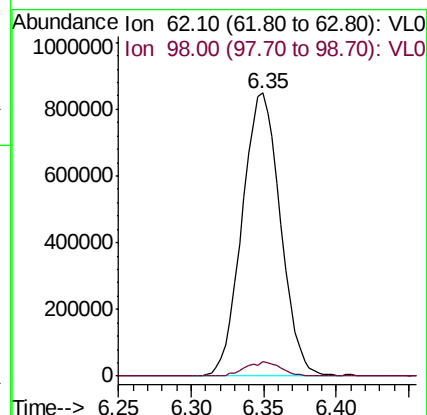

#38

Trichloroethene

Concen: 8.744 ppbv

RT: 7.89 min Scan# 1588

Delta R.T. -0.00 min

Lab File: VL034184.D

Acq: 18 Sep 2019 14:39

Tgt Ion: 130 Resp: 705019

Ion Ratio Lower Upper

130 100

95 121.6 99.8 149.6

132 91.6 75.2 112.8

97 81.6 65.0 97.4

