

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL091819\
Data File : VL034191.D
Acq On : 18 Sep 2019 20:31
Operator : SY/AP
Sample : OC CAN 10298
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC CAN 10298

Quant Time: Sep 19 10:29:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL091719AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed Sep 18 12:53:31 2019
QLast Update : Wed Sep 18 12:53:31 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.70	49	1131749	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.22	114	1820038	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.16	117	1830990	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.50	95	1663217	10.45	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	104.50%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL091819\
Data File : VL034191.D
Acq On : 18 Sep 2019 20:31
Operator : SY/AP
Sample : OC CAN 10298
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC CAN 10298

Quant Time: Sep 19 10:29:41 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL091719AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Sep 18 12:53:31 2019
QLast Update : Wed Sep 18 12:53:31 2019
Response via : Initial Calibration

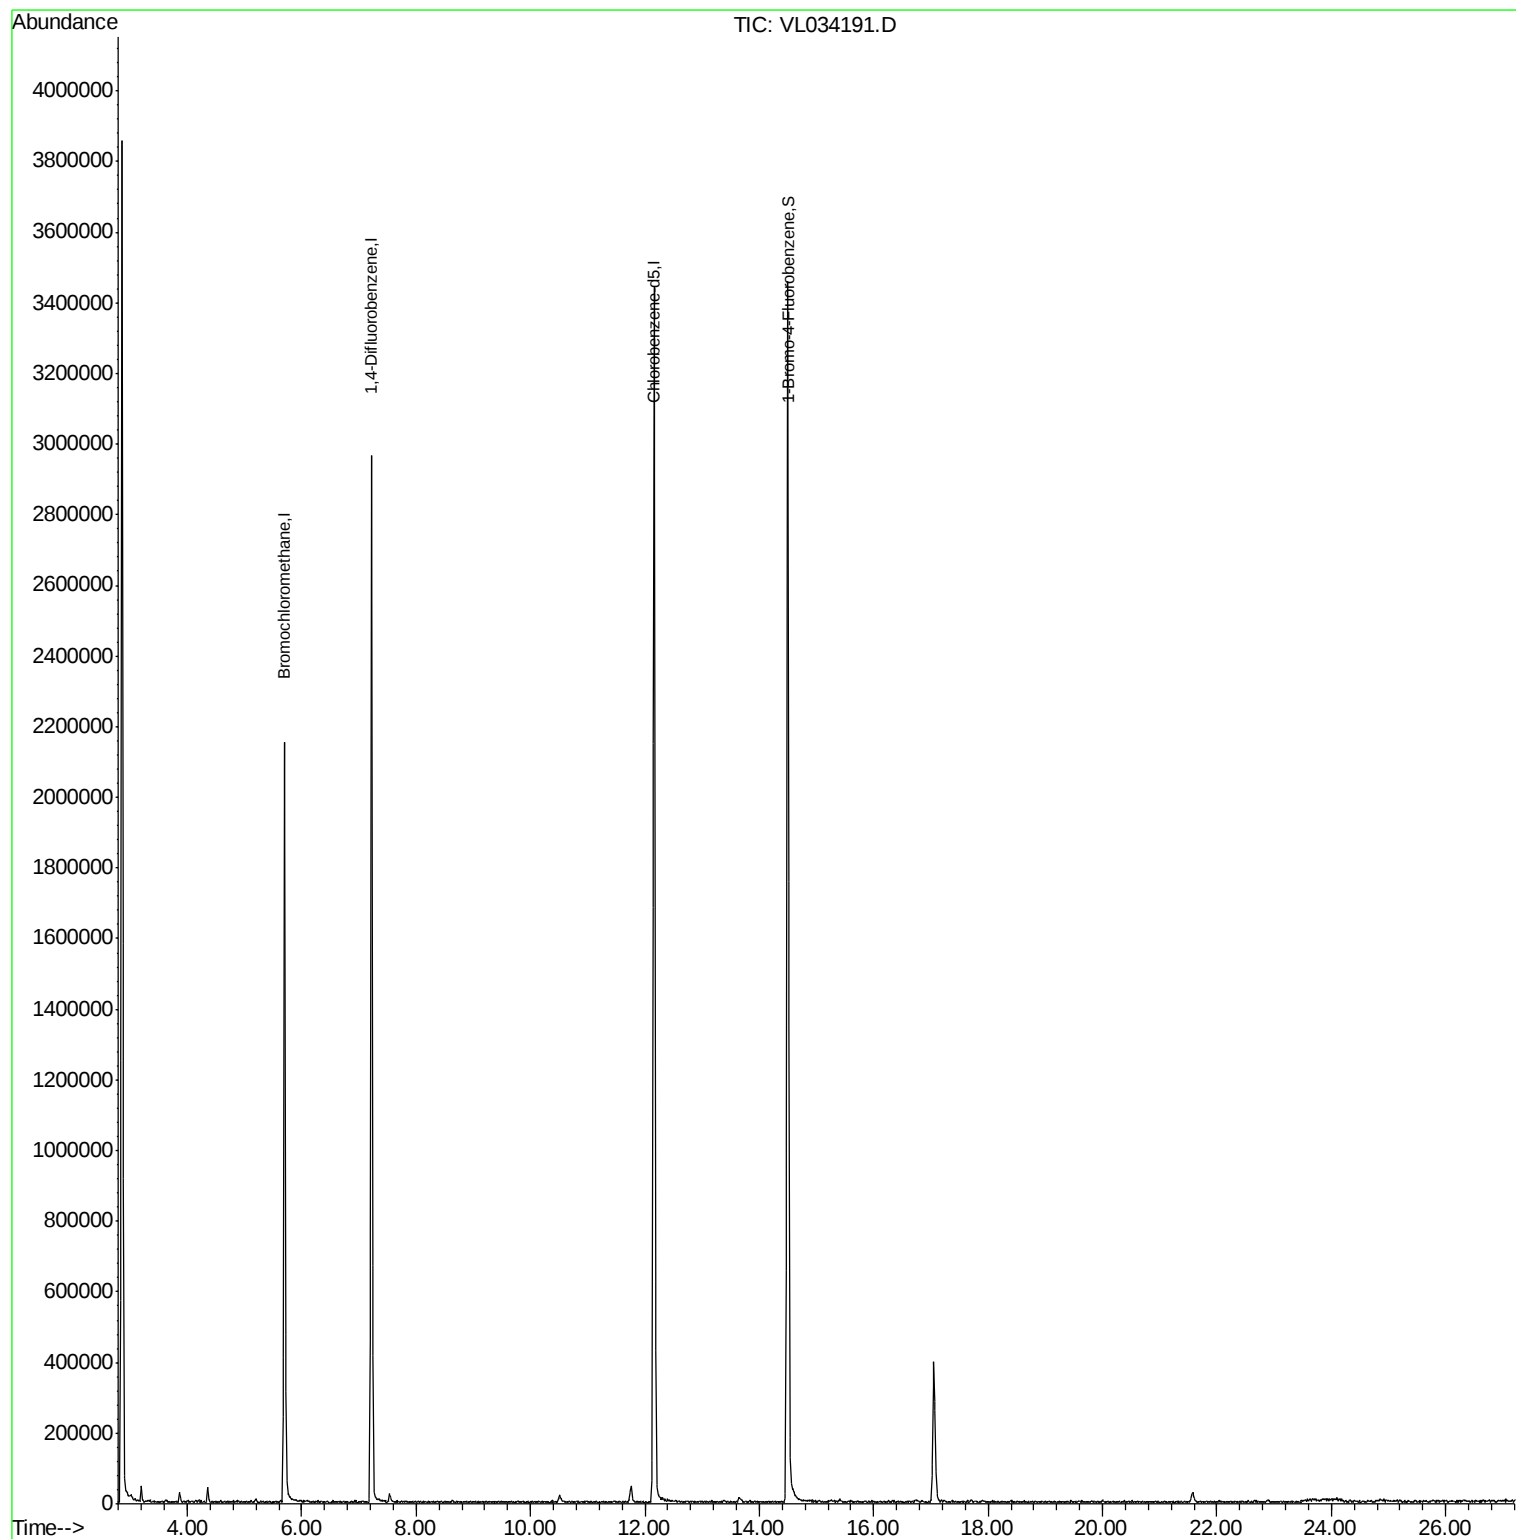

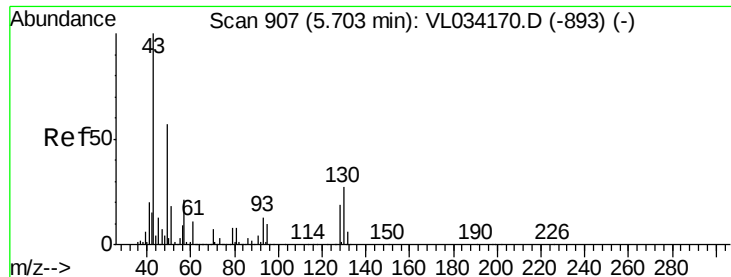

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.70 min Scan# 905

Delta R.T. -0.01 min

Lab File: VL034191.D

Acq: 18 Sep 2019 20:31

Instrument :


MSVOA_L

ClientSampleId :

QC CAN 10298

Tot Ion: 49 Resp: 1131749


Ion	Ratio	Lower	Upper
49	100		
128	34.6	17.6	52.9
130	44.7	22.3	66.9

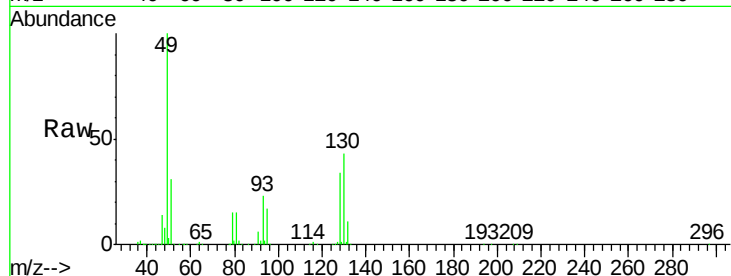


Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

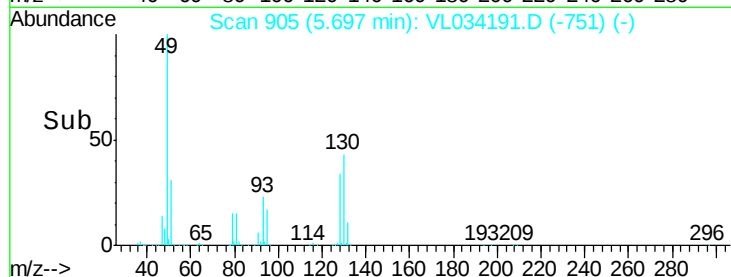

Time--> 5.60 5.65 5.70 5.75 5.80

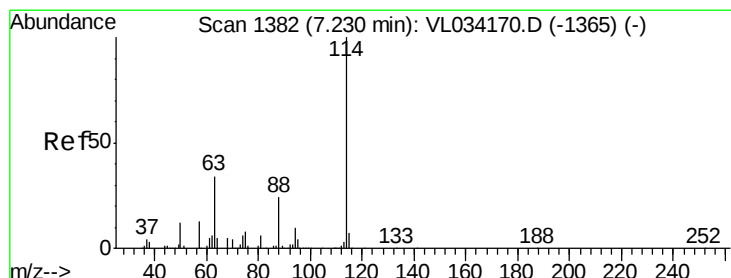

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.22 min Scan# 1380


Delta R.T. -0.01 min

Lab File: VL034191.D

Acq: 18 Sep 2019 20:31

Tgt Ion: 114 Resp: 1820038


Ion	Ratio	Lower	Upper
114	100		
63	34.1	27.8	41.6
88	21.5	17.1	25.7

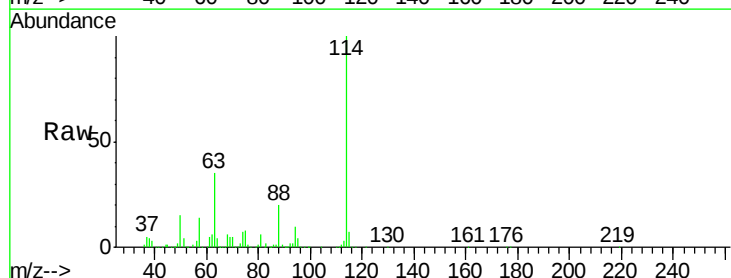


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0

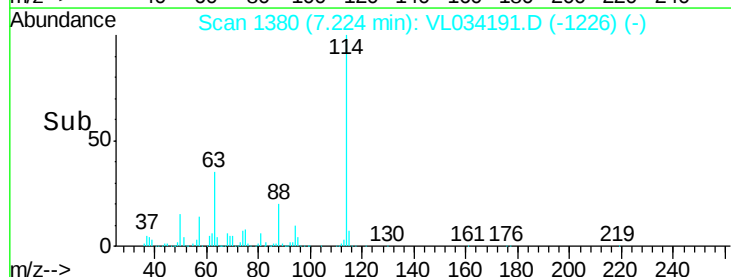





Time--> 7.15 7.20 7.25 7.30

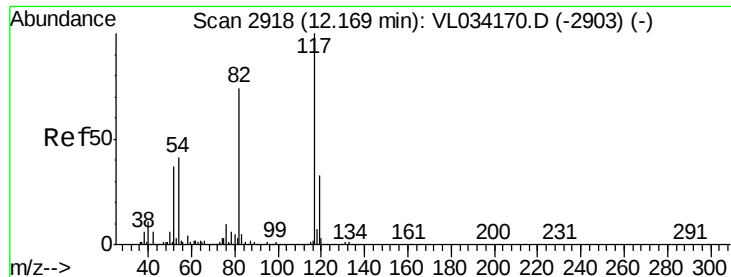

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.16 min Scan# 2916
Delta R.T. -0.01 min
Lab File: VL034191.D
Acq: 18 Sep 2019 20:31

Instrument :
MSVOA_L
ClientSampleId :
QC CAN 10298

Tot Ion:117 Resp: 1830990
Ion Ratio Lower Upper
117 100
82 78.7 58.2 87.4
119 33.1 23.7 35.5

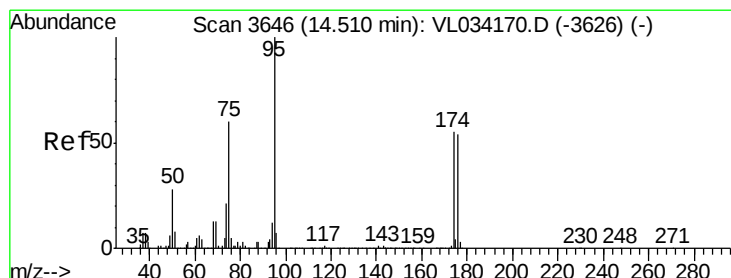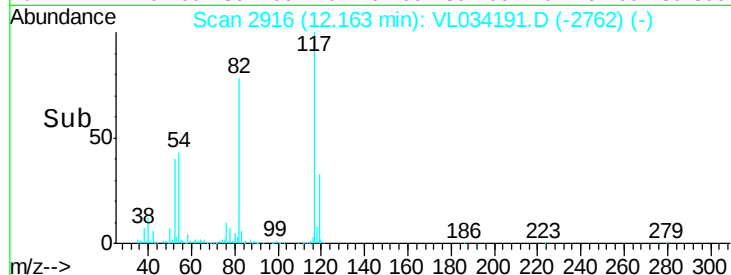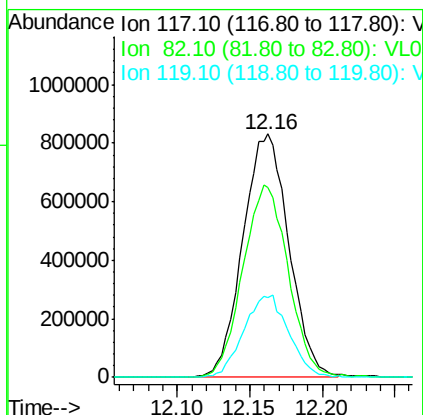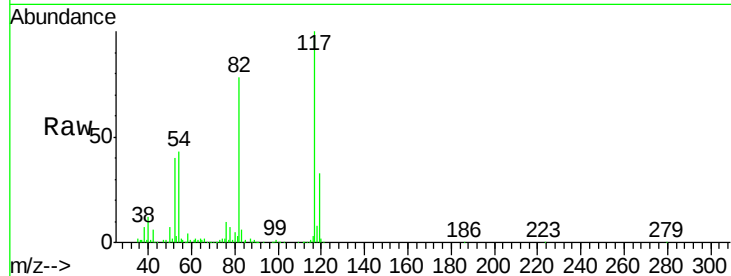

#68
1-Bromo-4-Fluorobenzene
Concen: 10.454 ppbv
RT: 14.50 min Scan# 3643
Delta R.T. -0.01 min
Lab File: VL034191.D
Acq: 18 Sep 2019 20:31

Tgt Ion: 95 Resp: 1663217
Ion Ratio Lower Upper
95 100
174 55.3 45.1 67.7
175 3.7 3.3 4.9

