


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL091819\
 Data File : VL034183.D
 Acq On : 18 Sep 2019 14:00
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL091719AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Sep 18 12:53:31 2019
 Last Update : Wed Sep 18 12:53:31 2019

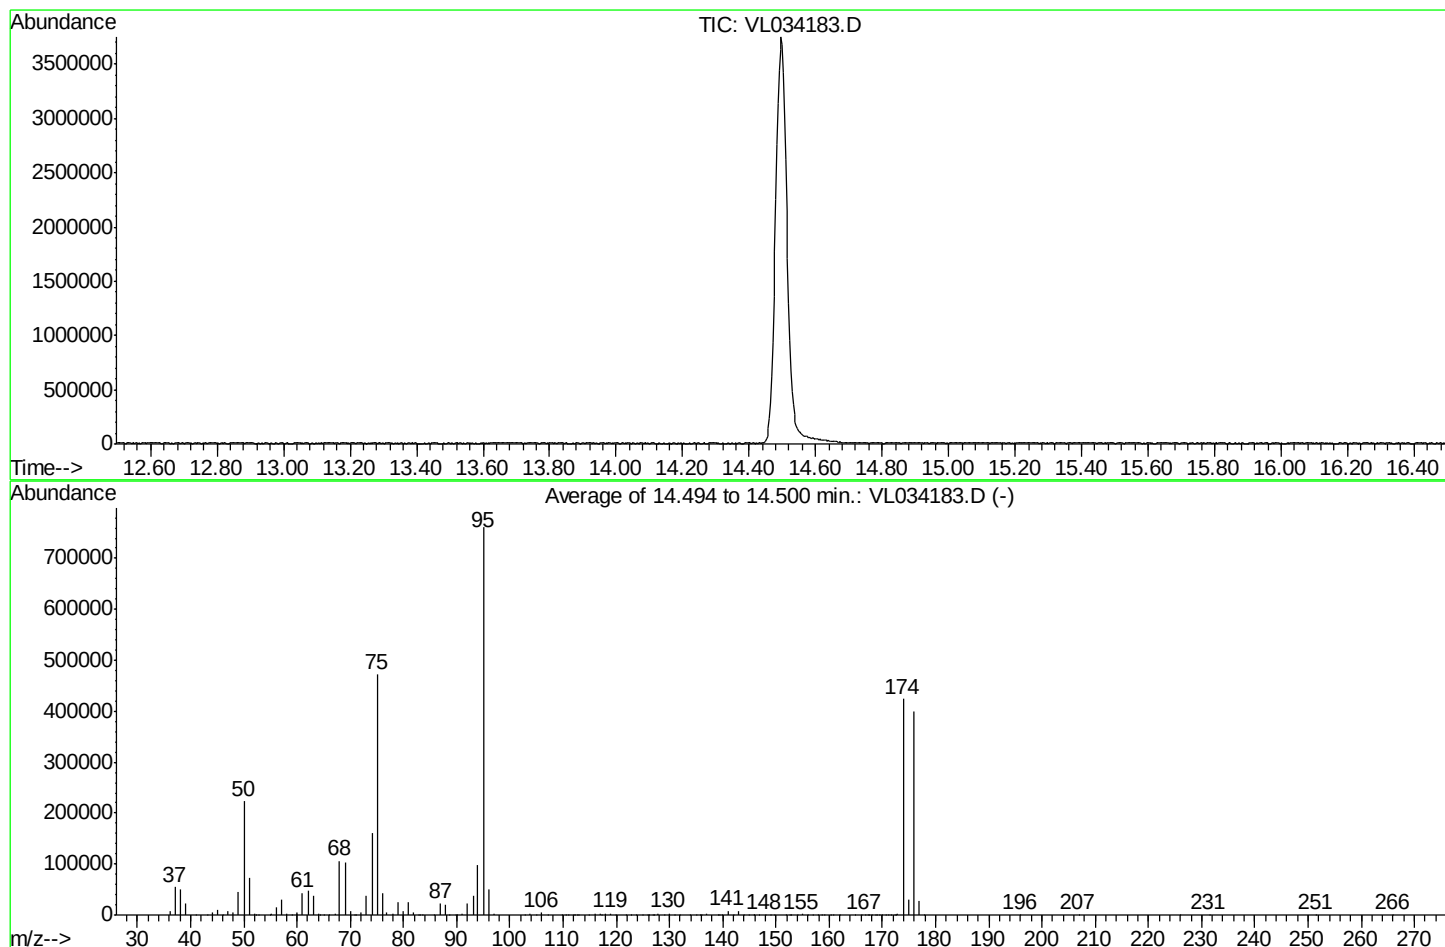

AutoFind: Scans 3641, 3642, 3643; Background Corrected with Scan 3615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	29.3	223189	PASS
75	95	30	66	62.0	471829	PASS
95	95	100	100	100.0	760960	PASS
96	95	5	9	6.5	49688	PASS
173	174	0.00	2	0.9	3613	PASS
174	95	50	120	55.7	423658	PASS
175	174	4	9	6.9	29221	PASS
176	174	93	101	94.0	398400	PASS
177	176	5	9	6.8	27026	PASS