


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL091824\
Data File : VL041600.D
Acq On : 18 Sep 2024 8:06
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091624AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Sep 17 09:12:21 2024

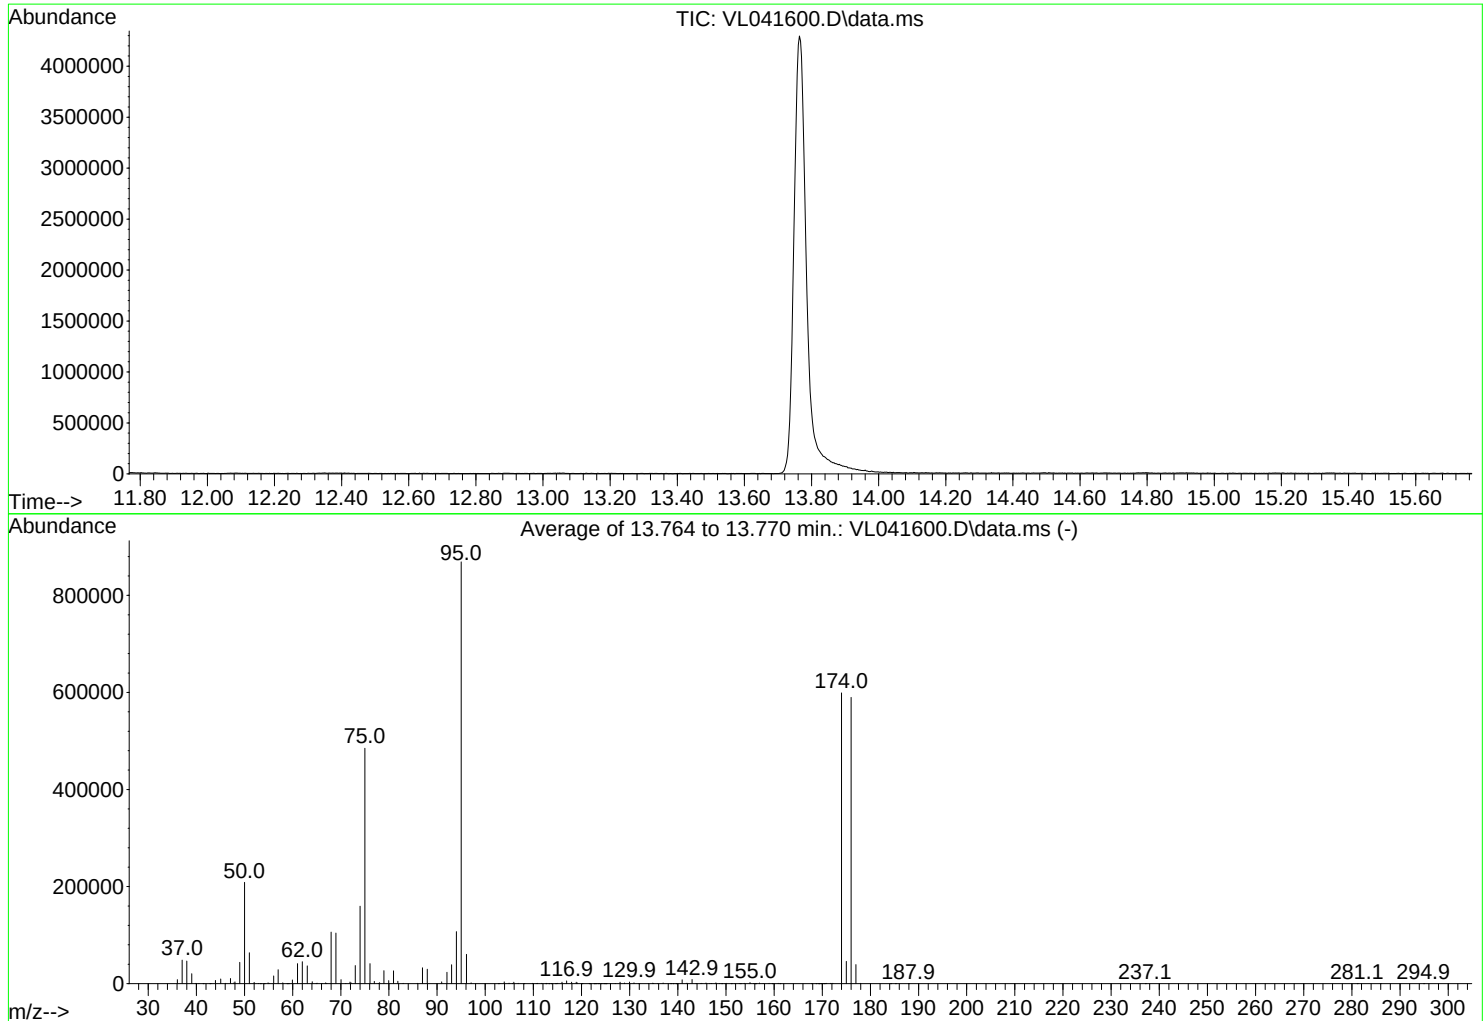

AutoFind: Scans 3471, 3472, 3473; Background Corrected with Scan 3447

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.0	208555	PASS
75	95	30	66	55.8	485056	PASS
95	95	100	100	100.0	869077	PASS
96	95	5	9	7.0	60467	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.9	599040	PASS
175	174	4	9	7.6	45741	PASS
176	174	93	101	98.5	589888	PASS
177	176	5	9	6.7	39323	PASS

Average of 13.764 to 13.770 min.: VL041600.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8287	46.10	728	54.90	1694	64.05	3904
37.05	48448	47.10	10428	55.10	728	64.90	421
38.00	46435	47.80	1687	56.05	15877	65.05	94
39.05	20501	48.00	3522	57.00	28669	66.10	32
39.90	766	49.00	43911	57.95	1511	66.85	1580
40.55	321	50.00	208555	58.80	125	67.10	739
41.40	60	51.00	63683	59.10	184	68.00	106219
42.80	101	52.00	2795	59.95	7722	69.00	104251
43.05	265	52.95	277	61.00	41149	70.05	8179
43.95	6505	53.30	54	62.00	45043	71.05	414
45.05	9705	54.10	59	63.05	36611	71.90	3247

Average of 13.764 to 13.770 min.: VL041600.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
72.10	1868	81.85	5029	97.05	1576	110.85	531
73.00	37304	82.95	677	102.70	86	111.75	704
74.00	159531	85.90	816	103.00	383	112.60	191
75.00	485056	86.95	32720	103.95	3521	112.80	542
76.05	41088	87.95	29635	104.95	1169	113.20	107
76.95	4624	90.95	3582	105.70	672	113.70	50
77.80	556	92.05	23309	105.95	3107	114.60	177
78.05	1946	93.00	38944	106.85	823	115.05	708
78.95	26675	94.00	107195	108.00	60	115.95	2942
79.95	6374	95.00	869077	109.85	558	116.90	5742
80.95	26384	96.10	60467	110.60	238	117.95	3122

Average of 13.764 to 13.770 min.: VL041600.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.90	3147	124.60	78	134.80	900	143.80	262
119.10	1785	124.90	116	135.00	591	143.95	508
120.10	153	125.10	71	135.85	194	144.80	475
121.60	112	126.05	332	136.95	1363	145.00	521
121.80	59	127.00	308	138.50	134	145.85	1423
122.60	89	128.00	2916	139.00	169	146.65	442
122.80	142	128.95	1345	139.60	97	147.00	346
123.05	150	129.95	3376	139.85	162	147.90	1597
123.50	86	130.90	1617	140.90	7912	148.70	444
123.75	318	131.90	80	141.90	1107	149.10	147
124.10	138	133.90	238	142.95	8728	149.80	273

Average of 13.764 to 13.770 min.: VL041600.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
150.05	516	157.70	211	170.40	107	184.20	59
151.10	81	158.95	735	170.60	192	185.20	53
151.85	422	159.60	64	170.90	562	187.90	67
152.75	431	160.85	777	171.70	544	237.10	51
153.00	158	161.20	183	172.00	734	281.10	160
153.80	521	167.80	83	172.20	627	285.90	65
155.00	2254	168.70	72	174.00	599040	294.90	53
155.75	263	169.20	67	175.00	45741		
156.00	97	169.35	138	176.00	589888		
156.20	83	169.70	144	177.00	39323		
156.95	1373	170.00	109	177.95	803		