
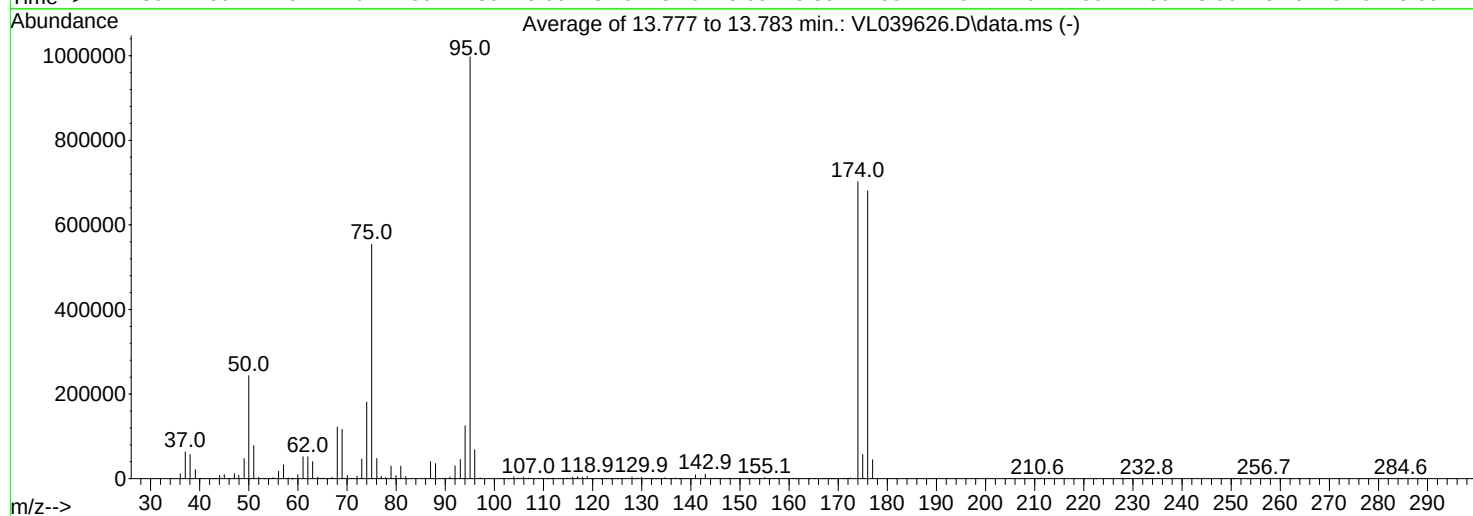


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL091922\
 Data File : VL039626.D
 Acq On : 19 Sep 2022 8:11
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL091922AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Mon Sep 19 14:26:28 2022

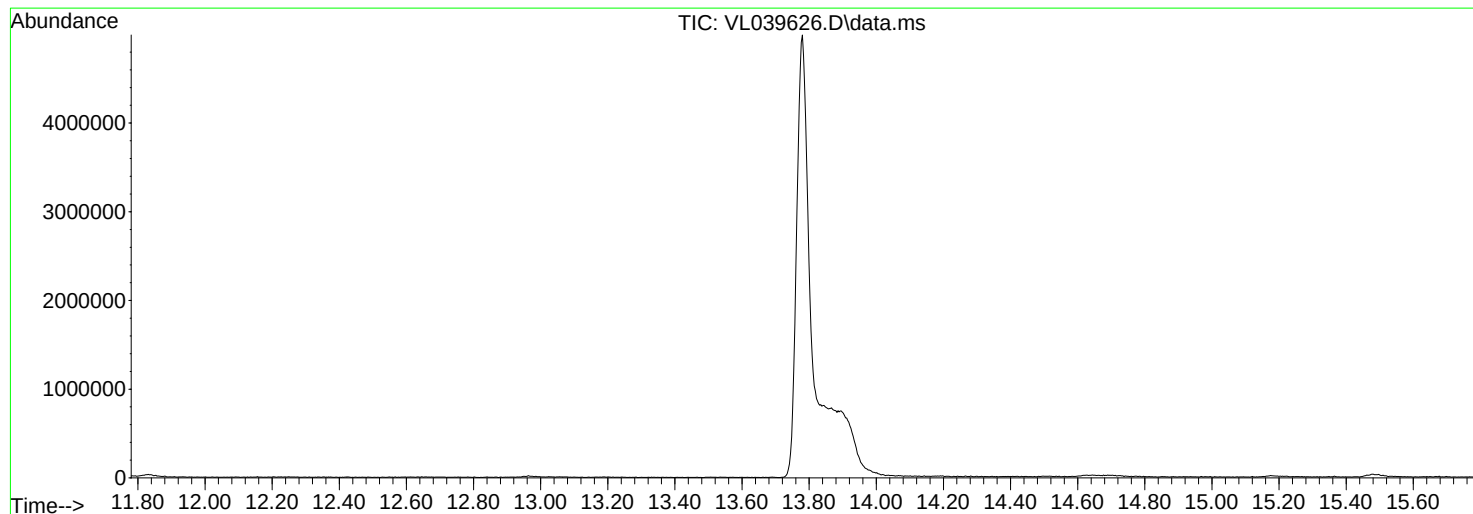

AutoFind: Scans 3475, 3476, 3477; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	243712	PASS
75	95	30	66	55.6	554091	PASS
95	95	100	100	100.0	997397	PASS
96	95	5	9	6.9	68389	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.4	702165	PASS
175	174	4	9	8.2	57331	PASS
176	174	93	101	96.9	680597	PASS
177	176	5	9	6.6	44584	PASS

Average of 13.777 to 13.783 min.: VL039626.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	11228	45.90	709	55.10	823	64.80	1114
37.05	63051	46.20	289	56.05	17388	65.25	114
38.05	57053	47.05	11595	57.05	32696	65.90	20
39.10	21352	47.95	7557	58.05	1754	66.90	252
40.15	892	49.05	47488	58.70	163	67.10	1186
42.10	285	50.00	243712	58.90	111	68.00	121819
42.60	118	51.00	78392	59.95	9557	69.00	117088
42.90	232	52.00	3313	61.05	51784	70.05	7722
43.20	197	53.10	195	62.00	52027	70.85	278
44.05	7496	54.15	117	63.00	40547	72.00	6130
45.00	9627	54.90	2364	64.05	3853	73.00	46283

Average of 13.777 to 13.783 min.: VL039626.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.00	181288	86.10	426	102.85	408	114.85	1043
75.00	554091	87.00	40651	103.95	4177	115.90	3451
76.05	47675	88.00	35771	104.85	1416	116.95	4719
76.95	5525	90.95	4310	105.90	3896	117.90	3611
77.85	2896	92.00	30299	106.95	1544	118.90	5001
78.95	29541	93.05	45256	109.80	646	119.85	154
79.95	7266	94.05	124739	110.75	49	120.10	115
80.95	29619	95.05	997397	111.05	551	121.70	61
81.95	5047	96.00	68389	111.85	1101	121.90	87
83.10	584	97.10	1823	113.00	939	122.85	435
85.80	774	101.80	90	113.90	72	123.70	83

Average of 13.777 to 13.783 min.: VL039626.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.00	440	131.70	242	139.55	441	147.75	1024
124.65	299	132.10	123	139.95	559	147.90	817
125.10	83	132.90	120	140.95	8955	148.10	563
125.90	411	133.90	91	141.70	674	148.90	707
126.70	244	134.75	2344	142.05	961	149.85	994
128.00	3701	135.80	62	142.95	10473	151.60	95
128.80	555	136.05	290	143.95	564	151.90	389
129.05	1224	136.85	1955	144.95	1076	152.40	243
129.95	3512	137.60	182	145.70	431	152.95	432
130.80	775	138.70	265	146.00	1160	153.90	804
131.00	317	139.10	357	146.85	505	154.20	236

Average of 13.777 to 13.783 min.: VL039626.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.05	2825	164.10	115	170.75	734	210.60	52
156.00	156	165.10	206	171.10	300	222.50	61
156.90	665	166.70	76	171.30	522	227.80	97
157.10	354	167.10	364	171.90	801	232.85	112
157.70	237	167.30	130	172.10	1284	250.50	62
157.95	260	168.15	388	172.50	1502	253.30	100
159.00	1259	168.50	167	174.00	702165	256.70	101
159.80	75	168.95	197	175.00	57331	262.30	52
160.85	1082	169.50	336	176.00	680597	263.80	53
161.40	136	169.75	410	177.00	44584	284.60	142
163.80	88	170.15	897	177.95	1109	288.70	123

Average of 13.777 to 13.783 min.: VL039626.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
289.40	132						