


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL092018\
Data File : VL032506.D
Acq On : 20 Sep 2018 12:52
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL083118AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Sep 21 02:39:49 2018
Last Update : Fri Sep 21 02:39:49 2018

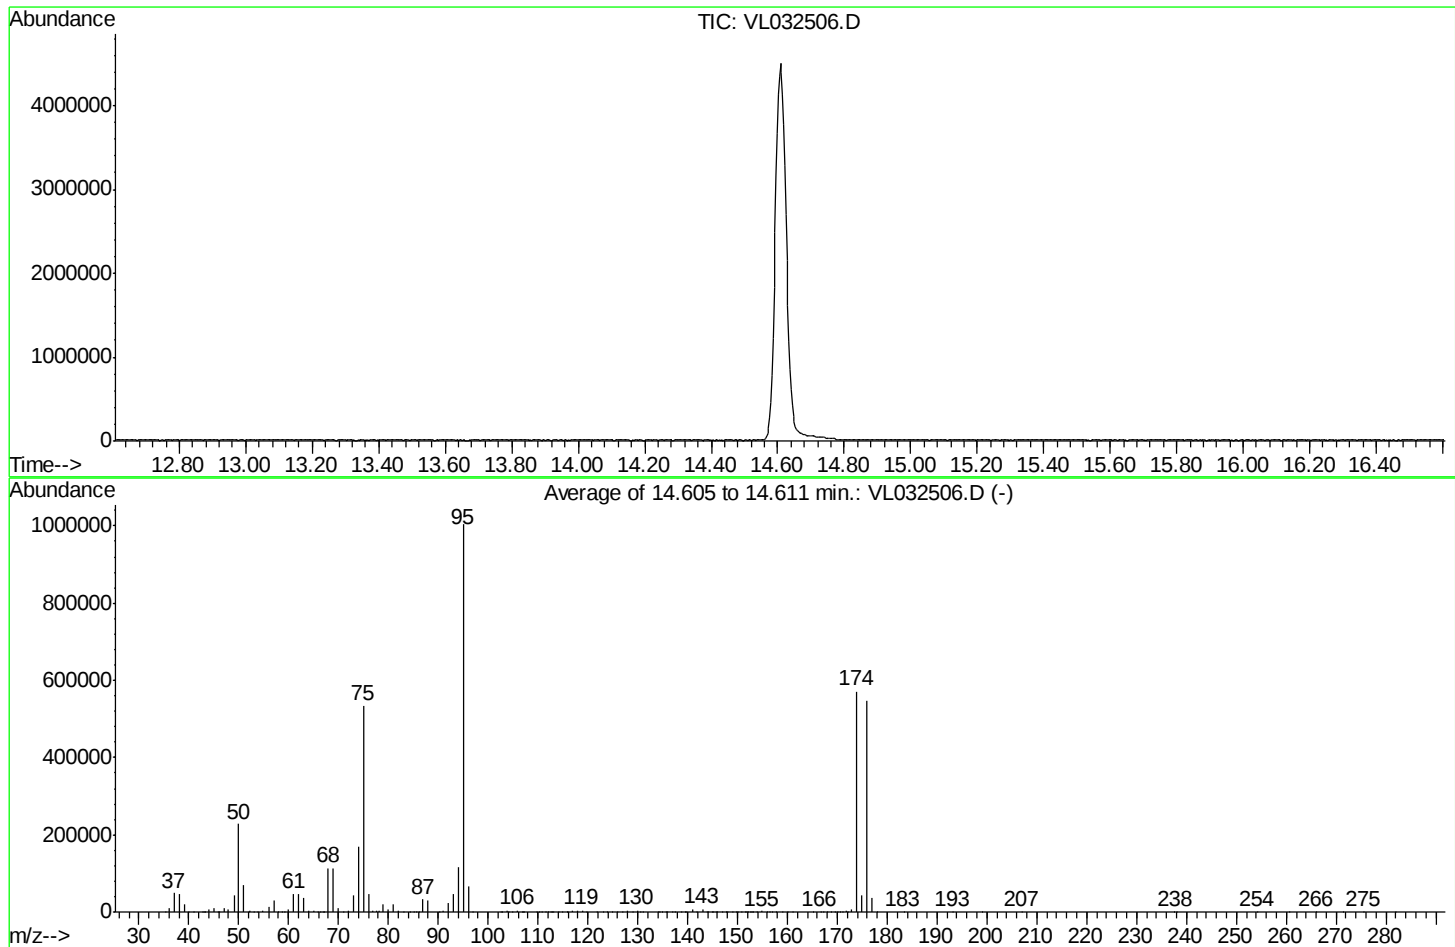

AutoFind: Scans 3629, 3630, 3631; Background Corrected with Scan 3603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.8	228522	PASS
75	95	30	66	53.2	534464	PASS
95	95	100	100	100.0	1004010	PASS
96	95	5	9	6.6	66250	PASS
173	174	0.00	2	1.1	6103	PASS
174	95	50	120	56.8	570666	PASS
175	174	4	9	7.7	43690	PASS
176	174	93	101	95.9	547089	PASS
177	176	5	9	6.4	35013	PASS