

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL092122\
 Data File : VL039648.D
 Acq On : 21 Sep 2022 23:37
 Operator : SY/AP
 Sample : N4669-04DL 10X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :

Quant Time: Sep 22 08:21:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091922AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Mon Sep 19 14:26:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	5.214	49	1092075	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.671	114	2812926	10.000	ppbv	0.01
55) Chlorobenzene-d5	11.484	117	2567052	10.000	ppbv	0.01
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.793	95	1892526	9.876	ppbv	0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	98.800%
Target Compounds						
					Qvalue	
3) Chlorodifluoromethane	2.681	51	1867244	14.408	ppbv #	57
9) Propene	2.902	41	356592	6.025	ppbv	95
13) Ethanol	3.263	45	494235	109.589	ppbv	72
15) Acetone	3.497	43	92437	0.761	ppbv #	27
16) 1,3-Butadiene	3.037	39	4264	0.069	ppbv #	28
19) Isopropyl Alcohol	3.607	45	27848	0.450	ppbv #	75
20) Methylene Chloride	3.957	84	19918	0.355	ppbv #	92
23) Vinyl Acetate	4.645	43	5220	0.095	ppbv #	74
25) Ethyl Acetate	5.237	43	23690	0.089	ppbv #	89
26) Hexane	5.240	57	7493	0.067	ppbv #	16
34) 2-Butanone	4.819	43	7590	0.055	ppbv #	53
39) 1,2-Dichloropropane	6.674	63	688894	8.296	ppbv #	26
76) 1,4-Dichlorobenzene	16.493	146	25567	0.145	ppbv #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL092122\
Data File : VL039648.D
Acq On : 21 Sep 2022 23:37
Operator : SY/AP
Sample : N4669-04DL 10X
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :

Quant Time: Sep 22 08:21:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091922AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Mon Sep 19 14:26:28 2022
Response via : Initial Calibration




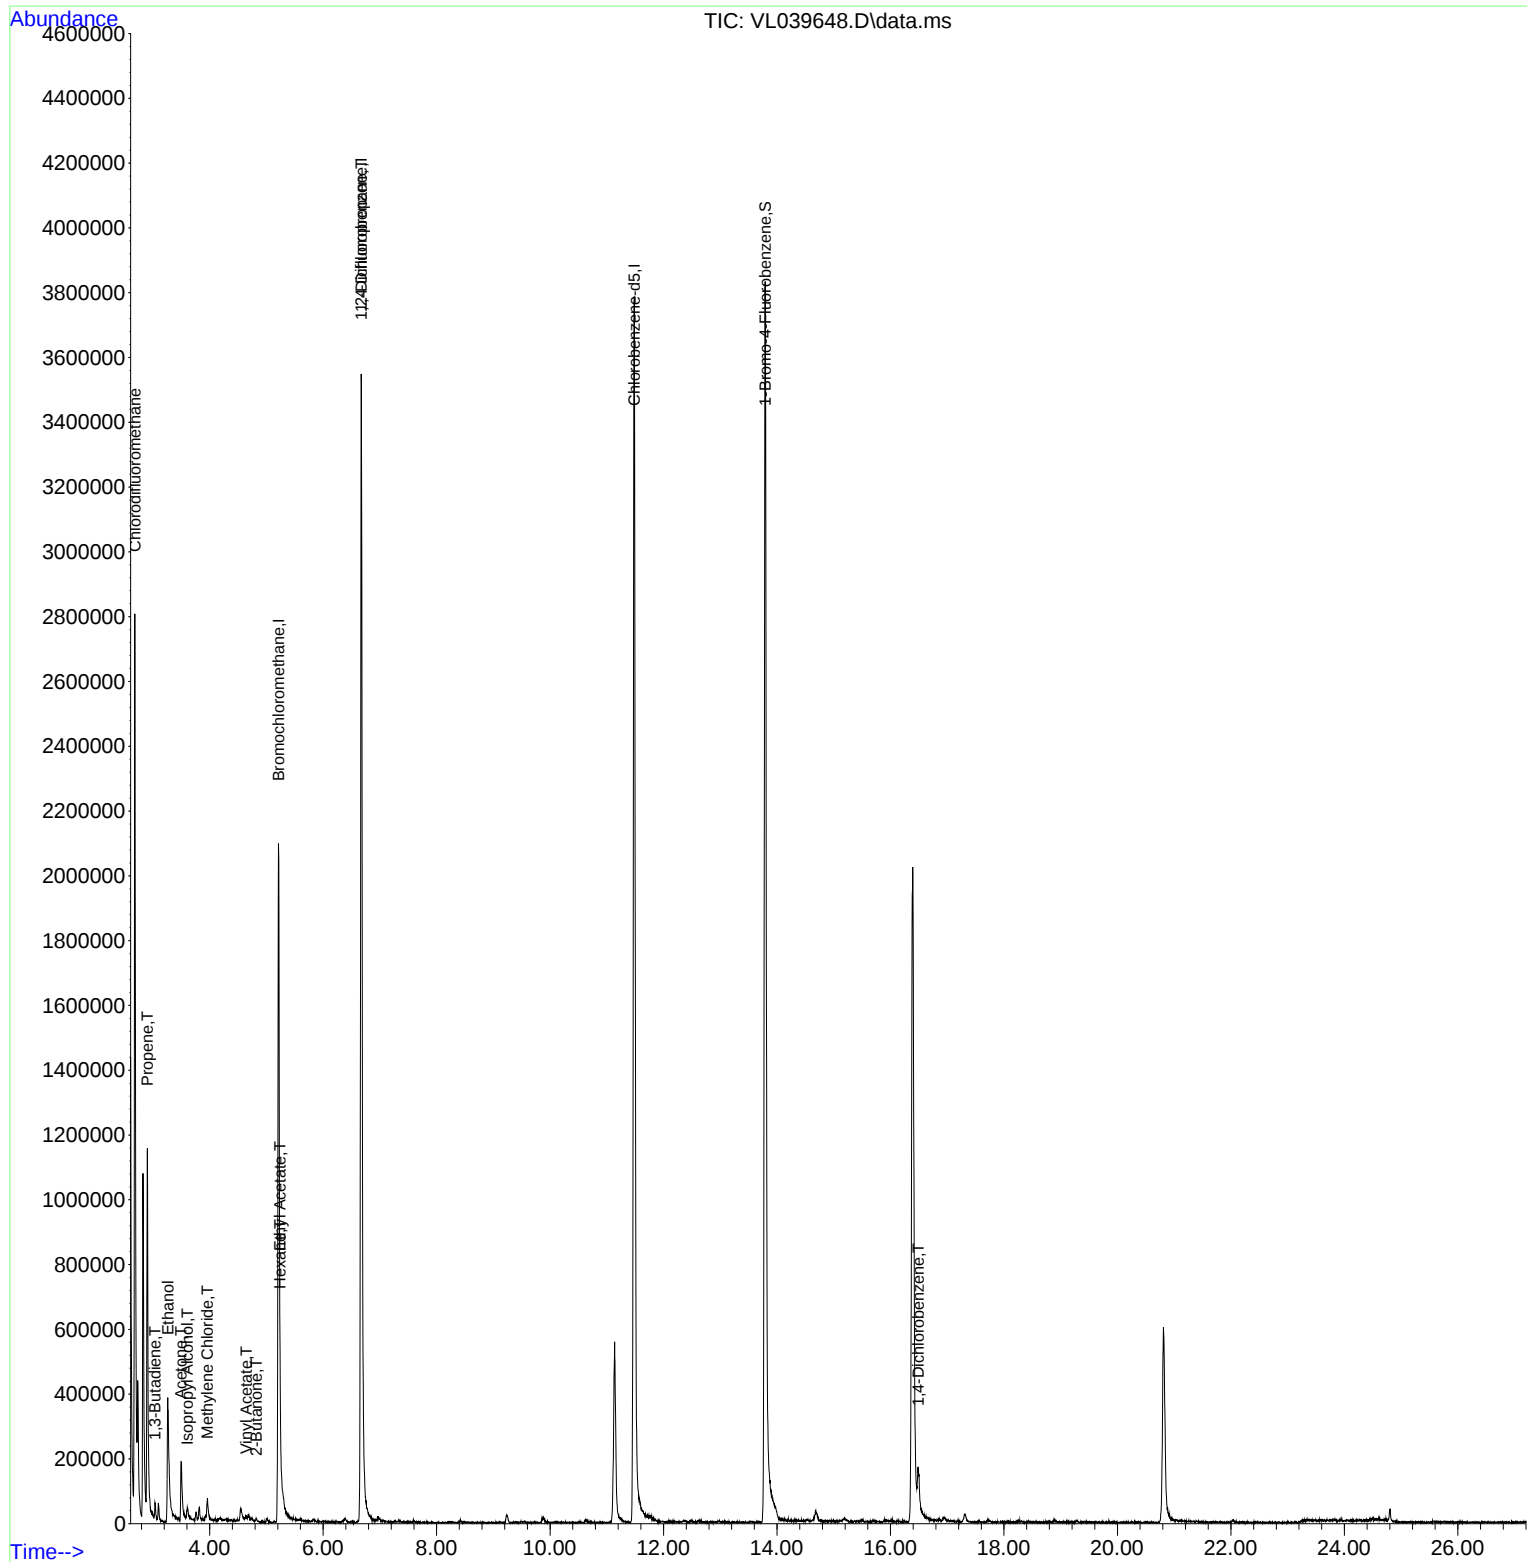


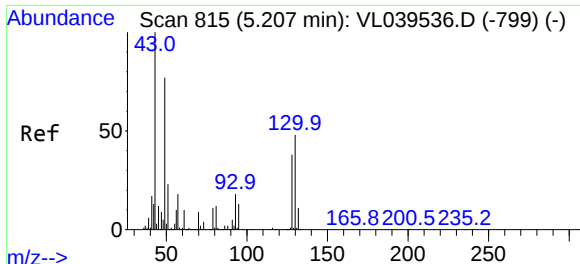

#1
 Bromochloromethane
 Concen: 10.000 ppbv
 RT: 5.214 min Scan# 81
 Delta R.T. 0.007 min
 Lab File: VL039648.D
 Acq: 21 Sep 2022 23:37




Instrument :
 MSVOA_L
 ClientSampleId :


Tgt Ion: 49 Resp: 1092075
 Ion Ratio Lower Upper
 49 100
 128 49.6 26.7 80.0
 130 63.5 34.3 102.8

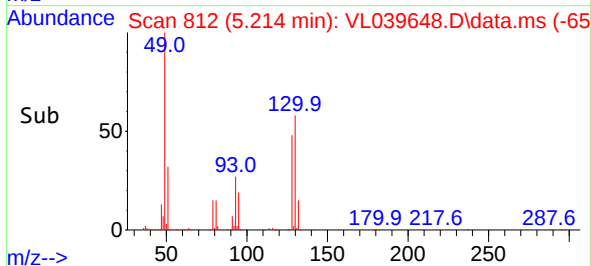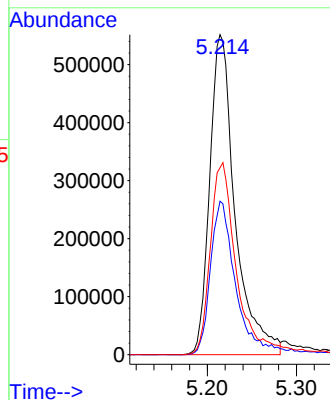

#3
 Chlorodifluoromethane
 Concen: 14.408 ppbv
 RT: 2.681 min Scan# 24
 Delta R.T. -0.012 min
 Lab File: VL039648.D
 Acq: 21 Sep 2022 23:37

Tgt Ion: 51 Resp: 1867244
 Ion Ratio Lower Upper
 51 100
 67 0.0 15.7 23.5#


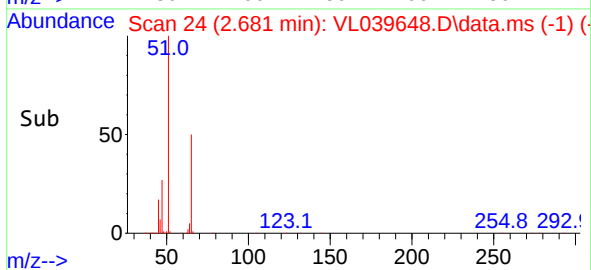
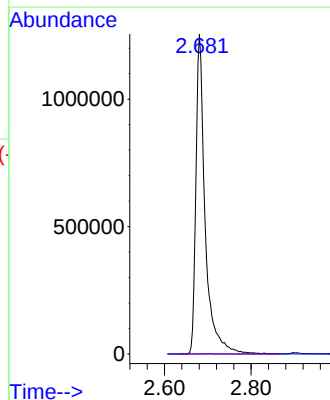
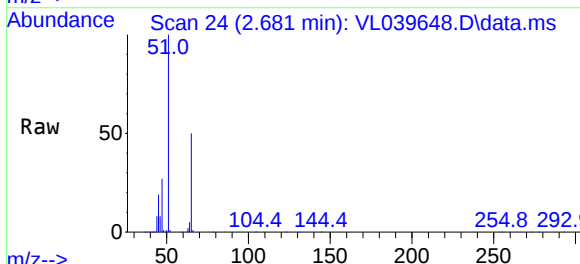


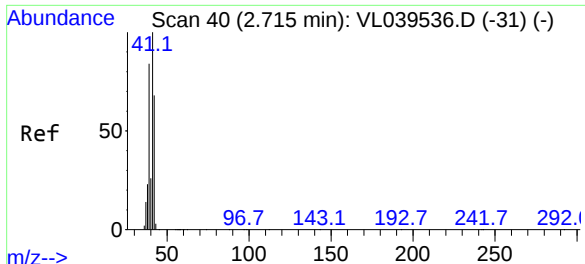

#9
 Propene
 Concen: 6.025 ppbv
 RT: 2.902 min Scan# 91
 Delta R.T. 0.187 min
 Lab File: VL039648.D
 Acq: 21 Sep 2022 23:37




Instrument :
 MSVOA_L
 ClientSampleId :


Tgt Ion: 41 Resp: 356592
 Ion Ratio Lower Upper
 41 100
 42 65.3 55.2 82.8

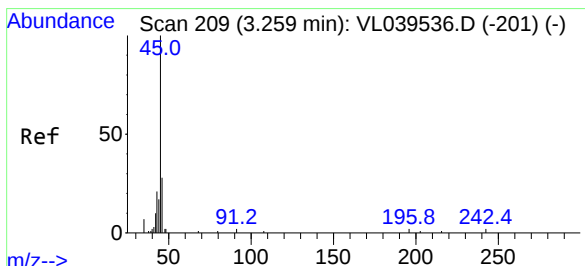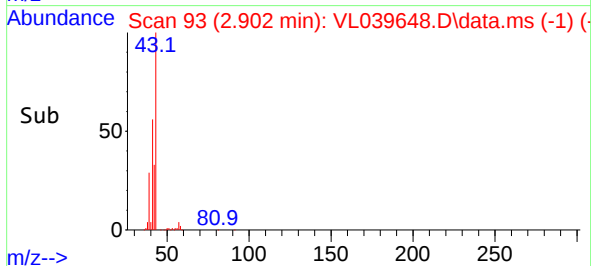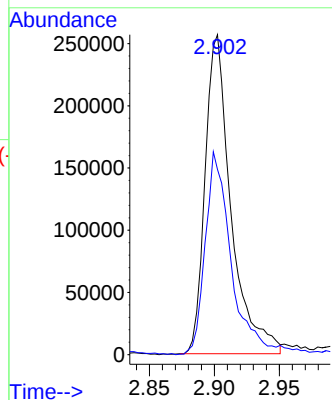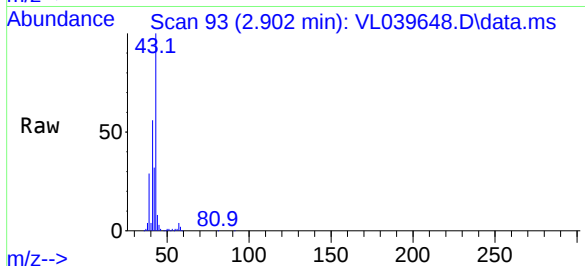

#13
 Ethanol
 Concen: 109.589 ppbv
 RT: 3.263 min Scan# 205
 Delta R.T. 0.004 min
 Lab File: VL039648.D
 Acq: 21 Sep 2022 23:37

Tgt Ion: 45 Resp: 494235
 Ion Ratio Lower Upper
 45 100
 46 36.7 22.8 91.2


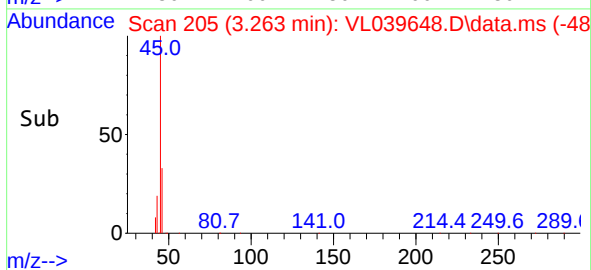
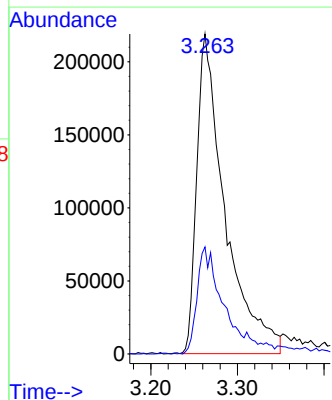
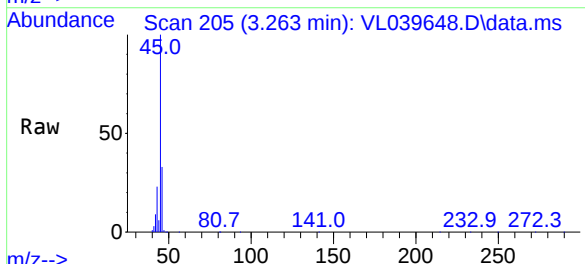




#15
Acetone
Concen: 0.761 ppbv
RT: 3.497 min Scan# 21
Delta R.T. 0.013 min
Lab File: VL039648.D
Acq: 21 Sep 2022 23:37




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 43 Resp: 92437
Ion Ratio Lower Upper
43 100
58 63.6 21.0 31.6#

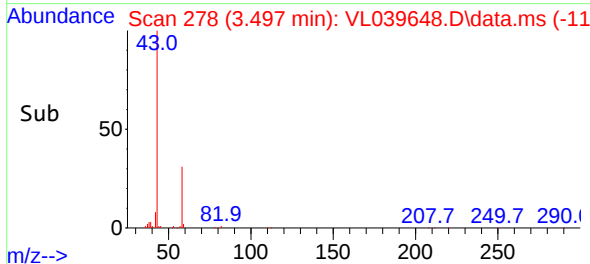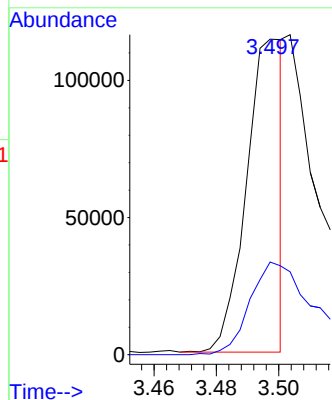

#16
1,3-Butadiene
Concen: 0.069 ppbv
RT: 3.037 min Scan# 135
Delta R.T. 0.033 min
Lab File: VL039648.D
Acq: 21 Sep 2022 23:37

Tgt Ion: 39 Resp: 4264
Ion Ratio Lower Upper
39 100
54 16.7 63.7 95.5#

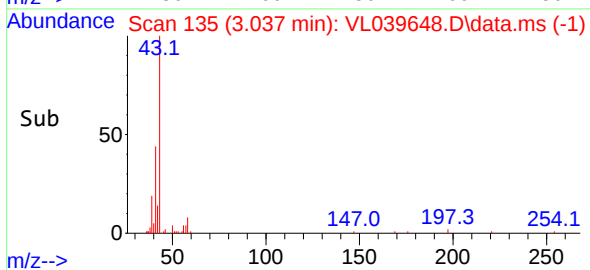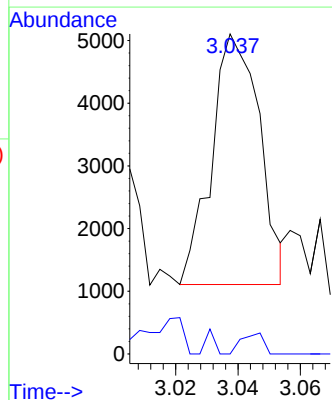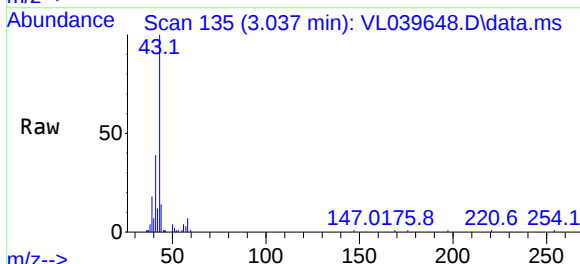



#19

Isopropyl Alcohol

Concen: 0.450 ppbv

RT: 3.607 min Scan# 312

Delta R.T. 0.017 min

Lab File: VL039648.D

Acq: 21 Sep 2022 23:37

Instrument :

MSVOA_L





ClientSampleId :

Tgt Ion: 45 Resp: 27848

Ion Ratio Lower Upper

45 100

58 12.3 3.2 4.8#

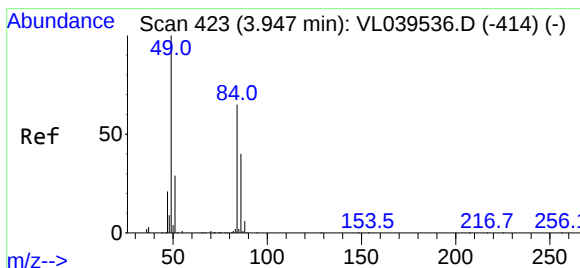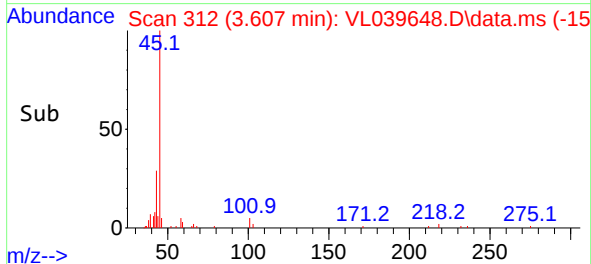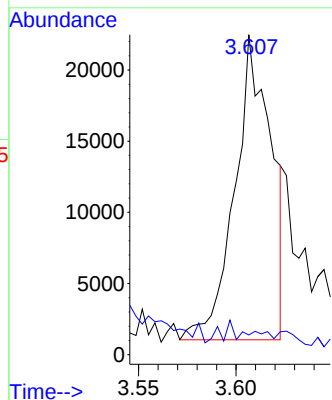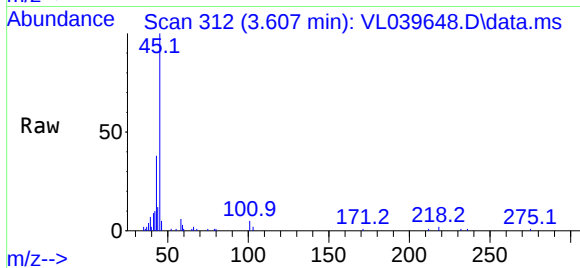

#20

Methylene Chloride

Concen: 0.355 ppbv

RT: 3.957 min Scan# 421

Delta R.T. 0.010 min

Lab File: VL039648.D

Acq: 21 Sep 2022 23:37

Tgt Ion: 84 Resp: 19918




Ion Ratio Lower Upper


84 100

49 150.3 123.1 184.7

51 39.2 34.4 51.6

86 45.7 51.1 76.7#

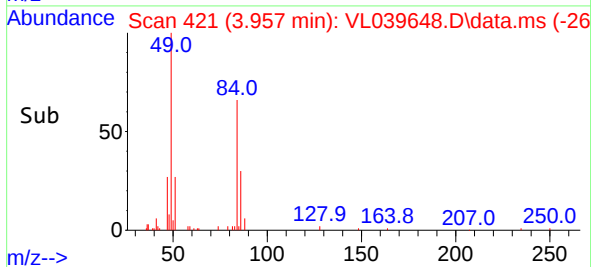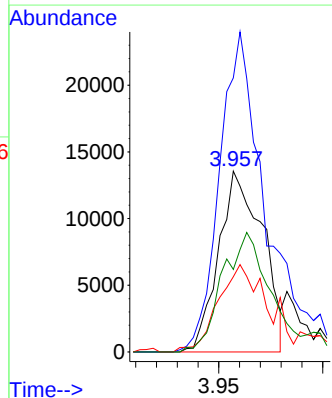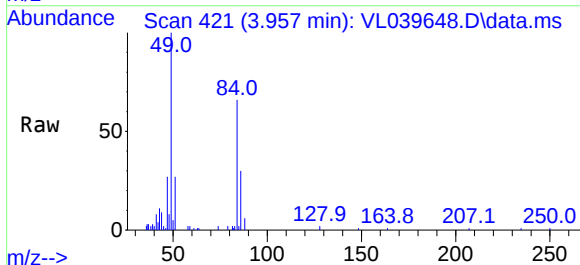







#23
Vinyl Acetate
Concen: 0.095 ppbv
RT: 4.645 min Scan# 61
Delta R.T. 0.007 min
Lab File: VL039648.D
Acq: 21 Sep 2022 23:37

Instrument :
MSVOA_L
ClientSampleId :

Tgt Ion: 43 Resp: 5220




Ion	Ratio	Lower	Upper
43	100		
86	0.0	5.0	7.6#
42	23.2	7.7	11.5#
44	0.0	4.6	7.0#

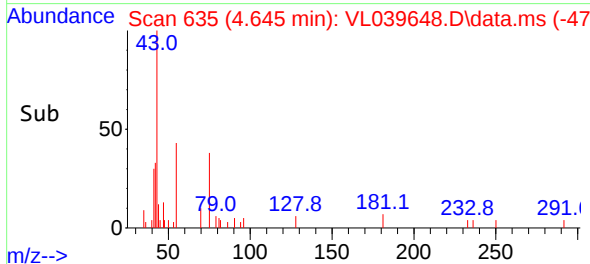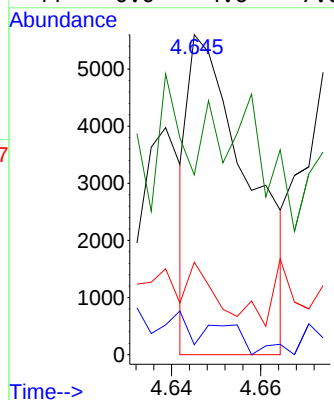


#25
Ethyl Acetate
Concen: 0.089 ppbv
RT: 5.237 min Scan# 819
Delta R.T. 0.020 min
Lab File: VL039648.D
Acq: 21 Sep 2022 23:37

Tgt Ion: 43 Resp: 23690


Ion	Ratio	Lower	Upper
43	100		
45	18.6	8.2	12.4#
61	13.3	8.3	12.5#
70	7.7	5.9	8.9

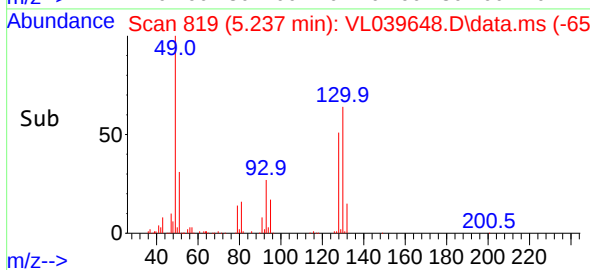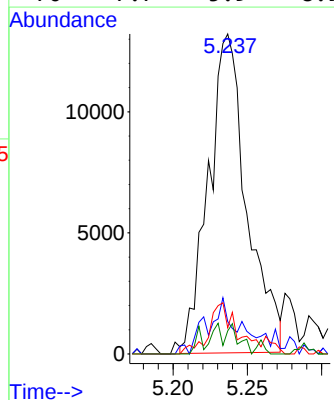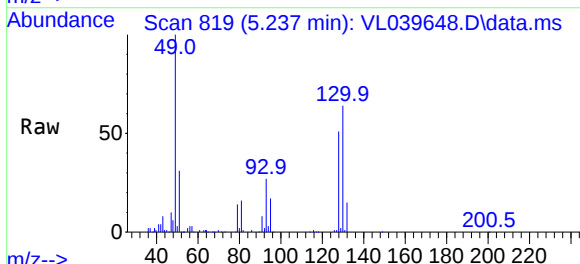






#26
Hexane
Concen: 0.067 ppbv
RT: 5.240 min Scan# 81
Delta R.T. 0.017 min
Lab File: VL039648.D
Acq: 21 Sep 2022 23:37

Instrument :
MSVOA_L
ClientSampleId :

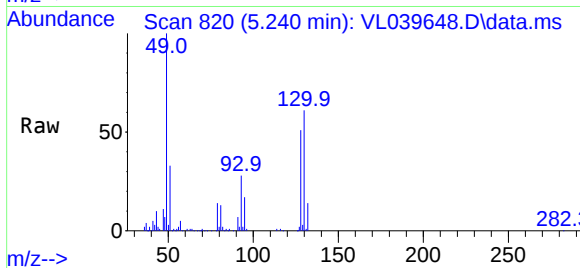

Tgt Ion: 57 Resp: 7493




Ion	Ratio	Lower	Upper
57	100		
41	188.0	76.9	115.3#
43	381.9	191.0	286.6#
56	98.0	43.2	64.8#

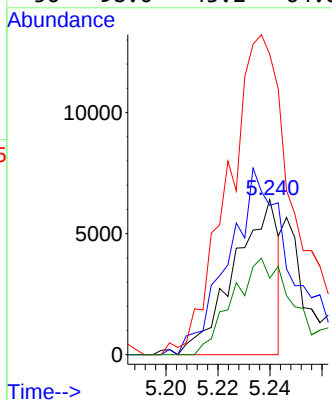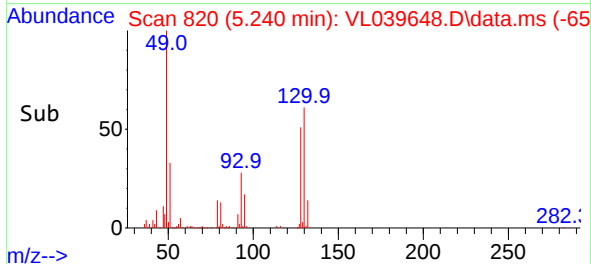


#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.671 min Scan# 1265
Delta R.T. 0.010 min
Lab File: VL039648.D
Acq: 21 Sep 2022 23:37

Tgt Ion: 114 Resp: 2812926

Ion	Ratio	Lower	Upper
114	100		
63	25.5	20.2	30.4
88	18.4	14.5	21.7

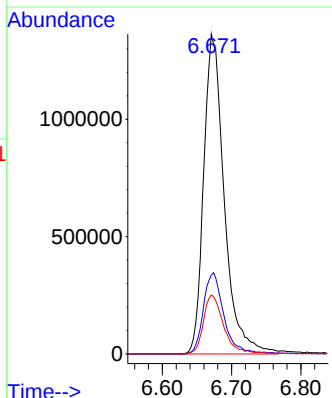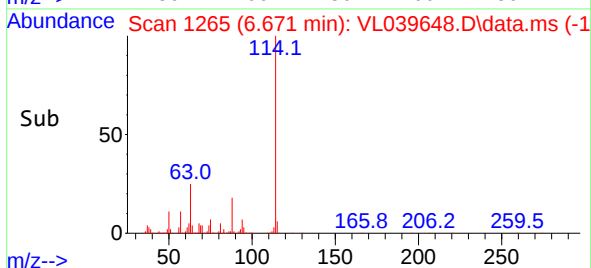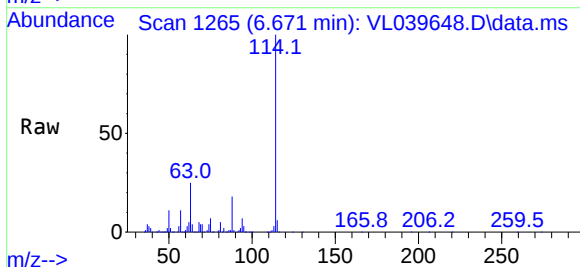



#34

2-Butanone

Concen: 0.055 ppbv

RT: 4.819 min Scan# 61

Delta R.T. 0.017 min

Lab File: VL039648.D

Acq: 21 Sep 2022 23:37

Instrument :

MSVOA_L





ClientSampleId :

Tgt Ion: 43 Resp: 7590

Ion Ratio Lower Upper

43 100

72 0.0 17.9 26.9#

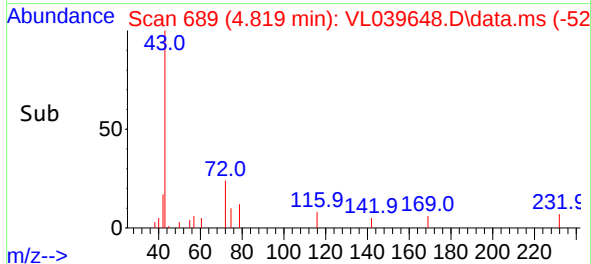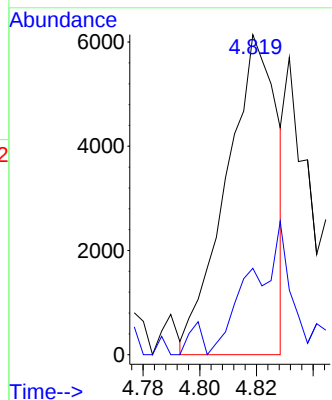

#39

1,2-Dichloropropane

Concen: 8.296 ppbv

RT: 6.674 min Scan# 1266

Delta R.T. -0.408 min

Lab File: VL039648.D

Acq: 21 Sep 2022 23:37




Tgt Ion: 63 Resp: 688894


Ion Ratio Lower Upper

63 100

41 0.0 59.6 89.4#

62 18.8 51.4 77.0#

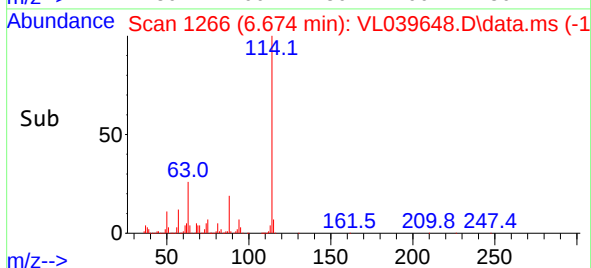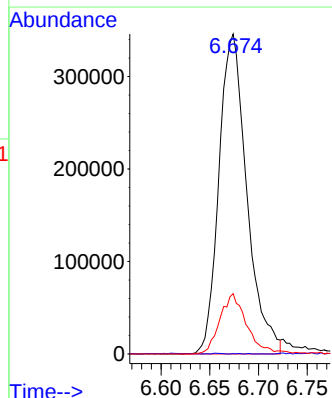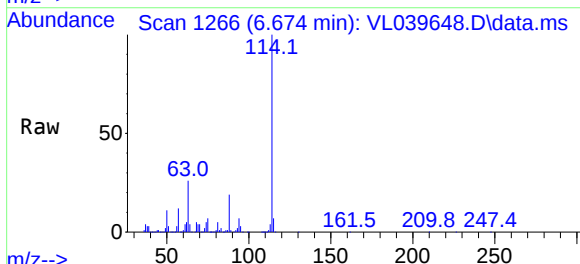




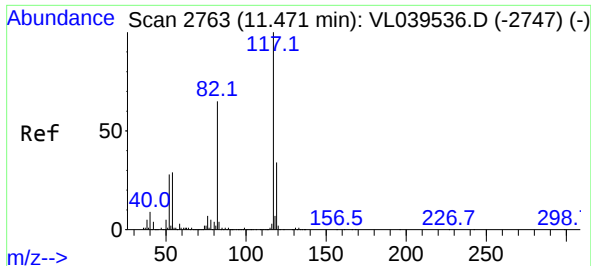


#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.484 min Scan# 21
Delta R.T. 0.013 min
Lab File: VL039648.D
Acq: 21 Sep 2022 23:37

Instrument :
MSVOA_L
ClientSampleId :

Tgt Ion: 117 Resp: 2567052




Ion	Ratio	Lower	Upper
117	100		
82	65.0	50.8	76.2
119	33.4	24.1	36.1

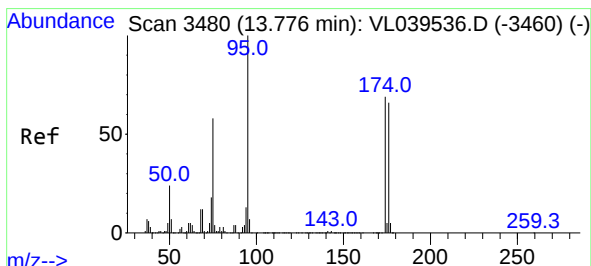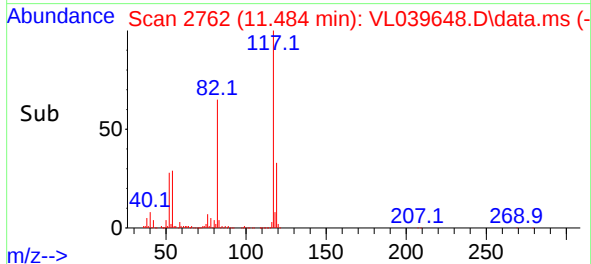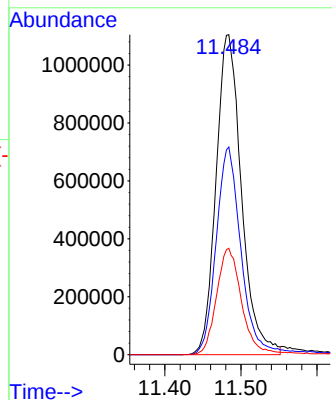


#68
1-Bromo-4-Fluorobenzene
Concen: 9.876 ppbv
RT: 13.793 min Scan# 3480
Delta R.T. 0.017 min
Lab File: VL039648.D
Acq: 21 Sep 2022 23:37

Tgt Ion: 95 Resp: 1892526


Ion	Ratio	Lower	Upper
95	100		
174	73.5	55.9	83.9
175	5.4	4.2	6.4

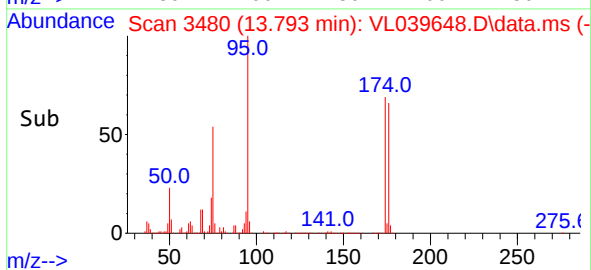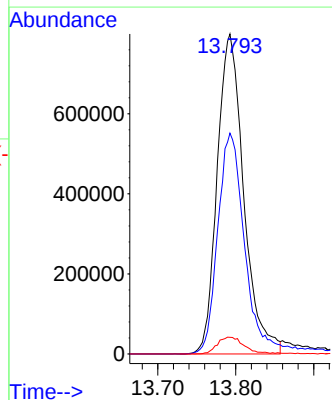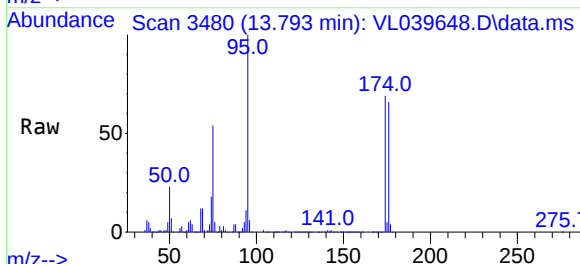

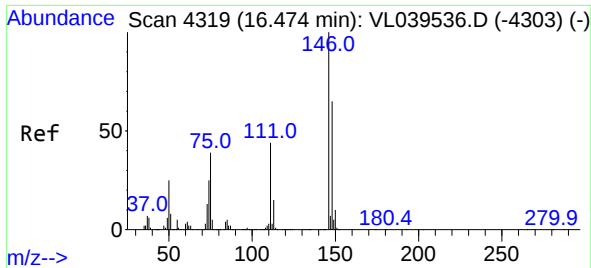

#76
 1,4-Dichlorobenzene
 Concen: 0.145 ppbv
 RT: 16.493 min Scan# 41
 Delta R.T. 0.020 min
 Lab File: VL039648.D
 Acq: 21 Sep 2022 23:37

Instrument :
 MSVOA_L
 ClientSampleId :

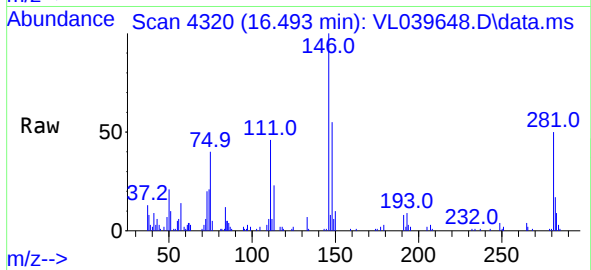

Tgt Ion:146 Resp: 25567
 Ion Ratio Lower Upper
 146 100
 111 117.2 22.9 68.8#
 148 176.0 33.6 100.8#

