
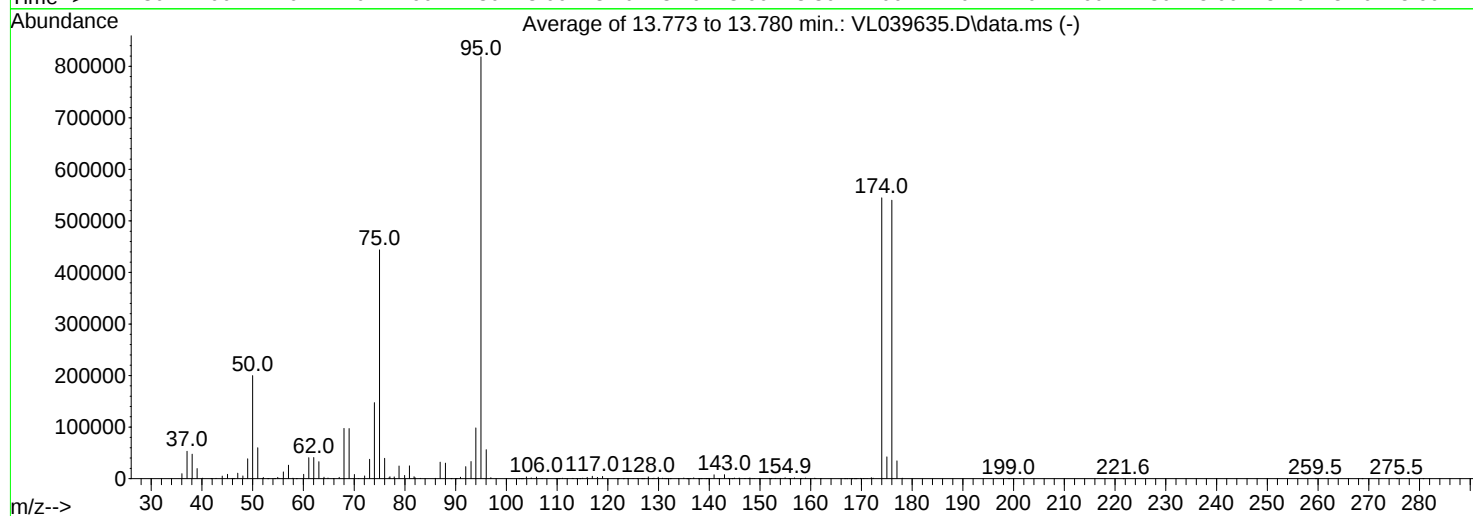


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL092122\
 Data File : VL039635.D
 Acq On : 21 Sep 2022 12:12
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091922AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Mon Sep 19 14:26:28 2022

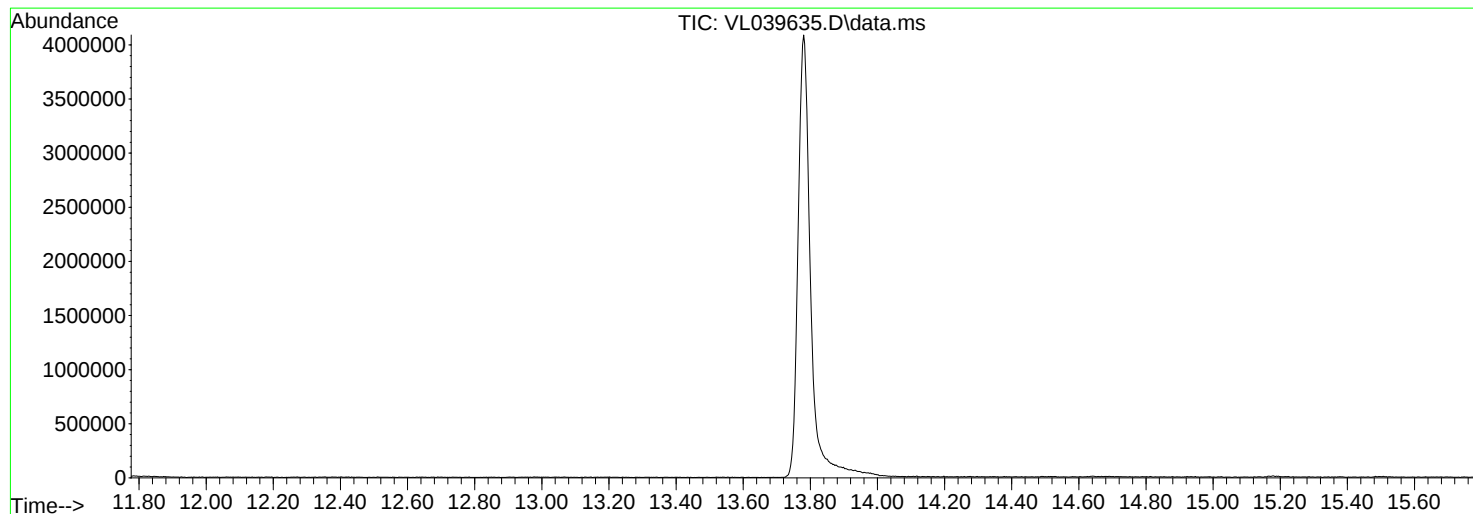

AutoFind: Scans 3474, 3475, 3476; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	200085	PASS
75	95	30	66	54.3	444032	PASS
95	95	100	100	100.0	818347	PASS
96	95	5	9	6.9	56149	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	66.6	544960	PASS
175	174	4	9	7.8	42285	PASS
176	174	93	101	99.1	540011	PASS
177	176	5	9	6.4	34616	PASS

Average of 13.773 to 13.780 min.: VL039635.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	9683	47.05	10675	55.20	597	65.95	361
37.05	53237	48.05	5202	56.05	13114	67.05	255
38.05	47374	49.00	38596	57.05	25971	68.00	9744
39.05	19501	50.00	200085	57.95	1108	69.00	9727
40.10	814	51.00	59928	58.60	125	70.05	7941
41.80	152	51.90	579	60.05	8434	70.90	273
42.75	600	52.10	2098	61.05	40824	72.05	5319
44.00	5003	52.95	173	62.05	41045	73.05	37517
45.05	8336	53.20	362	63.05	33027	74.00	147371
45.95	497	54.30	112	64.05	2680	75.00	444032
46.20	191	54.95	2593	64.85	1340	76.00	39360

Average of 13.773 to 13.780 min.: VL039635.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.90	1754	88.00	30067	102.90	122	111.60	199
77.05	3675	89.10	73	103.20	137	112.00	360
77.90	3363	90.10	187	103.95	3579	113.00	586
78.85	24435	90.95	2790	104.90	1642	113.20	263
79.95	6135	92.00	23451	105.95	3292	113.90	59
80.90	25005	93.05	33224	106.85	326	114.50	111
81.80	3661	94.00	98312	107.10	246	115.05	1105
82.00	1841	95.00	818347	109.80	176	115.95	2477
83.05	631	96.05	56149	110.00	149	116.95	4743
86.00	710	96.95	1759	110.40	98	117.95	2486
86.95	32093	102.50	58	111.05	921	118.95	4397

Average of 13.773 to 13.780 min.: VL039635.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
121.90	108	129.10	987	136.30	212	142.00	289
122.10	63	129.95	2757	136.95	1566	143.00	7799
123.05	160	130.80	1036	137.90	109	143.85	491
123.90	451	131.10	463	138.30	138	144.50	115
124.10	289	131.40	76	138.60	257	144.95	1138
125.00	235	131.80	152	139.00	222	145.90	1154
125.85	324	132.30	71	139.30	123	146.90	393
126.70	156	133.95	273	139.70	314	147.10	319
127.05	160	135.00	1137	139.95	728	147.70	335
128.00	3315	135.60	80	140.95	7409	148.00	1337
128.80	402	135.80	121	141.70	369	148.60	383

Average of 13.773 to 13.780 min.: VL039635.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.95	394	159.00	1295	169.80	587	199.00	174
149.80	323	160.80	832	170.40	207	221.60	53
150.00	525	161.00	612	170.70	201	259.50	115
151.90	488	161.90	71	171.10	320	268.70	68
152.10	113	166.70	178	171.95	1809	275.50	85
153.00	720	167.10	57	172.30	819	280.70	58
154.05	658	167.70	258	174.00	544960		
154.95	1813	168.10	126	175.00	42285		
155.70	61	168.60	167	176.00	540011		
156.80	1515	168.90	82	177.00	34616		
158.05	138	169.30	348	178.05	1079		