


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL092222\
Data File : VL039667.D
Acq On : 22 Sep 2022 14:48
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091922AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Mon Sep 19 14:26:28 2022

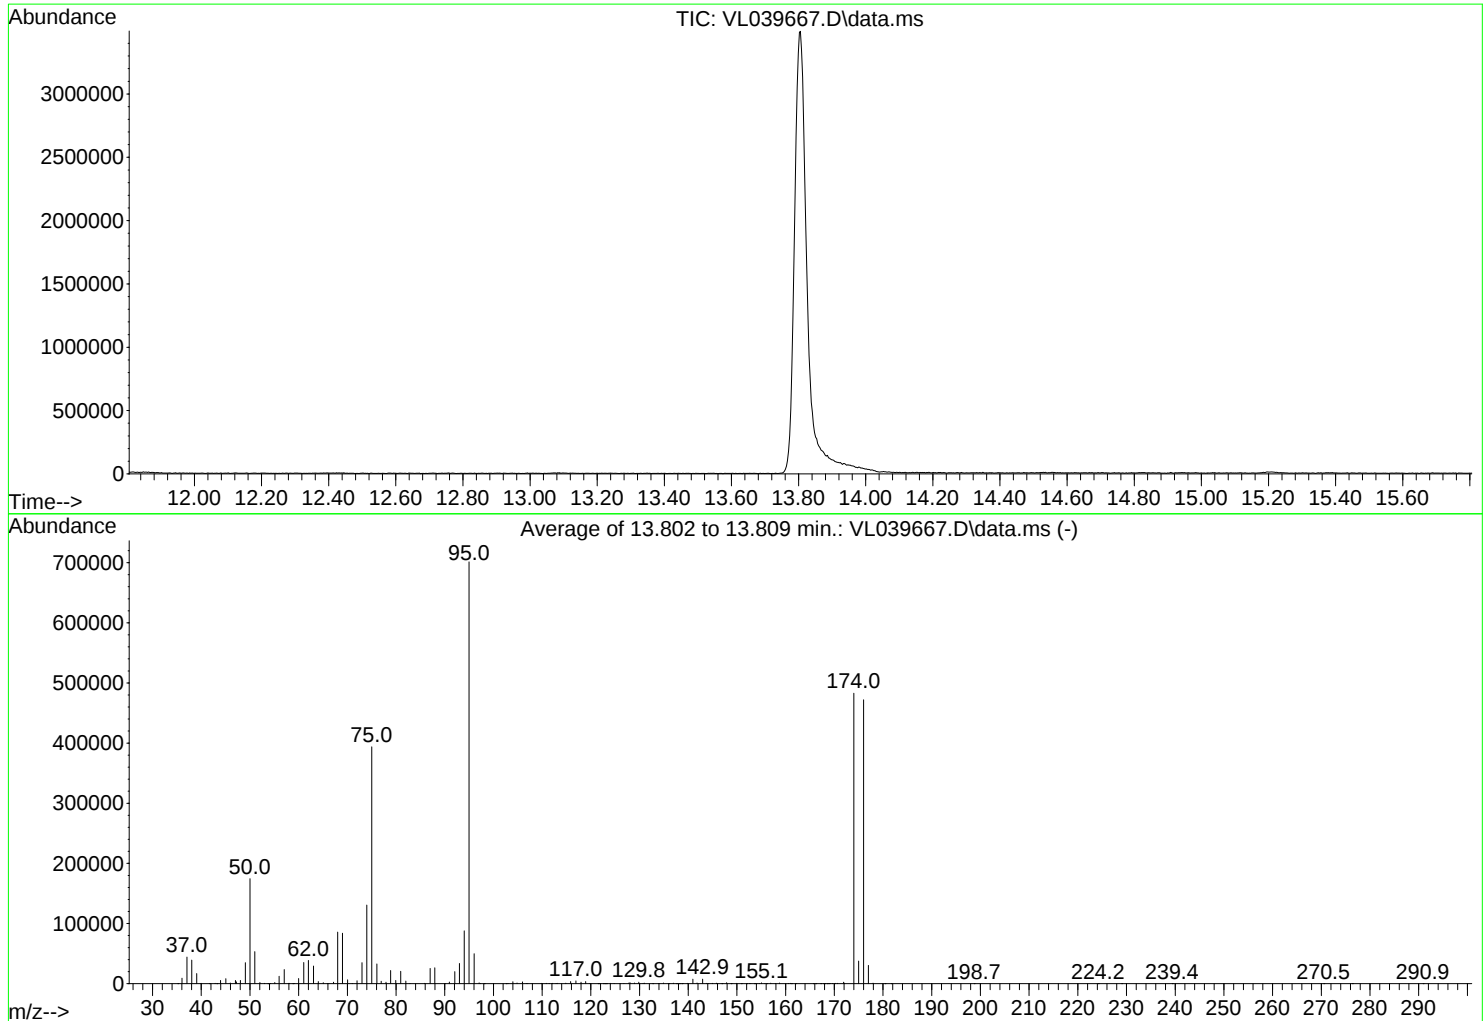

AutoFind: Scans 3483, 3484, 3485; Background Corrected with Scan 3462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.9	174613	PASS
75	95	30	66	56.1	393771	PASS
95	95	100	100	100.0	701419	PASS
96	95	5	9	7.1	49640	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.9	483008	PASS
175	174	4	9	7.8	37645	PASS
176	174	93	101	97.7	471915	PASS
177	176	5	9	6.4	30299	PASS

Average of 13.802 to 13.809 min.: VL039667.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.20	147	45.95	1176	55.10	1988	64.05	339
36.05	8984	47.00	5369	56.00	12204	65.05	164
37.05	44133	47.20	2937	57.05	23467	65.90	21
38.05	39083	48.05	5347	57.90	659	66.20	22
39.05	16836	49.05	34877	58.10	417	67.15	2375
39.95	591	50.00	174613	58.80	92	68.00	85611
41.70	100	51.00	53163	59.10	271	69.00	83715
42.85	450	52.05	1986	60.00	8483	70.05	6388
43.20	83	53.00	583	61.05	35093	71.00	247
43.95	5326	53.70	114	62.00	38483	72.00	4899
45.05	8218	54.20	206	63.05	29253	73.00	34987

Average of 13.802 to 13.809 min.: VL039667.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.00	130544	87.00	25277	98.10	61	110.85	556
75.00	393771	87.95	26296	102.60	86	111.45	312
76.05	32715	90.10	260	103.00	265	112.00	234
76.95	3956	90.95	2687	104.00	3181	112.15	505
77.95	2442	92.05	20027	104.85	1138	112.85	378
78.90	21925	93.00	33587	105.95	2966	113.10	423
79.95	5321	94.00	87829	106.75	398	114.85	722
80.95	20571	95.00	701419	107.05	362	115.85	3525
82.00	4269	96.05	49640	107.95	206	116.95	4481
82.85	402	97.05	1416	109.80	697	118.00	2445
85.90	424	97.30	191	110.05	373	118.95	3427

Average of 13.802 to 13.809 min.: VL039667.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.80	199	128.05	1581	136.95	952	144.95	575
121.50	138	128.95	1166	137.60	126	145.80	949
121.80	51	129.85	2558	138.20	85	146.00	279
122.60	119	130.75	549	138.70	132	146.90	144
122.90	55	131.00	712	138.95	244	147.05	261
123.20	69	132.70	79	139.80	609	147.90	1515
124.00	684	133.90	340	140.95	7494	148.80	154
124.80	316	134.10	405	141.80	1002	148.95	401
126.00	191	134.90	1215	142.95	7551	149.95	667
126.80	187	135.90	70	143.80	600	150.90	60
127.80	1175	136.20	166	144.20	302	152.00	149

Average of 13.802 to 13.809 min.: VL039667.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
152.60	200	158.75	1020	168.80	54	177.95	760
152.85	304	160.60	339	169.15	214	180.40	127
153.60	129	161.00	447	169.65	211	181.70	73
153.90	372	161.20	157	170.20	526	198.70	89
154.10	186	162.00	54	170.65	610	224.20	108
154.60	213	165.70	73	171.90	2500	229.00	83
155.05	1302	166.20	81	172.10	726	239.40	69
155.75	203	167.20	138	174.00	483008	270.50	70
156.10	135	167.80	152	175.00	37645	276.40	50
156.95	906	168.00	69	176.00	471915	290.90	110
157.90	247	168.50	71	177.00	30299		