

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL092320\
 Data File : VL035720.D
 Acq On : 23 Sep 2020 15:46
 Operator : SY/AP
 Sample : QC092220 CAN 10258
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC092220 CAN 10258

Quant Time: Sep 24 11:53:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL092320AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed Sep 23 07:38:05 2020
 QLast Update : Wed Sep 23 07:38:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.68	49	1223850	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.19	114	4569929	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.11	117	4522225	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.45	95	3358977	9.91	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.10%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL092320\
Data File : VL035720.D
Acq On : 23 Sep 2020 15:46
Operator : SY/AP
Sample : QC092220 CAN 10258
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC092220 CAN 10258

Quant Time: Sep 24 11:53:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL092320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Sep 23 07:38:05 2020
QLast Update : Wed Sep 23 07:38:05 2020
Response via : Initial Calibration

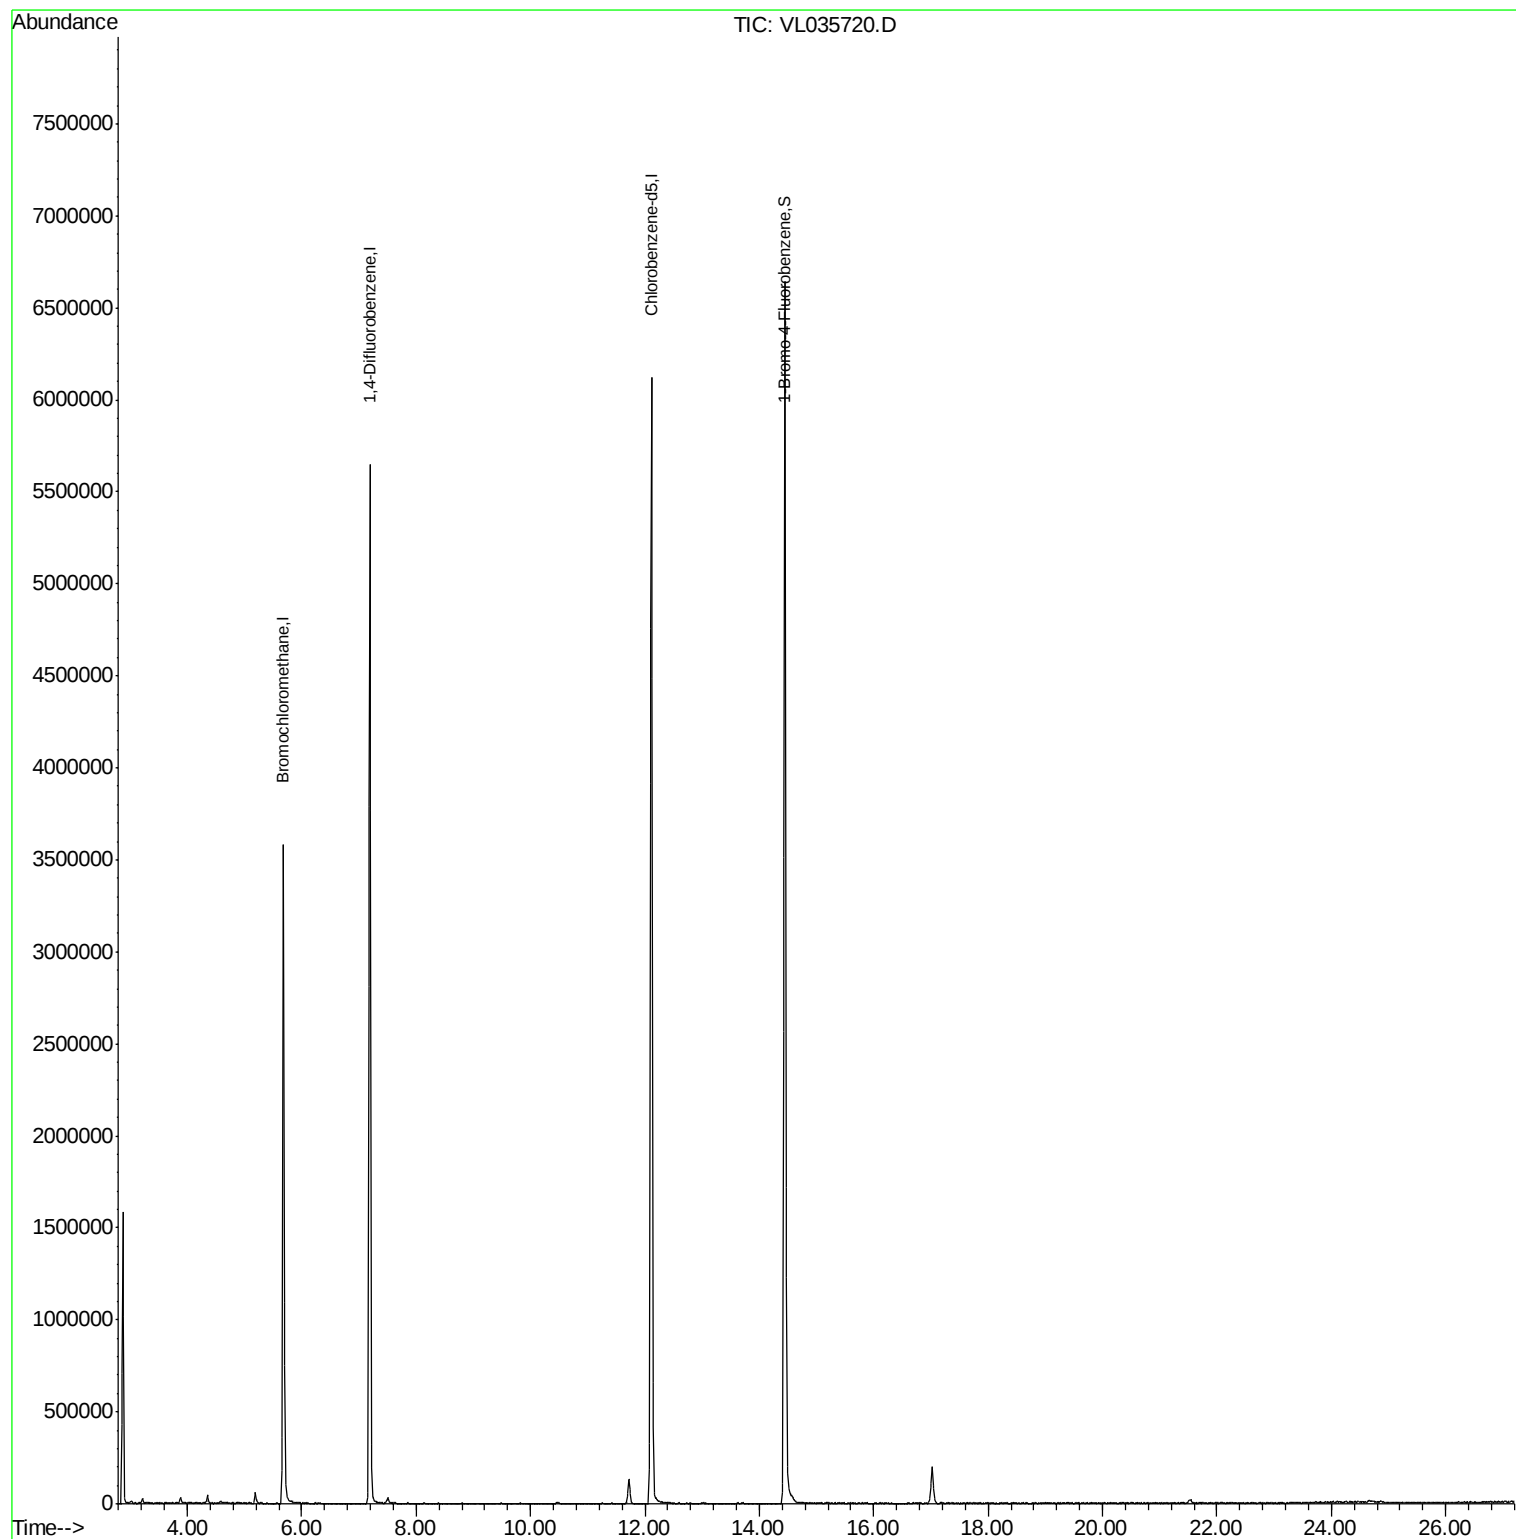

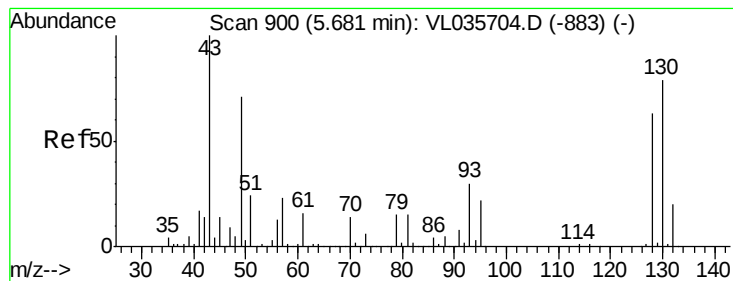

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.68 min Scan# 899

Delta R.T. -0.00 min

Lab File: VL035720.D

Acq: 23 Sep 2020 15:46

Instrument :

MSVOA_L

ClientSampleId :

QC092220 CAN 10258





Tot Ion: 49 Resp: 1223850

Ion Ratio Lower Upper

49 100

128 85.7 43.1 129.4

130 109.5 54.9 164.7

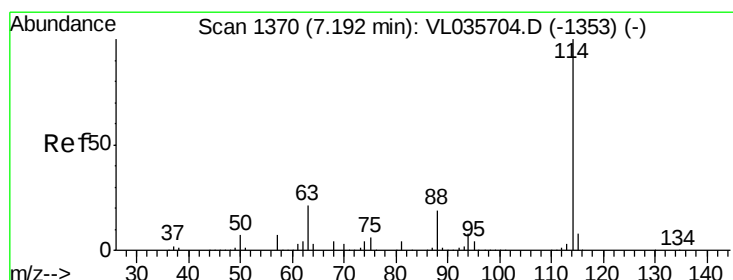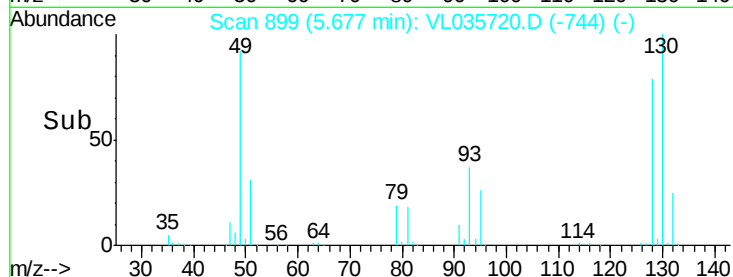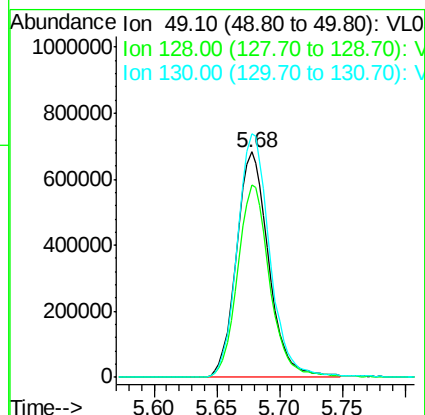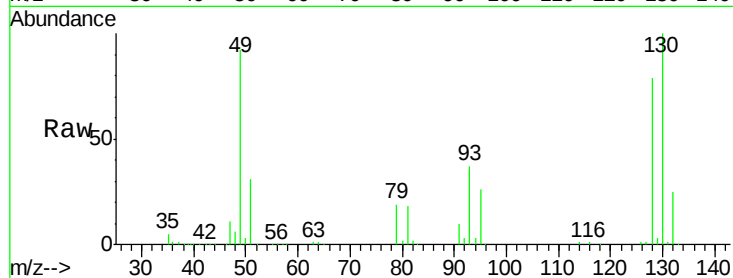

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.19 min Scan# 1369

Delta R.T. -0.00 min

Lab File: VL035720.D

Acq: 23 Sep 2020 15:46




Tgt Ion: 114 Resp: 4569929


Ion Ratio Lower Upper

114 100

63 19.8 16.1 24.1

88 17.5 14.1 21.1


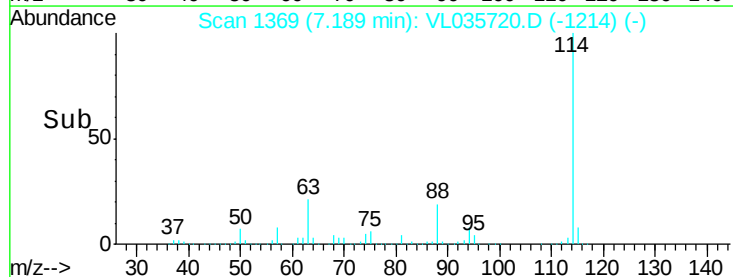
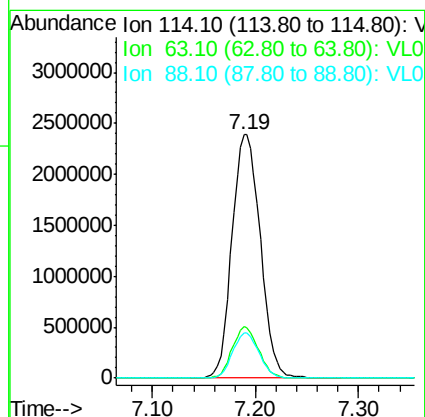
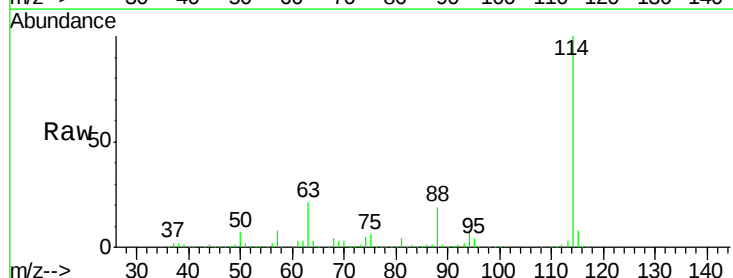


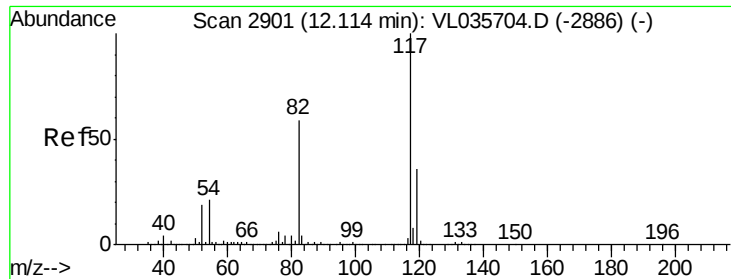

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.11 min Scan# 2900
Delta R.T. -0.00 min
Lab File: VL035720.D
Acq: 23 Sep 2020 15:46

Instrument :
MSVOA_L
ClientSampleId :
QC092220 CAN 10258

Tot Ion:117 Resp: 4522225
Ion Ratio Lower Upper
117 100
82 57.7 46.1 69.1
119 34.8 28.0 42.0

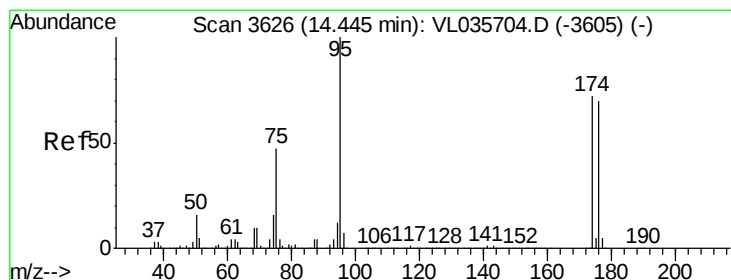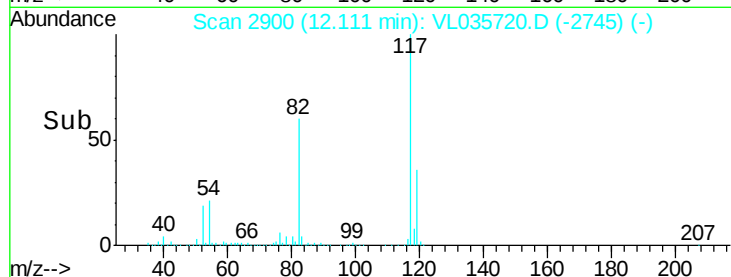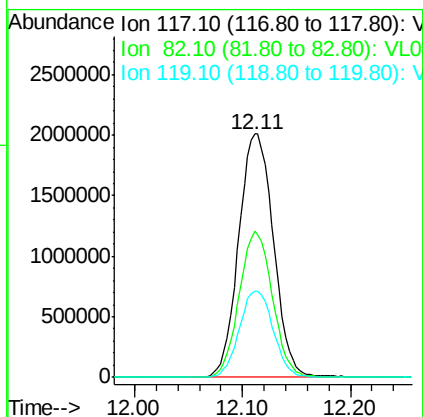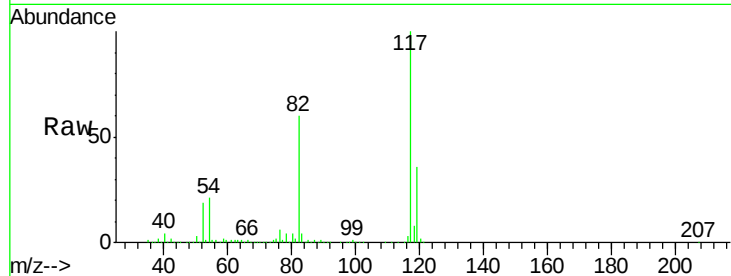

#68
1-Bromo-4-Fluorobenzene
Concen: 9.912 ppbv
RT: 14.45 min Scan# 3626
Delta R.T. 0.00 min
Lab File: VL035720.D
Acq: 23 Sep 2020 15:46

Tgt Ion: 95 Resp: 3358977
Ion Ratio Lower Upper
95 100
174 78.2 59.6 89.4
175 5.7 4.2 6.4

