

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL092320\
 Data File : VL035721.D
 Acq On : 23 Sep 2020 16:27
 Operator : SY/AP
 Sample : QC092220 CAN 10258
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC092220 CAN 10258

Quant Time: Sep 24 11:54:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL092320AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed Sep 23 07:38:05 2020
 QLast Update : Wed Sep 23 07:38:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.68	49	1048529	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.19	114	3900278	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.11	117	3913698	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.45	95	2872418	9.79	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	97.90%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL092320\
Data File : VL035721.D
Acq On : 23 Sep 2020 16:27
Operator : SY/AP
Sample : QC092220 CAN 10258
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC092220 CAN 10258

Quant Time: Sep 24 11:54:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL092320AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Sep 23 07:38:05 2020
QLast Update : Wed Sep 23 07:38:05 2020
Response via : Initial Calibration

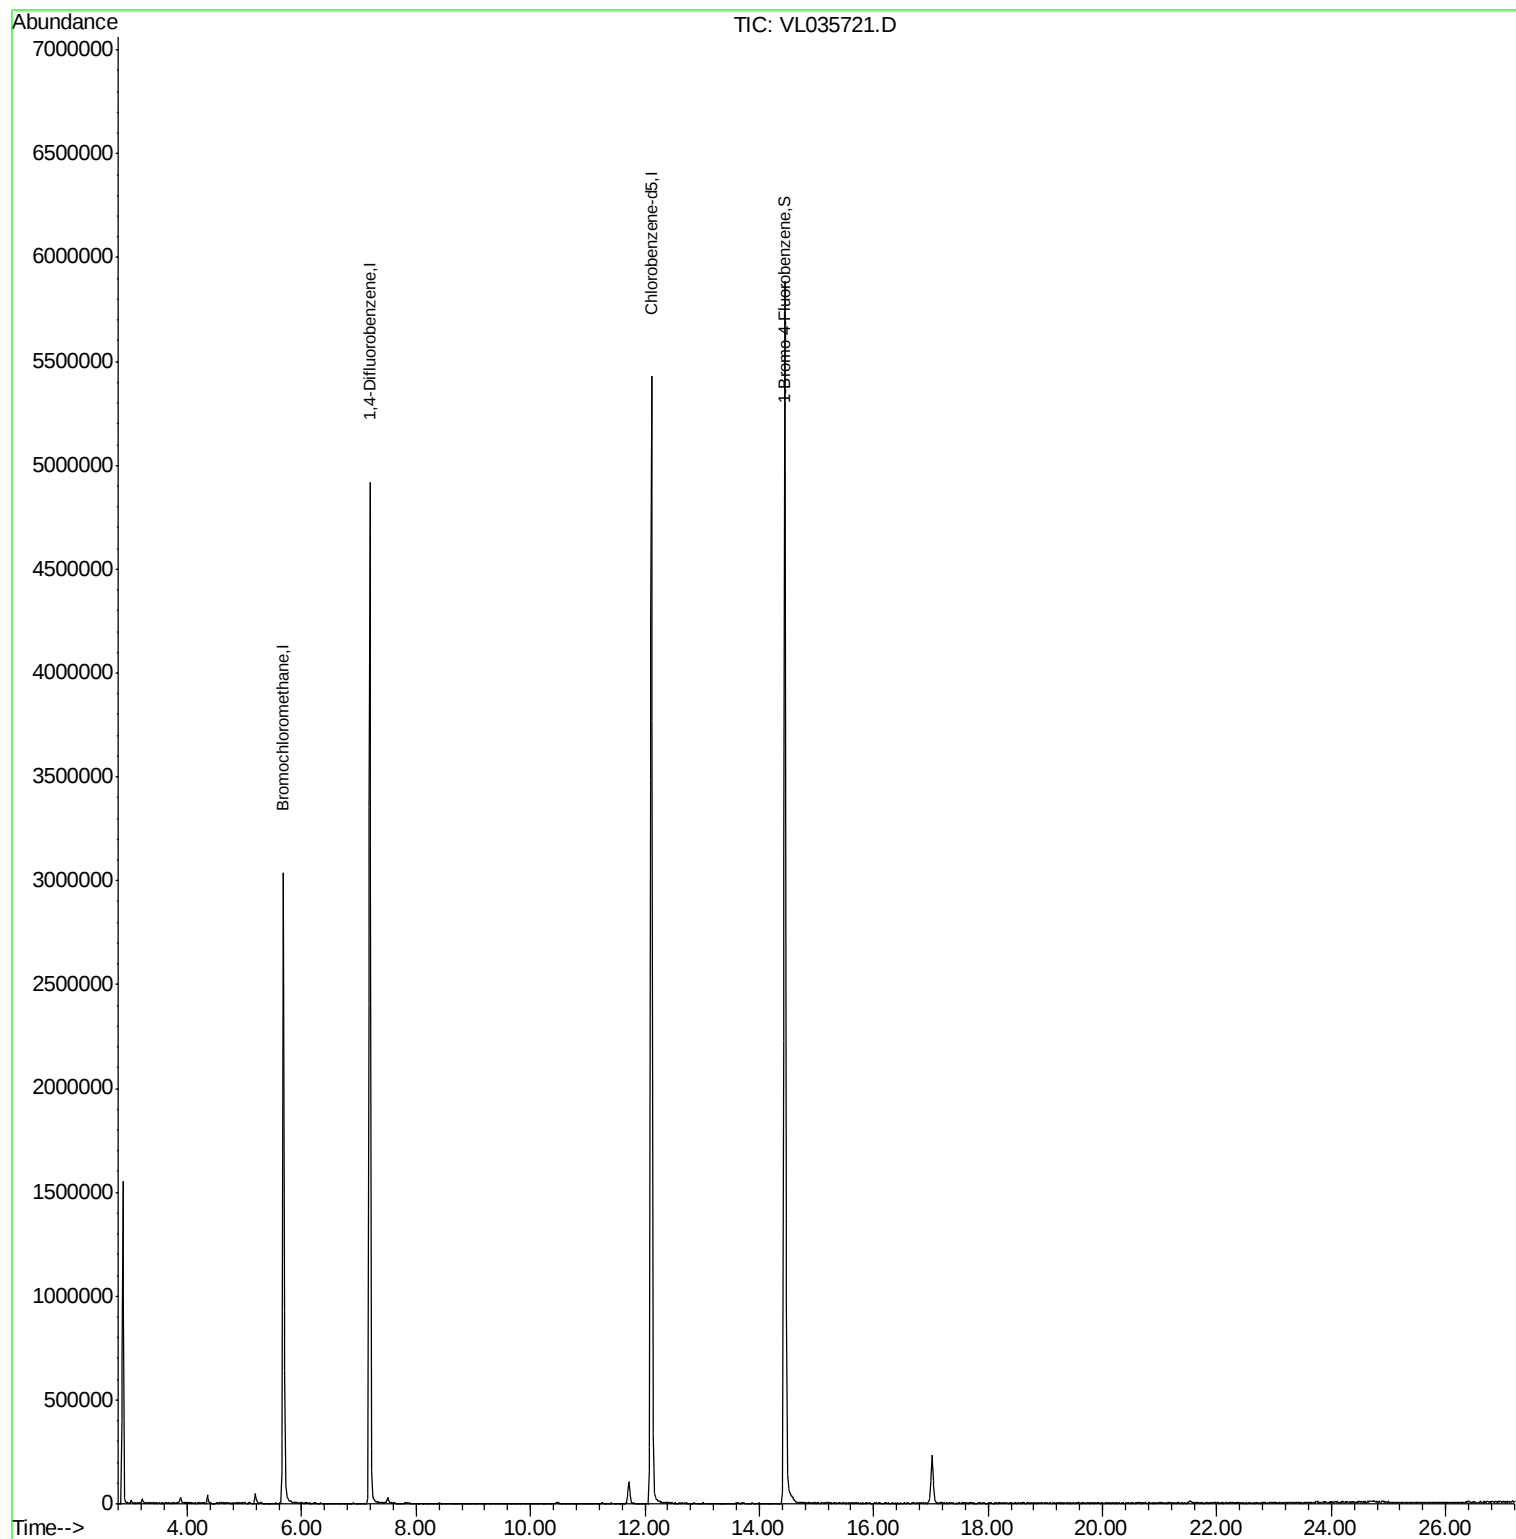

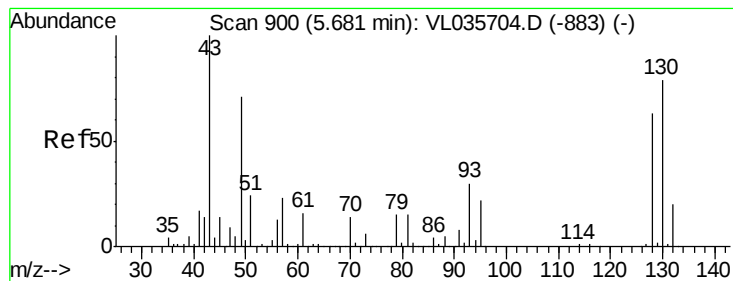

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.68 min Scan# 899

Delta R.T. -0.00 min

Lab File: VL035721.D

Acq: 23 Sep 2020 16:27

Instrument :

MSVOA_L

ClientSampleId :

QC092220 CAN 10258


Tot Ion: 49 Resp: 1048529

Ion Ratio Lower Upper

49 100

128 85.1 43.1 129.4




130 109.3 54.9 164.7

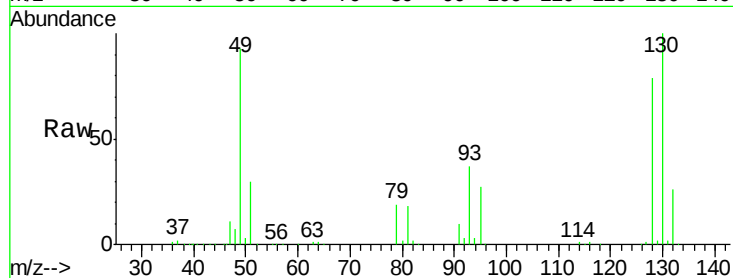

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

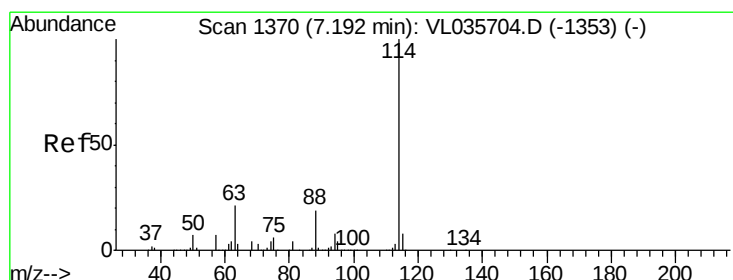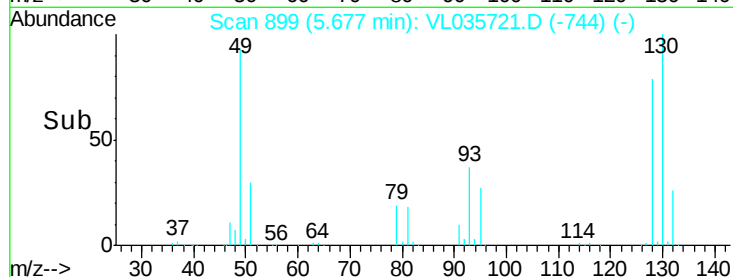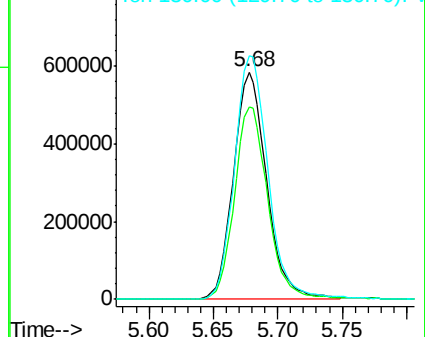

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.19 min Scan# 1370

Delta R.T. 0.00 min

Lab File: VL035721.D

Acq: 23 Sep 2020 16:27


Tgt Ion: 114 Resp: 3900278

Ion Ratio Lower Upper

114 100

63 19.6 16.1 24.1



88 17.3 14.1 21.1

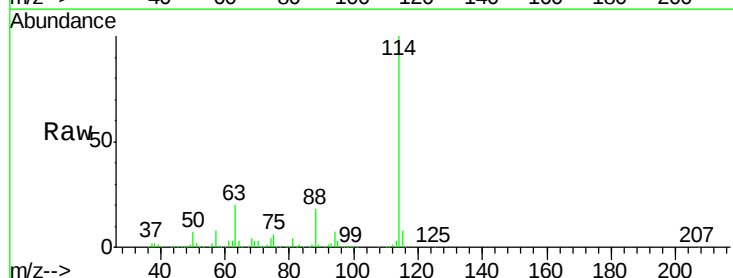


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



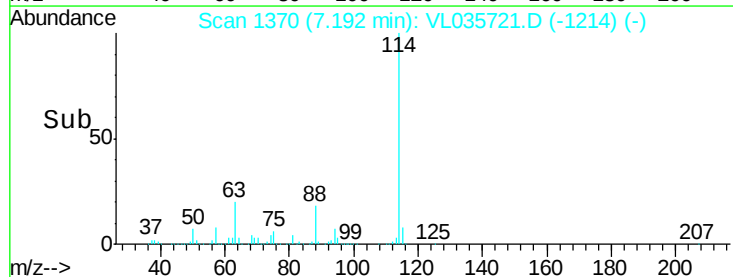
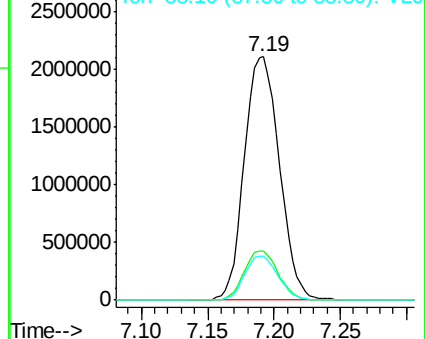


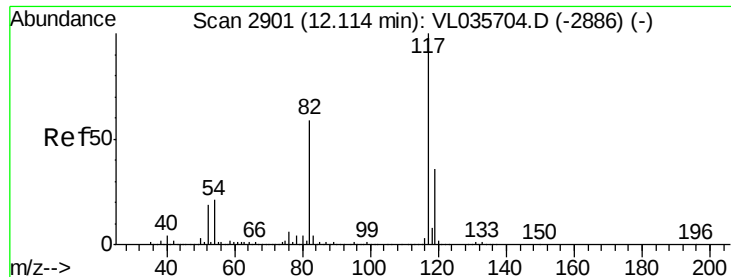

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.11 min Scan# 2900
Delta R.T. -0.00 min
Lab File: VL035721.D
Acq: 23 Sep 2020 16:27

Instrument :
MSVOA_L
ClientSampleId :
QC092220 CAN 10258

Tot Ion:117 Resp: 3913698
Ion Ratio Lower Upper
117 100
82 57.5 46.1 69.1
119 34.3 28.0 42.0

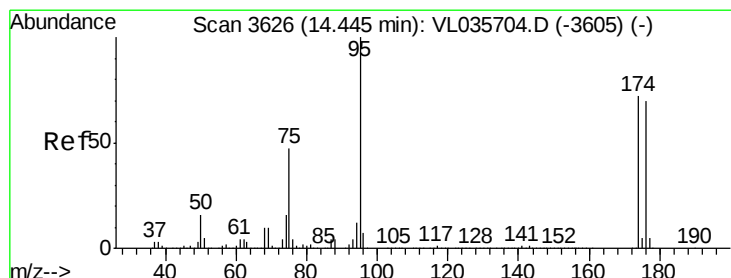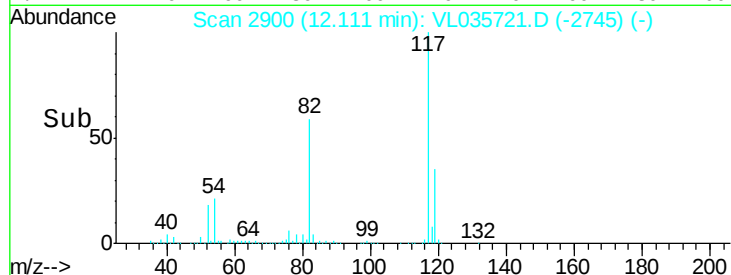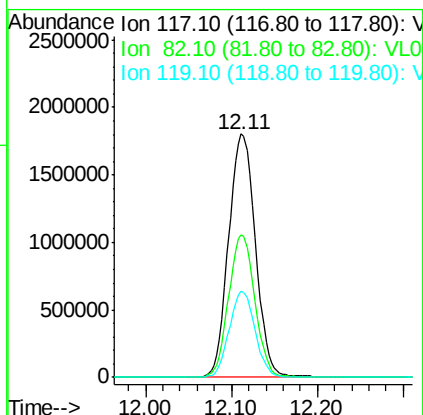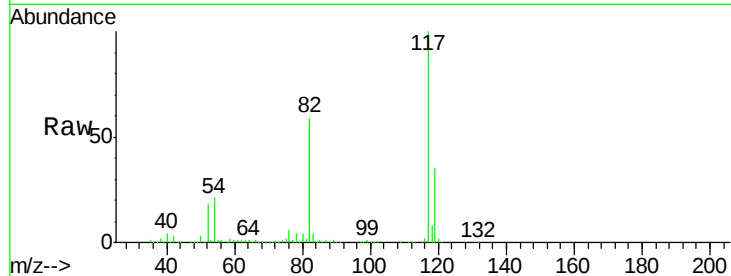

#68
1-Bromo-4-Fluorobenzene
Concen: 9.794 ppbv
RT: 14.45 min Scan# 3626
Delta R.T. 0.00 min
Lab File: VL035721.D
Acq: 23 Sep 2020 16:27

Tgt Ion: 95 Resp: 2872418
Ion Ratio Lower Upper
95 100
174 78.9 59.6 89.4
175 5.6 4.2 6.4

