


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL092320\  
 Data File : VL035703.D  
 Acq On : 23 Sep 2020 2:05  
 Operator : SY/AP  
 Sample : BFB  
 Misc : 400ml/MSVOA L  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_L  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL092320AIR.M  
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA\_L Wed Sep 23 07:38:05 2020  
 Last Update : Wed Sep 23 07:38:05 2020

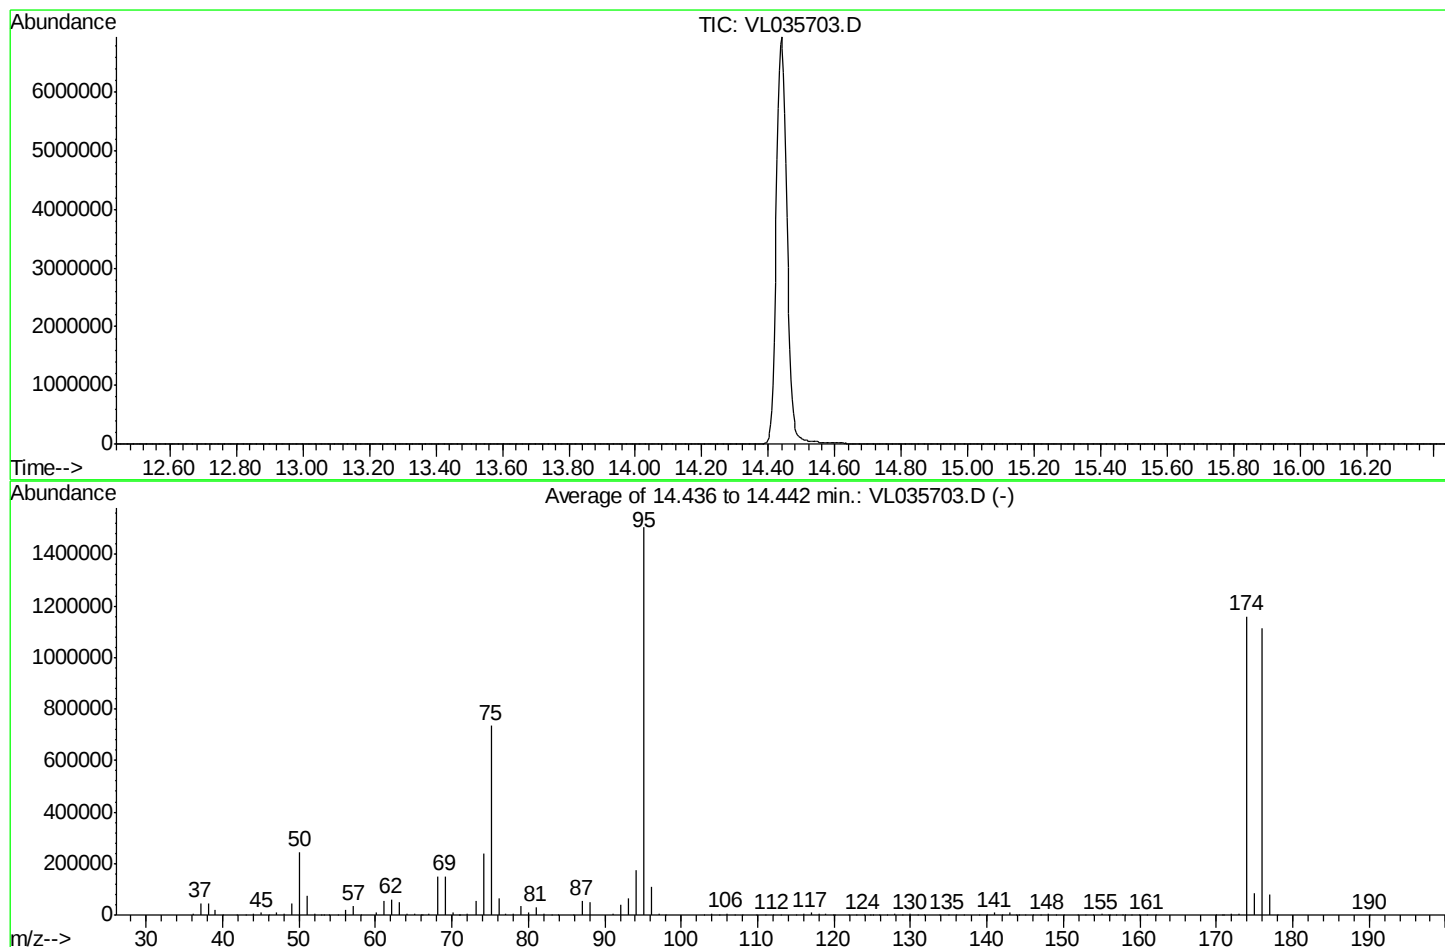

AutoFind: Scans 3623, 3624, 3625; Background Corrected with Scan 3597

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 8            | 40           | 16.2      | 244309  | PASS             |
| 75          | 95           | 30           | 66           | 48.8      | 734890  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 1505280 | PASS             |
| 96          | 95           | 5            | 9            | 7.4       | 111069  | PASS             |
| 173         | 174          | 0.00         | 2            | 0.5       | 6260    | PASS             |
| 174         | 95           | 50           | 120          | 77.0      | 1159338 | PASS             |
| 175         | 174          | 4            | 9            | 7.5       | 86501   | PASS             |
| 176         | 174          | 93           | 101          | 96.1      | 1113941 | PASS             |
| 177         | 176          | 5            | 9            | 7.2       | 80221   | PASS             |