
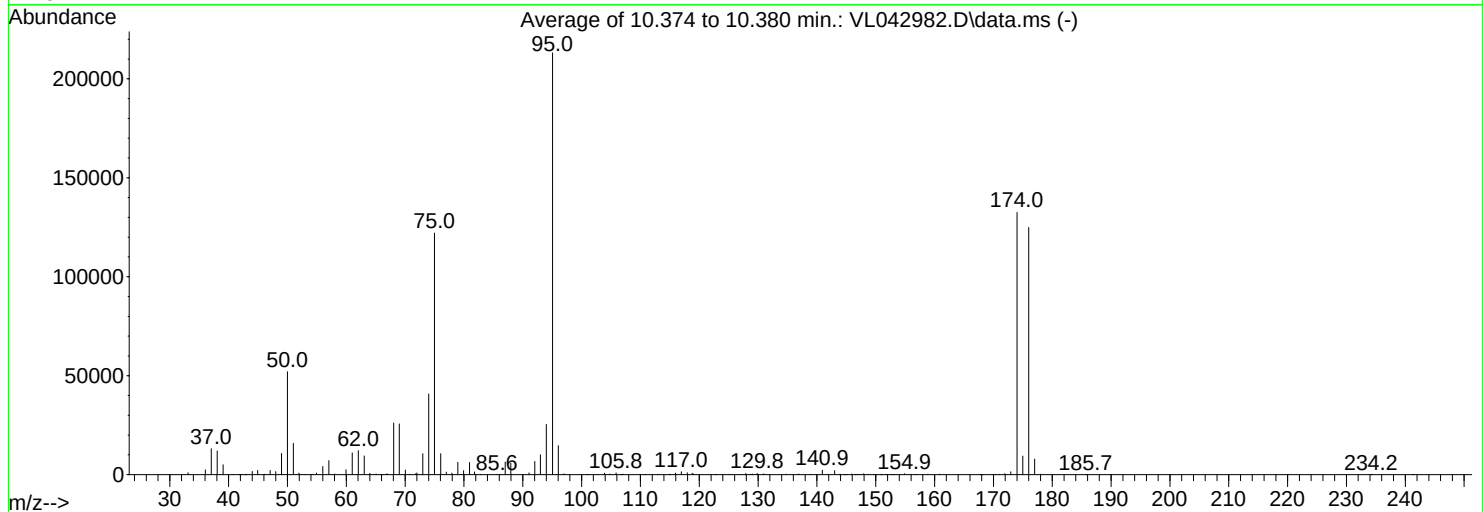


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL092325\
Data File : VL042982.D
Acq On : 23 Sep 2025 08:30
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL092225AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Sep 23 02:39:16 2025

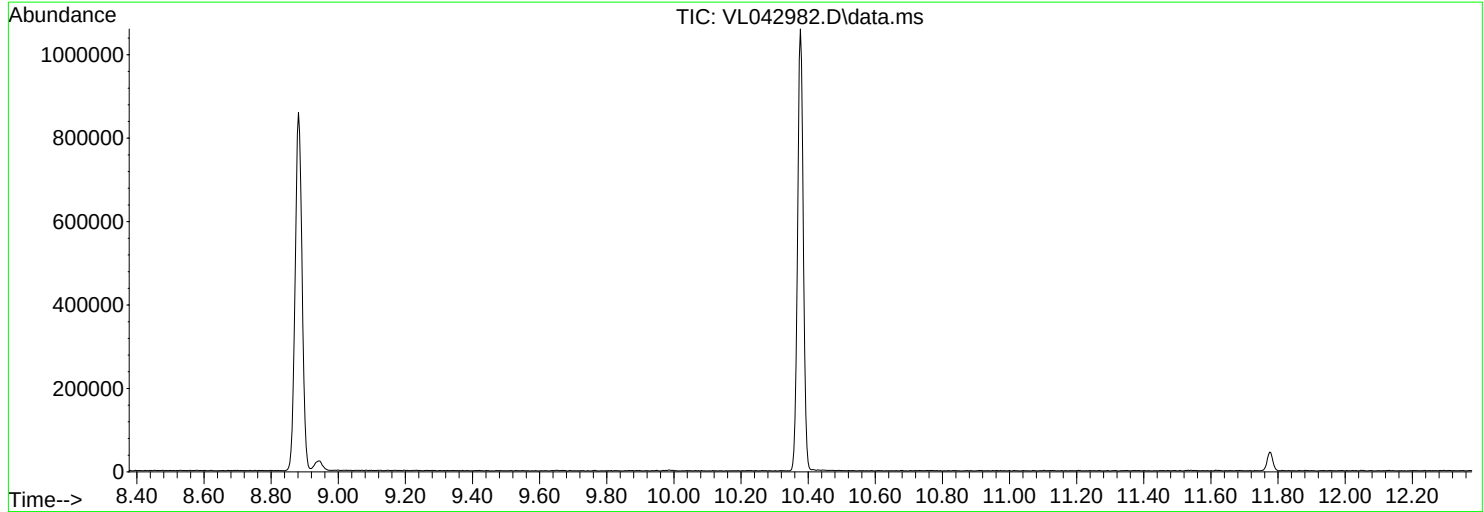

AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	52027	PASS
75	95	30	66	57.3	122083	PASS
95	95	100	100	100.0	213141	PASS
96	95	5	9	6.9	14633	PASS
173	174	0.00	2	1.1	1487	PASS
174	95	50	120	62.2	132544	PASS
175	174	4	9	7.1	9369	PASS
176	174	93	101	94.3	124939	PASS
177	176	5	9	6.3	7833	PASS

Average of 10.374 to 10.380 min.: VL042982.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1015	44.95	2127	56.00	4143	66.95	411
36.05	2397	46.15	210	57.05	7144	68.05	2612
37.05	13103	47.05	2101	58.05	345	69.00	2561
38.05	11973	48.00	1573	59.95	2498	70.05	232
39.05	5025	49.00	10713	61.00	10975	70.80	72
40.80	49	50.00	52027	62.05	12162	71.80	450
41.80	23	51.00	15871	63.05	9491	72.00	885
42.00	32	51.95	788	64.00	671	73.00	10564
42.80	29	52.95	56	65.05	355	74.00	40773
43.10	156	54.20	66	65.90	44	75.00	122083
44.00	1612	54.95	780	66.80	218	76.05	10589

Average of 10.374 to 10.380 min.: VL042982.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.00	1278	91.05	890	105.85	864	116.95	1446
77.95	852	92.05	6751	106.70	39	117.95	942
78.95	6271	93.00	10004	107.05	271	118.80	757
79.95	2066	94.00	25363	110.00	159	119.00	367
80.95	6188	95.05	213141	110.70	79	122.80	25
81.80	1379	96.05	14633	110.90	179	123.95	108
82.85	197	97.00	395	112.05	180	125.05	149
85.60	61	100.90	40	112.95	160	125.60	110
86.10	257	102.85	86	114.90	190	126.95	61
87.00	6377	103.90	747	115.10	161	127.90	575
87.95	5949	104.80	290	115.95	793	128.70	89

Average of 10.374 to 10.380 min.: VL042982.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
129.00	365	143.00	2024	149.70	187	158.05	51
129.85	662	143.80	48	149.90	46	158.85	275
130.95	378	143.95	257	150.90	47	160.85	219
134.80	275	144.70	32	151.75	144	167.70	46
135.90	64	145.10	200	152.65	94	168.00	31
136.60	92	145.95	297	153.00	47	169.90	50
136.95	365	146.50	27	154.05	97	170.10	52
138.90	133	146.85	97	154.90	531	170.40	57
139.95	78	147.10	68	156.00	158	170.95	168
140.90	2279	147.95	516	156.80	78	171.95	471
141.90	285	148.70	176	157.00	156	172.95	1487

Average of 10.374 to 10.380 min.: VL042982.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.00	132544						
175.00	9369						
176.00	124939						
177.00	7833						
178.00	228						
185.70	21						
234.20	24						
241.30	17						

Instrument :

MSVOA_L

ClientSampleId :

BFB