


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL092419\
 Data File : VL034196.D
 Acq On : 24 Sep 2019 9:41
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL091719AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Sep 18 12:53:31 2019
 Last Update : Wed Sep 18 12:53:31 2019

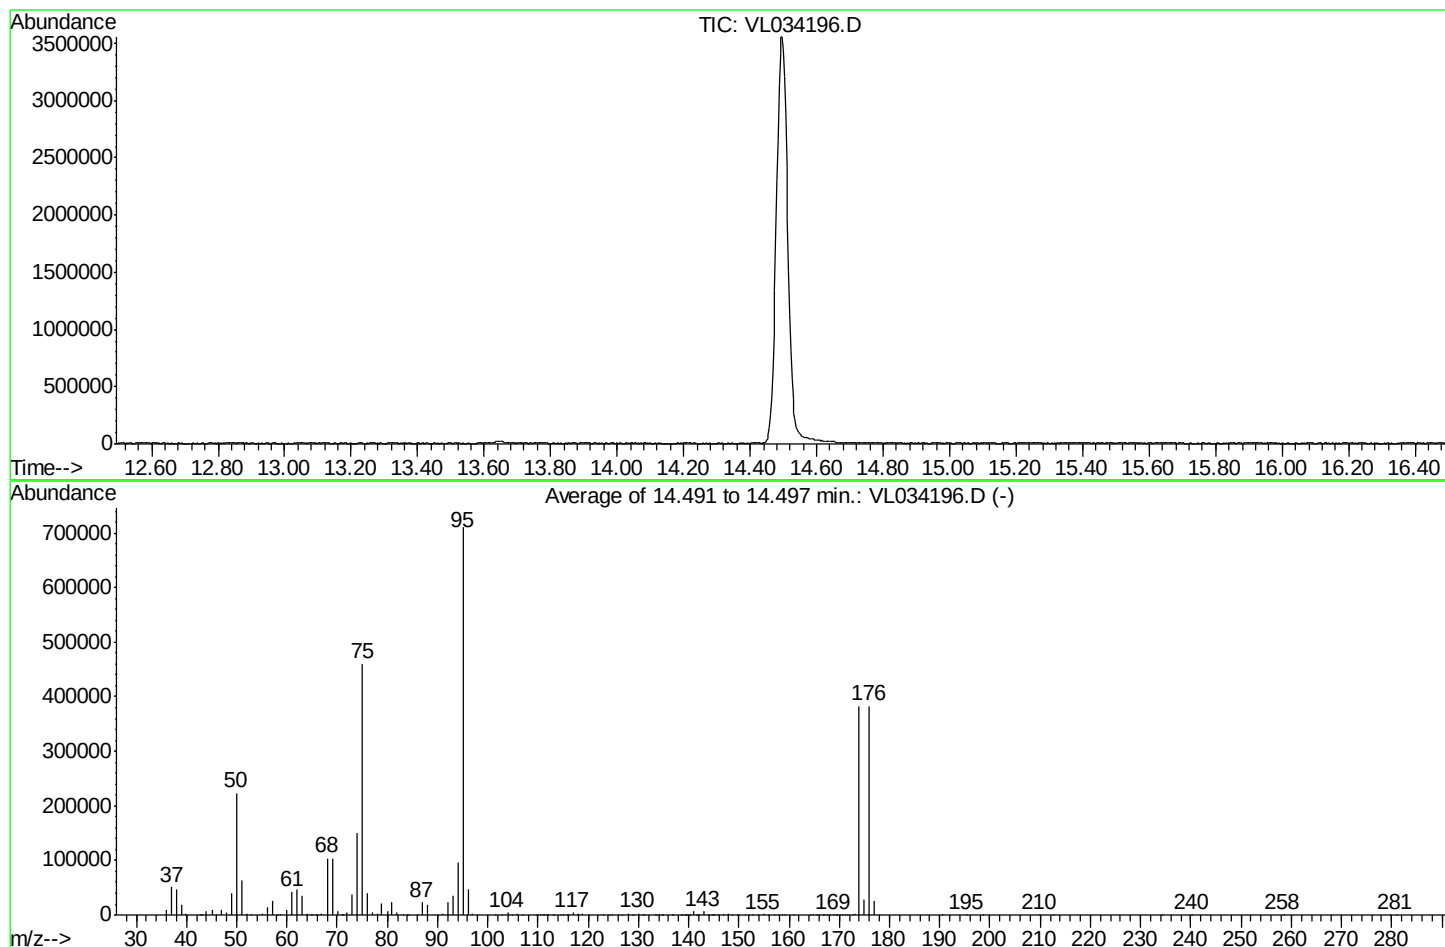

AutoFind: Scans 3640, 3641, 3642; Background Corrected with Scan 3612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	31.4	222912	PASS
75	95	30	66	64.9	460864	PASS
95	95	100	100	100.0	710378	PASS
96	95	5	9	6.6	47216	PASS
173	174	0.00	2	0.7	2590	PASS
174	95	50	120	54.0	383381	PASS
175	174	4	9	7.4	28389	PASS
176	174	93	101	100.0	383530	PASS
177	176	5	9	6.6	25381	PASS