

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL092524\
 Data File : VL041624.D
 Acq On : 25 Sep 2024 15:15
 Operator : SY/MD
 Sample : P4174-02
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :

Quant Time: Sep 26 01:20:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091624AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Sep 17 09:12:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.169	49	984915	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.632	114	2630467	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.449	117	2395289	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.761	95	1805386	10.239	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.400%


Target Compounds						Qvalue
2) Dichlorodifluoromethane	2.697	85	34707	0.244	ppbv	91
3) Chlorodifluoromethane	2.645	51	416875	3.490	ppbv	99
4) Chloromethane	2.784	50	33078	0.503	ppbv	95
9) Propene	2.674	41	77138	1.531	ppbv #	70
11) Trichlorofluoromethane	3.536	101	33046	0.218	ppbv	96
12) 1,1,2-Trichlorotrifluo...	4.041	101	4918	0.045	ppbv #	53
13) Ethanol	3.218	45	2004921	529.238	ppbv	95
15) Acetone	3.436	43	2905446	23.497	ppbv	100
16) 1,3-Butadiene	2.980	39	54116	0.900	ppbv #	13
17) tert-Butyl alcohol	3.874	59	28761	0.264	ppbv #	88
19) Isopropyl Alcohol	3.565	45	24001410	379.178	ppbv #	97
20) Methylene Chloride	3.906	84	23593	0.508	ppbv	97
21) Allyl Chloride	3.565	41	3970055	55.395	ppbv #	77
23) Vinyl Acetate	4.591	43	15948	0.234	ppbv #	1
25) Ethyl Acetate	5.189	43	20618	0.093	ppbv #	77
26) Hexane	5.189	57	9293	0.100	ppbv #	58
27) Carbon Disulfide	4.102	76	4857	0.049	ppbv #	66
29) Chloroform	5.250	83	102851	0.679	ppbv #	82
34) 2-Butanone	4.767	43	105134	0.838	ppbv	95
35) Carbon Tetrachloride	6.478	117	5849	0.045	ppbv #	87
36) Benzene	6.349	78	20609	0.113	ppbv	95
39) 1,2-Dichloropropane	6.629	63	654135	8.802	ppbv #	24
41) Tetrahydrofuran	5.539	42	4839	0.070	ppbv #	38
43) Methyl Methacrylate	7.455	69	13578	0.208	ppbv #	1
50) 4-Methyl-2-Pentanone	8.166	43	24504	0.127	ppbv #	84
53) Toluene	9.201	91	42438	0.219	ppbv	95
58) Ethyl Benzene	12.073	91	30455	0.119	ppbv	96
59) m/p-Xylene	12.327	91	169121	0.741	ppbv	95
60) o-Xylene	13.037	91	32925	0.150	ppbv #	30
61) Styrene	12.883	104	3076	0.034	ppbv #	1
71) 2-Chlorotoluene	14.899	91	84737	0.347	ppbv #	43
72) 4-Ethyltoluene	15.172	105	100202	0.392	ppbv #	95
73) 1,3,5-Trimethylbenzene	15.330	105	31464	0.139	ppbv	94
74) 1,2,4-Trimethylbenzene	16.092	105	253845	0.960	ppbv #	73
79) Naphthalene	21.358	128	9038	0.046	ppbv #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL092524\
Data File : VL041624.D
Acq On : 25 Sep 2024 15:15
Operator : SY/MD
Sample : P4174-02
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :

Quant Time: Sep 26 01:20:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091624AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue Sep 17 09:12:21 2024
Response via : Initial Calibration




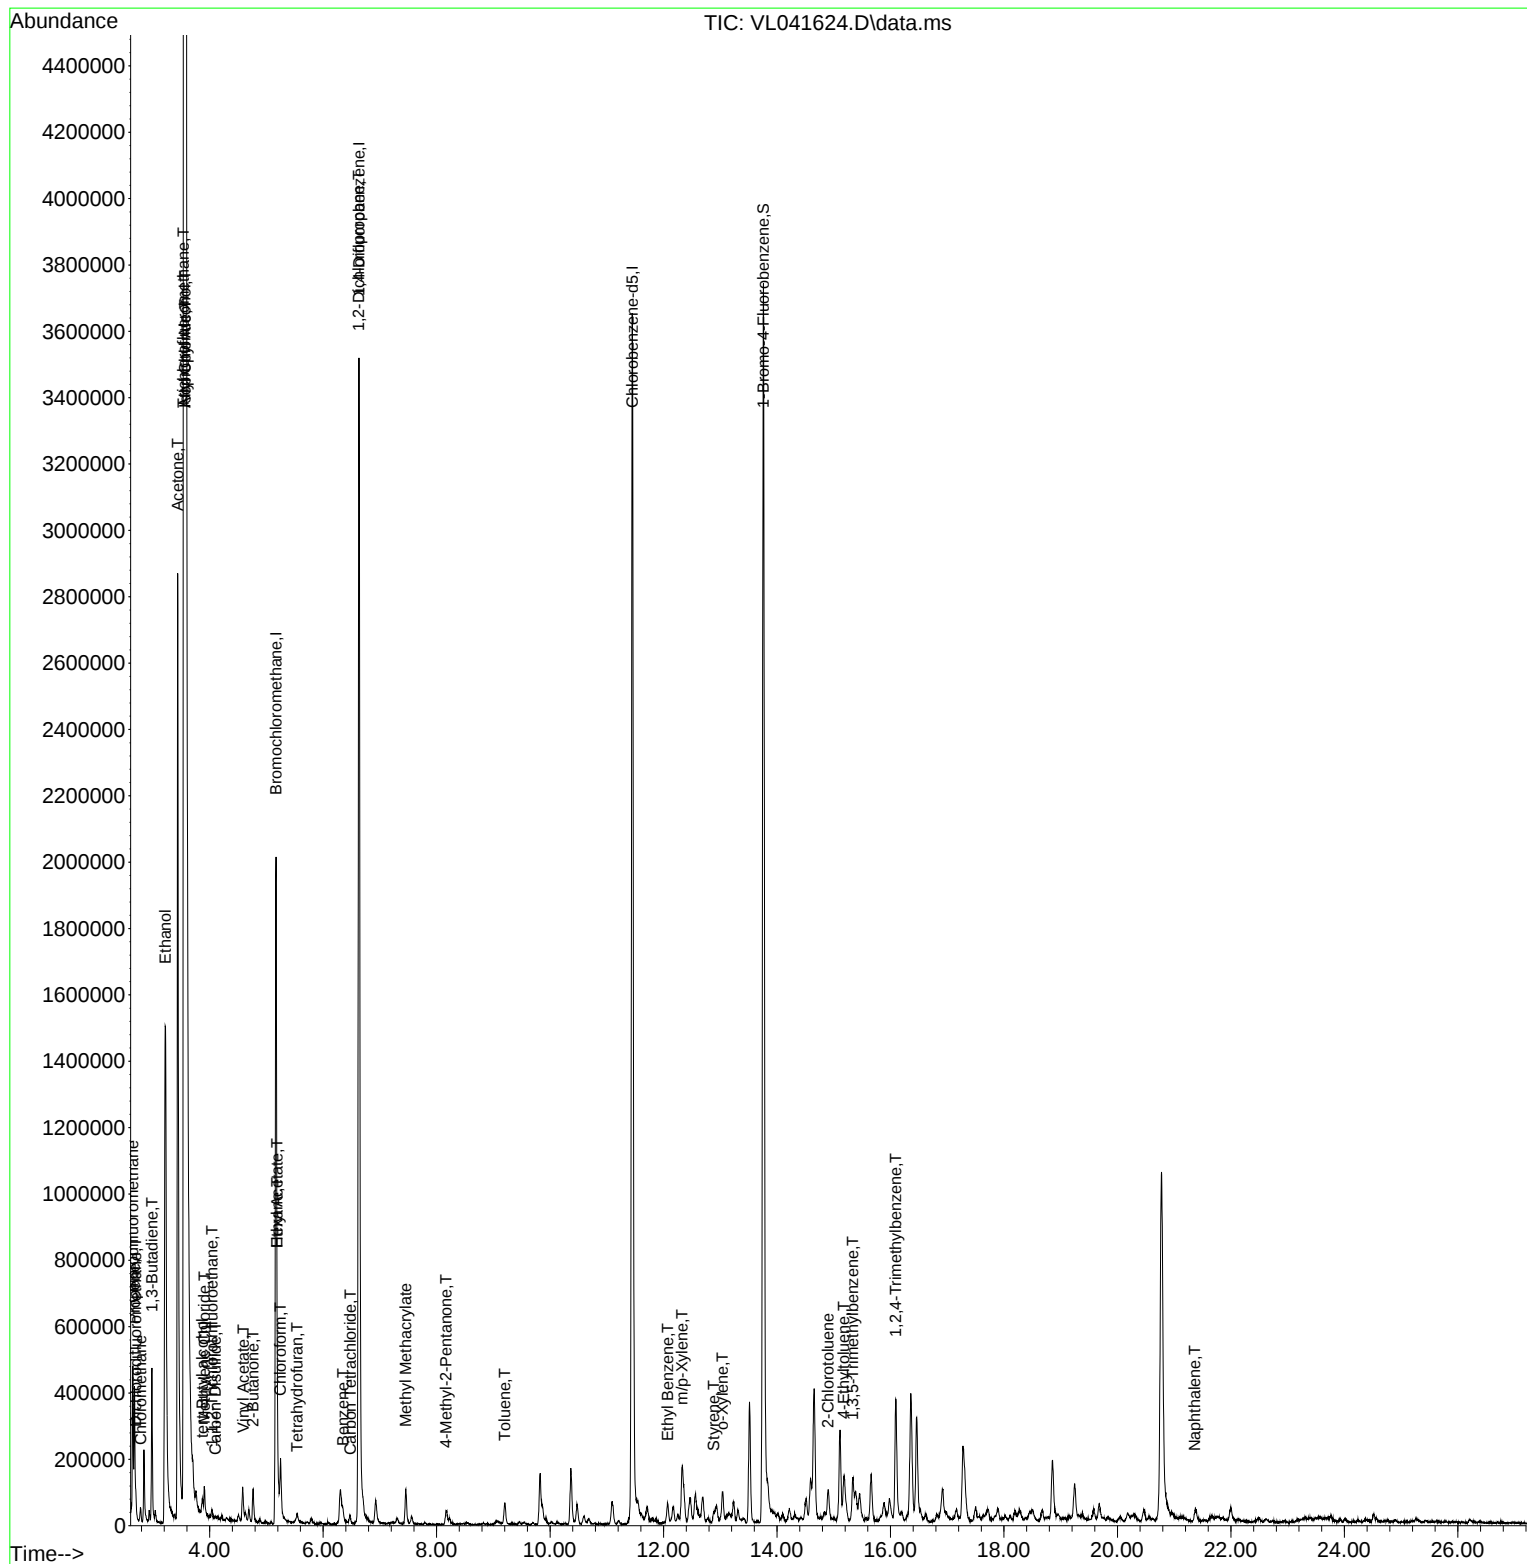




#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.169 min Scan# 798
Delta R.T. 0.000 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 49 Resp: 984915
Ion Ratio Lower Upper
49 100
128 46.6 23.8 71.5
130 60.3 30.4 91.3

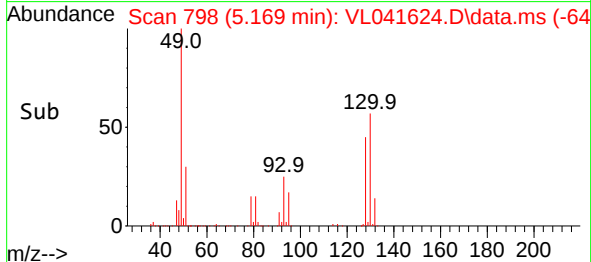

#2
Dichlorodifluoromethane
Concen: 0.244 ppbv
RT: 2.697 min Scan# 29
Delta R.T. -0.013 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15

Tgt Ion: 85 Resp: 34707
Ion Ratio Lower Upper
85 100
87 27.6 26.3 39.5


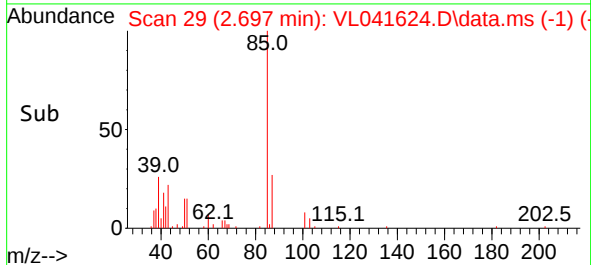

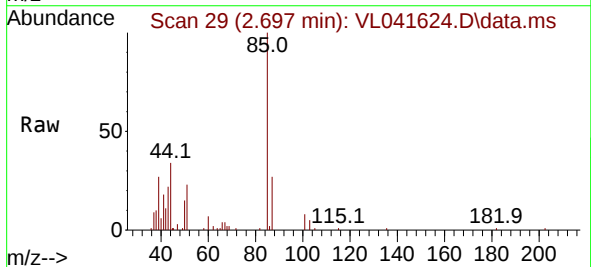




#3
Chlorodifluoromethane
Concen: 3.490 ppbv
RT: 2.645 min Scan# 11
Delta R.T. -0.006 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 51 Resp: 416875
Ion Ratio Lower Upper
51 100
67 17.4 14.1 21.1

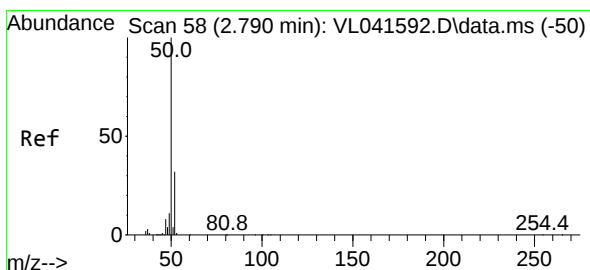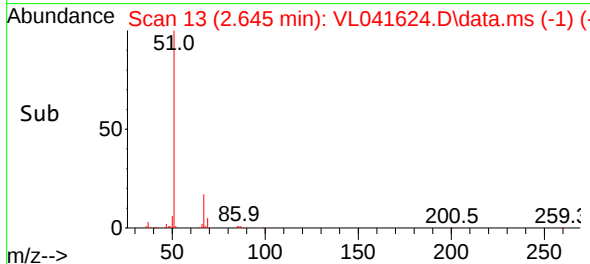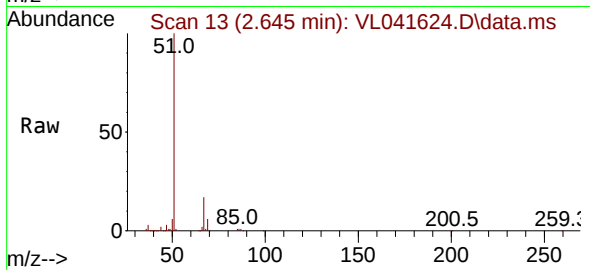

#4
Chloromethane
Concen: 0.503 ppbv
RT: 2.784 min Scan# 56
Delta R.T. -0.006 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15

Tgt Ion: 50 Resp: 33078
Ion Ratio Lower Upper
50 100
52 29.3 25.4 38.2


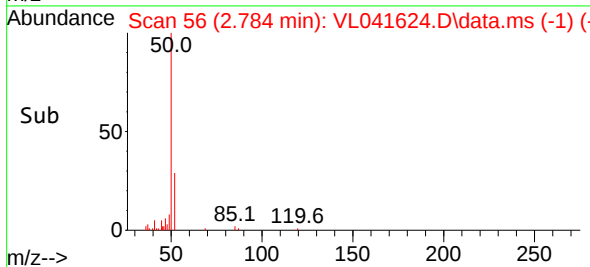

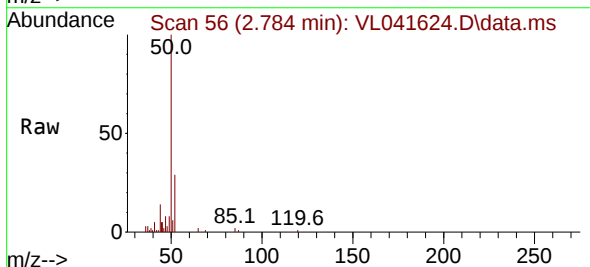


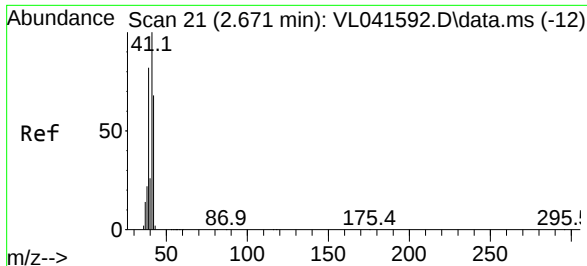

#9
Propene
Concen: 1.531 ppbv
RT: 2.674 min Scan# 21
Delta R.T. 0.003 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 41 Resp: 77138
Ion Ratio Lower Upper
41 100
42 44.3 55.2 82.8#

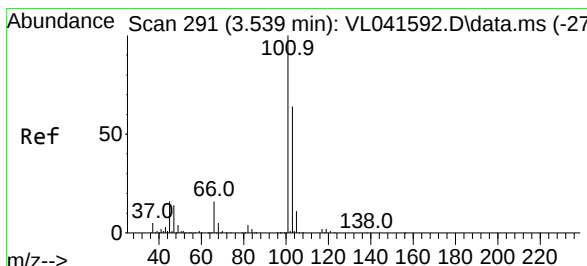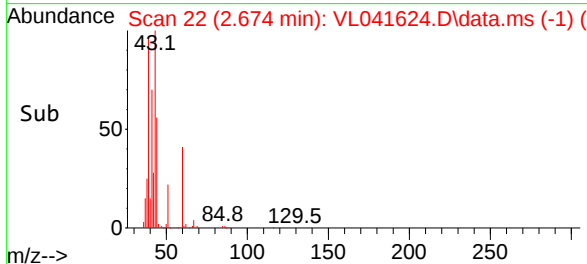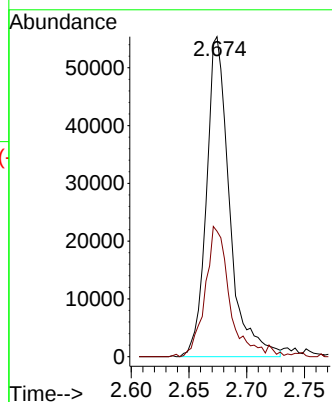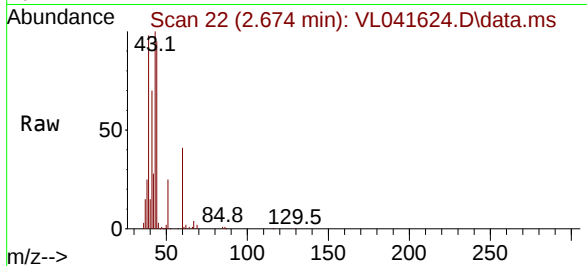

#11
Trichlorofluoromethane
Concen: 0.218 ppbv
RT: 3.536 min Scan# 290
Delta R.T. -0.003 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15

Tgt Ion: 101 Resp: 33046
Ion Ratio Lower Upper
101 100
103 67.1 51.2 76.8

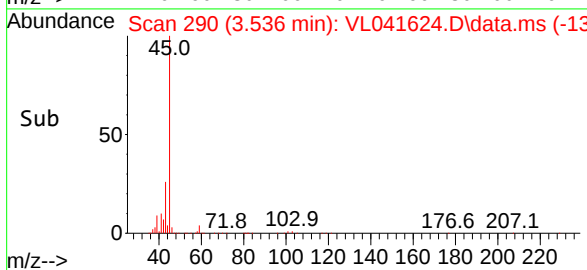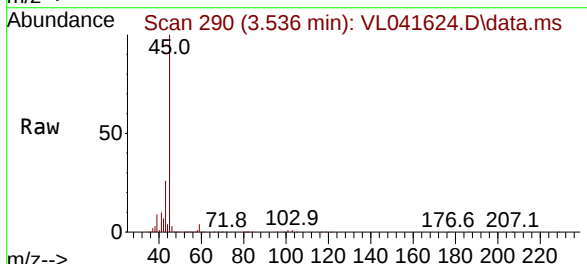



#12

1,1,2-Trichlorotrifluoroethane

Concen: 0.045 ppbv

RT: 4.041 min Scan# 447

Delta R.T. 0.000 min

Lab File: VL041624.D

Acq: 25 Sep 2024 15:15

Instrument :

MSVOA_L





ClientSampleId :

Tgt Ion:101 Resp: 4918

Ion Ratio Lower Upper

101 100

151 114.5 59.4 89.2#

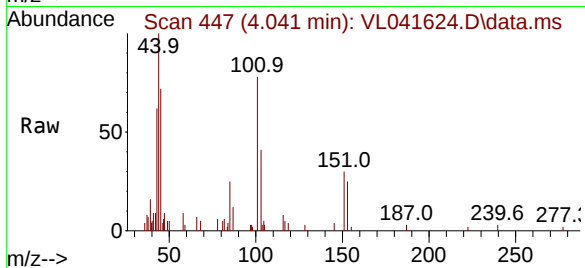

#13

Ethanol

Concen: 529.238 ppbv

RT: 3.218 min Scan# 191

Delta R.T. -0.006 min

Lab File: VL041624.D




Acq: 25 Sep 2024 15:15


Tgt Ion: 45 Resp: 2004921

Ion Ratio Lower Upper

45 100

46 35.3 15.2 60.8

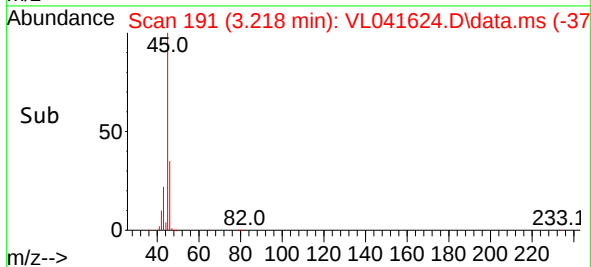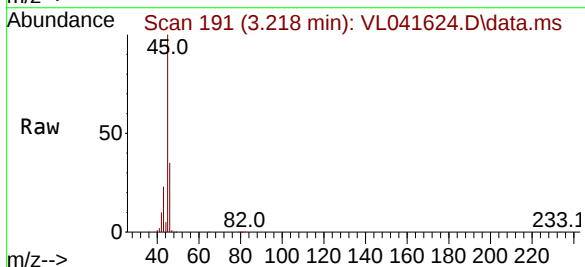



#15

Acetone

Concen: 23.497 ppbv

RT: 3.436 min Scan# 21

Delta R.T. -0.006 min

Lab File: VL041624.D

Acq: 25 Sep 2024 15:15

Instrument :

MSVOA_L





ClientSampleId :

Tgt Ion: 43 Resp: 2905446

Ion Ratio Lower Upper

43 100

58 27.1 21.5 32.3

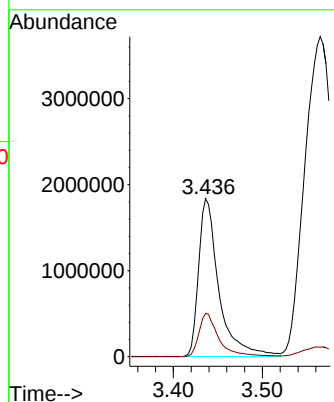

#16

1,3-Butadiene

Concen: 0.900 ppbv

RT: 2.980 min Scan# 117

Delta R.T. 0.016 min

Lab File: VL041624.D




Acq: 25 Sep 2024 15:15


Tgt Ion: 39 Resp: 54116

Ion Ratio Lower Upper

39 100

54 2.6 62.9 94.3#





#17

tert-Butyl alcohol

Concen: 0.264 ppbv

RT: 3.874 min Scan# 395

Delta R.T. 0.023 min

Lab File: VL041624.D

Acq: 25 Sep 2024 15:15

Instrument :

MSVOA_L





ClientSampleId :

Tgt Ion: 59 Resp: 28761

Ion Ratio Lower Upper

59 100

57 15.6 8.7 13.1#

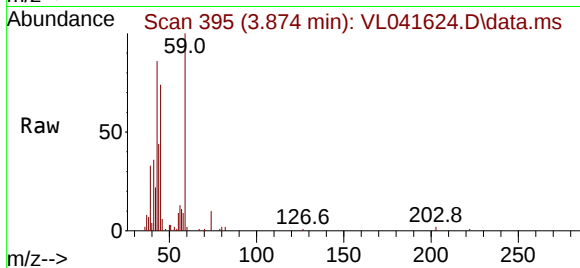

#19

Isopropyl Alcohol

Concen: 379.178 ppbv

RT: 3.565 min Scan# 299

Delta R.T. 0.013 min

Lab File: VL041624.D




Acq: 25 Sep 2024 15:15


Tgt Ion: 45 Resp: 24001410

Ion Ratio Lower Upper

45 100

58 1.5 2.1 3.1#

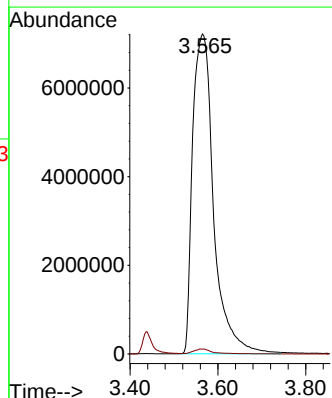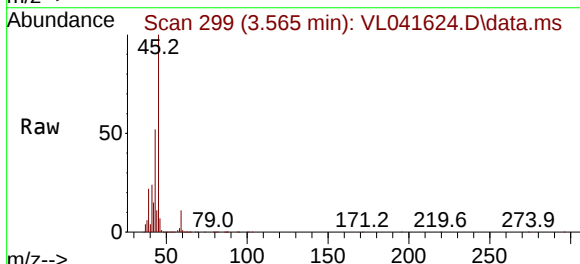



#20

Methylene Chloride

Concen: 0.508 ppbv

RT: 3.906 min Scan# 406

Delta R.T. -0.003 min


Lab File: VL041624.D

Acq: 25 Sep 2024 15:15

Instrument :

MSVOA_L

ClientSampleId :



Tgt Ion: 84 Resp: 23593




Ion Ratio Lower Upper

84 100

49 157.4 124.3 186.5

51 49.6 36.3 54.5

86 63.1 47.4 71.2



#21

Allyl Chloride

Concen: 55.395 ppbv

RT: 3.565 min Scan# 299

Delta R.T. -0.408 min

Lab File: VL041624.D

Acq: 25 Sep 2024 15:15




Tgt Ion: 41 Resp: 3970055


Ion Ratio Lower Upper

41 100

76 0.0 23.8 35.6#

39 89.3 63.9 95.9


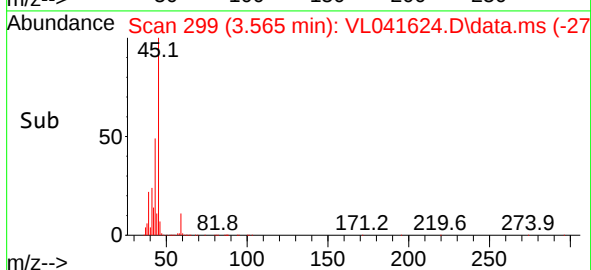






#23
Vinyl Acetate
Concen: 0.234 ppbv
RT: 4.591 min Scan# 618
Delta R.T. -0.013 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion:	43	Resp:	15948
Ion	Ratio	Lower	Upper
43	100		
86	8.8	4.9	7.3#
42	130.3	8.0	12.0#
44	7.6	6.1	9.1

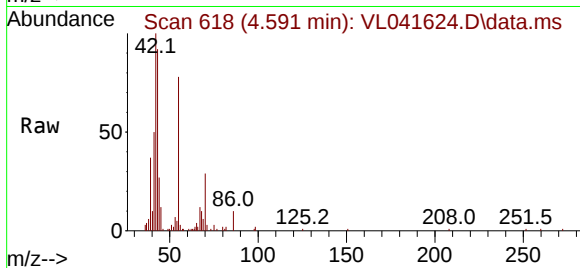

#25
Ethyl Acetate
Concen: 0.093 ppbv
RT: 5.189 min Scan# 804
Delta R.T. 0.010 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15


Tgt Ion:	43	Resp:	20618
Ion	Ratio	Lower	Upper
43	100		
45	31.5	8.2	12.2#
61	9.5	8.0	12.0
70	8.2	5.7	8.5

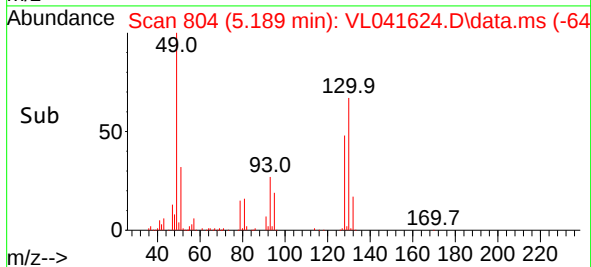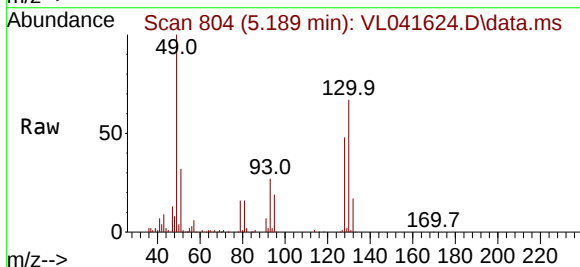






#26
Hexane
Concen: 0.100 ppbv
RT: 5.189 min Scan# 804
Delta R.T. 0.000 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15

Instrument :
MSVOA_L
ClientSampleId :

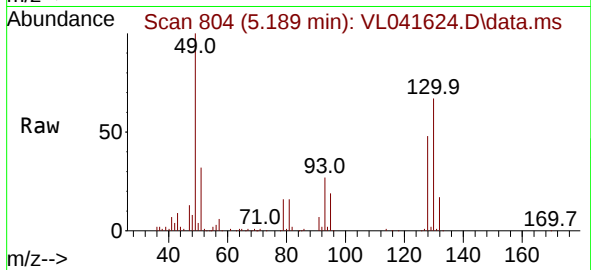

Tgt Ion: 57 Resp: 9293




Ion	Ratio	Lower	Upper
57	100		
41	190.2	75.7	113.5#
43	268.6	198.5	297.7
56	111.0	44.1	66.1#




#27
Carbon Disulfide
Concen: 0.049 ppbv
RT: 4.102 min Scan# 466
Delta R.T. 0.003 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15

Tgt Ion: 76 Resp: 4857

Ion	Ratio	Lower	Upper
76	100		
44	0.0	15.8	23.8#
78	14.2	7.5	11.3#

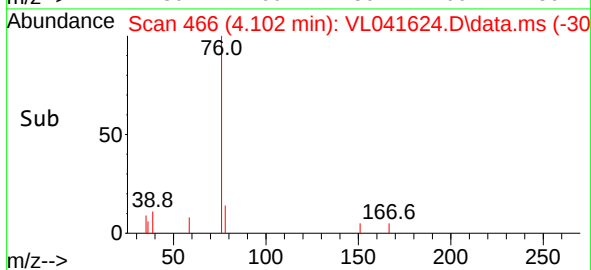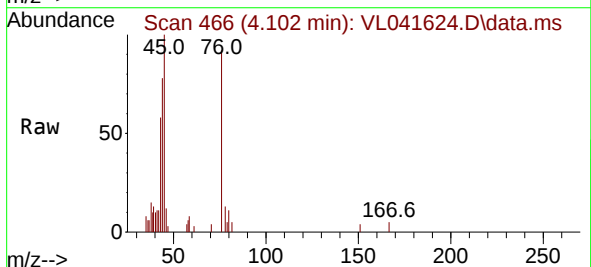



#29

Chloroform

Concen: 0.679 ppbv

RT: 5.250 min Scan# 81

Delta R.T. 0.000 min

Lab File: VL041624.D

Acq: 25 Sep 2024 15:15

Instrument :

MSVOA_L





ClientSampleId :

Tgt Ion: 83 Resp: 102851

Ion Ratio Lower Upper

83 100

85 53.1 53.8 80.6#

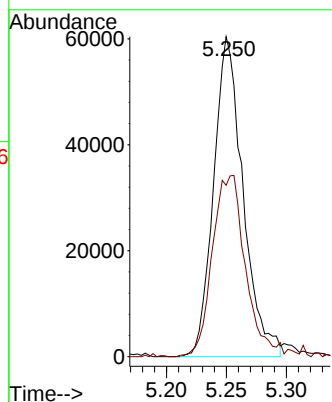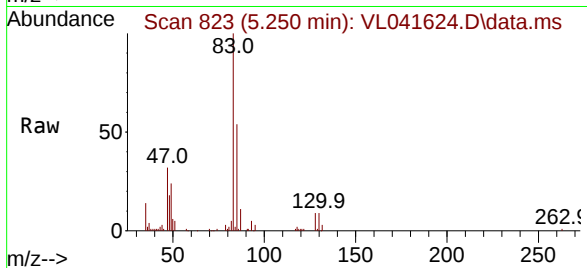

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 6.632 min Scan# 1253

Delta R.T. 0.003 min

Lab File: VL041624.D

Acq: 25 Sep 2024 15:15




Tgt Ion: 114 Resp: 2630467


Ion Ratio Lower Upper

114 100

63 25.1 20.2 30.2

88 17.9 14.2 21.4


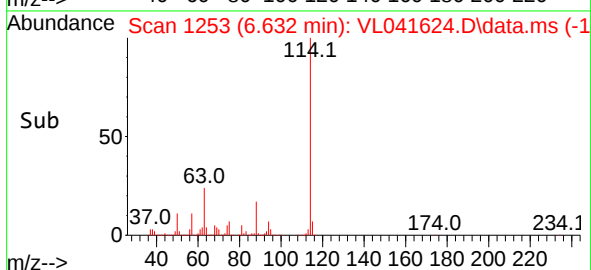

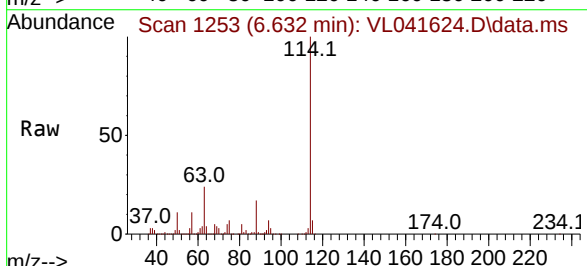




#34
2-Butanone
Concen: 0.838 ppbv
RT: 4.767 min Scan# 61
Delta R.T. 0.007 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 43 Resp: 105134
Ion Ratio Lower Upper
43 100
72 23.4 16.8 25.2

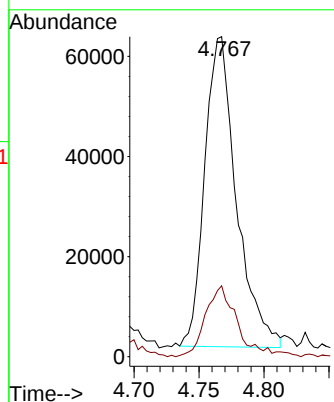

#35
Carbon Tetrachloride
Concen: 0.045 ppbv
RT: 6.478 min Scan# 1205
Delta R.T. 0.007 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15

Tgt Ion: 117 Resp: 5849
Ion Ratio Lower Upper
117 100
119 85.2 76.8 115.2
121 21.2 25.0 37.6#


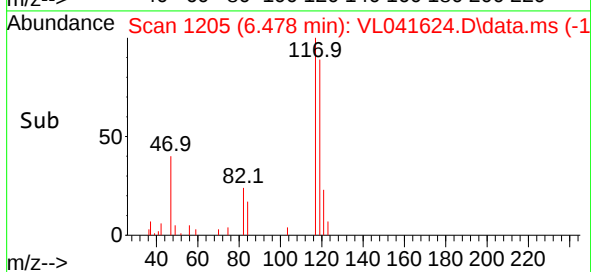
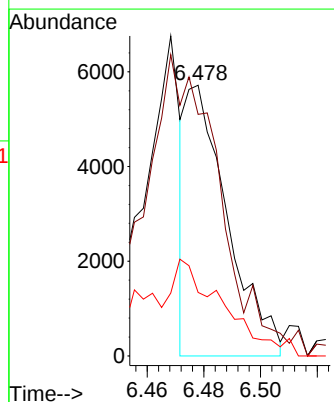





#36
Benzene
Concen: 0.113 ppbv
RT: 6.349 min Scan# 1165
Delta R.T. 0.003 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 78 Resp: 20609
Ion Ratio Lower Upper
78 100
77 25.8 17.8 26.6
50 20.0 15.4 23.0



#39
1,2-Dichloropropane
Concen: 8.802 ppbv
RT: 6.629 min Scan# 1252
Delta R.T. -0.421 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15

Tgt Ion: 63 Resp: 654135
Ion Ratio Lower Upper
63 100
41 0.0 59.5 89.3#
62 17.5 56.2 84.2#

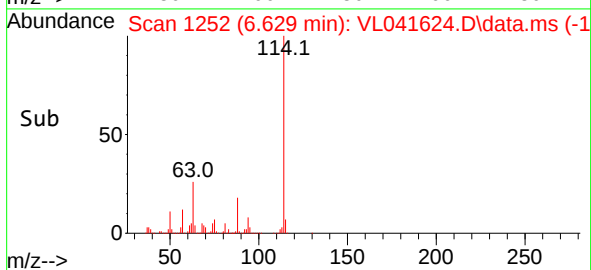



#41

Tetrahydrofuran

Concen: 0.070 ppbv

RT: 5.539 min Scan# 911

Delta R.T. 0.007 min

Lab File: VL041624.D

Acq: 25 Sep 2024 15:15

Instrument :

MSVOA_L

ClientSampleId :





Tgt Ion: 42 Resp: 4839

Ion Ratio Lower Upper

42 100

72 0.0 30.2 45.2#

71 0.0 29.6 44.4#

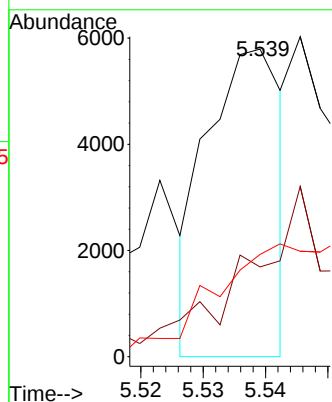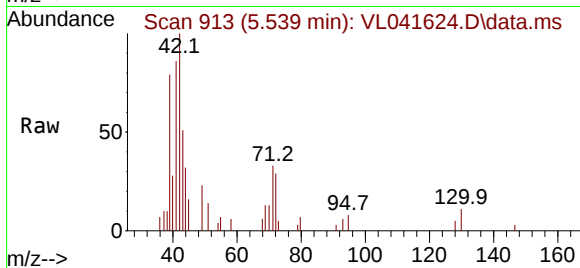

#43

Methyl Methacrylate

Concen: 0.208 ppbv

RT: 7.455 min Scan# 1509

Delta R.T. 0.007 min

Lab File: VL041624.D

Acq: 25 Sep 2024 15:15




Tgt Ion: 69 Resp: 13578


Ion Ratio Lower Upper

69 100

41 0.0 121.8 182.6#

100 0.0 26.5 39.7#

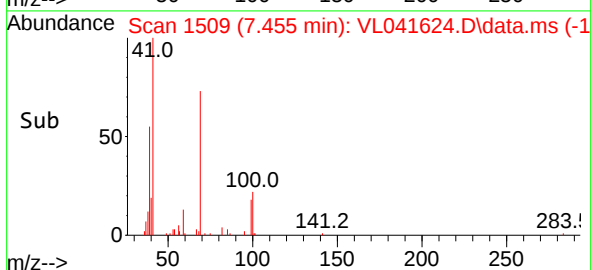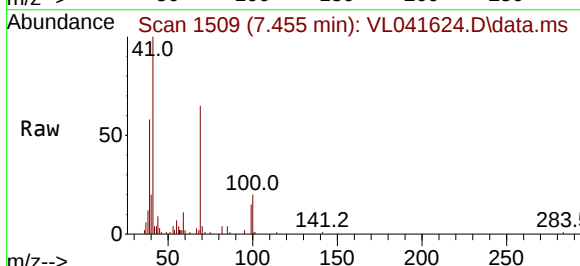



#50

4-Methyl-2-Pentanone

Concen: 0.127 ppbv

RT: 8.166 min Scan# 1730

Delta R.T. 0.010 min

Lab File: VL041624.D

Acq: 25 Sep 2024 15:15

Instrument :

MSVOA_L





ClientSampleId :

Tgt Ion: 43 Resp: 24504

Ion Ratio Lower Upper

43 100

58 44.3 27.8 41.8#

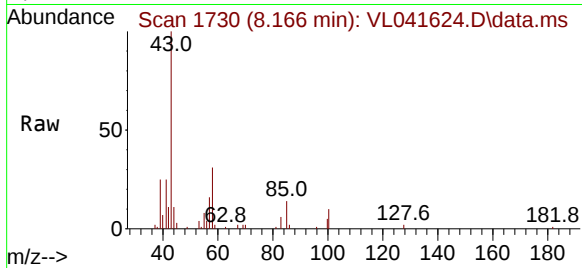

#53

Toluene

Concen: 0.219 ppbv

RT: 9.201 min Scan# 2052

Delta R.T. 0.003 min

Lab File: VL041624.D




Acq: 25 Sep 2024 15:15


Tgt Ion: 91 Resp: 42438

Ion Ratio Lower Upper

91 100

92 57.0 48.9 73.3


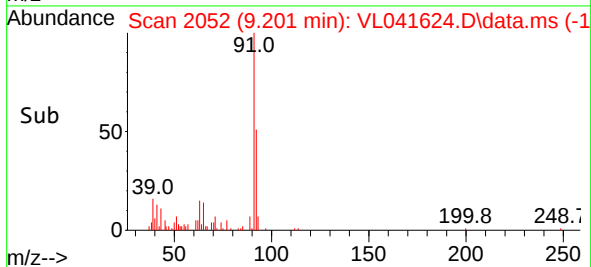

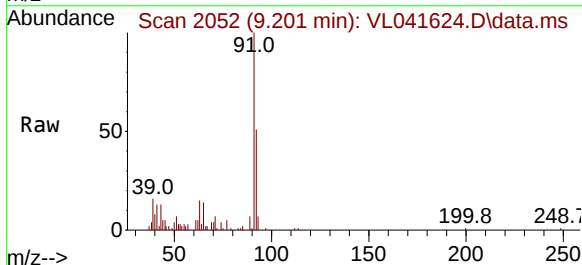




#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.449 min Scan# 21
Delta R.T. 0.003 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion:117 Resp: 2395289
Ion Ratio Lower Upper
117 100
82 64.1 49.4 74.2
119 33.1 24.4 36.6

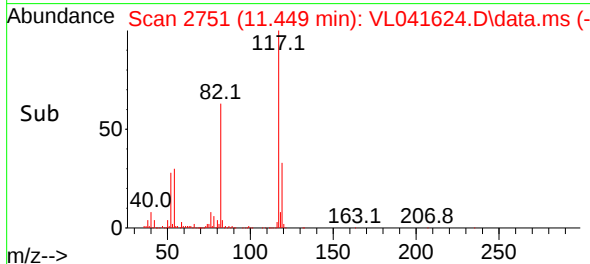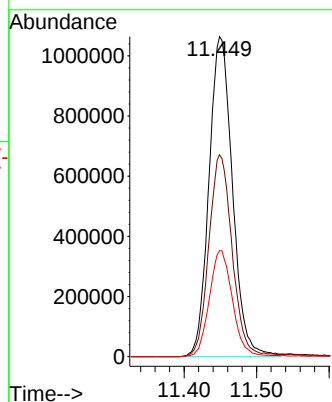

#58
Ethyl Benzene
Concen: 0.119 ppbv
RT: 12.073 min Scan# 2945
Delta R.T. 0.007 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15

Tgt Ion: 91 Resp: 30455
Ion Ratio Lower Upper
91 100
106 30.2 25.8 38.6


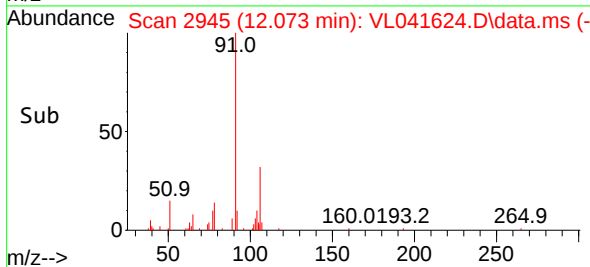
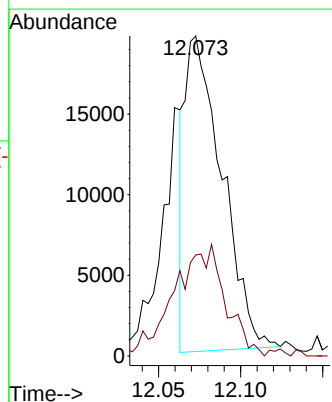
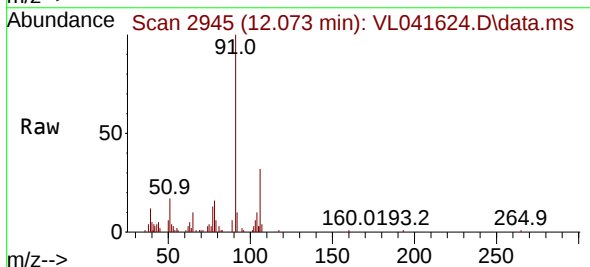




#59
m/p-Xylene
Concen: 0.741 ppbv
RT: 12.327 min Scan# 3030
Delta R.T. -0.019 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 91 Resp: 169121
Ion Ratio Lower Upper
91 100
106 49.2 36.8 55.2

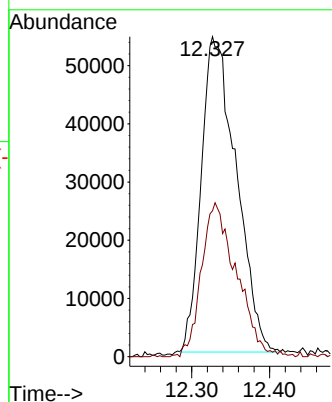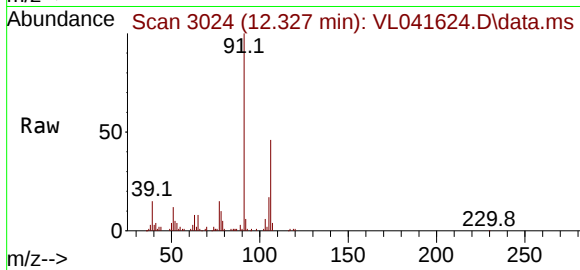

#60
o-Xylene
Concen: 0.150 ppbv
RT: 13.037 min Scan# 3245
Delta R.T. 0.003 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15

Tgt Ion: 91 Resp: 32925
Ion Ratio Lower Upper
91 100
106 0.0 23.1 69.3#


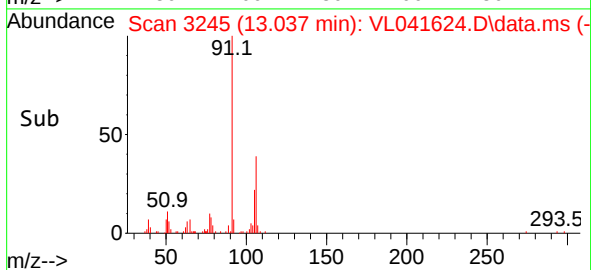
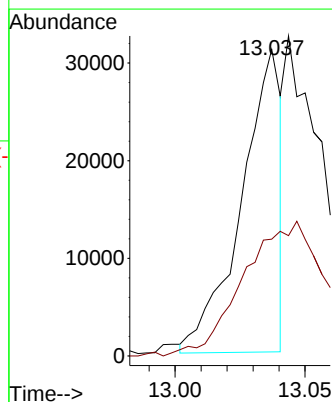
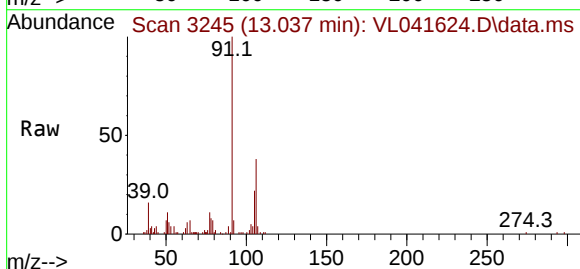


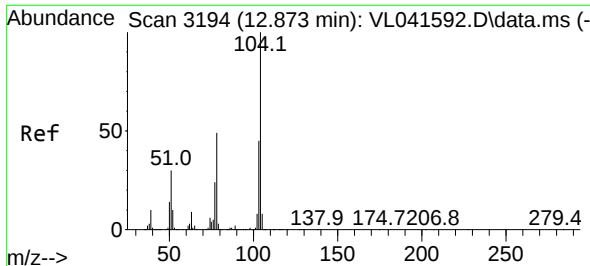

#61
Styrene
Concen: 0.034 ppbv
RT: 12.883 min Scan# 3194
Delta R.T. 0.010 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion:104 Resp: 3076
Ion Ratio Lower Upper
104 100
78 148.4 39.8 59.6#
103 142.5 37.4 56.0#

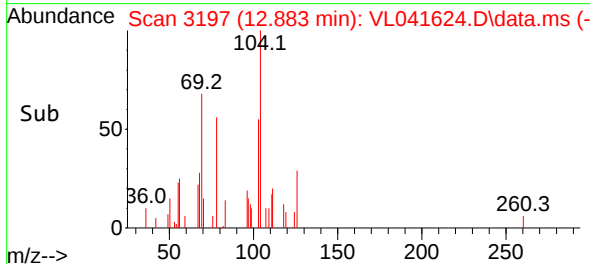

#68
1-Bromo-4-Fluorobenzene
Concen: 10.239 ppbv
RT: 13.761 min Scan# 3470
Delta R.T. 0.010 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15

Tgt Ion: 95 Resp: 1805386
Ion Ratio Lower Upper
95 100
174 69.6 55.8 83.8
175 5.1 4.1 6.1


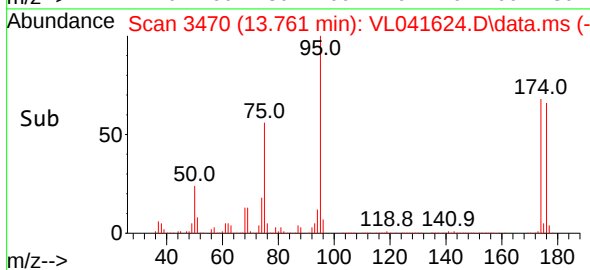

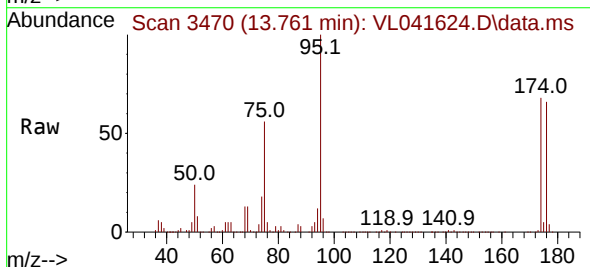




#71
2-Chlorotoluene
Concen: 0.347 ppbv
RT: 14.899 min Scan# 3824
Delta R.T. 0.122 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15




Instrument :
MSVOA_L
ClientSampleId :


Tgt Ion: 91 Resp: 84737
Ion Ratio Lower Upper
91 100
126 0.2 12.9 51.5#

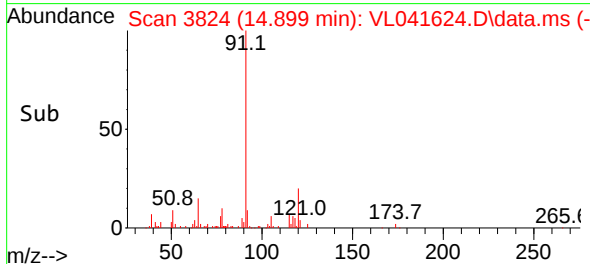

#72
4-Ethyltoluene
Concen: 0.392 ppbv
RT: 15.172 min Scan# 3909
Delta R.T. 0.003 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15

Tgt Ion: 105 Resp: 100202
Ion Ratio Lower Upper
105 100
120 30.7 24.1 36.1
91 16.1 10.2 15.2#
77 17.1 10.9 16.3#


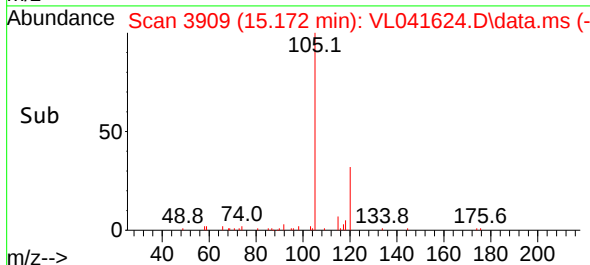
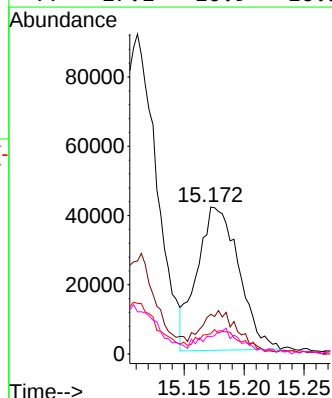
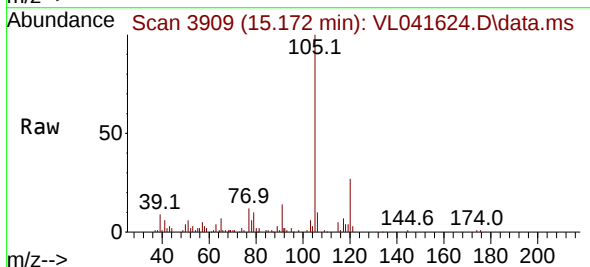


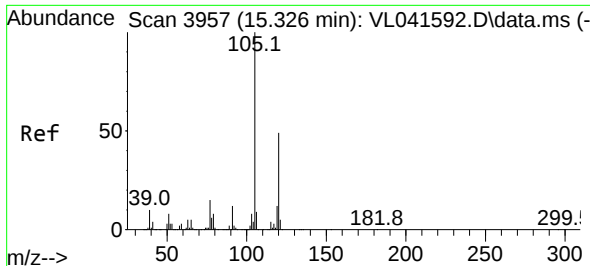

#73
 1,3,5-Trimethylbenzene
 Concen: 0.139 ppbv
 RT: 15.330 min Scan# 3957
 Delta R.T. 0.003 min
 Lab File: VL041624.D
 Acq: 25 Sep 2024 15:15




Instrument :
 MSVOA_L
 ClientSampleId :


Tgt Ion:105 Resp: 31464
 Ion Ratio Lower Upper
 105 100
 120 45.2 39.4 59.0

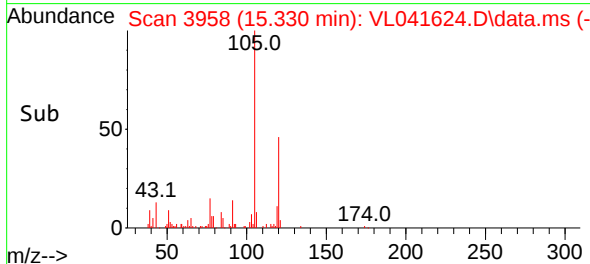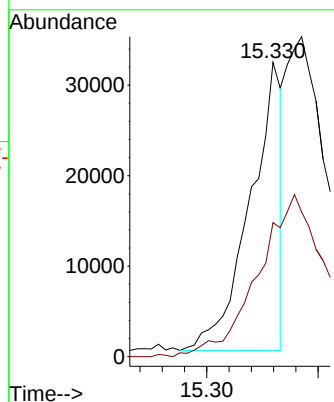

#74
 1,2,4-Trimethylbenzene
 Concen: 0.960 ppbv
 RT: 16.092 min Scan# 4195
 Delta R.T. 0.007 min
 Lab File: VL041624.D
 Acq: 25 Sep 2024 15:15

Tgt Ion:105 Resp: 253845
 Ion Ratio Lower Upper
 105 100
 120 49.6 39.9 59.9
 91 12.4 42.6 63.8#
 77 15.5 18.2 27.2#

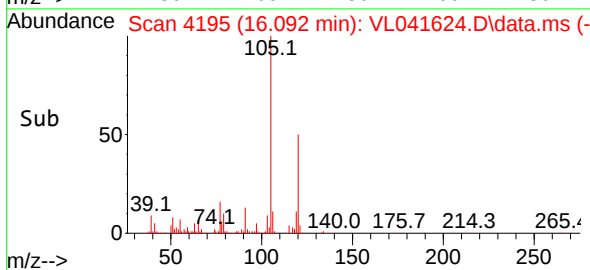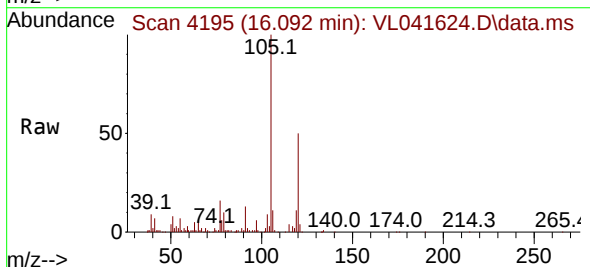

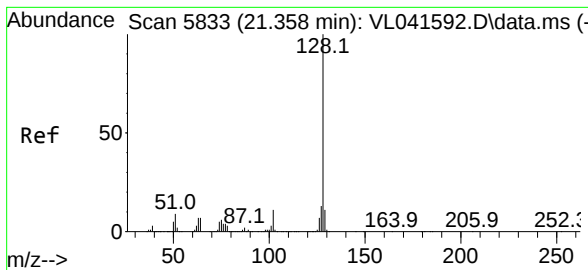

#79
Naphthalene
Concen: 0.046 ppbv
RT: 21.358 min Scan# 5833
Delta R.T. 0.000 min
Lab File: VL041624.D
Acq: 25 Sep 2024 15:15

Instrument :
MSVOA_L
ClientSampleId :

Tgt Ion:	128	Resp:	9038
Ion Ratio	Lower	Upper	
128	100		
127	9.6	10.1	15.1#
129	17.5	9.1	13.7#

