


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL092524\
Data File : VL041619.D
Acq On : 25 Sep 2024 11:50
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL091624AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Sep 17 09:12:21 2024

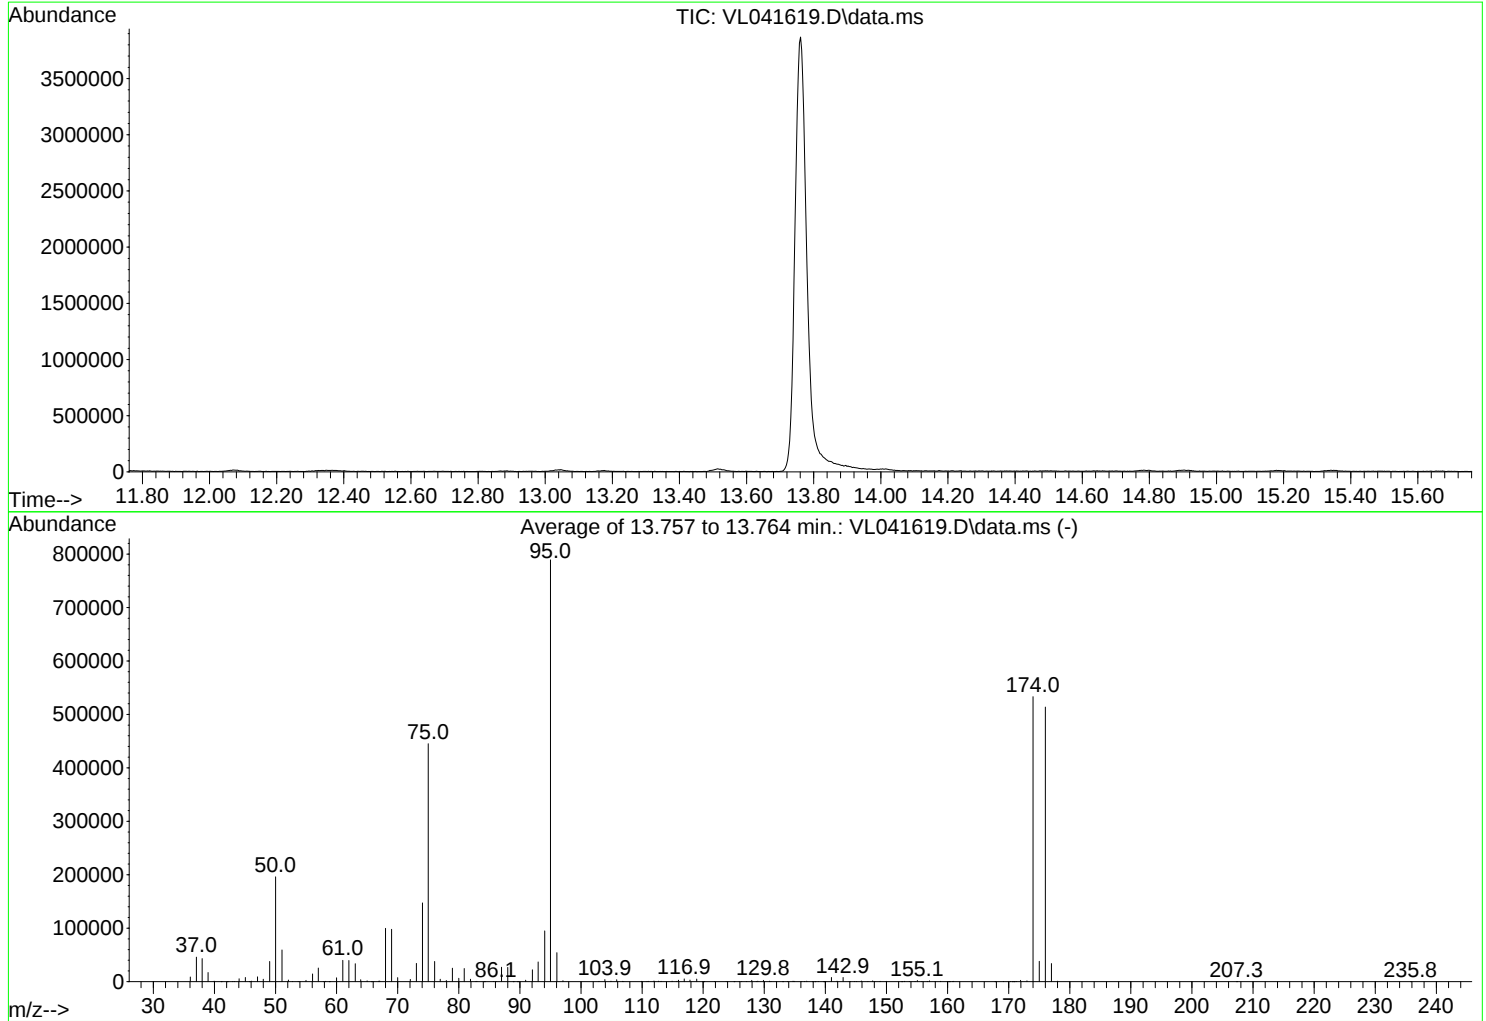

AutoFind: Scans 3469, 3470, 3471; Background Corrected with Scan 3447

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.8	196053	PASS
75	95	30	66	56.4	445141	PASS
95	95	100	100	100.0	789205	PASS
96	95	5	9	6.9	54339	PASS
173	174	0.00	2	0.3	1464	PASS
174	95	50	120	67.6	533312	PASS
175	174	4	9	7.1	38085	PASS
176	174	93	101	96.3	513600	PASS
177	176	5	9	6.6	33995	PASS

Average of 13.757 to 13.764 min.: VL041619.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	8779	45.75	70	55.00	2506	65.00	160
37.05	45667	46.05	942	56.05	14480	65.70	7
38.00	43248	47.05	8986	57.00	25315	66.10	29
38.95	17030	48.00	4600	57.90	379	66.90	92
39.95	1074	49.05	37651	58.20	536	67.05	1312
41.10	153	50.00	196053	58.80	66	68.00	99752
42.10	139	51.05	59163	60.00	7157	69.00	98013
43.00	325	52.10	2934	61.00	39912	70.00	7442
43.25	353	52.80	161	62.00	39560	72.05	4329
44.05	5544	53.70	166	63.05	33656	73.05	34267
45.05	7909	54.00	276	63.95	3456	74.05	147221

Average of 13.757 to 13.764 min.: VL041619.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.00	445141	85.70	306	96.05	54339	111.95	1096
76.05	37616	86.10	321	97.05	1880	112.70	850
76.95	4390	87.00	26973	102.95	516	113.10	634
77.95	2169	88.00	26624	103.90	3834	114.90	771
78.95	25248	88.90	106	104.90	1041	115.70	490
80.00	6214	89.60	81	105.85	3510	115.95	2793
80.90	24472	90.95	2767	106.80	588	116.90	5044
81.90	4487	92.05	22291	107.00	332	117.85	3024
82.80	279	93.00	36776	109.90	559	118.95	4932
82.95	579	94.05	94861	110.80	226	119.90	65
84.20	72	95.00	789205	111.00	529	120.10	146

Average of 13.757 to 13.764 min.: VL041619.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
121.85	335	130.85	916	138.30	63	145.90	1250
123.75	196	131.10	310	138.85	376	146.95	363
124.00	255	131.95	292	139.70	70	147.75	1408
125.05	114	133.00	50	139.90	56	148.10	397
125.90	396	133.80	339	141.00	7909	148.95	574
126.30	233	134.70	867	141.90	915	149.95	757
127.10	224	134.90	513	142.90	7948	152.50	104
127.95	2358	136.05	191	143.90	334	152.95	646
128.70	418	136.60	186	144.10	208	153.75	406
128.95	791	136.95	1013	144.80	347	154.70	457
129.85	2557	137.90	53	145.10	471	155.05	2014

Average of 13.757 to 13.764 min.: VL041619.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.80	441	170.30	368	207.30	96		
156.70	404	170.60	143	235.80	58		
157.05	1560	170.90	135				
157.95	203	171.30	316				
158.85	719	171.95	2315				
159.95	123	173.00	1464				
160.30	86	174.00	533312				
160.80	301	175.00	38085				
161.00	639	176.00	513600				
167.75	145	177.00	33995				
169.15	301	178.00	1070				